

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032719\
 Data File : PP029576.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 21:03
 Operator : EI\MA
 Sample : PB118291BL
 Misc : hexane
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB118291BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 03:09:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.925	12.119	20326535	22613099	621.322	526.604
Target Compounds							
2) T	3,5-DICHL...	0.000	10.157	0	321416	N.D.	5.911 #
5) T	DICAMBA	12.268	12.365	301713	-43562	2.042	N.D. #
8) T	DICHLORPROP	0.000	13.554	0	1768121	N.D.	43.661 #
12) T	2,4,5-T	0.000	15.849	0	621022	N.D.	3.746 #
13) T	2,4-DB	16.242	0.000	797768	0	38.365	N.D. #
14) T	DINOSEB	0.000	16.898	0	314485	N.D.	2.082 #
15) T	Picloram	17.462	18.239	442963	750652	1.352	3.149 #
16) T	DCPA	18.047	18.101	977580	1191957	3.081	4.543 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032719\
Data File : PP029576.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 21:03
Operator : EI\MA
Sample : PB118291BL
Misc : hexane
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB118291BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 03:09:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

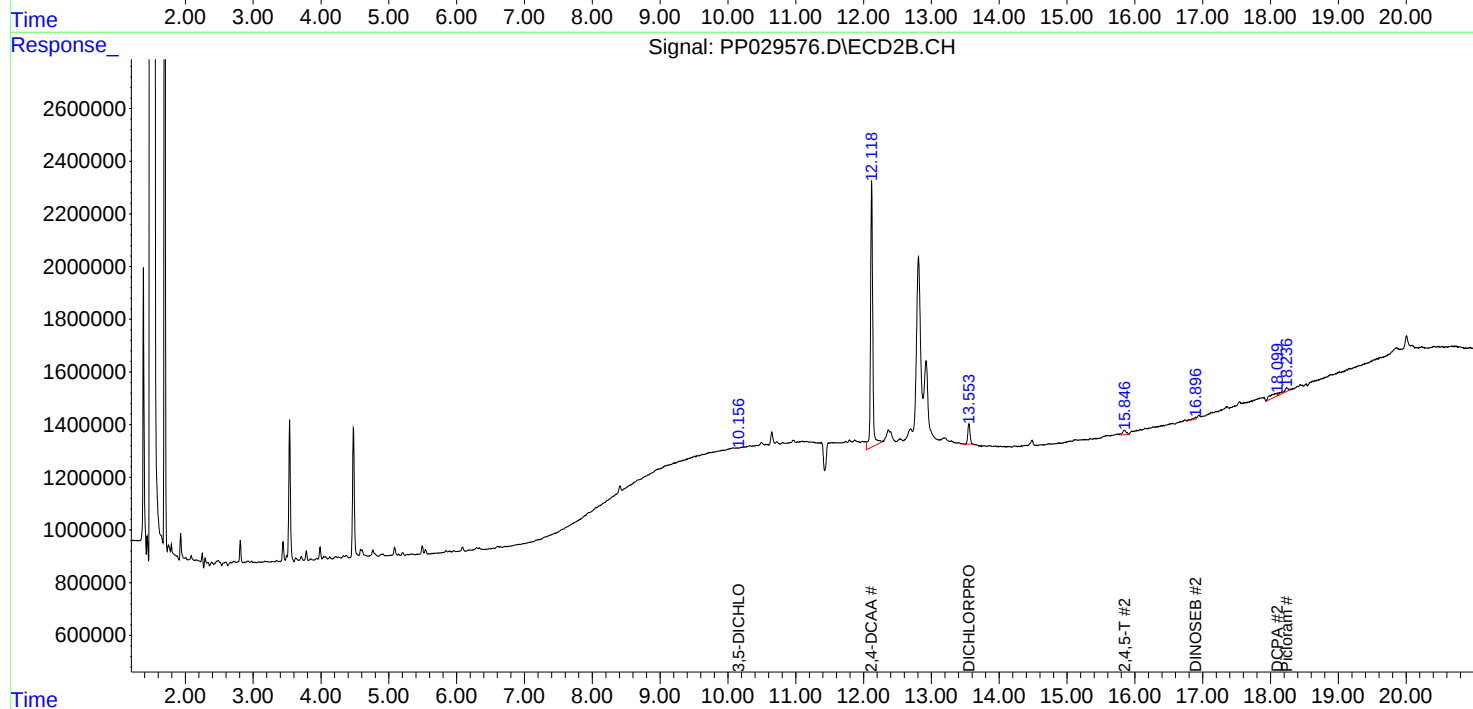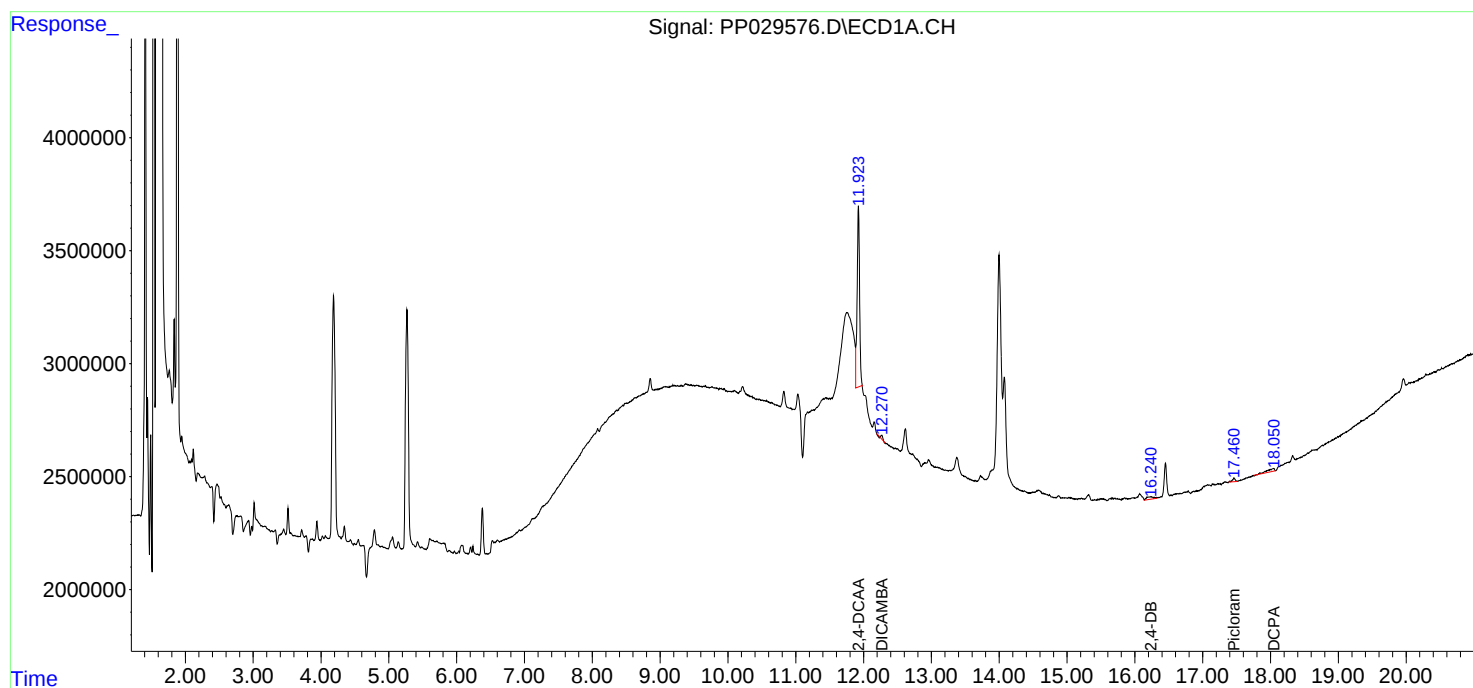


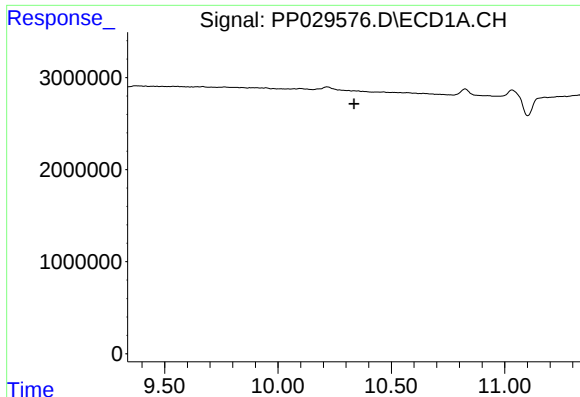

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB118291BL

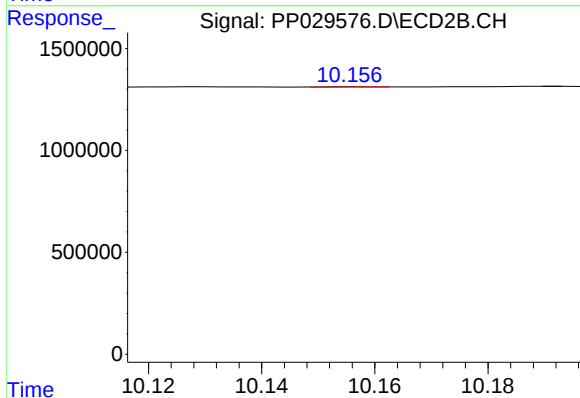


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.157 min
Delta R.T.: -0.052 min
Response: 321416
Conc: 5.91 ng/ml

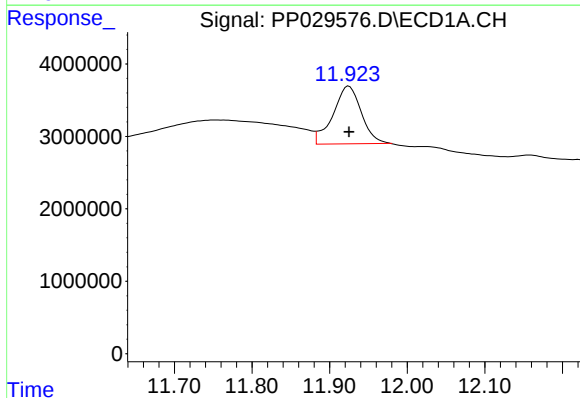


#4 2,4-DCAA

R.T.: 11.925 min
Delta R.T.: 0.000 min
Response: 20326535
Conc: 621.32 ng/ml

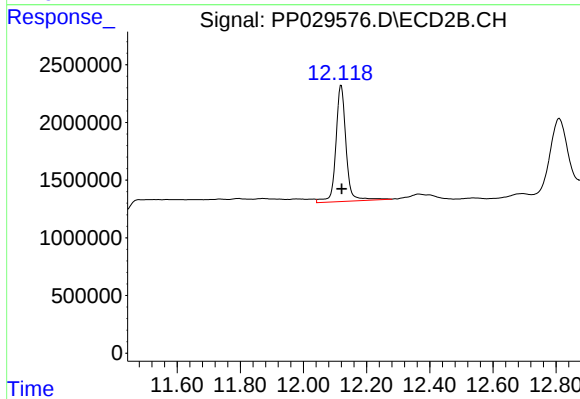

#4 2,4-DCAA


R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 22613099
Conc: 526.60 ng/ml

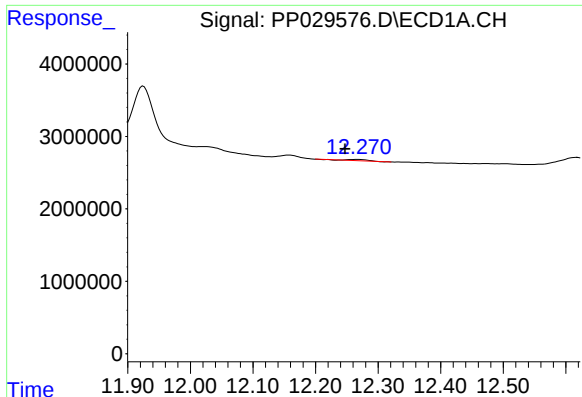

#5 DICAMBA


R.T.: 12.268 min
Delta R.T.: 0.021 min
Response: 301713
Conc: 2.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118291BL

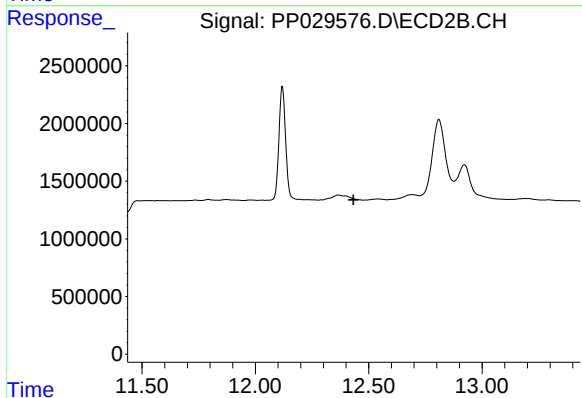


#5 DICAMBA

R.T.: 12.365 min
Delta R.T.: -0.068 min
Response: -43562
Conc: N.D.

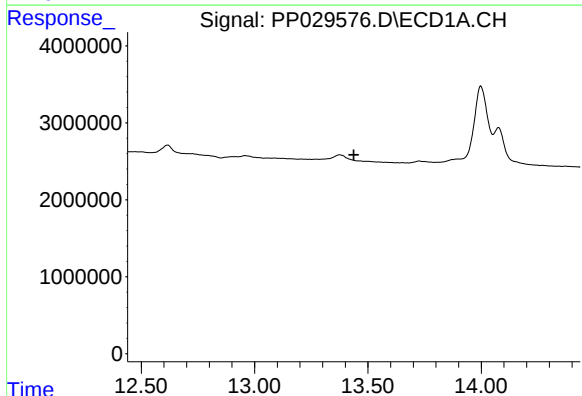


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.438 min
Response: 0
Conc: N.D.

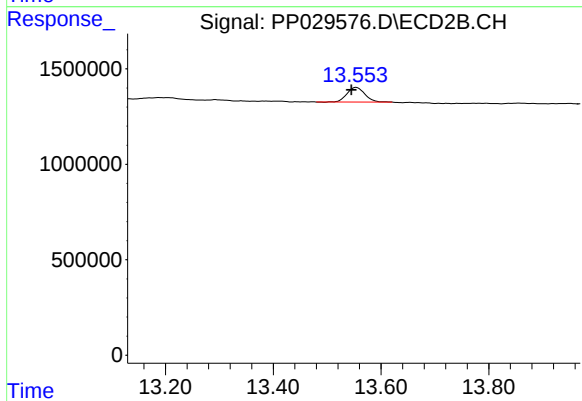

#8 DICHLORPROP


R.T.: 13.554 min
Delta R.T.: 0.009 min
Response: 1768121
Conc: 43.66 ng/ml

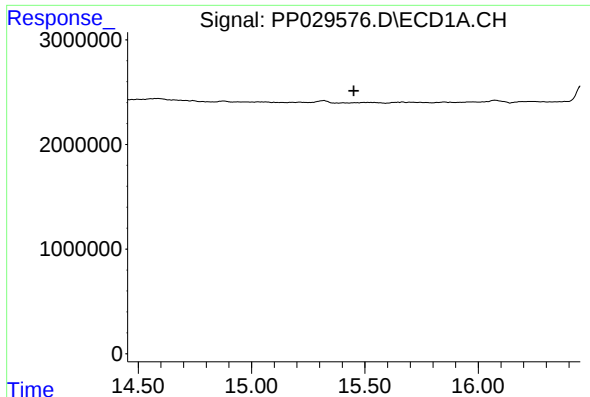

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB118291BL

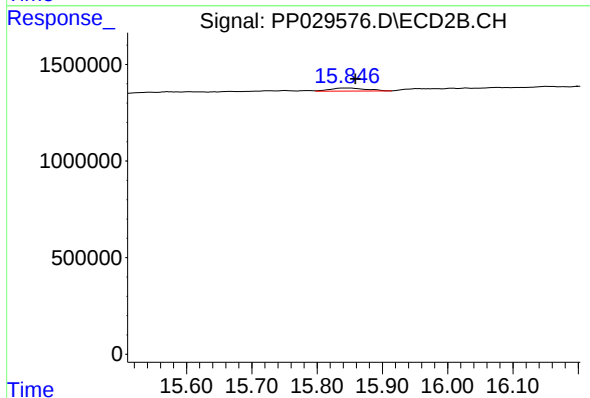


#12 2,4,5-T

R.T.: 15.849 min
Delta R.T.: -0.010 min
Response: 621022
Conc: 3.75 ng/ml

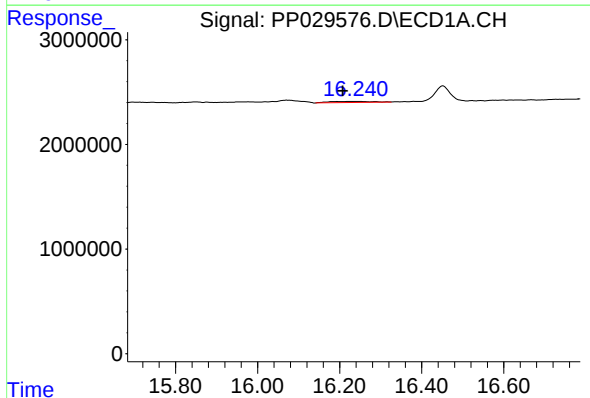


#13 2,4-DB

R.T.: 16.242 min
Delta R.T.: 0.034 min
Response: 797768
Conc: 38.37 ng/ml

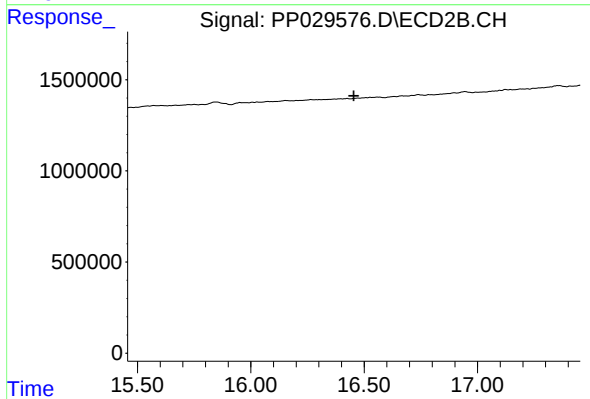

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.455 min
Response: 0
Conc: N.D.

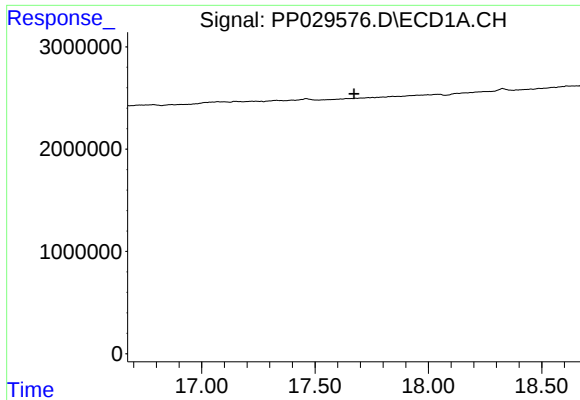

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.672 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB118291BL

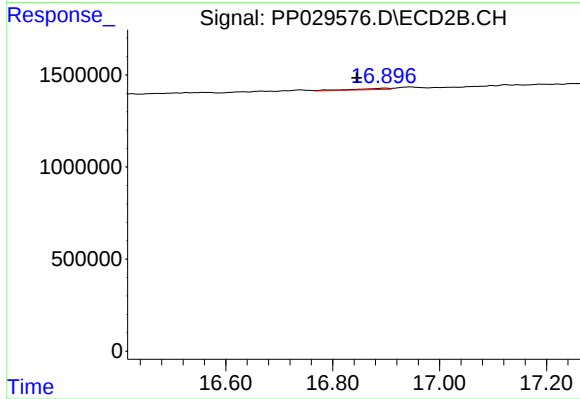


#14 DINOSEB

R.T.: 16.898 min
Delta R.T.: 0.053 min
Response: 314485
Conc: 2.08 ng/ml

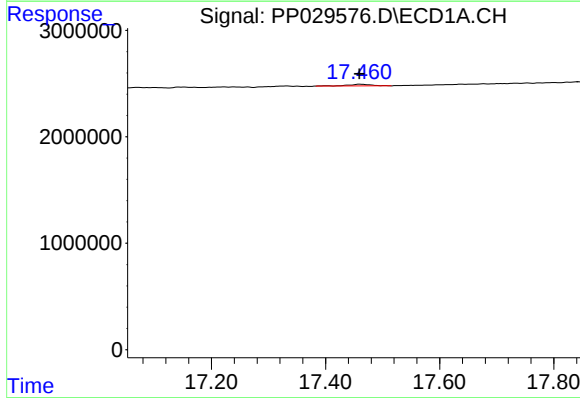


#15 Picloram

R.T.: 17.462 min
Delta R.T.: 0.002 min
Response: 442963
Conc: 1.35 ng/ml

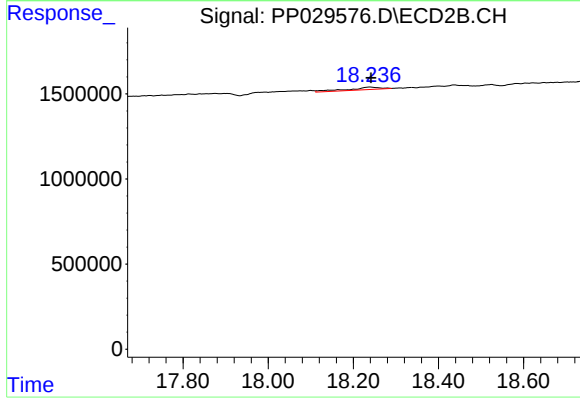

#15 Picloram


R.T.: 18.239 min
Delta R.T.: -0.003 min
Response: 750652
Conc: 3.15 ng/ml

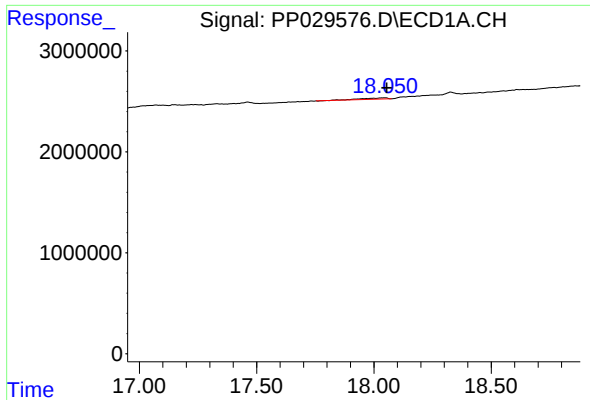

#16 DCPA

R.T.: 18.047 min
Delta R.T.: -0.007 min
Response: 977580
Conc: 3.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118291BL

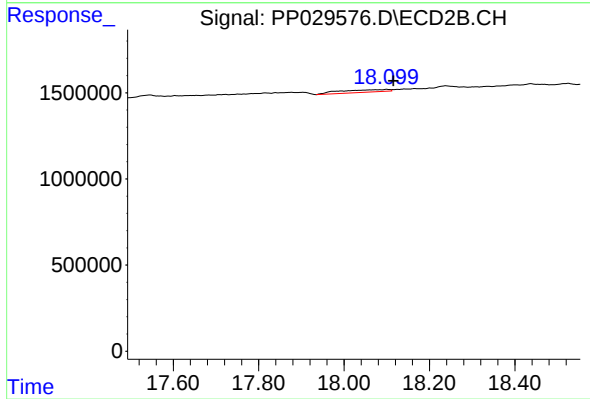

#16 DCPA

R.T.: 18.101 min
Delta R.T.: -0.015 min
Response: 1191957
Conc: 4.54 ng/ml