

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032719\
 Data File : PP029579.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 22:20
 Operator : EI\MA
 Sample : PB118241BL
 Misc : hexane
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB118241BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 03:10:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.119	21713009	18806669	663.702	437.962 #
Target Compounds							
1) T	Dalapon	3.251	0.000	483282	0	7.209	N.D. #
3) T	4-Nitroph...	11.433	0.000	9160790	0	139.833	N.D. #
8) T	DICHLORPROP	13.372	13.553	-807433	1275557	N.D.	31.498
12) T	2,4,5-T	0.000	15.848	0	700947	N.D.	4.228 #
13) T	2,4-DB	16.202	0.000	119274	0	5.736	N.D. #
14) T	DINOSEB	17.684	16.820	33666	258175	0.200	1.709 #
15) T	Picloram	17.462	18.236	582570	446586	1.778	1.874
16) T	DCPA	18.047	18.056	249421	175078	0.786	0.667



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032719\
Data File : PP029579.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 22:20
Operator : EI\MA
Sample : PB118241BL
Misc : hexane
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB118241BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 03:10:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

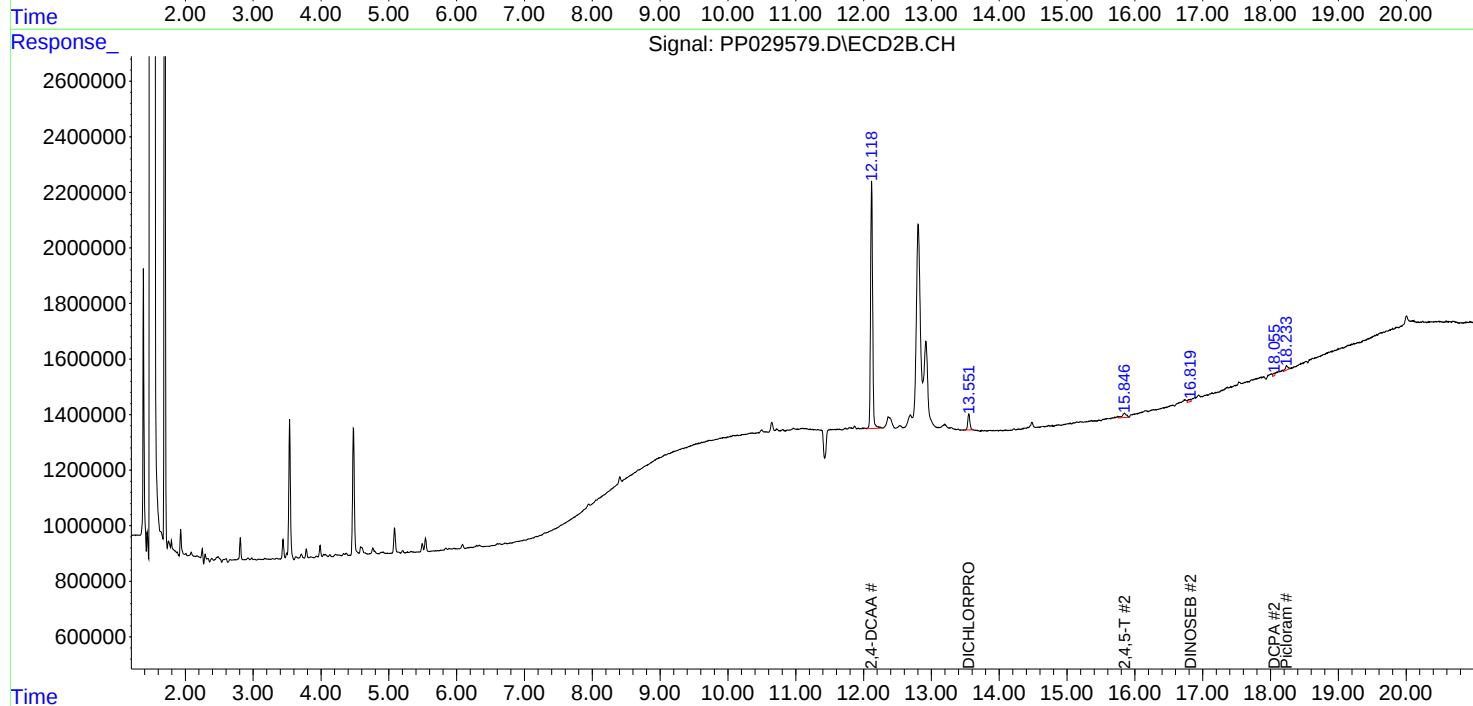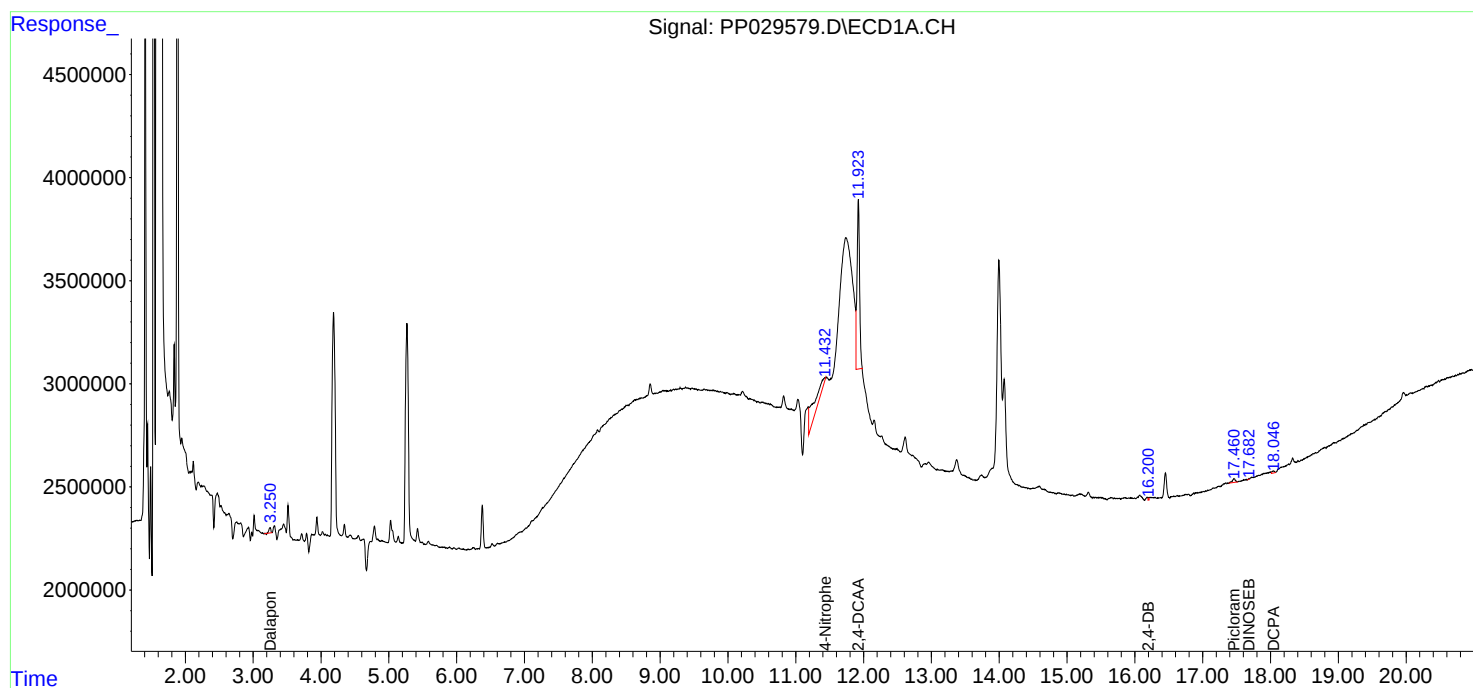


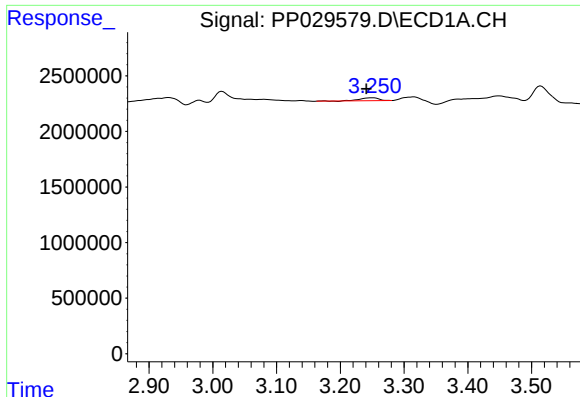

#1 Dalapon


R.T.: 3.251 min
Delta R.T.: 0.010 min
Response: 483282
Conc: 7.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118241BL

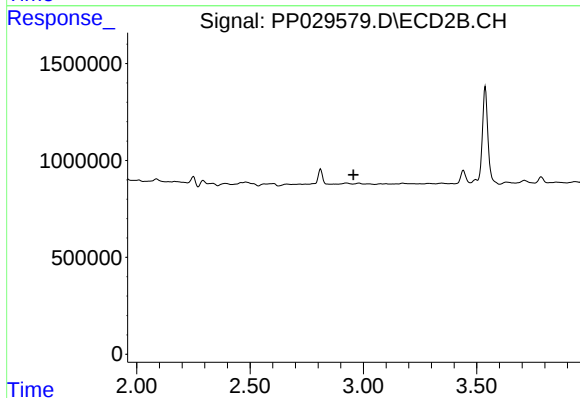


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.956 min
Response: 0
Conc: N.D.

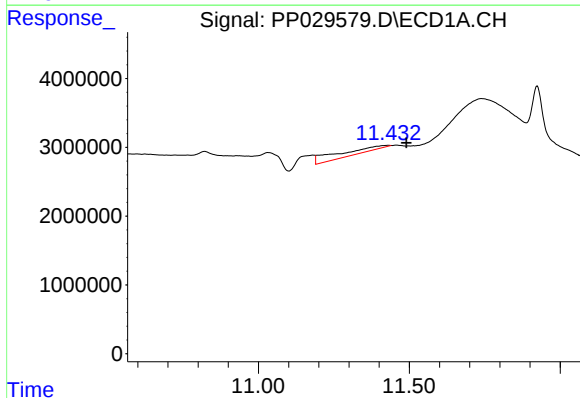


#3 4-Nitrophenol

R.T.: 11.433 min
Delta R.T.: -0.058 min
Response: 9160790
Conc: 139.83 ng/ml

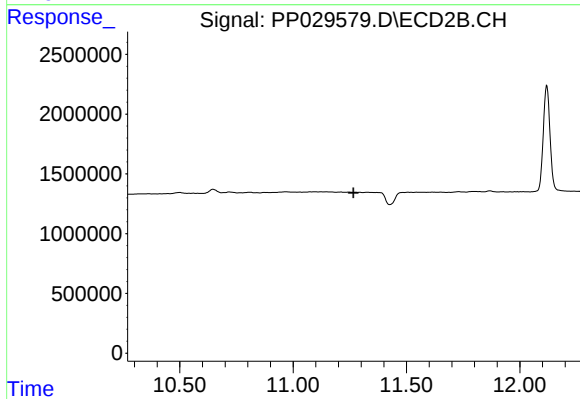

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 11.266 min
Response: 0
Conc: N.D.

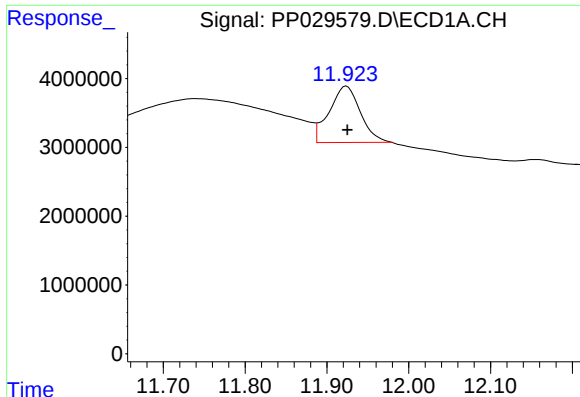

#4 2,4-DCAA


R.T.: 11.924 min
Delta R.T.: 0.000 min
Response: 21713009
Conc: 663.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118241BL

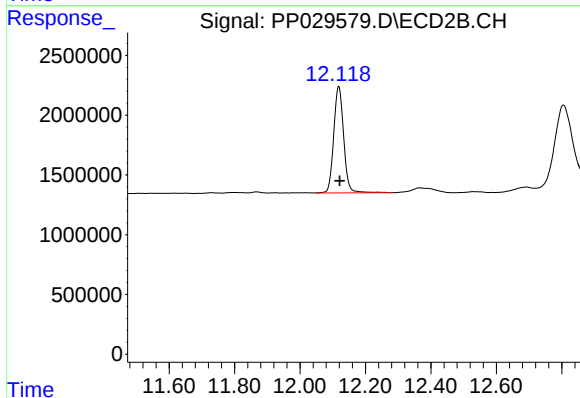


#4 2,4-DCAA

R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 18806669
Conc: 437.96 ng/ml

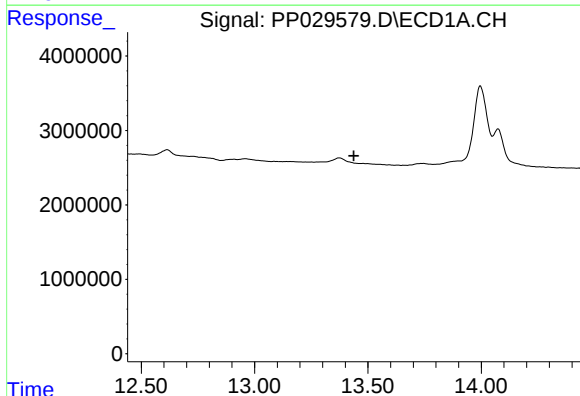


#8 DICHLORPROP

R.T.: 13.372 min
Delta R.T.: -0.065 min
Response: -807433
Conc: N.D.

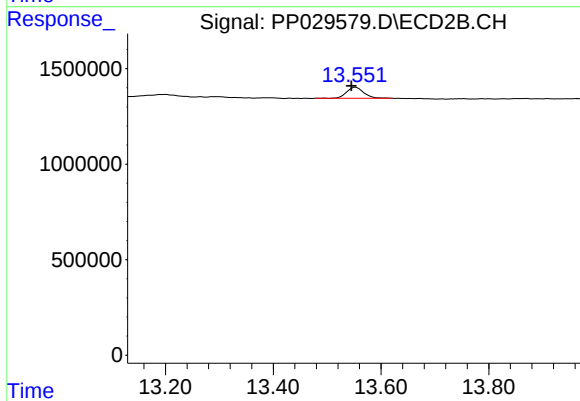

#8 DICHLORPROP


R.T.: 13.553 min
Delta R.T.: 0.008 min
Response: 1275557
Conc: 31.50 ng/ml

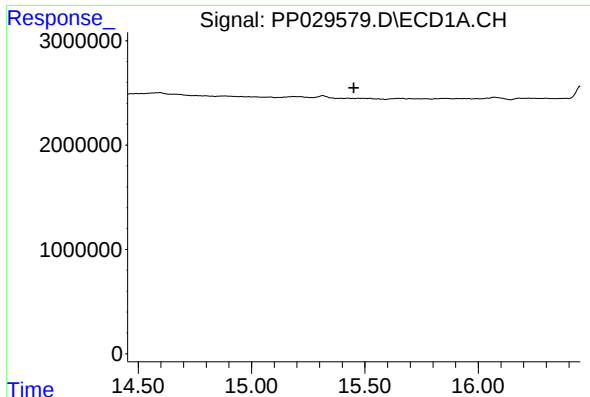

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB118241BL

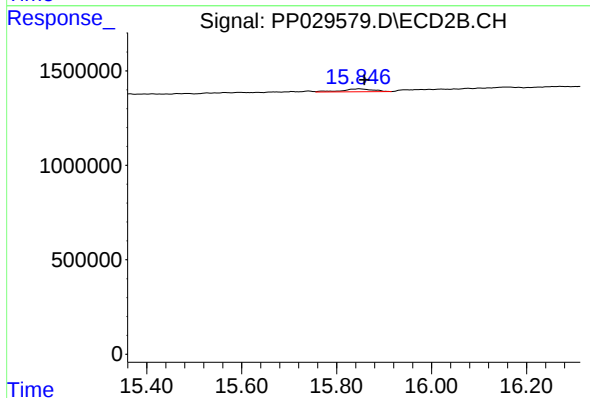


#12 2,4,5-T

R.T.: 15.848 min
Delta R.T.: -0.011 min
Response: 700947
Conc: 4.23 ng/ml

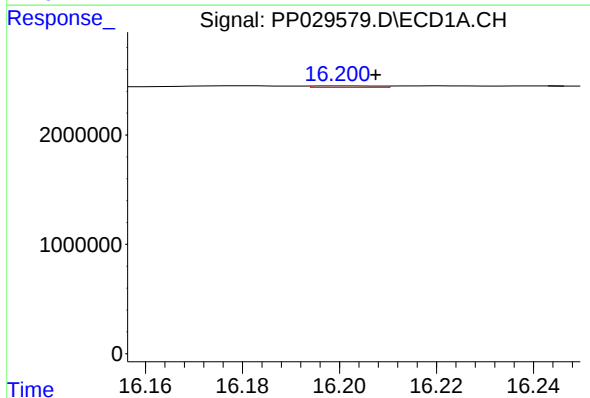


#13 2,4-DB

R.T.: 16.202 min
Delta R.T.: -0.006 min
Response: 119274
Conc: 5.74 ng/ml

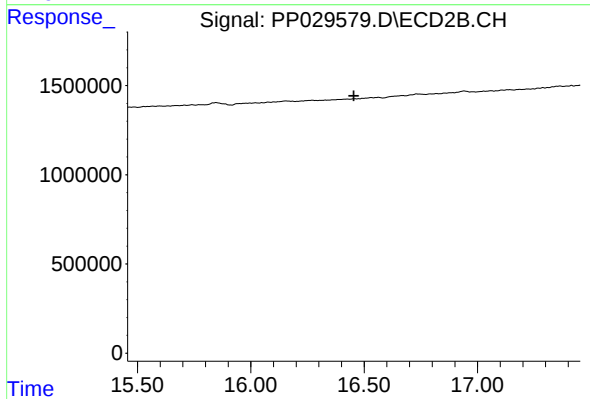

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.455 min
Response: 0
Conc: N.D.

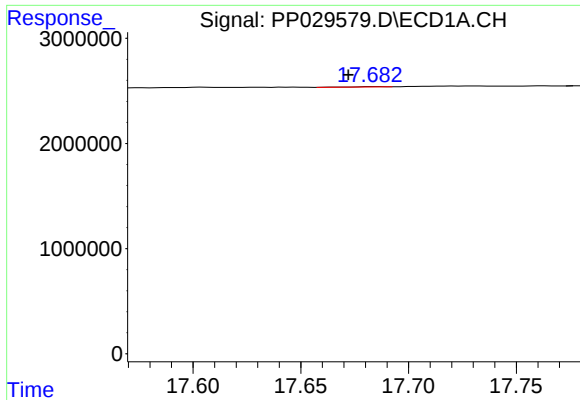

#14 DINOSEB


R.T.: 17.684 min
Delta R.T.: 0.012 min
Response: 33666
Conc: 0.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118241BL

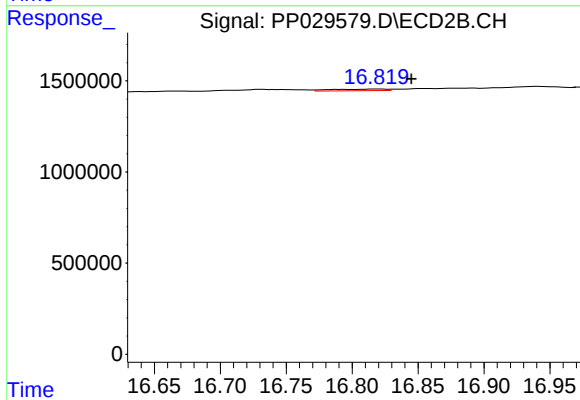


#14 DINOSEB

R.T.: 16.820 min
Delta R.T.: -0.025 min
Response: 258175
Conc: 1.71 ng/ml

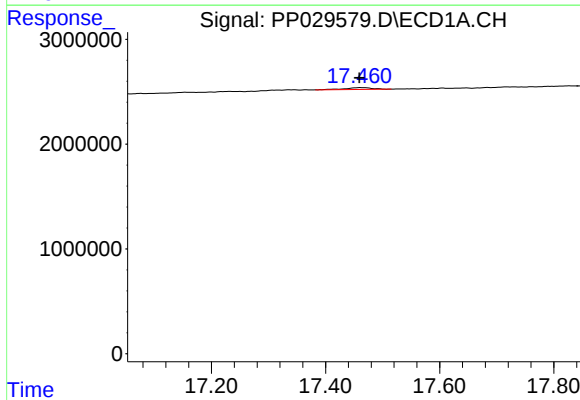


#15 Picloram

R.T.: 17.462 min
Delta R.T.: 0.002 min
Response: 582570
Conc: 1.78 ng/ml

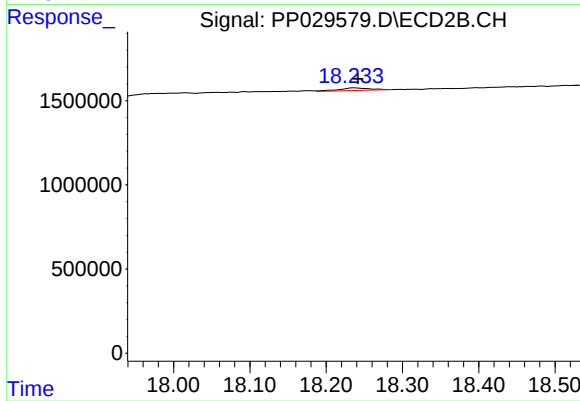

#15 Picloram


R.T.: 18.236 min
Delta R.T.: -0.006 min
Response: 446586
Conc: 1.87 ng/ml

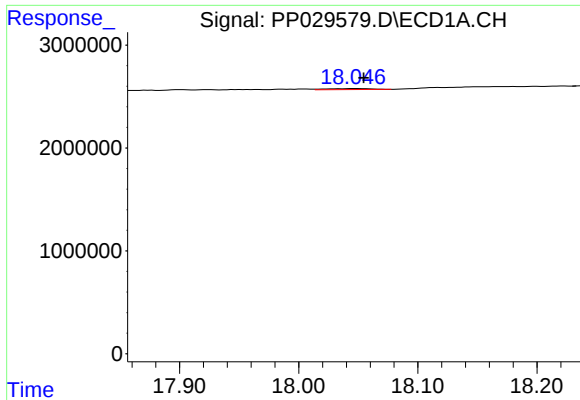

#16 DCPA

R.T.: 18.047 min
Delta R.T.: -0.008 min
Response: 249421
Conc: 0.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118241BL

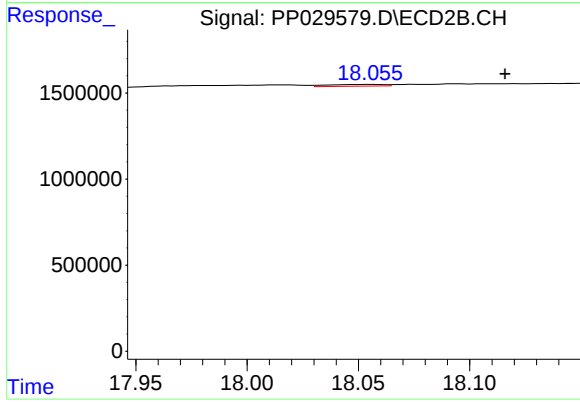

#16 DCPA

R.T.: 18.056 min
Delta R.T.: -0.060 min
Response: 175078
Conc: 0.67 ng/ml