

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032819\
 Data File : PP029611.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 19:16
 Operator : EI\MA
 Sample : PB118377TB
 Misc : hexane
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:06:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	11.924	12.119	24444258	22734945	747.188	529.442	#
Target Compounds								
3) T	4-Nitroph...	11.428	0.000	10169861	0	155.235	N.D.	#
5) T	DICAMBA	12.223	0.000	505246	0	3.419	N.D.	#
8) T	DICHLORPROP	13.373	13.552	132534	1588248	3.872	39.219	#
11) T	2,4,5-TP ...	0.000	15.143	0	237529	N.D.	1.148	#
12) T	2,4,5-T	0.000	15.864	0	453858	N.D.	2.738	#
13) T	2,4-DB	16.226	0.000	831144	0	39.971	N.D.	#
14) T	DINOSEB	17.673	0.000	46557	0	0.276	N.D.	#
15) T	Picloram	17.464	18.241	496825	2053415	1.516	8.615	#
16) T	DCPA	18.039	0.000	577016	0	1.819	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032819\
Data File : PP029611.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 19:16
Operator : EI\MA
Sample : PB118377TB
Misc : hexane
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:06:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

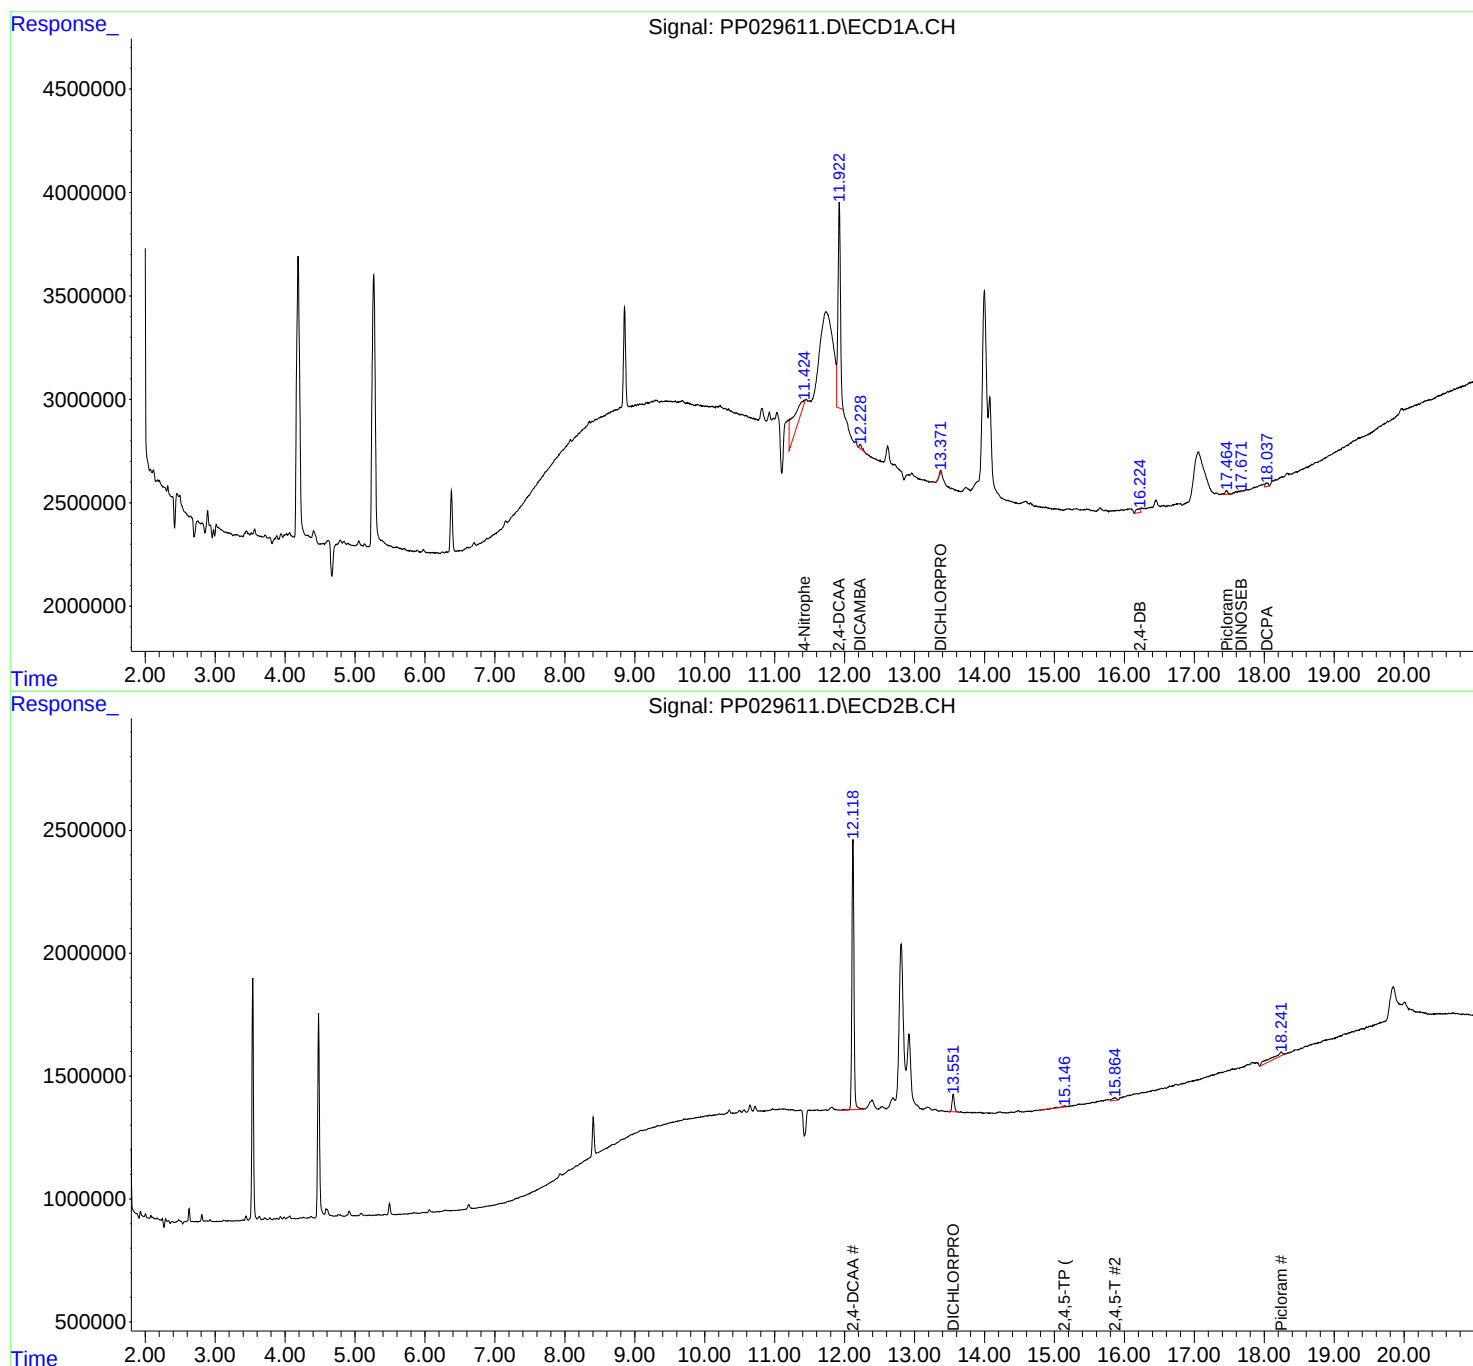


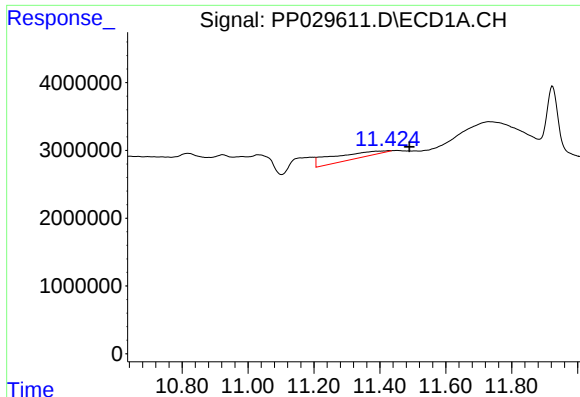

#3 4-Nitrophenol


R.T.: 11.428 min
Delta R.T.: -0.062 min
Response: 10169861
Conc: 155.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

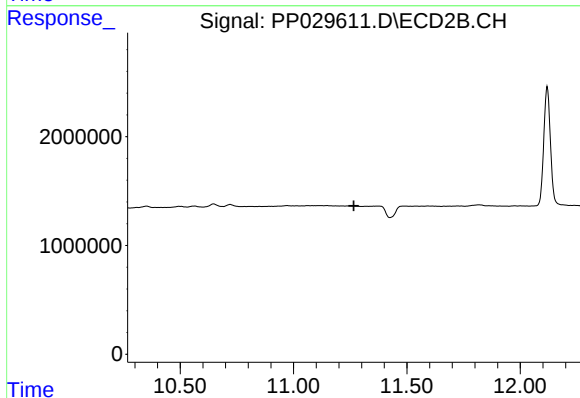


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.266 min
Response: 0
Conc: N.D.

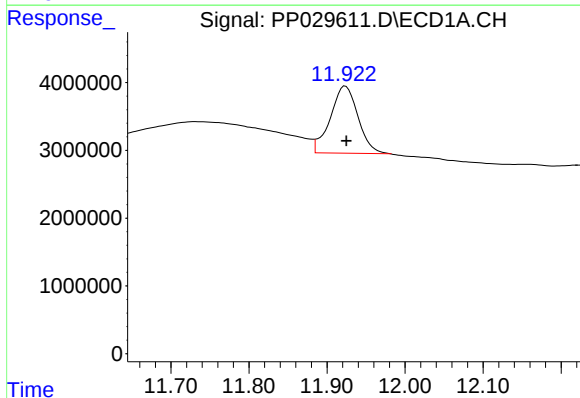


#4 2,4-DCAA

R.T.: 11.924 min
Delta R.T.: -0.001 min
Response: 24444258
Conc: 747.19 ng/ml

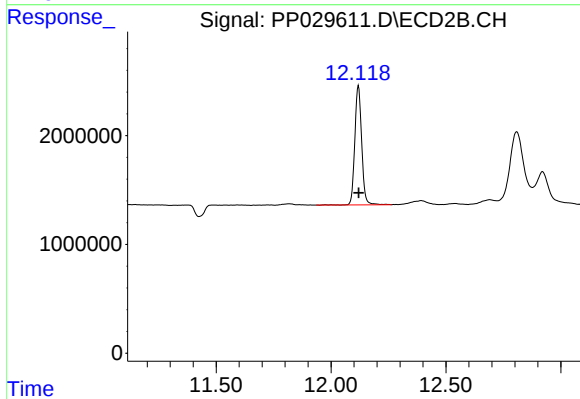

#4 2,4-DCAA


R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 22734945
Conc: 529.44 ng/ml

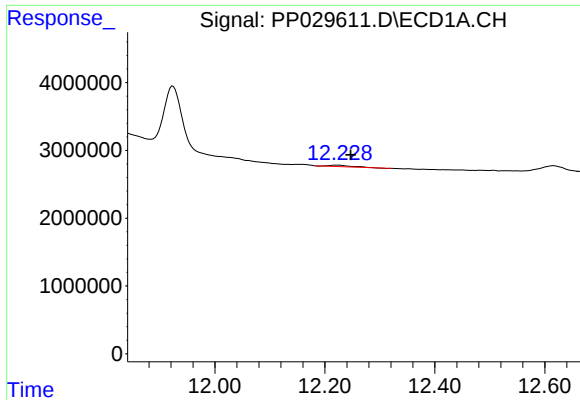

#5 DICAMBA


R.T.: 12.223 min
Delta R.T.: -0.025 min
Response: 505246
Conc: 3.42 ng/ml

Instrument :
ECD_P
ClientSampleId :

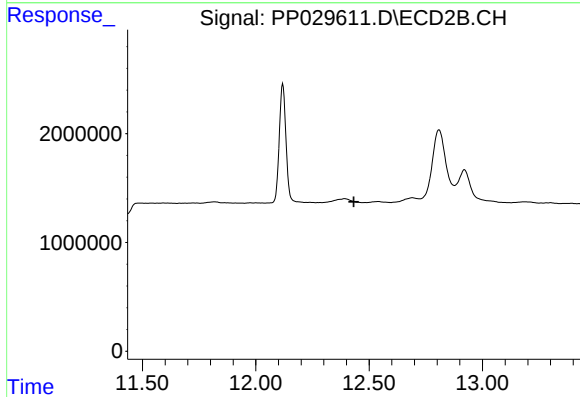


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 12.433 min
Response: 0
Conc: N.D.

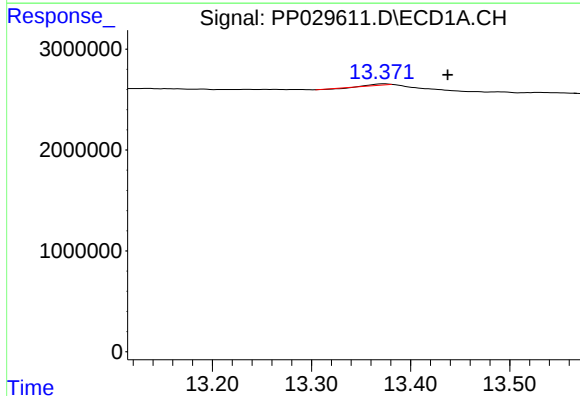


#8 DICHLORPROP

R.T.: 13.373 min
Delta R.T.: -0.064 min
Response: 132534
Conc: 3.87 ng/ml

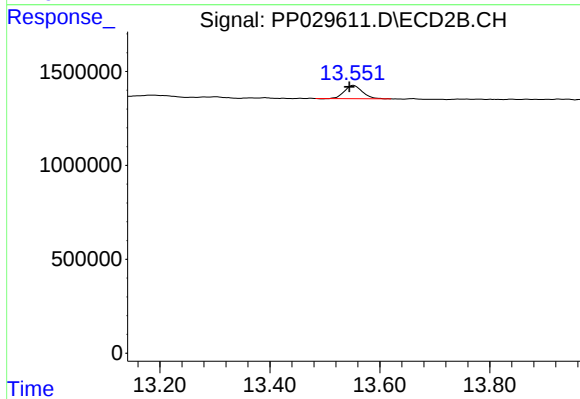

#8 DICHLORPROP


R.T.: 13.552 min
Delta R.T.: 0.007 min
Response: 1588248
Conc: 39.22 ng/ml

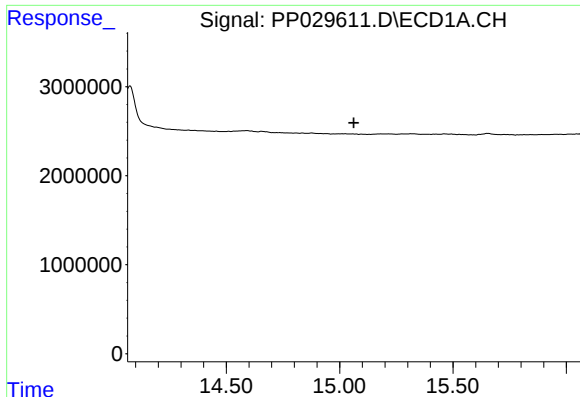

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

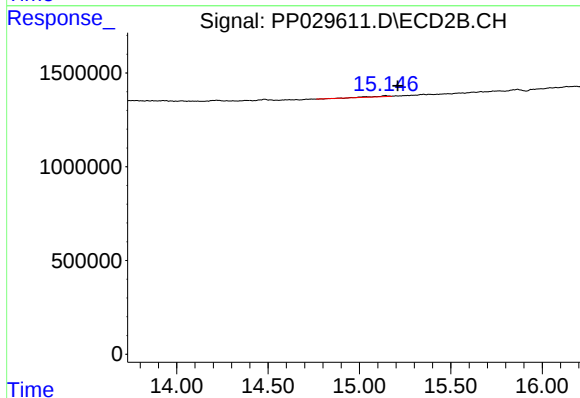


#11 2,4,5-TP (SILVEX)

R.T.: 15.143 min
Delta R.T.: -0.067 min
Response: 237529
Conc: 1.15 ng/ml

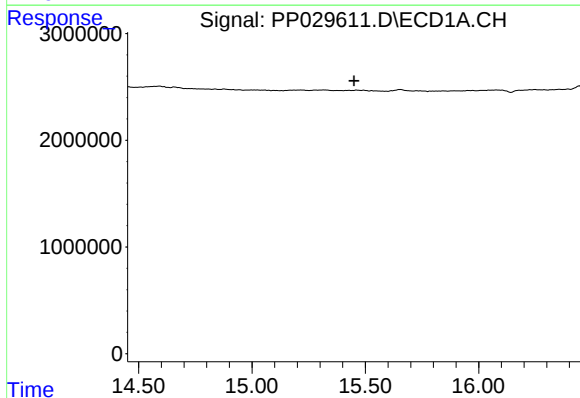


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

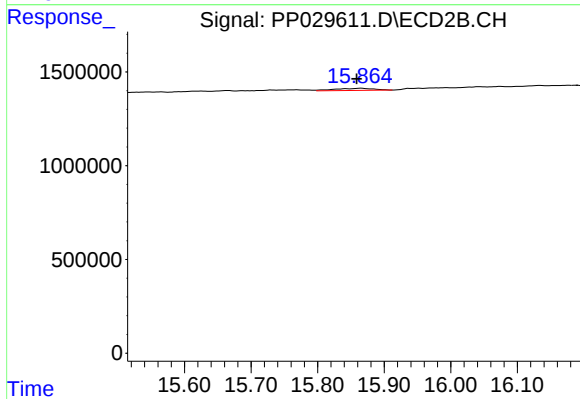

#12 2,4,5-T


R.T.: 15.864 min
Delta R.T.: 0.006 min
Response: 453858
Conc: 2.74 ng/ml

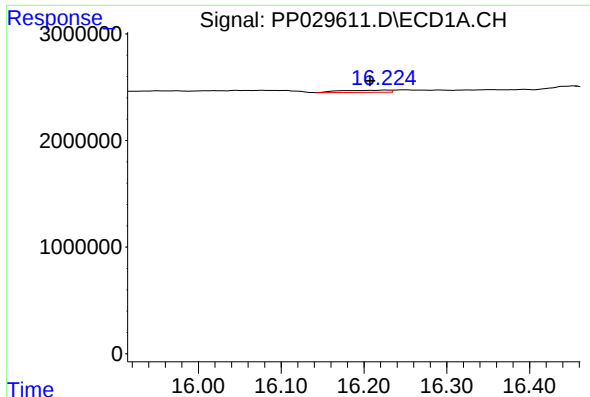

#13 2,4-DB


R.T.: 16.226 min
Delta R.T.: 0.019 min
Response: 831144
Conc: 39.97 ng/ml

Instrument :
ECD_P
ClientSampleId :

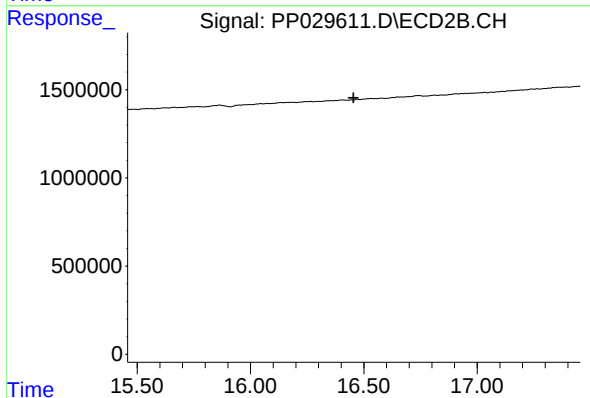


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

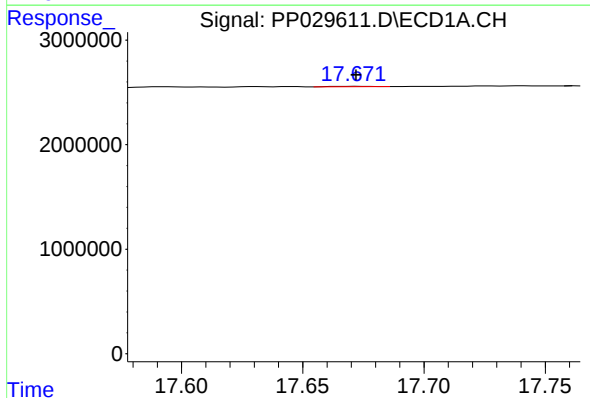


#14 DINOSEB

R.T.: 17.673 min
Delta R.T.: 0.001 min
Response: 46557
Conc: 0.28 ng/ml

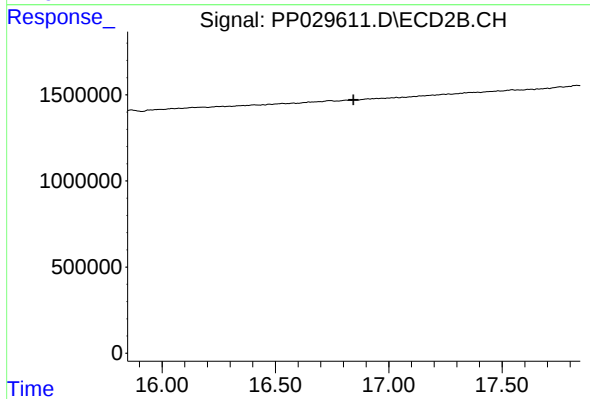

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.845 min
Response: 0
Conc: N.D.

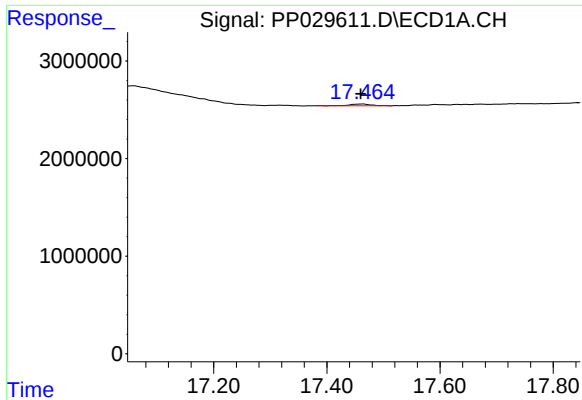

#15 Picloram


R.T.: 17.464 min
Delta R.T.: 0.004 min
Response: 496825
Conc: 1.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

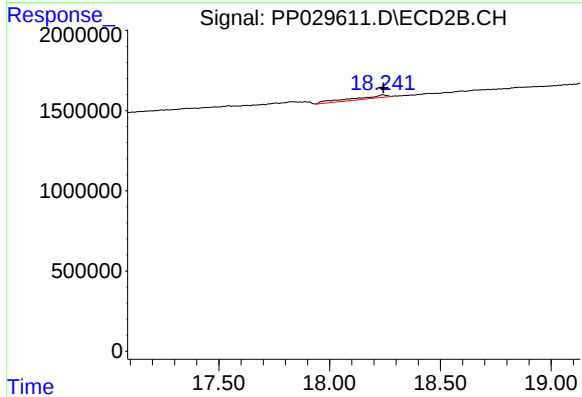


#15 Picloram

R.T.: 18.241 min
Delta R.T.: -0.001 min
Response: 2053415
Conc: 8.62 ng/ml

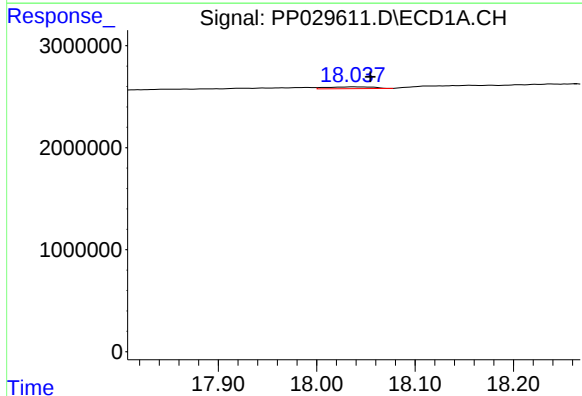

#16 DCPA

R.T.: 18.039 min
Delta R.T.: -0.016 min
Response: 577016
Conc: 1.82 ng/ml

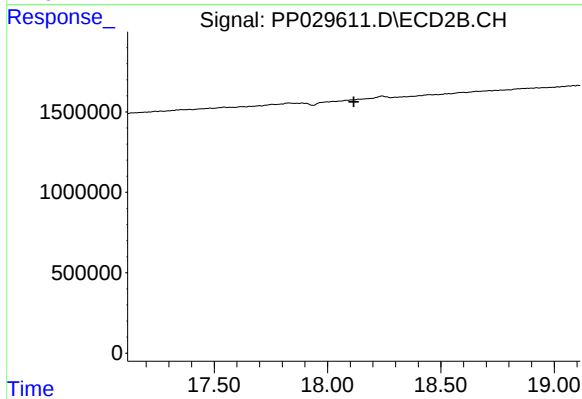

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.116 min
Response: 0
Conc: N.D.