

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032819\
 Data File : PP029622.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Mar 2019 23:57
 Operator : EI\MA
 Sample : K2107-12
 Misc : hexane
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:08:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.119	19558912	21182654	597.858	493.293
Target Compounds							
3) T	4-Nitroph...	11.424	0.000	86549	0	1.321	N.D. #
5) T	DICAMBA	12.227	0.000	458414	0	3.102	N.D. #
8) T	DICHLORPROP	0.000	13.553	0	786457	N.D.	19.420 #
11) T	2,4,5-TP ...	0.000	15.140	0	147046	N.D.	0.710 #
12) T	2,4,5-T	0.000	15.850	0	875772	N.D.	5.283 #
13) T	2,4-DB	16.189	0.000	576674	0	27.733	N.D. #
14) T	DINOSEB	17.667	16.868	70426	121623	0.418	0.805 #
15) T	Picloram	17.461	18.245	184607	73976	0.563	0.310 #
16) T	DCPA	18.049	18.109	517917	308079	1.632	1.174 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032819\
Data File : PP029622.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Mar 2019 23:57
Operator : EI\MA
Sample : K2107-12
Misc : hexane
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:08:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

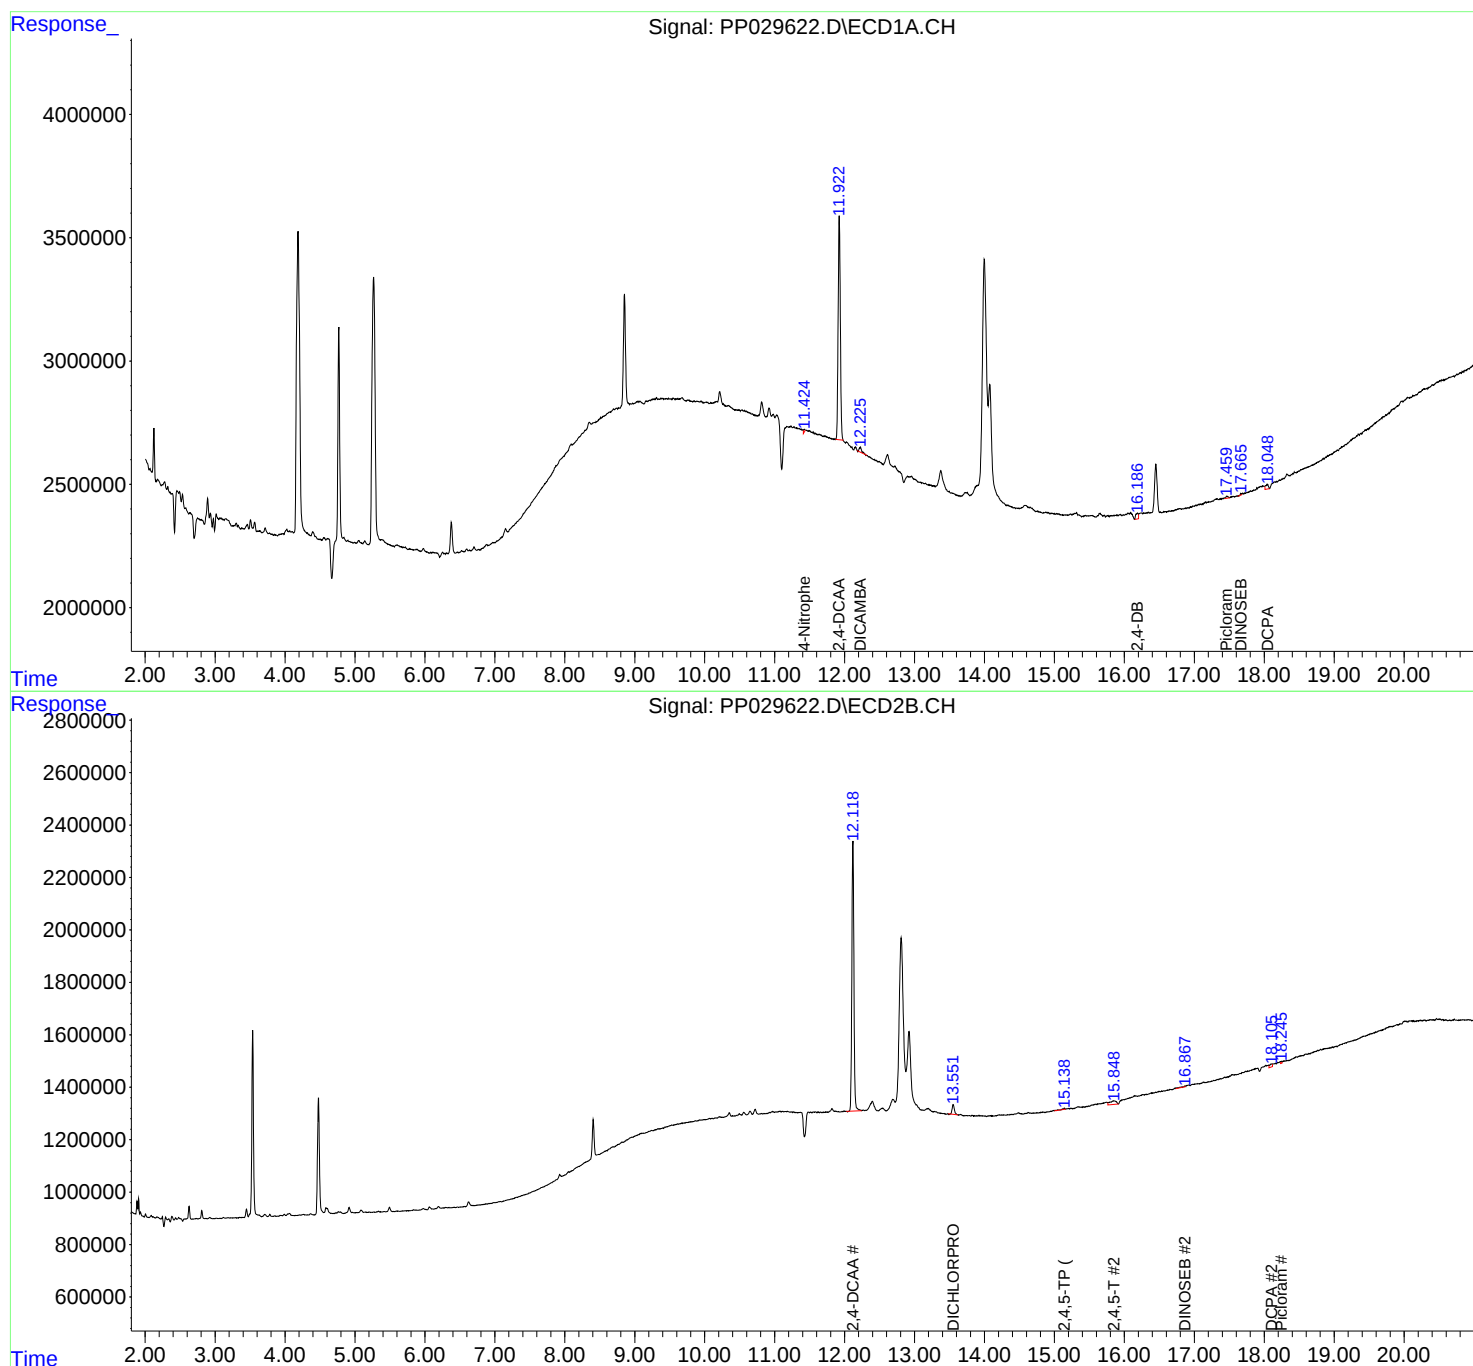


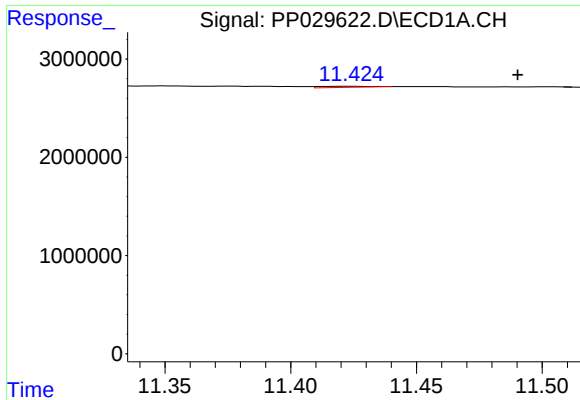

#3 4-Nitrophenol


R.T.: 11.424 min
Delta R.T.: -0.066 min
Response: 86549
Conc: 1.32 ng/ml

Instrument :
ECD_P
ClientSampleId :

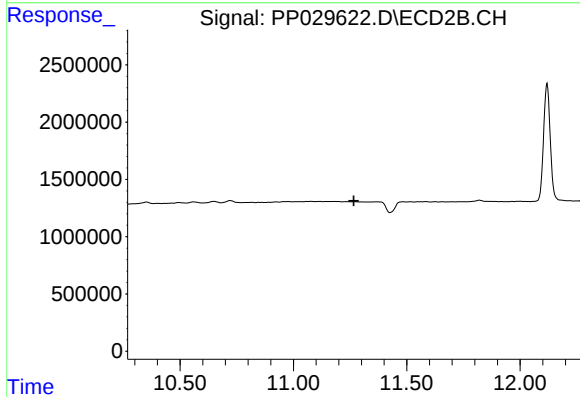


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.266 min
Response: 0
Conc: N.D.

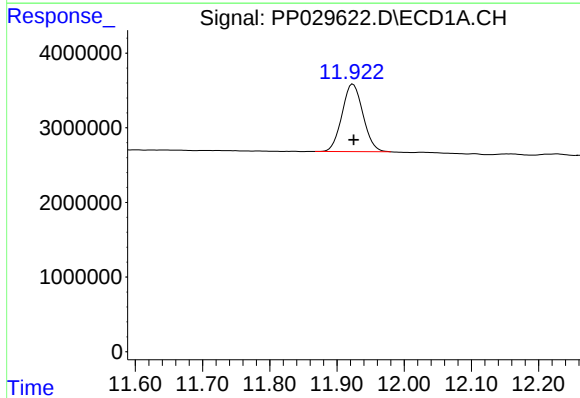


#4 2,4-DCAA

R.T.: 11.924 min
Delta R.T.: -0.001 min
Response: 19558912
Conc: 597.86 ng/ml

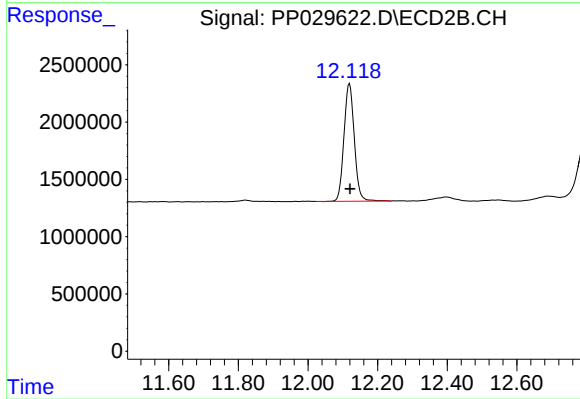

#4 2,4-DCAA


R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 21182654
Conc: 493.29 ng/ml

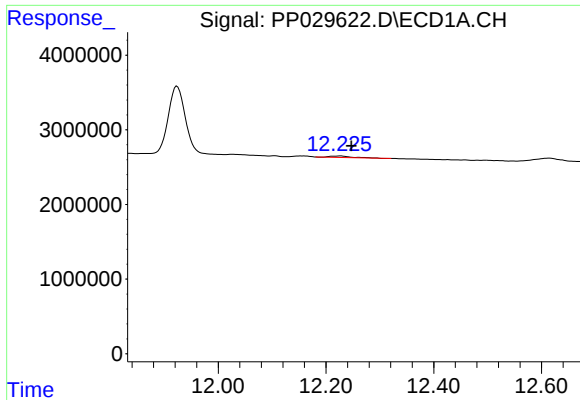

#5 DICAMBA


R.T.: 12.227 min
Delta R.T.: -0.020 min
Response: 458414
Conc: 3.10 ng/ml

Instrument :
ECD_P
ClientSampleId :

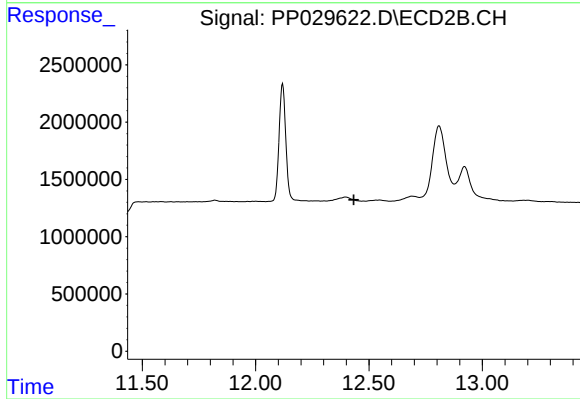


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.433 min
Response: 0
Conc: N.D.

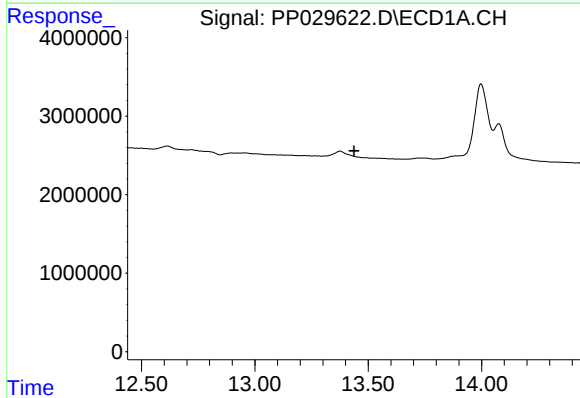


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.438 min
Response: 0
Conc: N.D.

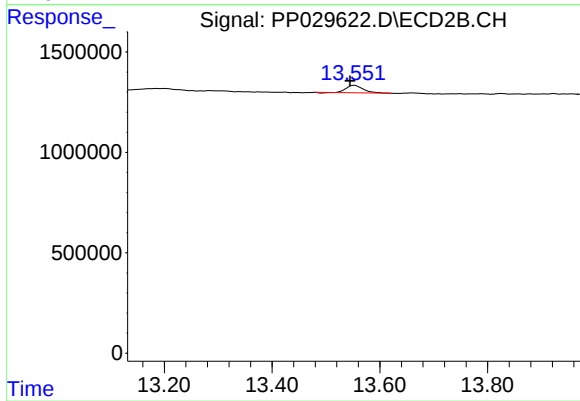

#8 DICHLORPROP


R.T.: 13.553 min
Delta R.T.: 0.008 min
Response: 786457
Conc: 19.42 ng/ml

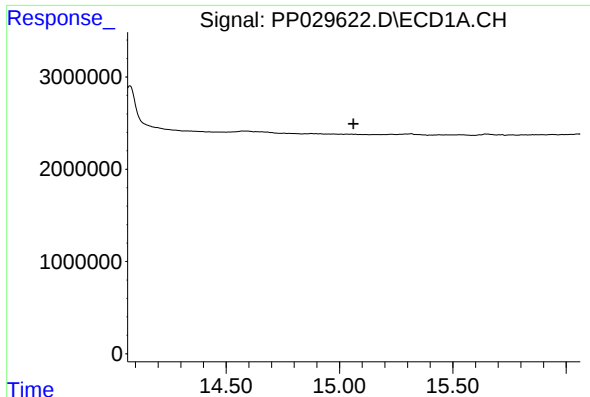

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

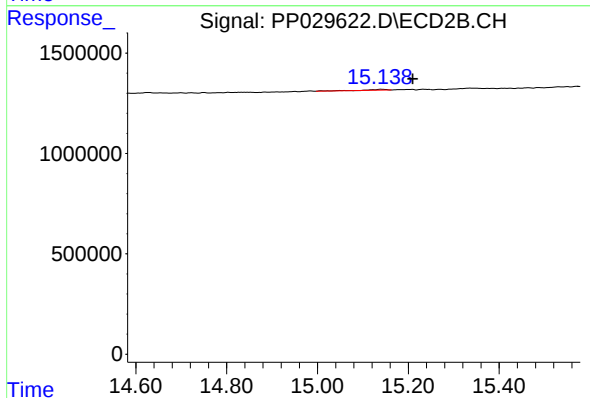


#11 2,4,5-TP (SILVEX)

R.T.: 15.140 min
Delta R.T.: -0.070 min
Response: 147046
Conc: 0.71 ng/ml

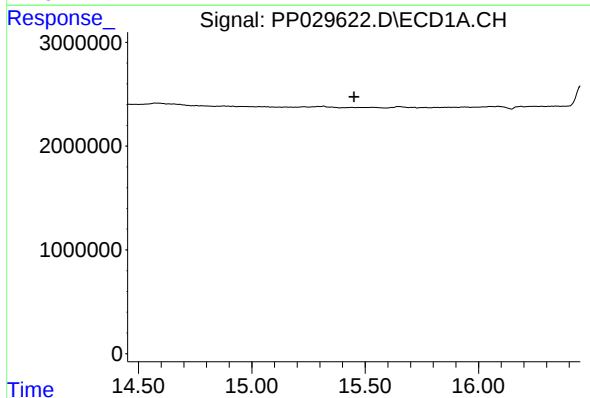


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

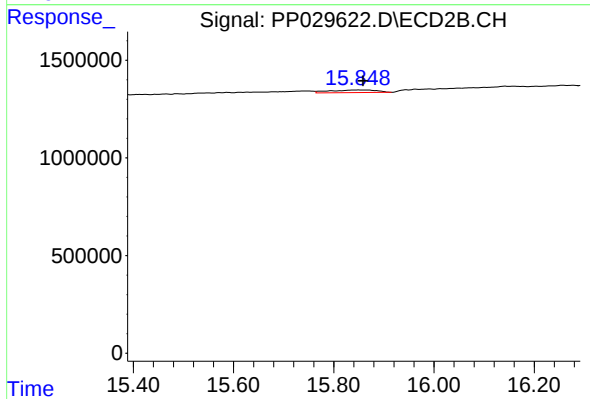

#12 2,4,5-T


R.T.: 15.850 min
Delta R.T.: -0.008 min
Response: 875772
Conc: 5.28 ng/ml

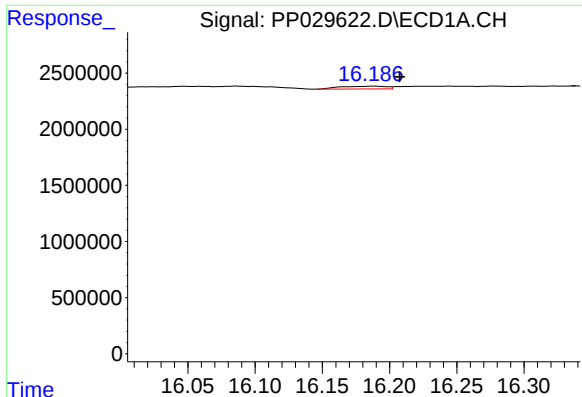

#13 2,4-DB


R.T.: 16.189 min
Delta R.T.: -0.019 min
Response: 576674
Conc: 27.73 ng/ml

Instrument :
ECD_P
ClientSampleId :

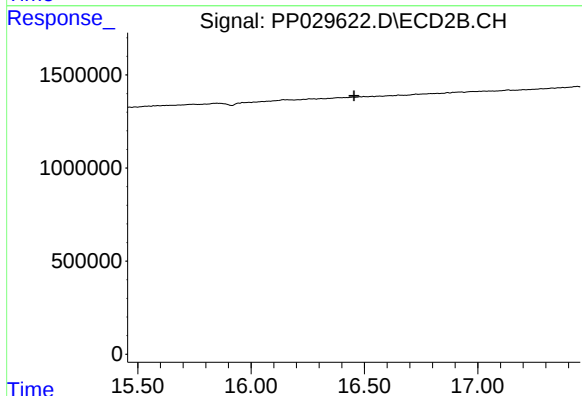


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

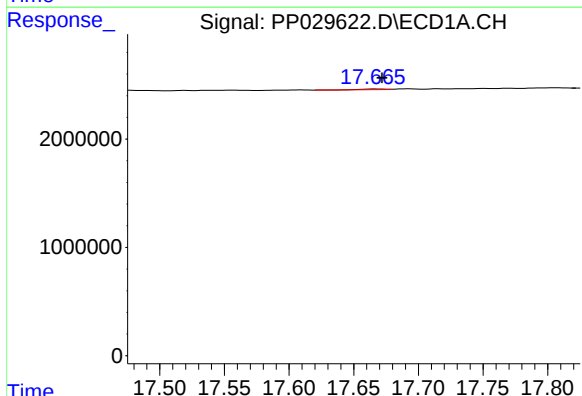


#14 DINOSEB

R.T.: 17.667 min
Delta R.T.: -0.005 min
Response: 70426
Conc: 0.42 ng/ml

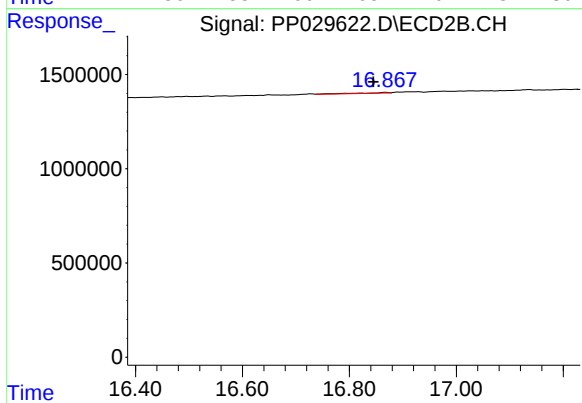

#14 DINOSEB


R.T.: 16.868 min
Delta R.T.: 0.023 min
Response: 121623
Conc: 0.81 ng/ml

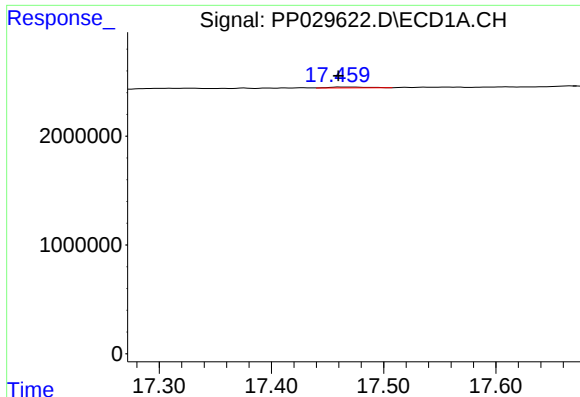

#15 Picloram


R.T.: 17.461 min
Delta R.T.: 0.001 min
Response: 184607
Conc: 0.56 ng/ml

Instrument :
ECD_P
ClientSampleId :

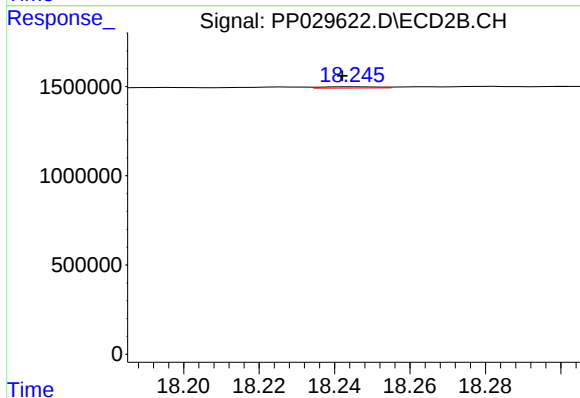


#15 Picloram

R.T.: 18.245 min
Delta R.T.: 0.003 min
Response: 73976
Conc: 0.31 ng/ml

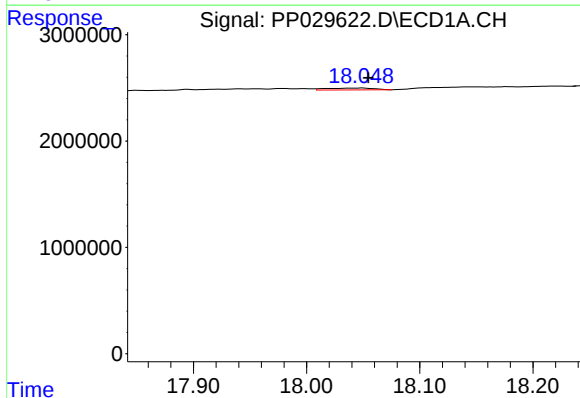

#16 DCPA

R.T.: 18.049 min
Delta R.T.: -0.005 min
Response: 517917
Conc: 1.63 ng/ml

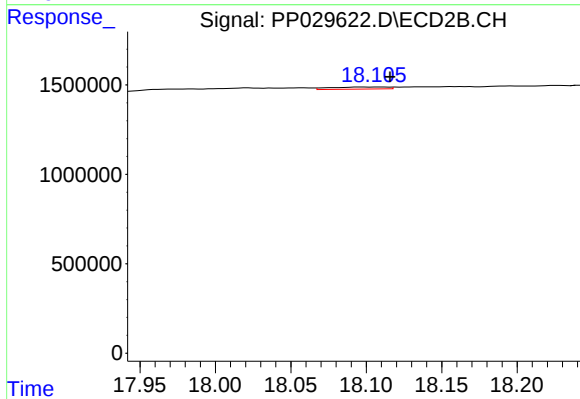

#16 DCPA

R.T.: 18.109 min
Delta R.T.: -0.007 min
Response: 308079
Conc: 1.17 ng/ml