

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032825\
 Data File : PP070956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2025 09:50
 Operator : YP\AJ
 Sample : Q1648-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/28/2025
 Supervised By :mohammad ahmed 04/02/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 11:00:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.514	3.816	26771513	21160232	18.317m	20.412
2) SA Decachlor...	10.228	8.858	12882212	8875108	12.238	11.260

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032825\
Data File : PP070956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2025 09:50
Operator : YP\AJ
Sample : Q1648-07
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2025
Supervised By :mohammad ahmed 04/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 11:00:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

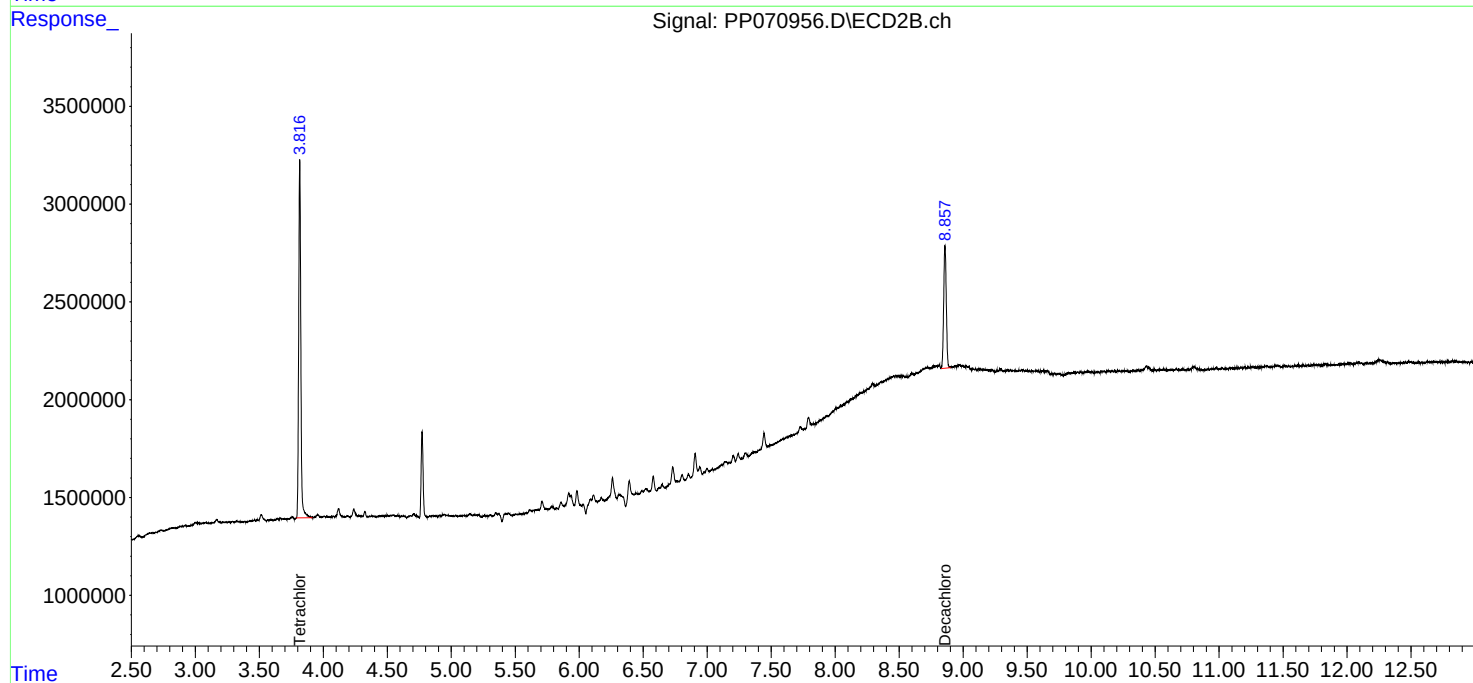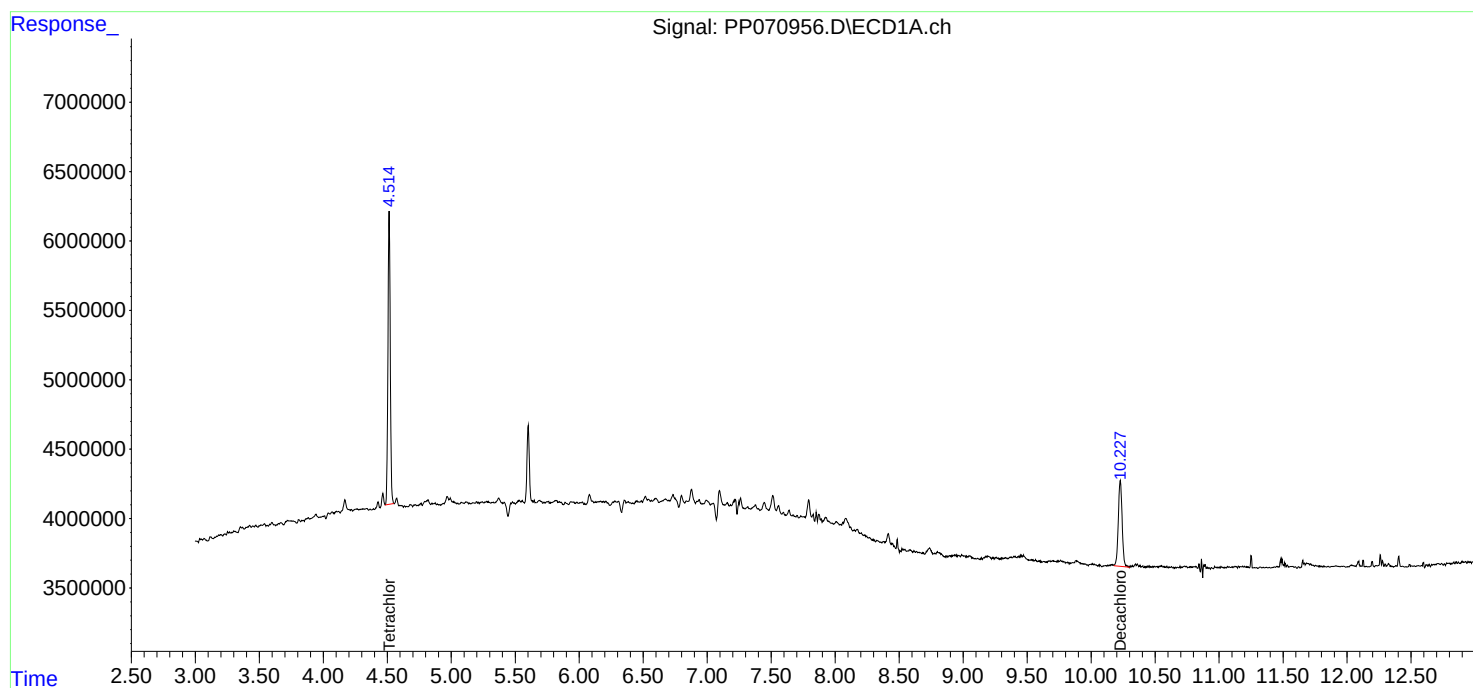

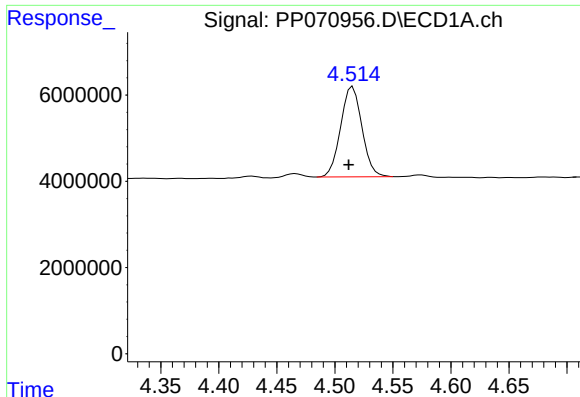


#1 Tetrachloro-m-xylene

R.T.: 4.514 min
Delta R.T.: 0.002 min
Response: 26771513
Conc: 18.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2025
Supervised By :mohammad ahmed 04/02/2025

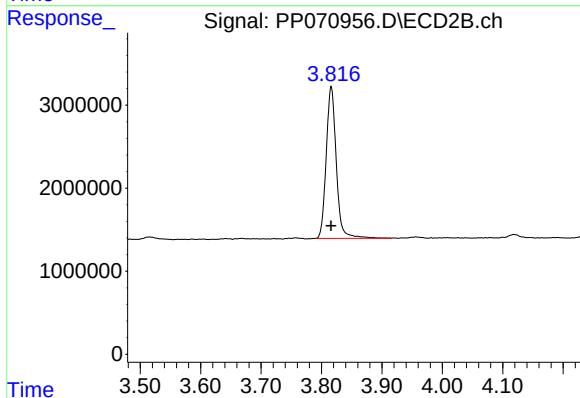


#1 Tetrachloro-m-xylene

R.T.: 3.816 min
Delta R.T.: 0.000 min
Response: 21160232
Conc: 20.41 ng/ml

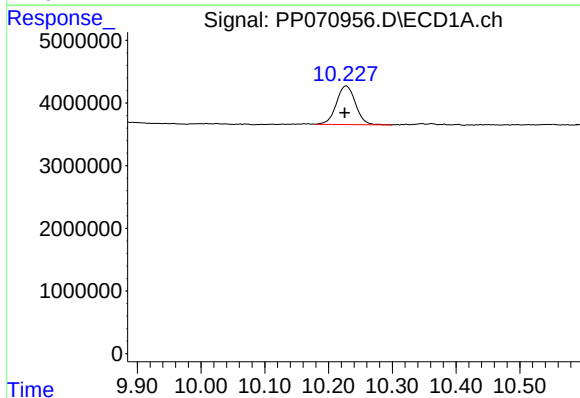

#2 Decachlorobiphenyl

R.T.: 10.228 min
Delta R.T.: 0.003 min
Response: 12882212
Conc: 12.24 ng/ml

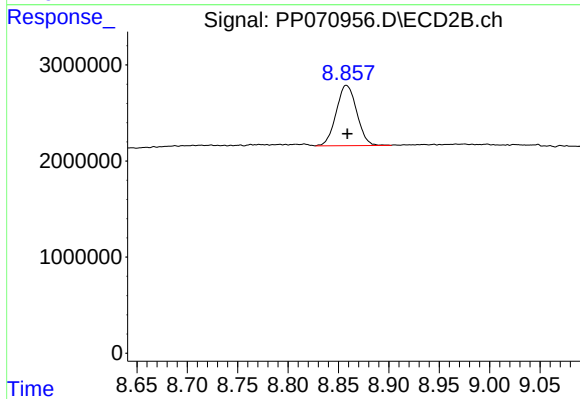

#2 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 8875108
Conc: 11.26 ng/ml