

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032825\
 Data File : PP070964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2025 12:00
 Operator : YP\AJ
 Sample : Q1650-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 STOCK-PILE-BIN2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/31/2025
 Supervised By :mohammad ahmed 04/02/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 12:40:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.515	3.816	27488237	22623669	18.807m	21.824
2) SA Decachlor...	10.234	8.858	22000315	14737398	20.901	18.698

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032825\
Data File : PP070964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2025 12:00
Operator : YP\AJ
Sample : Q1650-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
STOCK-PILE-BIN2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/31/2025
Supervised By :mohammad ahmed 04/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 12:40:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

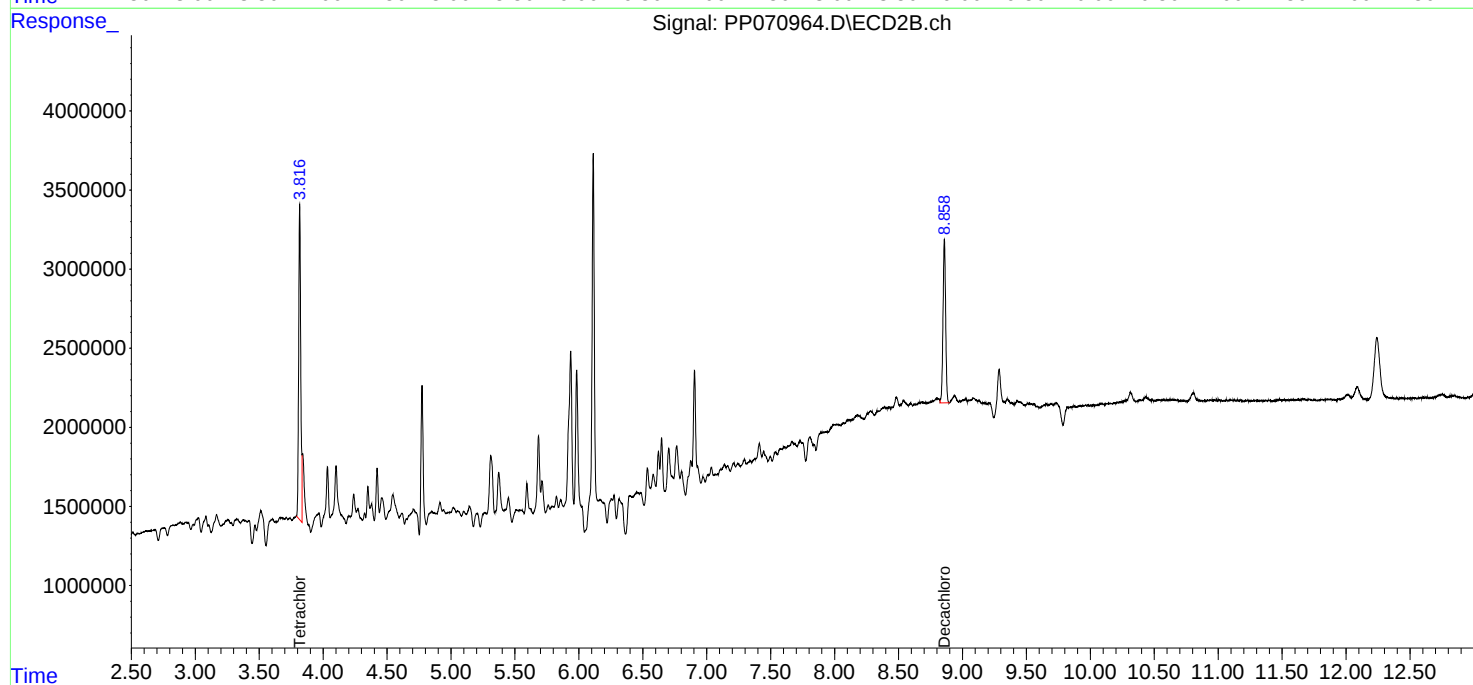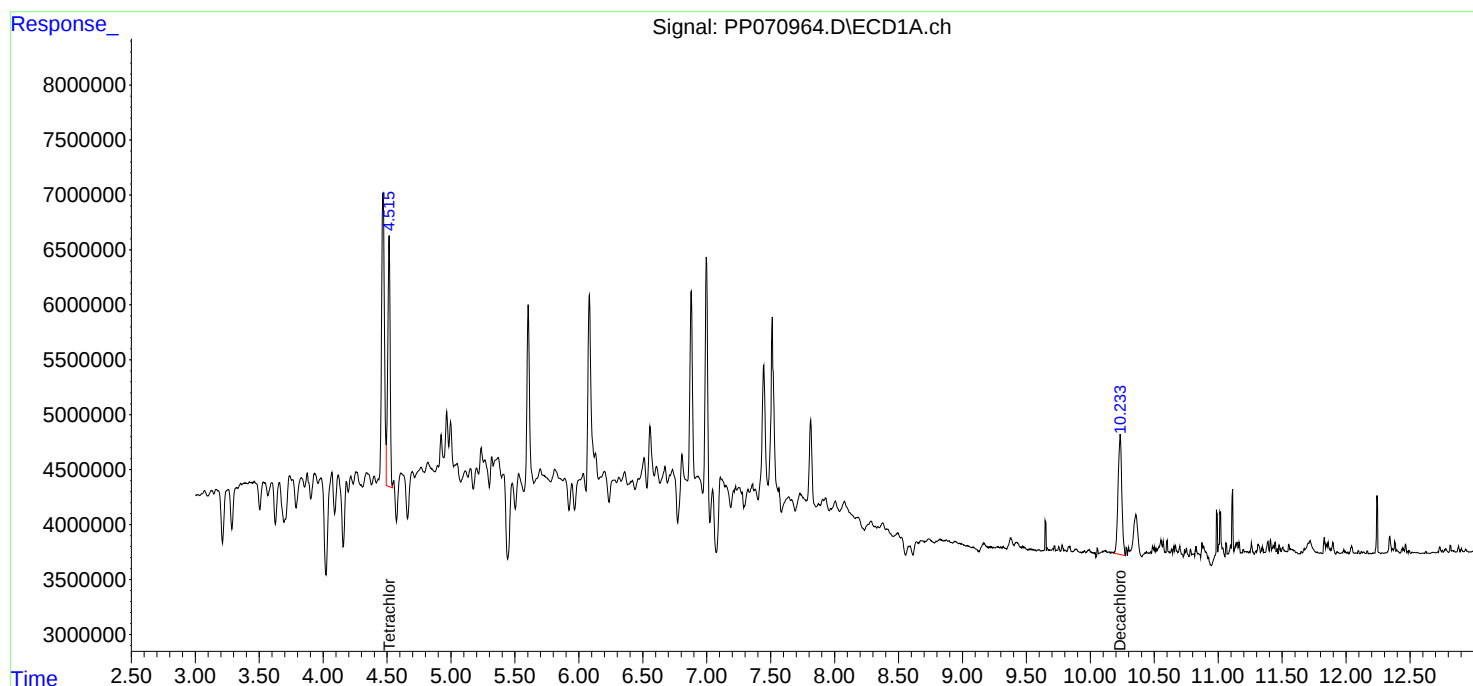

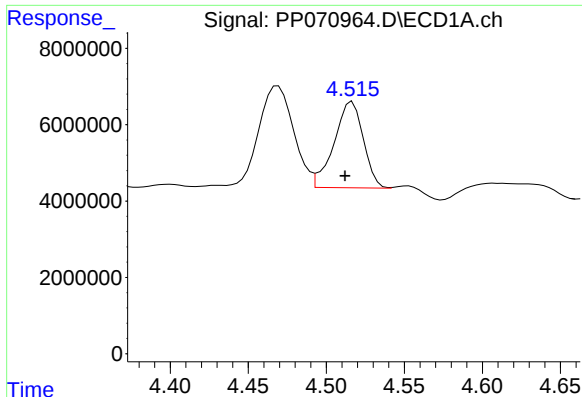


#1 Tetrachloro-m-xylene

R.T.: 4.515 min
Delta R.T.: 0.003 min
Response: 27488237
Conc: 18.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
STOCK-PILE-BIN2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/31/2025
Supervised By :mohammad ahmed 04/02/2025

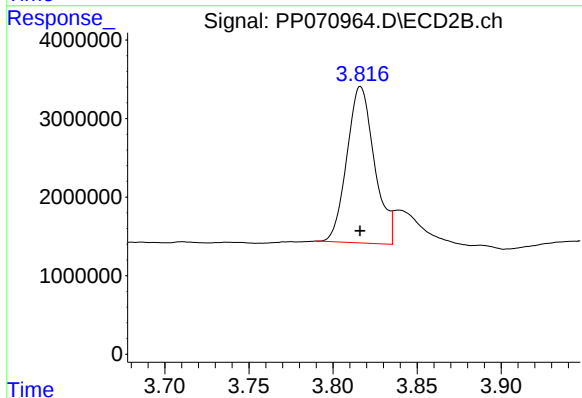


#1 Tetrachloro-m-xylene

R.T.: 3.816 min
Delta R.T.: 0.000 min
Response: 22623669
Conc: 21.82 ng/ml

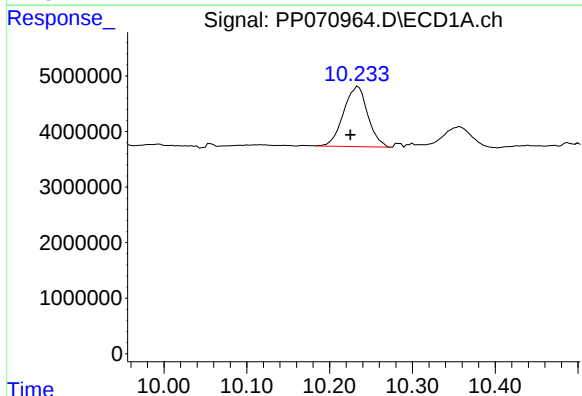

#2 Decachlorobiphenyl

R.T.: 10.234 min
Delta R.T.: 0.009 min
Response: 22000315
Conc: 20.90 ng/ml

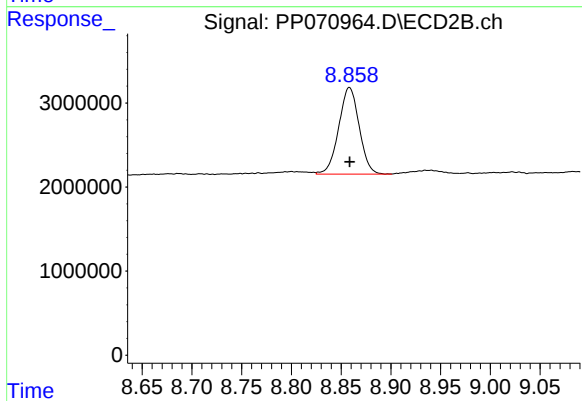

#2 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 14737398
Conc: 18.70 ng/ml