

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032825\
 Data File : PP070992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2025 22:08
 Operator : YP\AJ
 Sample : Q1663-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 0324-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/31/2025
 Supervised By :mohammad ahmed 04/02/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 01:02:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.522	3.816	31267016	21938249	21.393	21.163
2) SA Decachlor...	10.245	8.859	24893056	15776668	23.649m	20.016

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032825\
Data File : PP070992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2025 22:08
Operator : YP\AJ
Sample : Q1663-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
0324-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/31/2025
Supervised By :mohammad ahmed 04/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 01:02:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

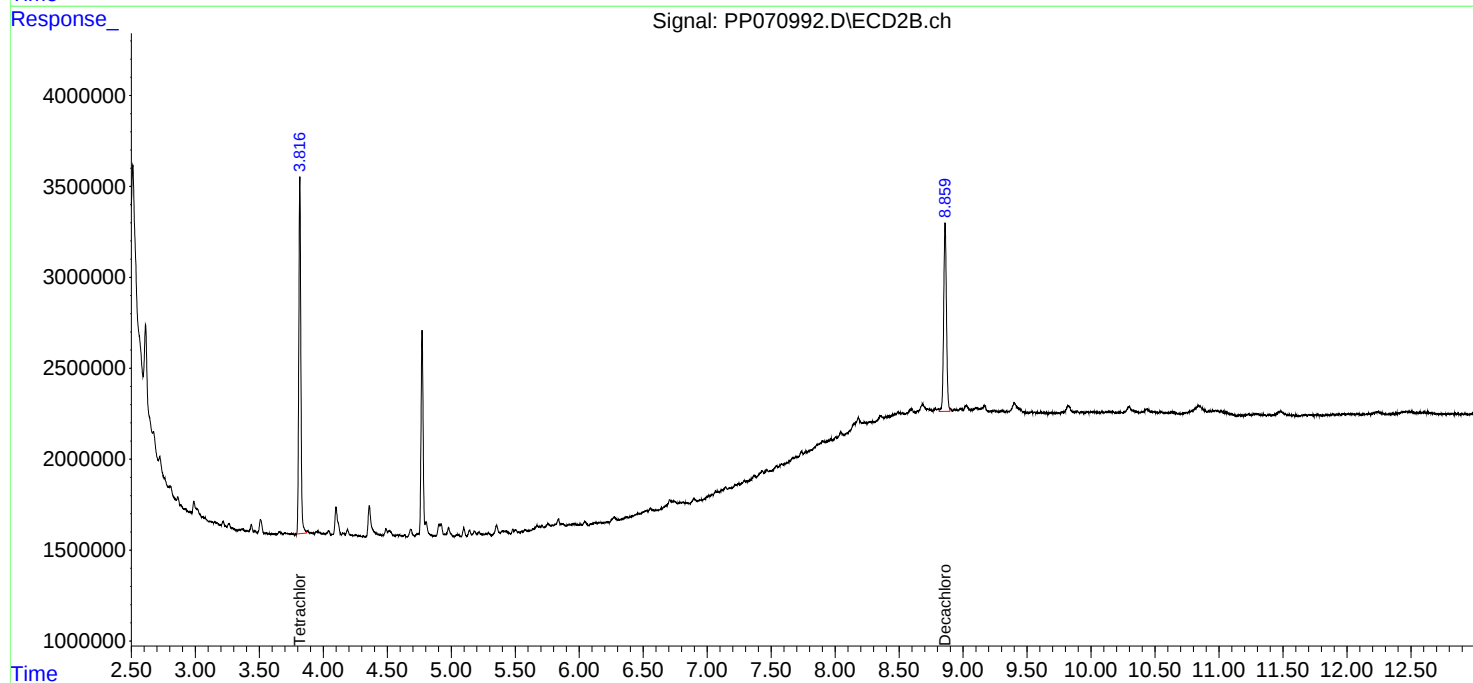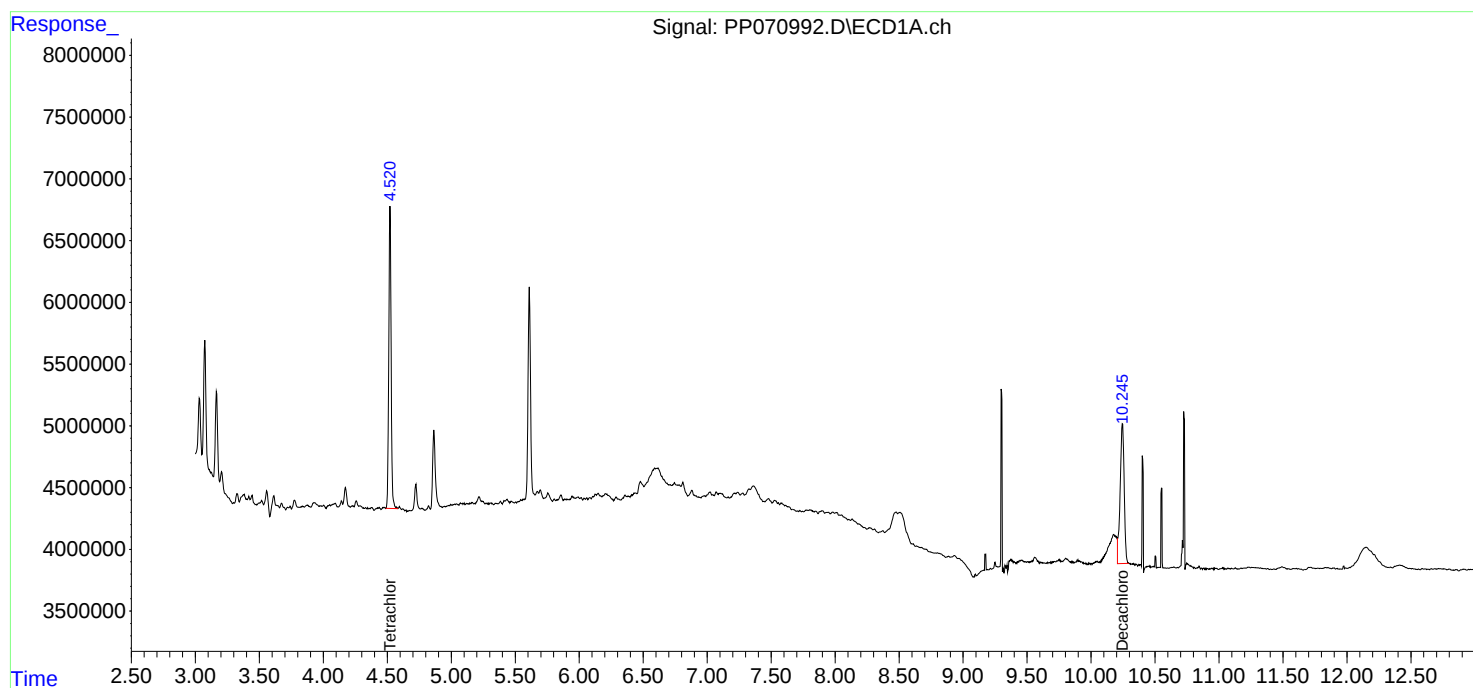

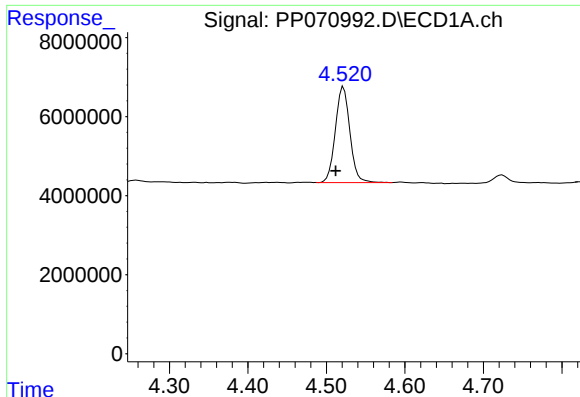


#1 Tetrachloro-m-xylene

R.T.: 4.522 min
Delta R.T.: 0.010 min
Response: 31267016
Conc: 21.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
0324-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/31/2025
Supervised By :mohammad ahmed 04/02/2025

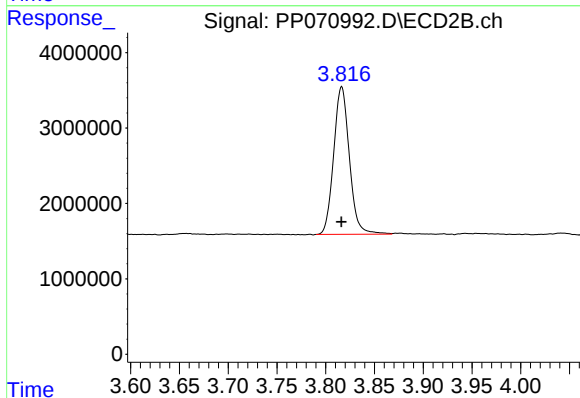


#1 Tetrachloro-m-xylene

R.T.: 3.816 min
Delta R.T.: 0.000 min
Response: 21938249
Conc: 21.16 ng/ml

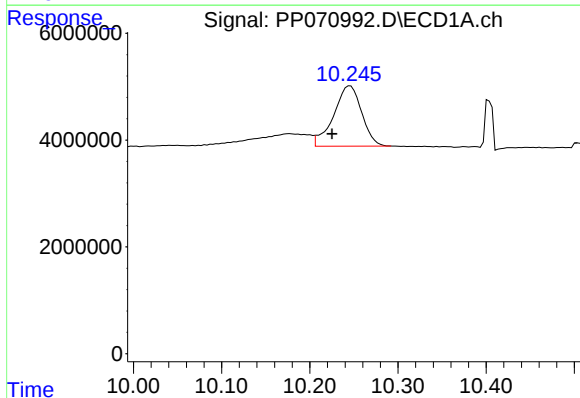

#2 Decachlorobiphenyl

R.T.: 10.245 min
Delta R.T.: 0.019 min
Response: 24893056
Conc: 23.65 ng/ml m

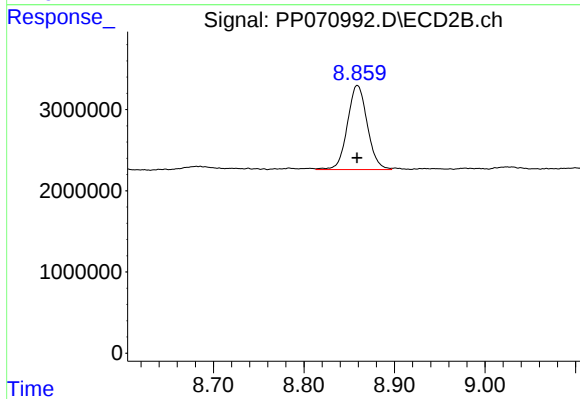

#2 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 15776668
Conc: 20.02 ng/ml