

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032825\
 Data File : PP071001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2025 02:18
 Operator : YP\AJ
 Sample : Q1677-01 10X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JEI299N-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/31/2025
 Supervised By :mohammad ahmed 04/02/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 05:18:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.517	3.815	4065276	2453224	2.781m	2.367m
2) SA Decachlor...	10.245	8.861	5588748	1430092	5.309m	1.814 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032825\
Data File : PP071001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2025 02:18
Operator : YP\AJ
Sample : Q1677-01 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JEI299N-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/31/2025
Supervised By :mohammad ahmed 04/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 05:18:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

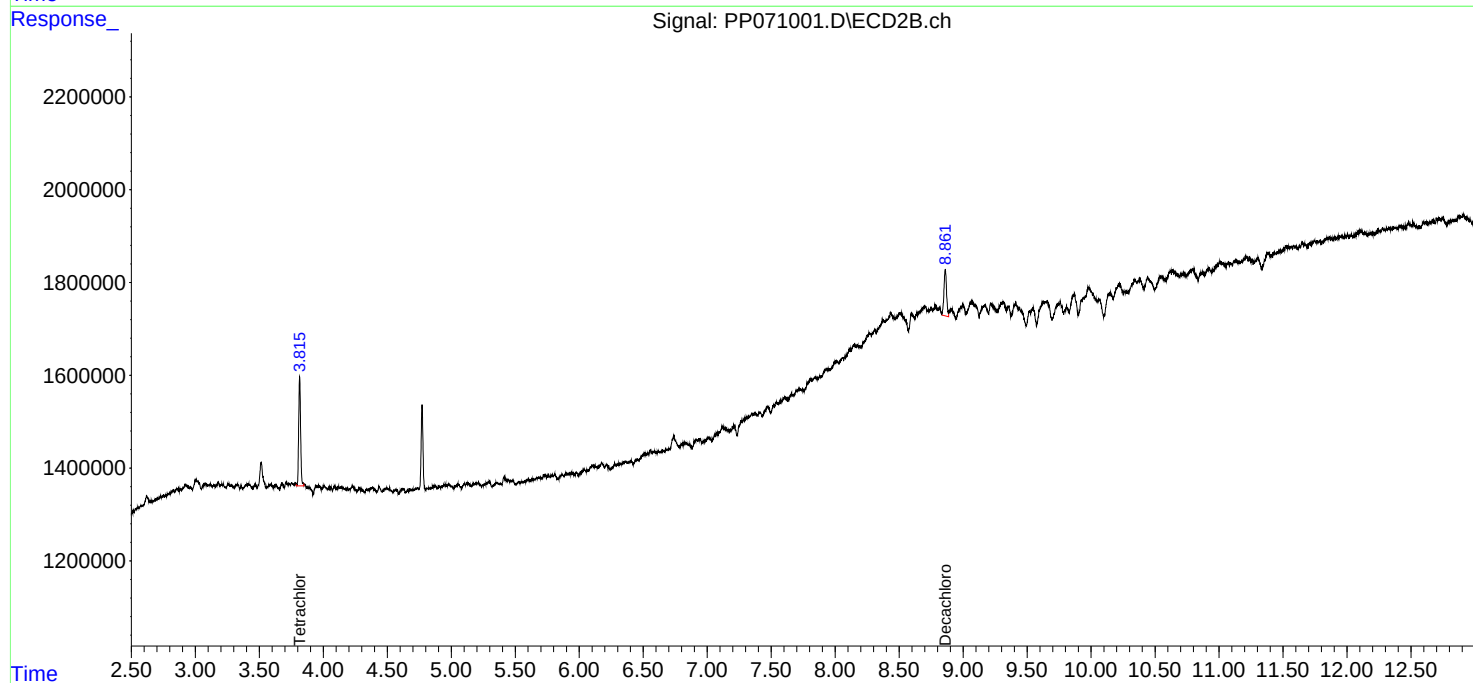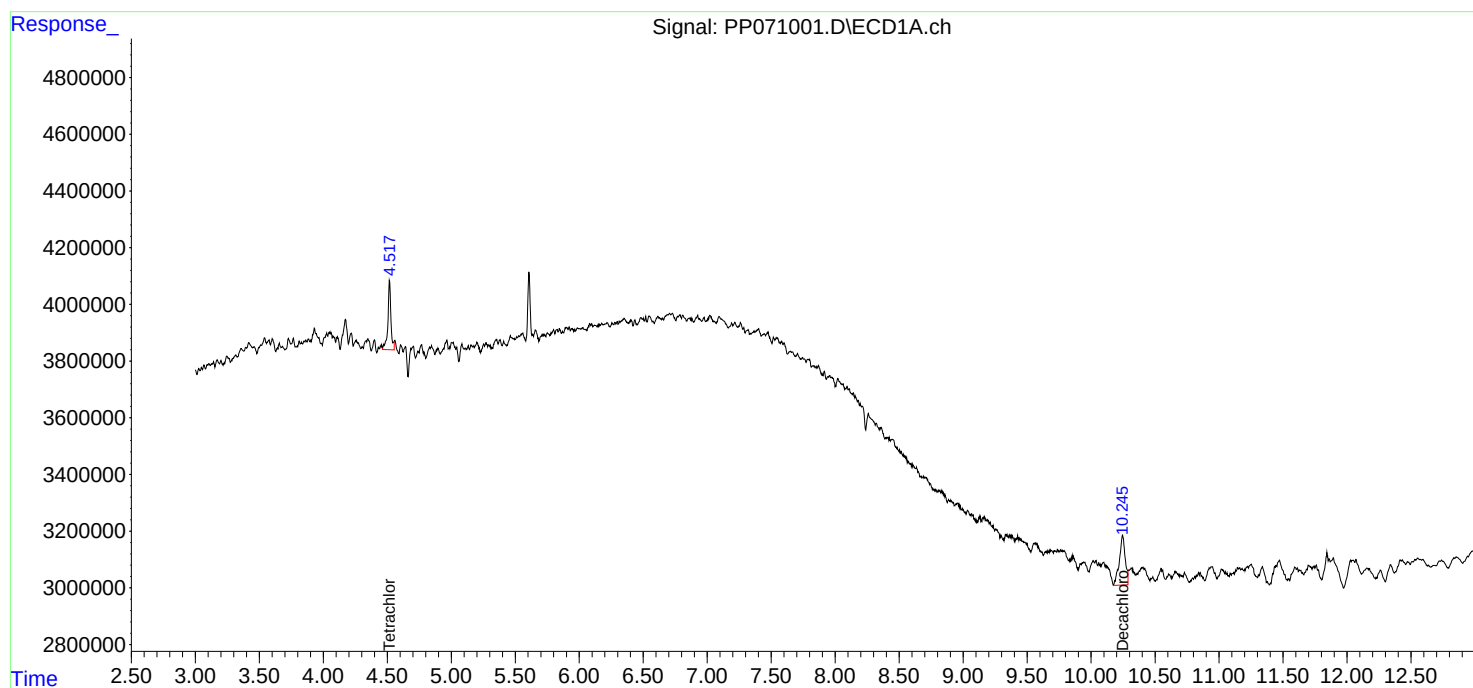

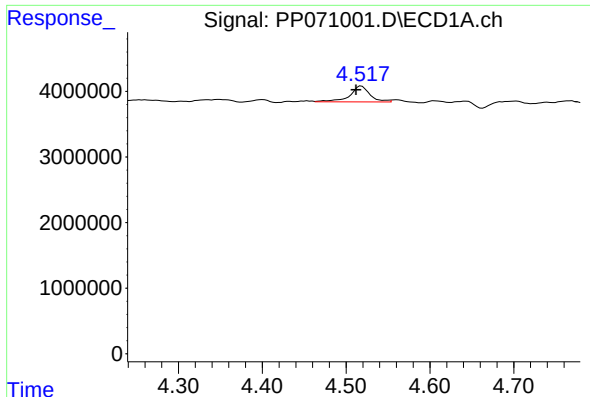


#1 Tetrachloro-m-xylene

R.T.: 4.517 min
Delta R.T.: 0.005 min
Response: 4065276
Conc: 2.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
JEI299N-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/31/2025
Supervised By :mohammad ahmed 04/02/2025

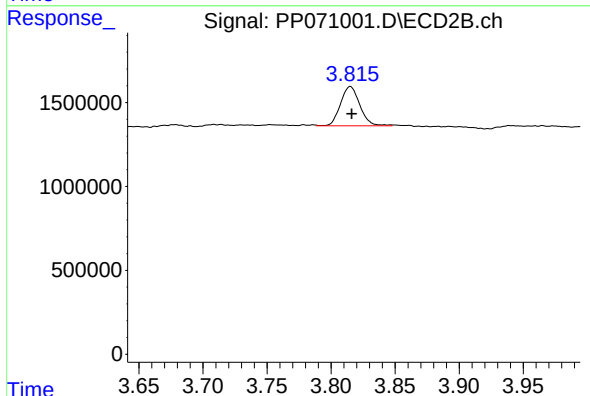


#1 Tetrachloro-m-xylene

R.T.: 3.815 min
Delta R.T.: -0.001 min
Response: 2453224
Conc: 2.37 ng/ml m

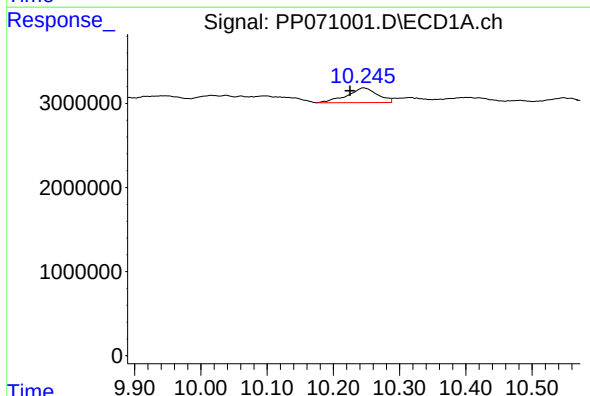

#2 Decachlorobiphenyl

R.T.: 10.245 min
Delta R.T.: 0.020 min
Response: 5588748
Conc: 5.31 ng/ml m

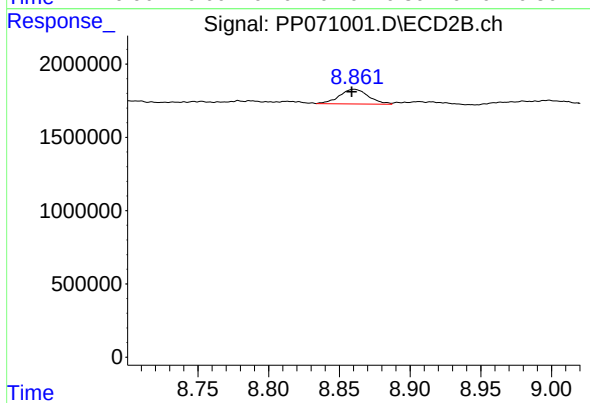

#2 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.002 min
Response: 1430092
Conc: 1.81 ng/ml