

Data Path : P:\HPCHEM1\ECD_P\Data\PP032918\
 Data File : PP024737.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2018 5:52
 Operator : UA/AJ
 Sample : J2021-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 J2021-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 07:43:50 2018
 Quant Method : P:\HPCHEM1\ECD_P\methods\PP032918.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 30 01:06:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.441	11.165	190.3E6	195.9E6	359.458	330.120
Target Compounds							
2) T	3,5-DICHL...	0.000	9.265	0	10926027	N.D.	13.554 #
3) T	4-Nitroph...	11.076	10.342	24172239	41761395	66.025	117.021 #
5) T	DICAMBA	11.786	11.497	15305818	595.4E6	6.201	257.763 #
6) T	MCPD	12.118	0.000	18469351	0	11.841	N.D. #
7) T	MCPA	12.357	0.000	16251454	0	6.987	N.D. #
8) T	DICHLORPROP	0.000	12.627	0	183.6E6	N.D.	311.753 #
9) T	2,4-D	0.000	13.061	0	23205227	N.D.	30.568 #
10) T	Pentachlo...	13.756	0.000	11274869	0	1.201	N.D. #
15) T	Picloram	16.992	0.000	27935356	0	4.773	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP032918\
Data File : PP024737.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2018 5:52
Operator : UA/AJ
Sample : J2021-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
J2021-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 07:43:50 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP032918.M
Quant Title : 8080.M
QLast Update : Fri Mar 30 01:06:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

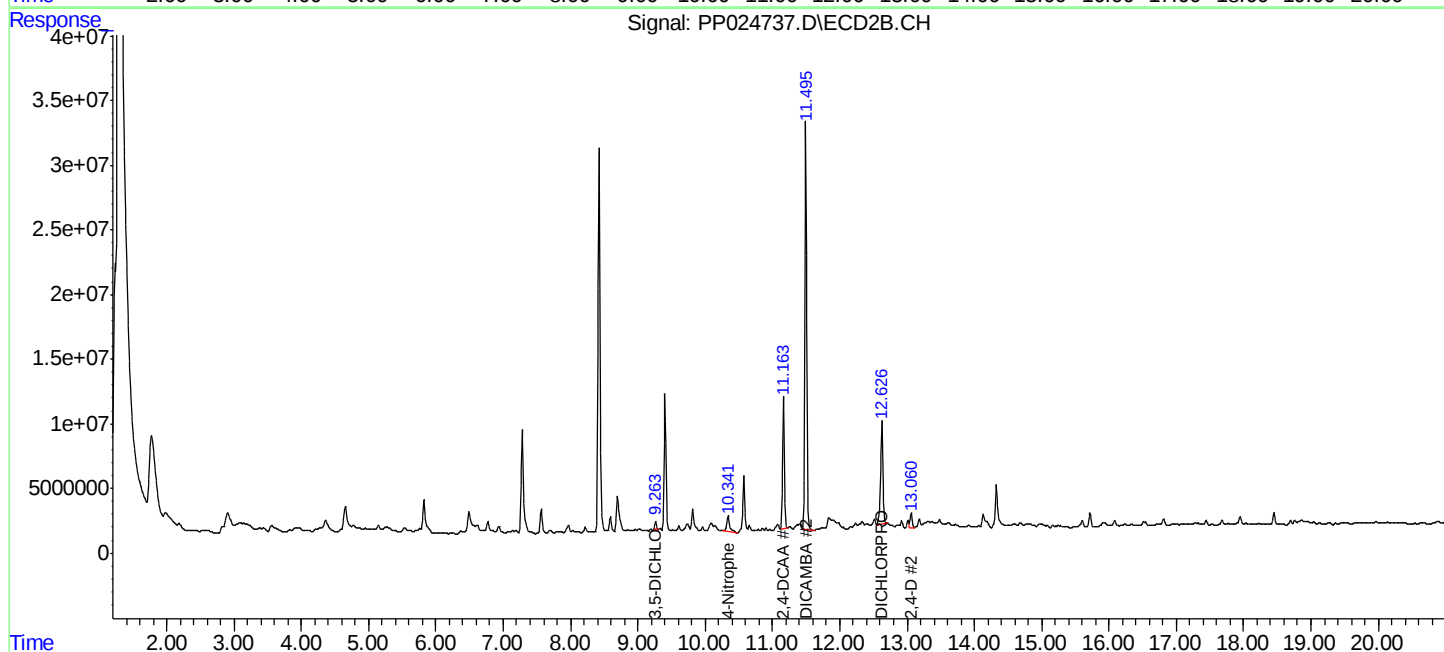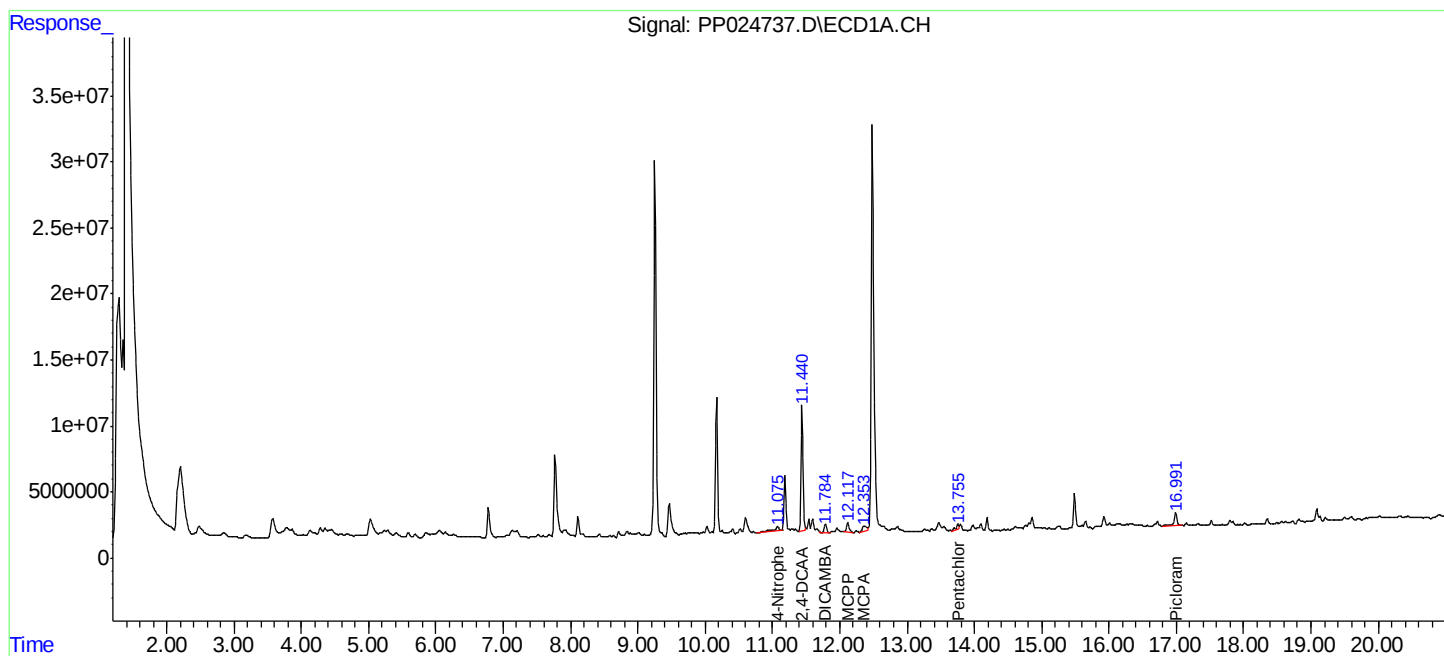


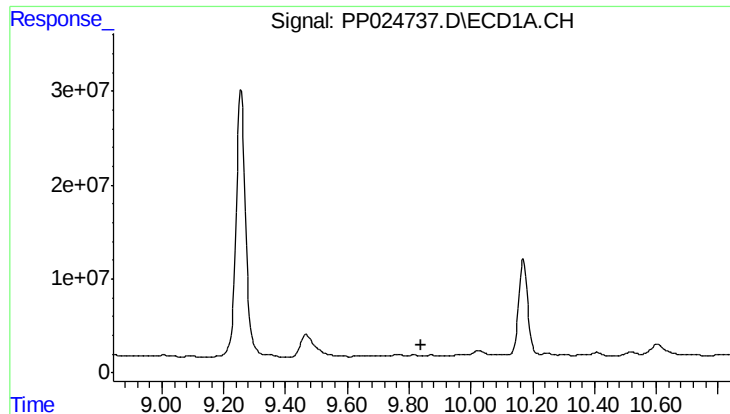

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.841 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
J2021-03

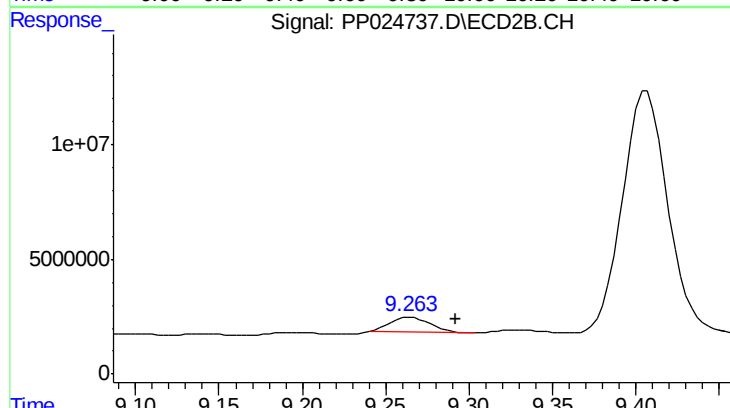


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.265 min
Delta R.T.: -0.027 min
Response: 10926027
Conc: 13.55 ng/ml

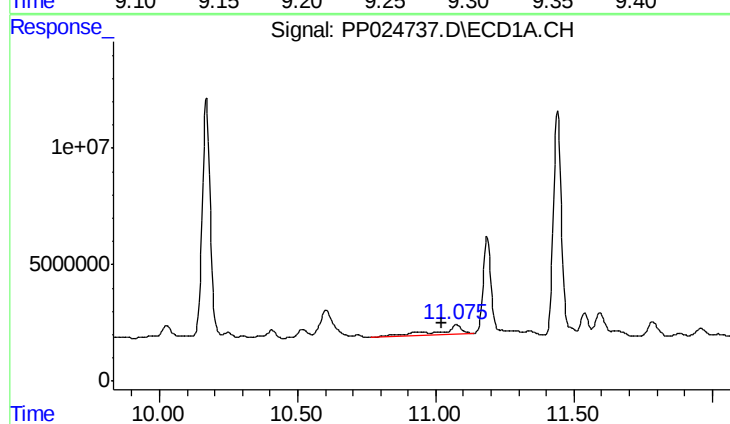


#3 4-Nitrophenol

R.T.: 11.076 min
Delta R.T.: 0.053 min
Response: 24172239
Conc: 66.03 ng/ml

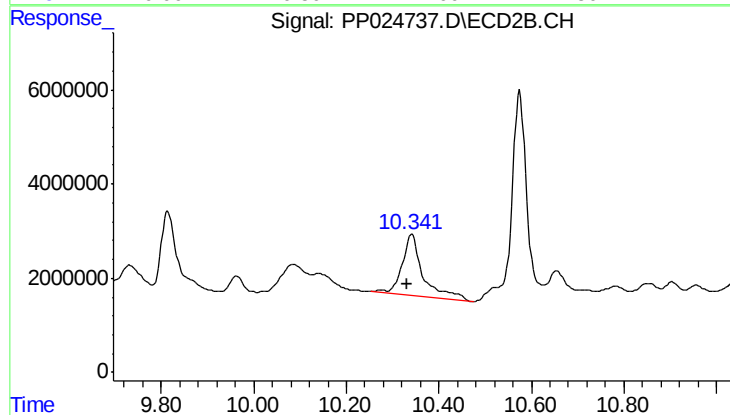

#3 4-Nitrophenol


R.T.: 10.342 min
Delta R.T.: 0.012 min
Response: 41761395
Conc: 117.02 ng/ml

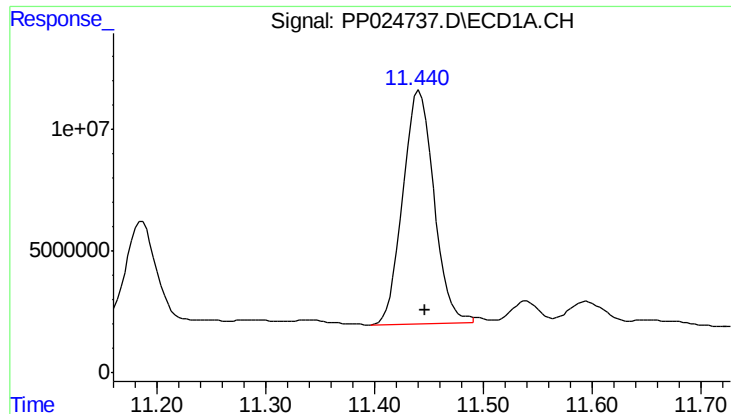

#4 2,4-DCAA


R.T.: 11.441 min
Delta R.T.: -0.005 min
Response: 190251345
Conc: 359.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
J2021-03

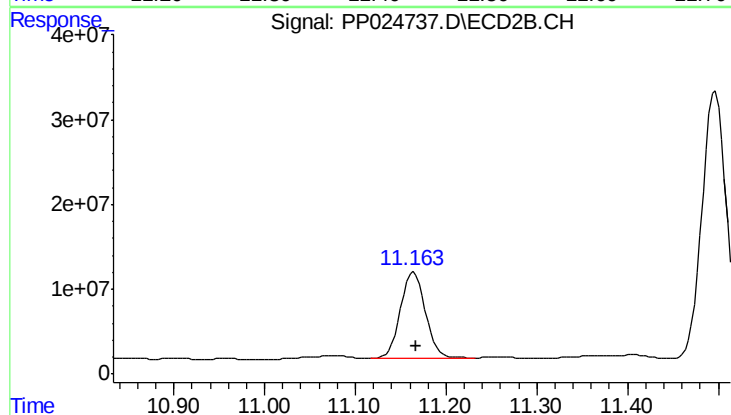


#4 2,4-DCAA

R.T.: 11.165 min
Delta R.T.: -0.003 min
Response: 195897447
Conc: 330.12 ng/ml

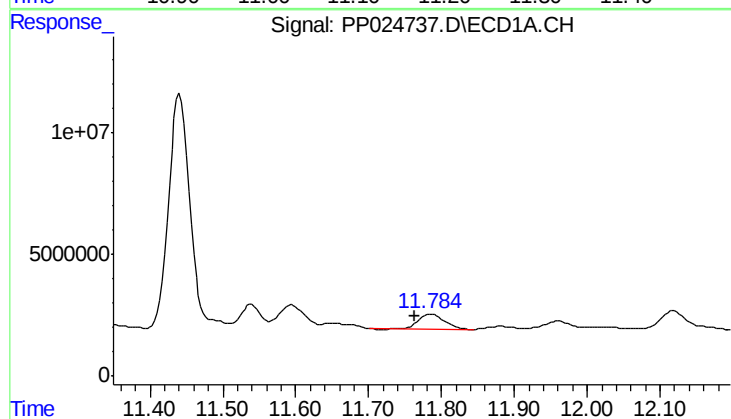


#5 DICAMBA

R.T.: 11.786 min
Delta R.T.: 0.022 min
Response: 15305818
Conc: 6.20 ng/ml

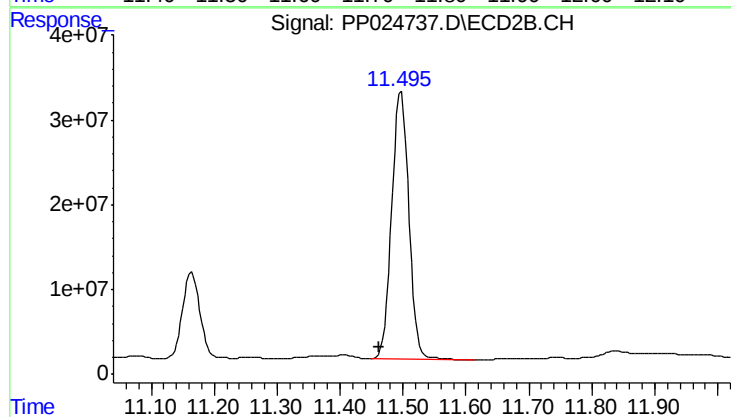

#5 DICAMBA


R.T.: 11.497 min
Delta R.T.: 0.036 min
Response: 595375579
Conc: 257.76 ng/ml

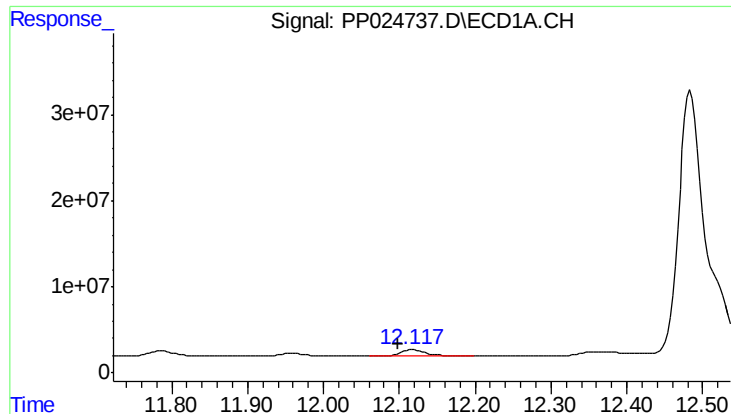

#6 MCPP


R.T.: 12.118 min
Delta R.T.: 0.020 min
Response: 18469351
Conc: 11.84 ug/ml

Instrument :
ECD_P
ClientSampleId :
J2021-03

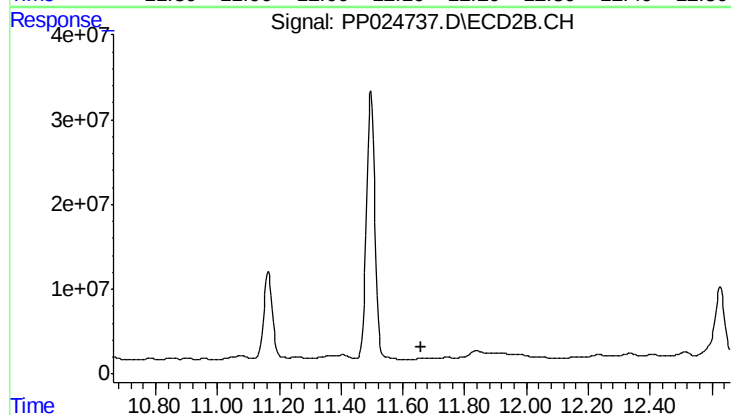


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 11.661 min
Response: 0
Conc: N.D.

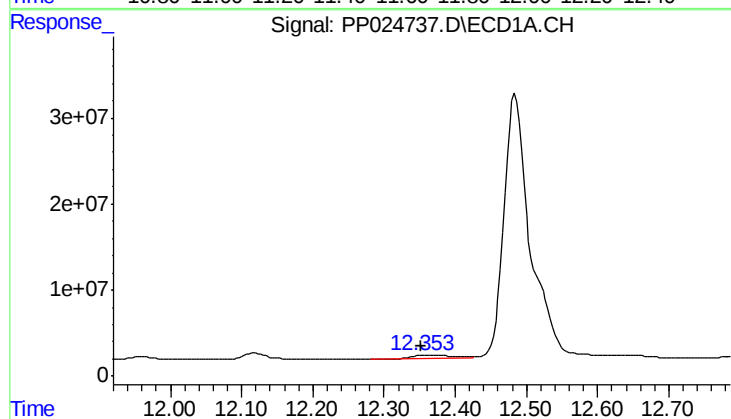


#7 MCPA

R.T.: 12.357 min
Delta R.T.: 0.004 min
Response: 16251454
Conc: 6.99 ug/ml

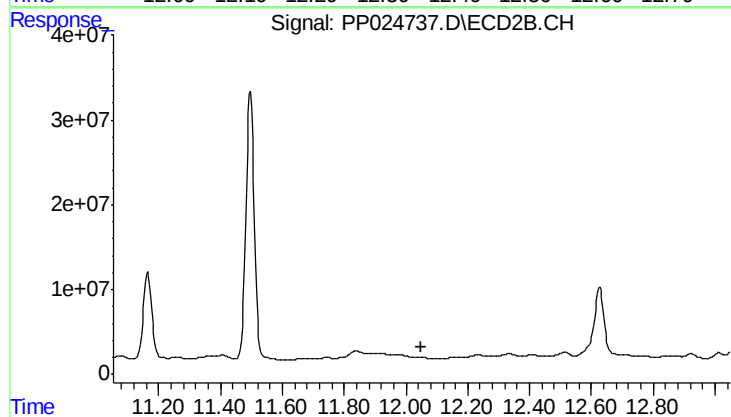

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.052 min
Response: 0
Conc: N.D.

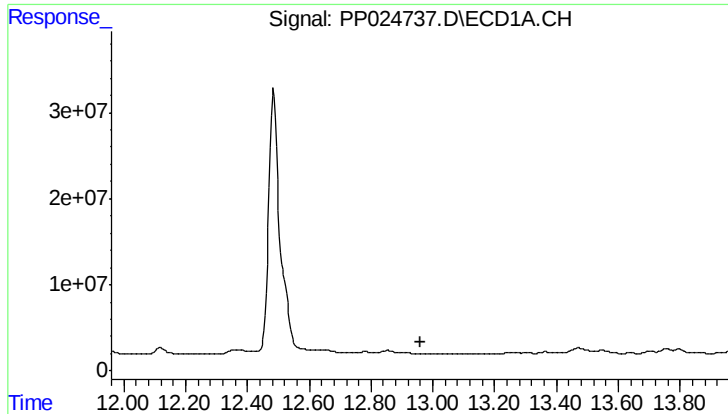

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.959 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
J2021-03

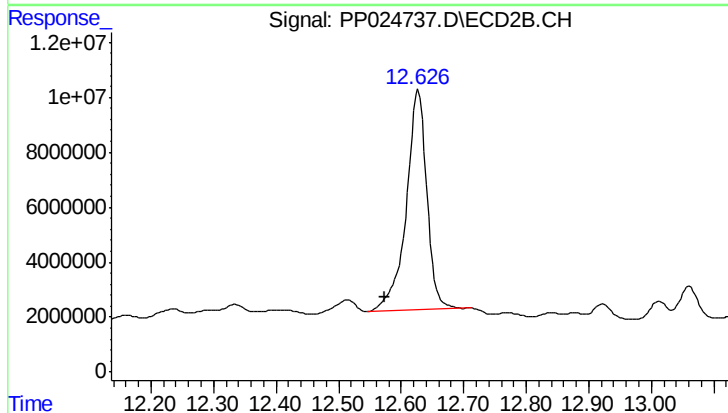


#8 DICHLORPROP

R.T.: 12.627 min
Delta R.T.: 0.054 min
Response: 183597521
Conc: 311.75 ng/ml

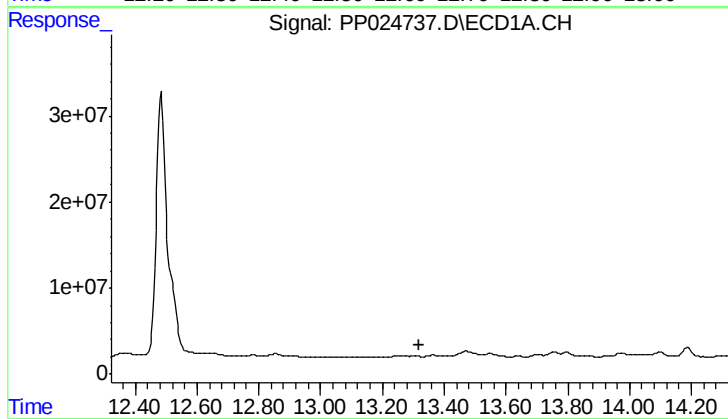


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.321 min
Response: 0
Conc: N.D.

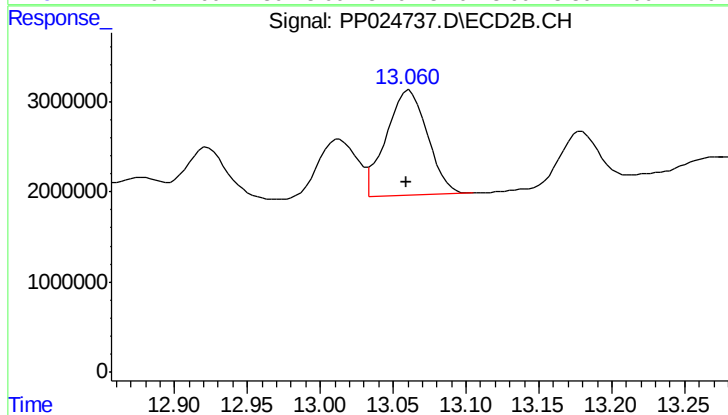

#9 2,4-D


R.T.: 13.061 min
Delta R.T.: 0.002 min
Response: 23205227
Conc: 30.57 ng/ml

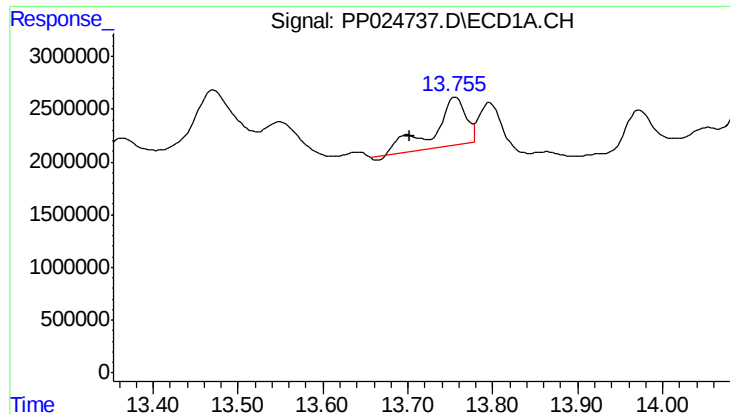

#10 Pentachlorophenol


R.T.: 13.756 min
Delta R.T.: 0.054 min
Response: 11274869
Conc: 1.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
J2021-03

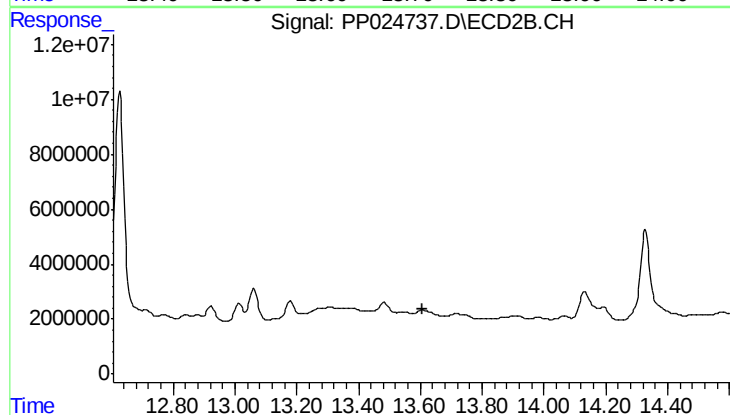


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.606 min
Response: 0
Conc: N.D.

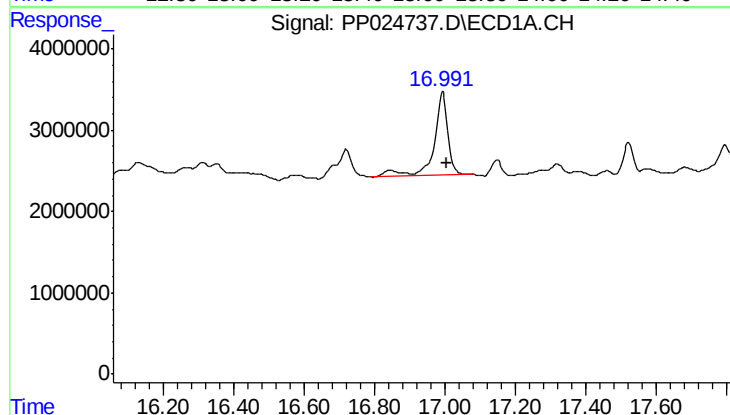

#15 Picloram

R.T.: 16.992 min
Delta R.T.: -0.013 min
Response: 27935356
Conc: 4.77 ng/ml

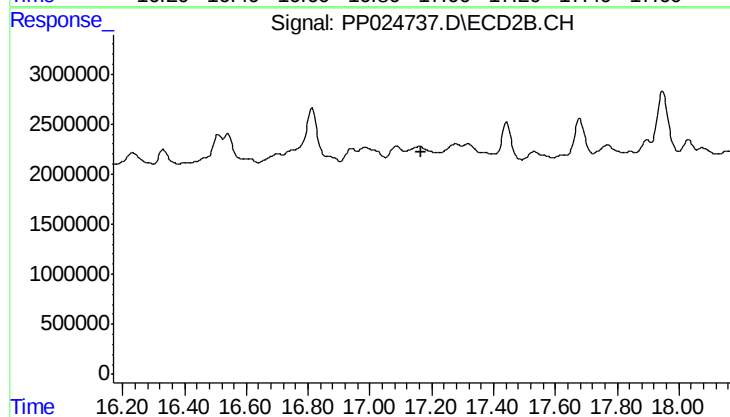

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.168 min
Response: 0
Conc: N.D.