

Data Path : P:\HPCHEM1\ECD_P\Data\PP032918\
Data File : PP024742.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2018 7:59
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 08:45:51 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP032918.M
Quant Title : 8080.M
QLast Update : Fri Mar 30 01:06:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.443	11.166	285.1E6	287.9E6	538.683	485.168
Target Compounds							
15) T	Picloram	16.957	0.000	16100002	0	2.751	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP032918\
Data File : PP024742.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2018 7:59
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 08:45:51 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP032918.M
Quant Title : 8080.M
QLast Update : Fri Mar 30 01:06:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

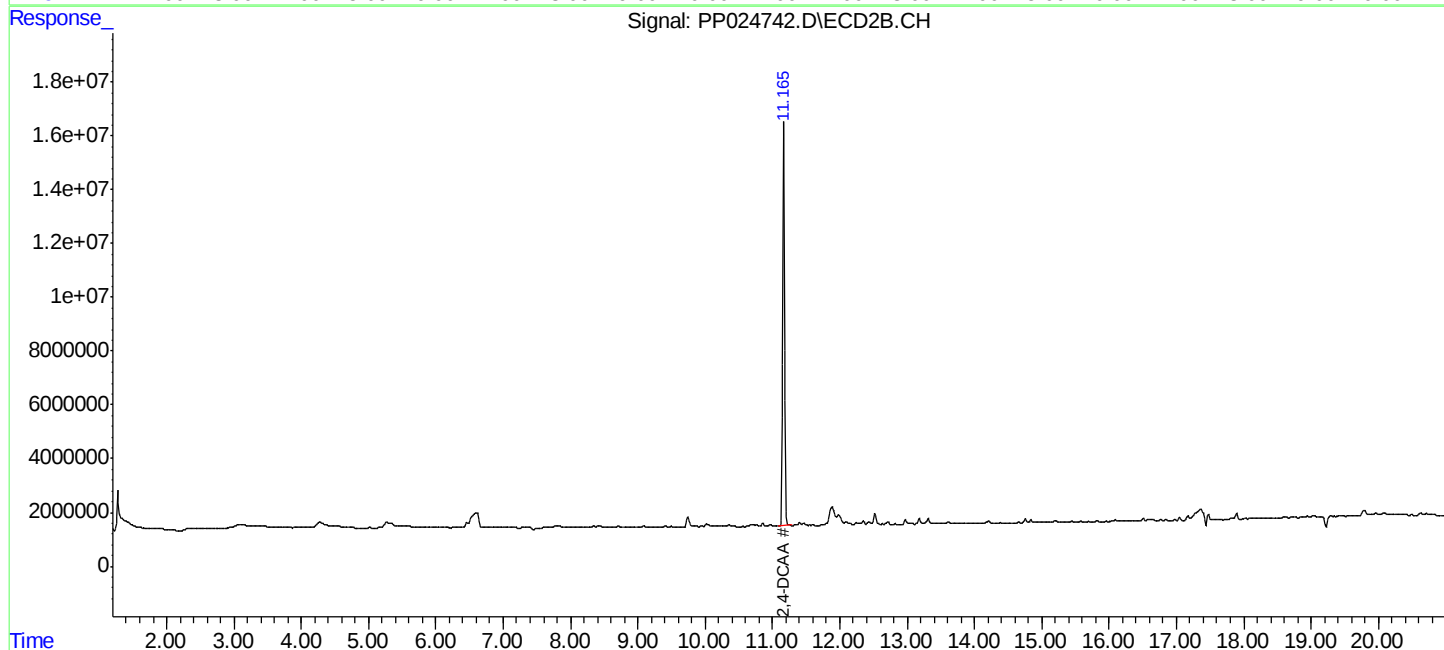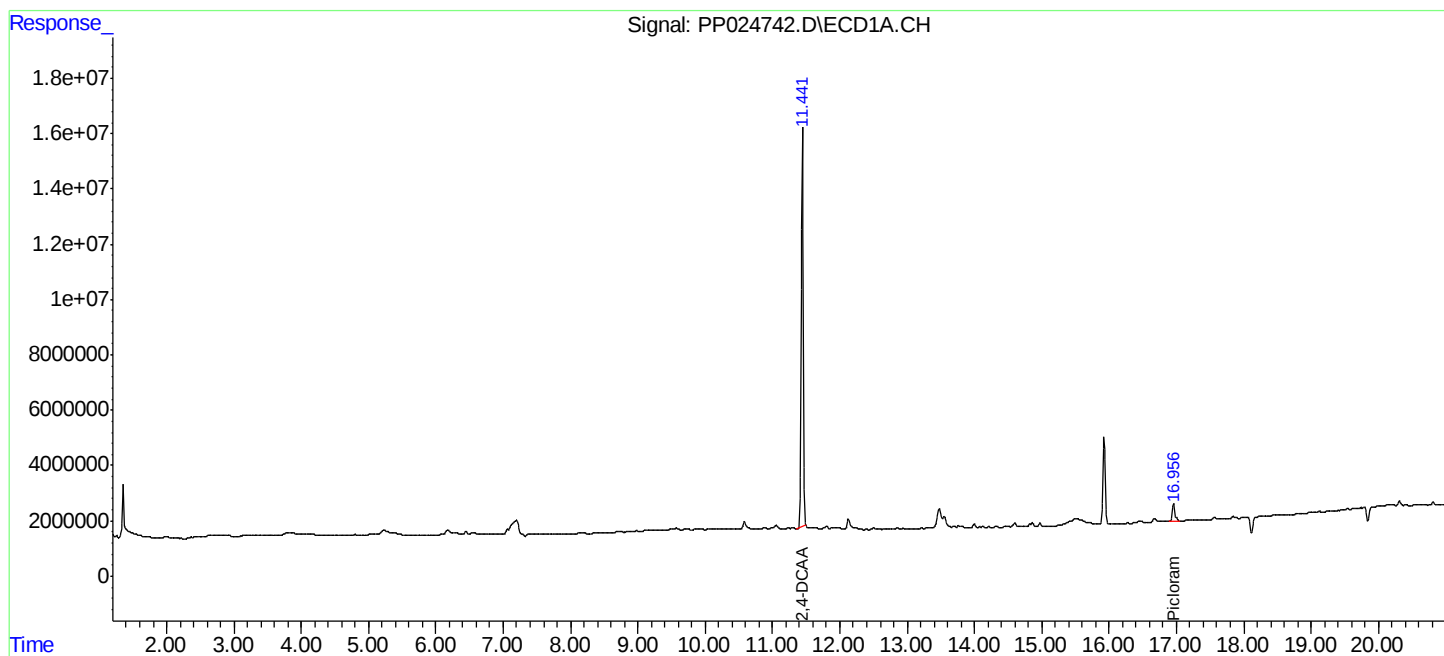


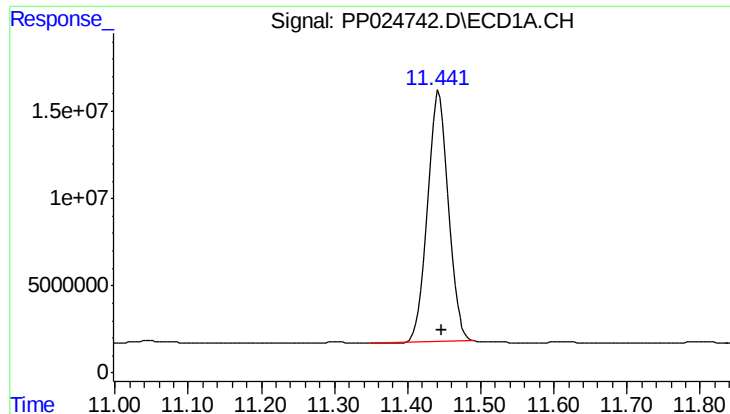

#4 2,4-DCAA


R.T.: 11.443 min
Delta R.T.: -0.003 min
Response: 285110369
Conc: 538.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

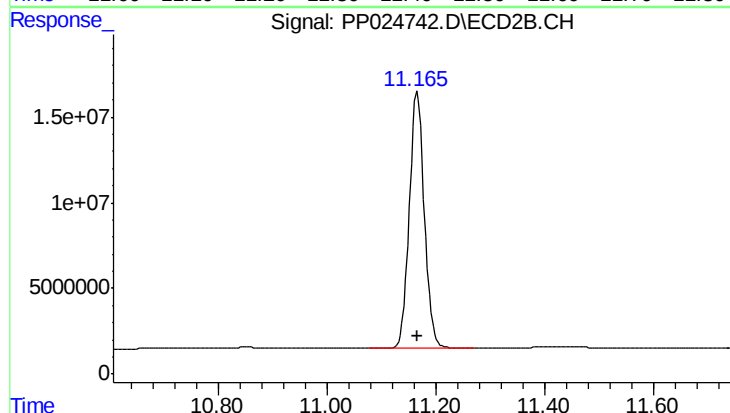


#4 2,4-DCAA

R.T.: 11.166 min
Delta R.T.: -0.001 min
Response: 287905097
Conc: 485.17 ng/ml

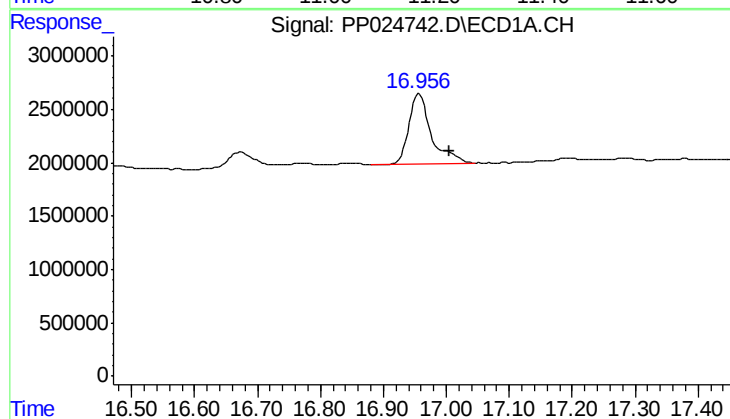

#15 Picloram

R.T.: 16.957 min
Delta R.T.: -0.048 min
Response: 16100002
Conc: 2.75 ng/ml

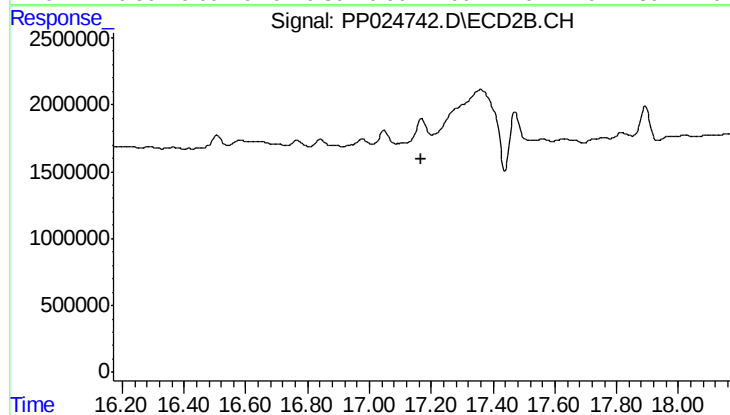

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.168 min
Response: 0
Conc: N.D.