

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032919\
 Data File : PP029651.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Mar 2019 22:15
 Operator : EI\MA
 Sample : I.BLK
 Misc : hexane
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 23:23:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.922	12.118	16054563	18417733	490.740	428.904
Target Compounds							
5) T	DICAMBA	0.000	12.398	0	562148	N.D.	3.832 #
8) T	DICHLORPROP	13.373	0.000	1311731	0	38.320	N.D. #
10) T	Pentachlo...	14.245	0.000	1408804	0	2.067	N.D. #
11) T	2,4,5-TP ...	15.012	0.000	398547	0	1.639	N.D. #
12) T	2,4,5-T	15.472	0.000	559601	0	2.470	N.D. #
13) T	2,4-DB	16.205	0.000	1379974	0	66.364	N.D. #
14) T	DINOSEB	17.701	0.000	2606439	0	15.464	N.D. #
15) T	Picloram	0.000	18.213	0	571075	N.D.	2.396 #
16) T	DCPA	18.008	18.114	1232119	68477	3.884	0.261 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032919\
Data File : PP029651.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Mar 2019 22:15
Operator : EI\MA
Sample : I.BLK
Misc : hexane
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 23:23:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

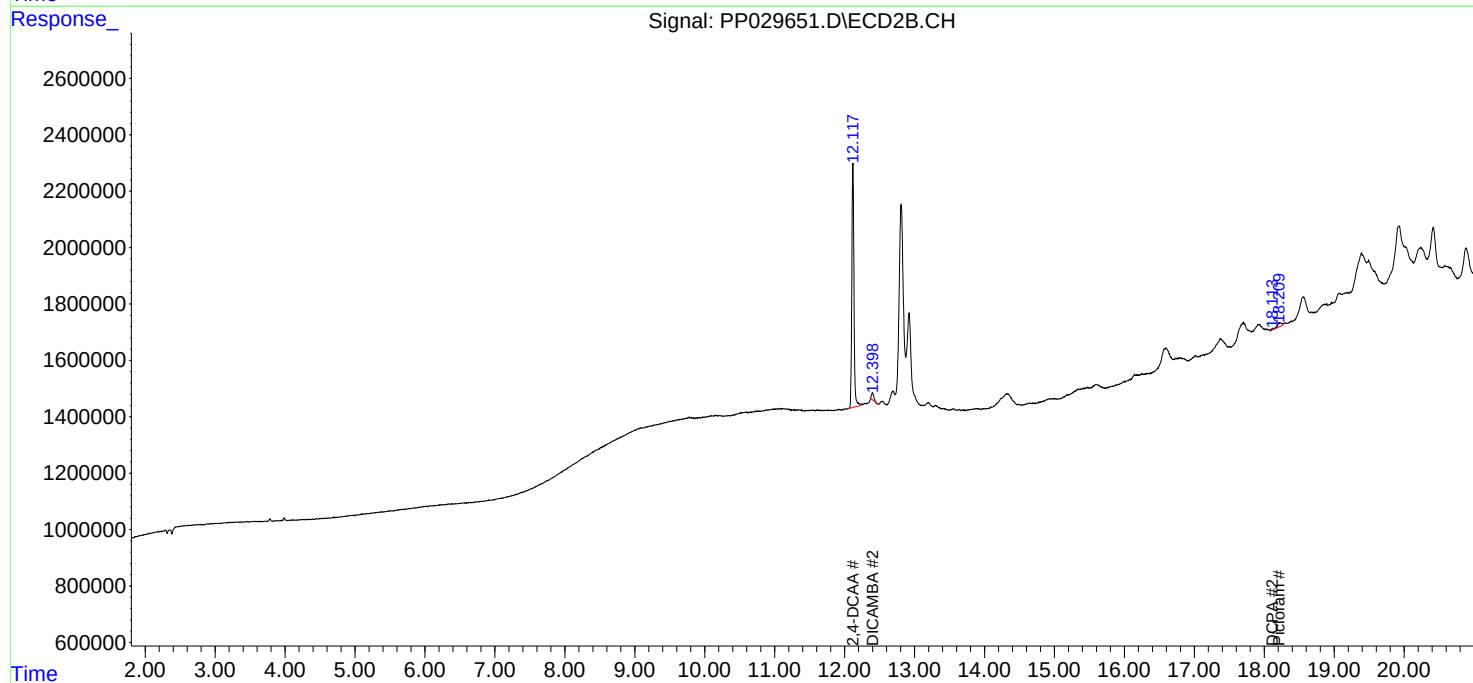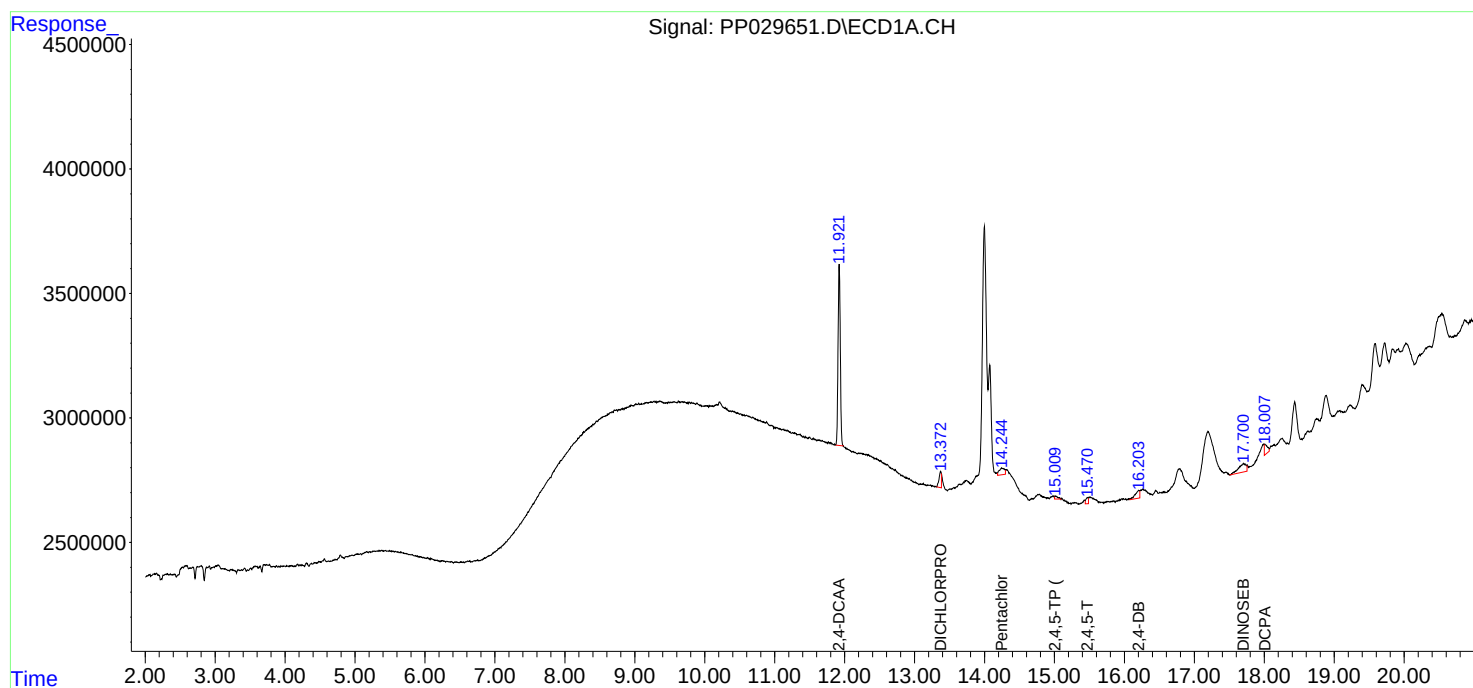


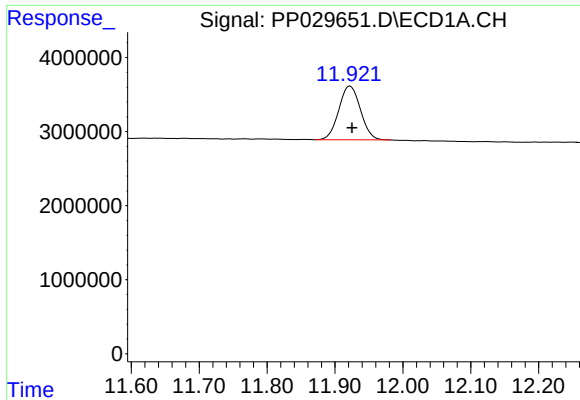

#4 2,4-DCAA


R.T.: 11.922 min
Delta R.T.: -0.003 min
Response: 16054563
Conc: 490.74 ng/ml

Instrument :
ECD_P
ClientSampleId :

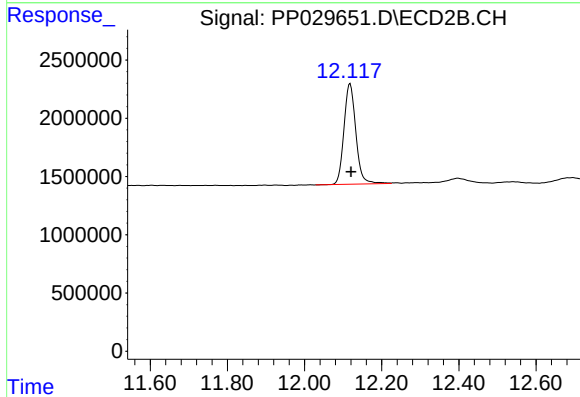


#4 2,4-DCAA

R.T.: 12.118 min
Delta R.T.: -0.003 min
Response: 18417733
Conc: 428.90 ng/ml

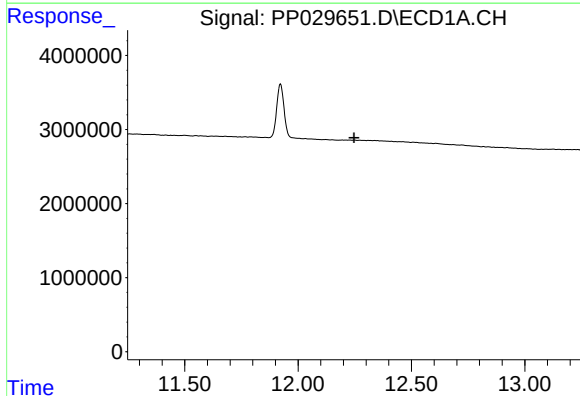


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.247 min
Response: 0
Conc: N.D.

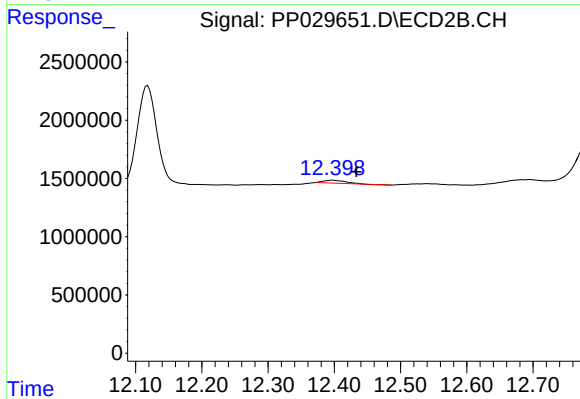

#5 DICAMBA


R.T.: 12.398 min
Delta R.T.: -0.035 min
Response: 562148
Conc: 3.83 ng/ml

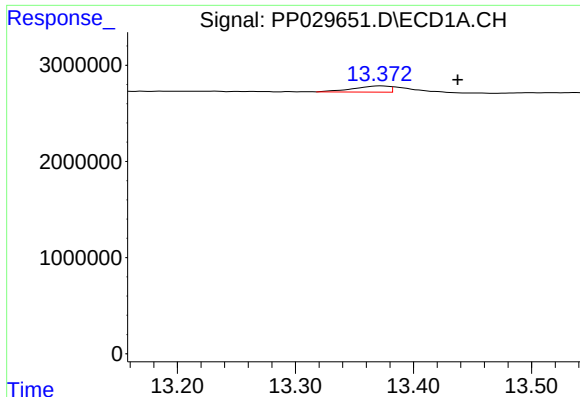

#8 DICHLORPROP


R.T.: 13.373 min
Delta R.T.: -0.065 min
Response: 1311731
Conc: 38.32 ng/ml

Instrument :
ECD_P
ClientSampleId :

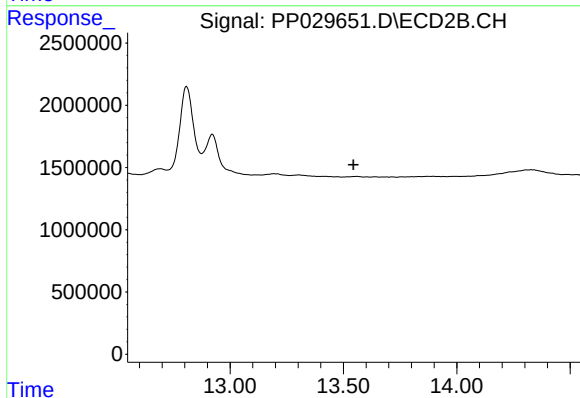


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.545 min
Response: 0
Conc: N.D.

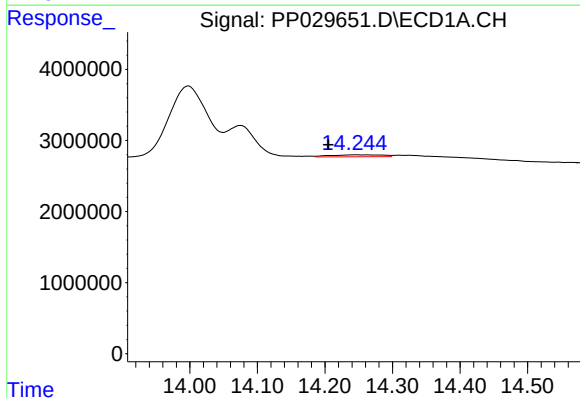


#10 Pentachlorophenol

R.T.: 14.245 min
Delta R.T.: 0.040 min
Response: 1408804
Conc: 2.07 ng/ml

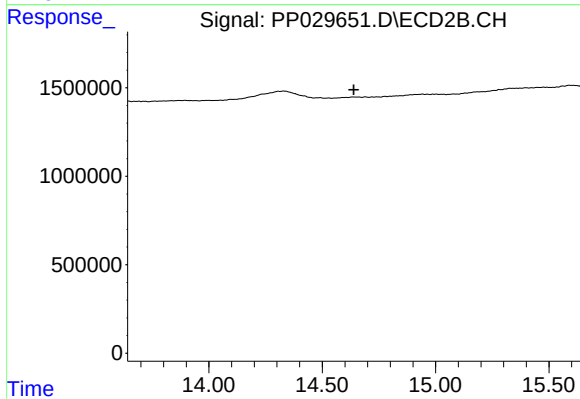

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 14.640 min
Response: 0
Conc: N.D.

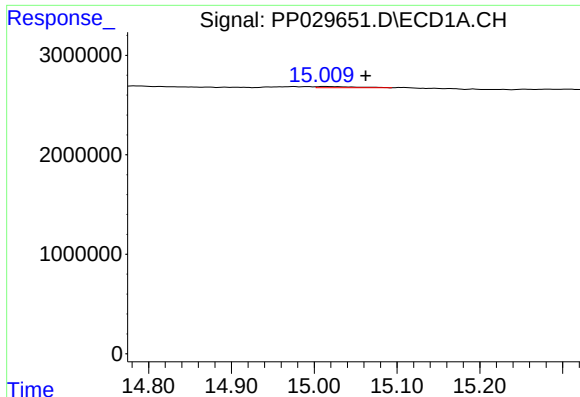

#11 2,4,5-TP (SILVEX)


R.T.: 15.012 min
Delta R.T.: -0.050 min
Response: 398547
Conc: 1.64 ng/ml

Instrument :
ECD_P
ClientSampleId :

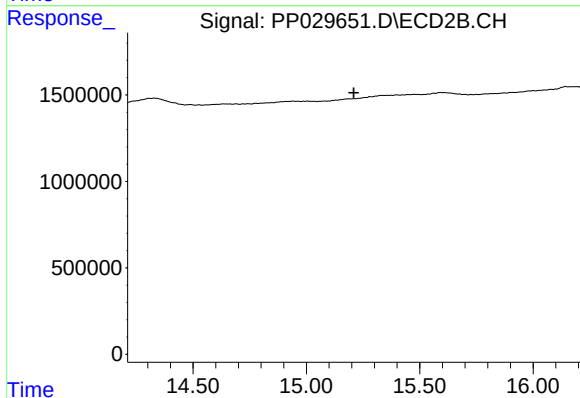


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.210 min
Response: 0
Conc: N.D.

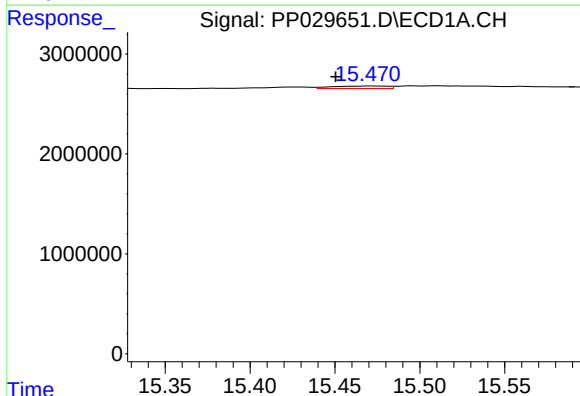


#12 2,4,5-T

R.T.: 15.472 min
Delta R.T.: 0.022 min
Response: 559601
Conc: 2.47 ng/ml

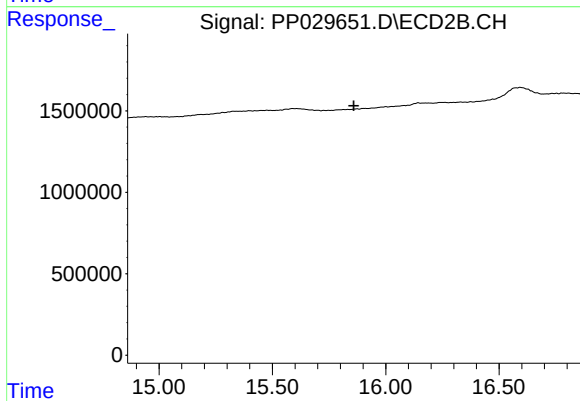

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 15.859 min
Response: 0
Conc: N.D.

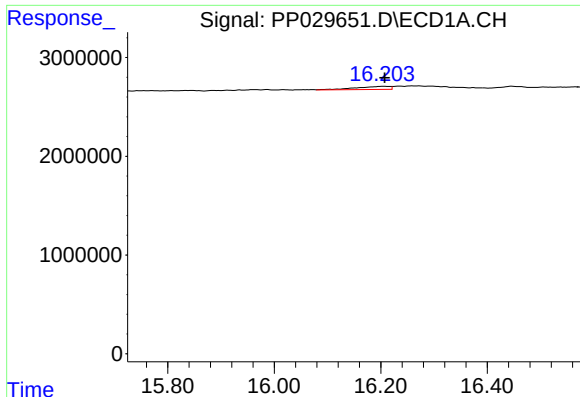

#13 2,4-DB


R.T.: 16.205 min
Delta R.T.: -0.003 min
Response: 1379974
Conc: 66.36 ng/ml

Instrument :
ECD_P
ClientSampleId :

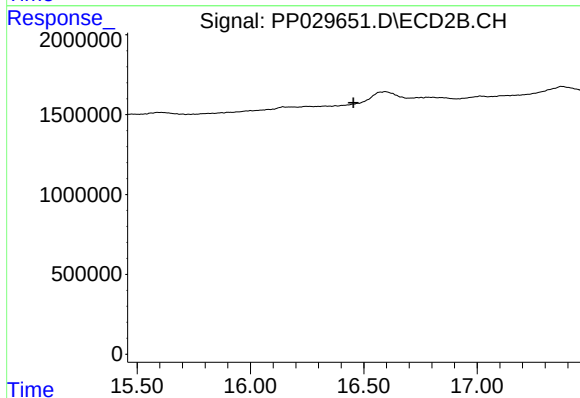


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

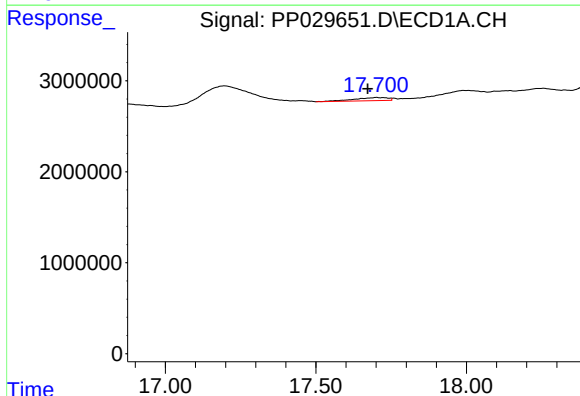


#14 DINOSEB

R.T.: 17.701 min
Delta R.T.: 0.029 min
Response: 2606439
Conc: 15.46 ng/ml

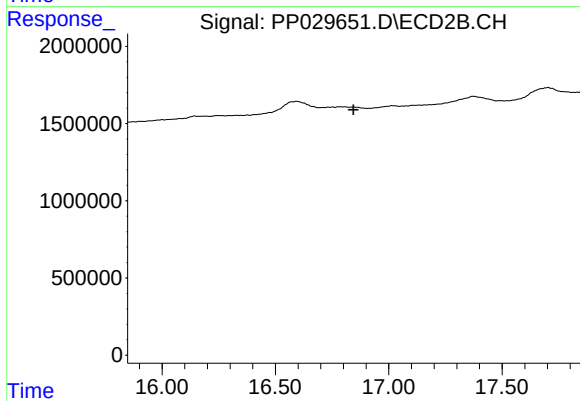

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.845 min
Response: 0
Conc: N.D.

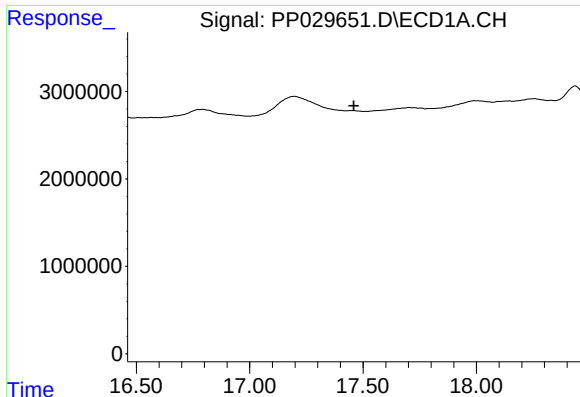

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

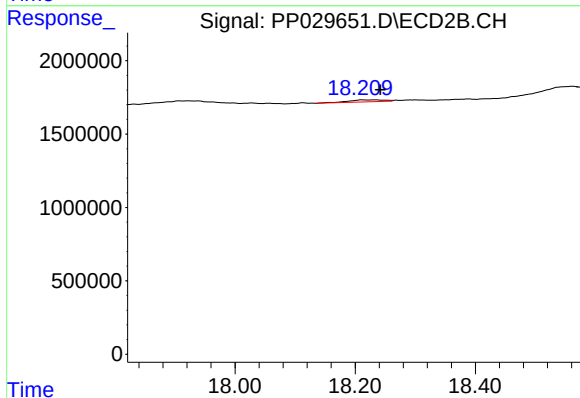


#15 Picloram

R.T.: 18.213 min
Delta R.T.: -0.029 min
Response: 571075
Conc: 2.40 ng/ml

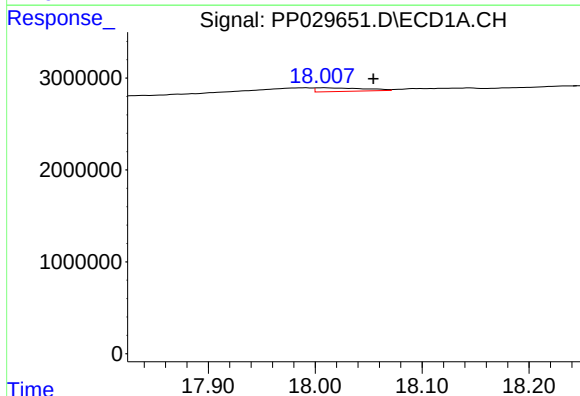

#16 DCPA

R.T.: 18.008 min
Delta R.T.: -0.047 min
Response: 1232119
Conc: 3.88 ng/ml

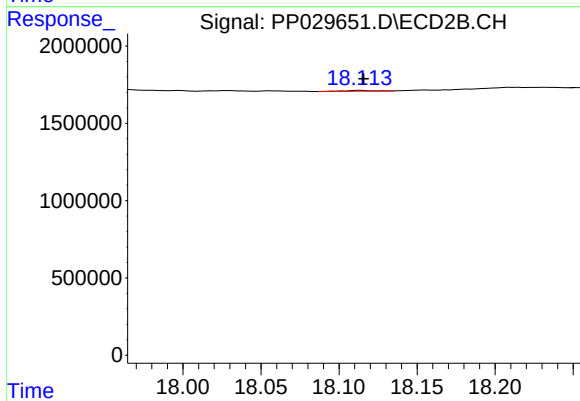

#16 DCPA

R.T.: 18.114 min
Delta R.T.: -0.002 min
Response: 68477
Conc: 0.26 ng/ml