

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032924\
 Data File : PP063965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Mar 2024 20:00
 Operator : YP\AJ
 Sample : P1922-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 50302

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/01/2024
 Supervised By :Ankita Jodhani 04/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 30 00:44:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 06:23:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.488	3.639	32607339	30877520	13.665	12.933
2) SA Decachlor...	10.374	8.688	33901585	28531319	13.352	10.557m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032924\
Data File : PP063965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Mar 2024 20:00
Operator : YP\AJ
Sample : P1922-03
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
50302


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/01/2024
Supervised By :Ankita Jodhani 04/01/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 30 00:44:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 06:23:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

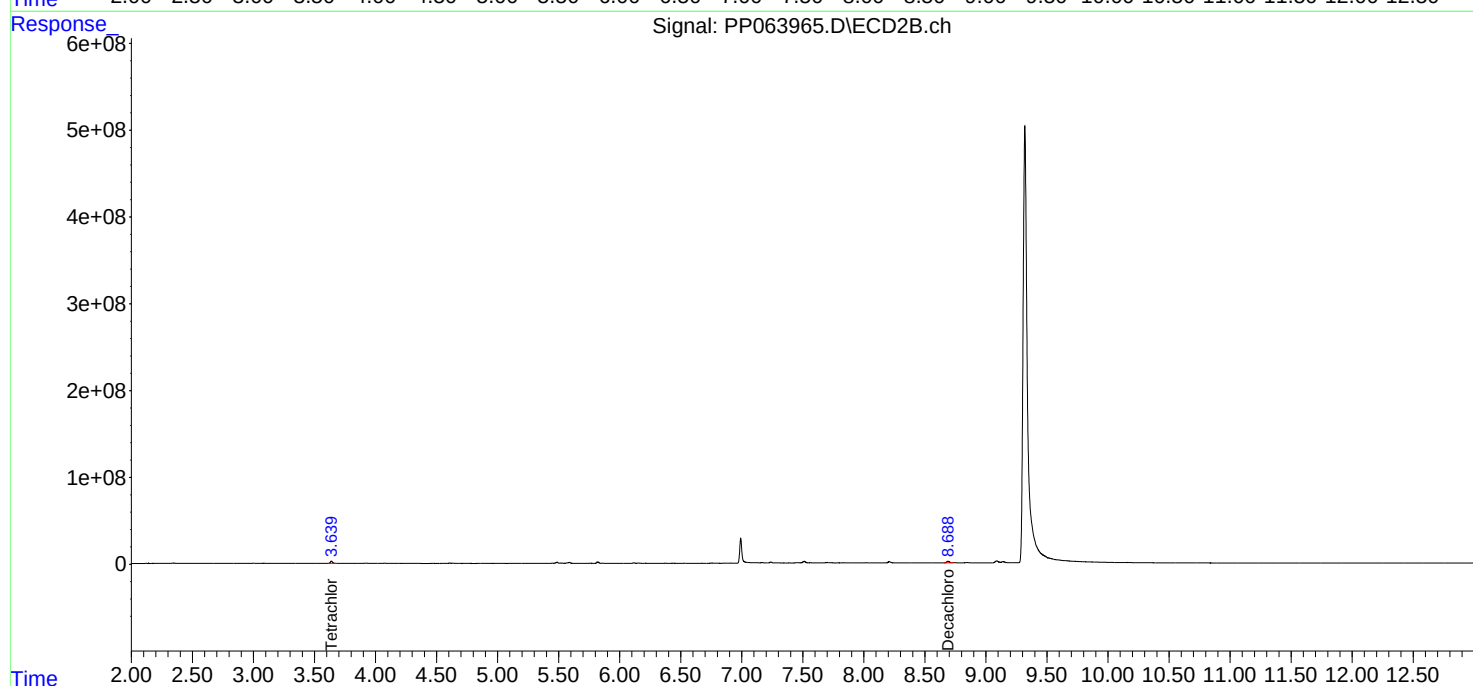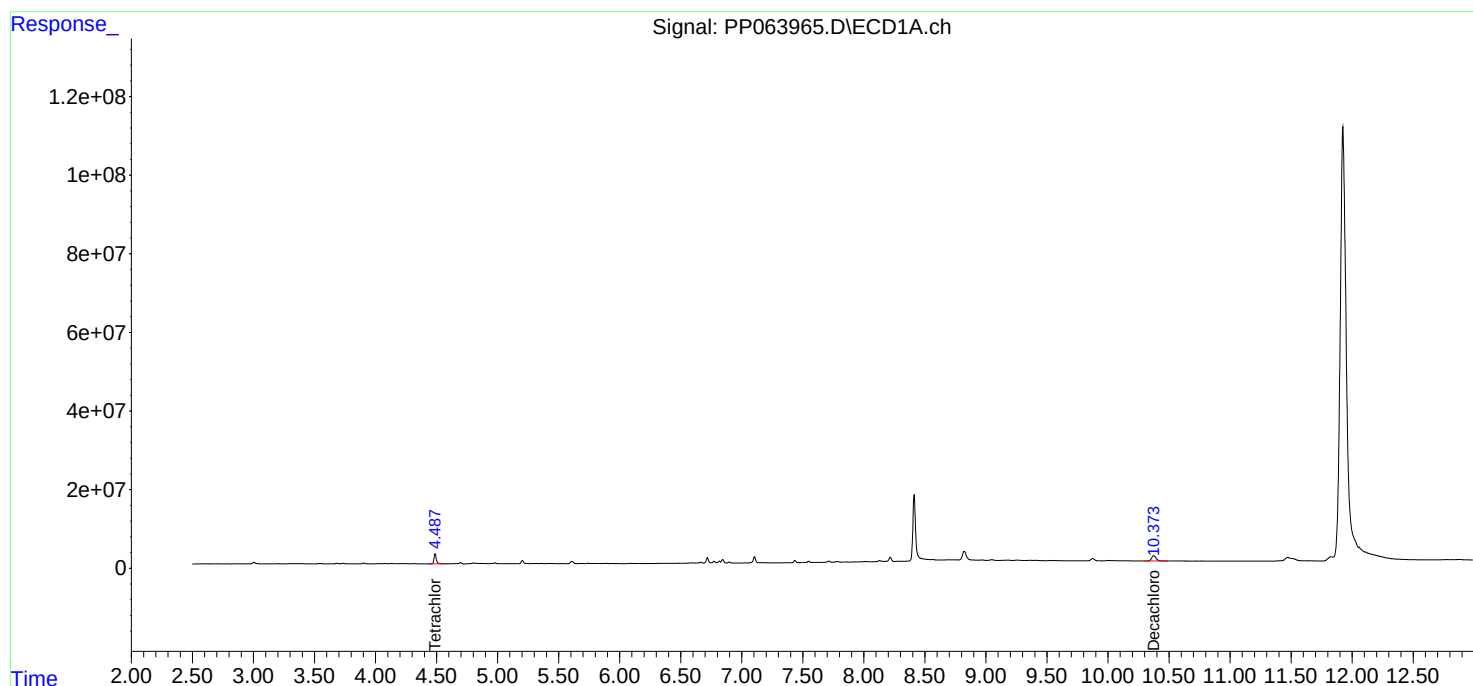

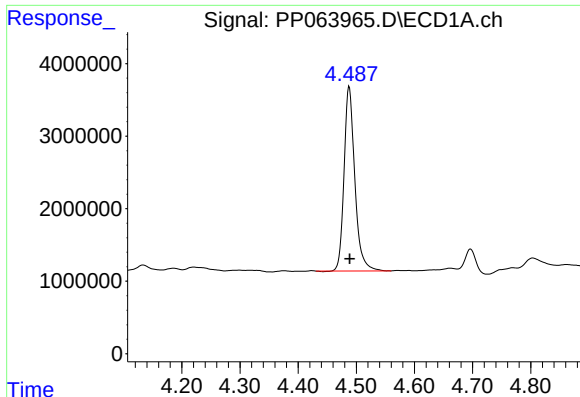


#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: -0.001 min
Response: 32607339
Conc: 13.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
50302


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/01/2024
Supervised By :Ankita Jodhani 04/01/2024

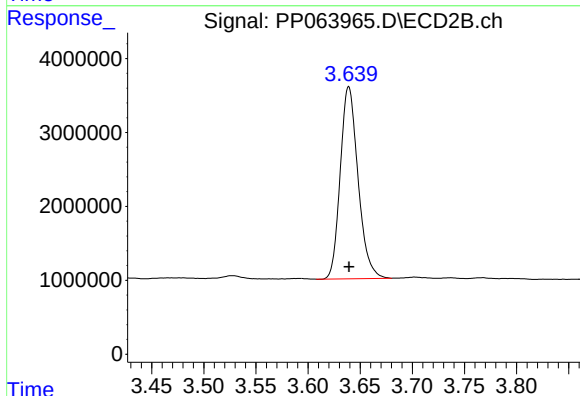


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: 0.000 min
Response: 30877520
Conc: 12.93 ng/ml

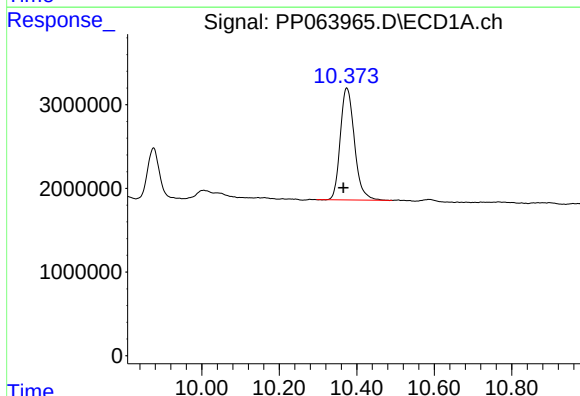

#2 Decachlorobiphenyl

R.T.: 10.374 min
Delta R.T.: 0.009 min
Response: 33901585
Conc: 13.35 ng/ml

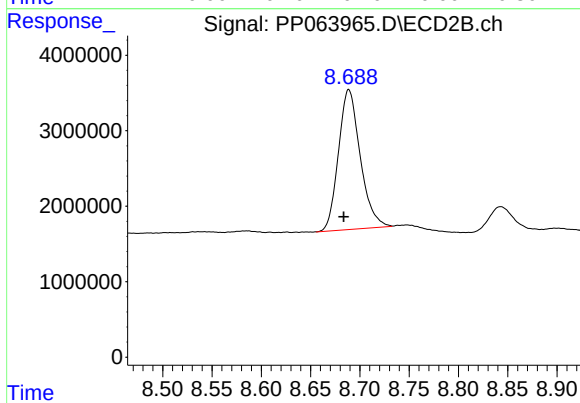

#2 Decachlorobiphenyl

R.T.: 8.688 min
Delta R.T.: 0.005 min
Response: 28531319
Conc: 10.56 ng/ml m