

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
 Data File : PP029656.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 10:17
 Operator : EI\MA
 Sample : PB118421BL
 Misc : hexane
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB118421BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:05:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.118	20875504	25920374	638.102	603.623
Target Compounds							
8) T	DICHLORPROP	0.000	13.547	0	394524	N.D.	9.742 #
9) T	2,4-D	13.752	0.000	183202	0	4.737	N.D. #
11) T	2,4,5-TP ...	0.000	15.268	0	131203	N.D.	0.634 #
12) T	2,4,5-T	15.444	15.856	666807	1758174	2.944	10.606 #
13) T	2,4-DB	16.213	0.000	1062571	0	51.100	N.D. #
14) T	DINOSEB	17.656	0.000	107717	0	0.639	N.D. #
15) T	Picloram	17.462	0.000	198558	0	0.606	N.D. #
16) T	DCPA	18.041	0.000	1427657	0	4.500	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
Data File : PP029656.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 10:17
Operator : EI\MA
Sample : PB118421BL
Misc : hexane
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB118421BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:05:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

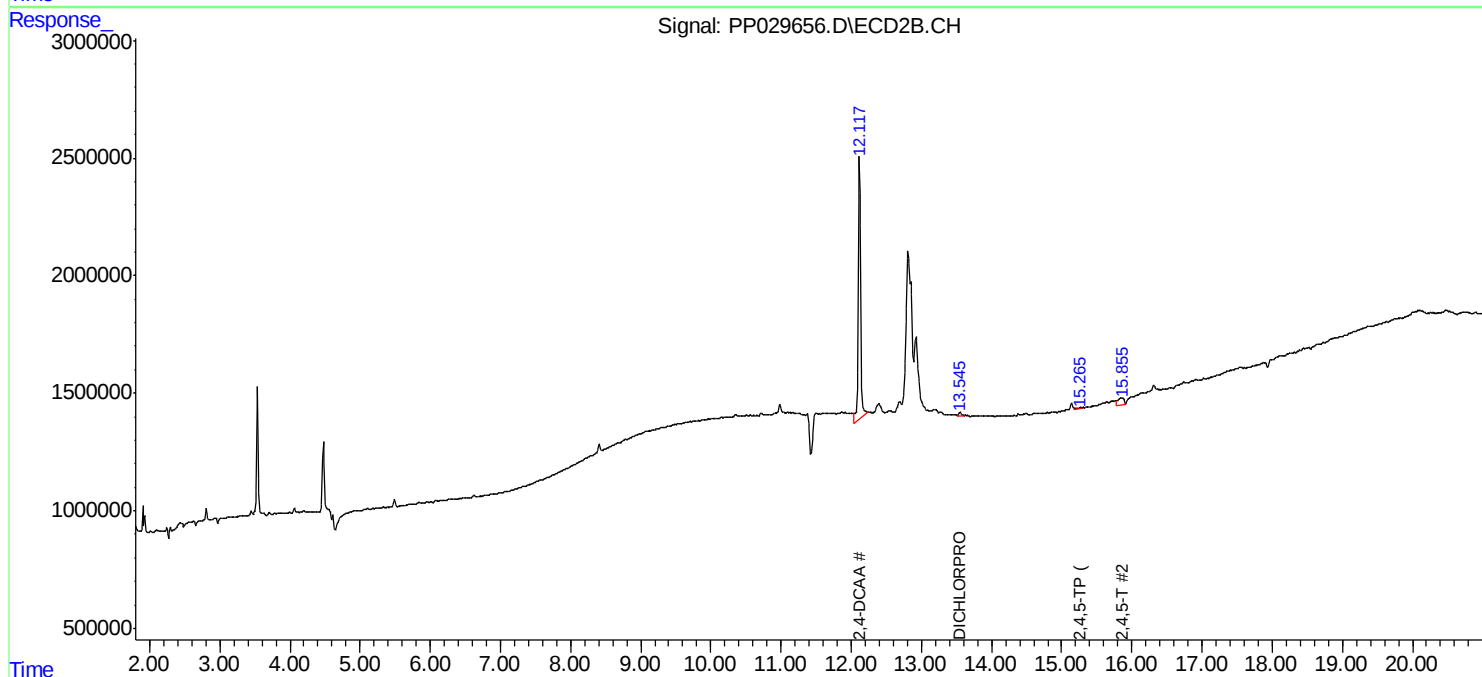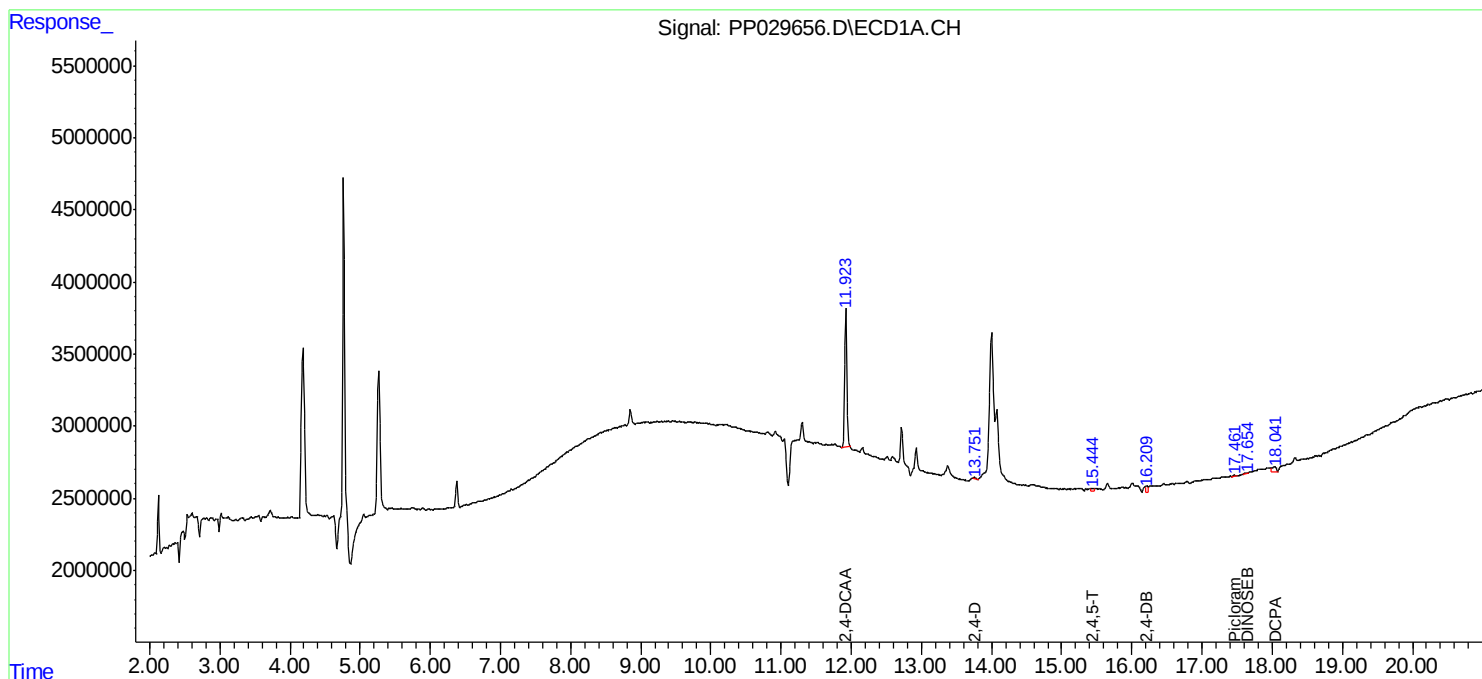


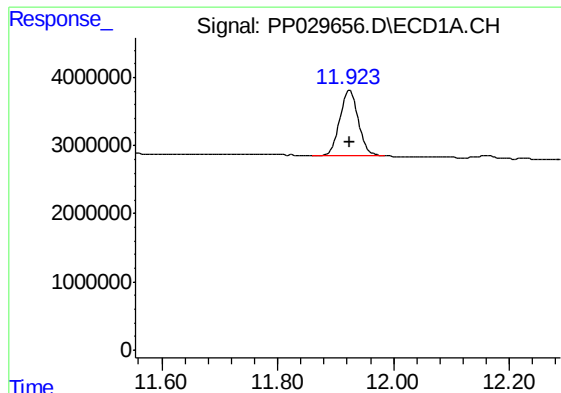

#4 2,4-DCAA


R.T.: 11.924 min
Delta R.T.: 0.000 min
Response: 20875504
Conc: 638.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118421BL

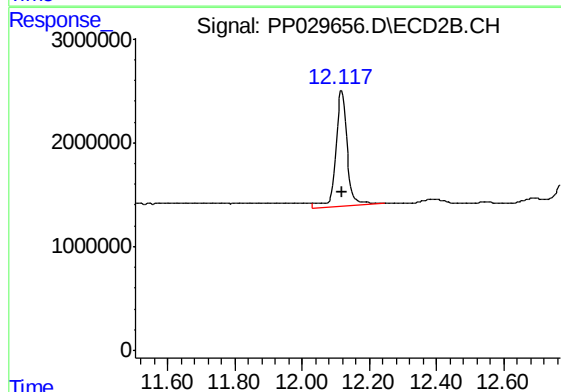


#4 2,4-DCAA

R.T.: 12.118 min
Delta R.T.: -0.003 min
Response: 25920374
Conc: 603.62 ng/ml

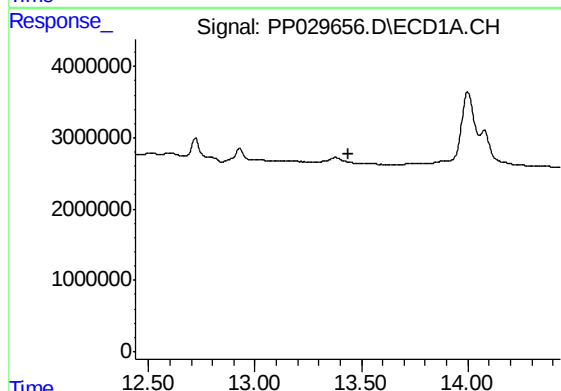


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.438 min
Response: 0
Conc: N.D.

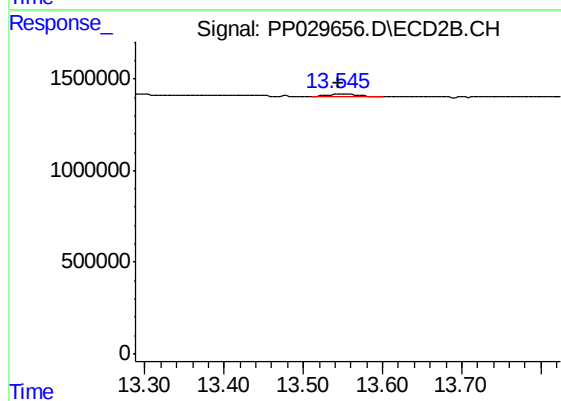

#8 DICHLORPROP


R.T.: 13.547 min
Delta R.T.: 0.002 min
Response: 394524
Conc: 9.74 ng/ml

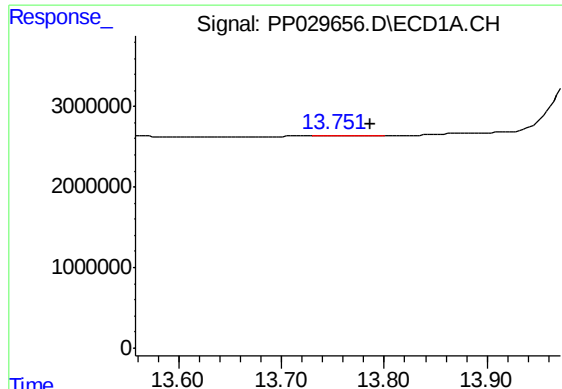

#9 2,4-D


R.T.: 13.752 min
Delta R.T.: -0.034 min
Response: 183202
Conc: 4.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118421BL

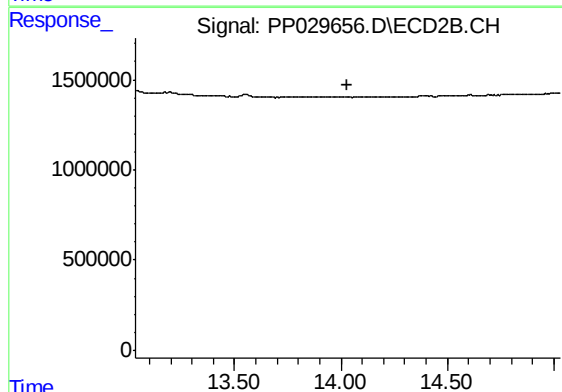


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 14.031 min
Response: 0
Conc: N.D.

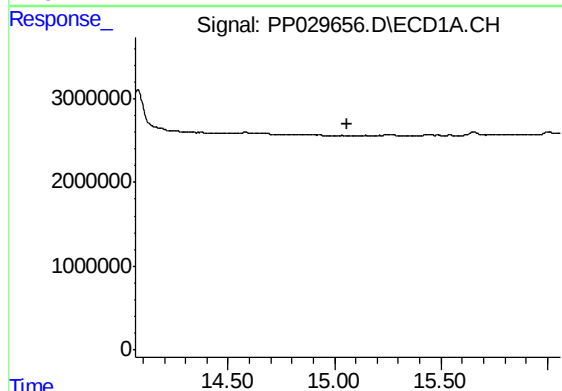


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.062 min
Response: 0
Conc: N.D.

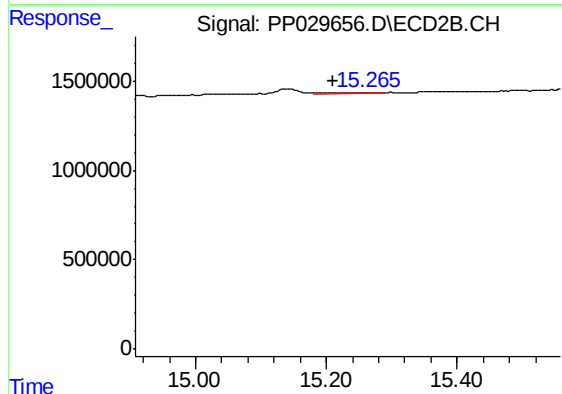

#11 2,4,5-TP (SILVEX)


R.T.: 15.268 min
Delta R.T.: 0.058 min
Response: 131203
Conc: 0.63 ng/ml

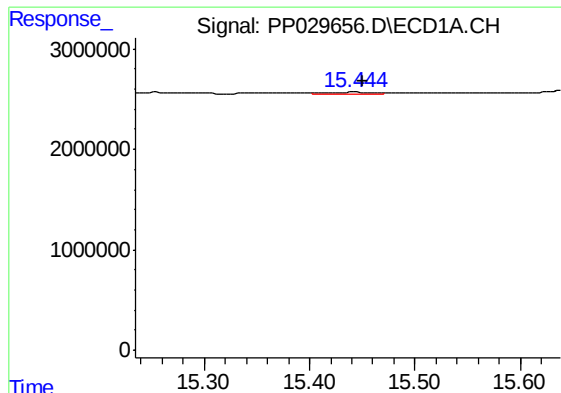

#12 2,4,5-T


R.T.: 15.444 min
Delta R.T.: -0.006 min
Response: 666807
Conc: 2.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118421BL

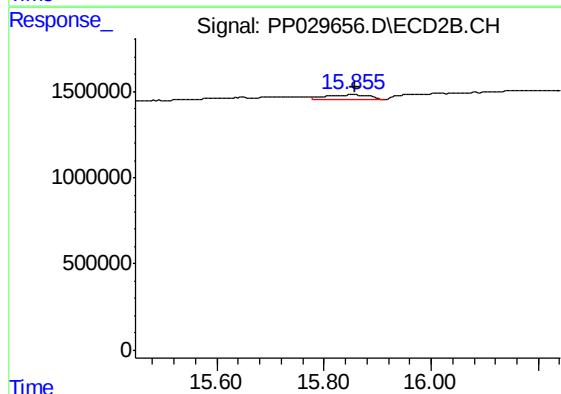


#12 2,4,5-T

R.T.: 15.856 min
Delta R.T.: -0.002 min
Response: 1758174
Conc: 10.61 ng/ml

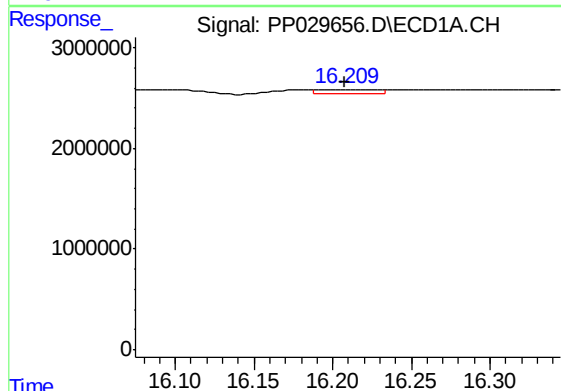


#13 2,4-DB

R.T.: 16.213 min
Delta R.T.: 0.006 min
Response: 1062571
Conc: 51.10 ng/ml

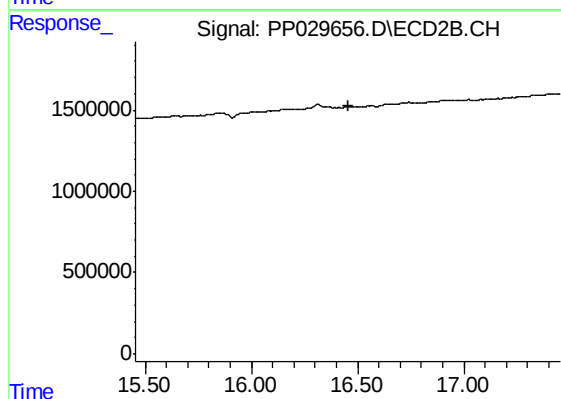

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

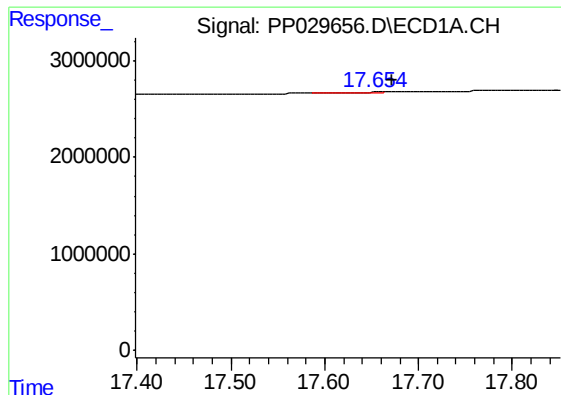

#14 DINOSEB


R.T.: 17.656 min
Delta R.T.: -0.016 min
Response: 107717
Conc: 0.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118421BL

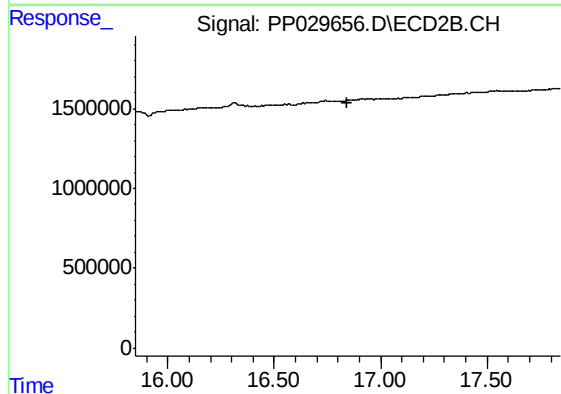


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.845 min
Response: 0
Conc: N.D.

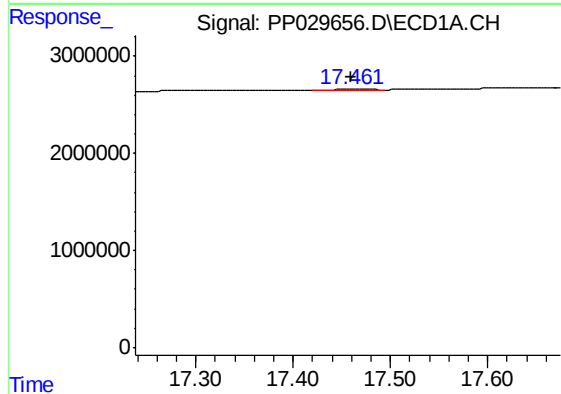


#15 Picloram

R.T.: 17.462 min
Delta R.T.: 0.002 min
Response: 198558
Conc: 0.61 ng/ml

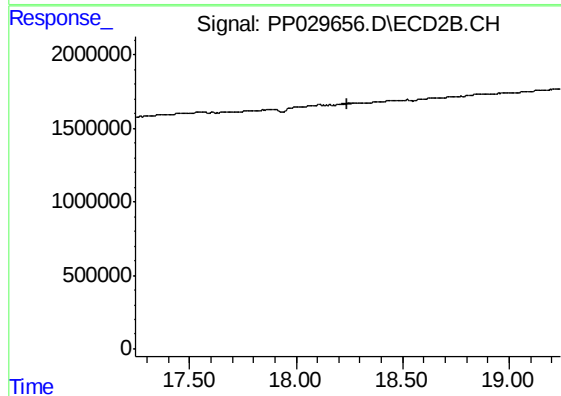

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 18.242 min
Response: 0
Conc: N.D.

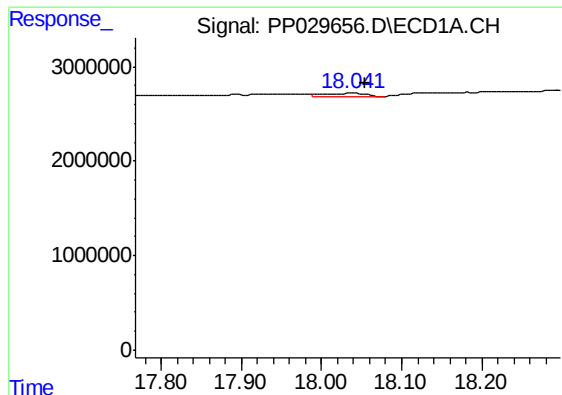

#16 DCPA

R.T.: 18.041 min
Delta R.T.: -0.013 min
Response: 1427657
Conc: 4.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118421BL

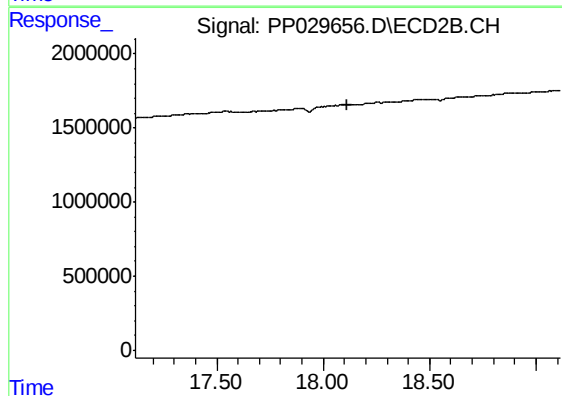

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.116 min
Response: 0
Conc: N.D.