

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
 Data File : PP029661.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 12:25
 Operator : EI\MA
 Sample : K1685-14
 Misc : hexane
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AU-06-032819-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:06:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.923	12.118	15022533	18422419	459.194	429.014
Target Compounds							
5) T	DICAMBA	12.265	0.000	299098	0	2.024	N.D. #
8) T	DICHLORPROP	0.000	13.552	0	577606	N.D.	14.263 #
9) T	2,4-D	13.717	0.000	195174	0	5.047	N.D. #
12) T	2,4,5-T	15.454	15.847	261207	544047	1.153	3.282 #
13) T	2,4-DB	16.222	0.000	453506	0	21.810	N.D. #
14) T	DINOSEB	17.669	16.890	238197	330419	1.413	2.187 #
15) T	Picloram	17.465	18.243	111803	1834227	0.341	7.696 #
16) T	DCPA	18.041	0.000	274658	0	0.866	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
Data File : PP029661.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 12:25
Operator : EI\MA
Sample : K1685-14
Misc : hexane
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
AU-06-032819-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:06:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

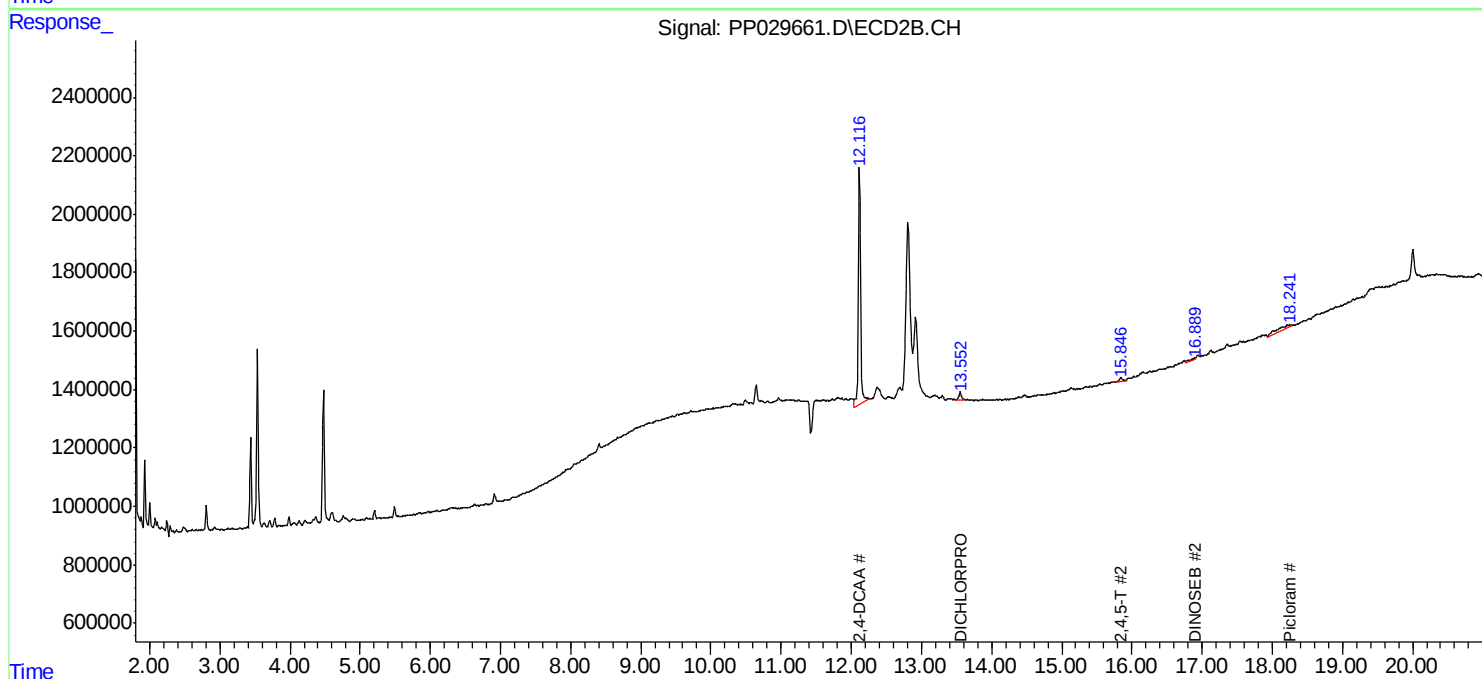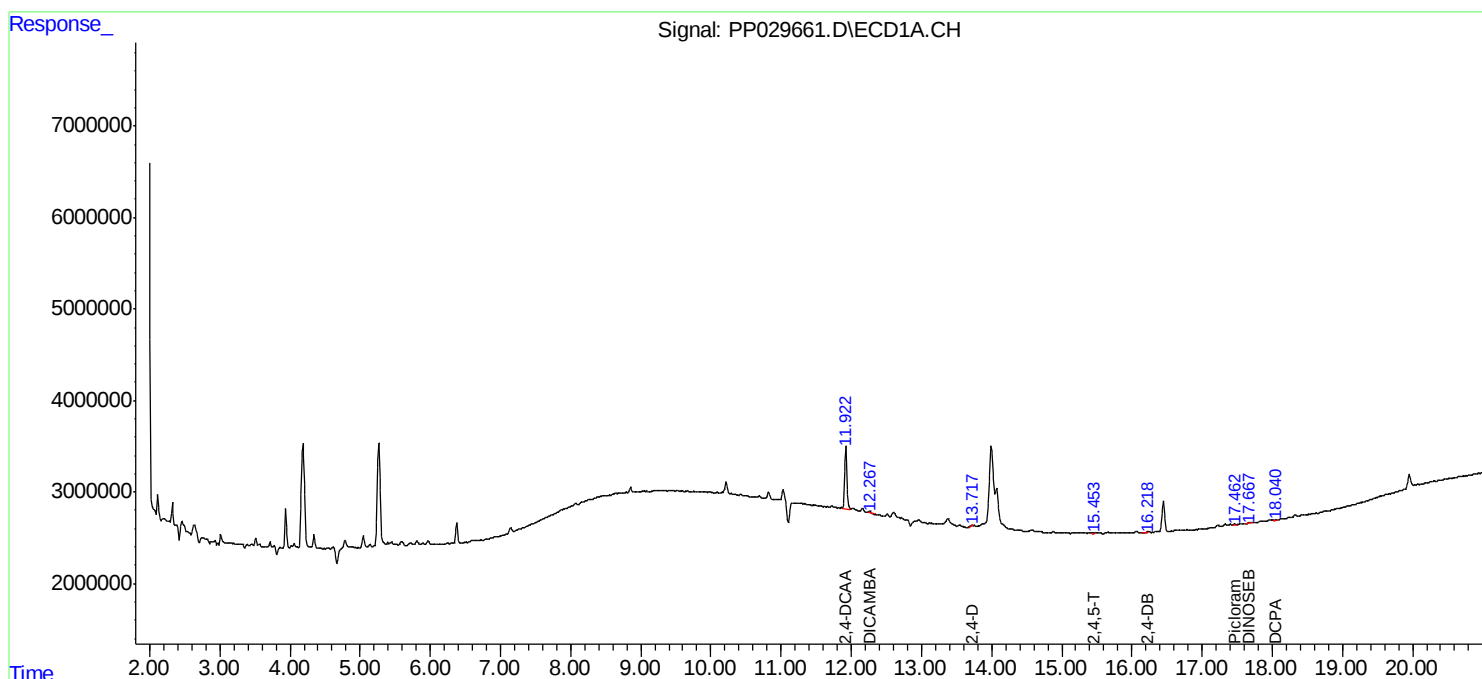


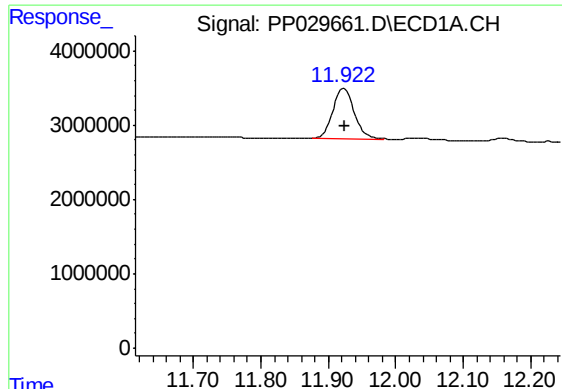

#4 2,4-DCAA


R.T.: 11.923 min
Delta R.T.: -0.002 min
Response: 15022533
Conc: 459.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
AU-06-032819-C

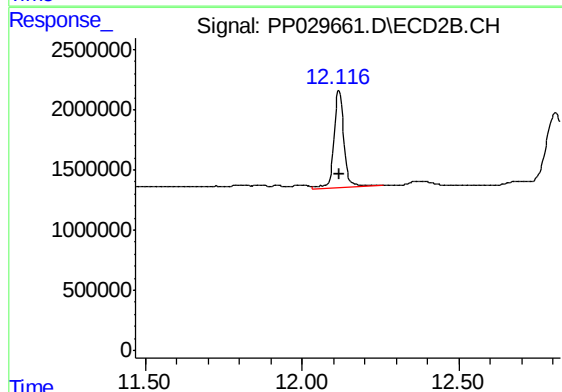


#4 2,4-DCAA

R.T.: 12.118 min
Delta R.T.: -0.003 min
Response: 18422419
Conc: 429.01 ng/ml

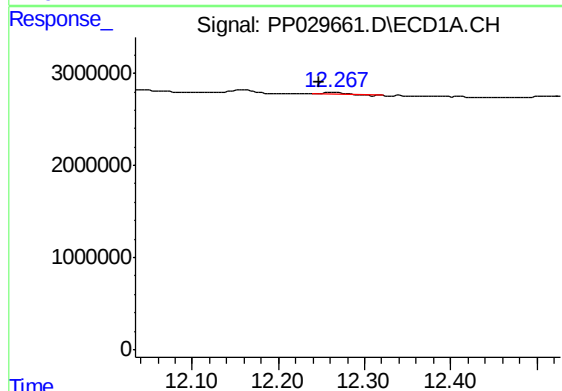


#5 DICAMBA

R.T.: 12.265 min
Delta R.T.: 0.018 min
Response: 299098
Conc: 2.02 ng/ml

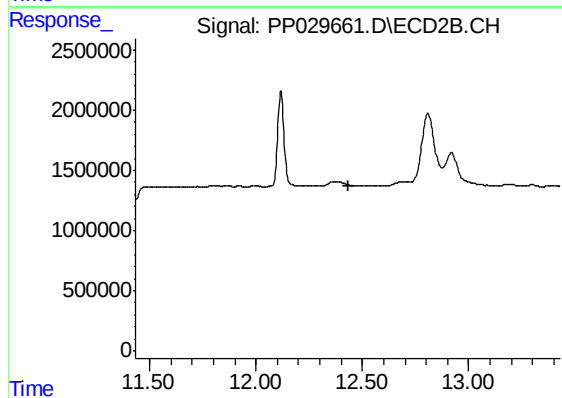

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 12.433 min
Response: 0
Conc: N.D.

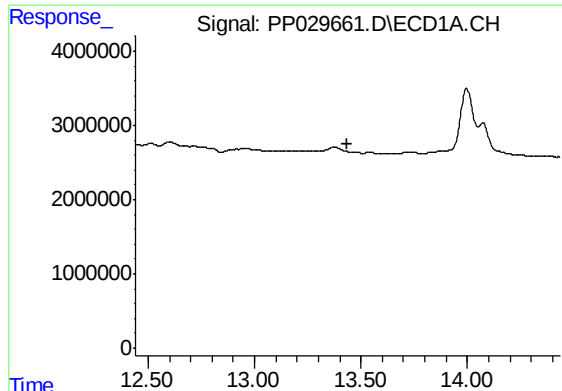

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AU-06-032819-C

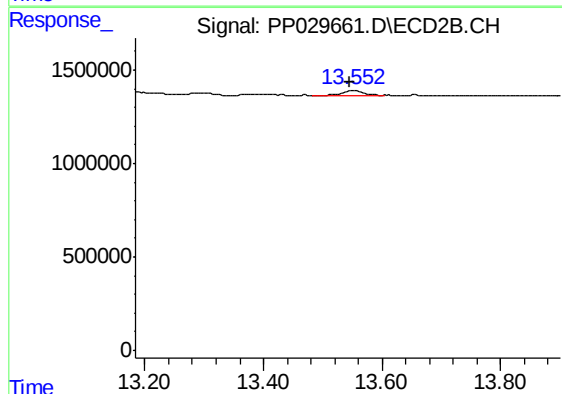


#8 DICHLORPROP

R.T.: 13.552 min
Delta R.T.: 0.007 min
Response: 577606
Conc: 14.26 ng/ml

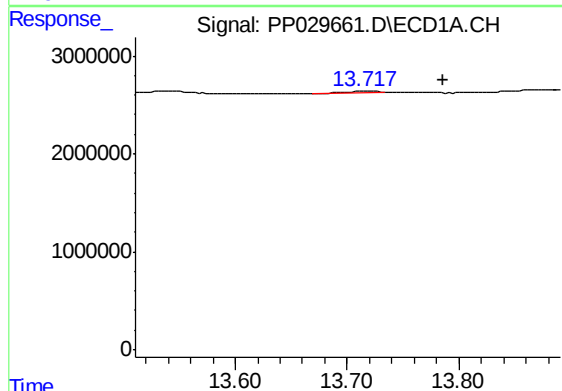


#9 2,4-D

R.T.: 13.717 min
Delta R.T.: -0.069 min
Response: 195174
Conc: 5.05 ng/ml

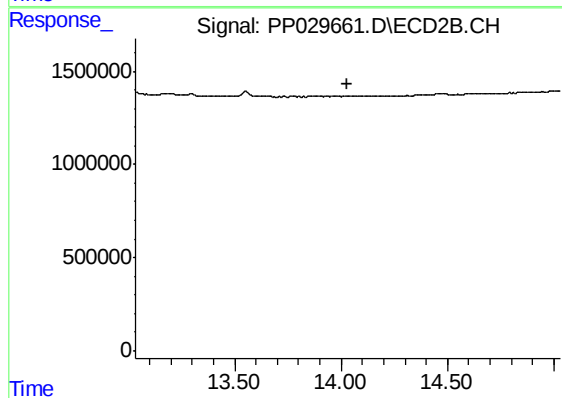

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 14.031 min
Response: 0
Conc: N.D.

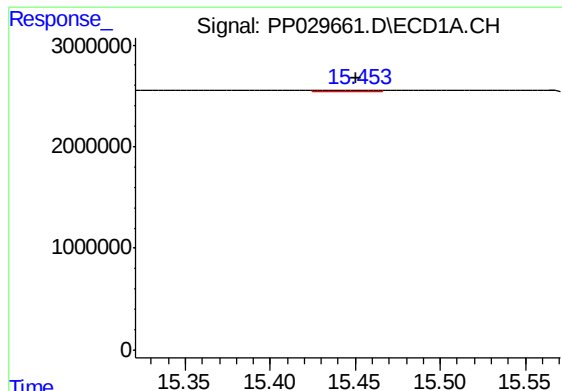

#12 2,4,5-T


R.T.: 15.454 min
Delta R.T.: 0.003 min
Response: 261207
Conc: 1.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
AU-06-032819-C

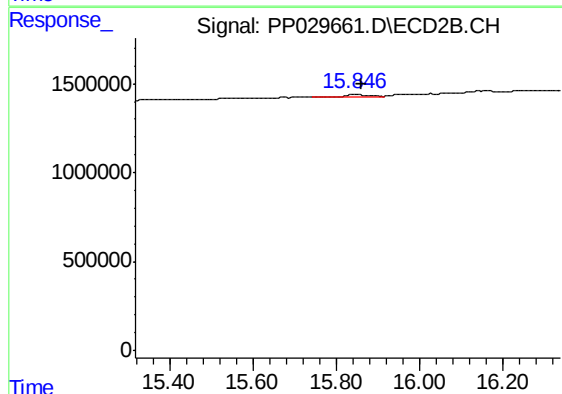


#12 2,4,5-T

R.T.: 15.847 min
Delta R.T.: -0.011 min
Response: 544047
Conc: 3.28 ng/ml

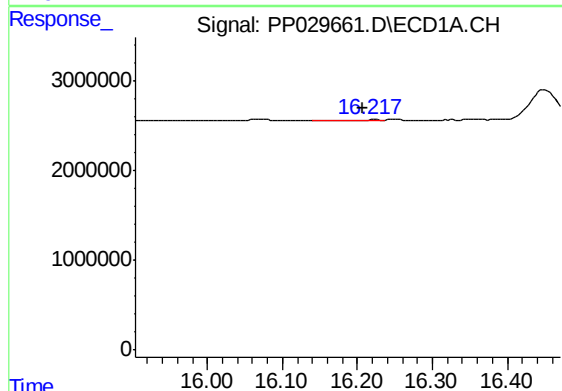


#13 2,4-DB

R.T.: 16.222 min
Delta R.T.: 0.015 min
Response: 453506
Conc: 21.81 ng/ml

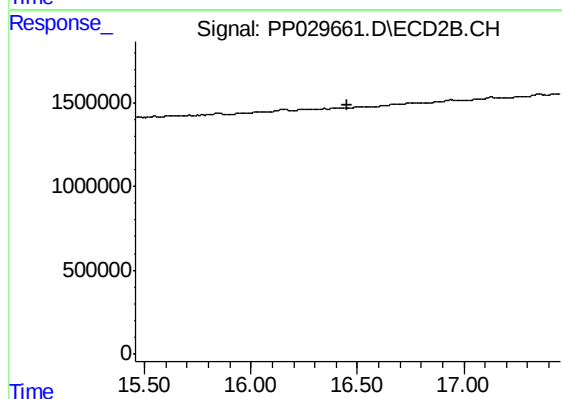

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

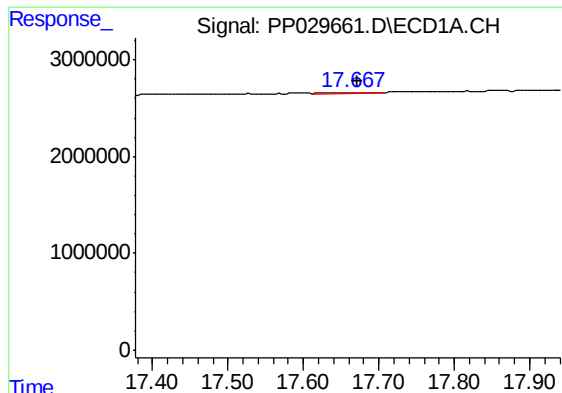

#14 DINOSEB


R.T.: 17.669 min
Delta R.T.: -0.003 min
Response: 238197
Conc: 1.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
AU-06-032819-C

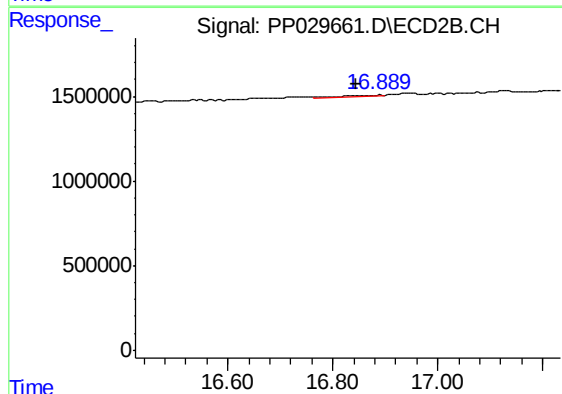


#14 DINOSEB

R.T.: 16.890 min
Delta R.T.: 0.045 min
Response: 330419
Conc: 2.19 ng/ml

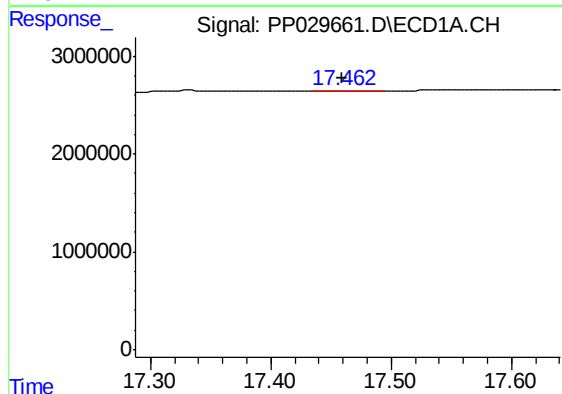


#15 Picloram

R.T.: 17.465 min
Delta R.T.: 0.005 min
Response: 111803
Conc: 0.34 ng/ml

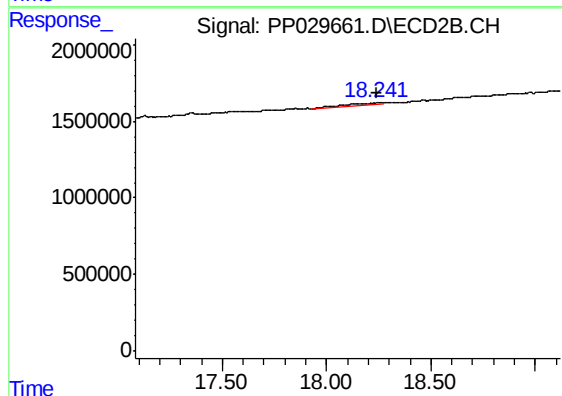

#15 Picloram


R.T.: 18.243 min
Delta R.T.: 0.000 min
Response: 1834227
Conc: 7.70 ng/ml

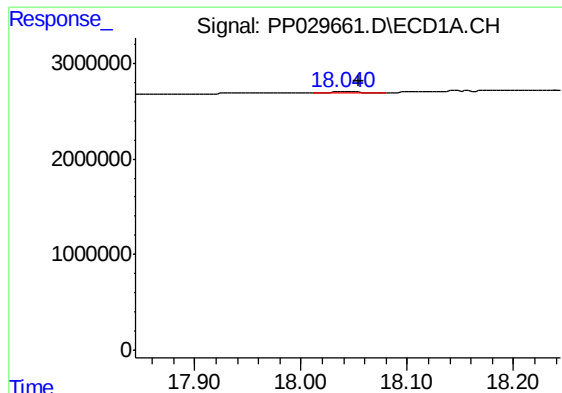

#16 DCPA

R.T.: 18.041 min
Delta R.T.: -0.013 min
Response: 274658
Conc: 0.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
AU-06-032819-C

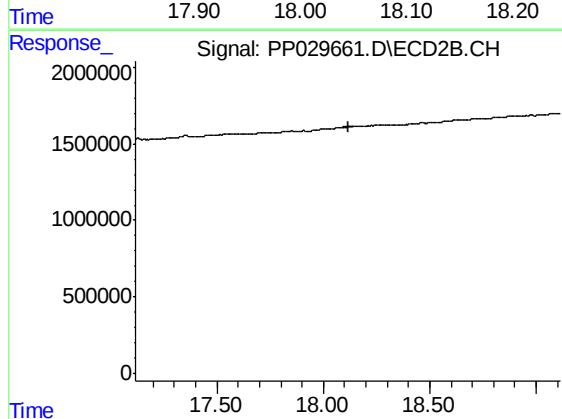

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.116 min
Response: 0
Conc: N.D.