

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
 Data File : PP029664.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 13:42
 Operator : EI\MA
 Sample : K2138-02
 Misc : hexane
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S6A(2-10)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:06:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.119	22806333	18925185	697.122	440.722 #
Target Compounds							
1) T	Dalapon	3.180	0.000	248449	0	3.706	N.D. #
8) T	DICHLORPROP	0.000	13.552	0	651249	N.D.	16.082 #
10) T	Pentachlo...	14.200	14.638	903374	341996	1.326	0.625 #
11) T	2,4,5-TP ...	0.000	15.195	0	5681278	N.D.	27.448 #
12) T	2,4,5-T	0.000	15.846	0	650111	N.D.	3.922 #
13) T	2,4-DB	16.219	0.000	243334	0	11.702	N.D. #
14) T	DINOSEB	17.616	0.000	38343	0	0.227	N.D. #
15) T	Picloram	17.455	18.239	687066	790652	2.097	3.317 #
16) T	DCPA	18.054	18.116	340551	821086	1.073	3.130 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
Data File : PP029664.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 13:42
Operator : EI\MA
Sample : K2138-02
Misc : hexane
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
S6A(2-10)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:06:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

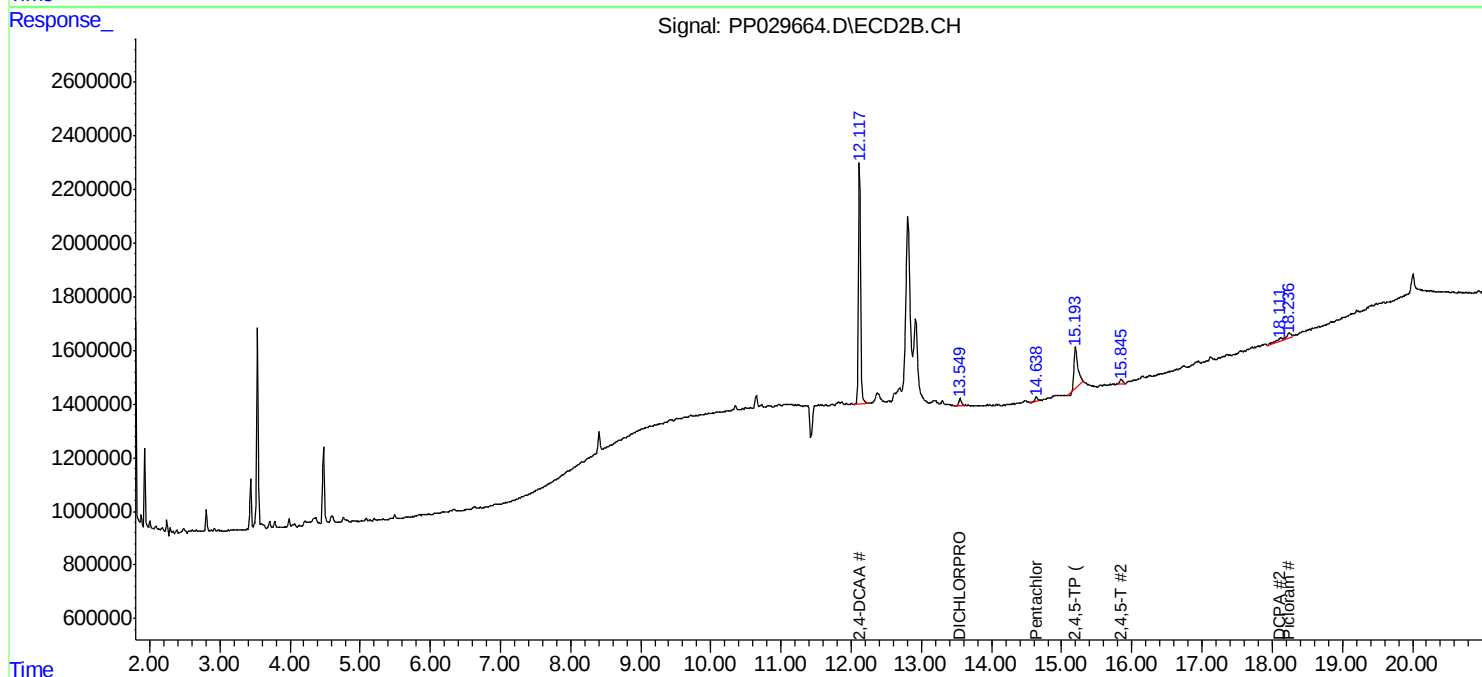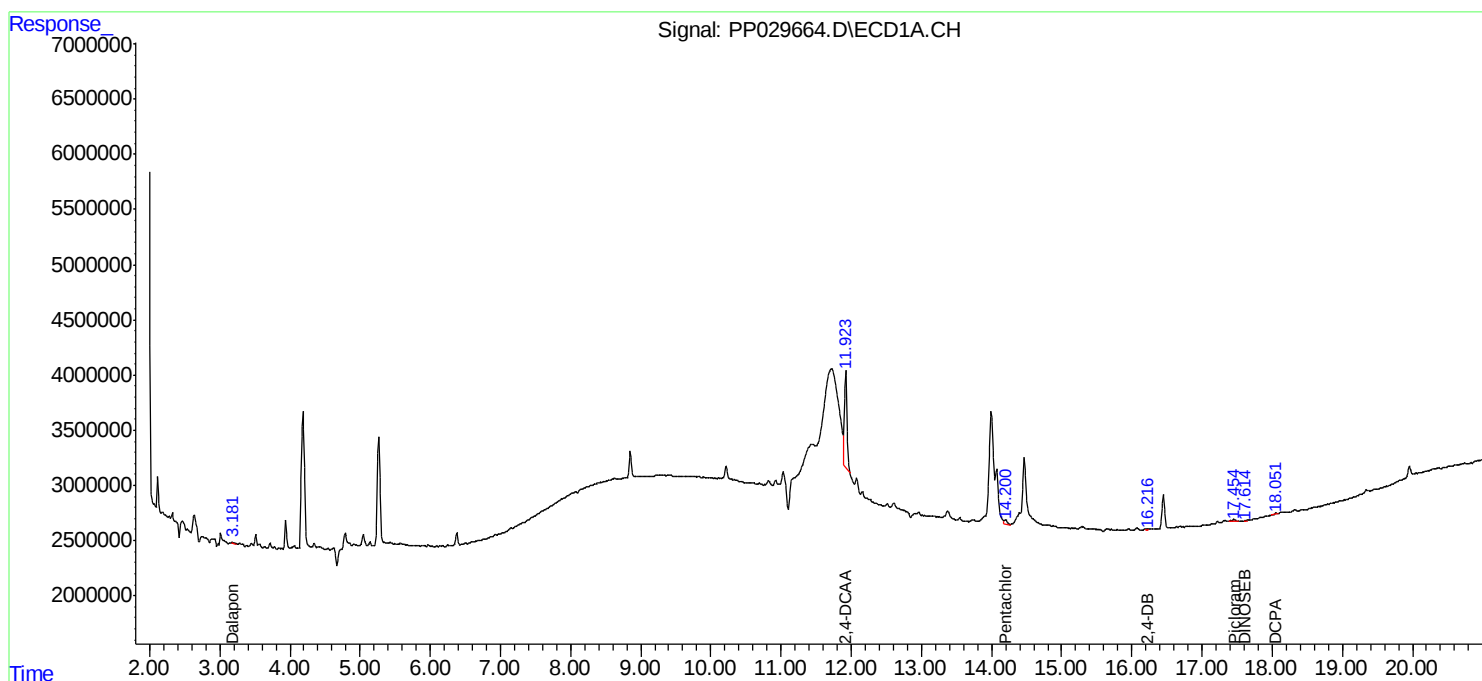


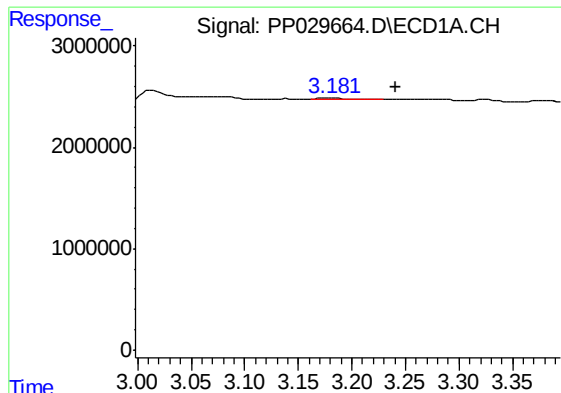

#1 Dalapon


R.T.: 3.180 min
Delta R.T.: -0.062 min
Response: 248449
Conc: 3.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6A(2-10)COMP

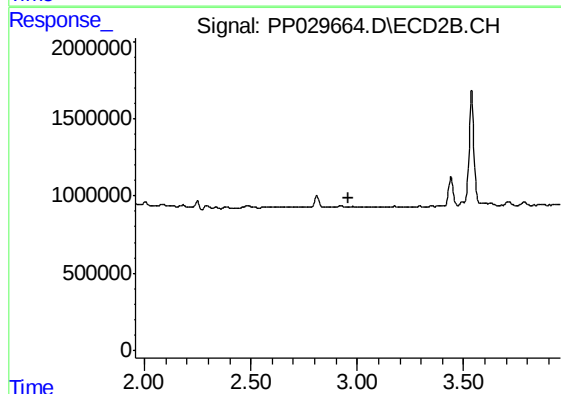


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.956 min
Response: 0
Conc: N.D.

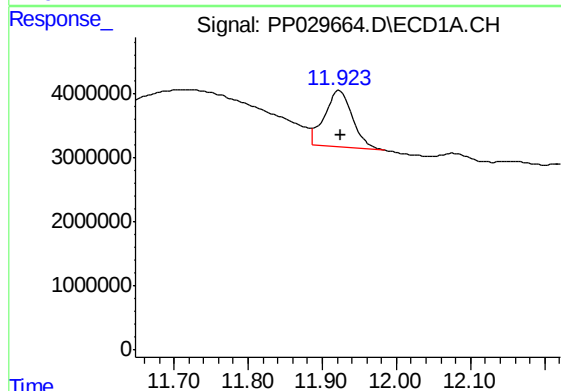


#4 2,4-DCAA

R.T.: 11.924 min
Delta R.T.: -0.001 min
Response: 22806333
Conc: 697.12 ng/ml

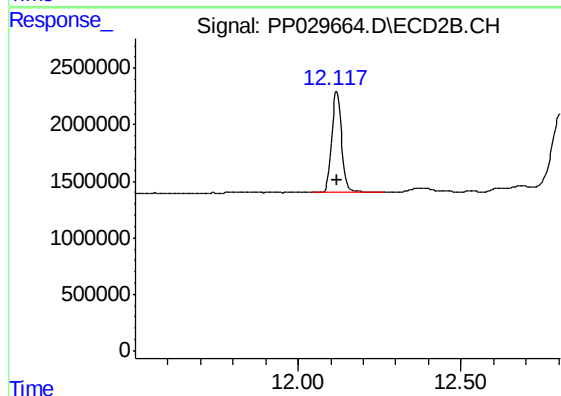

#4 2,4-DCAA


R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 18925185
Conc: 440.72 ng/ml

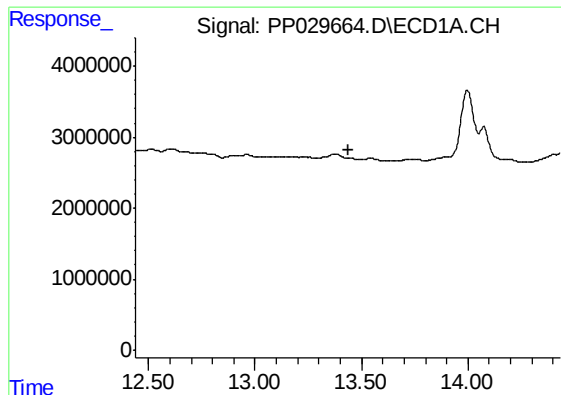

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S6A(2-10)COMP

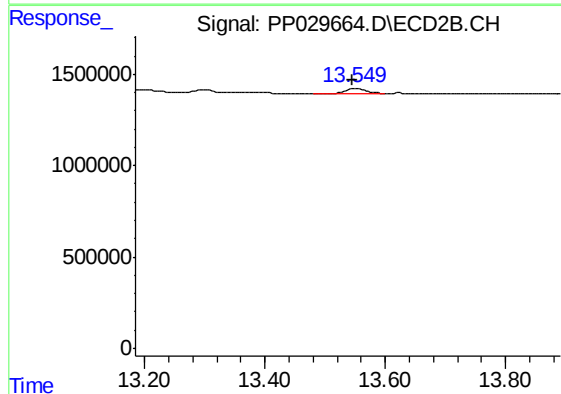


#8 DICHLORPROP

R.T.: 13.552 min
Delta R.T.: 0.007 min
Response: 651249
Conc: 16.08 ng/ml

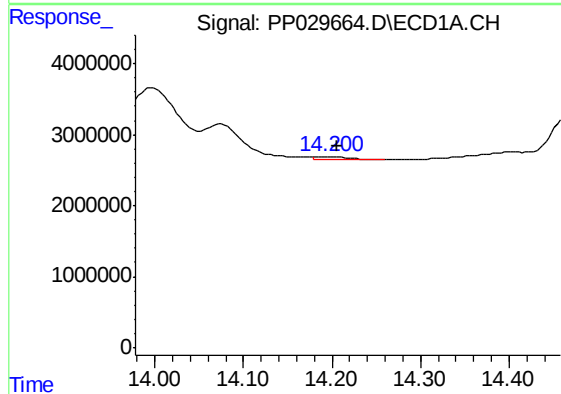


#10 Pentachlorophenol

R.T.: 14.200 min
Delta R.T.: -0.005 min
Response: 903374
Conc: 1.33 ng/ml

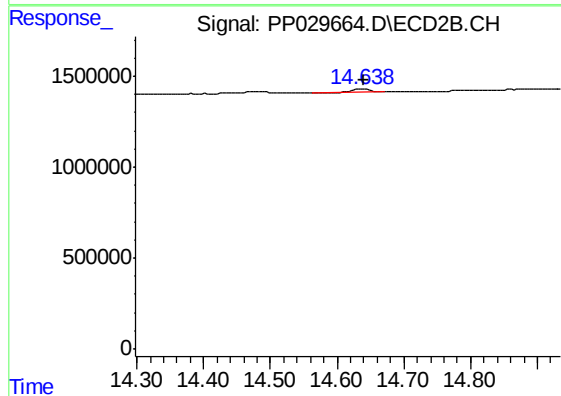

#10 Pentachlorophenol


R.T.: 14.638 min
Delta R.T.: -0.002 min
Response: 341996
Conc: 0.63 ng/ml

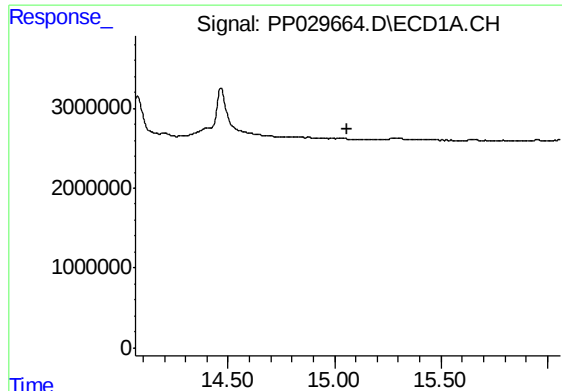

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 15.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S6A(2-10)COMP

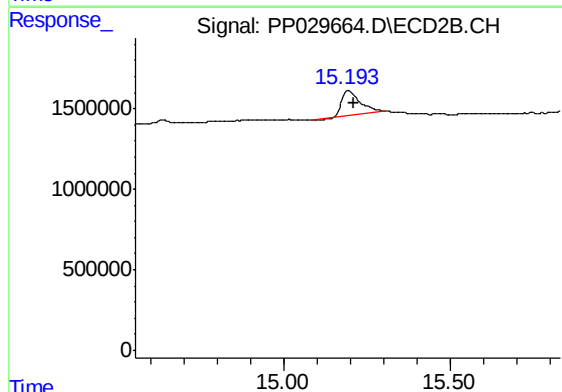


#11 2,4,5-TP (SILVEX)

R.T.: 15.195 min
Delta R.T.: -0.015 min
Response: 5681278
Conc: 27.45 ng/ml

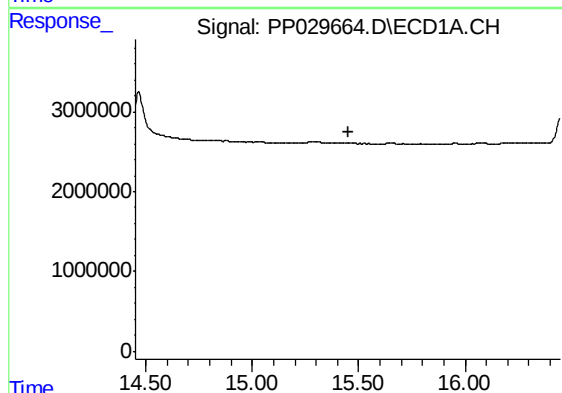


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.451 min
Response: 0
Conc: N.D.

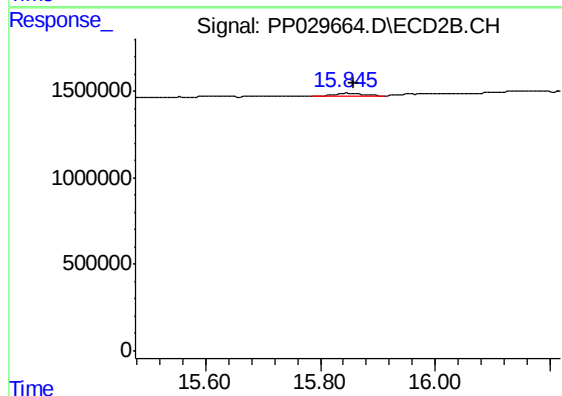

#12 2,4,5-T


R.T.: 15.846 min
Delta R.T.: -0.013 min
Response: 650111
Conc: 3.92 ng/ml

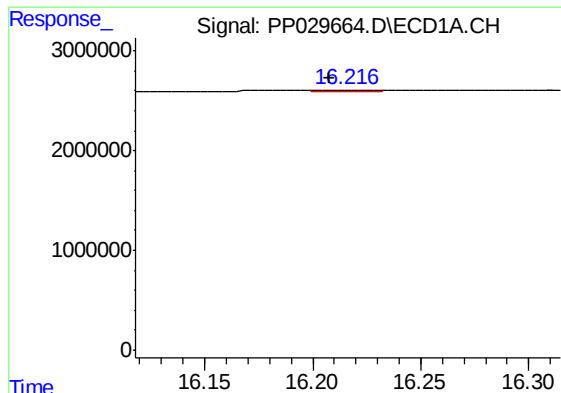

#13 2,4-DB


R.T.: 16.219 min
Delta R.T.: 0.012 min
Response: 243334
Conc: 11.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6A(2-10)COMP

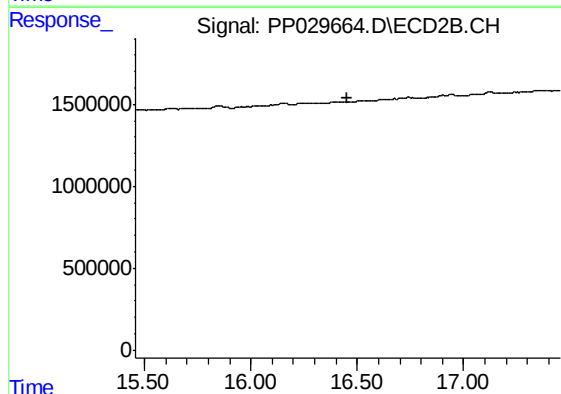


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

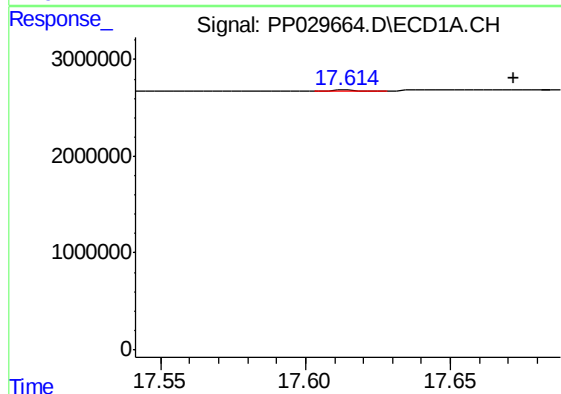


#14 DINOSEB

R.T.: 17.616 min
Delta R.T.: -0.056 min
Response: 38343
Conc: 0.23 ng/ml

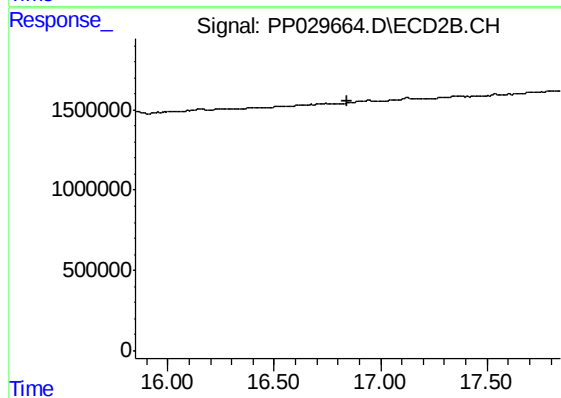

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.845 min
Response: 0
Conc: N.D.

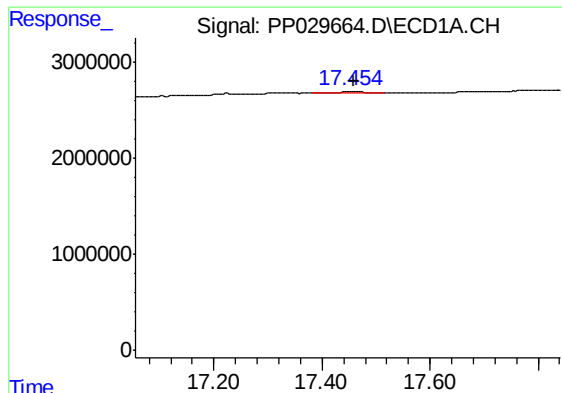

#15 Picloram


R.T.: 17.455 min
Delta R.T.: -0.004 min
Response: 687066
Conc: 2.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6A(2-10)COMP

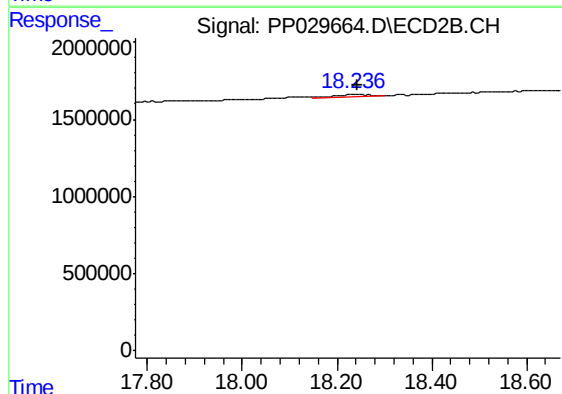


#15 Picloram

R.T.: 18.239 min
Delta R.T.: -0.003 min
Response: 790652
Conc: 3.32 ng/ml

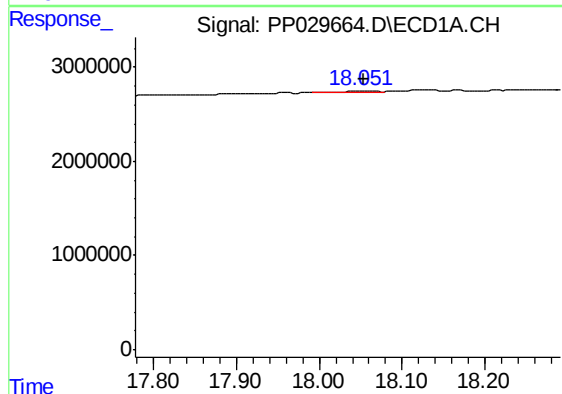

#16 DCPA

R.T.: 18.054 min
Delta R.T.: 0.000 min
Response: 340551
Conc: 1.07 ng/ml

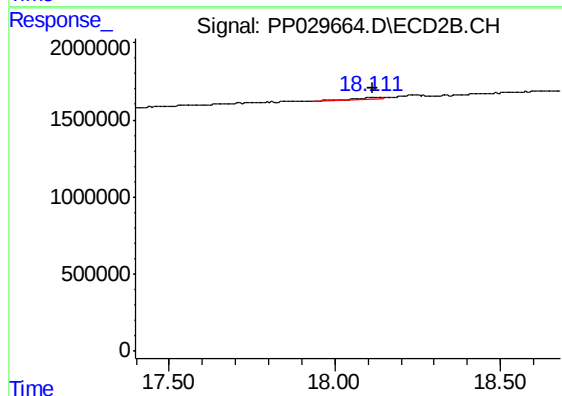

#16 DCPA

R.T.: 18.116 min
Delta R.T.: 0.000 min
Response: 821086
Conc: 3.13 ng/ml