

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
 Data File : PP029665.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 14:07
 Operator : EI\MA
 Sample : K2138-04
 Misc : hexane
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S6A(12-20)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:07:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.119	18188874	18984977	555.980	442.114
Target Compounds							
5) T	DICAMBA	12.224	0.000	416038	0	2.816	N.D. #
8) T	DICHLORPROP	0.000	13.552	0	623698	N.D.	15.401 #
9) T	2,4-D	0.000	14.065	0	297939	N.D.	6.316 #
10) T	Pentachlo...	0.000	14.635	0	168077	N.D.	0.307 #
11) T	2,4,5-TP ...	0.000	15.196	0	4142033	N.D.	20.011 #
12) T	2,4,5-T	0.000	15.852	0	480837	N.D.	2.901 #
13) T	2,4-DB	16.236	0.000	668814	0	32.164	N.D. #
14) T	DINOSEB	0.000	16.866	0	311816	N.D.	2.064 #
15) T	Picloram	17.471	18.254	235965	279226	0.720	1.172 #
16) T	DCPA	18.054	18.124	400179	69950	1.261	0.267 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
Data File : PP029665.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 14:07
Operator : EI\MA
Sample : K2138-04
Misc : hexane
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
S6A(12-20)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:07:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

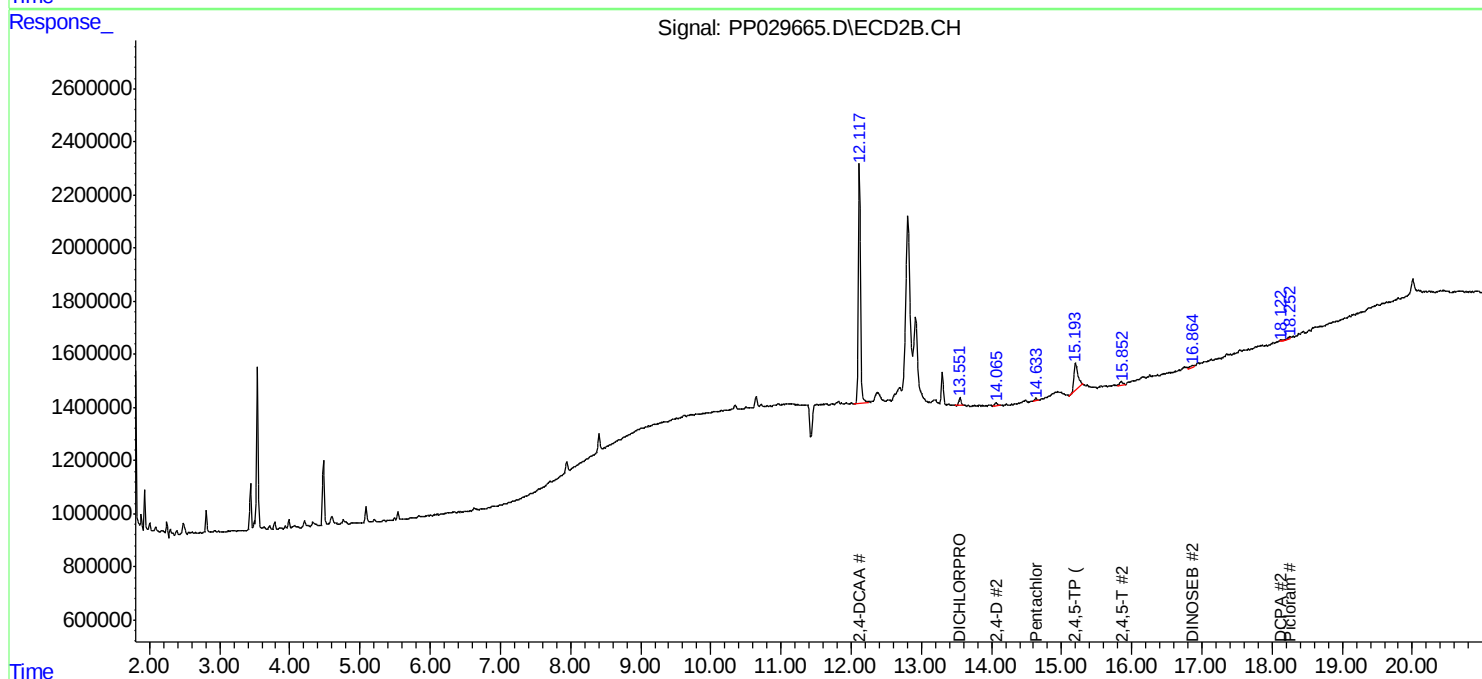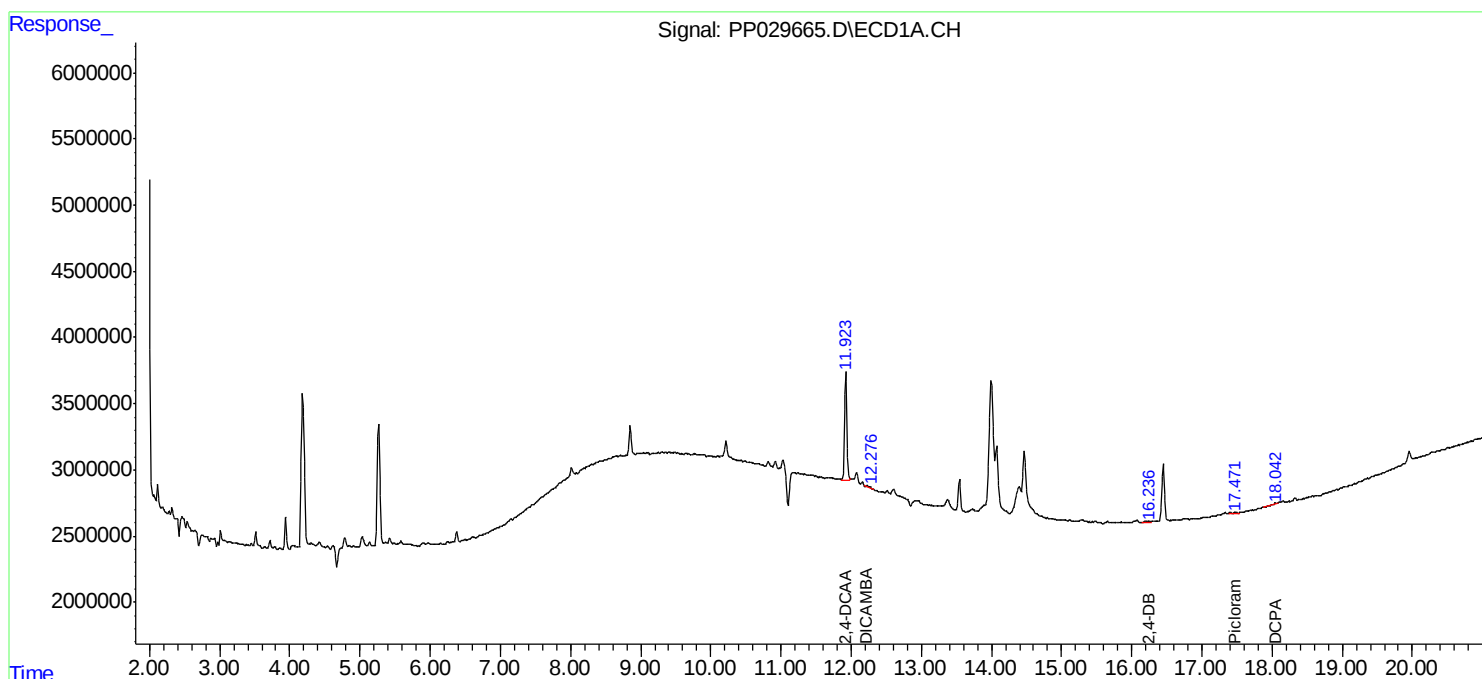


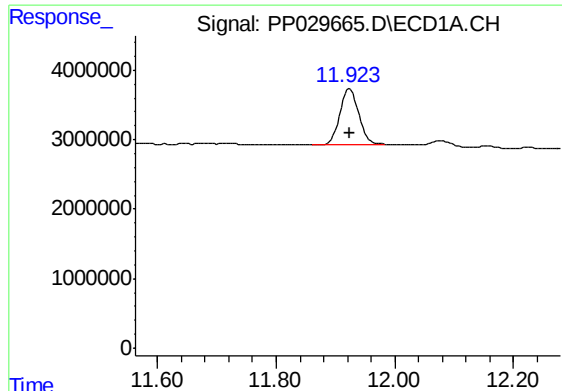

#4 2,4-DCAA


R.T.: 11.924 min
Delta R.T.: 0.000 min
Response: 18188874
Conc: 555.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6A(12-20)COMP

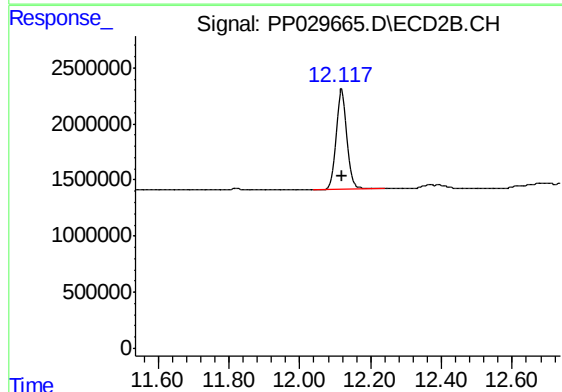


#4 2,4-DCAA

R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 18984977
Conc: 442.11 ng/ml

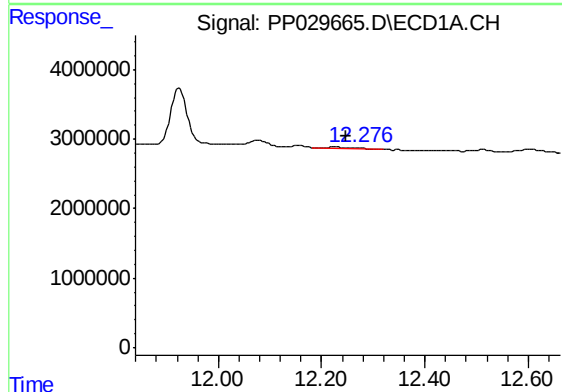


#5 DICAMBA

R.T.: 12.224 min
Delta R.T.: -0.023 min
Response: 416038
Conc: 2.82 ng/ml

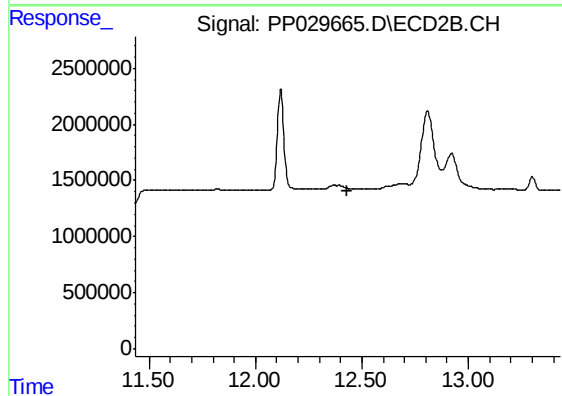

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.433 min
Response: 0
Conc: N.D.

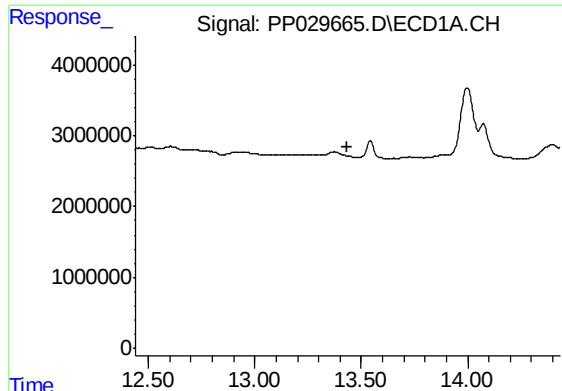

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S6A(12-20)COMP

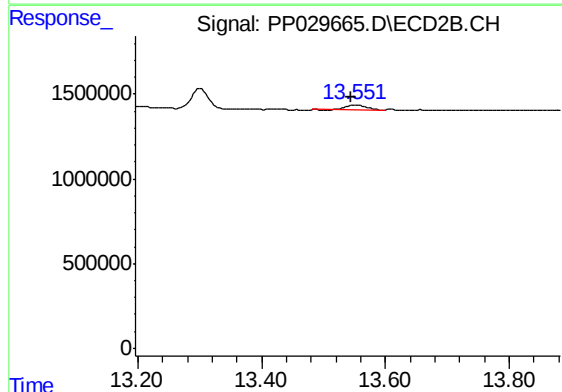


#8 DICHLORPROP

R.T.: 13.552 min
Delta R.T.: 0.007 min
Response: 623698
Conc: 15.40 ng/ml

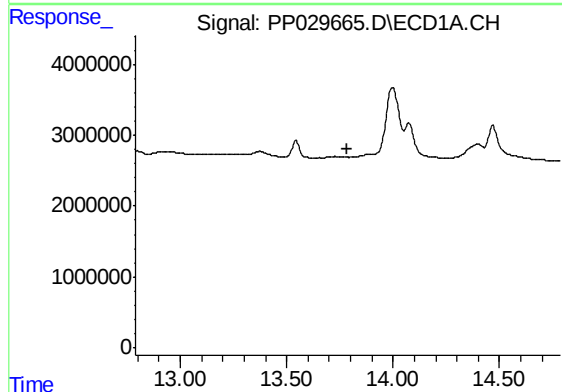


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.786 min
Response: 0
Conc: N.D.

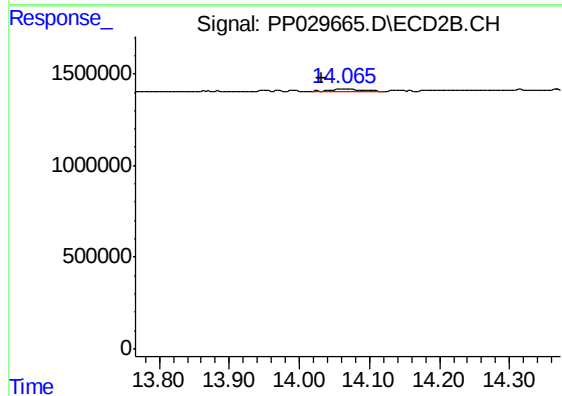

#9 2,4-D


R.T.: 14.065 min
Delta R.T.: 0.033 min
Response: 297939
Conc: 6.32 ng/ml

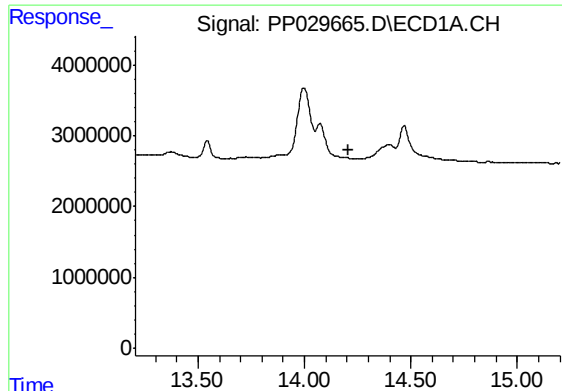

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 14.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S6A(12-20)COMP

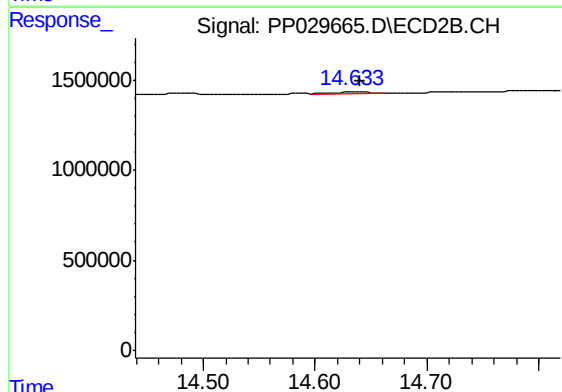


#10 Pentachlorophenol

R.T.: 14.635 min
Delta R.T.: -0.004 min
Response: 168077
Conc: 0.31 ng/ml

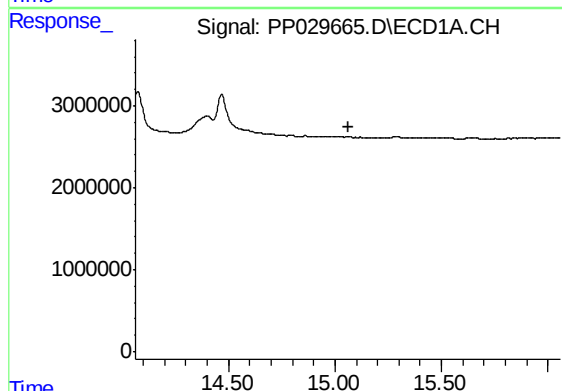


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.062 min
Response: 0
Conc: N.D.

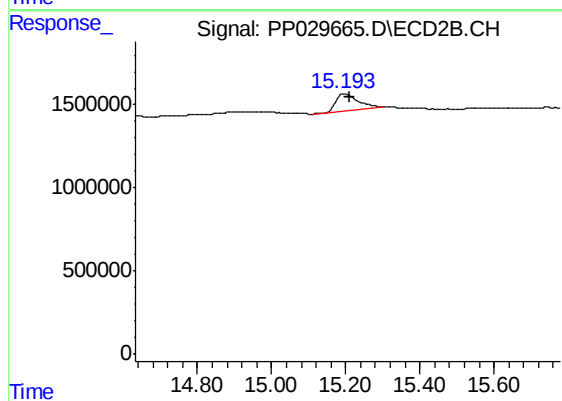

#11 2,4,5-TP (SILVEX)


R.T.: 15.196 min
Delta R.T.: -0.014 min
Response: 4142033
Conc: 20.01 ng/ml

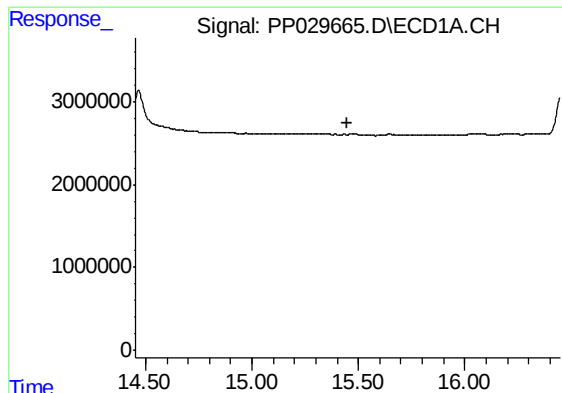

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S6A(12-20)COMP

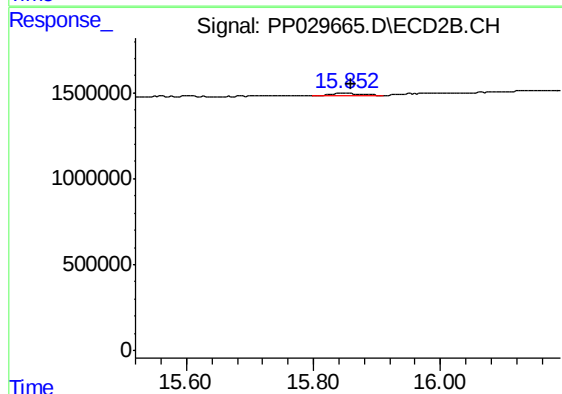


#12 2,4,5-T

R.T.: 15.852 min
Delta R.T.: -0.006 min
Response: 480837
Conc: 2.90 ng/ml

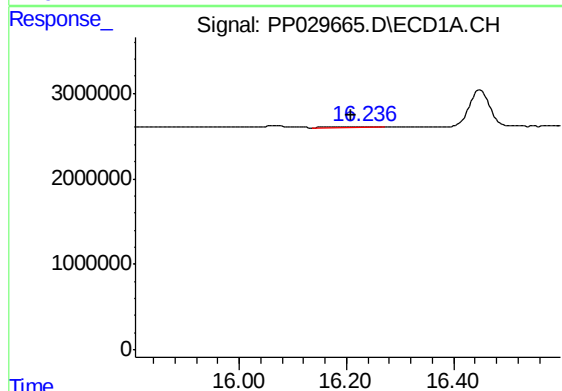


#13 2,4-DB

R.T.: 16.236 min
Delta R.T.: 0.028 min
Response: 668814
Conc: 32.16 ng/ml

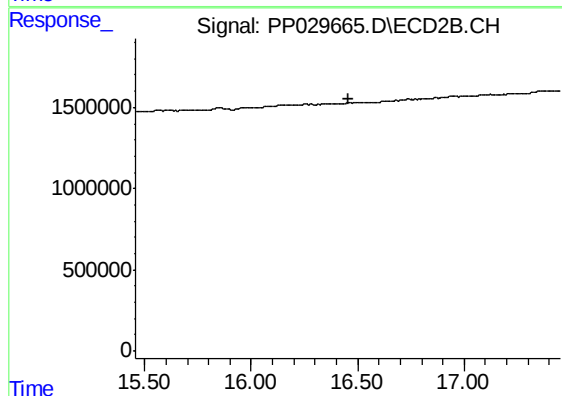

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.455 min
Response: 0
Conc: N.D.

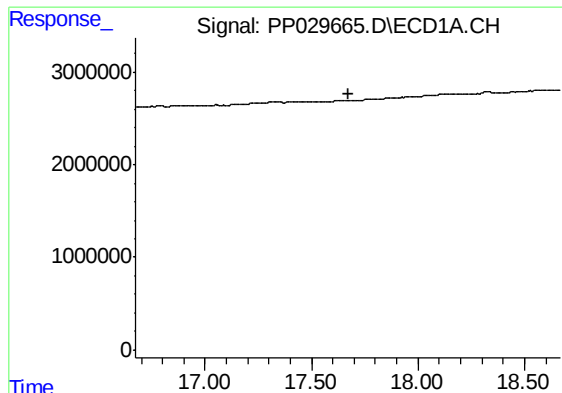

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.672 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S6A(12-20)COMP

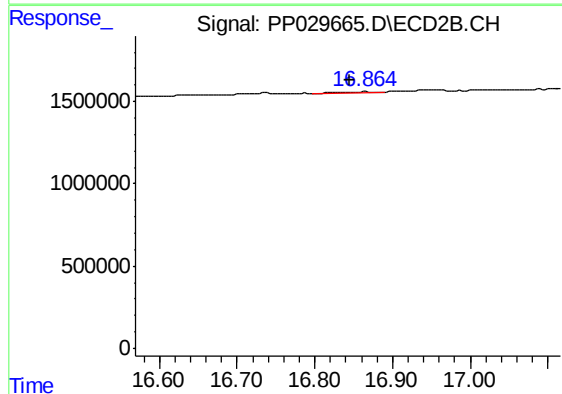


#14 DINOSEB

R.T.: 16.866 min
Delta R.T.: 0.021 min
Response: 311816
Conc: 2.06 ng/ml

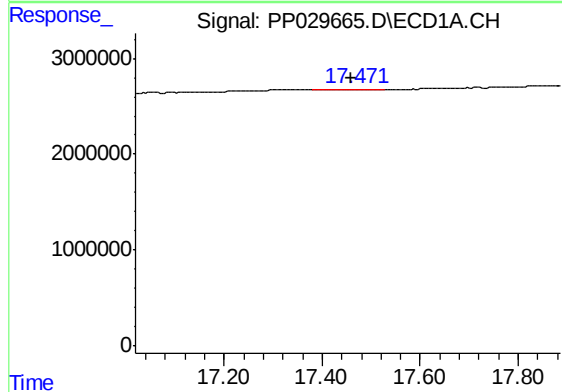


#15 Picloram

R.T.: 17.471 min
Delta R.T.: 0.011 min
Response: 235965
Conc: 0.72 ng/ml

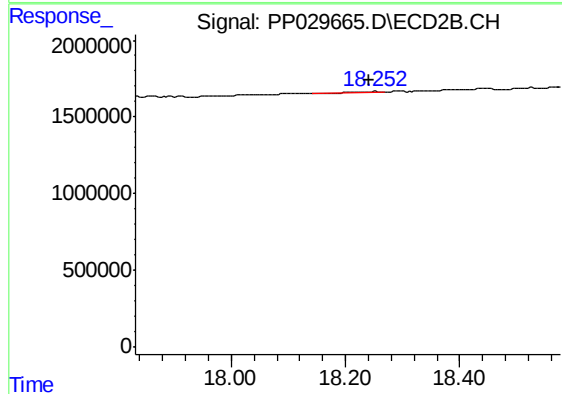

#15 Picloram


R.T.: 18.254 min
Delta R.T.: 0.012 min
Response: 279226
Conc: 1.17 ng/ml

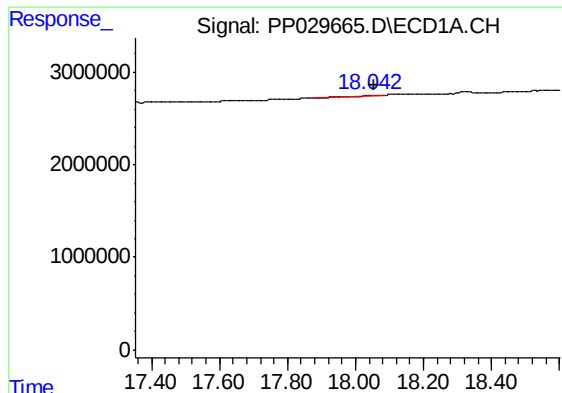

#16 DCPA

R.T.: 18.054 min
Delta R.T.: 0.000 min
Response: 400179
Conc: 1.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6A(12-20)COMP

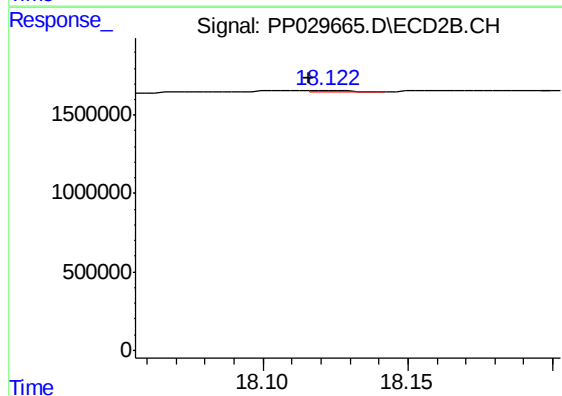

#16 DCPA

R.T.: 18.124 min
Delta R.T.: 0.008 min
Response: 69950
Conc: 0.27 ng/ml