

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
 Data File : PP029669.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 15:49
 Operator : EI\MA
 Sample : K2138-08
 Misc : hexane
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S6B(2-10)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:08:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.925	12.119	16877551	18458705	515.896	429.859
Target Compounds							
5) T	DICAMBA	12.217	0.000	462317	0	3.129	N.D. #
8) T	DICHLORPROP	0.000	13.551	0	714849	N.D.	17.652 #
9) T	2,4-D	13.723	0.000	61648	0	1.594	N.D. #
11) T	2,4,5-TP ...	0.000	15.201	0	761106	N.D.	3.677 #
12) T	2,4,5-T	0.000	15.851	0	488576	N.D.	2.947 #
13) T	2,4-DB	16.216	0.000	817794	0	39.328	N.D. #
14) T	DINOSEB	17.691	16.845	162334	103258	0.963	0.683 #
15) T	Picloram	17.471	18.242	217562	403433	0.664	1.693 #
16) T	DCPA	18.050	18.116	1126057	532024	3.549	2.028 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
Data File : PP029669.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 15:49
Operator : EI\MA
Sample : K2138-08
Misc : hexane
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
S6B(2-10)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:08:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

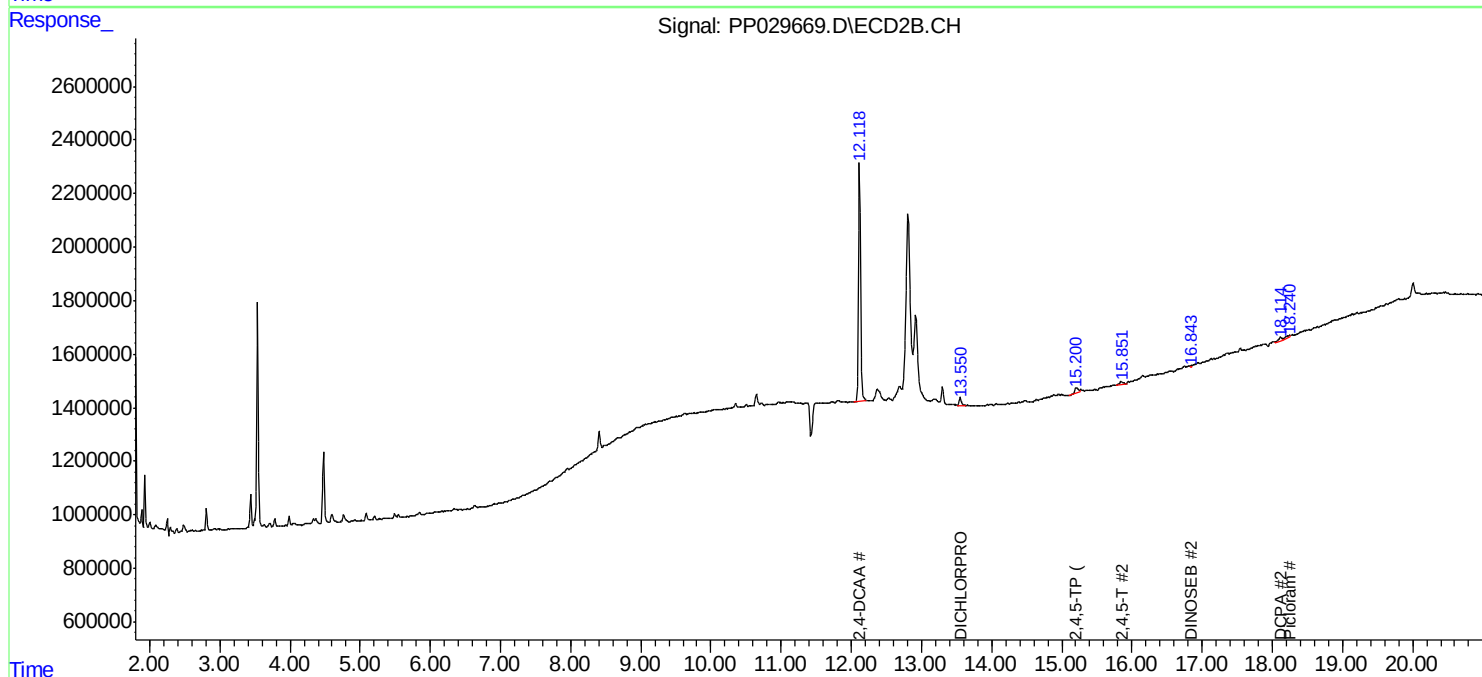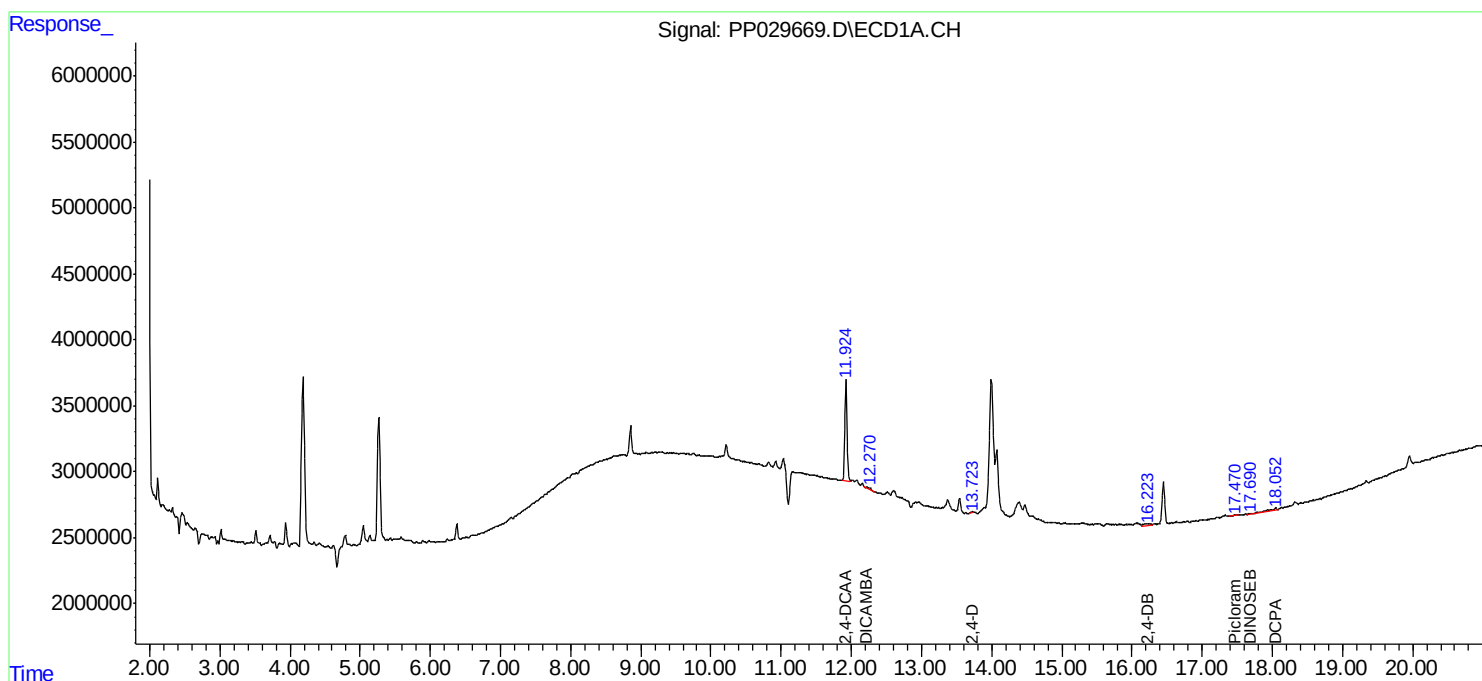


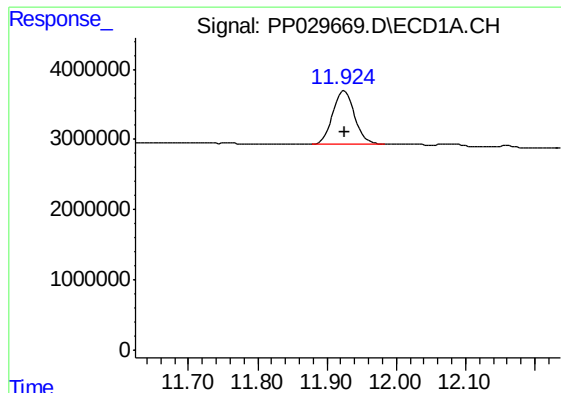

#4 2,4-DCAA


R.T.: 11.925 min
Delta R.T.: 0.000 min
Response: 16877551
Conc: 515.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6B(2-10)COMP

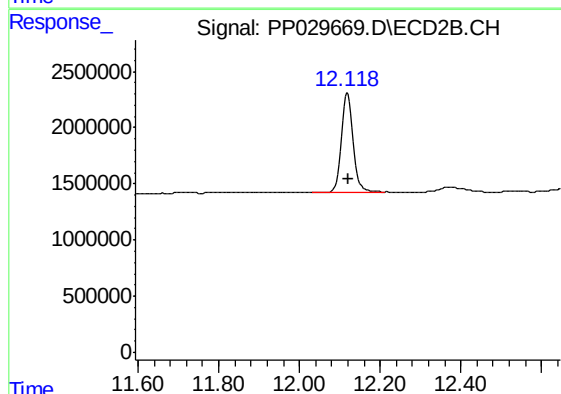


#4 2,4-DCAA

R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 18458705
Conc: 429.86 ng/ml

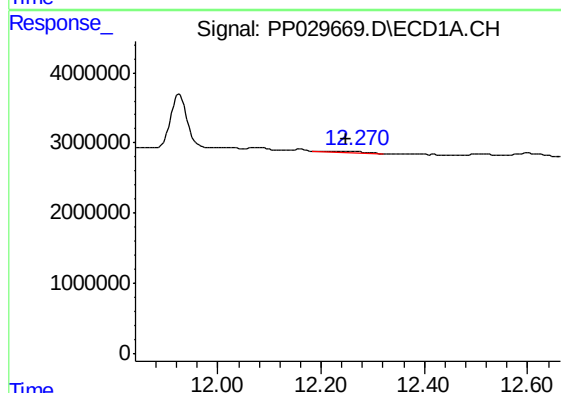


#5 DICAMBA

R.T.: 12.217 min
Delta R.T.: -0.030 min
Response: 462317
Conc: 3.13 ng/ml

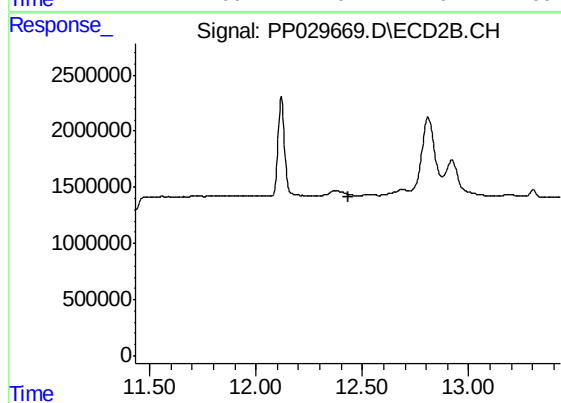

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 12.433 min
Response: 0
Conc: N.D.

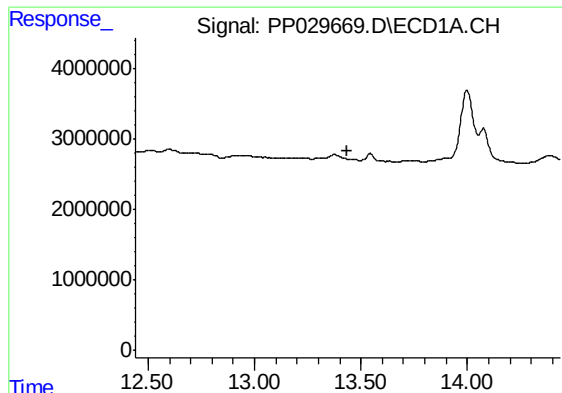

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S6B(2-10)COMP

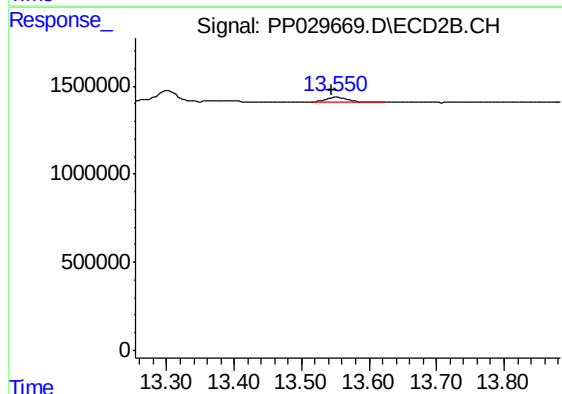


#8 DICHLORPROP

R.T.: 13.551 min
Delta R.T.: 0.007 min
Response: 714849
Conc: 17.65 ng/ml

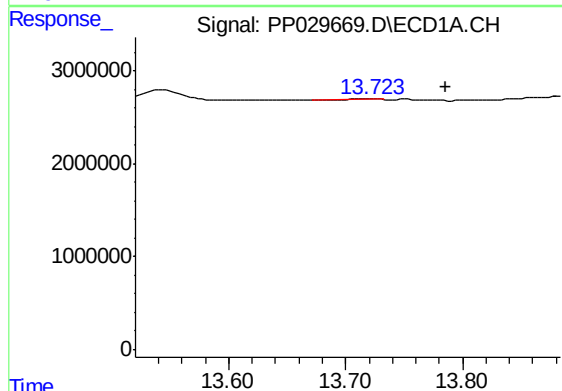


#9 2,4-D

R.T.: 13.723 min
Delta R.T.: -0.063 min
Response: 61648
Conc: 1.59 ng/ml

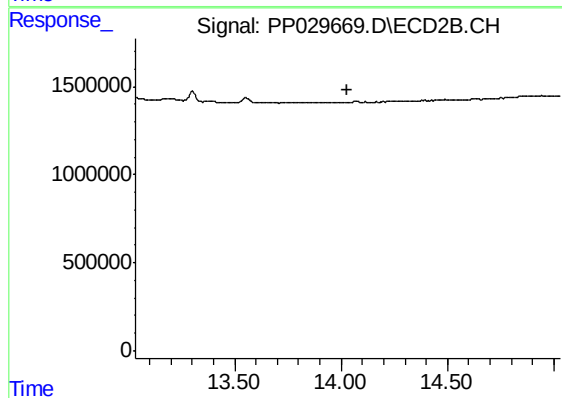

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 14.031 min
Response: 0
Conc: N.D.

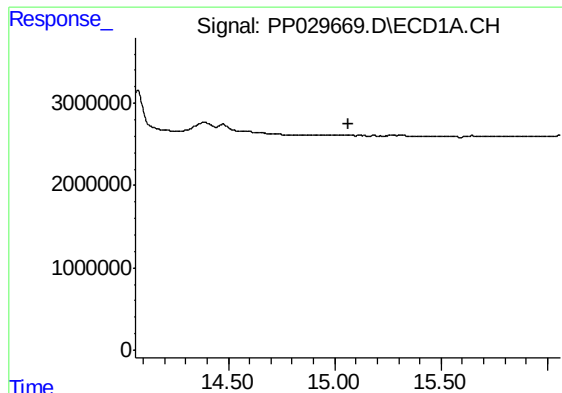

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S6B(2-10)COMP

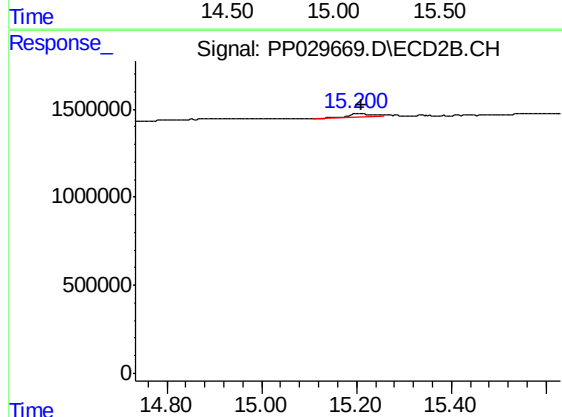


#11 2,4,5-TP (SILVEX)

R.T.: 15.201 min
Delta R.T.: -0.009 min
Response: 761106
Conc: 3.68 ng/ml

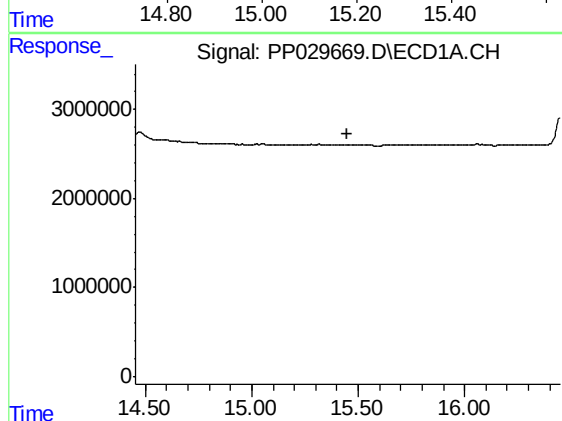


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

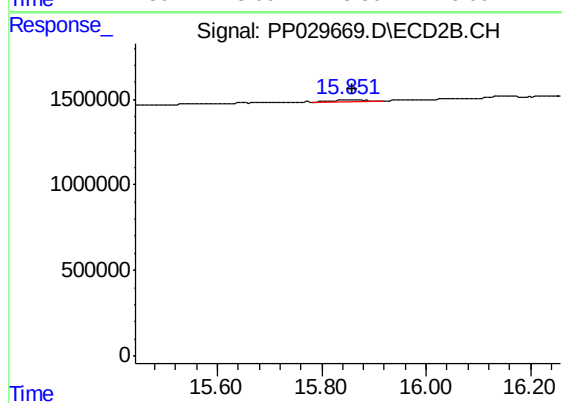

#12 2,4,5-T


R.T.: 15.851 min
Delta R.T.: -0.007 min
Response: 488576
Conc: 2.95 ng/ml

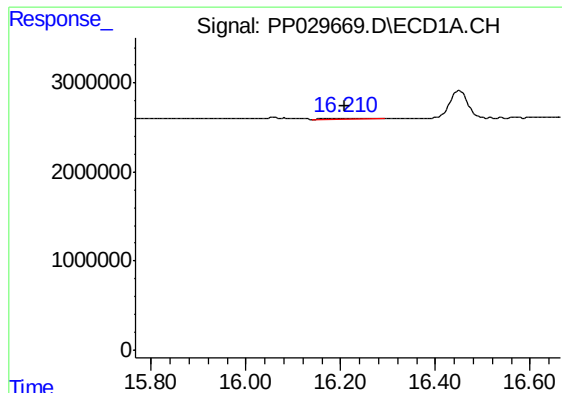

#13 2,4-DB


R.T.: 16.216 min
Delta R.T.: 0.008 min
Response: 817794
Conc: 39.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6B(2-10)COMP

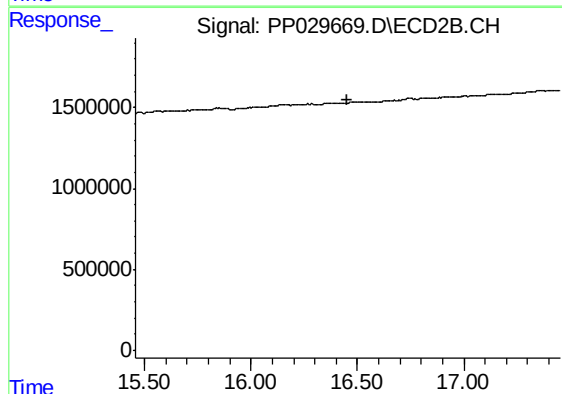


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

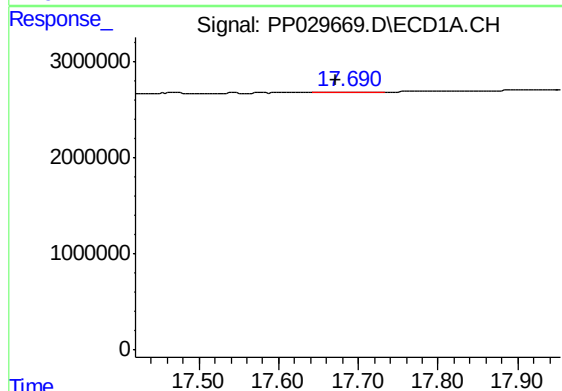


#14 DINOSEB

R.T.: 17.691 min
Delta R.T.: 0.019 min
Response: 162334
Conc: 0.96 ng/ml

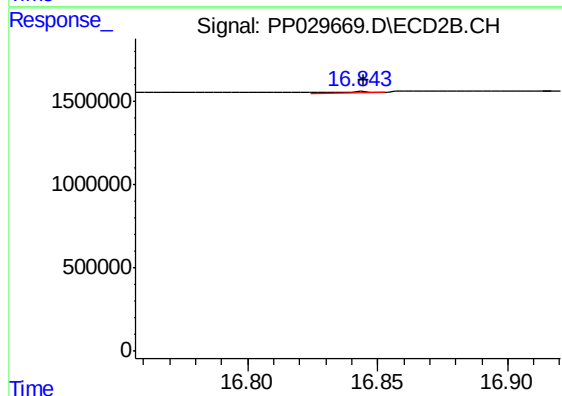

#14 DINOSEB


R.T.: 16.845 min
Delta R.T.: 0.000 min
Response: 103258
Conc: 0.68 ng/ml

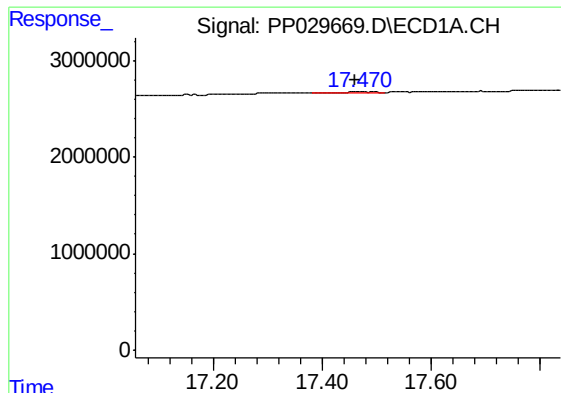

#15 Picloram


R.T.: 17.471 min
Delta R.T.: 0.012 min
Response: 217562
Conc: 0.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6B(2-10)COMP

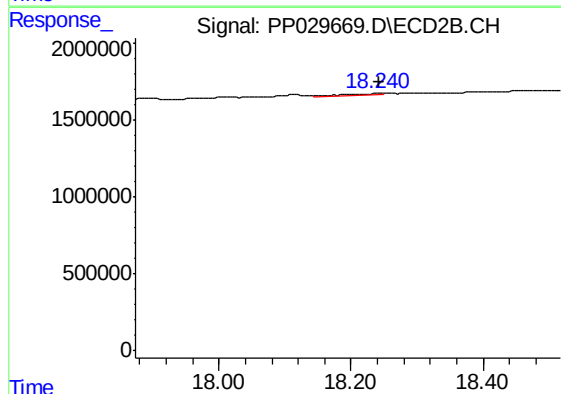


#15 Picloram

R.T.: 18.242 min
Delta R.T.: 0.000 min
Response: 403433
Conc: 1.69 ng/ml

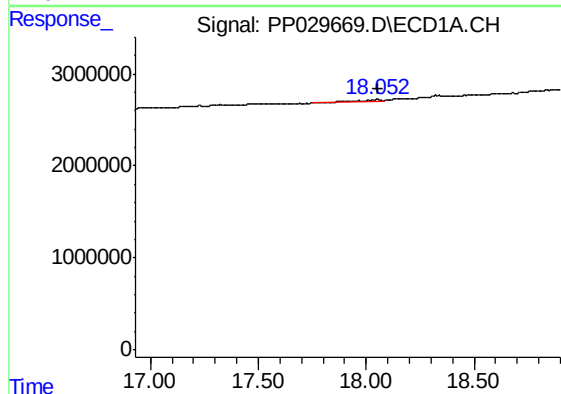

#16 DCPA

R.T.: 18.050 min
Delta R.T.: -0.004 min
Response: 1126057
Conc: 3.55 ng/ml

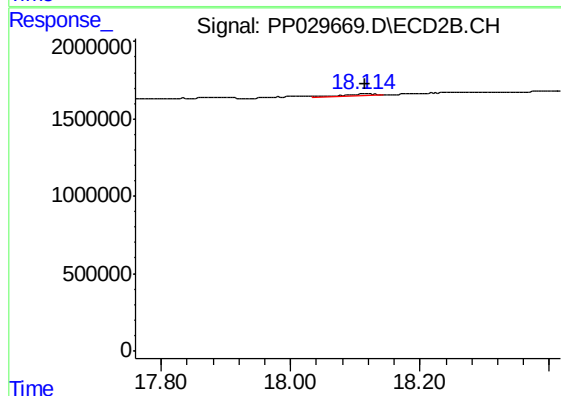

#16 DCPA

R.T.: 18.116 min
Delta R.T.: 0.000 min
Response: 532024
Conc: 2.03 ng/ml