

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
 Data File : PP029670.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 16:15
 Operator : EI\MA
 Sample : K2138-10
 Misc : hexane
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S6B(12-20)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:08:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.118	18392427	22301510	562.202	519.348
Target Compounds							
5) T	DICAMBA	12.226	0.000	101405	0	0.686	N.D. #
8) T	DICHLORPROP	0.000	13.551	0	553337	N.D.	13.664 #
9) T	2,4-D	13.719	0.000	12324	0	0.319	N.D. #
11) T	2,4,5-TP ...	0.000	15.210	0	325002	N.D.	1.570 #
12) T	2,4,5-T	0.000	15.847	0	727531	N.D.	4.389 #
13) T	2,4-DB	16.218	16.388	421801	84338	20.285	3.555 #
14) T	DINOSEB	17.675	16.860	336461	200491	1.996	1.327 #
15) T	Picloram	17.458	18.252	198202	300771	0.605	1.262 #
16) T	DCPA	18.051	18.115	155644	812324	0.491	3.096 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
Data File : PP029670.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 16:15
Operator : EI\MA
Sample : K2138-10
Misc : hexane
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
S6B(12-20)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:08:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

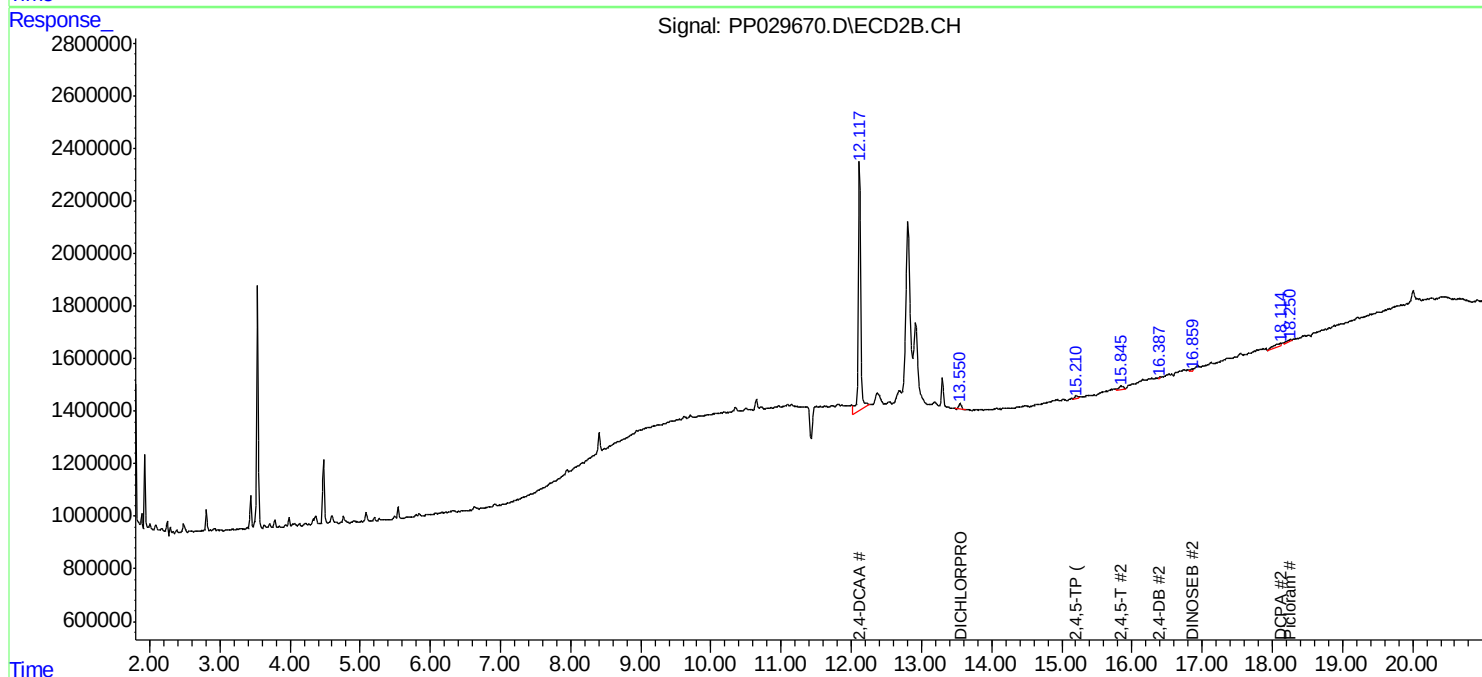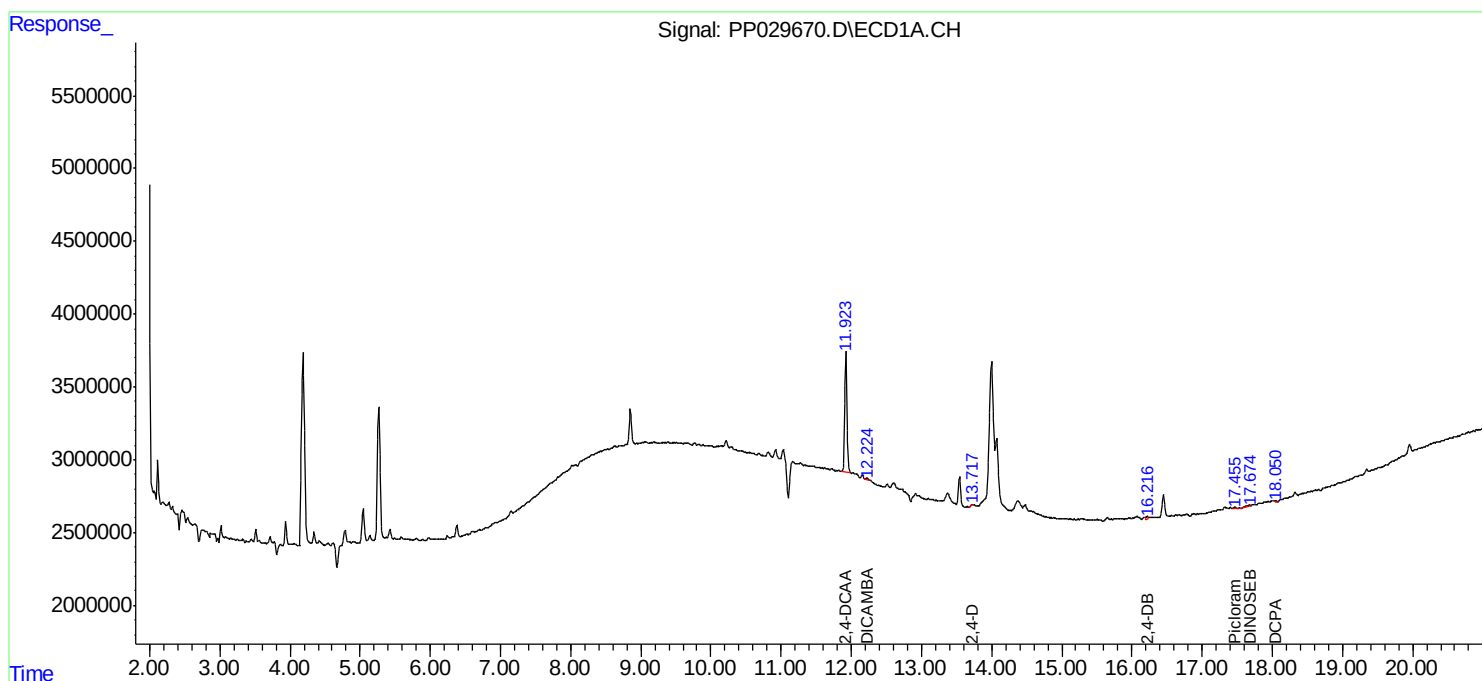


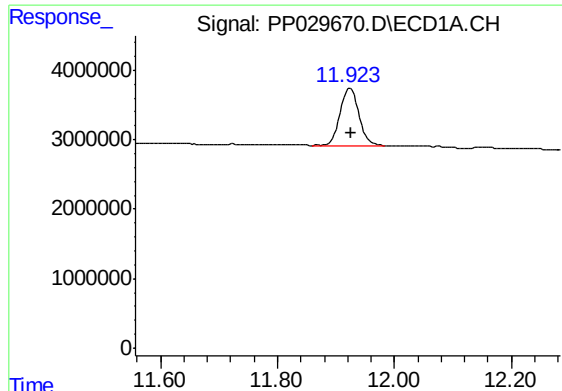

#4 2,4-DCAA


R.T.: 11.924 min
Delta R.T.: 0.000 min
Response: 18392427
Conc: 562.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6B(12-20)COMP

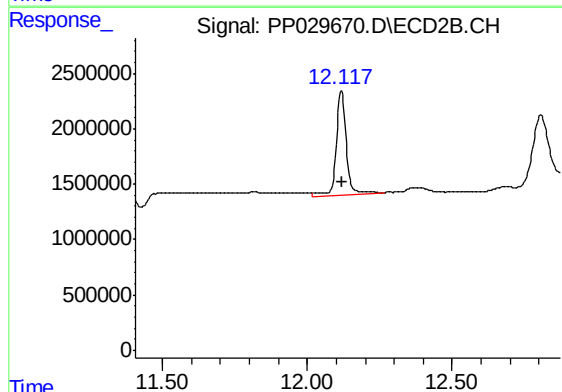


#4 2,4-DCAA

R.T.: 12.118 min
Delta R.T.: -0.003 min
Response: 22301510
Conc: 519.35 ng/ml

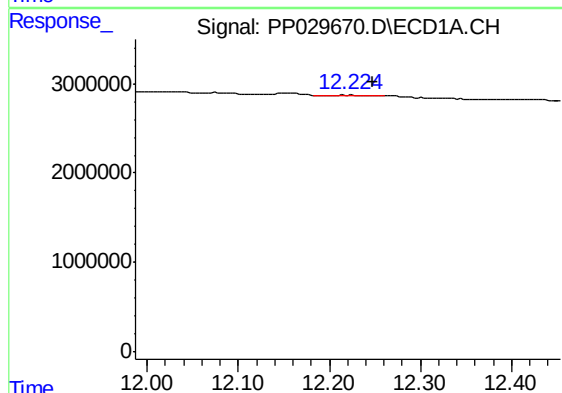


#5 DICAMBA

R.T.: 12.226 min
Delta R.T.: -0.021 min
Response: 101405
Conc: 0.69 ng/ml

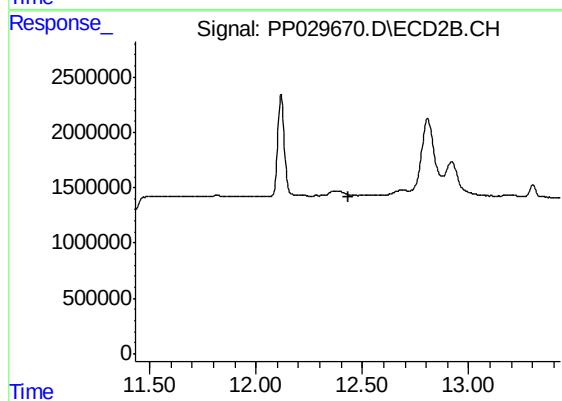

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 12.433 min
Response: 0
Conc: N.D.

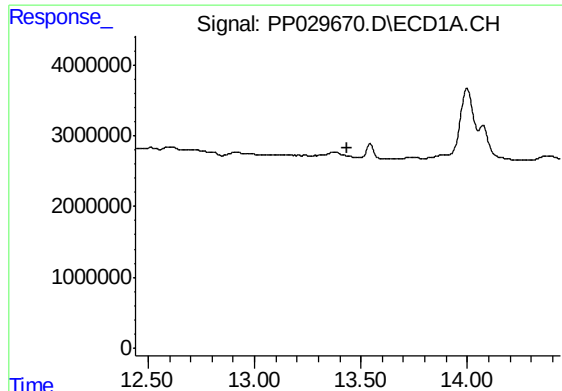

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S6B(12-20)COMP

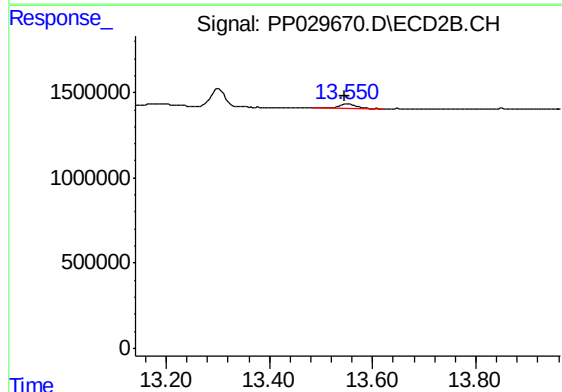


#8 DICHLORPROP

R.T.: 13.551 min
Delta R.T.: 0.006 min
Response: 553337
Conc: 13.66 ng/ml

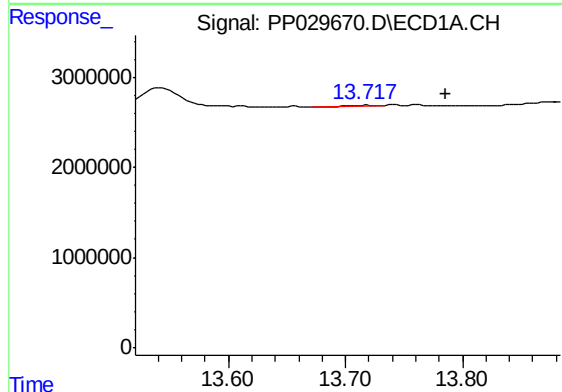


#9 2,4-D

R.T.: 13.719 min
Delta R.T.: -0.067 min
Response: 12324
Conc: 0.32 ng/ml

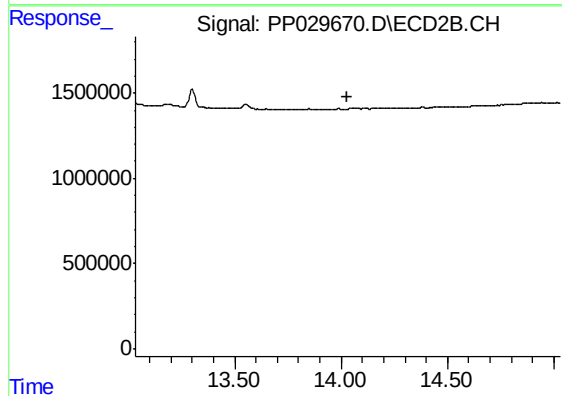

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 14.031 min
Response: 0
Conc: N.D.

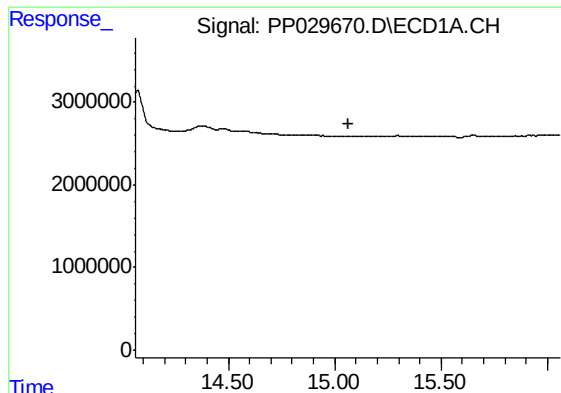

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 15.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S6B(12-20)COMP

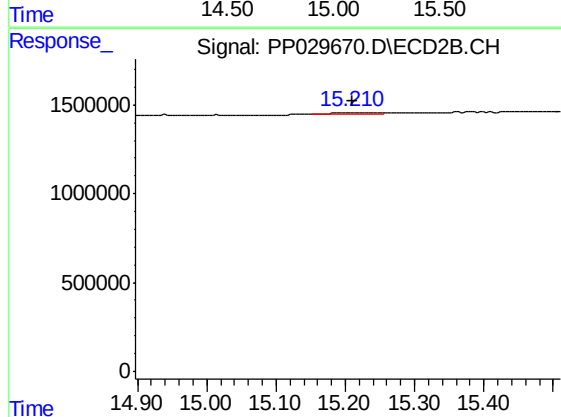


#11 2,4,5-TP (SILVEX)

R.T.: 15.210 min
Delta R.T.: 0.000 min
Response: 325002
Conc: 1.57 ng/ml

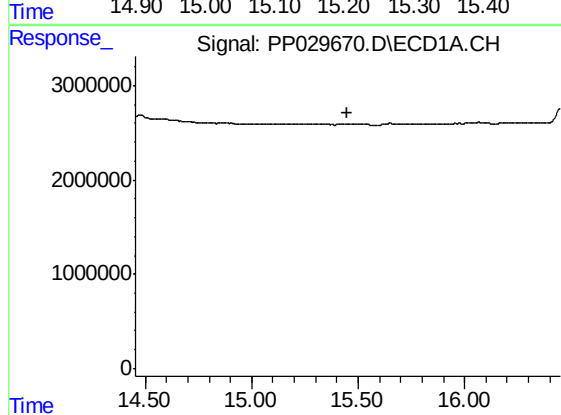


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.451 min
Response: 0
Conc: N.D.

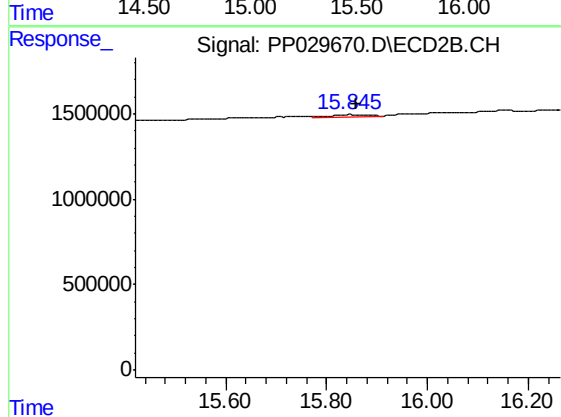

#12 2,4,5-T


R.T.: 15.847 min
Delta R.T.: -0.012 min
Response: 727531
Conc: 4.39 ng/ml

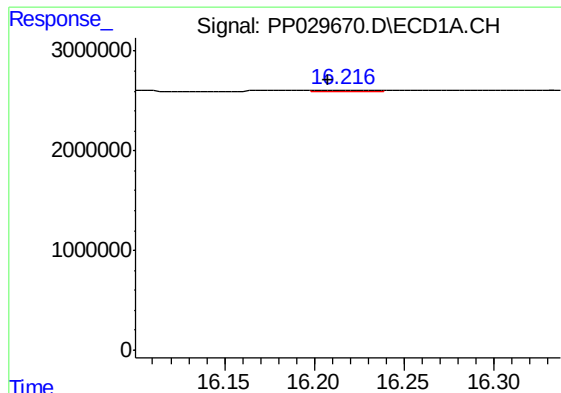

#13 2,4-DB


R.T.: 16.218 min
Delta R.T.: 0.010 min
Response: 421801
Conc: 20.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6B(12-20)COMP

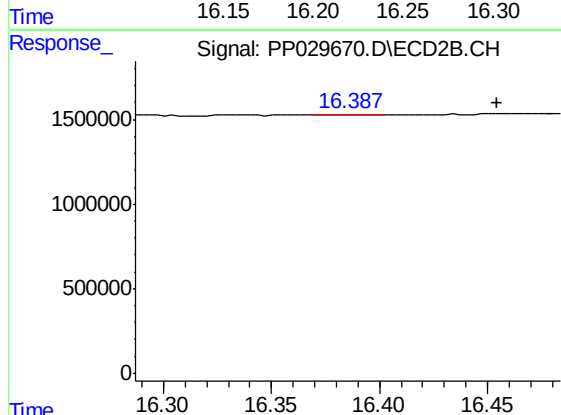


#13 2,4-DB

R.T.: 16.388 min
Delta R.T.: -0.066 min
Response: 84338
Conc: 3.56 ng/ml

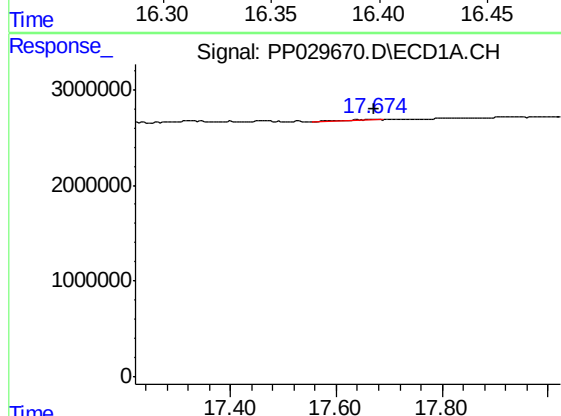


#14 DINOSEB

R.T.: 17.675 min
Delta R.T.: 0.003 min
Response: 336461
Conc: 2.00 ng/ml

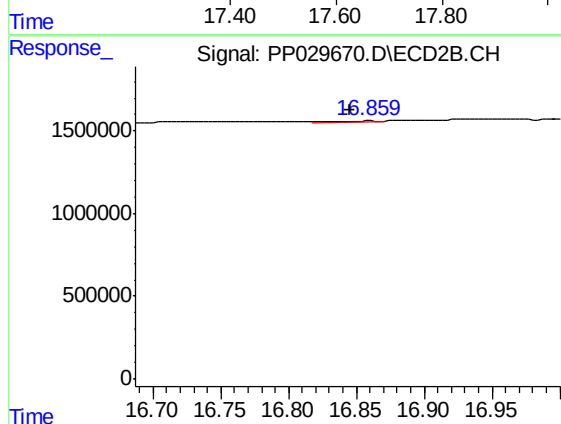

#14 DINOSEB


R.T.: 16.860 min
Delta R.T.: 0.015 min
Response: 200491
Conc: 1.33 ng/ml

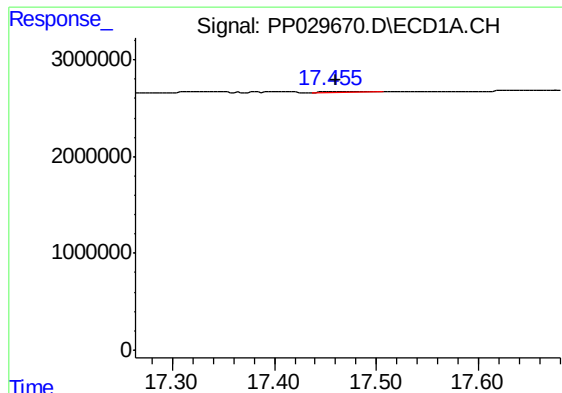

#15 Picloram


R.T.: 17.458 min
Delta R.T.: -0.002 min
Response: 198202
Conc: 0.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
S6B(12-20)COMP

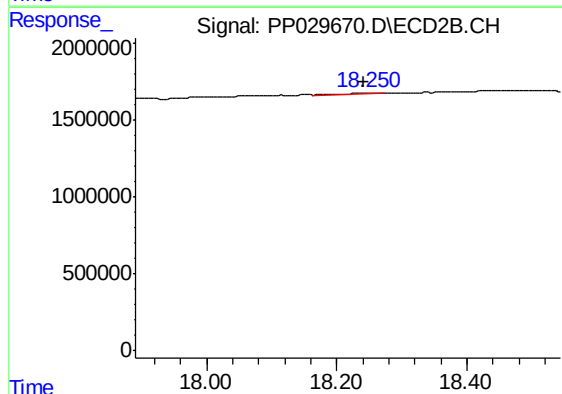


#15 Picloram

R.T.: 18.252 min
Delta R.T.: 0.010 min
Response: 300771
Conc: 1.26 ng/ml

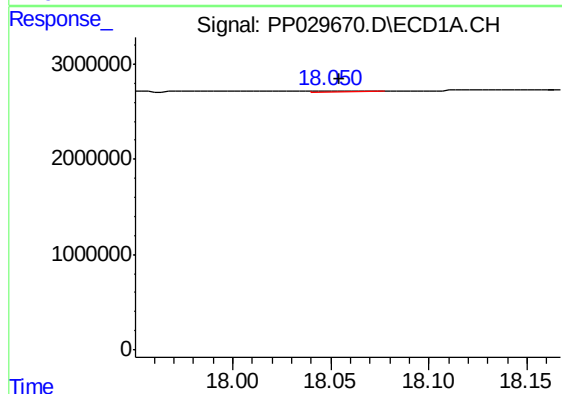

#16 DCPA

R.T.: 18.051 min
Delta R.T.: -0.003 min
Response: 155644
Conc: 0.49 ng/ml

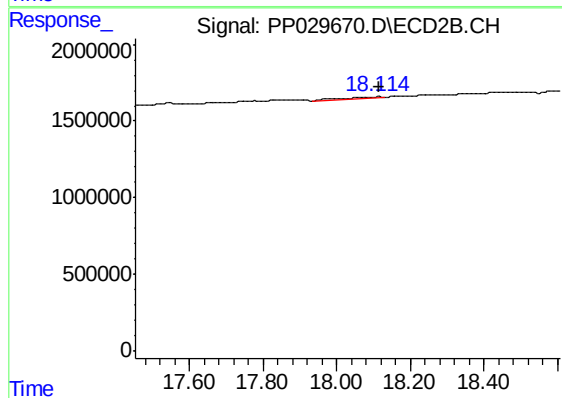

#16 DCPA

R.T.: 18.115 min
Delta R.T.: 0.000 min
Response: 812324
Conc: 3.10 ng/ml