

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
 Data File : PP029671.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 16:40
 Operator : EI\MA
 Sample : K2139-02
 Misc : hexane
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S7B(2-10)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:08:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.119	16086609	18812691	491.720	438.102
Target Compounds							
3) T	4-Nitroph...	11.434	0.000	71614	0	1.093	N.D. #
5) T	DICAMBA	12.219	0.000	569626	0	3.855	N.D. #
8) T	DICHLORPROP	13.372	13.553	-182583	402262	N.D.	9.933
11) T	2,4,5-TP ...	0.000	15.228	0	178335	N.D.	0.862 #
12) T	2,4,5-T	0.000	15.848	0	1408325	N.D.	8.495 #
13) T	2,4-DB	16.189	0.000	157421	0	7.571	N.D. #
14) T	DINOSEB	17.683	0.000	69172	0	0.410	N.D. #
15) T	Picloram	17.513	0.000	49088	0	0.150	N.D. #
16) T	DCPA	18.049	0.000	396861	0	1.251	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
Data File : PP029671.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 16:40
Operator : EI\MA
Sample : K2139-02
Misc : hexane
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
S7B(2-10)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:08:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

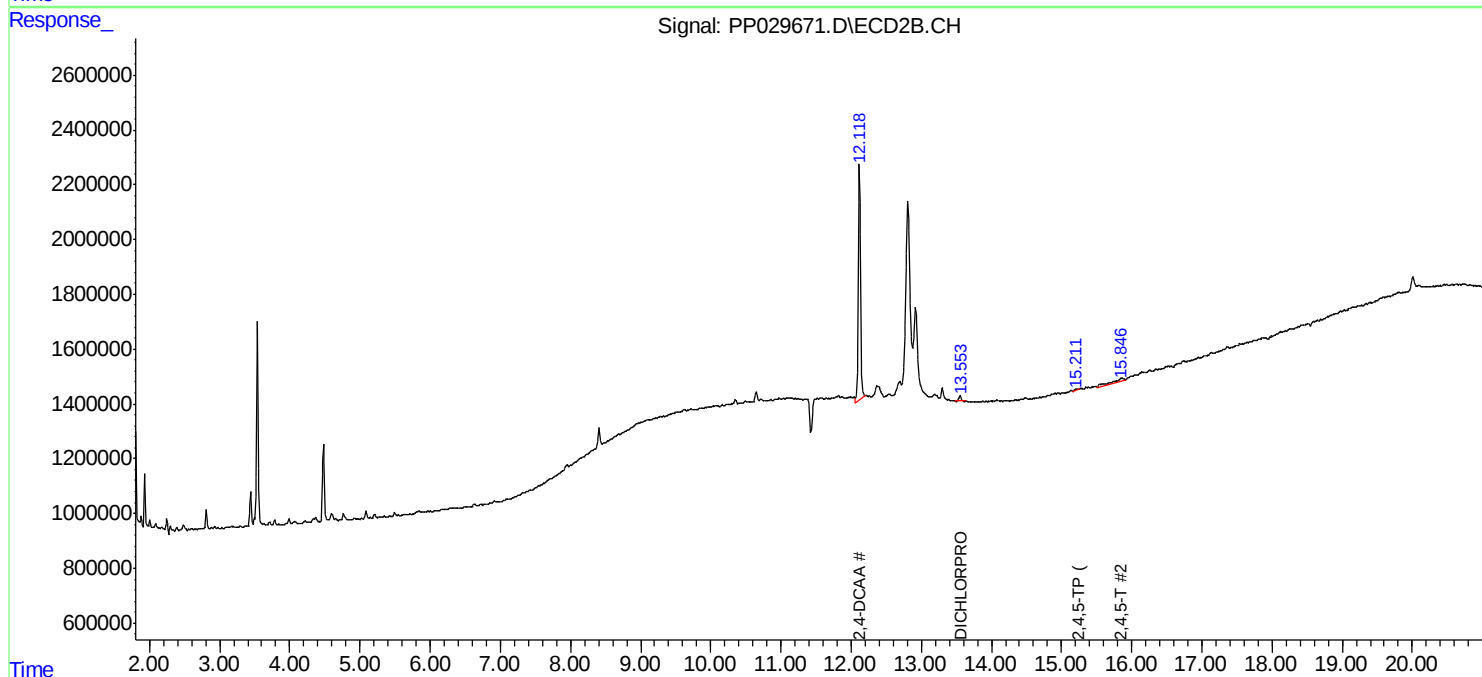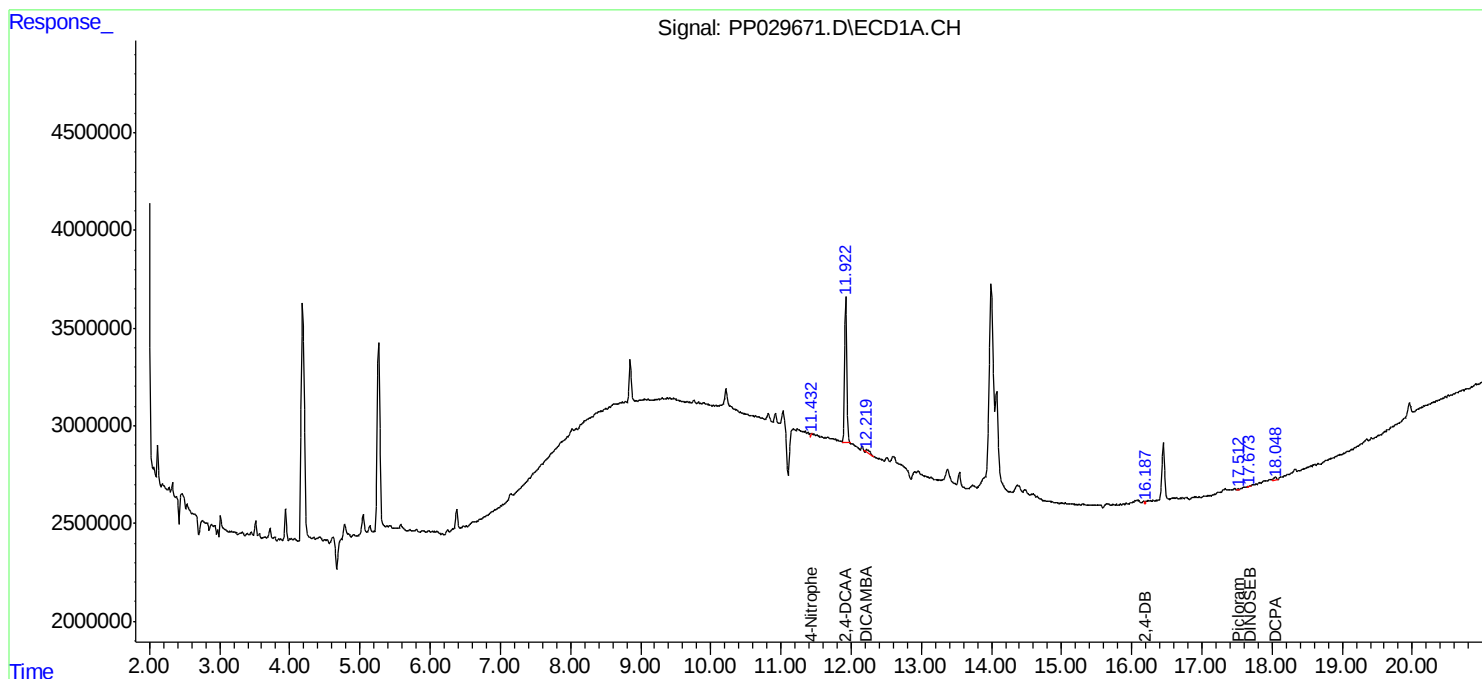


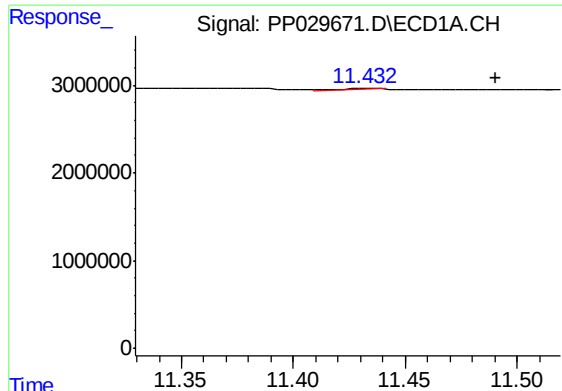

#3 4-Nitrophenol


R.T.: 11.434 min
Delta R.T.: -0.057 min
Response: 71614
Conc: 1.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
S7B(2-10)COMP

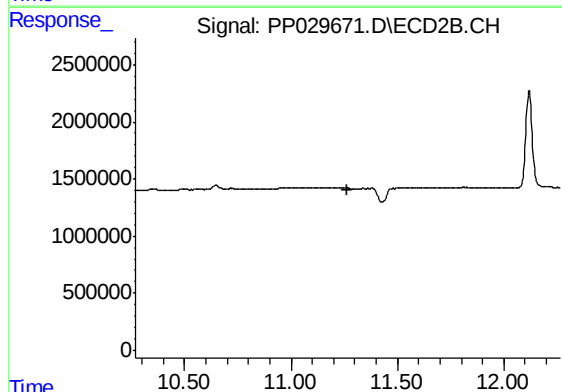


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.266 min
Response: 0
Conc: N.D.

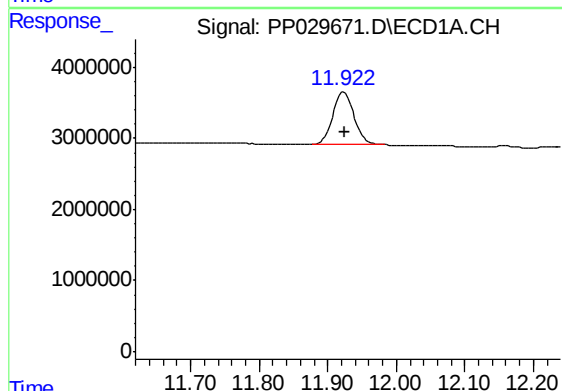


#4 2,4-DCAA

R.T.: 11.924 min
Delta R.T.: -0.001 min
Response: 16086609
Conc: 491.72 ng/ml

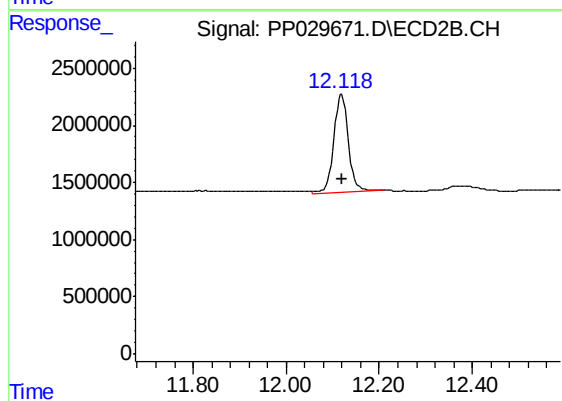

#4 2,4-DCAA


R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 18812691
Conc: 438.10 ng/ml

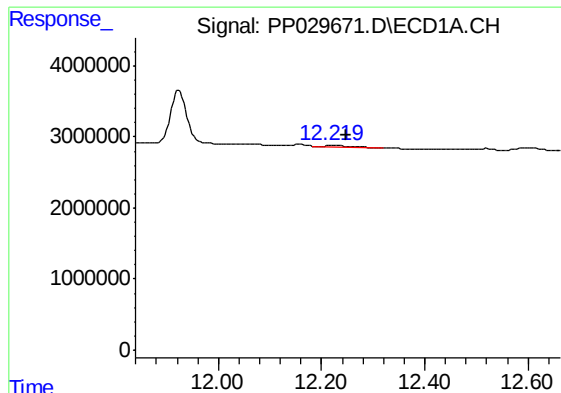

#5 DICAMBA


R.T.: 12.219 min
Delta R.T.: -0.029 min
Response: 569626
Conc: 3.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
S7B(2-10)COMP

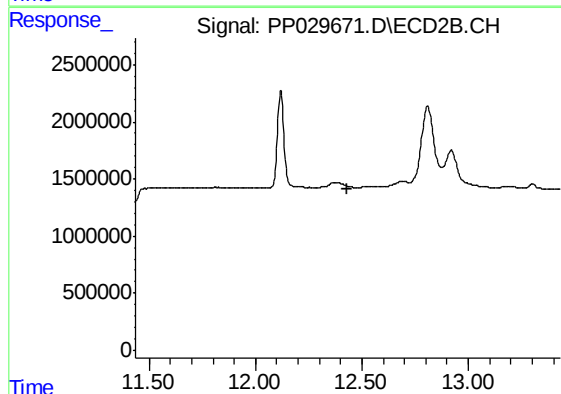


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.433 min
Response: 0
Conc: N.D.

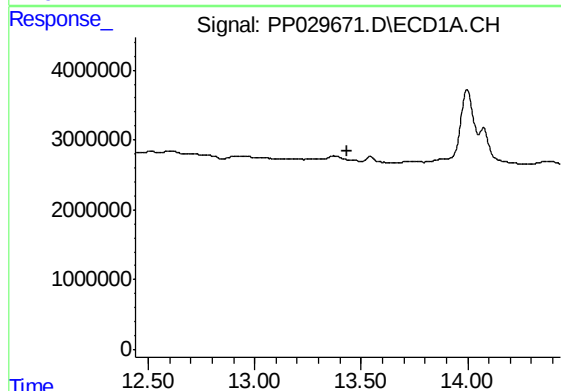


#8 DICHLORPROP

R.T.: 13.372 min
Delta R.T.: -0.066 min
Response: -182583
Conc: N.D.

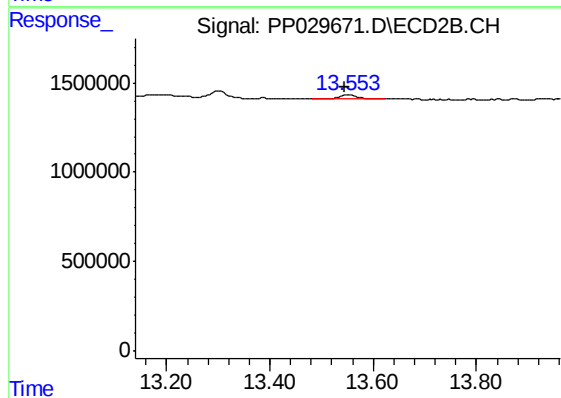

#8 DICHLORPROP


R.T.: 13.553 min
Delta R.T.: 0.008 min
Response: 402262
Conc: 9.93 ng/ml

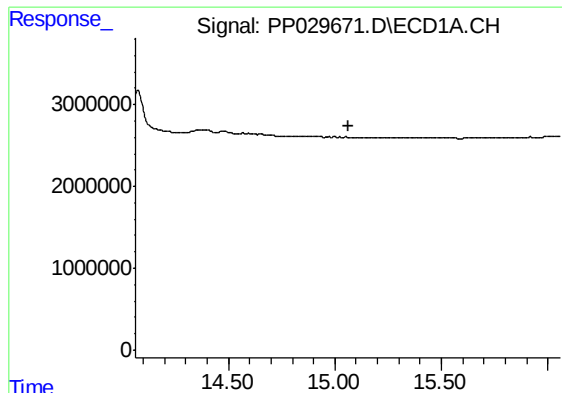

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S7B(2-10)COMP

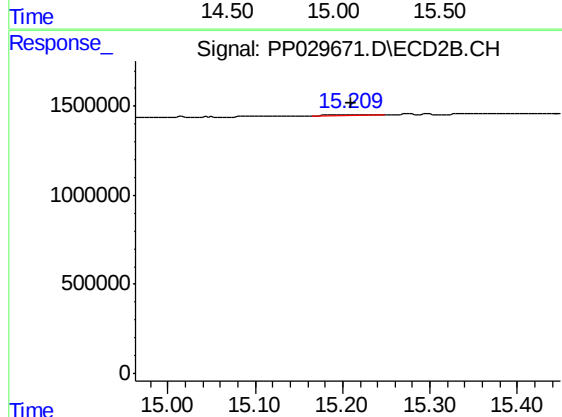


#11 2,4,5-TP (SILVEX)

R.T.: 15.228 min
Delta R.T.: 0.018 min
Response: 178335
Conc: 0.86 ng/ml

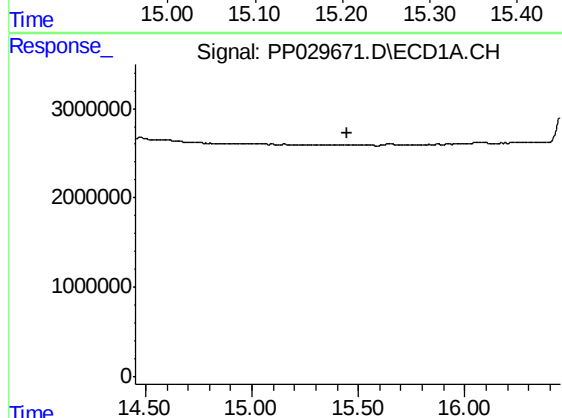


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

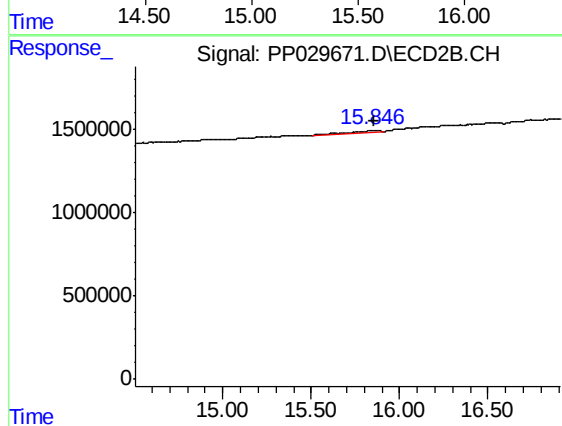

#12 2,4,5-T


R.T.: 15.848 min
Delta R.T.: -0.011 min
Response: 1408325
Conc: 8.50 ng/ml

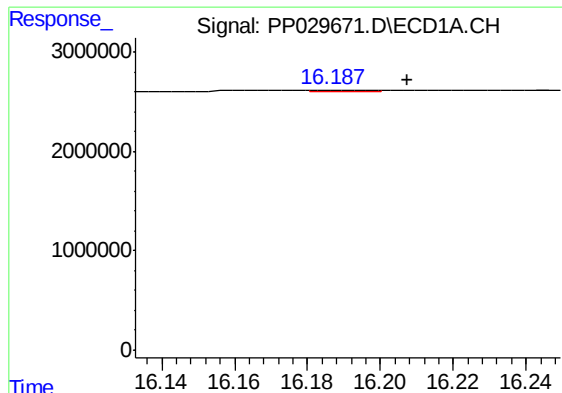

#13 2,4-DB


R.T.: 16.189 min
Delta R.T.: -0.018 min
Response: 157421
Conc: 7.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
S7B(2-10)COMP

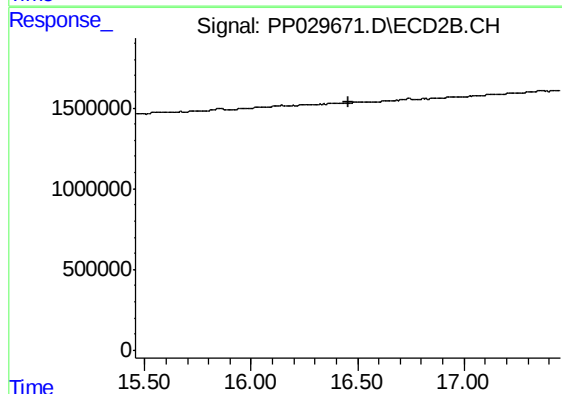


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

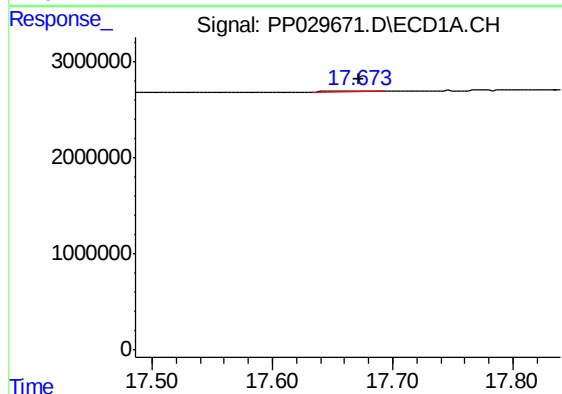


#14 DINOSEB

R.T.: 17.683 min
Delta R.T.: 0.011 min
Response: 69172
Conc: 0.41 ng/ml

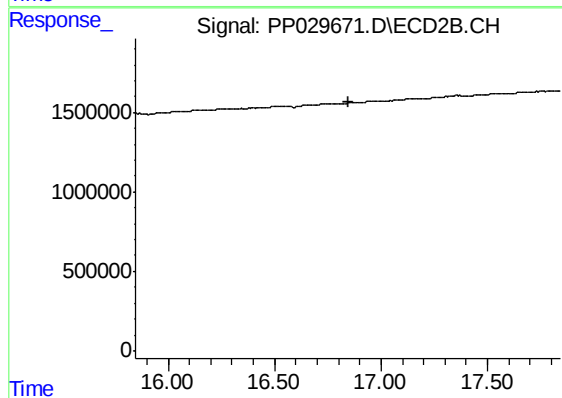

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.845 min
Response: 0
Conc: N.D.

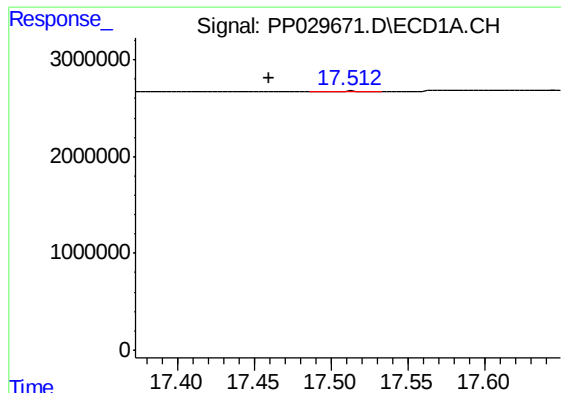

#15 Picloram


R.T.: 17.513 min
Delta R.T.: 0.053 min
Response: 49088
Conc: 0.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
S7B(2-10)COMP

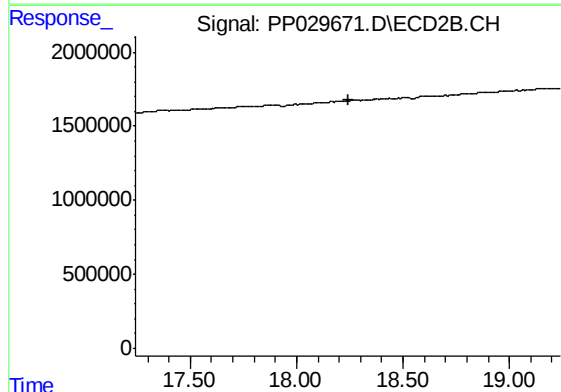


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.242 min
Response: 0
Conc: N.D.

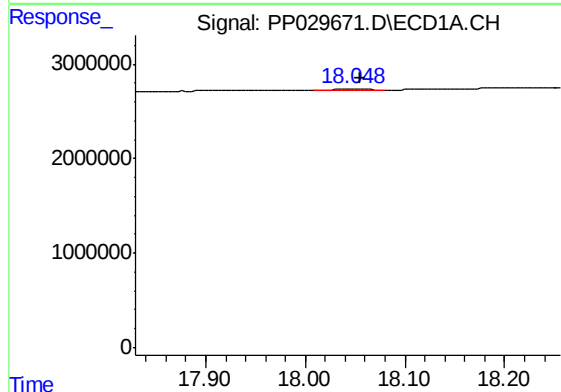

#16 DCPA

R.T.: 18.049 min
Delta R.T.: -0.005 min
Response: 396861
Conc: 1.25 ng/ml

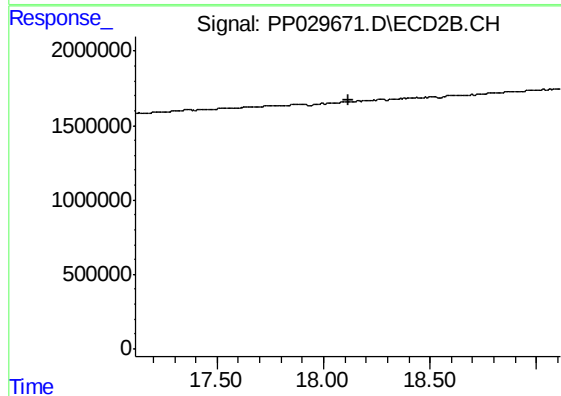

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.116 min
Response: 0
Conc: N.D.