

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
 Data File : PP029673.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 17:32
 Operator : EI\MA
 Sample : K2153-24
 Misc : hexane
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:09:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.119	19044851	20929870	582.144	487.406
Target Compounds							
8) T	DICHLORPROP	0.000	13.556	0	568547	N.D.	14.039 #
10) T	Pentachlo...	0.000	14.638	0	241291	N.D.	0.441 #
11) T	2,4,5-TP ...	0.000	15.218	0	85279	N.D.	0.412 #
12) T	2,4,5-T	0.000	15.844	0	482151	N.D.	2.908 #
13) T	2,4-DB	16.211	0.000	548037	0	26.356	N.D. #
14) T	DINOSEB	17.671	16.807	298137	274524	1.769	1.817
15) T	Picloram	17.470	18.243	241469	434706	0.737	1.824 #
16) T	DCPA	18.053	18.118	1024261	910695	3.228	3.471



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
Data File : PP029673.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 17:32
Operator : EI\MA
Sample : K2153-24
Misc : hexane
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
SP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:09:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

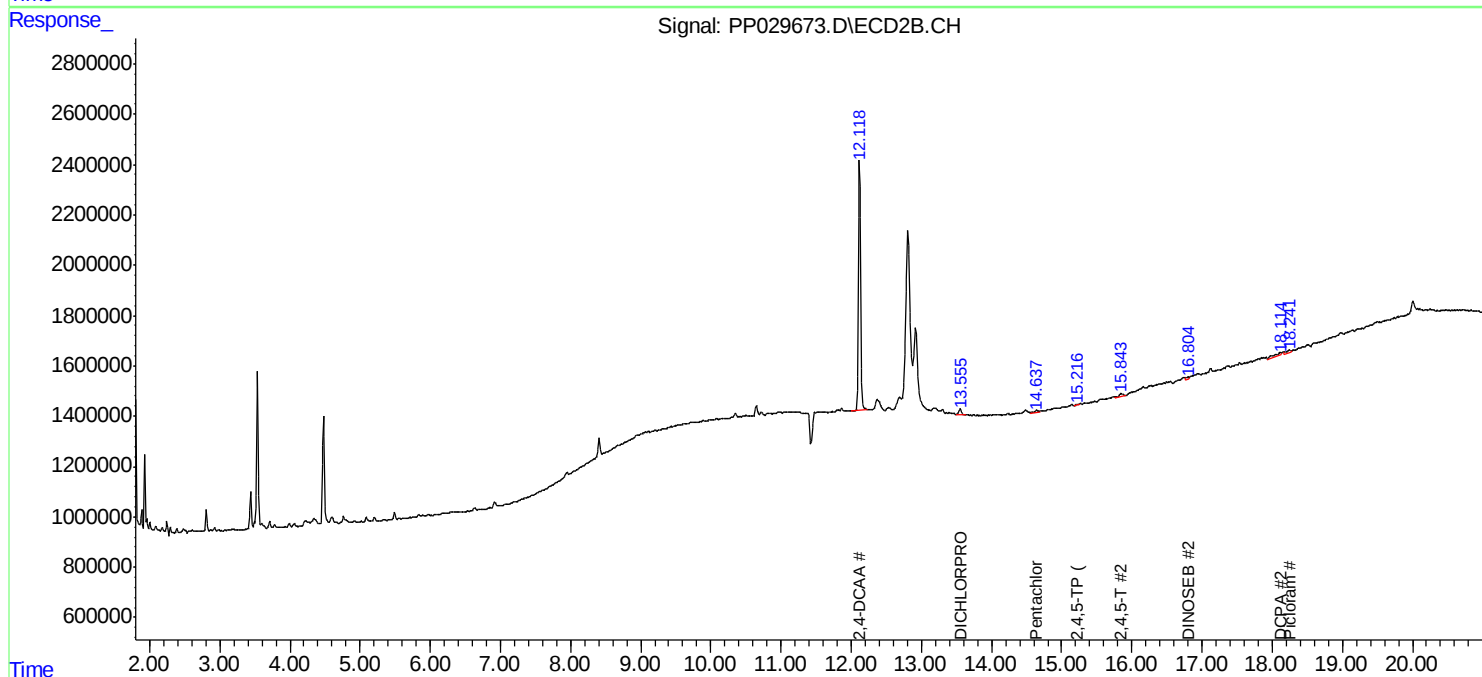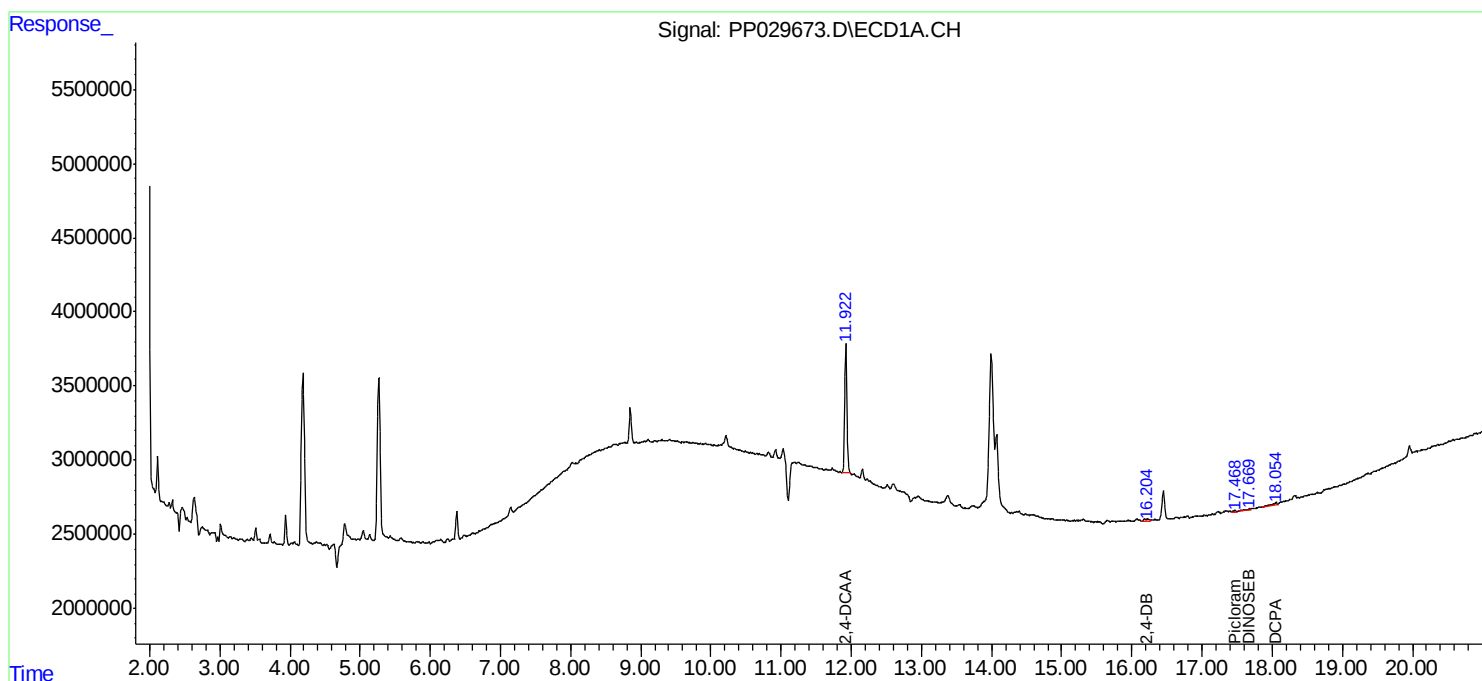


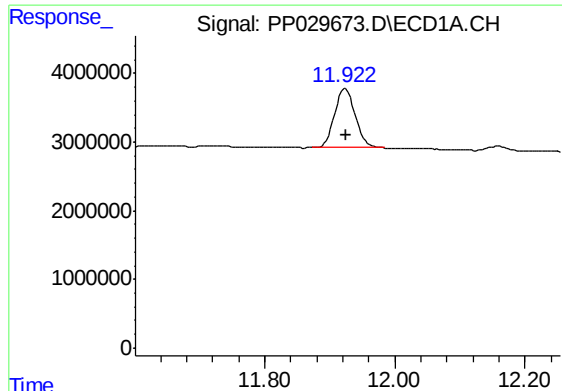

#4 2,4-DCAA


R.T.: 11.924 min
Delta R.T.: -0.001 min
Response: 19044851
Conc: 582.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
SP-1

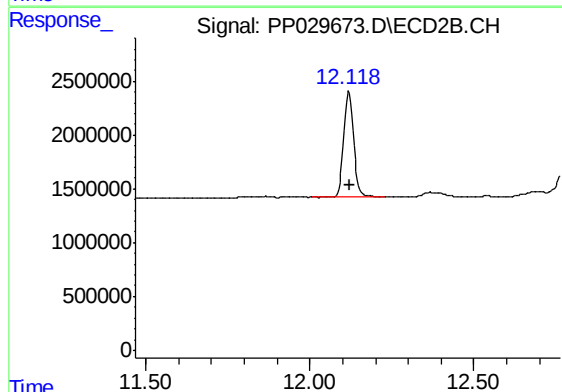


#4 2,4-DCAA

R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 20929870
Conc: 487.41 ng/ml

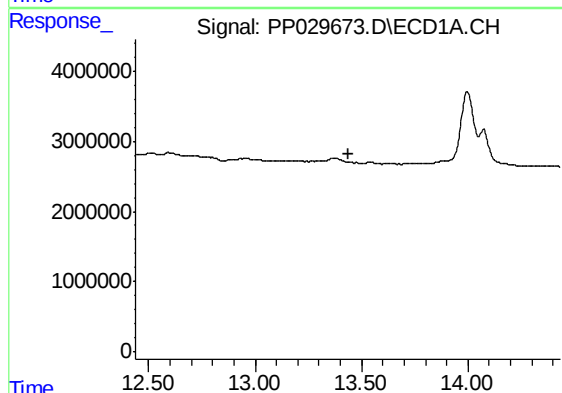


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.438 min
Response: 0
Conc: N.D.

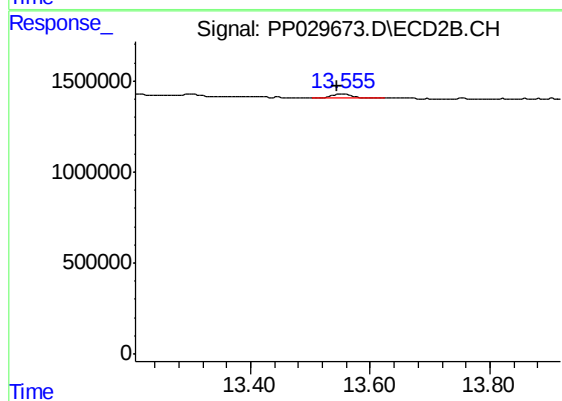

#8 DICHLORPROP


R.T.: 13.556 min
Delta R.T.: 0.011 min
Response: 568547
Conc: 14.04 ng/ml

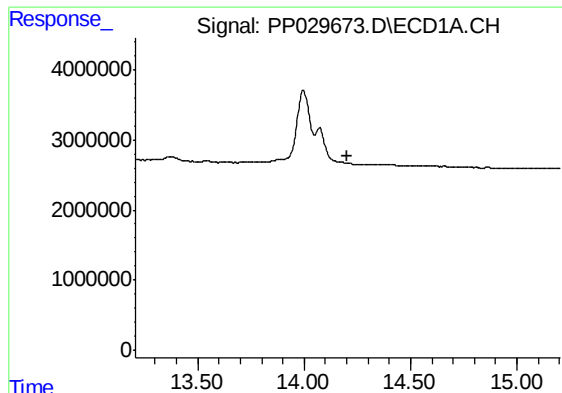

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 14.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SP-1

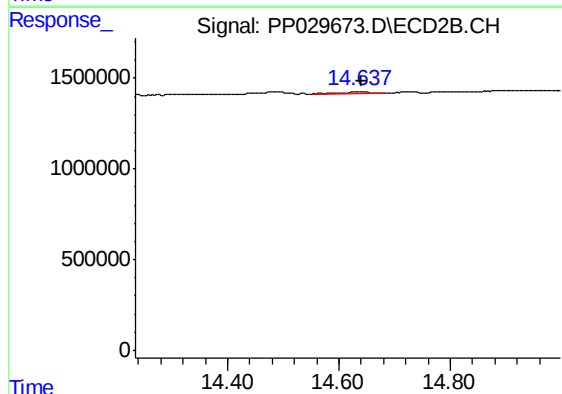


#10 Pentachlorophenol

R.T.: 14.638 min
Delta R.T.: -0.002 min
Response: 241291
Conc: 0.44 ng/ml

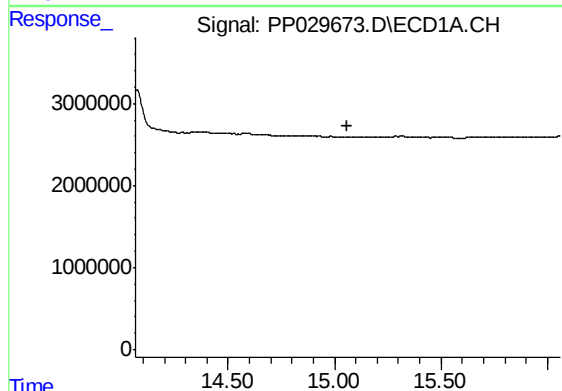


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.062 min
Response: 0
Conc: N.D.

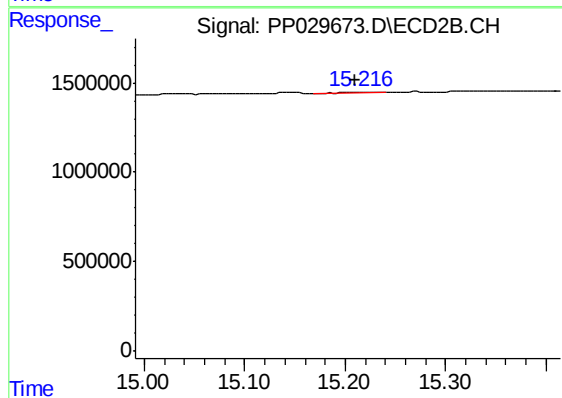

#11 2,4,5-TP (SILVEX)


R.T.: 15.218 min
Delta R.T.: 0.008 min
Response: 85279
Conc: 0.41 ng/ml

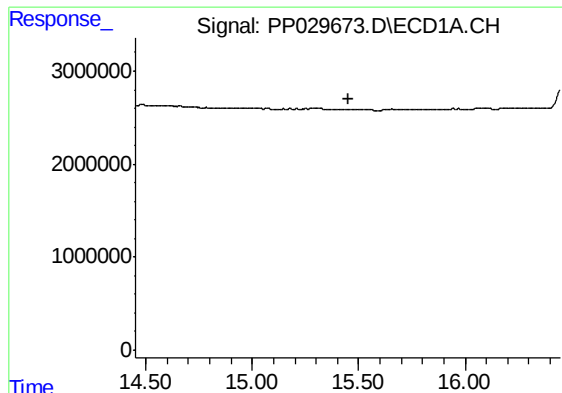

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 15.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SP-1

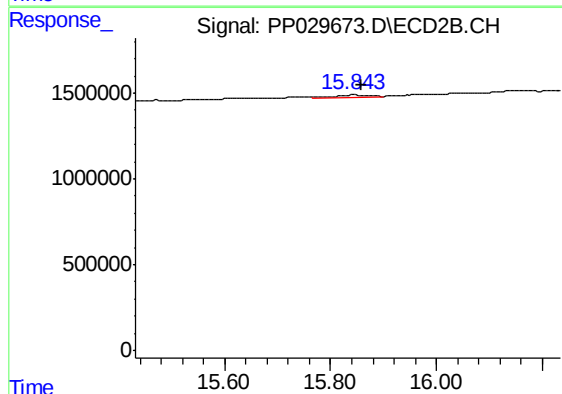


#12 2,4,5-T

R.T.: 15.844 min
Delta R.T.: -0.014 min
Response: 482151
Conc: 2.91 ng/ml

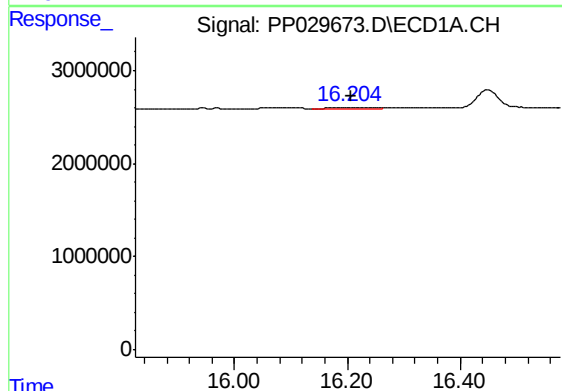


#13 2,4-DB

R.T.: 16.211 min
Delta R.T.: 0.003 min
Response: 548037
Conc: 26.36 ng/ml

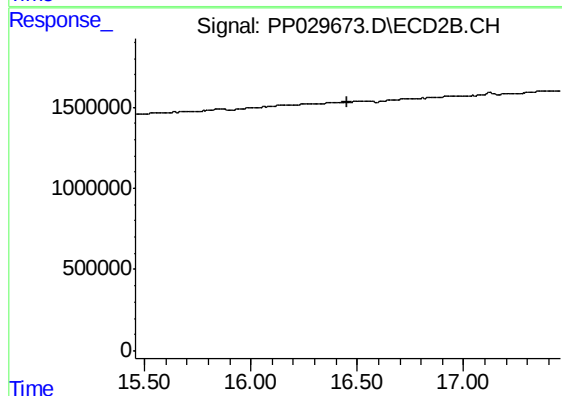

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

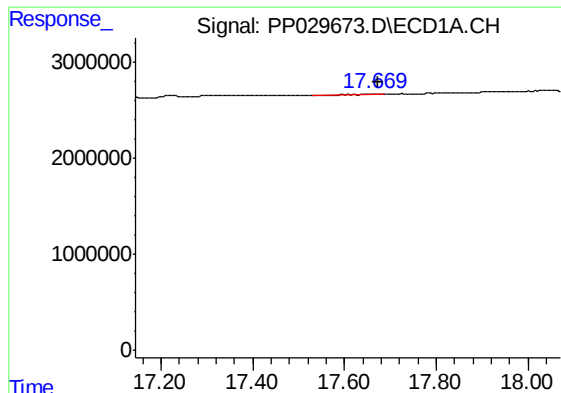

#14 DINOSEB


R.T.: 17.671 min
Delta R.T.: -0.001 min
Response: 298137
Conc: 1.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
SP-1

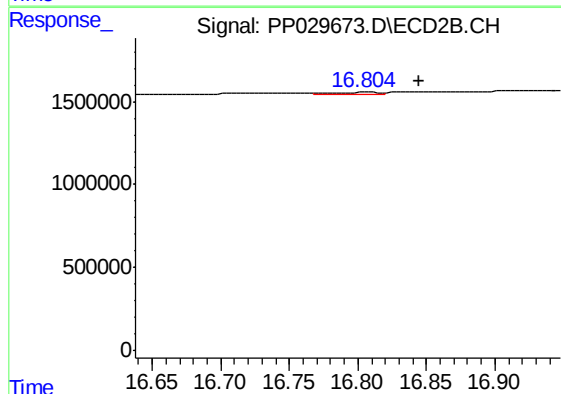


#14 DINOSEB

R.T.: 16.807 min
Delta R.T.: -0.037 min
Response: 274524
Conc: 1.82 ng/ml

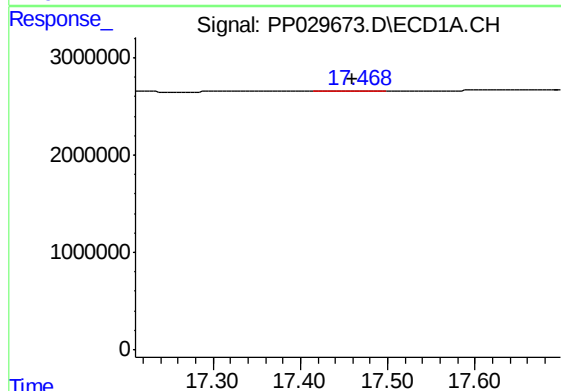


#15 Picloram

R.T.: 17.470 min
Delta R.T.: 0.011 min
Response: 241469
Conc: 0.74 ng/ml

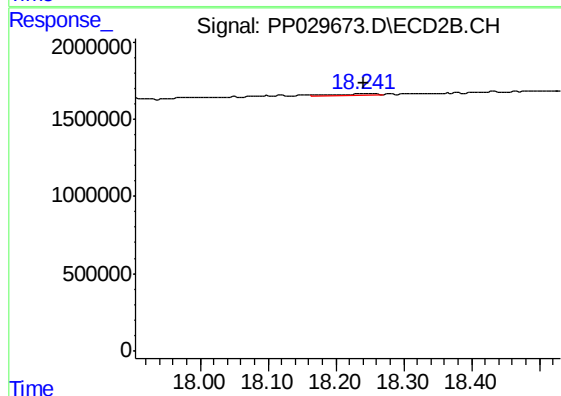

#15 Picloram


R.T.: 18.243 min
Delta R.T.: 0.000 min
Response: 434706
Conc: 1.82 ng/ml

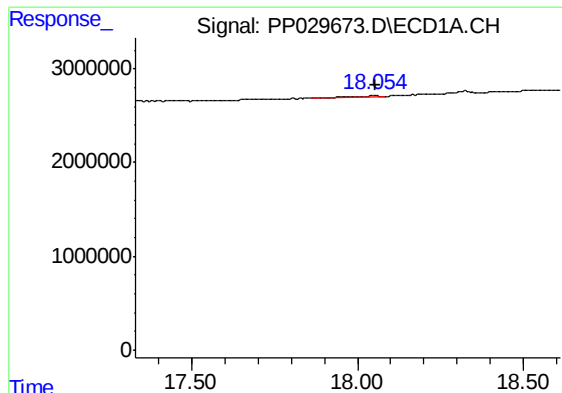

#16 DCPA

R.T.: 18.053 min
Delta R.T.: -0.002 min
Response: 1024261
Conc: 3.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
SP-1

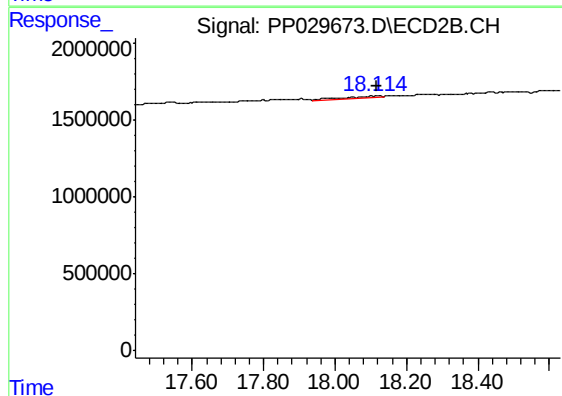

#16 DCPA

R.T.: 18.118 min
Delta R.T.: 0.002 min
Response: 910695
Conc: 3.47 ng/ml