

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
 Data File : PP029675.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2019 18:23
 Operator : EI\MA
 Sample : I.BLK
 Misc : hexane
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:09:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.119	17496457	20823405	534.815	484.927
Target Compounds							
5) T	DICAMBA	0.000	12.397	0	461735	N.D.	3.148 #
13) T	2,4-DB	16.209	0.000	143549	0	6.903	N.D. #
14) T	DINOSEB	17.690	0.000	43377	0	0.257	N.D. #
15) T	Picloram	17.479	0.000	155943	0	0.476	N.D. #
16) T	DCPA	18.050	0.000	127098	0	0.401	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033019\
Data File : PP029675.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2019 18:23
Operator : EI\MA
Sample : I.BLK
Misc : hexane
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:09:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

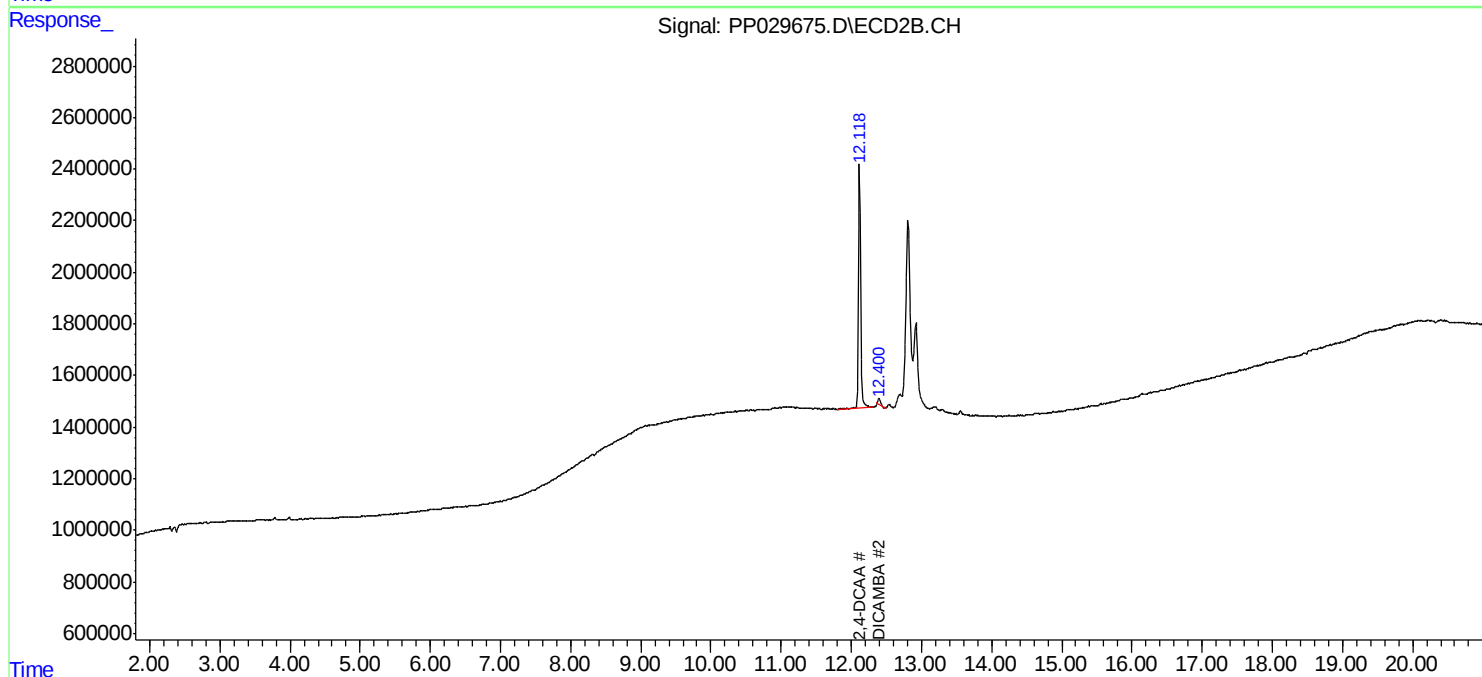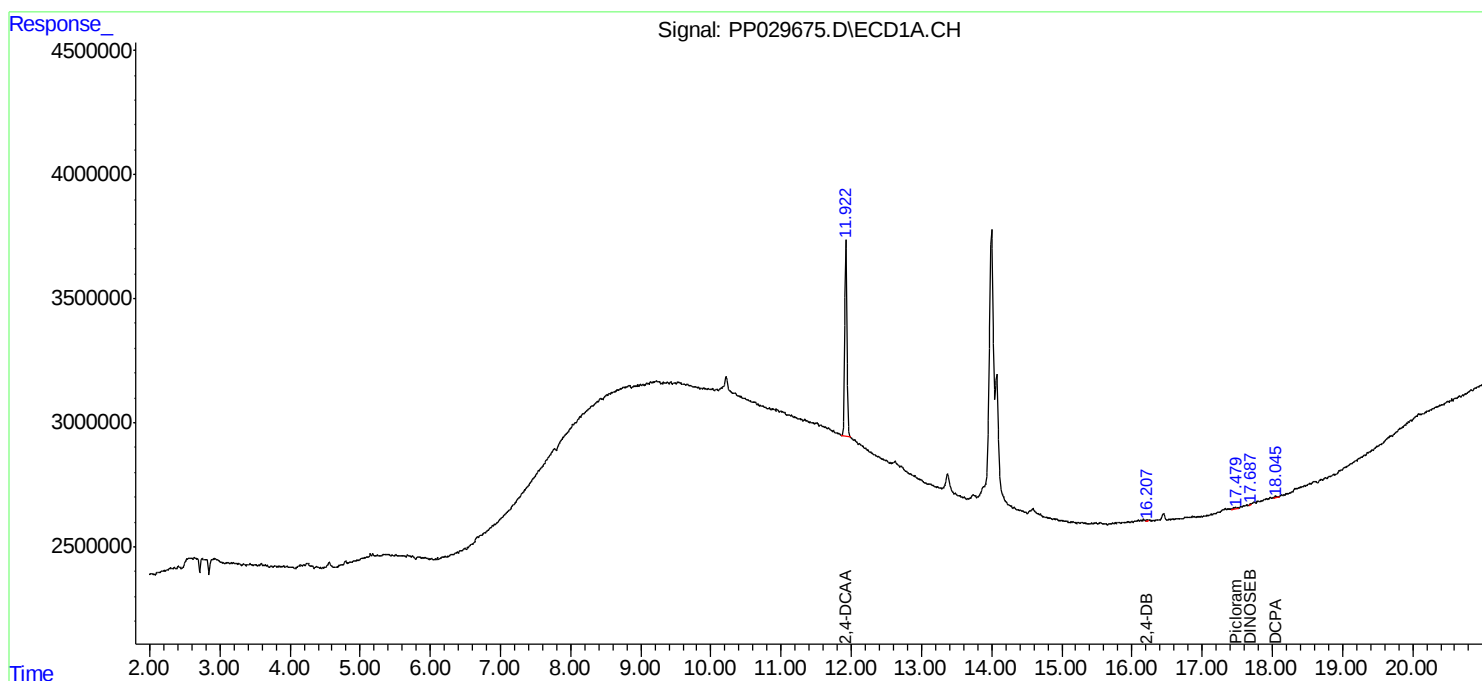


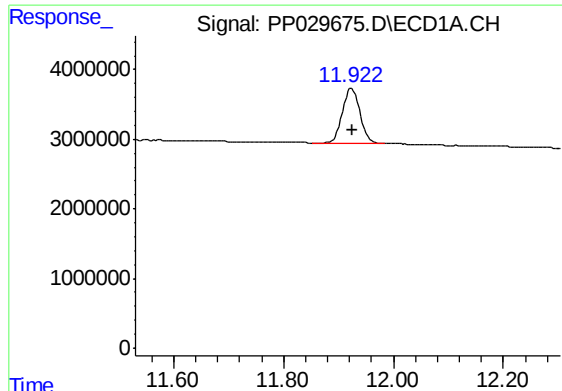

#4 2,4-DCAA


R.T.: 11.924 min
Delta R.T.: -0.001 min
Response: 17496457
Conc: 534.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

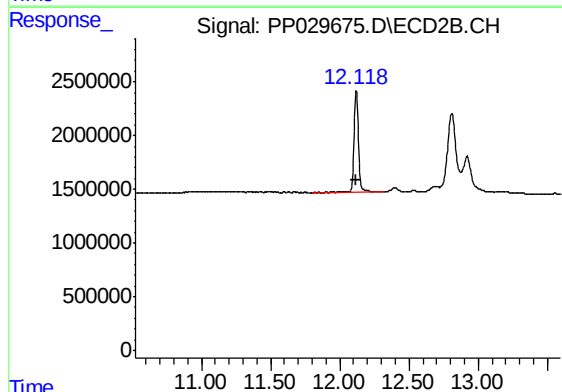


#4 2,4-DCAA

R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 20823405
Conc: 484.93 ng/ml

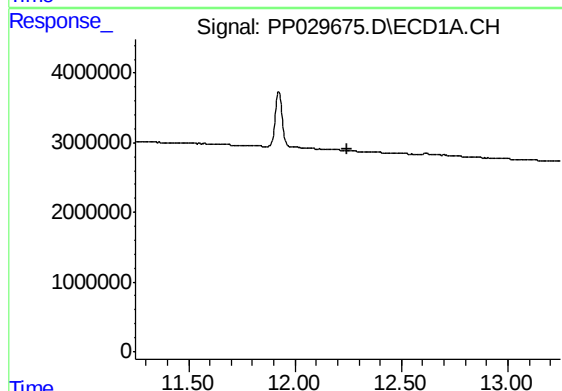


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.247 min
Response: 0
Conc: N.D.

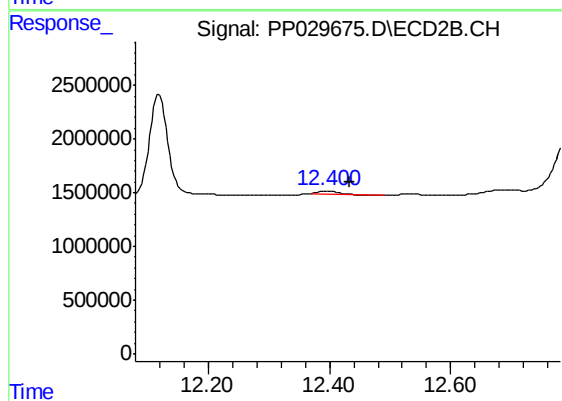

#5 DICAMBA


R.T.: 12.397 min
Delta R.T.: -0.036 min
Response: 461735
Conc: 3.15 ng/ml

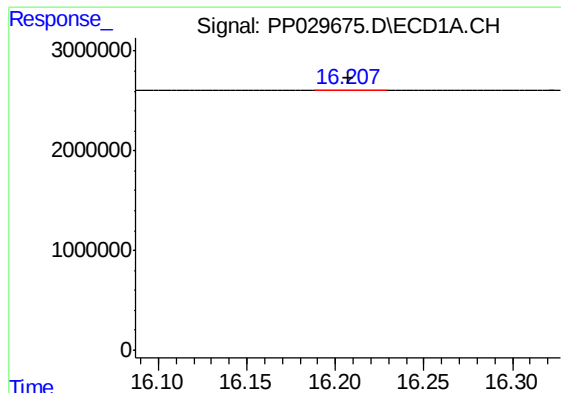

#13 2,4-DB


R.T.: 16.209 min
Delta R.T.: 0.001 min
Response: 143549
Conc: 6.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

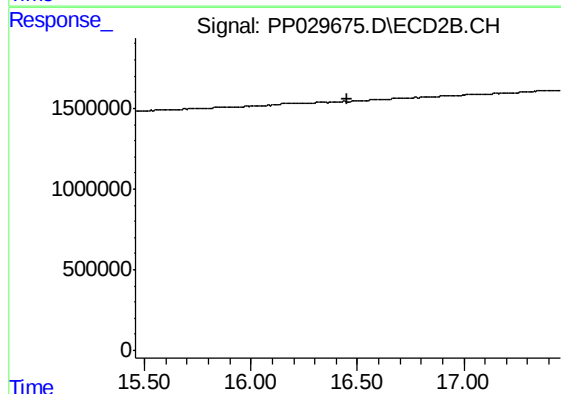


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

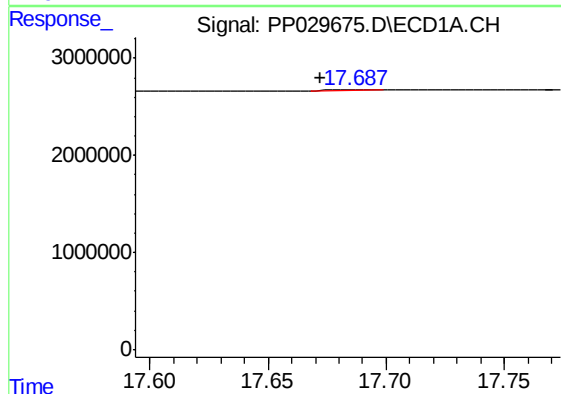


#14 DINOSEB

R.T.: 17.690 min
Delta R.T.: 0.018 min
Response: 43377
Conc: 0.26 ng/ml

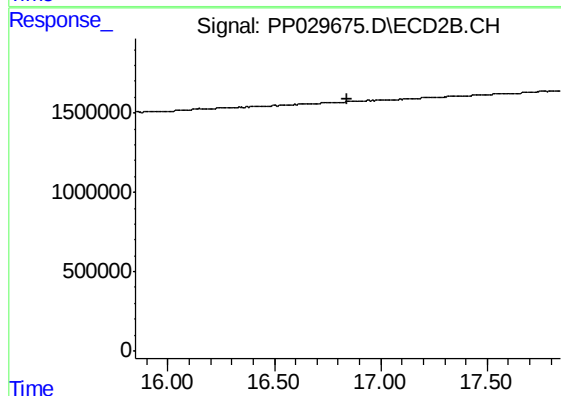

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.845 min
Response: 0
Conc: N.D.

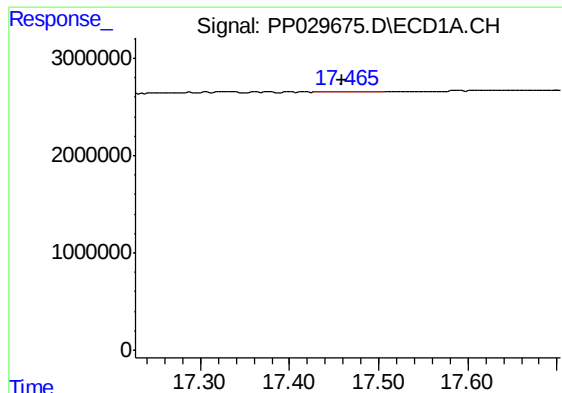

#15 Picloram


R.T.: 17.479 min
Delta R.T.: 0.019 min
Response: 155943
Conc: 0.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

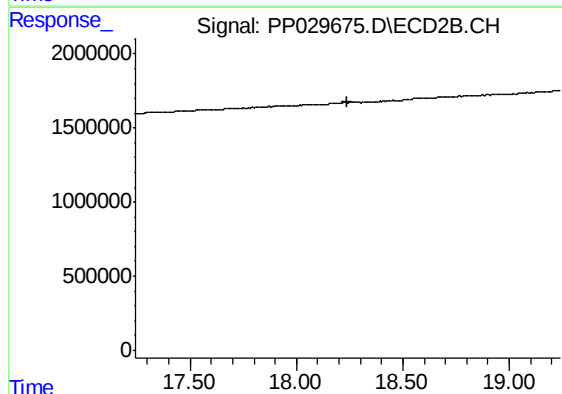


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.242 min
Response: 0
Conc: N.D.

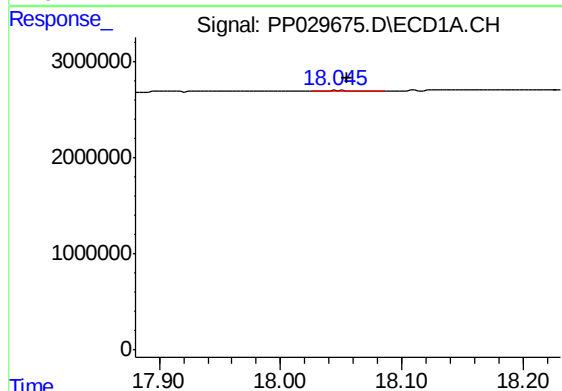

#16 DCPA

R.T.: 18.050 min
Delta R.T.: -0.005 min
Response: 127098
Conc: 0.40 ng/ml

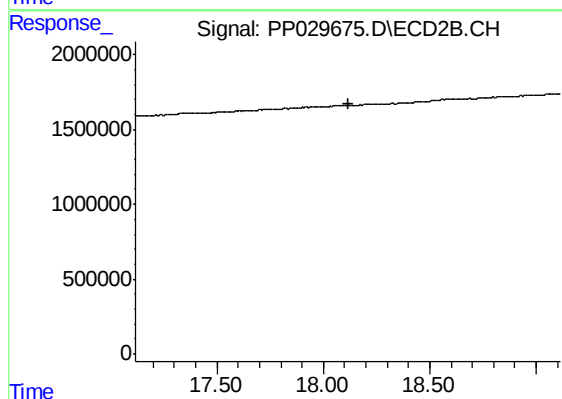

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.116 min
Response: 0
Conc: N.D.