

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033021\
 Data File : PP034464.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Mar 2021 18:22
 Operator : DD\AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:51:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 04:10:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 04:08:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.846	4.259	391742	245722	5.005	5.431
2) SA Decachlor...	10.765	9.566	408809	147696	5.388	5.377
Target Compounds						
21) L5 AR-1248-1	6.159	5.512	78880	42104	56.523	58.908
22) L5 AR-1248-2	6.450	5.774	110275	57602	56.842m	57.069
23) L5 AR-1248-3	6.666	5.819	122196	61740	51.087	57.444
24) L5 AR-1248-4	7.093	6.004	135921	69216	53.446	55.623
25) L5 AR-1248-5	7.132	6.423	133880	62304	52.598	55.991m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033021\
Data File : PP034464.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Mar 2021 18:22
Operator : DD\AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
4/1/2021 12:51:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 04:10:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 04:08:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

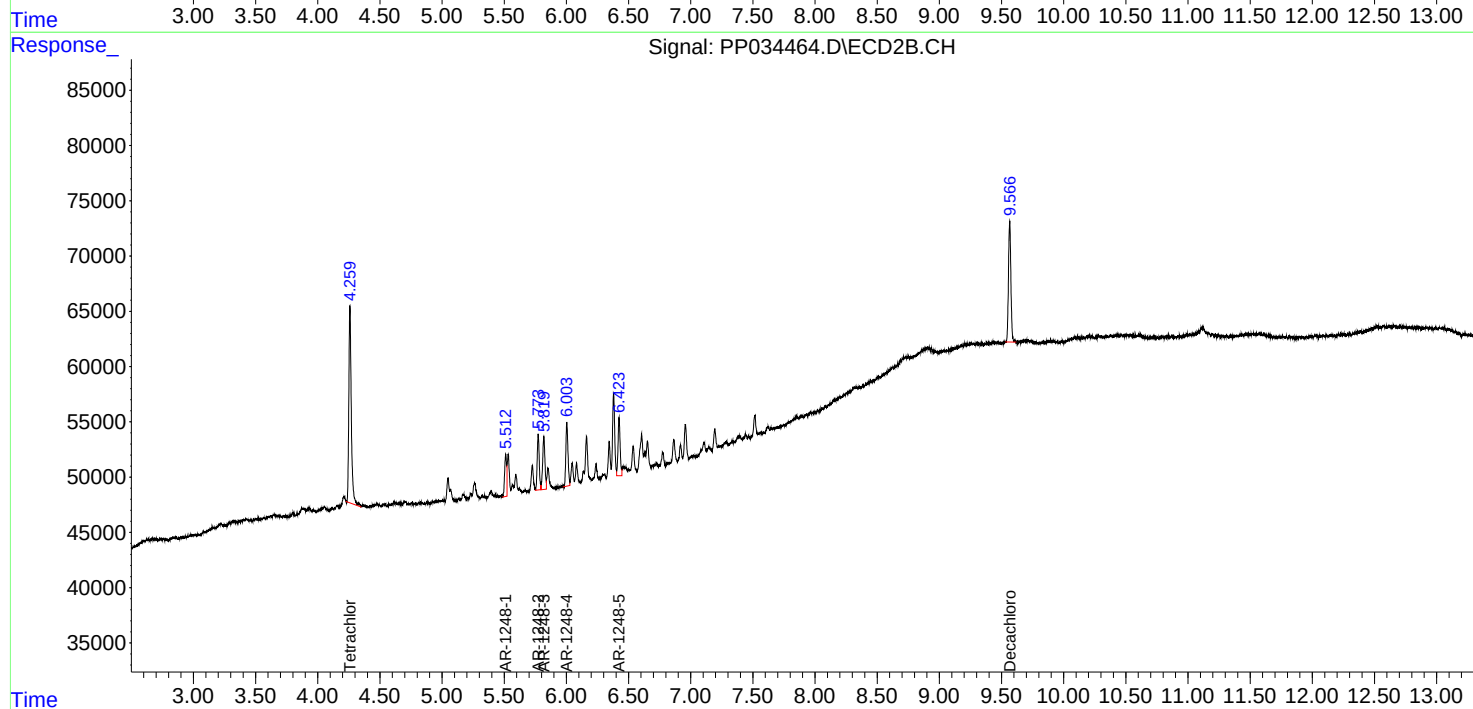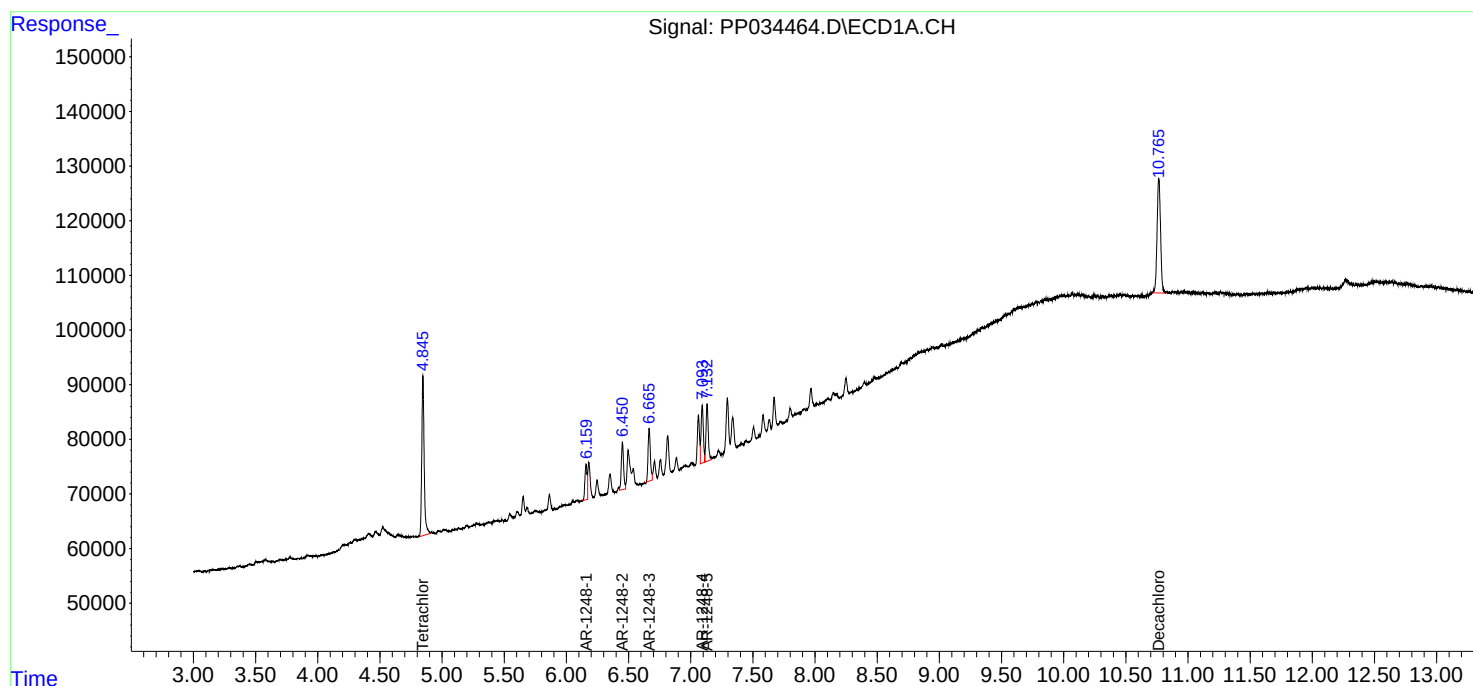

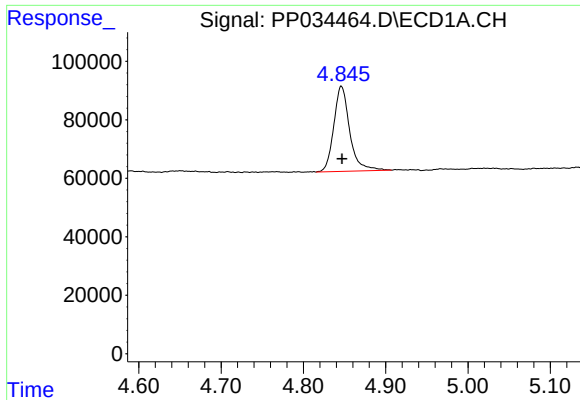


#1 Tetrachloro-m-xylene

R.T.: 4.846 min
Delta R.T.: -0.001 min
Response: 391742
Conc: 5.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
4/1/2021 12:51:18 PM

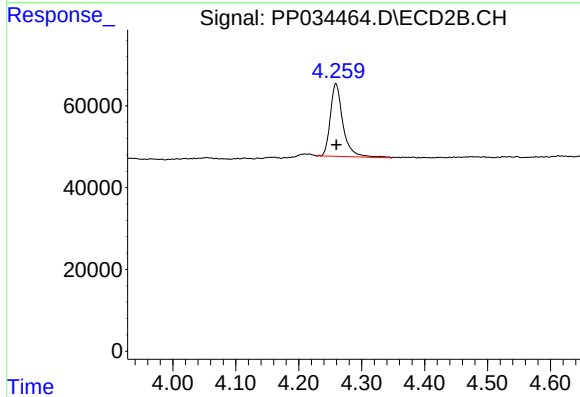


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 245722
Conc: 5.43 ng/ml

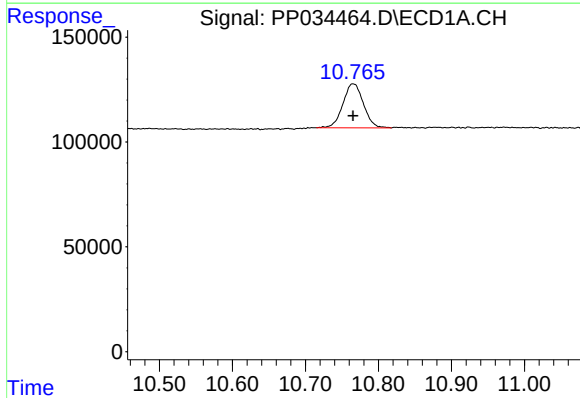


#2 Decachlorobiphenyl

R.T.: 10.765 min
Delta R.T.: 0.000 min
Response: 408809
Conc: 5.39 ng/ml

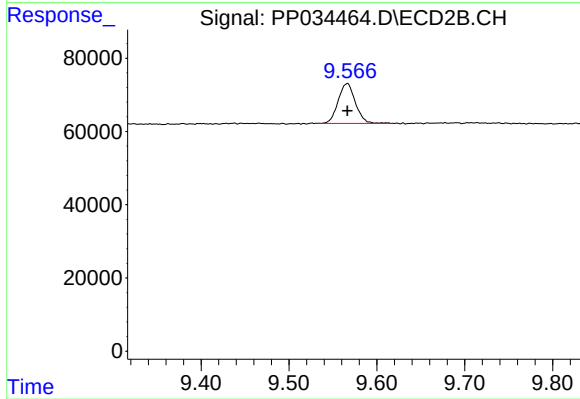

#2 Decachlorobiphenyl

R.T.: 9.566 min
Delta R.T.: 0.000 min
Response: 147696
Conc: 5.38 ng/ml

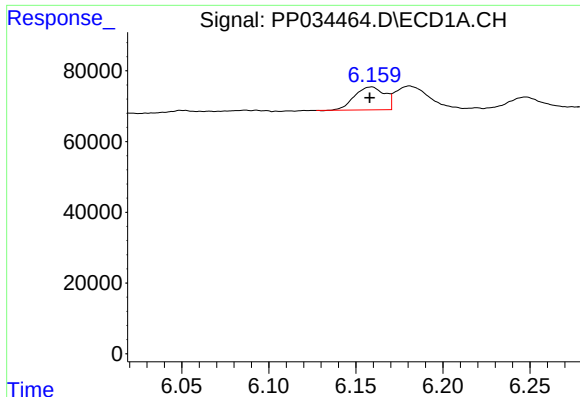


#21 AR-1248-1

R.T.: 6.159 min
Delta R.T.: 0.001 min
Response: 78880
Conc: 56.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
4/1/2021 12:51:18 PM

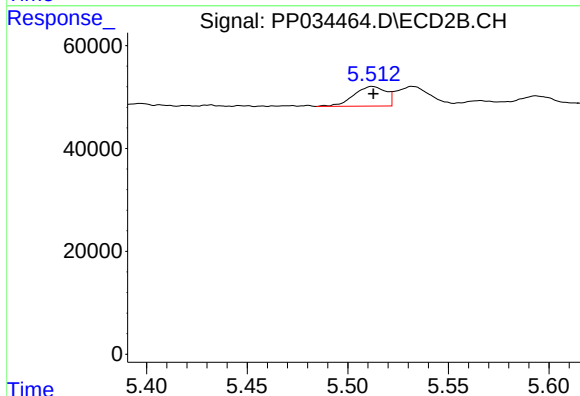


#21 AR-1248-1

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 42104
Conc: 58.91 ng/ml

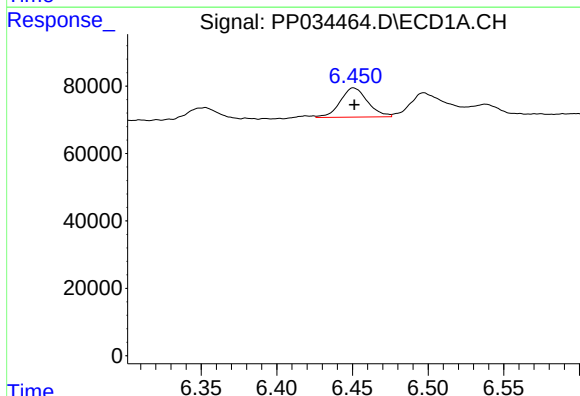


#22 AR-1248-2

R.T.: 6.450 min
Delta R.T.: -0.001 min
Response: 110275
Conc: 56.84 ng/ml m

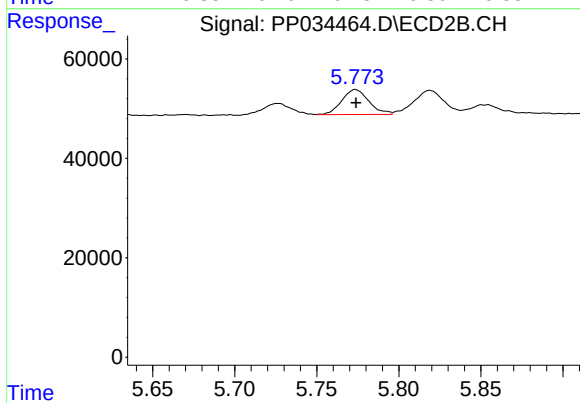

#22 AR-1248-2

R.T.: 5.774 min
Delta R.T.: 0.000 min
Response: 57602
Conc: 57.07 ng/ml

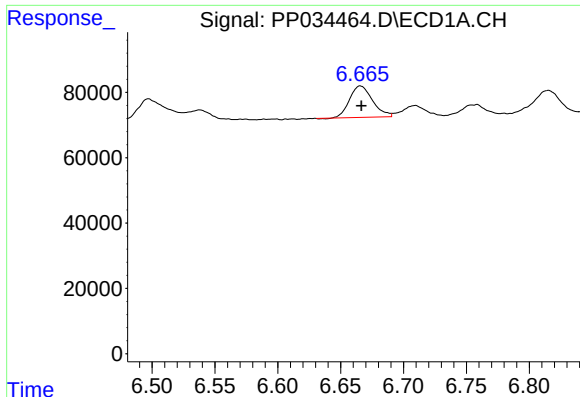


#23 AR-1248-3

R.T.: 6.666 min
Delta R.T.: -0.001 min
Response: 122196
Conc: 51.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050


Manual Integrations
APPROVED

Ankita
4/1/2021 12:51:18 PM

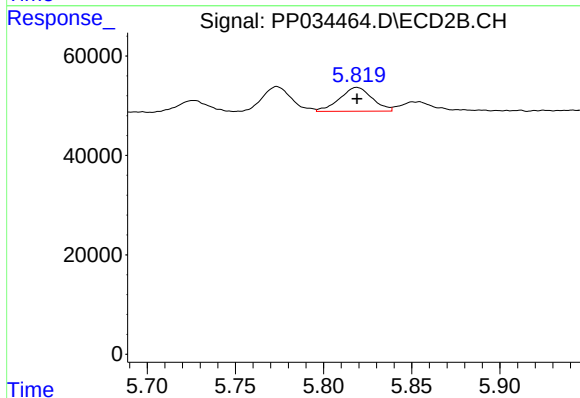


#23 AR-1248-3

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 61740
Conc: 57.44 ng/ml

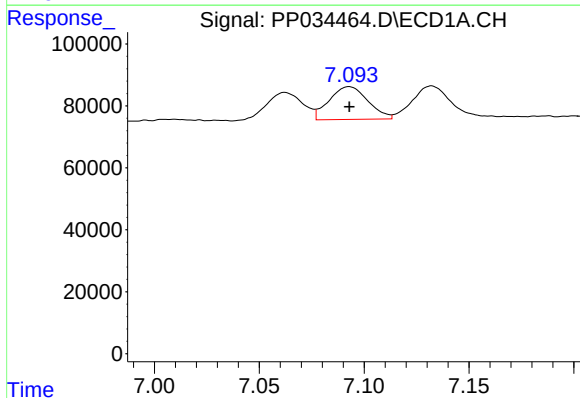


#24 AR-1248-4

R.T.: 7.093 min
Delta R.T.: 0.000 min
Response: 135921
Conc: 53.45 ng/ml

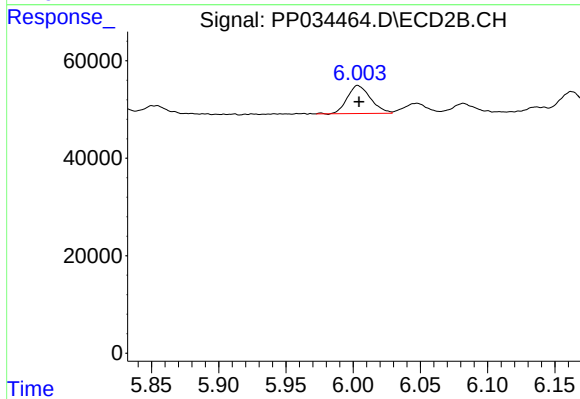

#24 AR-1248-4

R.T.: 6.004 min
Delta R.T.: 0.000 min
Response: 69216
Conc: 55.62 ng/ml

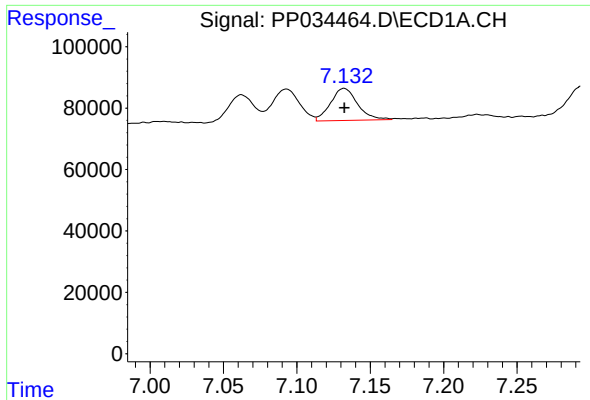


#25 AR-1248-5

R.T.: 7.132 min
Delta R.T.: 0.000 min
Response: 133880
Conc: 52.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Ankita
4/1/2021 12:51:18 PM

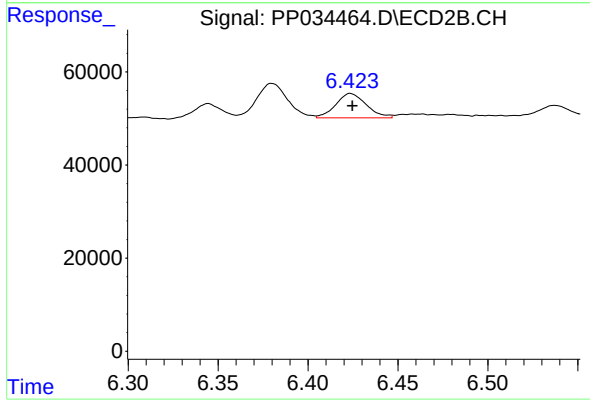

#25 AR-1248-5

R.T.: 6.423 min
Delta R.T.: -0.002 min
Response: 62304
Conc: 55.99 ng/ml m