

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033121\
 Data File : PP034489.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2021 9:56
 Operator : DD\AJ
 Sample : M1865-03 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-030321-SR-03

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:55:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 13:23:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.846	4.254	204995	116231	2.687m	2.587m
2) SA Decachlor...	10.763	9.565	142665	56003	1.853m	1.983

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033121\
Data File : PP034489.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2021 9:56
Operator : DD\AJ
Sample : M1865-03 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-03


Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 13:23:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

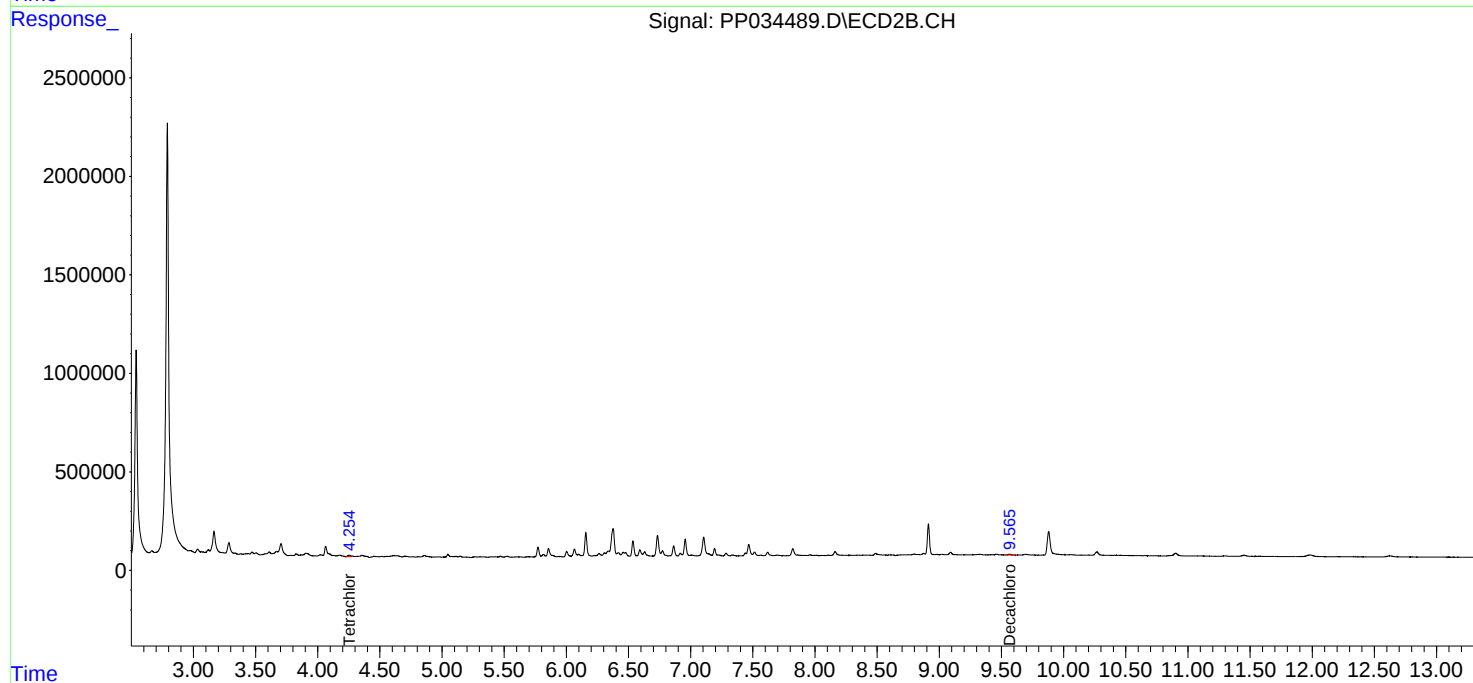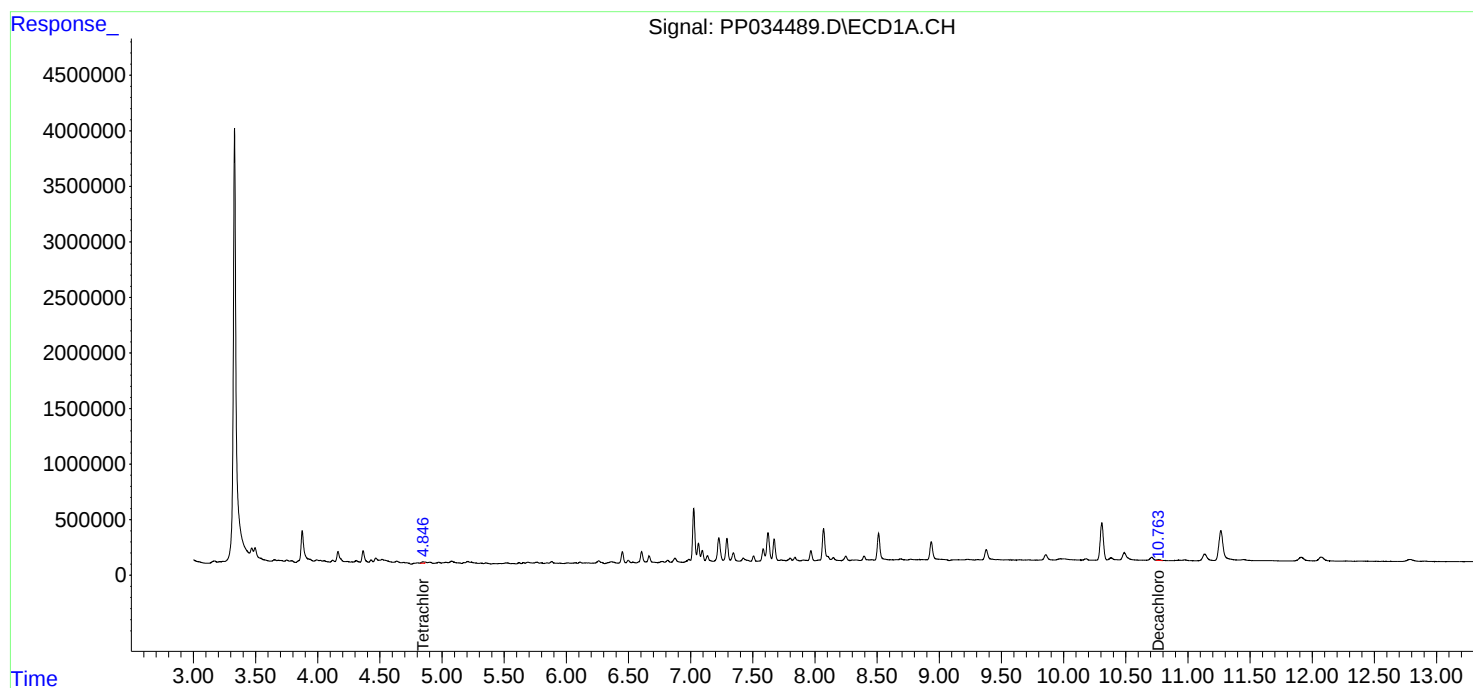

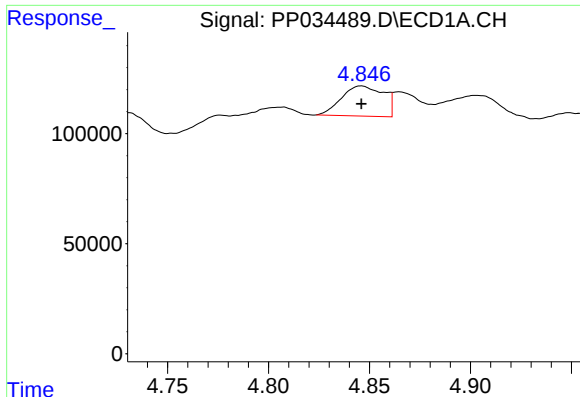


#1 Tetrachloro-m-xylene

R.T.: 4.846 min
Delta R.T.: 0.000 min
Response: 204995
Conc: 2.69 ng/ml m

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-03


Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:27 PM

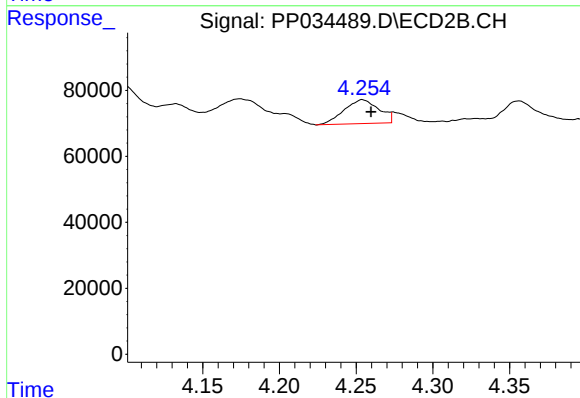


#1 Tetrachloro-m-xylene

R.T.: 4.254 min
Delta R.T.: -0.006 min
Response: 116231
Conc: 2.59 ng/ml m

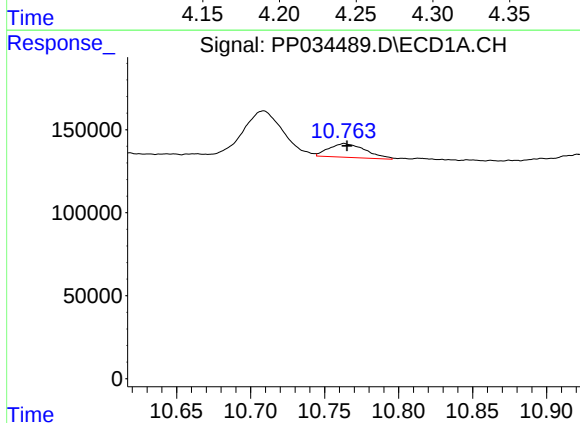

#2 Decachlorobiphenyl

R.T.: 10.763 min
Delta R.T.: -0.002 min
Response: 142665
Conc: 1.85 ng/ml m

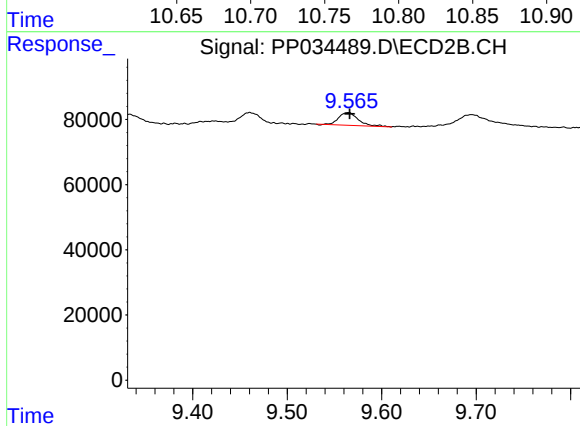

#2 Decachlorobiphenyl

R.T.: 9.565 min
Delta R.T.: -0.001 min
Response: 56003
Conc: 1.98 ng/ml