

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033121\
 Data File : PP034511.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2021 17:12
 Operator : DD\AJ
 Sample : M1865-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-030321-SR-06

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:55:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 17:48:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.846	4.258	1916166	911080	25.119	20.281
2) SA Decachlor...	10.765	9.564	1680569	763713	21.831m	27.048
Target Compounds						
26) L6 AR-1254-1	7.064	6.379	12052836	7306954	4383.599	3960.608
27) L6 AR-1254-2	7.292	6.536	16235925	5328672	3818.301	3330.652
28) L6 AR-1254-3	7.672	6.956	15158050	7375438	3321.087	2955.187
29) L6 AR-1254-4	7.968	7.193	7341734	2986413	2374.537	2271.827
30) L6 AR-1254-5	8.395	7.619	7162121	4227857	2015.322	2080.197

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033121\
Data File : PP034511.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2021 17:12
Operator : DD\AJ
Sample : M1865-06
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06


Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 17:48:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

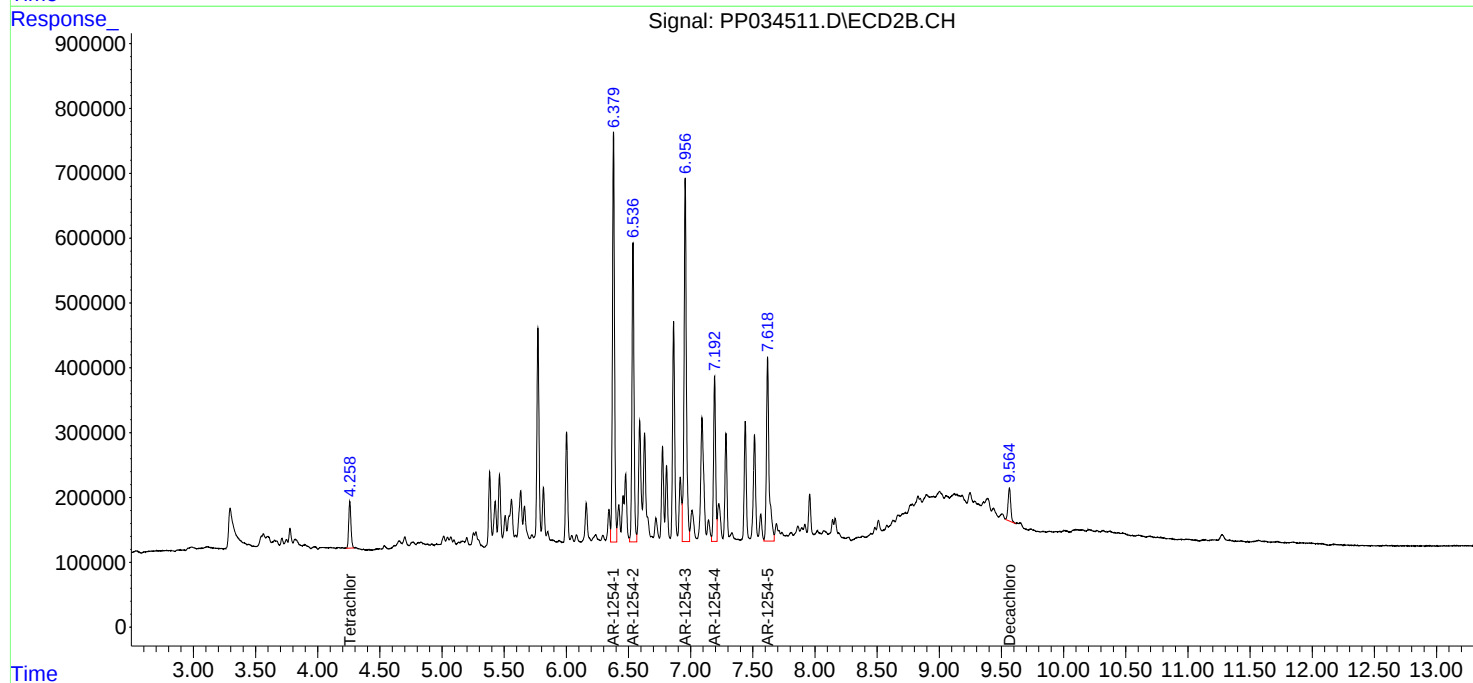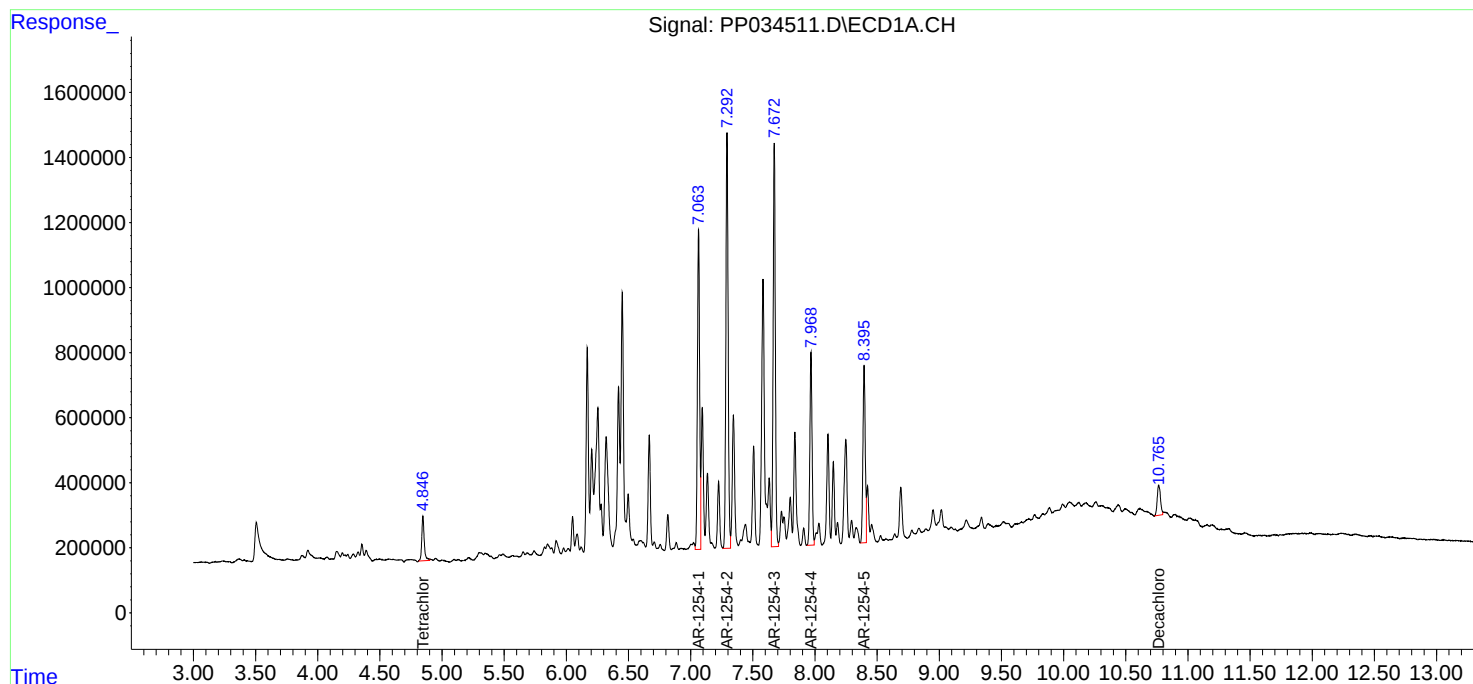

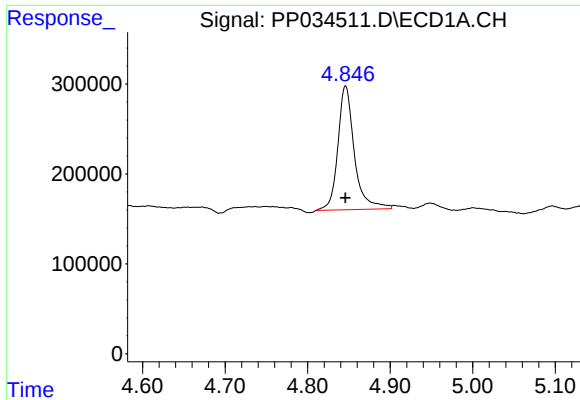


#1 Tetrachloro-m-xylene

R.T.: 4.846 min
Delta R.T.: 0.000 min
Response: 1916166
Conc: 25.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06


Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:39 PM

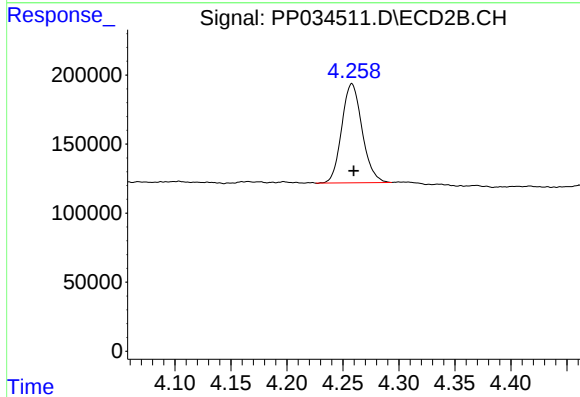


#1 Tetrachloro-m-xylene

R.T.: 4.258 min
Delta R.T.: -0.002 min
Response: 911080
Conc: 20.28 ng/ml

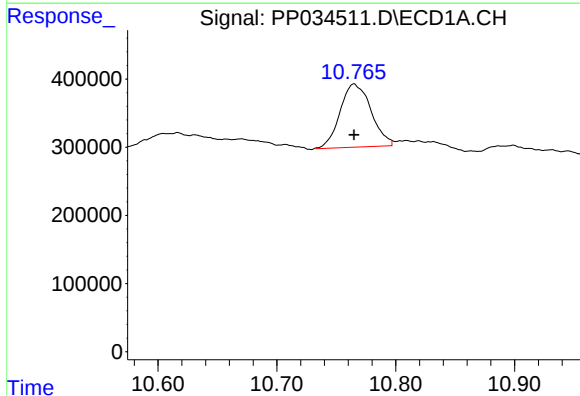


#2 Decachlorobiphenyl

R.T.: 10.765 min
Delta R.T.: 0.000 min
Response: 1680569
Conc: 21.83 ng/ml m

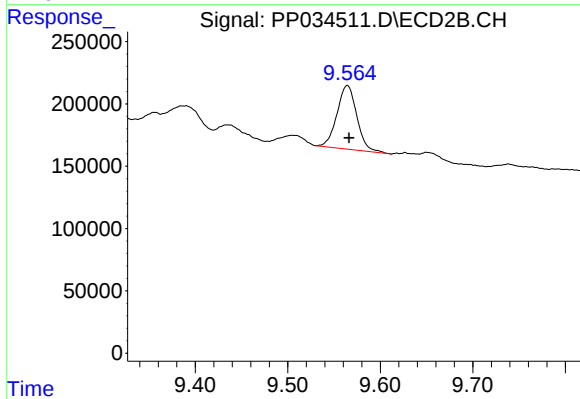

#2 Decachlorobiphenyl

R.T.: 9.564 min
Delta R.T.: -0.002 min
Response: 763713
Conc: 27.05 ng/ml

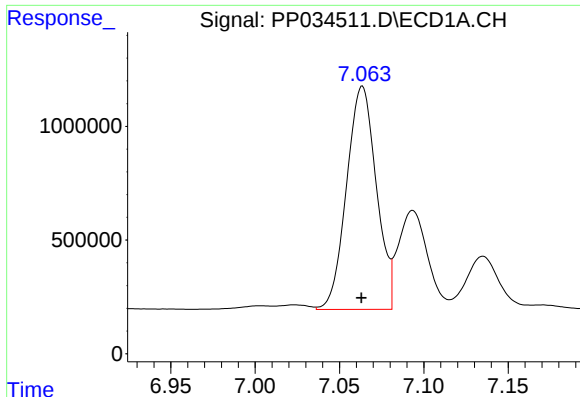


#26 AR-1254-1

R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 12052836
Conc: 4383.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06


Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:39 PM

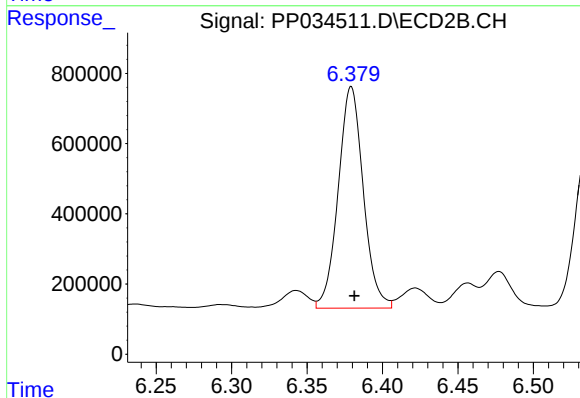


#26 AR-1254-1

R.T.: 6.379 min
Delta R.T.: -0.002 min
Response: 7306954
Conc: 3960.61 ng/ml

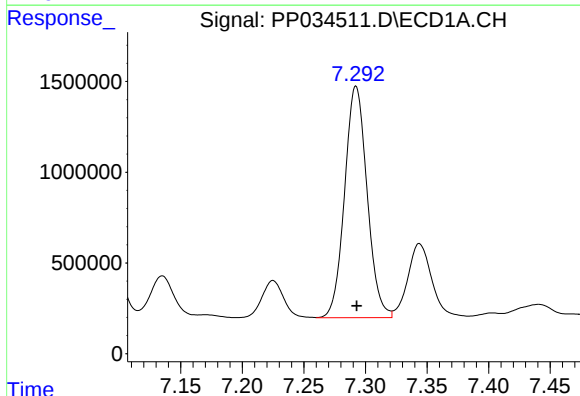


#27 AR-1254-2

R.T.: 7.292 min
Delta R.T.: 0.000 min
Response: 16235925
Conc: 3818.30 ng/ml

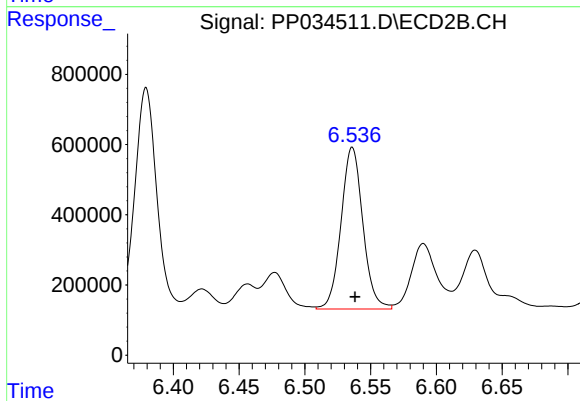

#27 AR-1254-2

R.T.: 6.536 min
Delta R.T.: -0.002 min
Response: 5328672
Conc: 3330.65 ng/ml

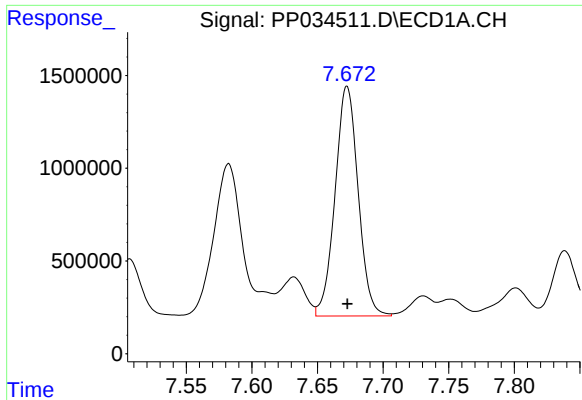


#28 AR-1254-3

R.T.: 7.672 min
Delta R.T.: 0.000 min
Response: 15158050
Conc: 3321.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06


Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:39 PM

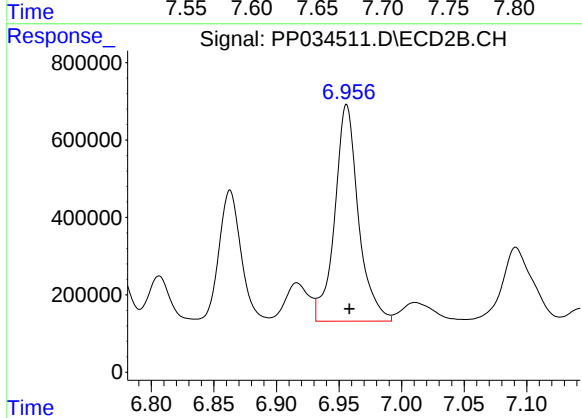


#28 AR-1254-3

R.T.: 6.956 min
Delta R.T.: -0.002 min
Response: 7375438
Conc: 2955.19 ng/ml

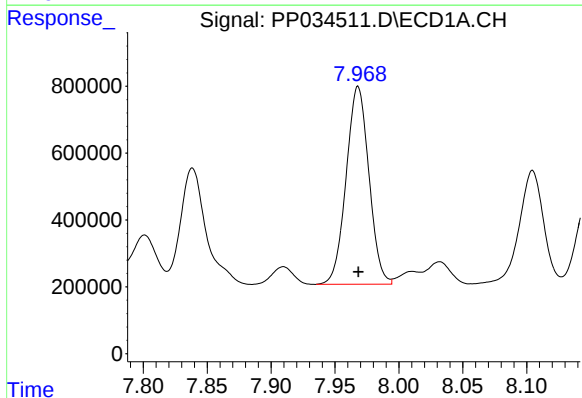


#29 AR-1254-4

R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 7341734
Conc: 2374.54 ng/ml

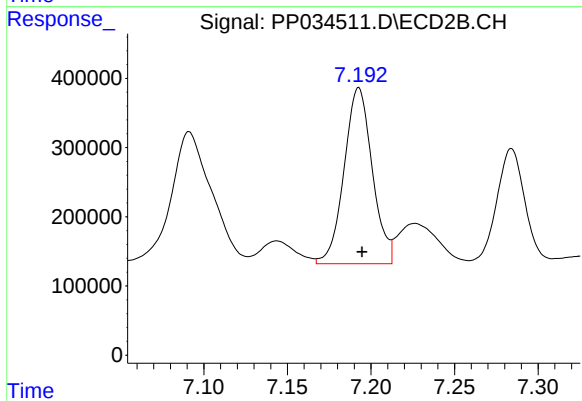

#29 AR-1254-4

R.T.: 7.193 min
Delta R.T.: -0.002 min
Response: 2986413
Conc: 2271.83 ng/ml

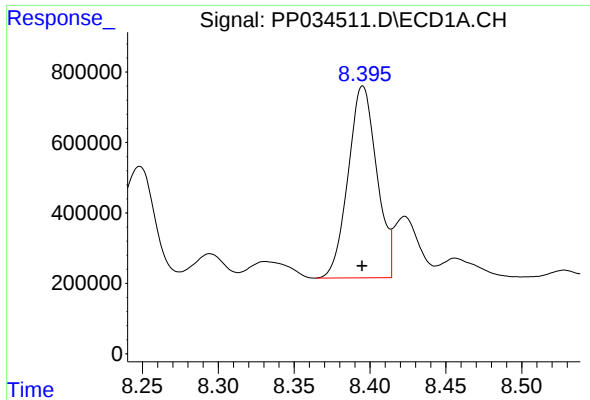


#30 AR-1254-5

R.T.: 8.395 min
Delta R.T.: 0.000 min
Response: 7162121
Conc: 2015.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06

Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:39 PM

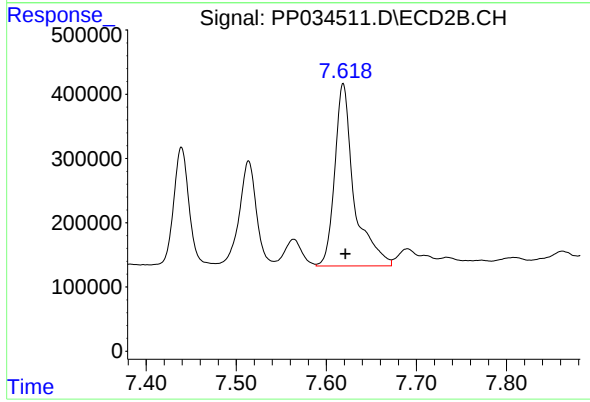

#30 AR-1254-5

R.T.: 7.619 min
Delta R.T.: -0.002 min
Response: 4227857
Conc: 2080.20 ng/ml