

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033121\
 Data File : PP034515.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Mar 2021 19:27
 Operator : DD\AJ
 Sample : M1865-07
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-030321-SR-07

Manual Integrations
 APPROVED

Ankita
 4/1/2021 12:55:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 03:13:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.847	4.258	1783829	968340	23.384	21.556
2) SA Decachlor...	10.769	9.565	1706132	622309	22.163	22.040
Target Compounds						
26) L6 AR-1254-1	7.064	6.381	2774034	1451431	1008.912m	786.723m
27) L6 AR-1254-2	7.293	6.535	2690421	739344	632.723m	462.122m#
28) L6 AR-1254-3	7.673	6.956	1922831	1034490	421.287m	414.499m
29) L6 AR-1254-4	7.968	7.192	725109	322776	234.522m	245.542m
30) L6 AR-1254-5	8.397	7.619	663196	568813	186.614m	279.868m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033121\
Data File : PP034515.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Mar 2021 19:27
Operator : DD\AJ
Sample : M1865-07
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
PCB-030321-SR-07


Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 03:13:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

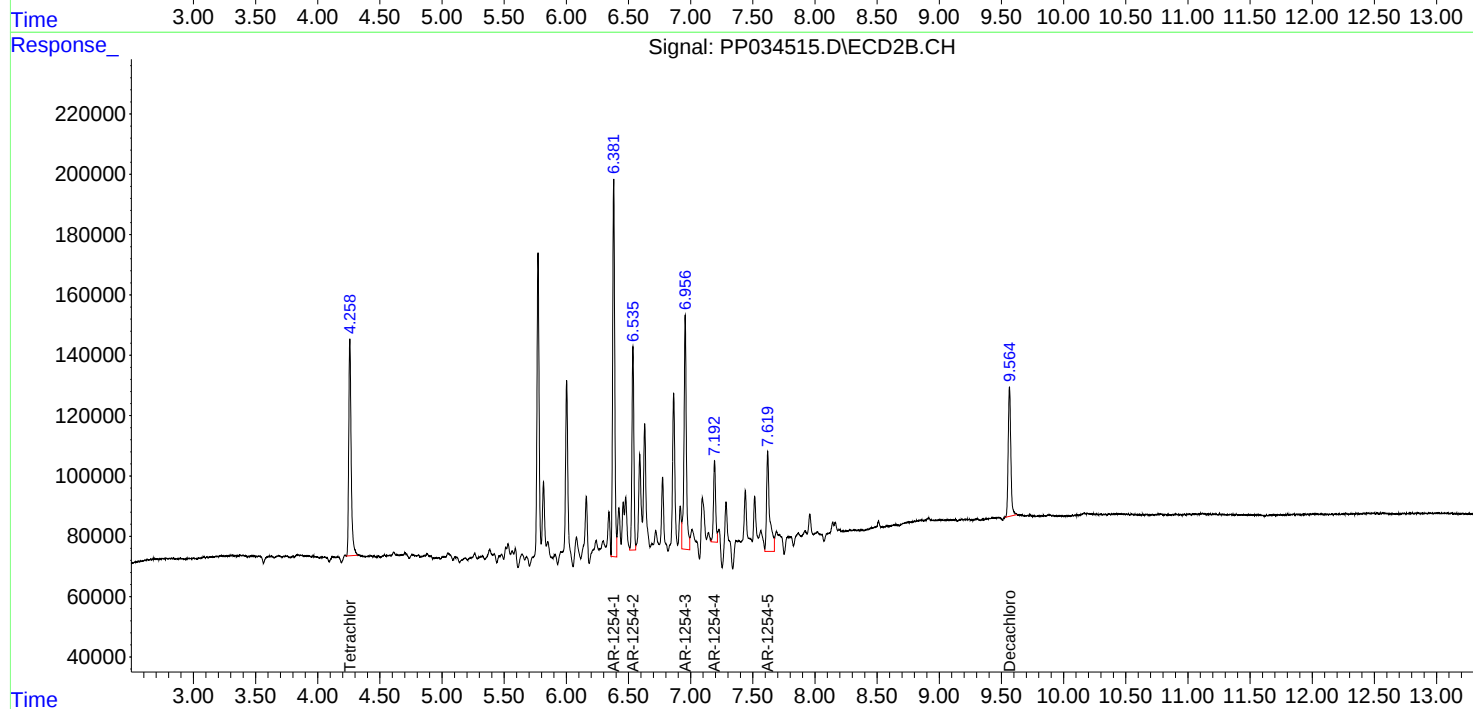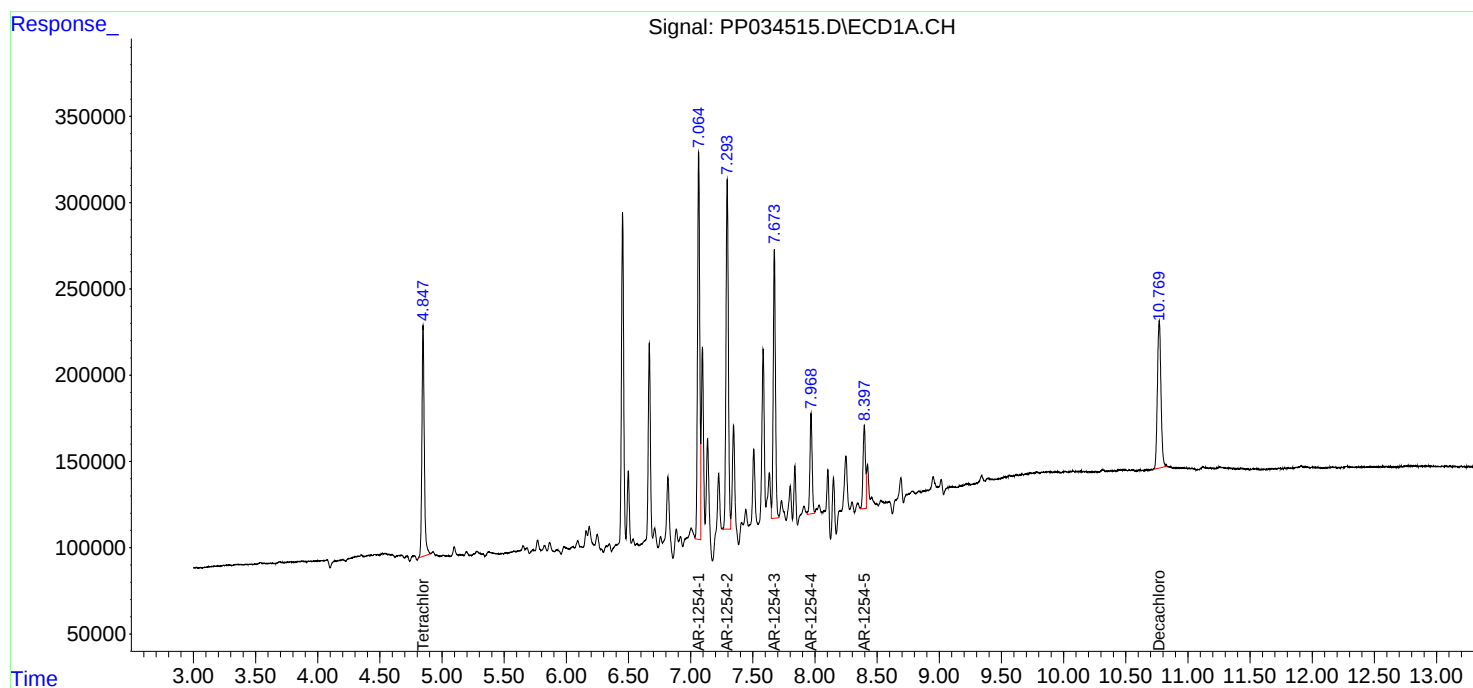

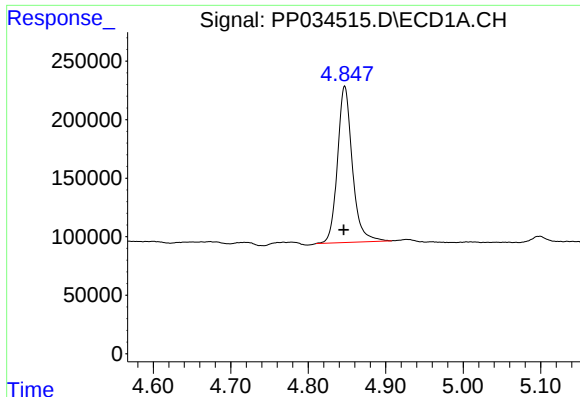


#1 Tetrachloro-m-xylene

R.T.: 4.847 min
Delta R.T.: 0.001 min
Response: 1783829
Conc: 23.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-07


Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:45 PM

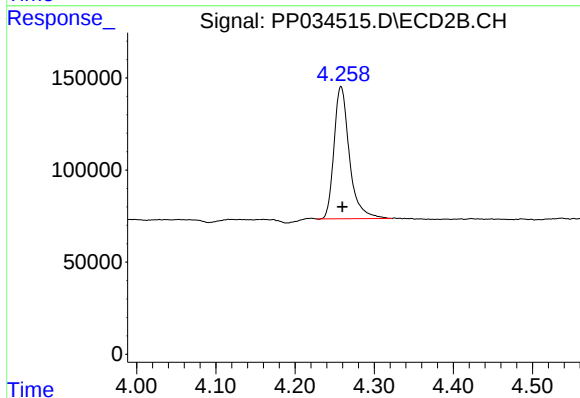


#1 Tetrachloro-m-xylene

R.T.: 4.258 min
Delta R.T.: -0.002 min
Response: 968340
Conc: 21.56 ng/ml

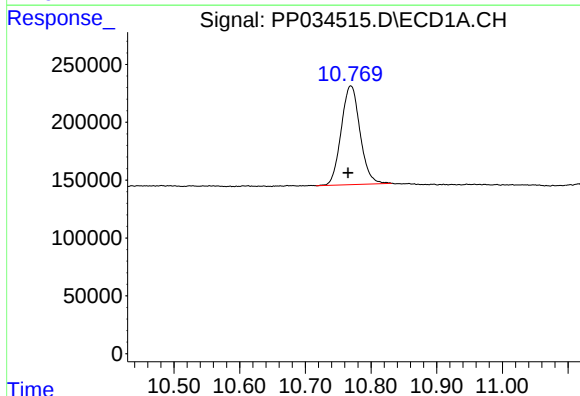


#2 Decachlorobiphenyl

R.T.: 10.769 min
Delta R.T.: 0.004 min
Response: 1706132
Conc: 22.16 ng/ml

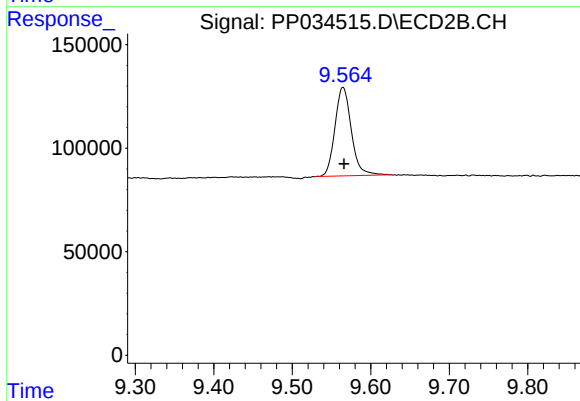

#2 Decachlorobiphenyl

R.T.: 9.565 min
Delta R.T.: -0.002 min
Response: 622309
Conc: 22.04 ng/ml

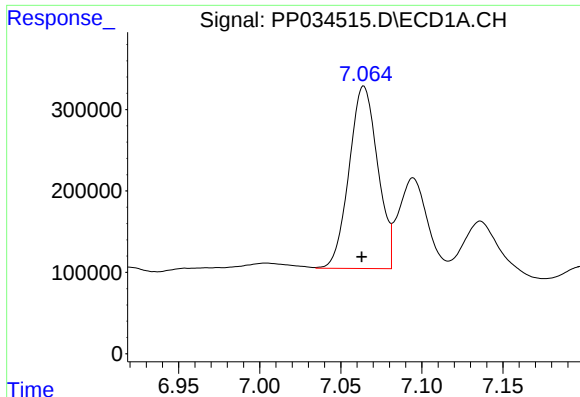


#26 AR-1254-1

R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 2774034
Conc: 1008.91 ng/ml m

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-07


Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:45 PM

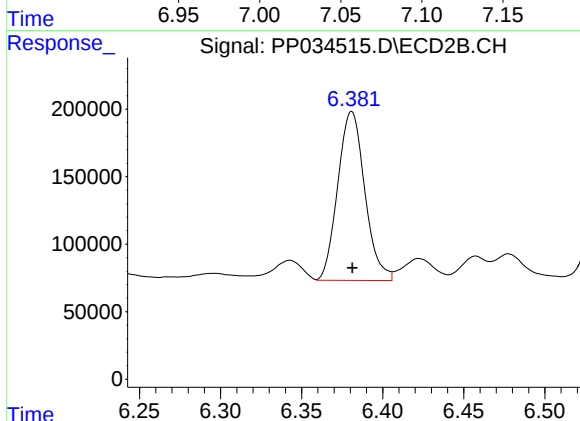


#26 AR-1254-1

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 1451431
Conc: 786.72 ng/ml m

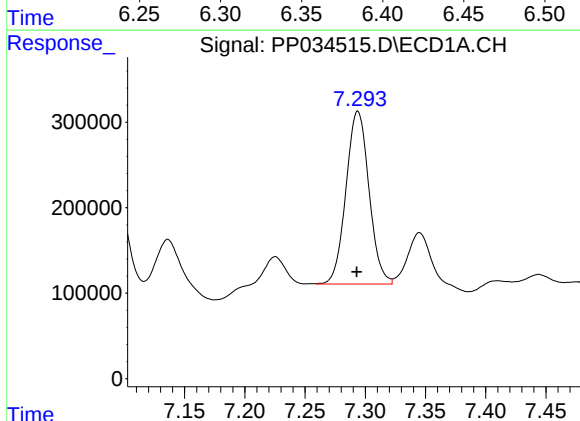


#27 AR-1254-2

R.T.: 7.293 min
Delta R.T.: 0.000 min
Response: 2690421
Conc: 632.72 ng/ml m

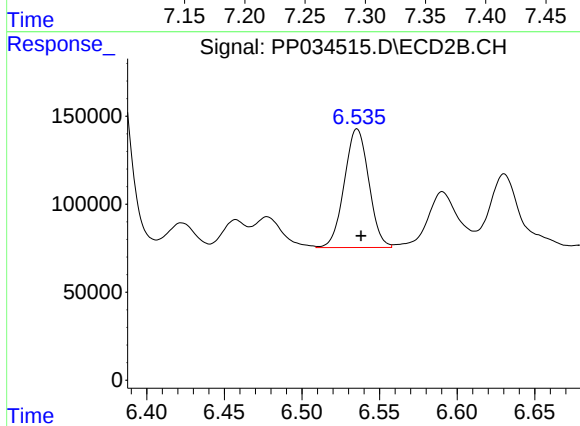

#27 AR-1254-2

R.T.: 6.535 min
Delta R.T.: -0.003 min
Response: 739344
Conc: 462.12 ng/ml m

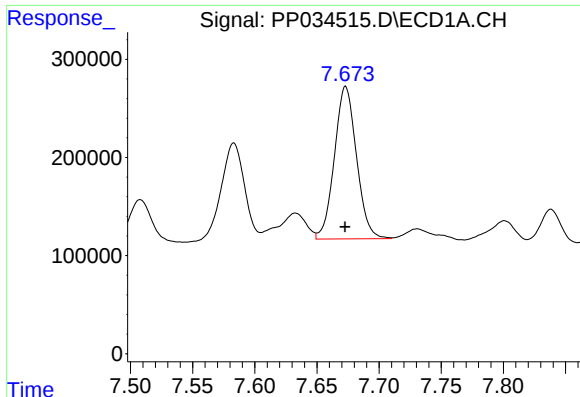


#28 AR-1254-3

R.T.: 7.673 min
Delta R.T.: 0.000 min
Response: 1922831
Conc: 421.29 ng/ml m

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-07


Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:45 PM

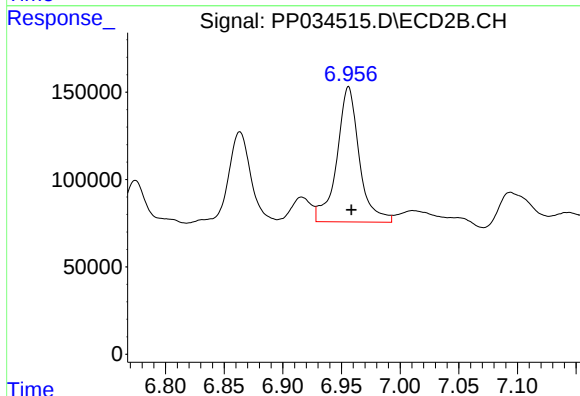


#28 AR-1254-3

R.T.: 6.956 min
Delta R.T.: -0.003 min
Response: 1034490
Conc: 414.50 ng/ml m

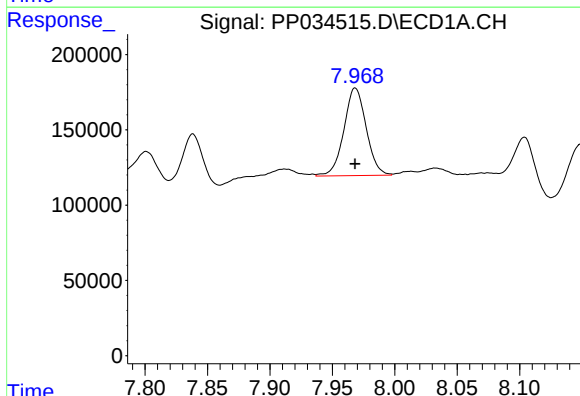


#29 AR-1254-4

R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 725109
Conc: 234.52 ng/ml m

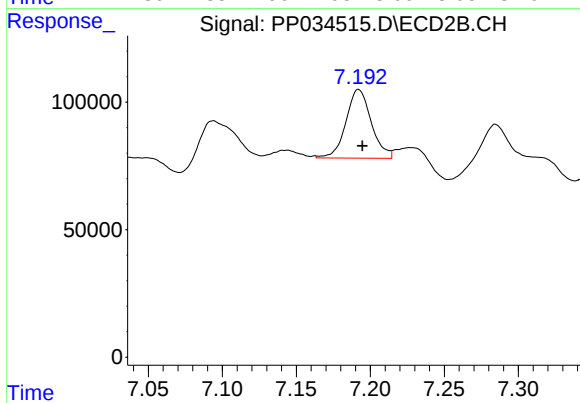

#29 AR-1254-4

R.T.: 7.192 min
Delta R.T.: -0.003 min
Response: 322776
Conc: 245.54 ng/ml m

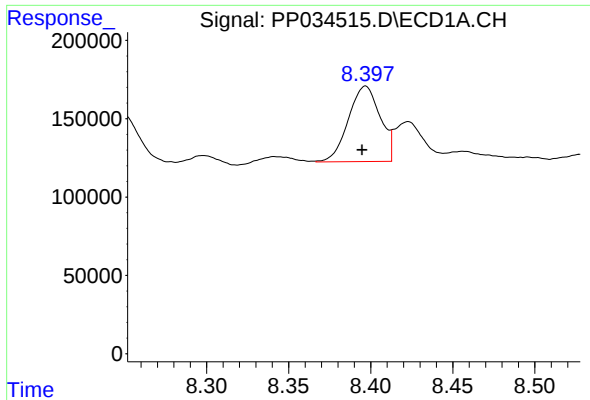


#30 AR-1254-5

R.T.: 8.397 min
Delta R.T.: 0.002 min
Response: 663196
Conc: 186.61 ng/ml m

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-07

Manual Integrations
APPROVED

Ankita
4/1/2021 12:55:45 PM

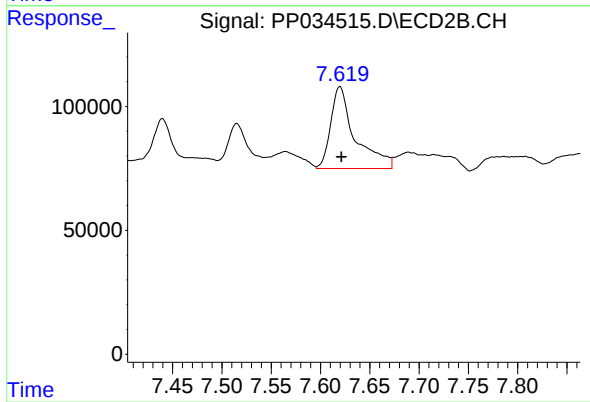

#30 AR-1254-5

R.T.: 7.619 min
Delta R.T.: -0.002 min
Response: 568813
Conc: 279.87 ng/ml m