

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033122\
 Data File : PP045376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2022 12:54
 Operator : YP\AJ
 Sample : N2177-02RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TT-039-IDWGW-20220329RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 13:50:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 31 07:54:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.887	3.146	53181702	35051431	22.041	22.152
2) SA Decachlor...	10.003	8.496	7925829	9293781	5.532	6.129

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033122\
Data File : PP045376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2022 12:54
Operator : YP\AJ
Sample : N2177-02RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TT-039-IDWGW-20220329RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 13:50:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 31 07:54:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

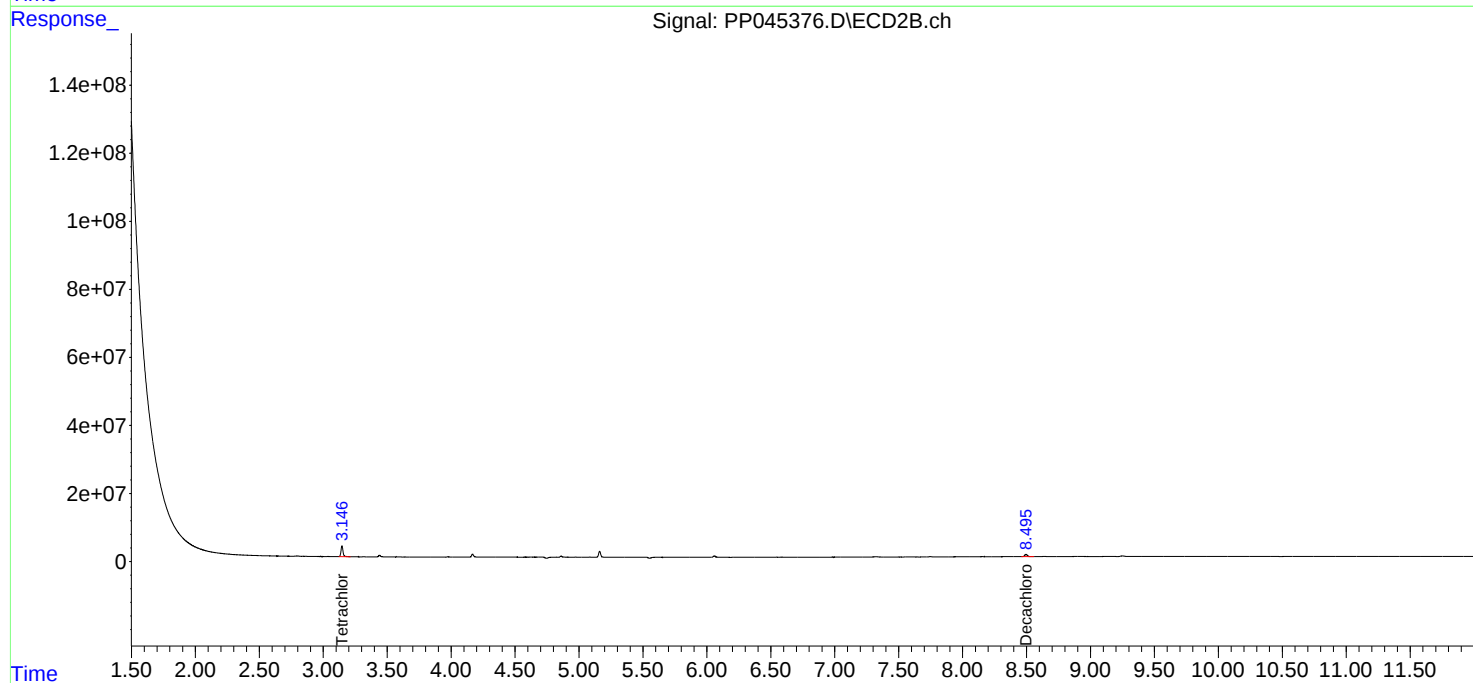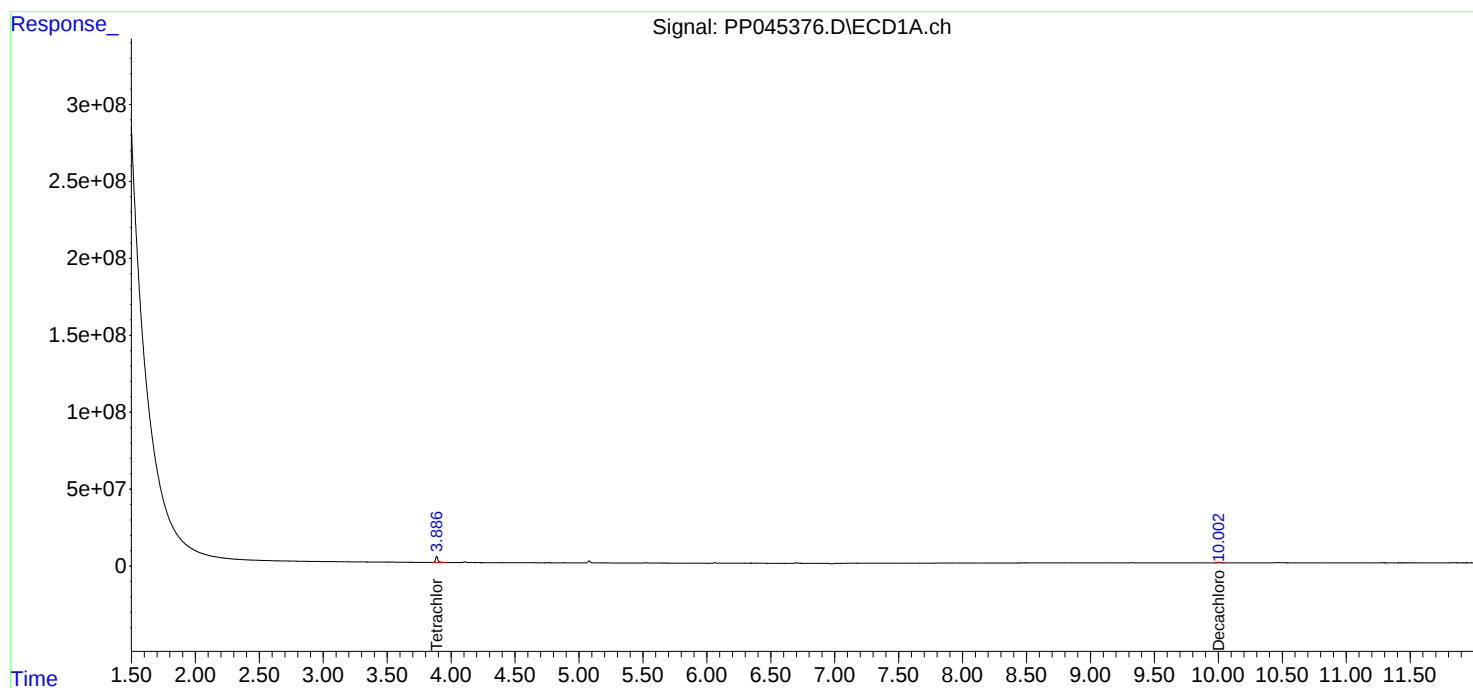


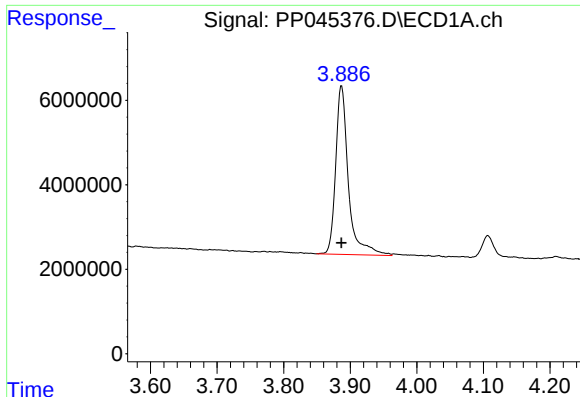

#1 Tetrachloro-m-xylene


R.T.: 3.887 min
Delta R.T.: 0.000 min
Response: 53181702
Conc: 22.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
TT-039-IDWGW-20220329RE

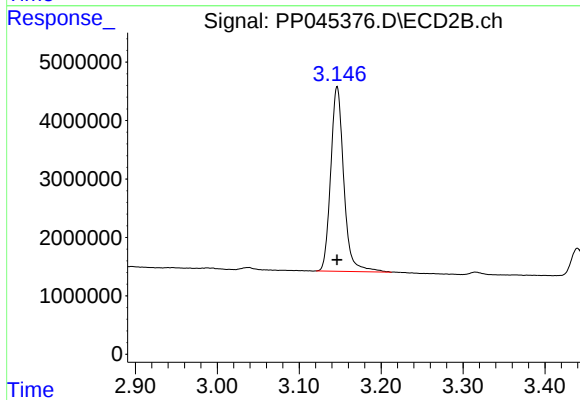


#1 Tetrachloro-m-xylene

R.T.: 3.146 min
Delta R.T.: 0.000 min
Response: 35051431
Conc: 22.15 ng/ml

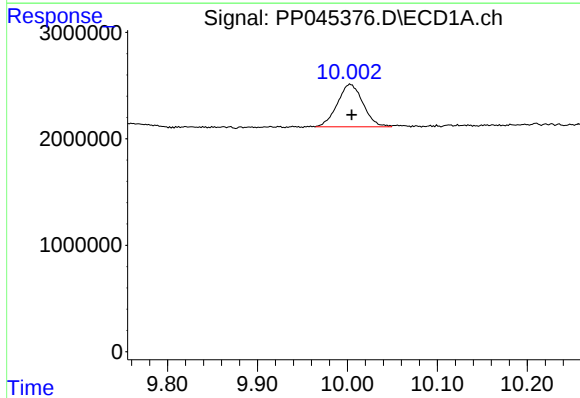

#2 Decachlorobiphenyl

R.T.: 10.003 min
Delta R.T.: -0.002 min
Response: 7925829
Conc: 5.53 ng/ml

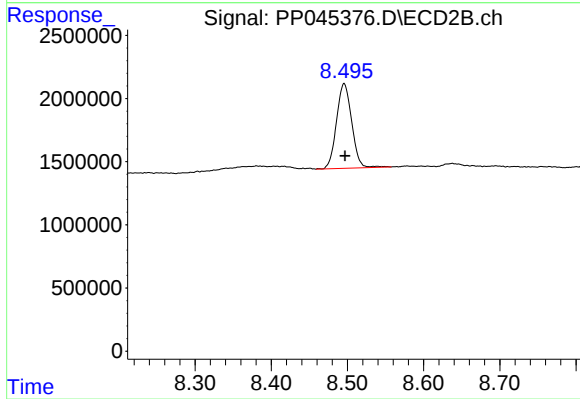

#2 Decachlorobiphenyl

R.T.: 8.496 min
Delta R.T.: -0.001 min
Response: 9293781
Conc: 6.13 ng/ml