

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033125\
 Data File : PP071017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2025 11:31
 Operator : YP\AJ
 Sample : Q1677-02 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JEI299N-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/01/2025
 Supervised By :mohammad ahmed 04/07/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 11:45:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.519	3.816	2508974	2437634	1.717m	2.351m#
2) SA Decachlor...	10.251	8.864	3241682	1492236	3.080m	1.893 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP033125\
Data File : PP071017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2025 11:31
Operator : YP\AJ
Sample : Q1677-02 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JEI299N-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/01/2025
Supervised By :mohammad ahmed 04/07/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 11:45:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

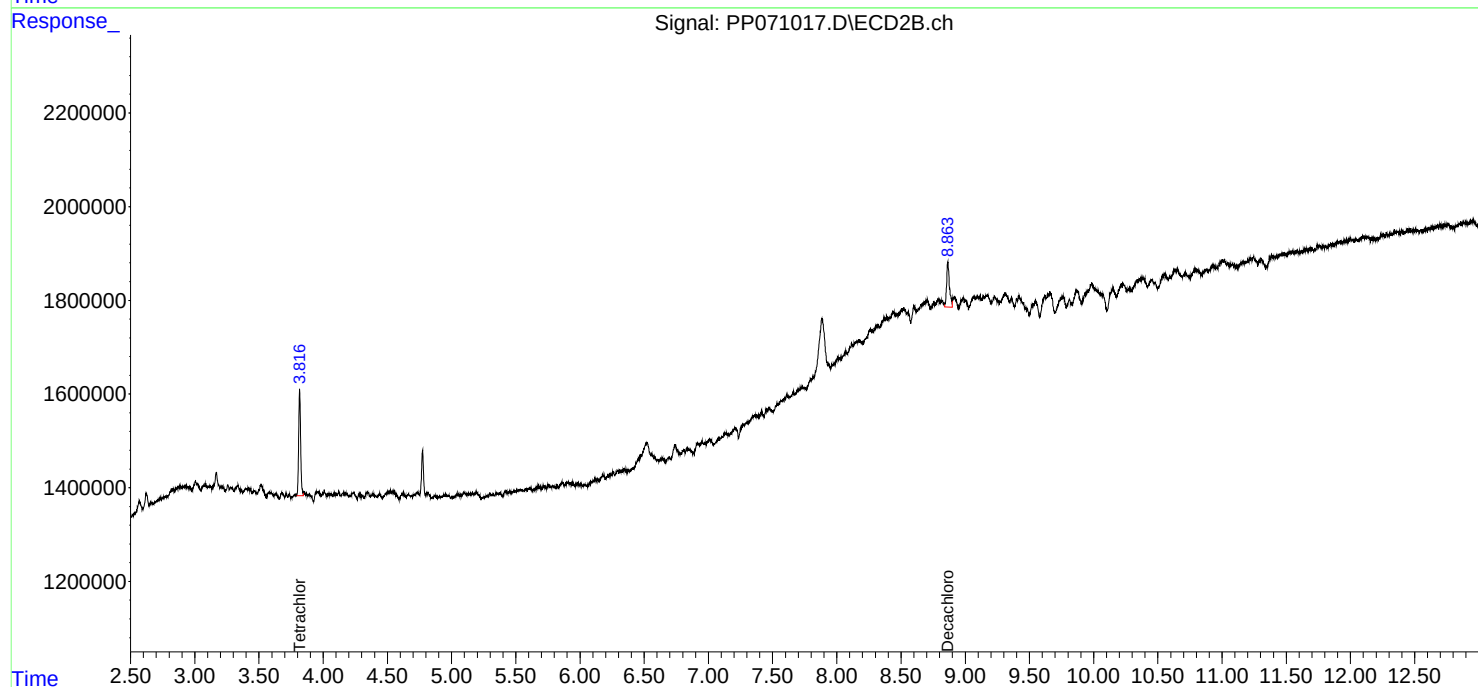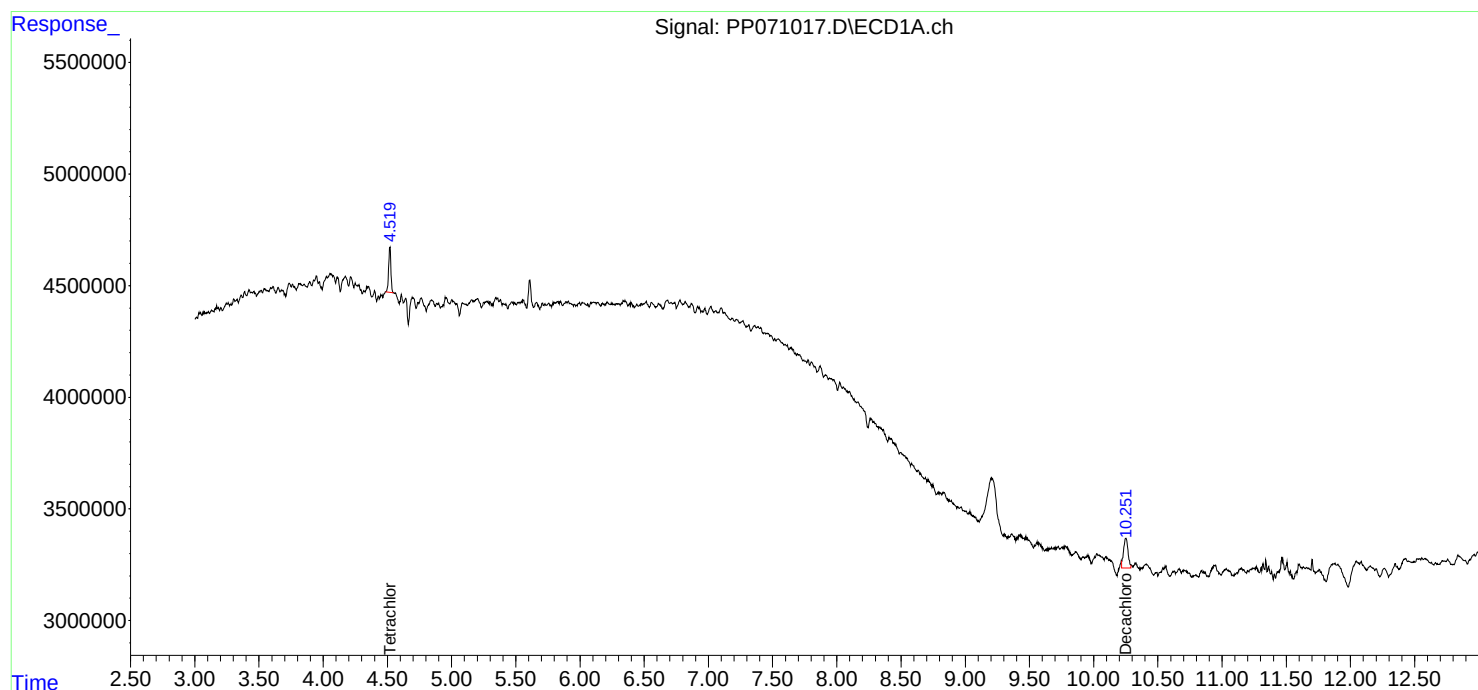

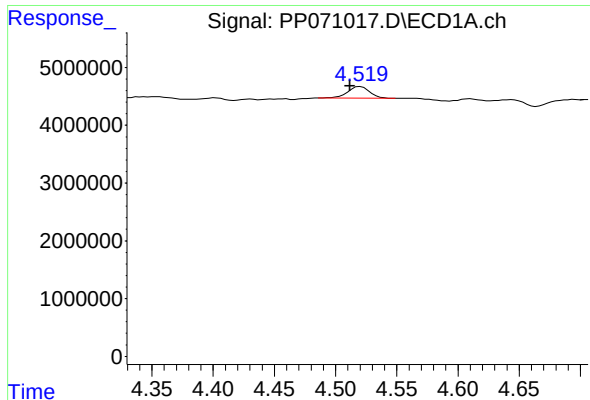


#1 Tetrachloro-m-xylene

R.T.: 4.519 min
Delta R.T.: 0.007 min
Response: 2508974
Conc: 1.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
JEI299N-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/01/2025
Supervised By :mohammad ahmed 04/07/2025

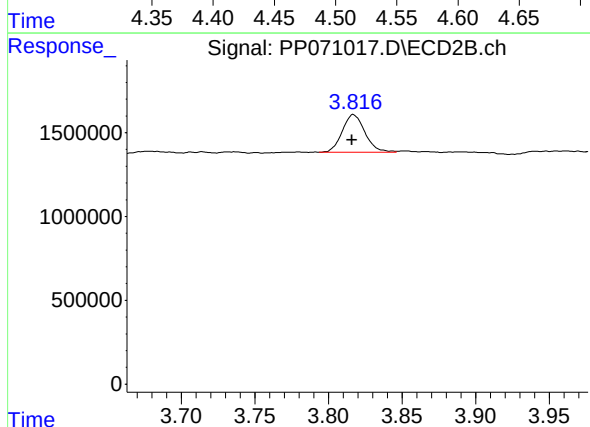


#1 Tetrachloro-m-xylene

R.T.: 3.816 min
Delta R.T.: 0.000 min
Response: 2437634
Conc: 2.35 ng/ml m

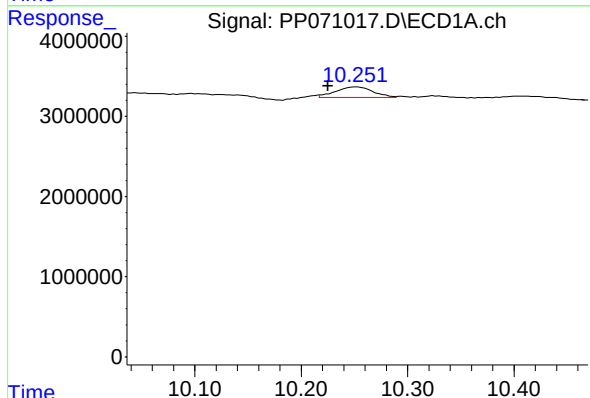

#2 Decachlorobiphenyl

R.T.: 10.251 min
Delta R.T.: 0.026 min
Response: 3241682
Conc: 3.08 ng/ml m

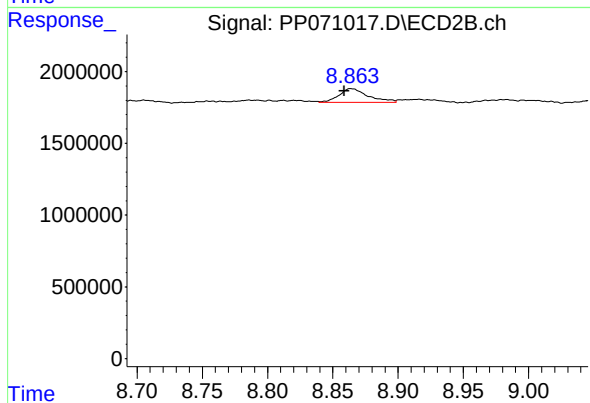

#2 Decachlorobiphenyl

R.T.: 8.864 min
Delta R.T.: 0.006 min
Response: 1492236
Conc: 1.89 ng/ml