

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
 Data File : PP034529.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2021 11:07
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 14:56:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
2)	SA Decachlor...	0.000	9.575	0	1331	N.D.	0.047 #
Target Compounds							
20)	L4 AR-1242-5	0.000	6.378	0	5177	N.D.	6.314 #
25)	L5 AR-1248-5	0.000	6.438	0	5445	N.D.	4.818 #
26)	L6 AR-1254-1	7.068	6.378	18940	5177	6.888	2.806 #
27)	L6 AR-1254-2	0.000	6.540	0	7320	N.D.	4.575 #
28)	L6 AR-1254-3	7.671	6.959	9565	18904	2.096	7.575 #
29)	L6 AR-1254-4	7.972	7.200	30693	10172	9.927	7.738
30)	L6 AR-1254-5	8.399	7.621	15408	28780	4.336	14.160 #
31)	L7 AR-1260-1	0.000	7.085	0	17843	N.D.	11.619 #
32)	L7 AR-1260-2	0.000	7.276	0	8620	N.D.	4.772 #
33)	L7 AR-1260-3	8.476	7.434	6993	15619	2.313	9.003 #
34)	L7 AR-1260-4	8.693	7.919	10686	7017	3.061	4.894 #
35)	L7 AR-1260-5	9.016	8.138f	8718	2554	1.217	0.748 #
36)	L8 AR-1262-1	8.476	7.621	6993	28780	1.528	26.797 #
37)	L8 AR-1262-2	9.016	8.138f	8718	2554	1.117	0.744 #
38)	L8 AR-1262-3	0.000	8.435	0	80	N.D.	0.053 #
40)	L8 AR-1262-5	0.000	9.011	0	1494	N.D.	1.317 #
41)	L9 AR-1268-1	0.000	8.435	0	80	N.D.	0.019 #
43)	L9 AR-1268-3	0.000	8.726	0	6157	N.D.	1.692 #
44)	L9 AR-1268-4	0.000	9.011	0	1494	N.D.	1.160 #
45)	L9 AR-1268-5	10.444	9.303	3433	5963	0.120	0.574 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
Data File : PP034529.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2021 11:07
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 14:56:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

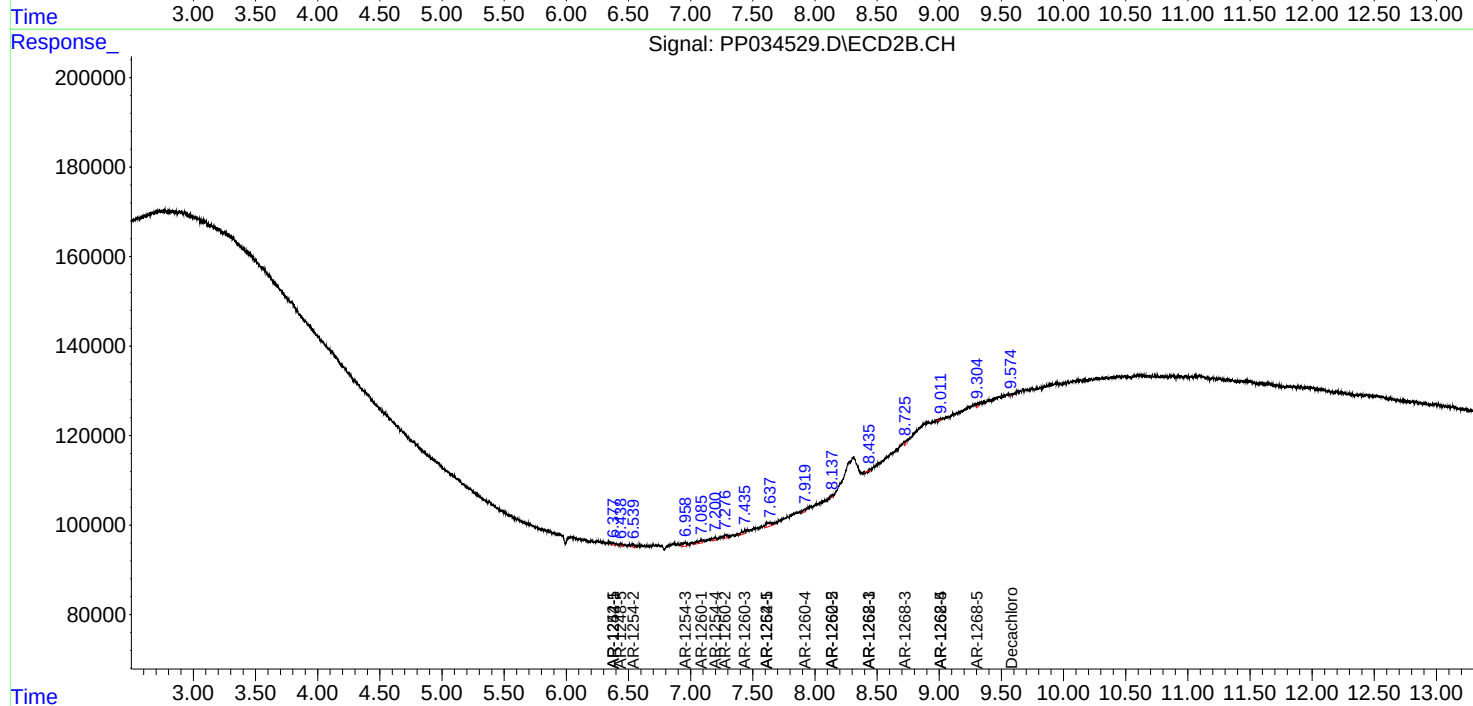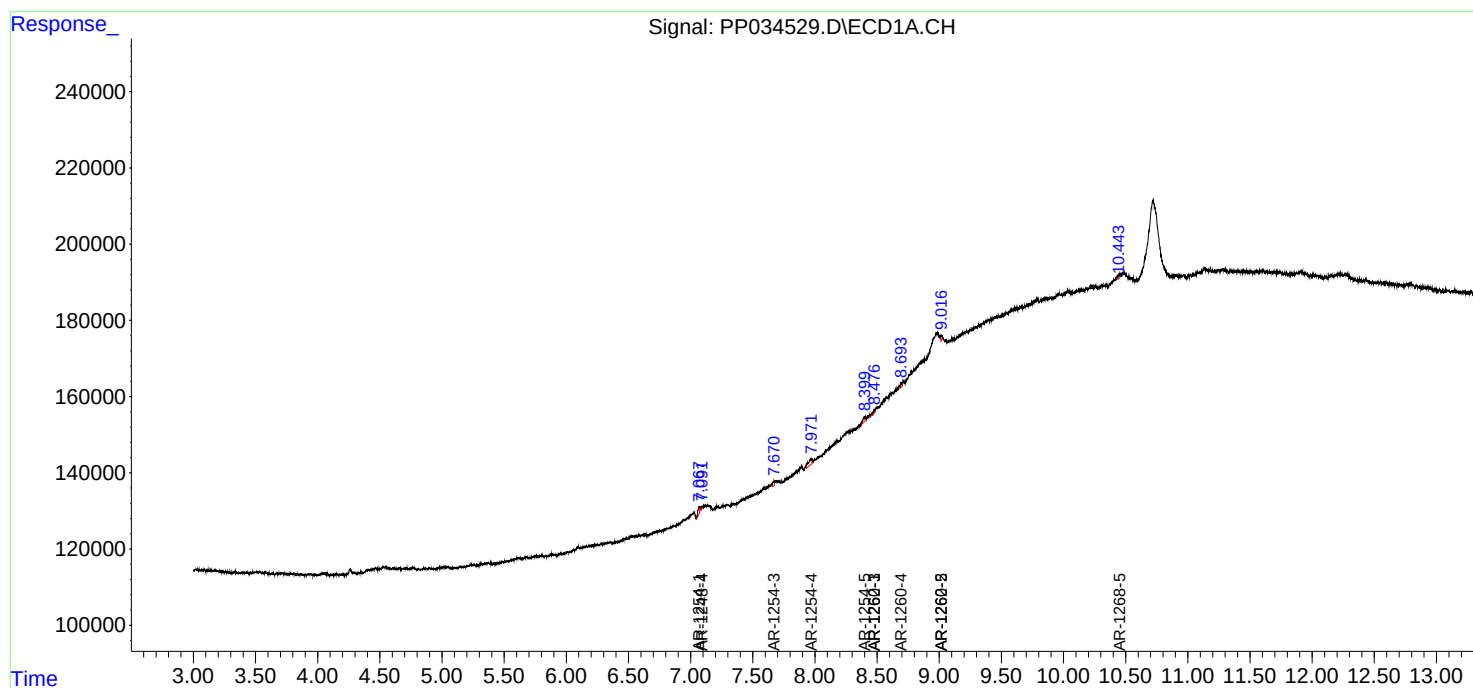


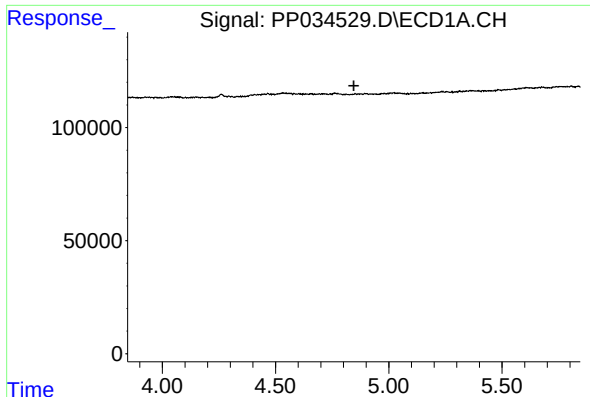

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

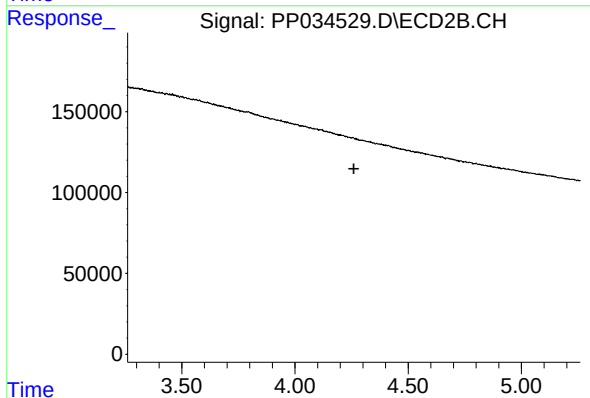


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.260 min
Response: 0
Conc: N.D.

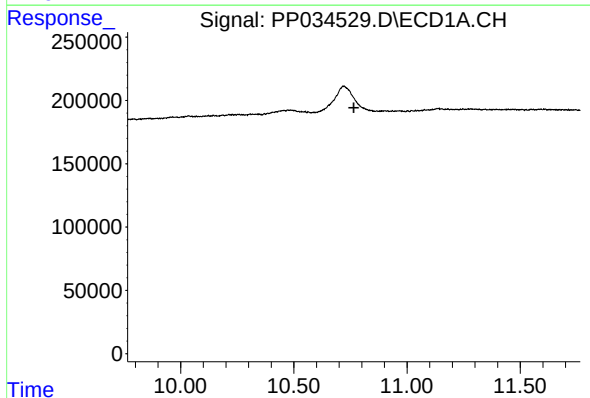


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.765 min
Response: 0
Conc: N.D.

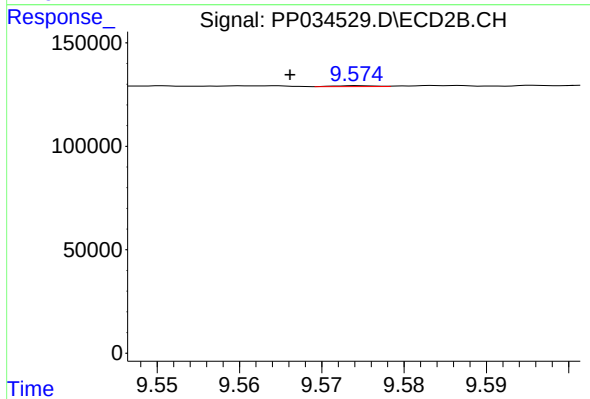

#2 Decachlorobiphenyl


R.T.: 9.575 min
Delta R.T.: 0.008 min
Response: 1331
Conc: 0.05 ng/ml

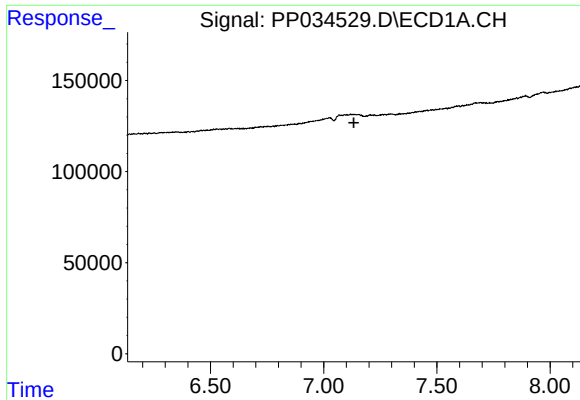

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

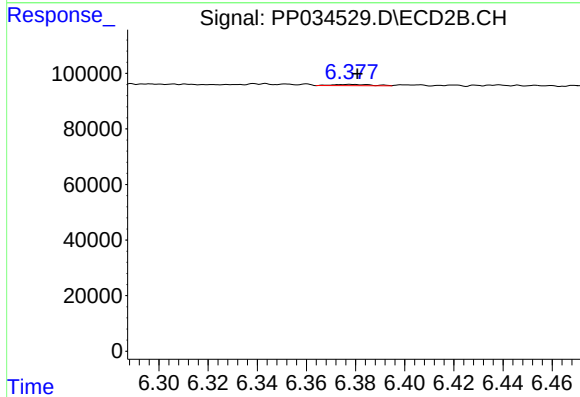


#20 AR-1242-5

R.T.: 6.378 min
Delta R.T.: -0.003 min
Response: 5177
Conc: 6.31 ng/ml

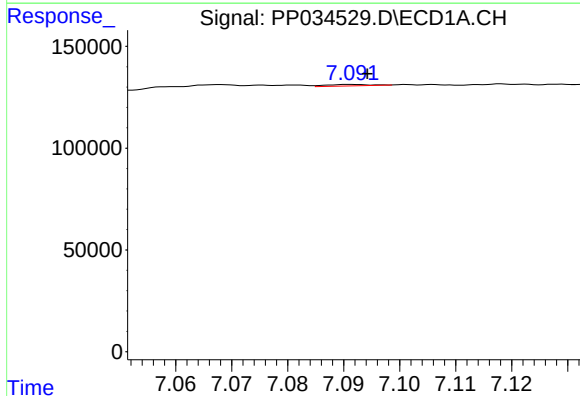


#24 AR-1248-4

R.T.: 7.091 min
Delta R.T.: -0.003 min
Response: 3883
Conc: 1.52 ng/ml

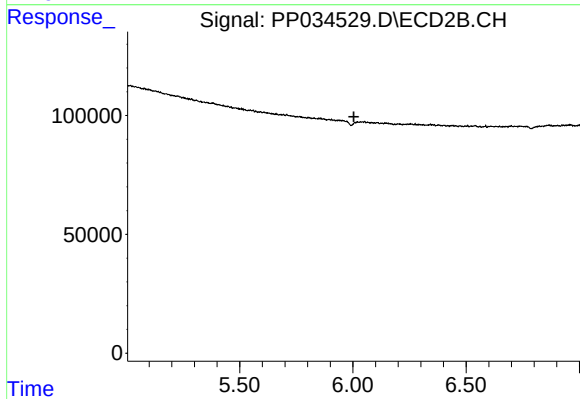

#24 AR-1248-4


R.T.: 6.021 min
Delta R.T.: 0.017 min
Response: -6278
Conc: N.D.

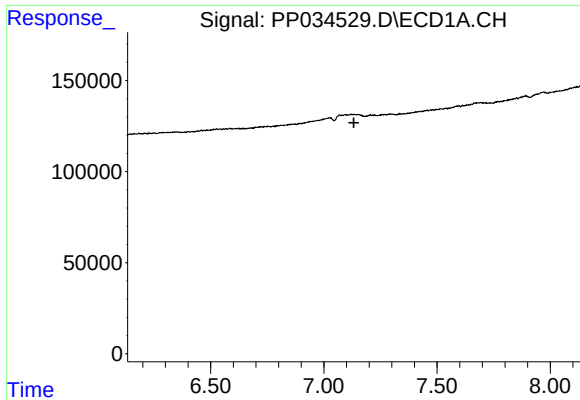

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

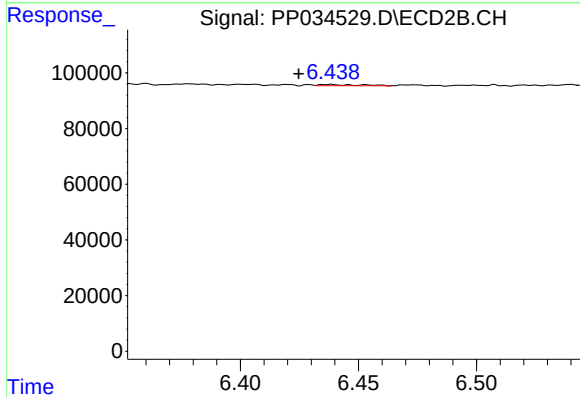


#25 AR-1248-5

R.T.: 6.438 min
Delta R.T.: 0.014 min
Response: 5445
Conc: 4.82 ng/ml

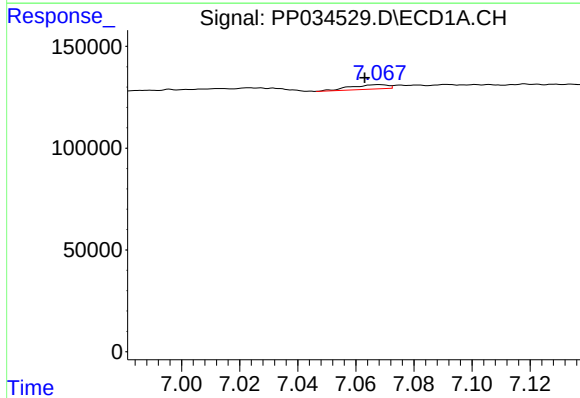


#26 AR-1254-1

R.T.: 7.068 min
Delta R.T.: 0.005 min
Response: 18940
Conc: 6.89 ng/ml

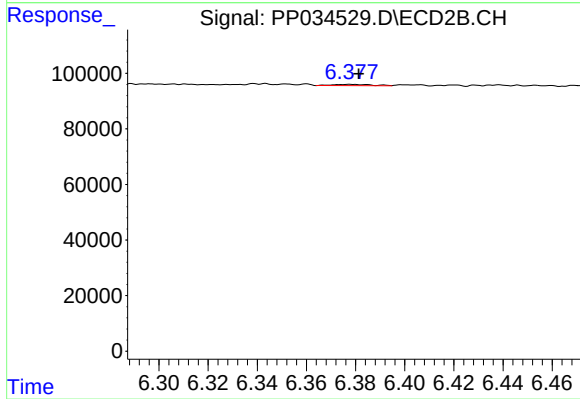

#26 AR-1254-1


R.T.: 6.378 min
Delta R.T.: -0.003 min
Response: 5177
Conc: 2.81 ng/ml

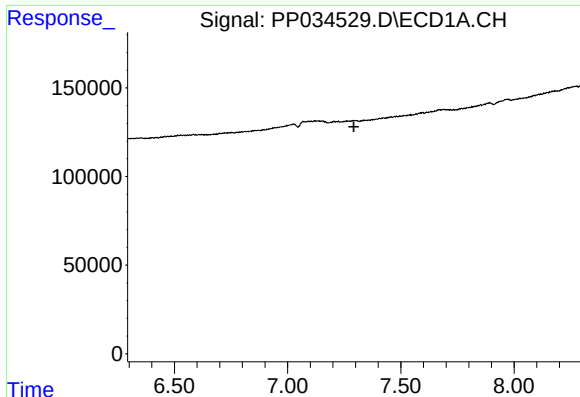

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 7.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

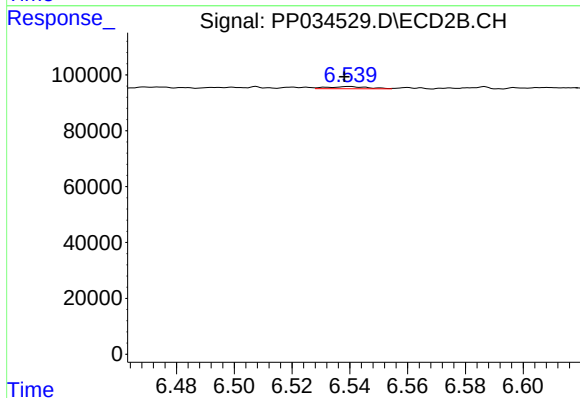


#27 AR-1254-2

R.T.: 6.540 min
Delta R.T.: 0.002 min
Response: 7320
Conc: 4.58 ng/ml

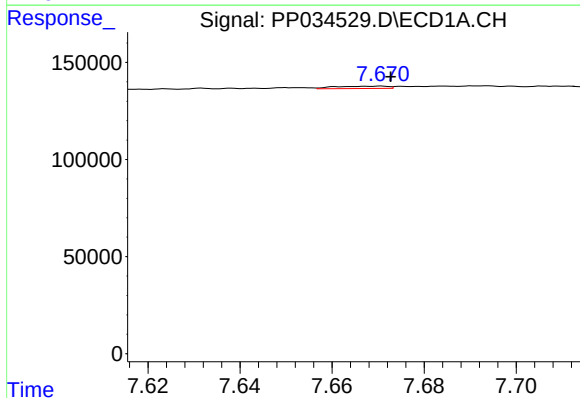


#28 AR-1254-3

R.T.: 7.671 min
Delta R.T.: -0.002 min
Response: 9565
Conc: 2.10 ng/ml

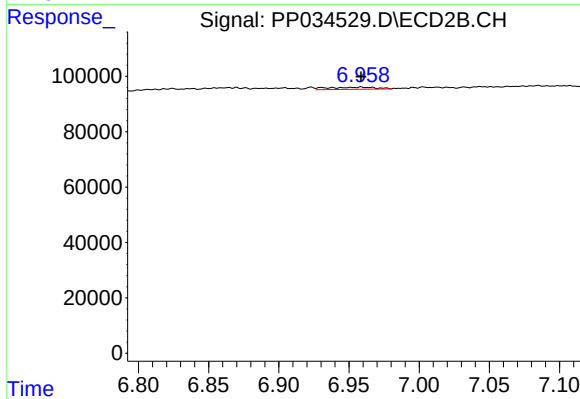

#28 AR-1254-3


R.T.: 6.959 min
Delta R.T.: 0.000 min
Response: 18904
Conc: 7.57 ng/ml

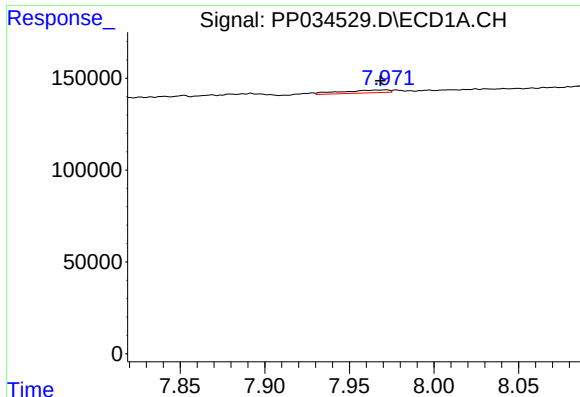

#29 AR-1254-4


R.T.: 7.972 min
Delta R.T.: 0.003 min
Response: 30693
Conc: 9.93 ng/ml

Instrument :
ECD_P
ClientSampleId :

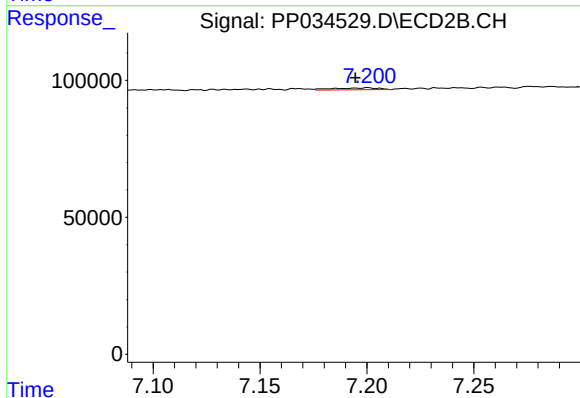


#29 AR-1254-4

R.T.: 7.200 min
Delta R.T.: 0.006 min
Response: 10172
Conc: 7.74 ng/ml

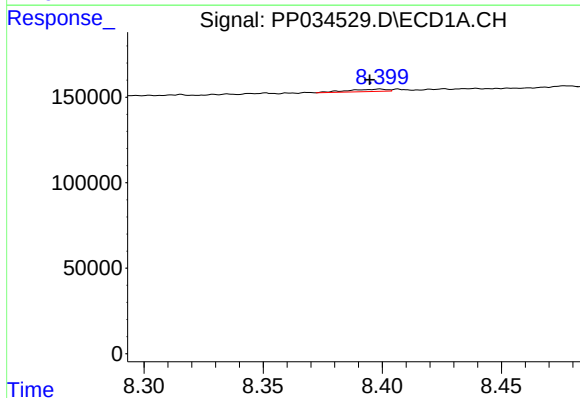


#30 AR-1254-5

R.T.: 8.399 min
Delta R.T.: 0.004 min
Response: 15408
Conc: 4.34 ng/ml

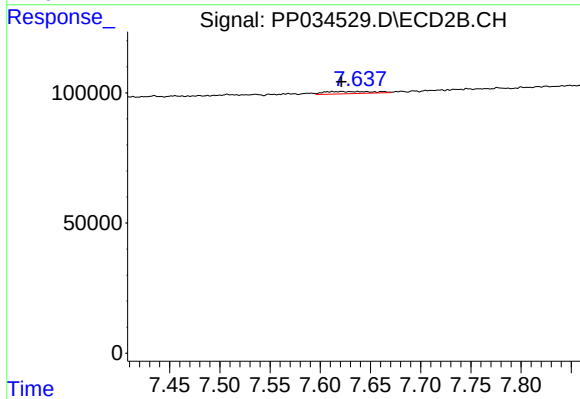

#30 AR-1254-5


R.T.: 7.621 min
Delta R.T.: 0.000 min
Response: 28780
Conc: 14.16 ng/ml

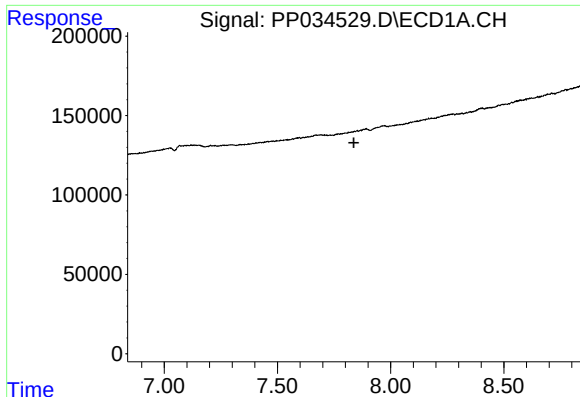

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

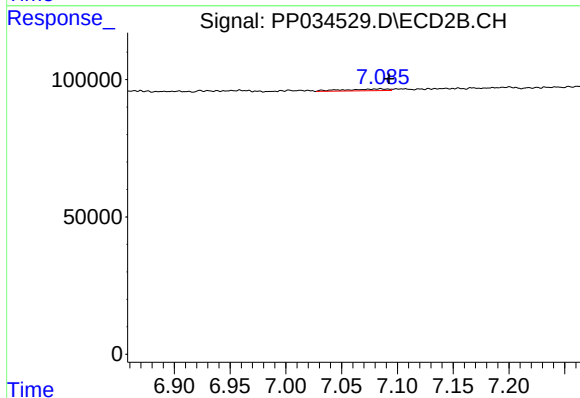


#31 AR-1260-1

R.T.: 7.085 min
Delta R.T.: -0.008 min
Response: 17843
Conc: 11.62 ng/ml

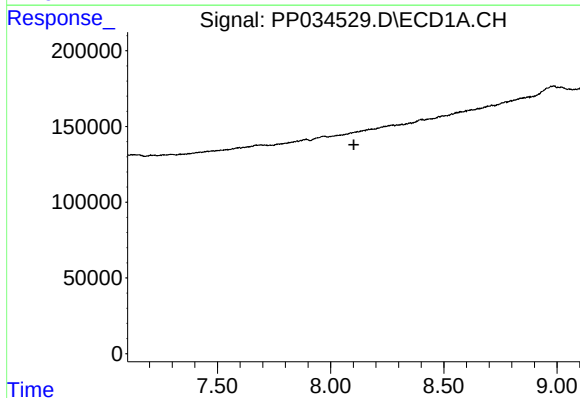


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 8.103 min
Response: 0
Conc: N.D.

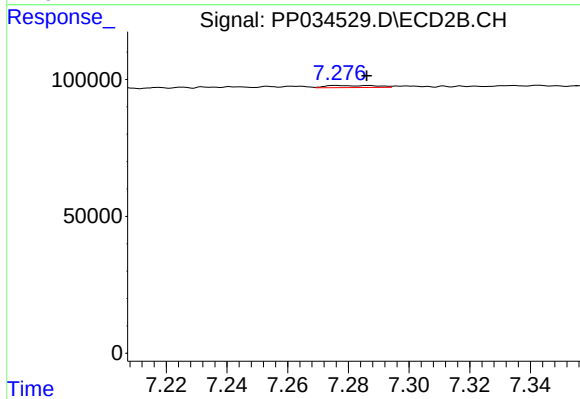

#32 AR-1260-2


R.T.: 7.276 min
Delta R.T.: -0.010 min
Response: 8620
Conc: 4.77 ng/ml

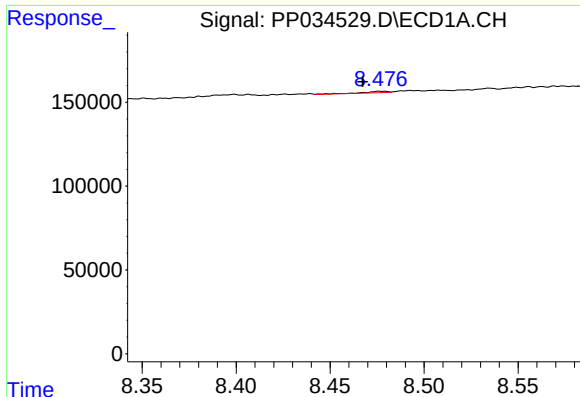

#33 AR-1260-3


R.T.: 8.476 min
Delta R.T.: 0.009 min
Response: 6993
Conc: 2.31 ng/ml

Instrument :
ECD_P
ClientSampleId :

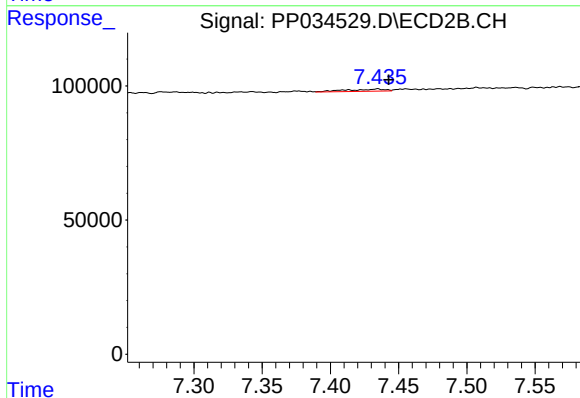


#33 AR-1260-3

R.T.: 7.434 min
Delta R.T.: -0.008 min
Response: 15619
Conc: 9.00 ng/ml

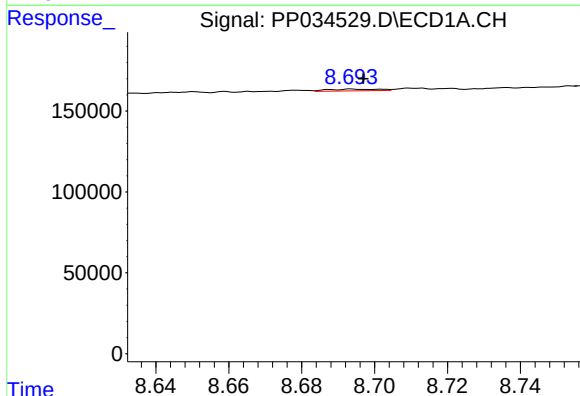


#34 AR-1260-4

R.T.: 8.693 min
Delta R.T.: -0.003 min
Response: 10686
Conc: 3.06 ng/ml

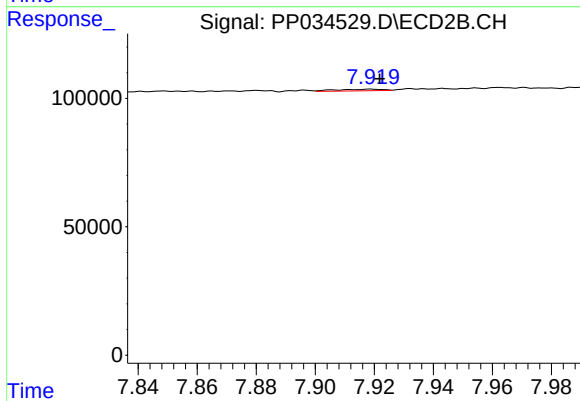

#34 AR-1260-4


R.T.: 7.919 min
Delta R.T.: -0.003 min
Response: 7017
Conc: 4.89 ng/ml

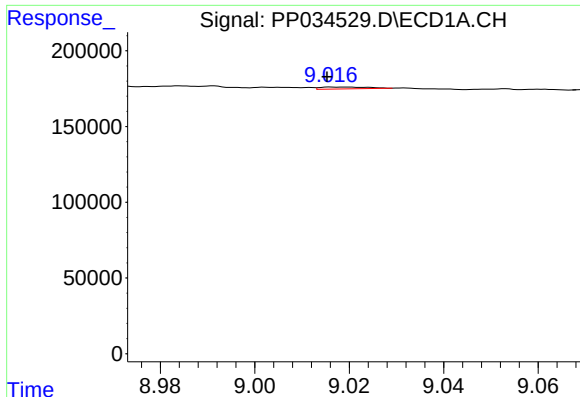

#35 AR-1260-5


R.T.: 9.016 min
Delta R.T.: 0.000 min
Response: 8718
Conc: 1.22 ng/ml

Instrument :
ECD_P
ClientSampleId :

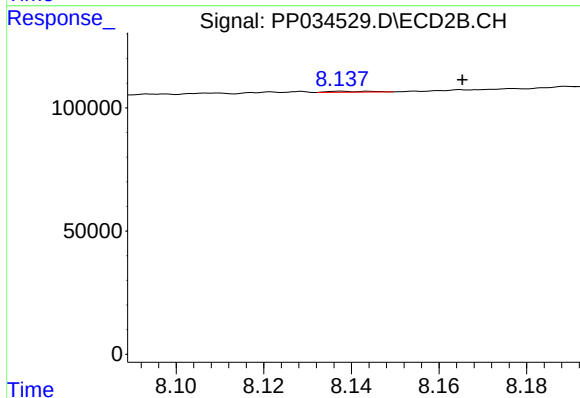


#35 AR-1260-5

R.T.: 8.138 min
Delta R.T.: -0.028 min
Response: 2554
Conc: 0.75 ng/ml

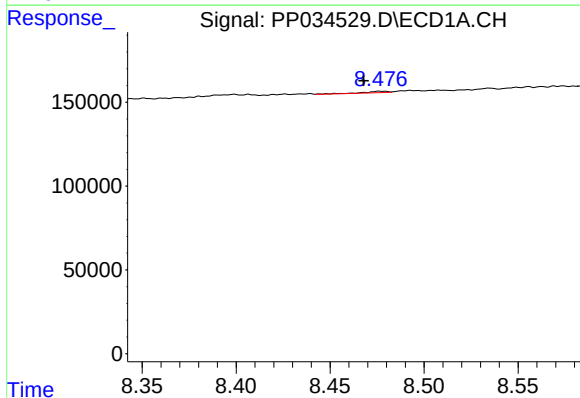


#36 AR-1262-1

R.T.: 8.476 min
Delta R.T.: 0.008 min
Response: 6993
Conc: 1.53 ng/ml

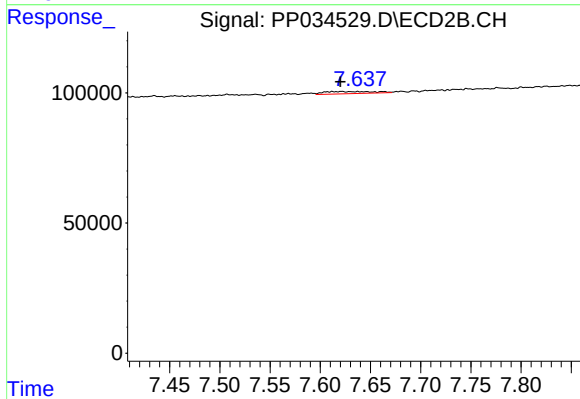

#36 AR-1262-1


R.T.: 7.621 min
Delta R.T.: 0.001 min
Response: 28780
Conc: 26.80 ng/ml

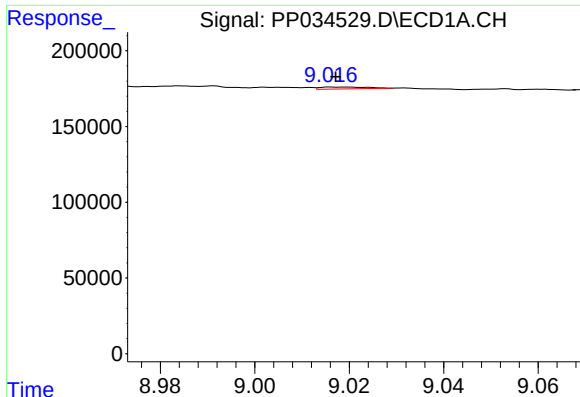

#37 AR-1262-2


R.T.: 9.016 min
Delta R.T.: 0.000 min
Response: 8718
Conc: 1.12 ng/ml

Instrument :
ECD_P
ClientSampleId :

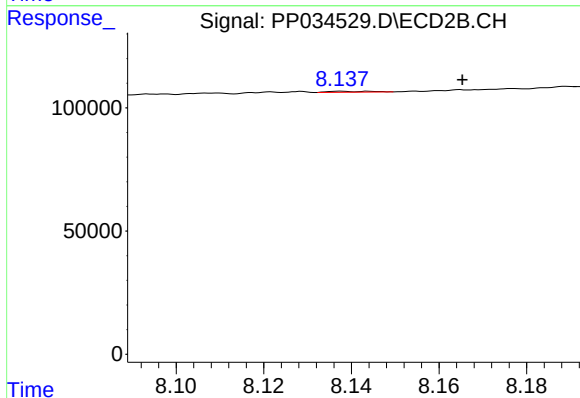


#37 AR-1262-2

R.T.: 8.138 min
Delta R.T.: -0.028 min
Response: 2554
Conc: 0.74 ng/ml

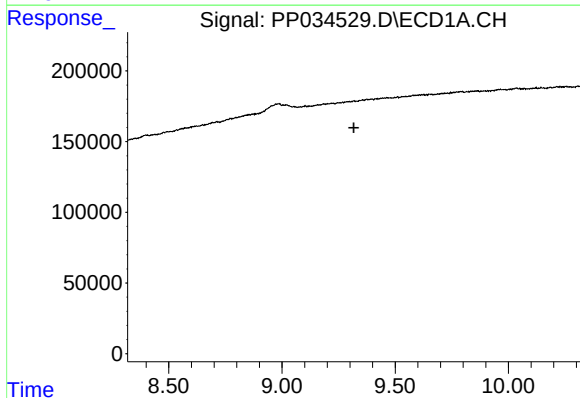


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.318 min
Response: 0
Conc: N.D.

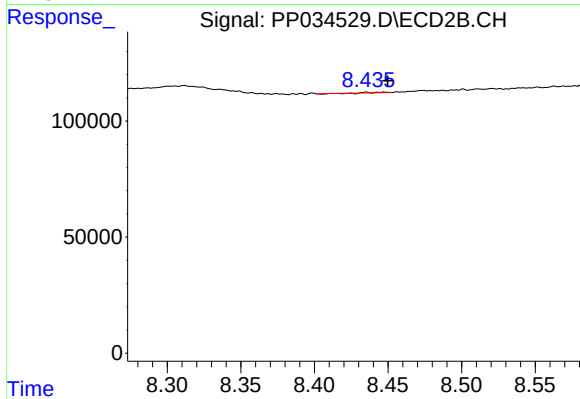

#38 AR-1262-3


R.T.: 8.435 min
Delta R.T.: -0.015 min
Response: 80
Conc: 0.05 ng/ml

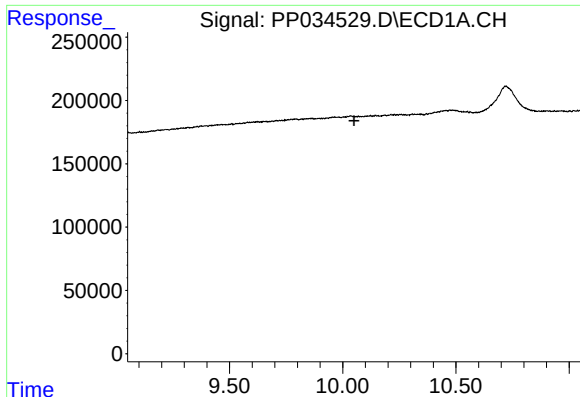

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

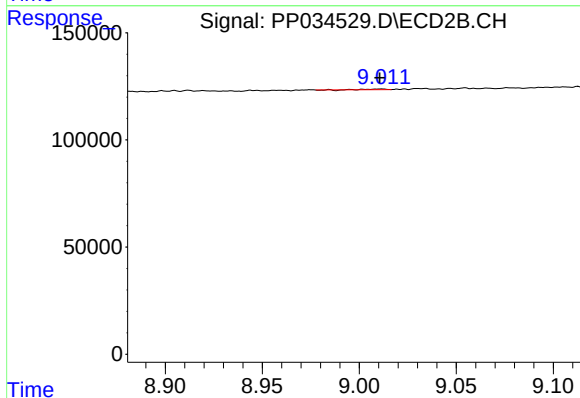


#40 AR-1262-5

R.T.: 9.011 min
Delta R.T.: 0.000 min
Response: 1494
Conc: 1.32 ng/ml

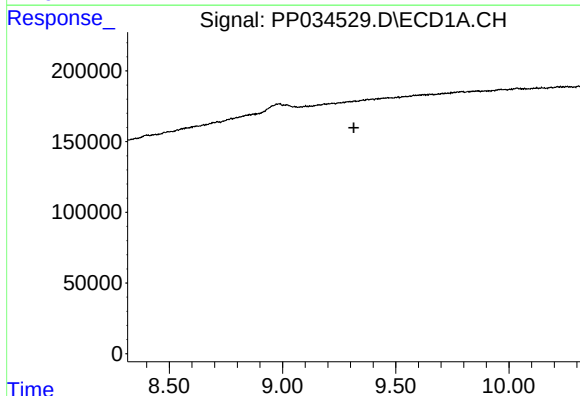


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.315 min
Response: 0
Conc: N.D.

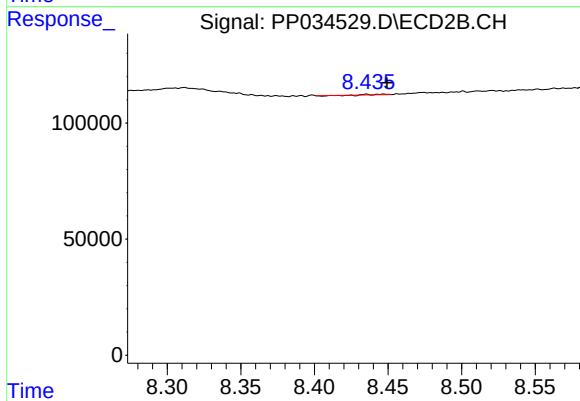

#41 AR-1268-1


R.T.: 8.435 min
Delta R.T.: -0.014 min
Response: 80
Conc: 0.02 ng/ml

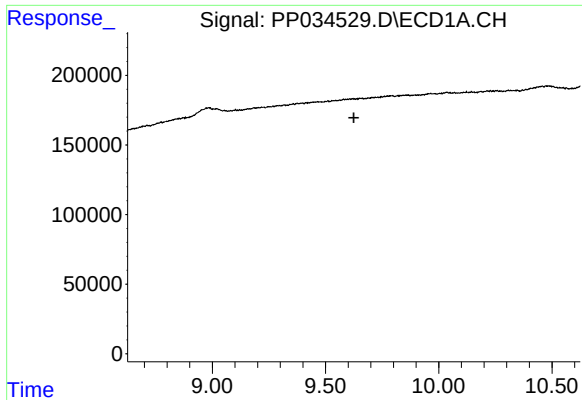

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

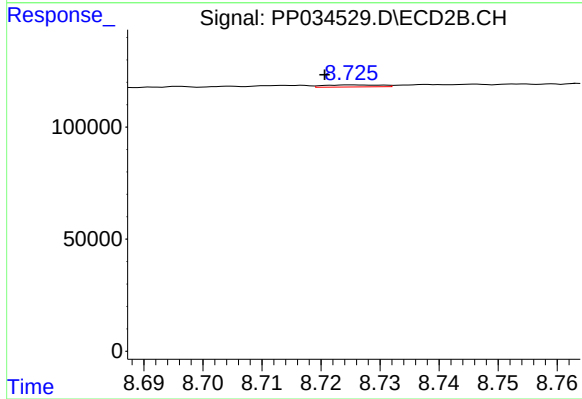


#43 AR-1268-3

R.T.: 8.726 min
Delta R.T.: 0.005 min
Response: 6157
Conc: 1.69 ng/ml

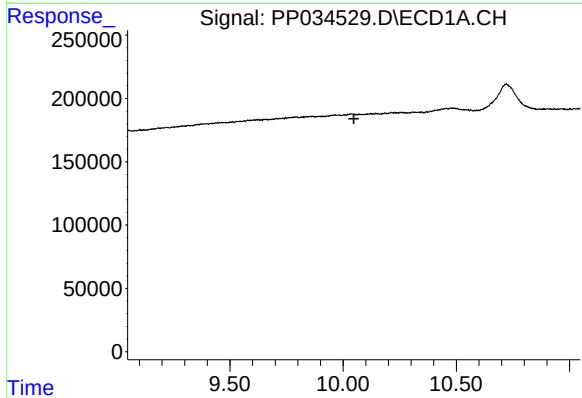


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 10.048 min
Response: 0
Conc: N.D.

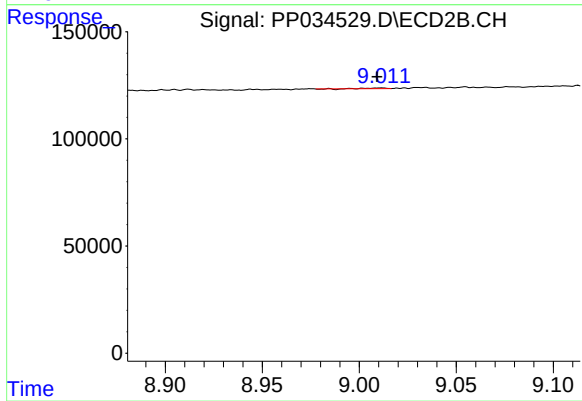

#44 AR-1268-4


R.T.: 9.011 min
Delta R.T.: 0.002 min
Response: 1494
Conc: 1.16 ng/ml

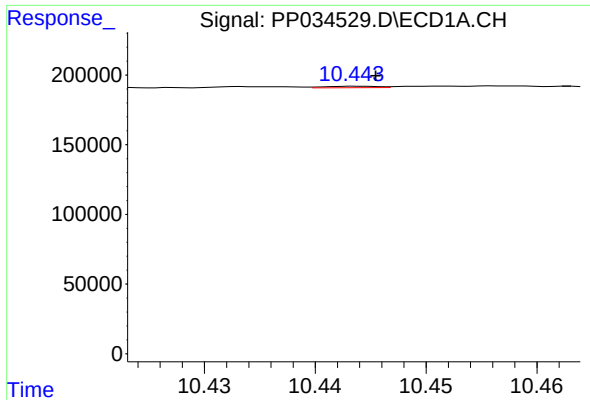

#45 AR-1268-5

R.T.: 10.444 min
Delta R.T.: -0.002 min
Response: 3433
Conc: 0.12 ng/ml

Instrument :
ECD_P
ClientSampleId :

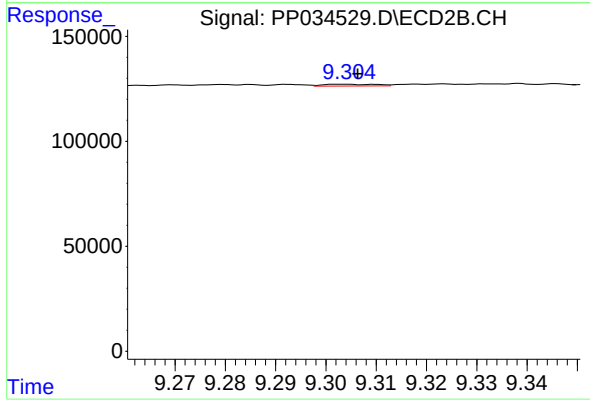

#45 AR-1268-5

R.T.: 9.303 min
Delta R.T.: -0.003 min
Response: 5963
Conc: 0.57 ng/ml