

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
 Data File : PP034536.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2021 13:47
 Operator : DD\AJ
 Sample : M1865-06DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-030321-SR-06DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 14:59:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.845	4.256	337251	196968	4.421	4.385
2)	SA Decachlor...	10.768	9.563	303566	137307	3.943	4.863
Target Compounds							
3)	L1 AR-1016-1	6.168	5.507	1693030	90393	719.587	76.196 #
4)	L1 AR-1016-2	6.168	5.556f	1693030	324043	476.680	182.494 #
5)	L1 AR-1016-3	6.253	5.722	1967468	-374	921.403	N.D. #
6)	L1 AR-1016-4	0.000	5.771	0	786618	N.D.	1083.063 #
7)	L1 AR-1016-5	6.667	6.002	844874	333638	489.687	364.769 #
8)	L2 AR-1221-1	5.093	4.534f	11659	32168	15.949	70.881 #
9)	L2 AR-1221-2	5.215f	4.616	36000	24554	63.198	70.380
10)	L2 AR-1221-3	0.000	4.699	0	70521	N.D.	67.225 #
11)	L3 AR-1232-1	0.000	4.699	0	70521	N.D.	83.483 #
12)	L3 AR-1232-2	5.848f	5.556f	149048	324043	196.412	430.588 #
13)	L3 AR-1232-3	6.168	5.722	1693030	-374	1154.736	N.D. #
14)	L3 AR-1232-4	0.000	5.815	0	208890	N.D.	607.307 #
15)	L3 AR-1232-5	6.450	6.002	2297692	333638	4883.036	938.610 #
16)	L4 AR-1242-1	6.168	5.507	1693030	90393	904.536	96.478 #
17)	L4 AR-1242-2	6.168	5.556f	1693030	324043	600.024	227.940 #
18)	L4 AR-1242-3	6.253	5.722	1967468	-374	1155.183	N.D. #
19)	L4 AR-1242-4	0.000	5.815	0	208890	N.D.	283.902 #
20)	L4 AR-1242-5	7.135	6.378	782928	1430996	531.688	1745.202 #
21)	L5 AR-1248-1	6.168	5.507	1693030	90393	1190.236	123.907 #
22)	L5 AR-1248-2	6.450	5.771	2297692	786618	1161.096	766.308 #
23)	L5 AR-1248-3	6.667	5.815	844874	208890	355.423	190.595 #
24)	L5 AR-1248-4	7.093	6.002	1145940	333638	449.055	264.346 #
25)	L5 AR-1248-5	7.135	6.421	782928	141129	307.248	124.877 #
26)	L6 AR-1254-1	7.063	6.378	2391635	1430996	869.834	775.647
27)	L6 AR-1254-2	7.292	6.536	3359739	1070847	790.130	669.326
28)	L6 AR-1254-3	7.673	6.956	3036249	1421760	665.234	569.670
29)	L6 AR-1254-4	7.968	7.192	1487680	568897	481.160	432.772
30)	L6 AR-1254-5	8.396	7.618	1404115	811500	395.099	399.276
31)	L7 AR-1260-1	7.839	7.090	1069574	635594	344.548	413.889
32)	L7 AR-1260-2	8.104	7.284	977894	417917	260.396	231.354
33)	L7 AR-1260-3	8.458	7.439	190595	434382	63.054	250.381 #
34)	L7 AR-1260-4	8.691	7.919	489792	66065	140.292	46.078 #
35)	L7 AR-1260-5	9.018	8.162	343492	102587	47.963	30.032 #
36)	L8 AR-1262-1	8.458	7.618	190595	811500	41.653	755.587 #
37)	L8 AR-1262-2	9.018	8.162	343492	102587	44.024	29.900 #
38)	L8 AR-1262-3	9.340f	8.450	109738	472	20.392	0.315 #
39)	L8 AR-1262-4	9.394	8.510	57595	42792	12.969	15.538
40)	L8 AR-1262-5	10.055	9.002	69395	47251	24.099	41.638 #
41)	L9 AR-1268-1	9.340f	8.450	109738	472	10.961	0.109 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
 Data File : PP034536.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2021 13:47
 Operator : DD\AJ
 Sample : M1865-06DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-030321-SR-06DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 14:59:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.394	8.510	57595	42792	6.021	10.339 #
43) L9	AR-1268-3	0.000	8.732	0	22072	N.D.	6.067 #
44) L9	AR-1268-4	10.055	9.002	69395	47251	21.724	36.678 #
45) L9	AR-1268-5	10.444	9.285f	279231	41659	9.779	4.011 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
Data File : PP034536.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2021 13:47
Operator : DD\AJ
Sample : M1865-06DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 14:59:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

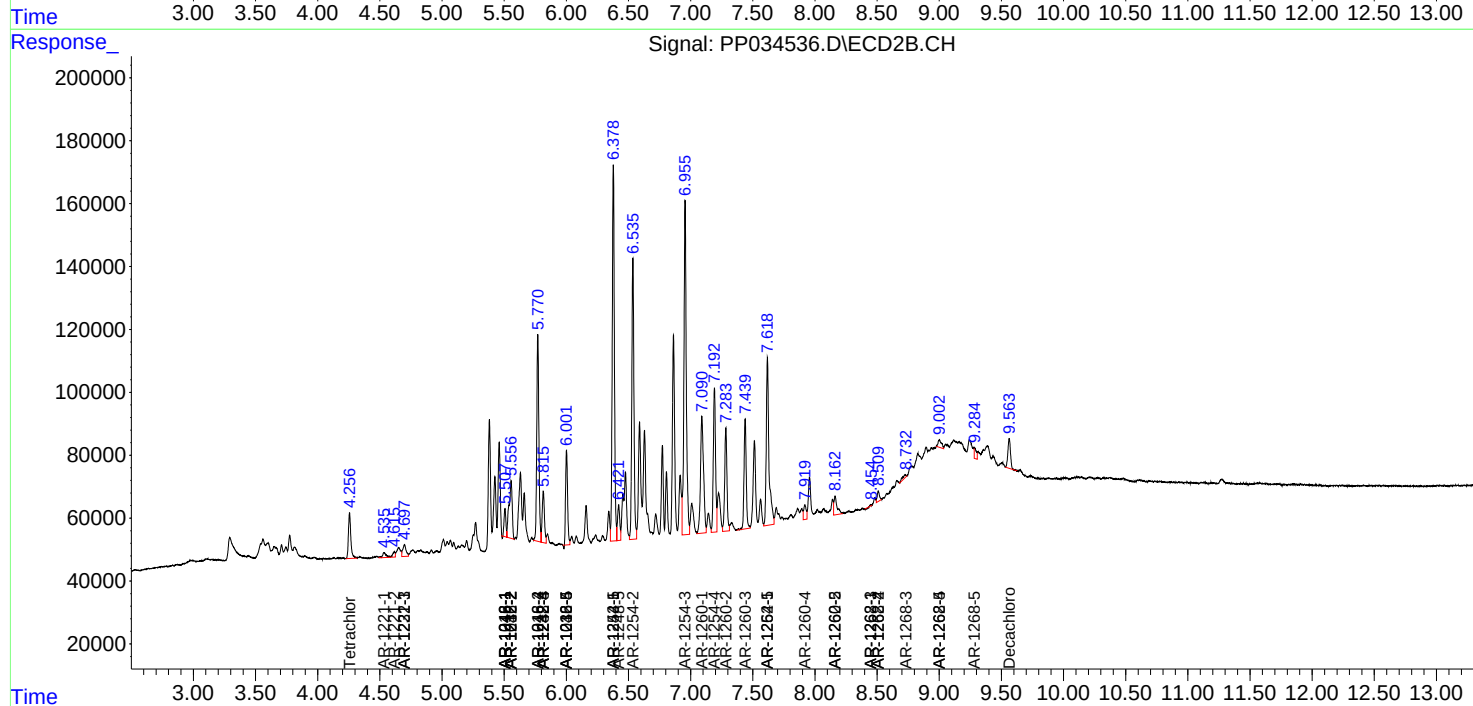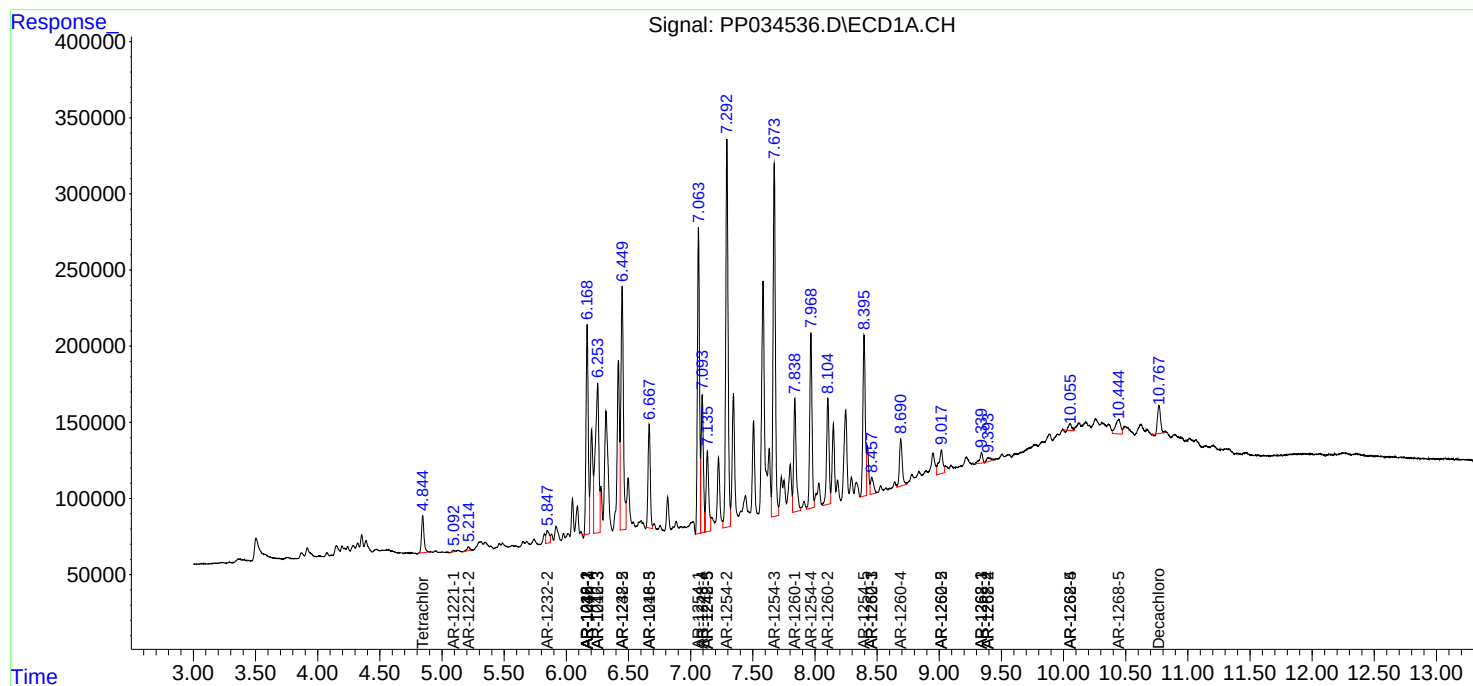


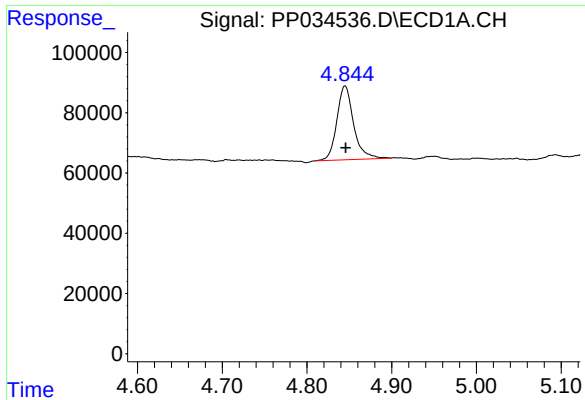

#1 Tetrachloro-m-xylene


R.T.: 4.845 min
Delta R.T.: -0.001 min
Response: 337251
Conc: 4.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

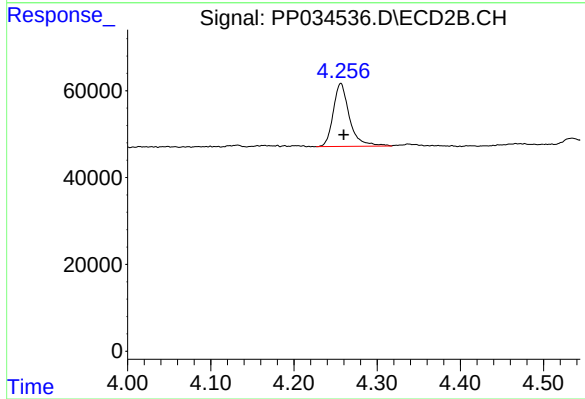


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: -0.003 min
Response: 196968
Conc: 4.38 ng/ml

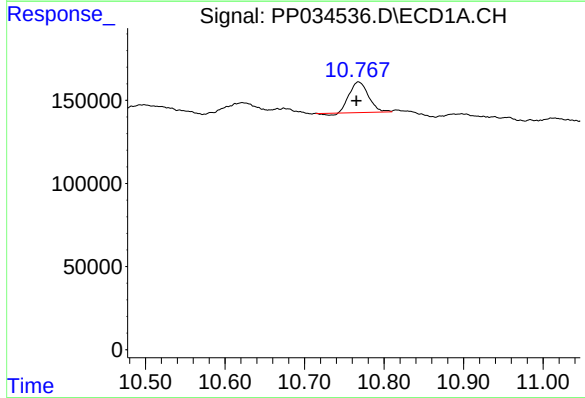


#2 Decachlorobiphenyl

R.T.: 10.768 min
Delta R.T.: 0.003 min
Response: 303566
Conc: 3.94 ng/ml

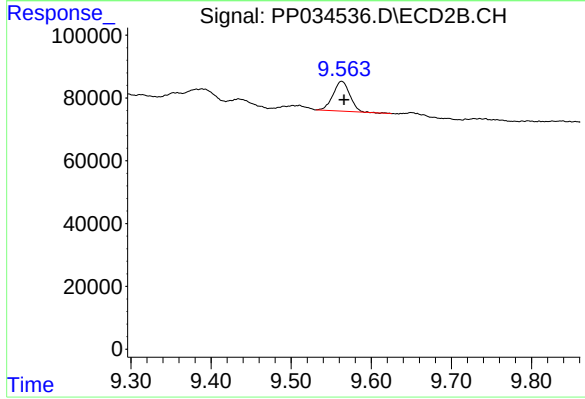

#2 Decachlorobiphenyl


R.T.: 9.563 min
Delta R.T.: -0.003 min
Response: 137307
Conc: 4.86 ng/ml

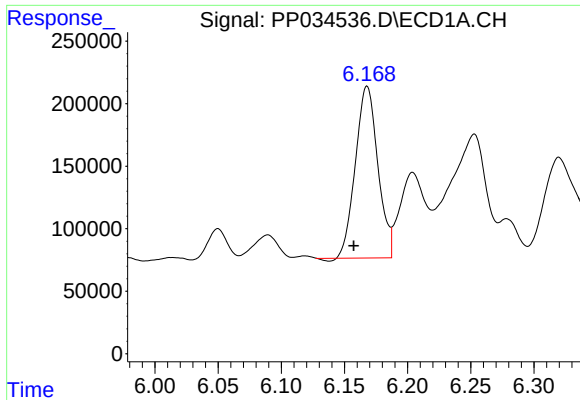

#3 AR-1016-1


R.T.: 6.168 min
Delta R.T.: 0.010 min
Response: 1693030
Conc: 719.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

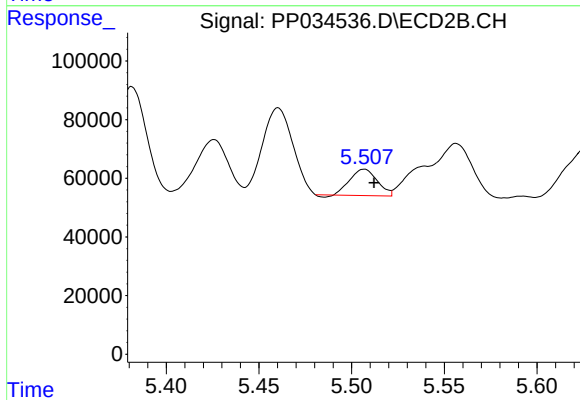


#3 AR-1016-1

R.T.: 5.507 min
Delta R.T.: -0.005 min
Response: 90393
Conc: 76.20 ng/ml

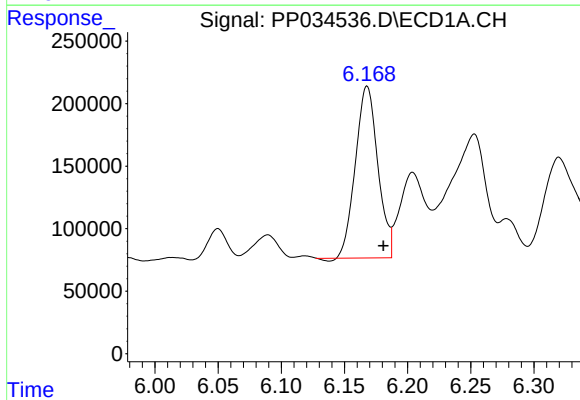


#4 AR-1016-2

R.T.: 6.168 min
Delta R.T.: -0.013 min
Response: 1693030
Conc: 476.68 ng/ml

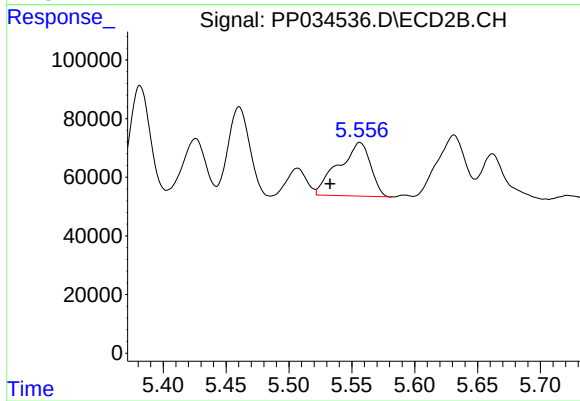

#4 AR-1016-2


R.T.: 5.556 min
Delta R.T.: 0.024 min
Response: 324043
Conc: 182.49 ng/ml

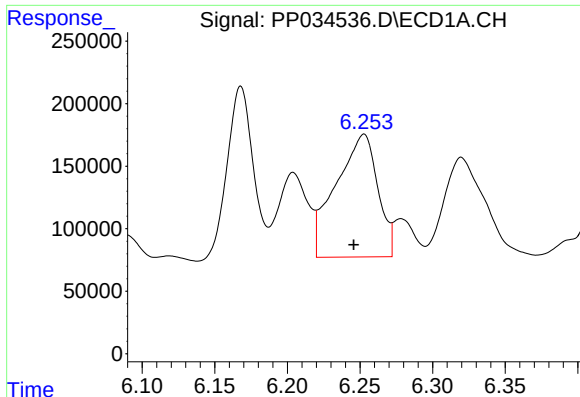

#5 AR-1016-3


R.T.: 6.253 min
Delta R.T.: 0.007 min
Response: 1967468
Conc: 921.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

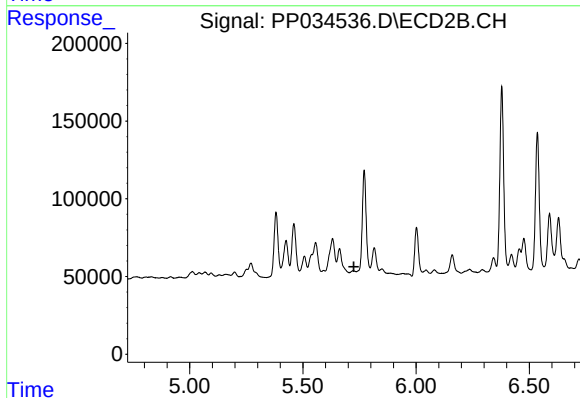


#5 AR-1016-3

R.T.: 5.722 min
Delta R.T.: -0.004 min
Response: -374
Conc: N.D.

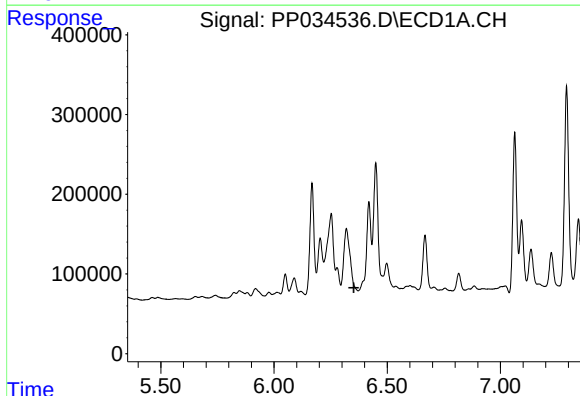


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

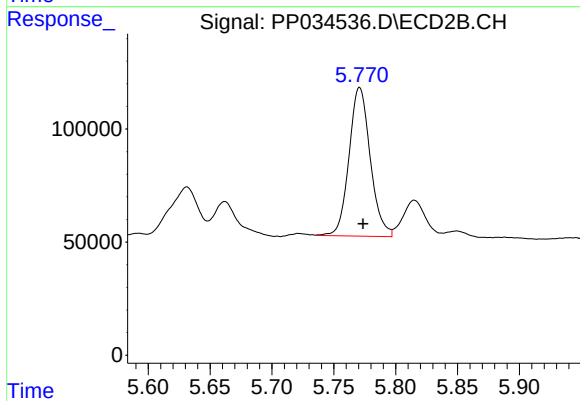

#6 AR-1016-4


R.T.: 5.771 min
Delta R.T.: -0.003 min
Response: 786618
Conc: 1083.06 ng/ml

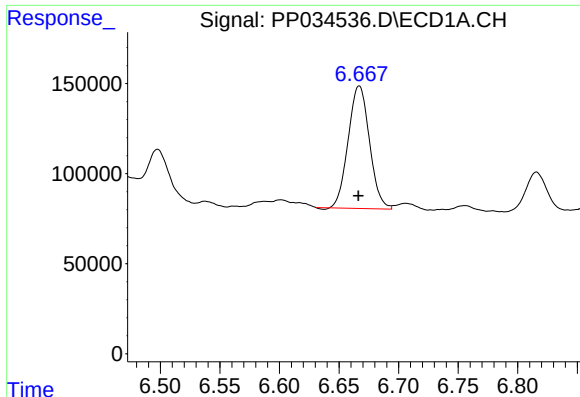

#7 AR-1016-5


R.T.: 6.667 min
Delta R.T.: 0.000 min
Response: 844874
Conc: 489.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

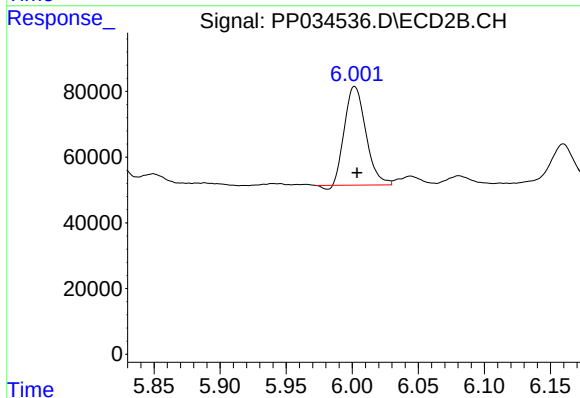


#7 AR-1016-5

R.T.: 6.002 min
Delta R.T.: -0.002 min
Response: 333638
Conc: 364.77 ng/ml

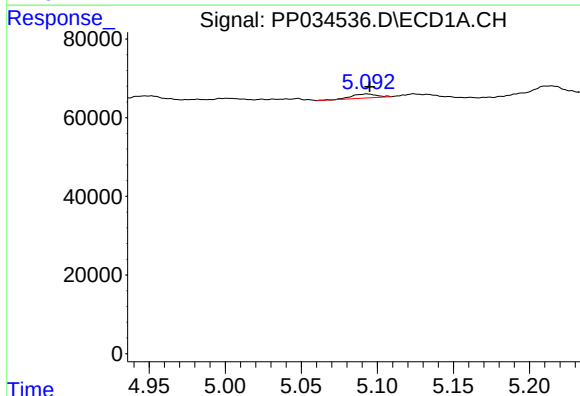


#8 AR-1221-1

R.T.: 5.093 min
Delta R.T.: -0.002 min
Response: 11659
Conc: 15.95 ng/ml

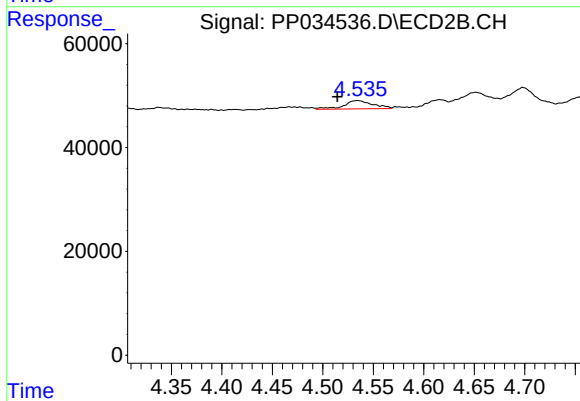

#8 AR-1221-1


R.T.: 4.534 min
Delta R.T.: 0.020 min
Response: 32168
Conc: 70.88 ng/ml

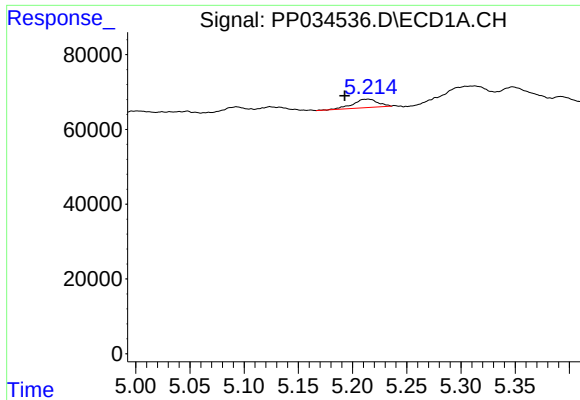

#9 AR-1221-2


R.T.: 5.215 min
Delta R.T.: 0.022 min
Response: 36000
Conc: 63.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

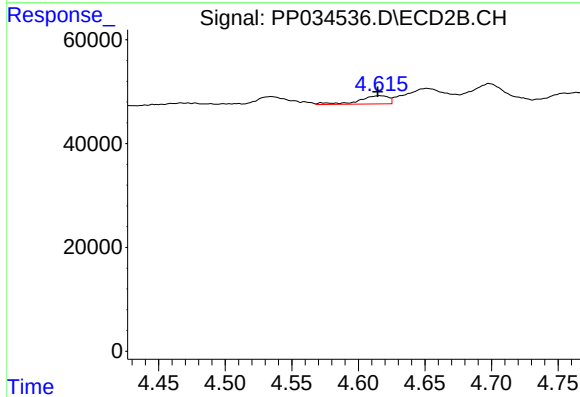


#9 AR-1221-2

R.T.: 4.616 min
Delta R.T.: 0.001 min
Response: 24554
Conc: 70.38 ng/ml

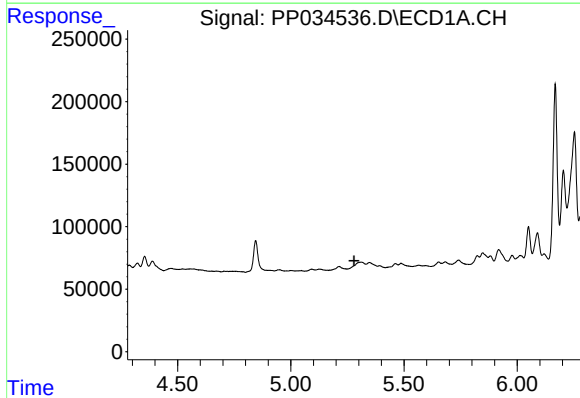


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 5.279 min
Response: 0
Conc: N.D.

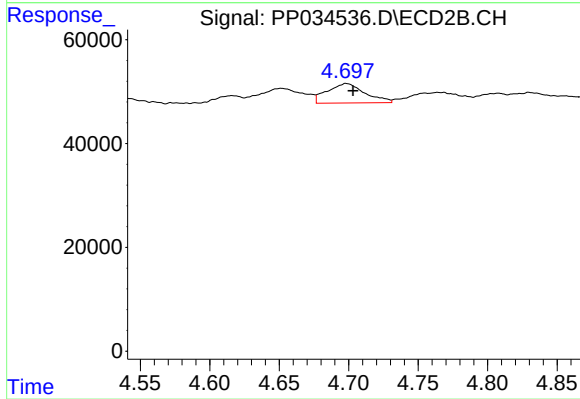

#10 AR-1221-3


R.T.: 4.699 min
Delta R.T.: -0.005 min
Response: 70521
Conc: 67.23 ng/ml

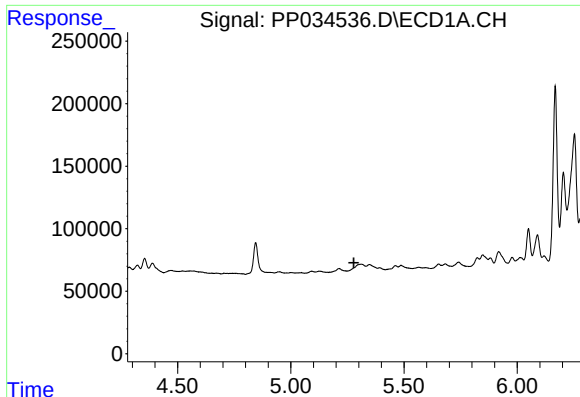

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 5.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

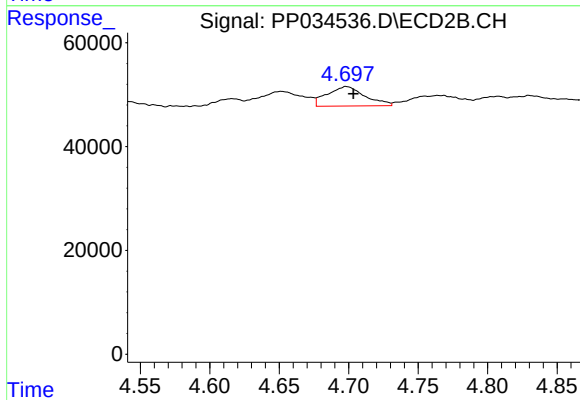


#11 AR-1232-1

R.T.: 4.699 min
Delta R.T.: -0.005 min
Response: 70521
Conc: 83.48 ng/ml

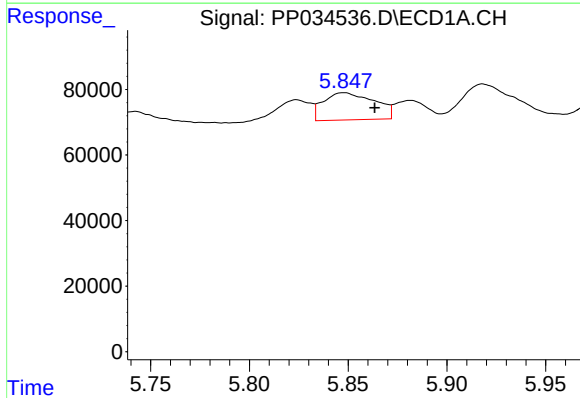


#12 AR-1232-2

R.T.: 5.848 min
Delta R.T.: -0.015 min
Response: 149048
Conc: 196.41 ng/ml

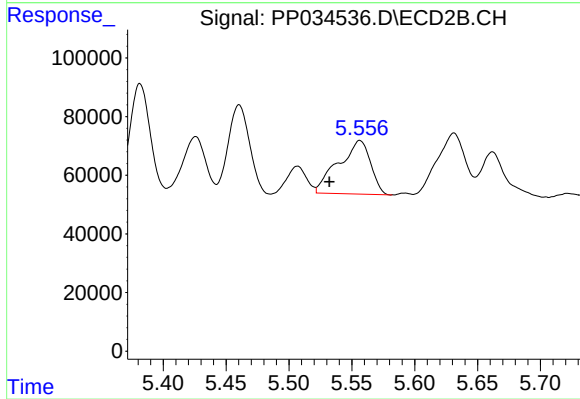

#12 AR-1232-2


R.T.: 5.556 min
Delta R.T.: 0.024 min
Response: 324043
Conc: 430.59 ng/ml

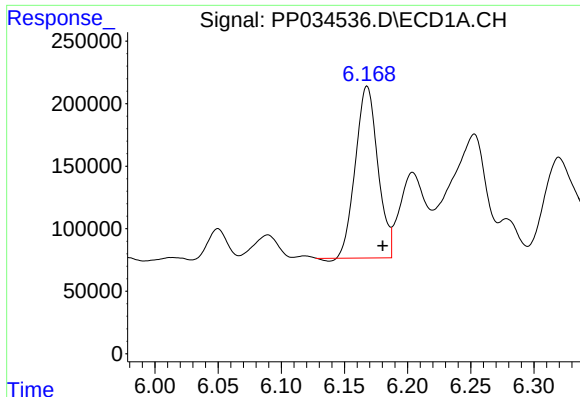

#13 AR-1232-3


R.T.: 6.168 min
Delta R.T.: -0.013 min
Response: 1693030
Conc: 1154.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

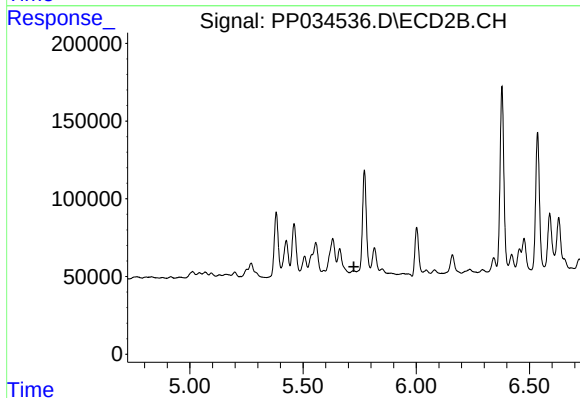


#13 AR-1232-3

R.T.: 5.722 min
Delta R.T.: -0.003 min
Response: -374
Conc: N.D.

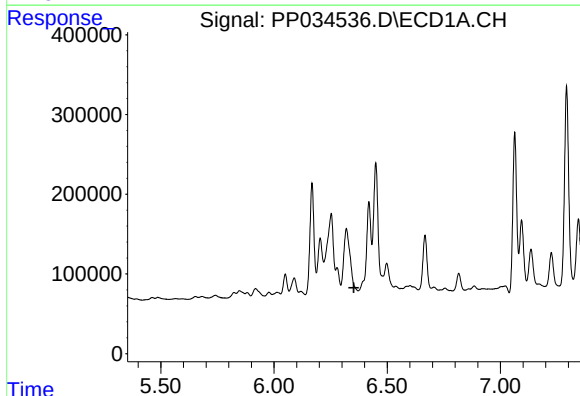


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

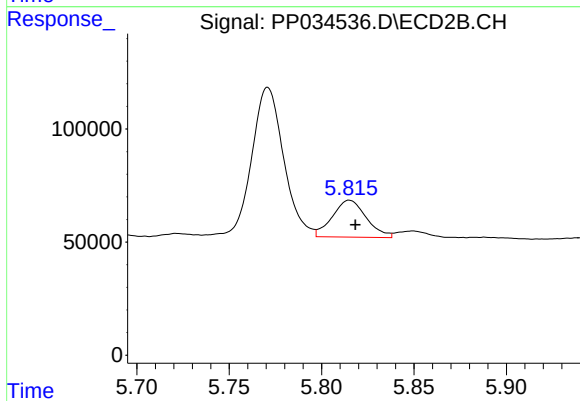

#14 AR-1232-4


R.T.: 5.815 min
Delta R.T.: -0.003 min
Response: 208890
Conc: 607.31 ng/ml

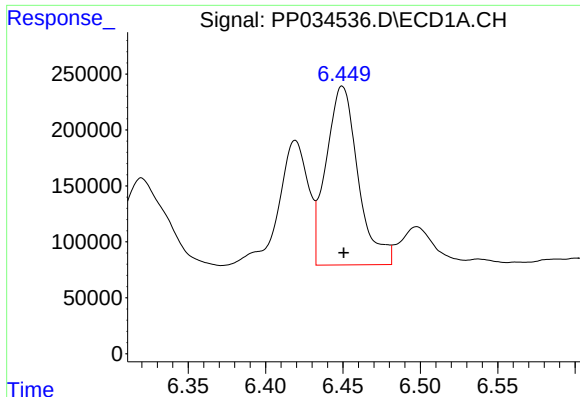

#15 AR-1232-5


R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 2297692
Conc: 4883.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

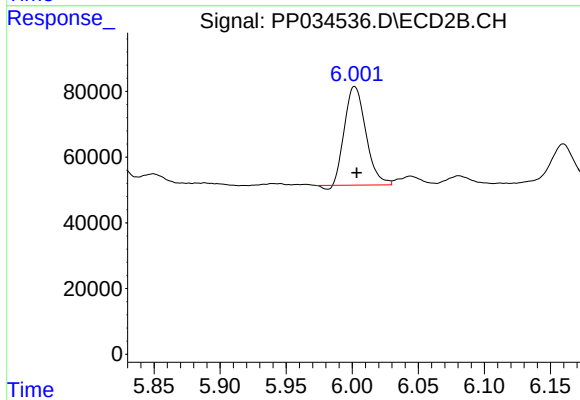


#15 AR-1232-5

R.T.: 6.002 min
Delta R.T.: -0.001 min
Response: 333638
Conc: 938.61 ng/ml

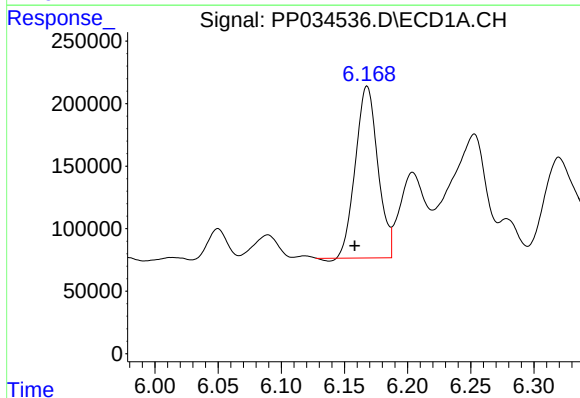


#16 AR-1242-1

R.T.: 6.168 min
Delta R.T.: 0.010 min
Response: 1693030
Conc: 904.54 ng/ml

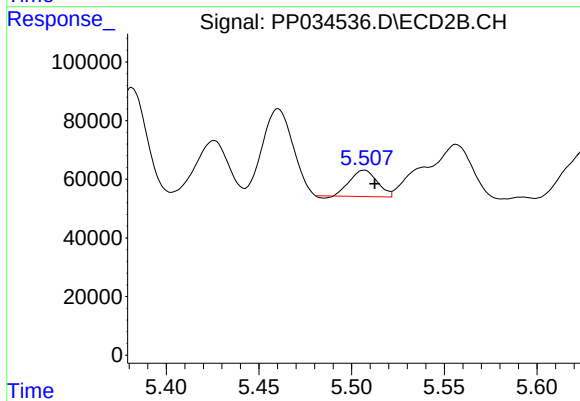

#16 AR-1242-1


R.T.: 5.507 min
Delta R.T.: -0.006 min
Response: 90393
Conc: 96.48 ng/ml

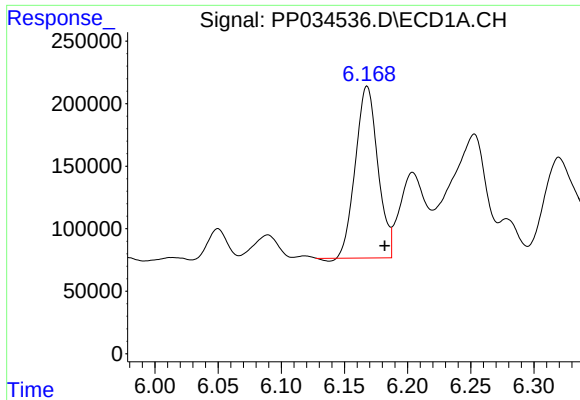

#17 AR-1242-2


R.T.: 6.168 min
Delta R.T.: -0.014 min
Response: 1693030
Conc: 600.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

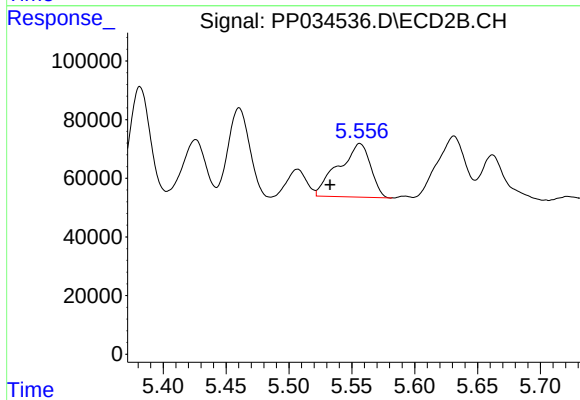


#17 AR-1242-2

R.T.: 5.556 min
Delta R.T.: 0.024 min
Response: 324043
Conc: 227.94 ng/ml

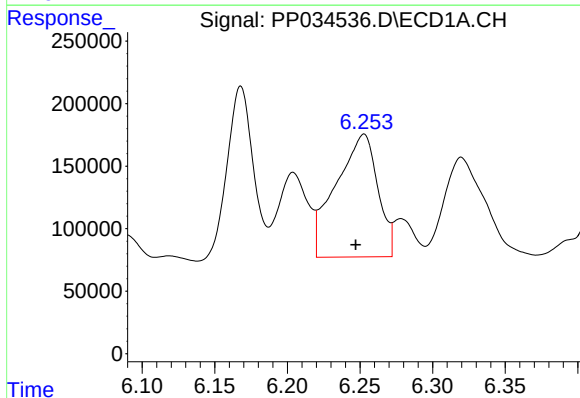


#18 AR-1242-3

R.T.: 6.253 min
Delta R.T.: 0.006 min
Response: 1967468
Conc: 1155.18 ng/ml

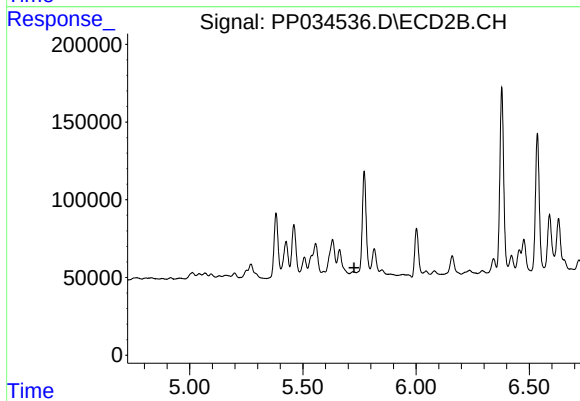

#18 AR-1242-3


R.T.: 5.722 min
Delta R.T.: -0.004 min
Response: -374
Conc: N.D.

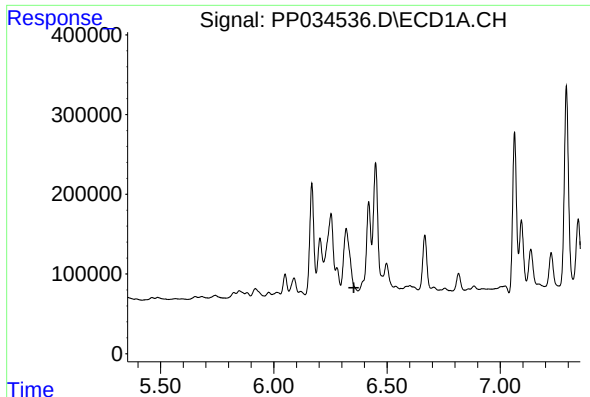

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 6.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

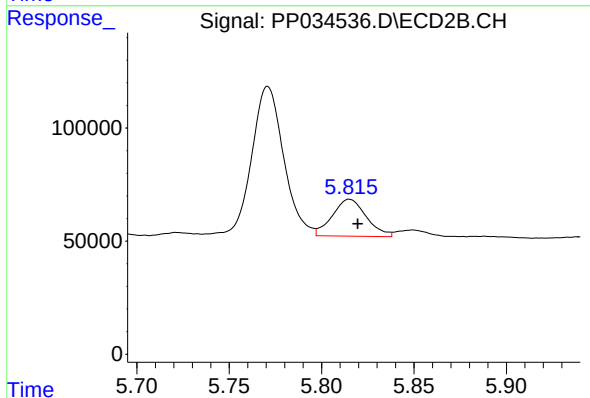


#19 AR-1242-4

R.T.: 5.815 min
Delta R.T.: -0.004 min
Response: 208890
Conc: 283.90 ng/ml

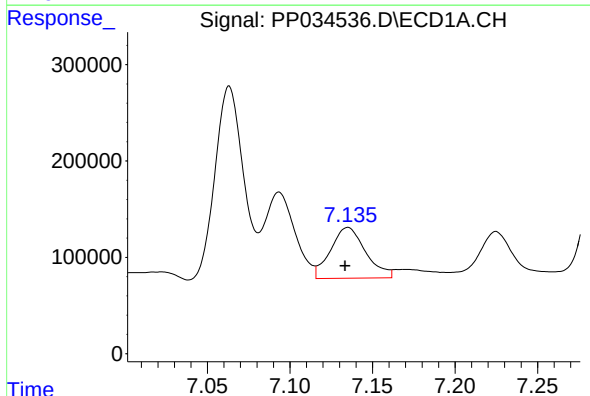


#20 AR-1242-5

R.T.: 7.135 min
Delta R.T.: 0.002 min
Response: 782928
Conc: 531.69 ng/ml

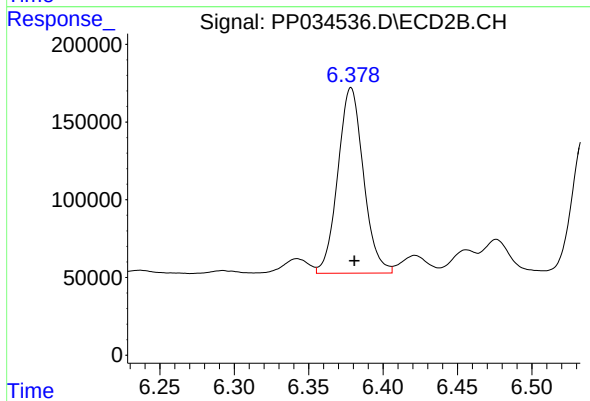

#20 AR-1242-5


R.T.: 6.378 min
Delta R.T.: -0.002 min
Response: 1430996
Conc: 1745.20 ng/ml

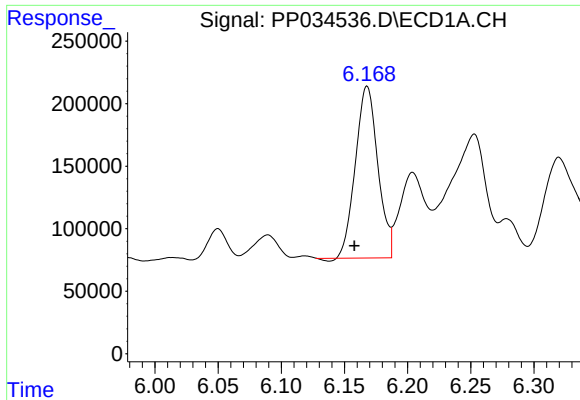

#21 AR-1248-1


R.T.: 6.168 min
Delta R.T.: 0.010 min
Response: 1693030
Conc: 1190.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

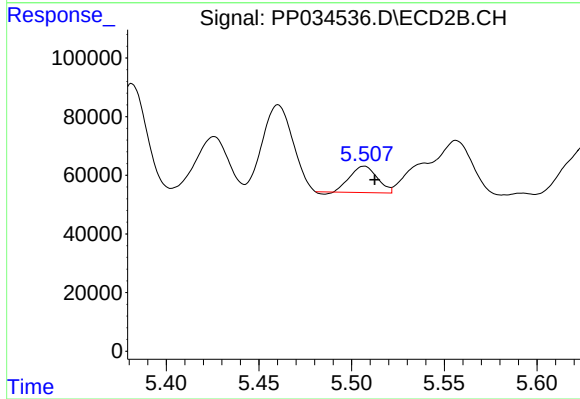


#21 AR-1248-1

R.T.: 5.507 min
Delta R.T.: -0.006 min
Response: 90393
Conc: 123.91 ng/ml

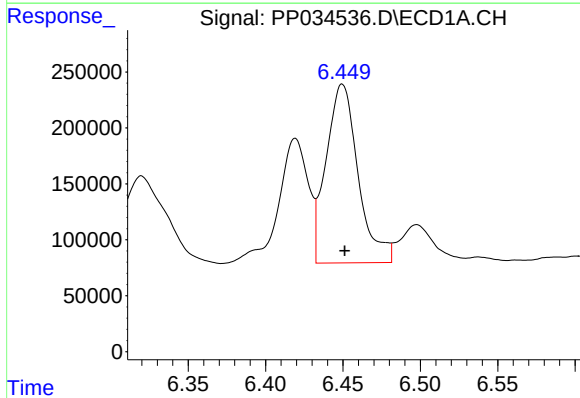


#22 AR-1248-2

R.T.: 6.450 min
Delta R.T.: -0.001 min
Response: 2297692
Conc: 1161.10 ng/ml

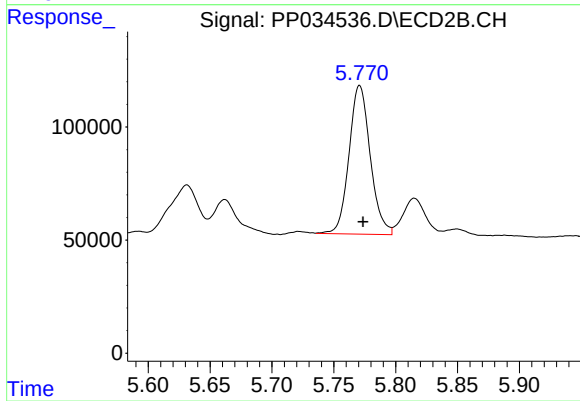

#22 AR-1248-2


R.T.: 5.771 min
Delta R.T.: -0.003 min
Response: 786618
Conc: 766.31 ng/ml

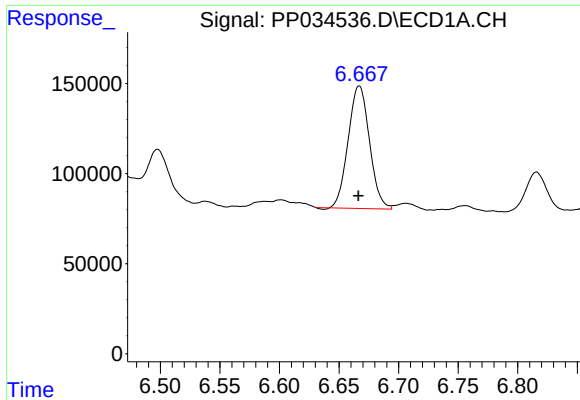

#23 AR-1248-3


R.T.: 6.667 min
Delta R.T.: 0.000 min
Response: 844874
Conc: 355.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

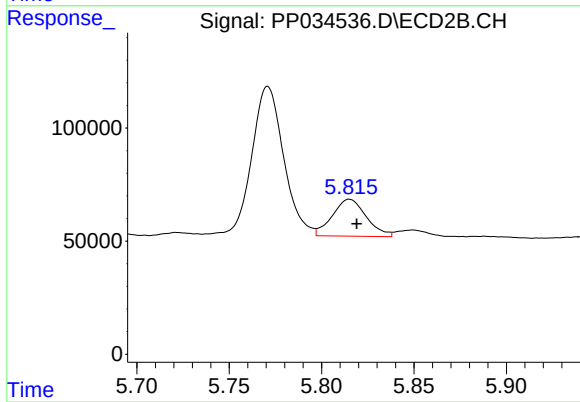


#23 AR-1248-3

R.T.: 5.815 min
Delta R.T.: -0.004 min
Response: 208890
Conc: 190.59 ng/ml

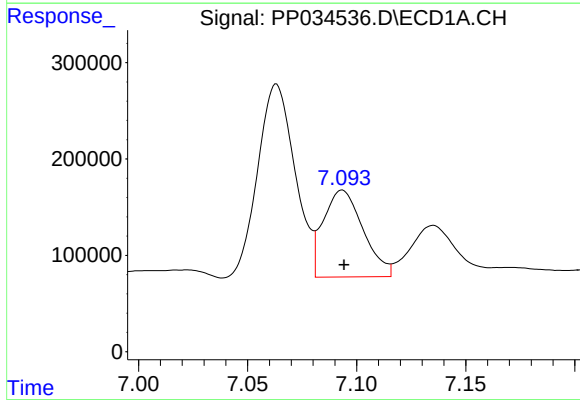


#24 AR-1248-4

R.T.: 7.093 min
Delta R.T.: 0.000 min
Response: 1145940
Conc: 449.06 ng/ml

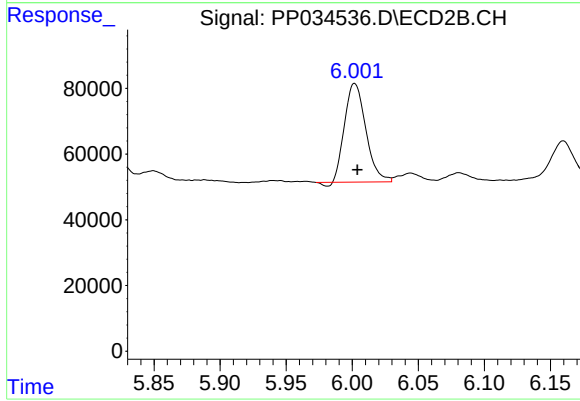

#24 AR-1248-4


R.T.: 6.002 min
Delta R.T.: -0.002 min
Response: 333638
Conc: 264.35 ng/ml

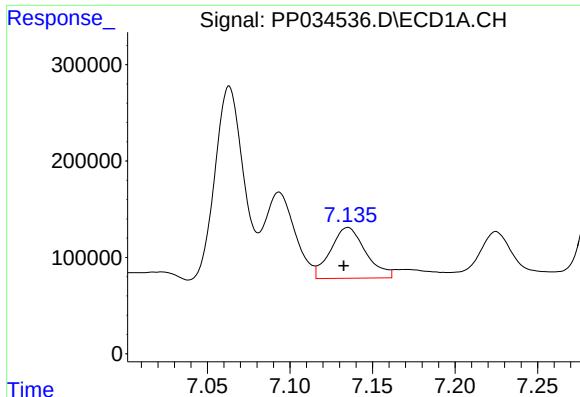

#25 AR-1248-5


R.T.: 7.135 min
Delta R.T.: 0.003 min
Response: 782928
Conc: 307.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

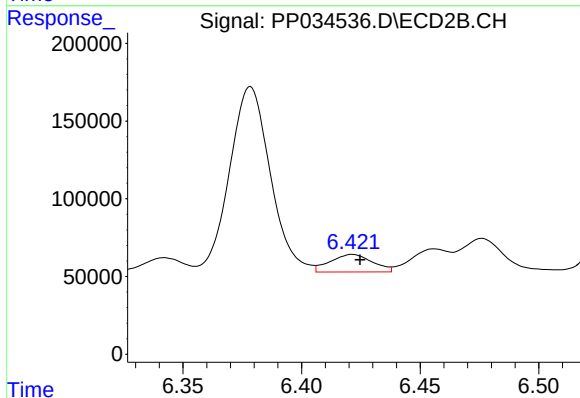


#25 AR-1248-5

R.T.: 6.421 min
Delta R.T.: -0.003 min
Response: 141129
Conc: 124.88 ng/ml

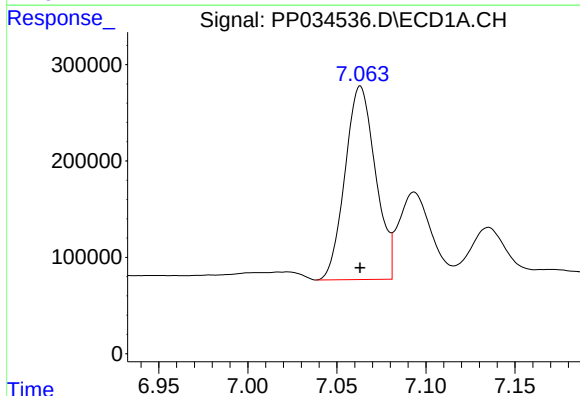


#26 AR-1254-1

R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 2391635
Conc: 869.83 ng/ml

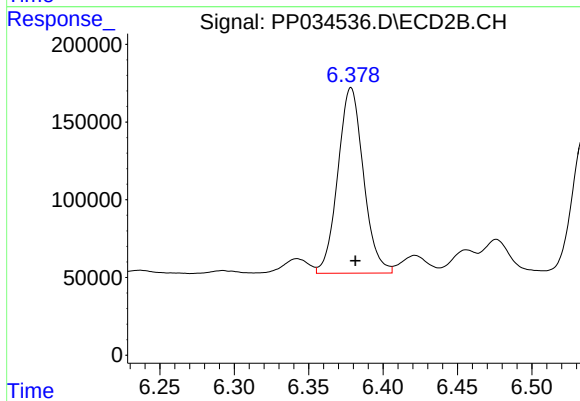

#26 AR-1254-1


R.T.: 6.378 min
Delta R.T.: -0.003 min
Response: 1430996
Conc: 775.65 ng/ml

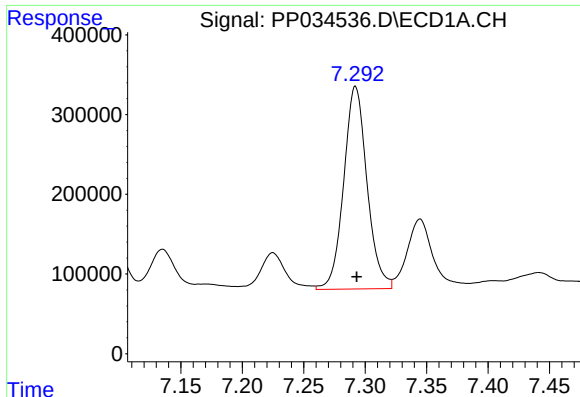

#27 AR-1254-2


R.T.: 7.292 min
Delta R.T.: 0.000 min
Response: 3359739
Conc: 790.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

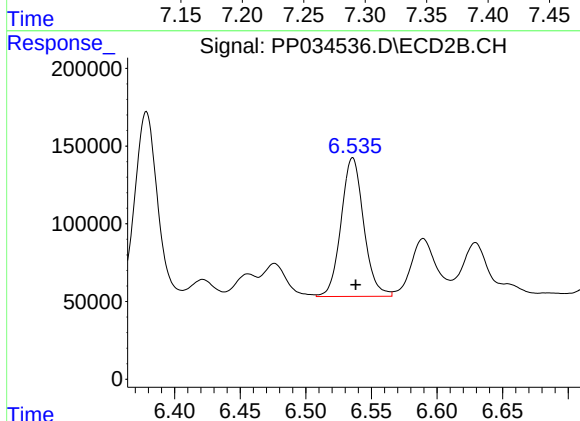


#27 AR-1254-2

R.T.: 6.536 min
Delta R.T.: -0.002 min
Response: 1070847
Conc: 669.33 ng/ml

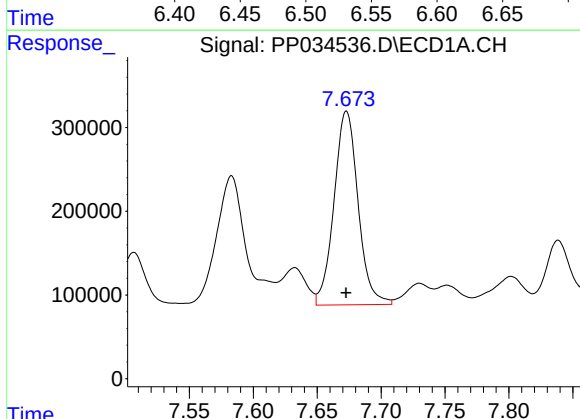


#28 AR-1254-3

R.T.: 7.673 min
Delta R.T.: 0.000 min
Response: 3036249
Conc: 665.23 ng/ml

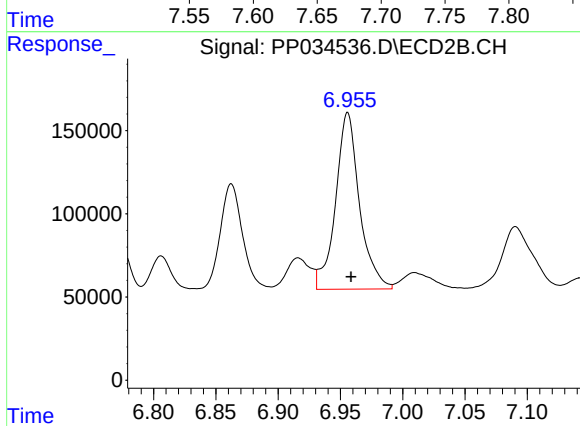

#28 AR-1254-3


R.T.: 6.956 min
Delta R.T.: -0.003 min
Response: 1421760
Conc: 569.67 ng/ml

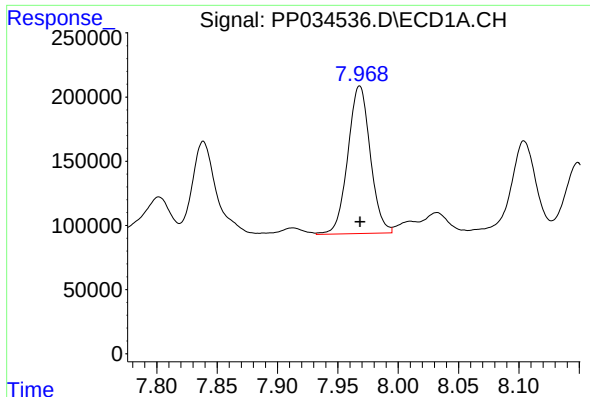

#29 AR-1254-4


R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 1487680
Conc: 481.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

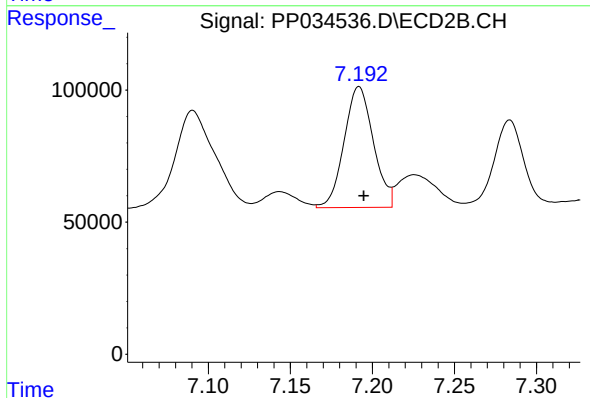


#29 AR-1254-4

R.T.: 7.192 min
Delta R.T.: -0.003 min
Response: 568897
Conc: 432.77 ng/ml

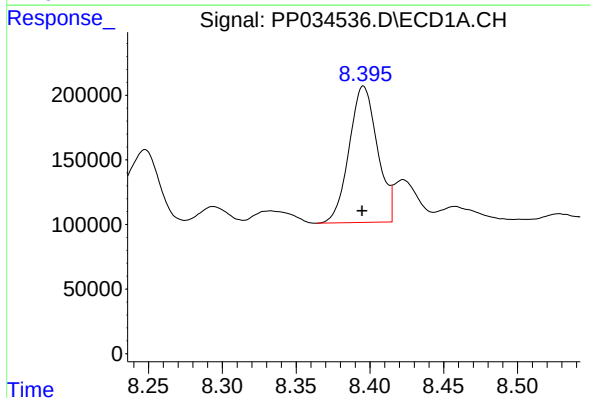


#30 AR-1254-5

R.T.: 8.396 min
Delta R.T.: 0.000 min
Response: 1404115
Conc: 395.10 ng/ml

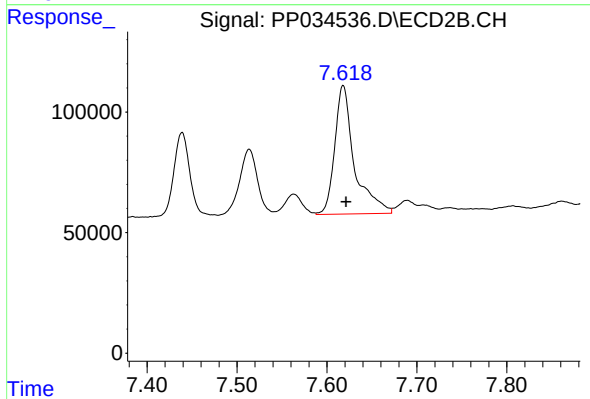

#30 AR-1254-5


R.T.: 7.618 min
Delta R.T.: -0.003 min
Response: 811500
Conc: 399.28 ng/ml

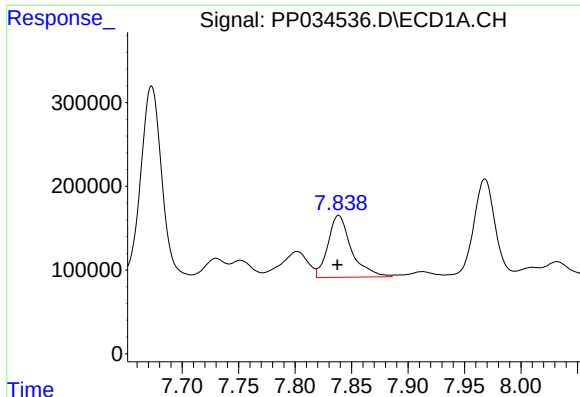

#31 AR-1260-1


R.T.: 7.839 min
Delta R.T.: 0.000 min
Response: 1069574
Conc: 344.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

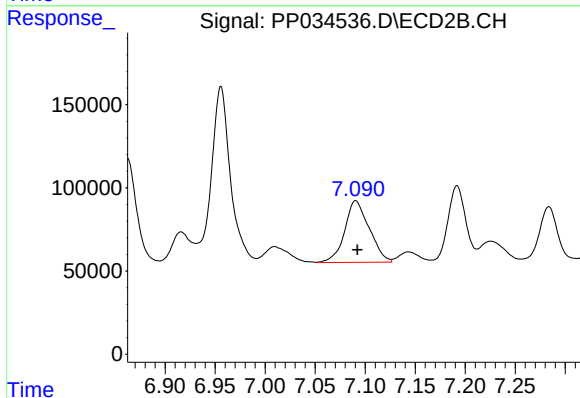


#31 AR-1260-1

R.T.: 7.090 min
Delta R.T.: -0.002 min
Response: 635594
Conc: 413.89 ng/ml

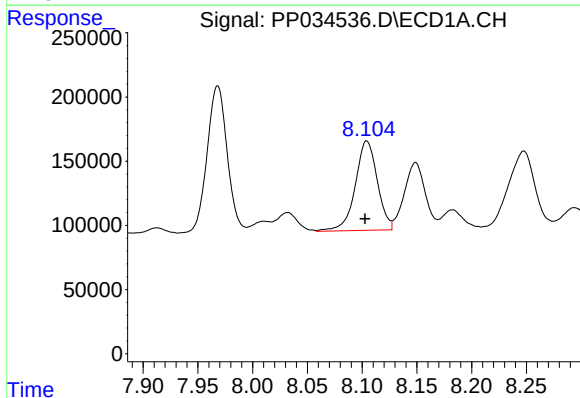


#32 AR-1260-2

R.T.: 8.104 min
Delta R.T.: 0.001 min
Response: 977894
Conc: 260.40 ng/ml

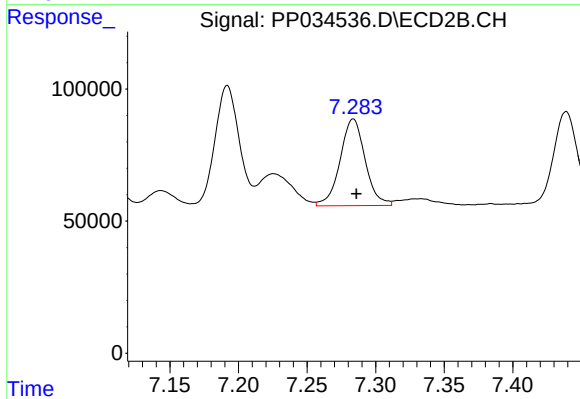

#32 AR-1260-2


R.T.: 7.284 min
Delta R.T.: -0.002 min
Response: 417917
Conc: 231.35 ng/ml

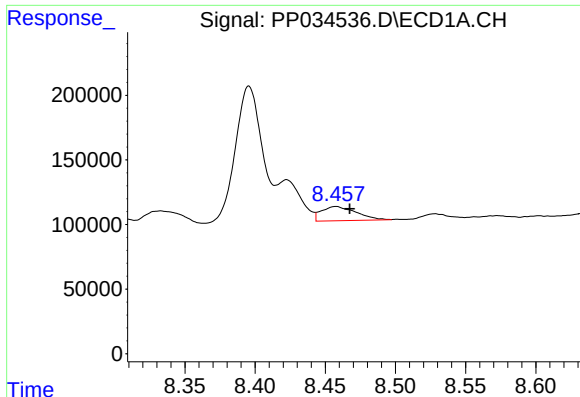

#33 AR-1260-3


R.T.: 8.458 min
Delta R.T.: -0.010 min
Response: 190595
Conc: 63.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

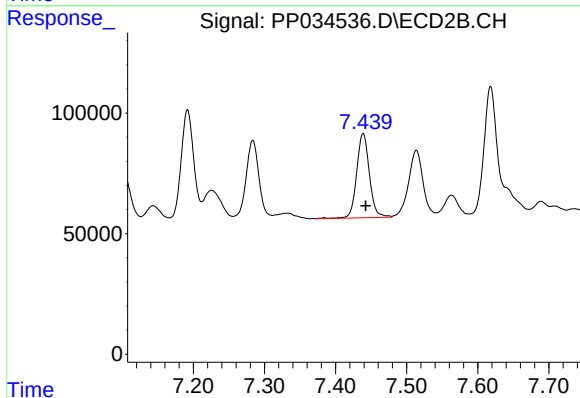


#33 AR-1260-3

R.T.: 7.439 min
Delta R.T.: -0.004 min
Response: 434382
Conc: 250.38 ng/ml

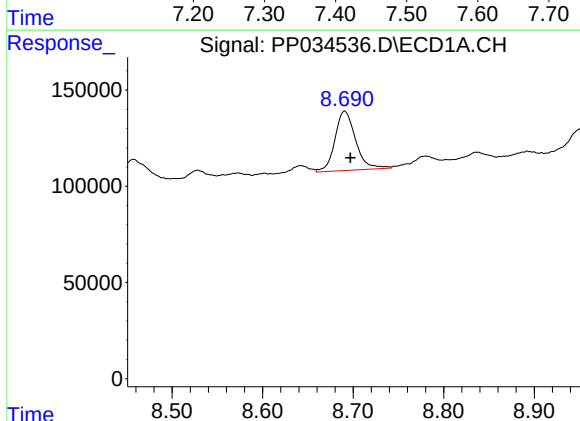


#34 AR-1260-4

R.T.: 8.691 min
Delta R.T.: -0.006 min
Response: 489792
Conc: 140.29 ng/ml

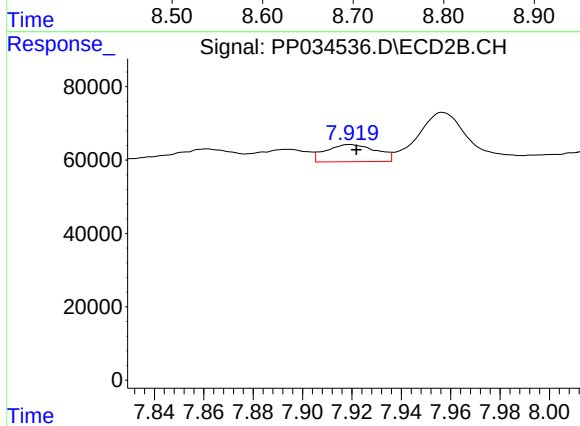

#34 AR-1260-4


R.T.: 7.919 min
Delta R.T.: -0.003 min
Response: 66065
Conc: 46.08 ng/ml

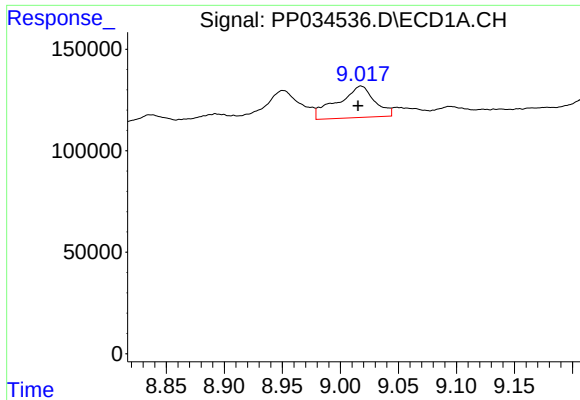

#35 AR-1260-5


R.T.: 9.018 min
Delta R.T.: 0.003 min
Response: 343492
Conc: 47.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

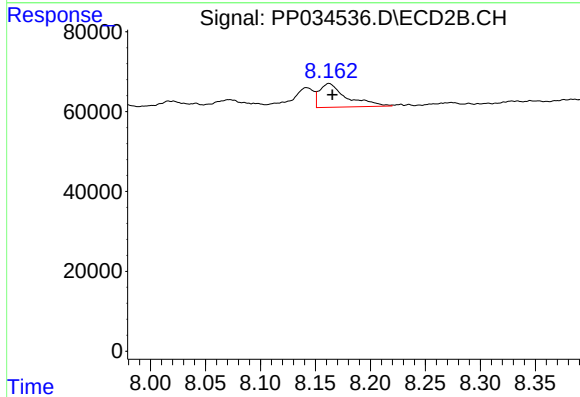


#35 AR-1260-5

R.T.: 8.162 min
Delta R.T.: -0.003 min
Response: 102587
Conc: 30.03 ng/ml

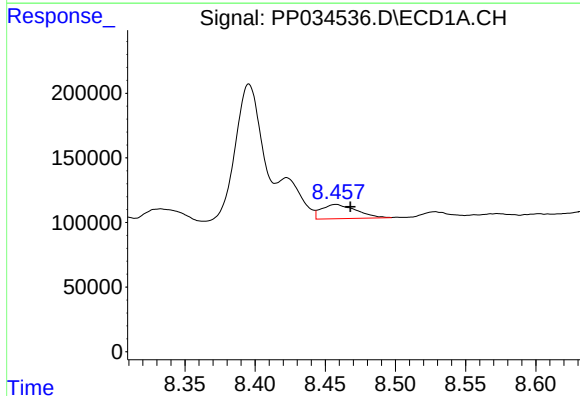


#36 AR-1262-1

R.T.: 8.458 min
Delta R.T.: -0.010 min
Response: 190595
Conc: 41.65 ng/ml

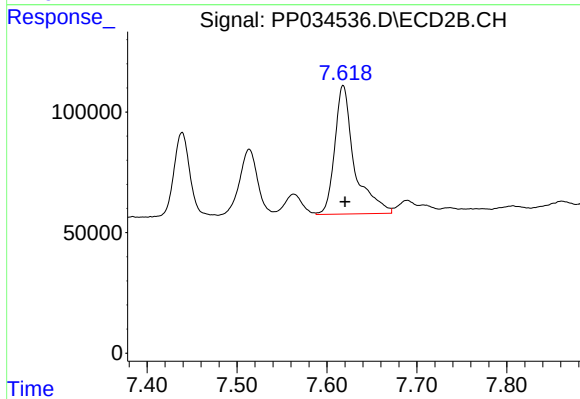

#36 AR-1262-1


R.T.: 7.618 min
Delta R.T.: -0.002 min
Response: 811500
Conc: 755.59 ng/ml

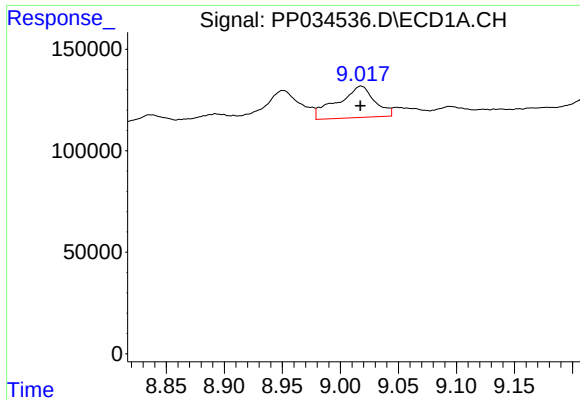

#37 AR-1262-2


R.T.: 9.018 min
Delta R.T.: 0.000 min
Response: 343492
Conc: 44.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

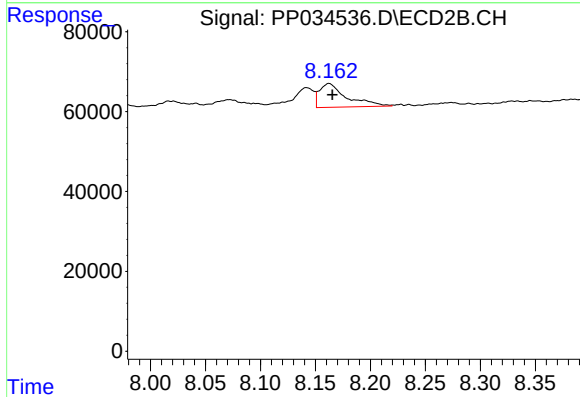


#37 AR-1262-2

R.T.: 8.162 min
Delta R.T.: -0.003 min
Response: 102587
Conc: 29.90 ng/ml

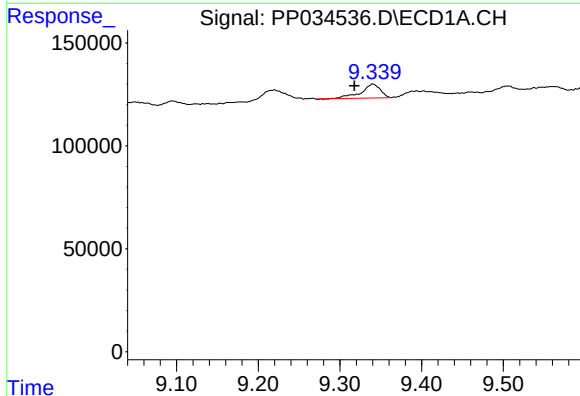


#38 AR-1262-3

R.T.: 9.340 min
Delta R.T.: 0.023 min
Response: 109738
Conc: 20.39 ng/ml

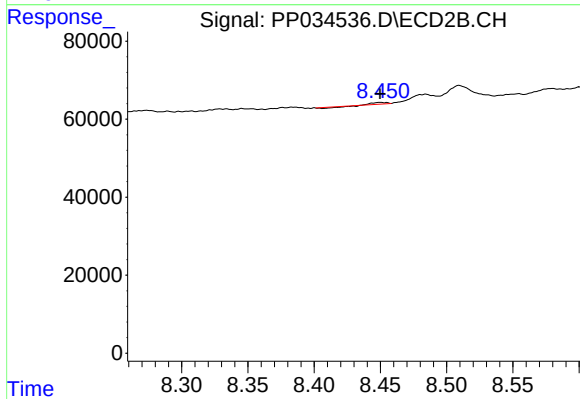

#38 AR-1262-3


R.T.: 8.450 min
Delta R.T.: 0.000 min
Response: 472
Conc: 0.32 ng/ml

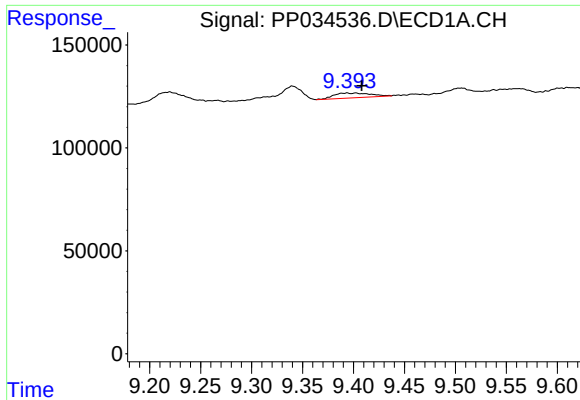

#39 AR-1262-4


R.T.: 9.394 min
Delta R.T.: -0.014 min
Response: 57595
Conc: 12.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

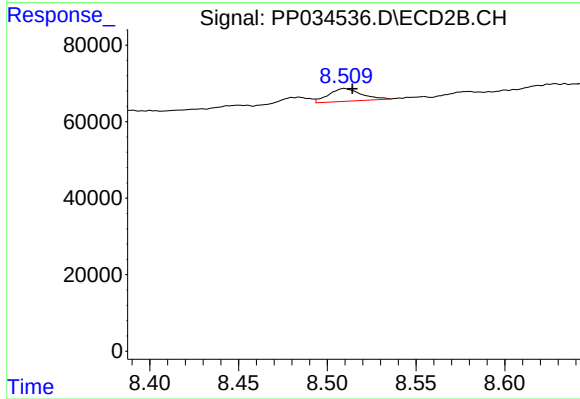


#39 AR-1262-4

R.T.: 8.510 min
Delta R.T.: -0.005 min
Response: 42792
Conc: 15.54 ng/ml

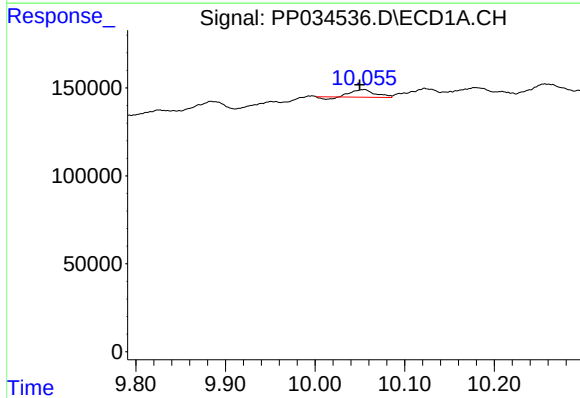


#40 AR-1262-5

R.T.: 10.055 min
Delta R.T.: 0.005 min
Response: 69395
Conc: 24.10 ng/ml

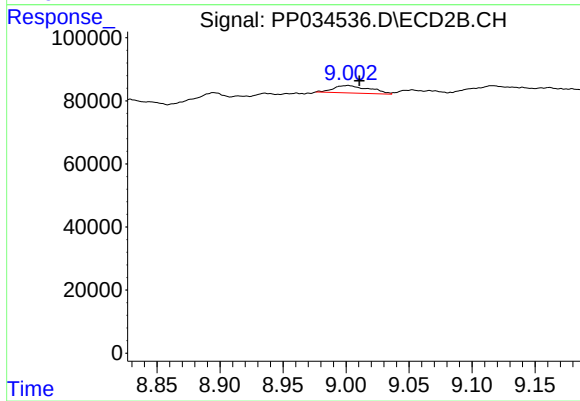

#40 AR-1262-5


R.T.: 9.002 min
Delta R.T.: -0.009 min
Response: 47251
Conc: 41.64 ng/ml

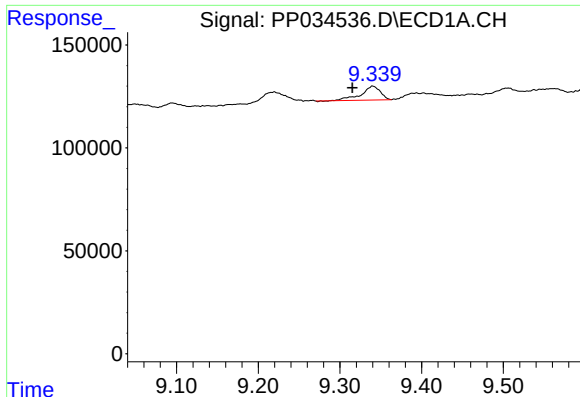

#41 AR-1268-1


R.T.: 9.340 min
Delta R.T.: 0.025 min
Response: 109738
Conc: 10.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

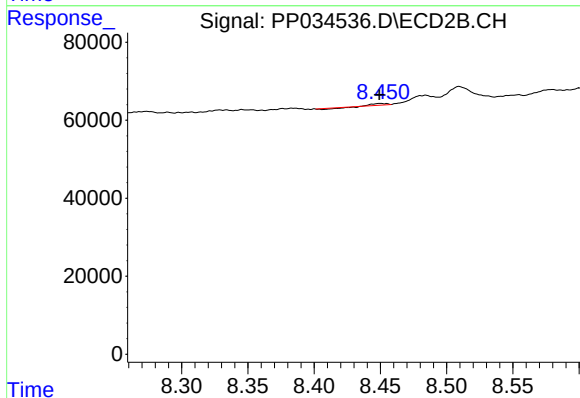


#41 AR-1268-1

R.T.: 8.450 min
Delta R.T.: 0.000 min
Response: 472
Conc: 0.11 ng/ml

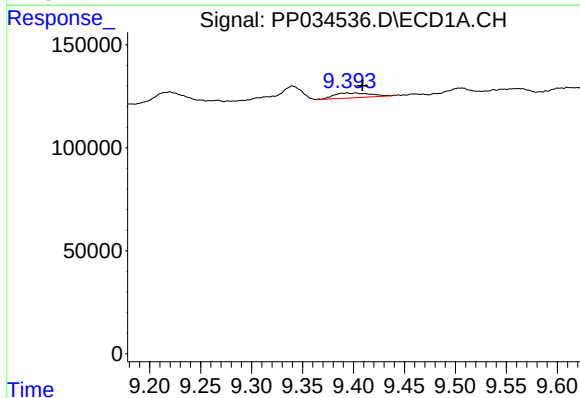


#42 AR-1268-2

R.T.: 9.394 min
Delta R.T.: -0.015 min
Response: 57595
Conc: 6.02 ng/ml

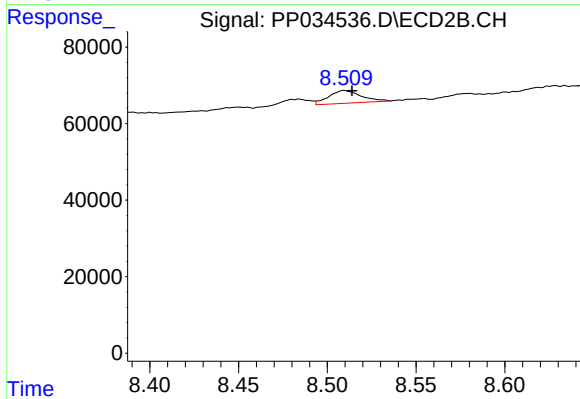

#42 AR-1268-2


R.T.: 8.510 min
Delta R.T.: -0.004 min
Response: 42792
Conc: 10.34 ng/ml

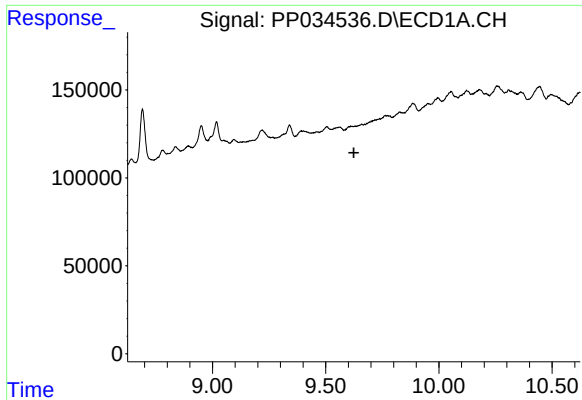

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

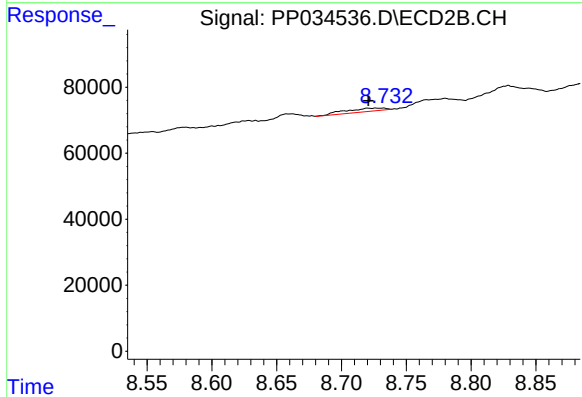


#43 AR-1268-3

R.T.: 8.732 min
Delta R.T.: 0.011 min
Response: 22072
Conc: 6.07 ng/ml

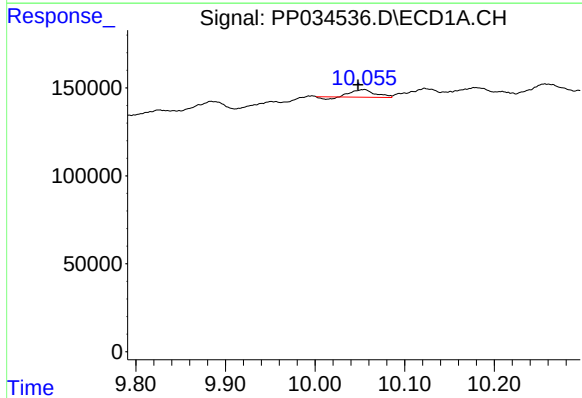


#44 AR-1268-4

R.T.: 10.055 min
Delta R.T.: 0.007 min
Response: 69395
Conc: 21.72 ng/ml

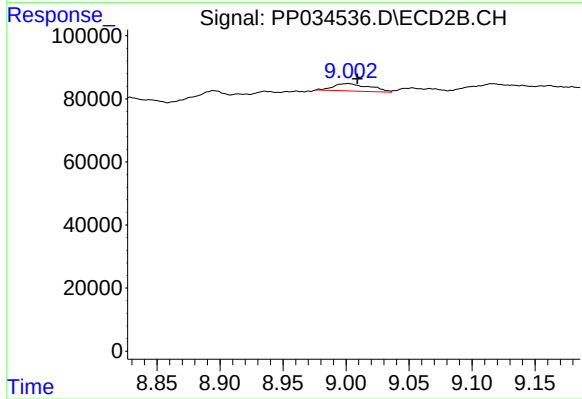

#44 AR-1268-4


R.T.: 9.002 min
Delta R.T.: -0.007 min
Response: 47251
Conc: 36.68 ng/ml

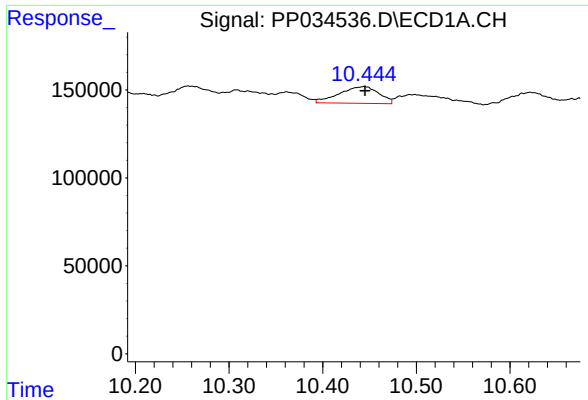

#45 AR-1268-5

R.T.: 10.444 min
Delta R.T.: -0.001 min
Response: 279231
Conc: 9.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

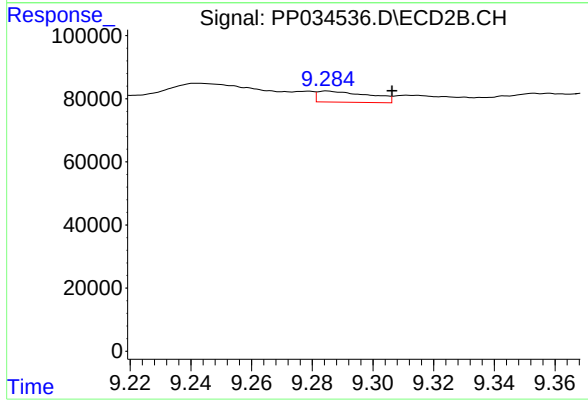

#45 AR-1268-5

R.T.: 9.285 min
Delta R.T.: -0.022 min
Response: 41659
Conc: 4.01 ng/ml