

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
 Data File : PP034566.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2021 22:48
 Operator : DD\AJ
 Sample : M1885-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SG1-8015-8025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 03:02:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.844	4.257	1602306	897547	21.004	19.980
2)	SA Decachlor...	10.764	9.561	1663278	602343	21.607	21.332
Target Compounds							
7)	L1 AR-1016-5	0.000	5.989	0	8891	N.D.	9.720 #
8)	L2 AR-1221-1	5.094	0.000	71763	0	98.169	N.D. #
9)	L2 AR-1221-2	5.192	4.612	23601	9239	41.433	26.481 #
15)	L3 AR-1232-5	0.000	5.989	0	8891	N.D.	25.012 #
20)	L4 AR-1242-5	0.000	6.377	0	5062	N.D.	6.174 #
24)	L5 AR-1248-4	0.000	5.989	0	8891	N.D.	7.044 #
26)	L6 AR-1254-1	0.000	6.377	0	5062	N.D.	2.744 #
27)	L6 AR-1254-2	0.000	6.536	0	6842	N.D.	4.276 #
28)	L6 AR-1254-3	7.673	6.956	6974	16089	1.528	6.447 #
30)	L6 AR-1254-5	8.400	7.618	82143	13475	23.114	6.630 #
31)	L7 AR-1260-1	0.000	7.089	0	10680	N.D.	6.954 #
32)	L7 AR-1260-2	0.000	7.290	0	19750	N.D.	10.933 #
33)	L7 AR-1260-3	0.000	7.440	0	16088	N.D.	9.273 #
34)	L7 AR-1260-4	8.678f	7.923	10584	5749	3.032	4.010 #
35)	L7 AR-1260-5	0.000	8.183f	0	3489	N.D.	1.021 #
36)	L8 AR-1262-1	0.000	7.618	0	13475	N.D.	12.546 #
37)	L8 AR-1262-2	0.000	8.183f	0	3489	N.D.	1.017 #
40)	L8 AR-1262-5	0.000	9.015	0	8228	N.D.	7.251 #
43)	L9 AR-1268-3	0.000	8.696f	0	111185	N.D.	30.561 #
44)	L9 AR-1268-4	0.000	9.015	0	8228	N.D.	6.387 #
45)	L9 AR-1268-5	0.000	9.303	0	7646	N.D.	0.736 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
Data File : PP034566.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2021 22:48
Operator : DD\AJ
Sample : M1885-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
SG1-8015-8025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 03:02:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

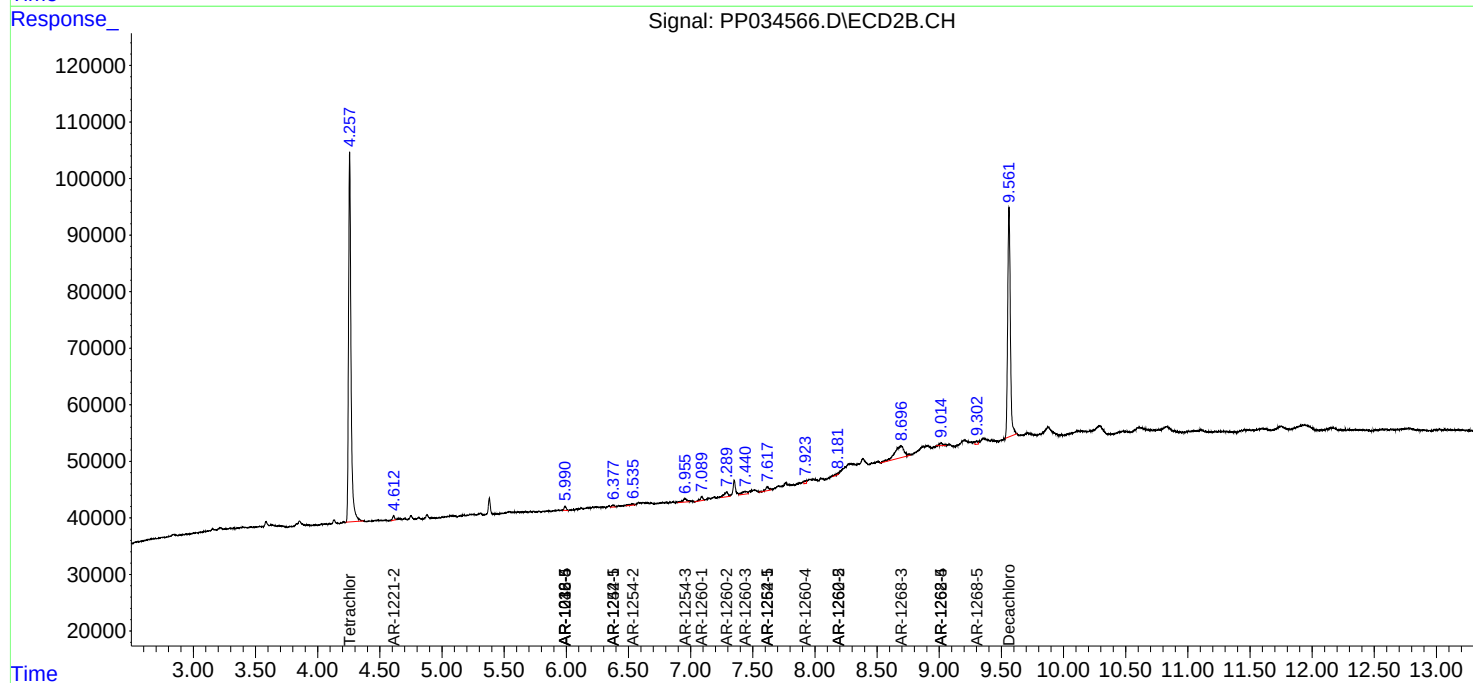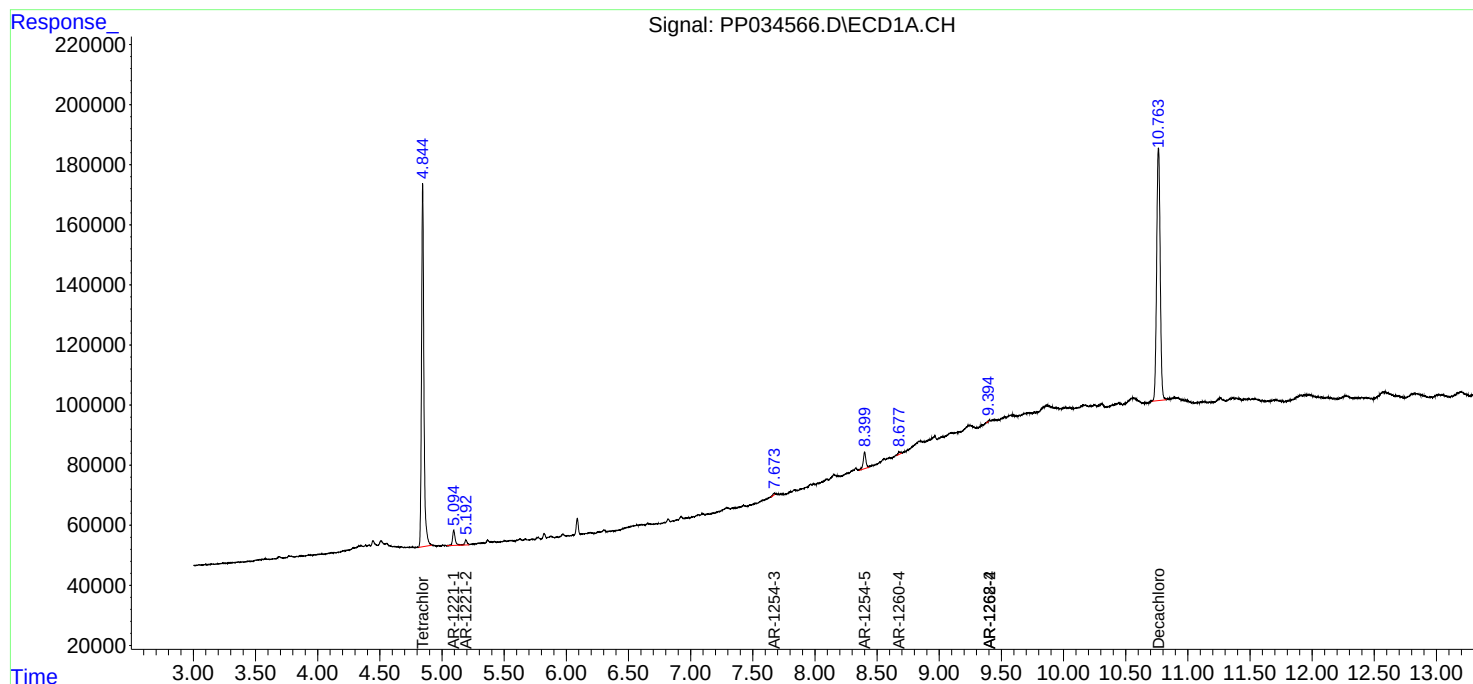


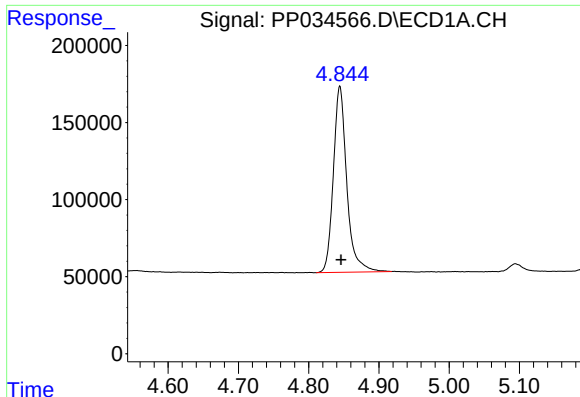

#1 Tetrachloro-m-xylene


R.T.: 4.844 min
Delta R.T.: -0.002 min
Response: 1602306
Conc: 21.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

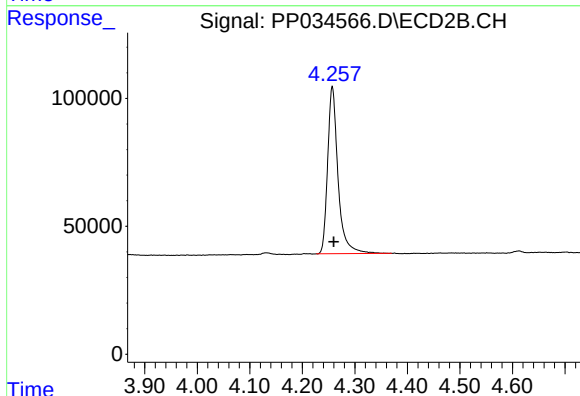


#1 Tetrachloro-m-xylene

R.T.: 4.257 min
Delta R.T.: -0.003 min
Response: 897547
Conc: 19.98 ng/ml

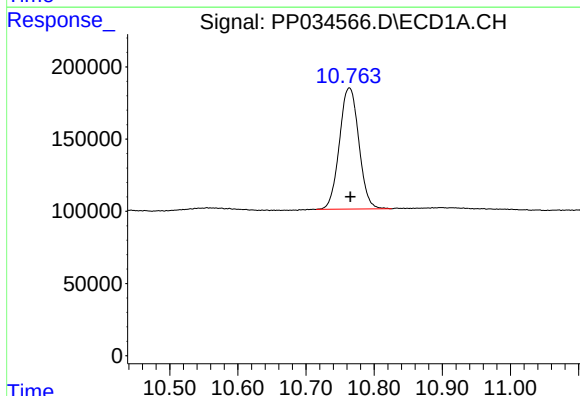


#2 Decachlorobiphenyl

R.T.: 10.764 min
Delta R.T.: -0.002 min
Response: 1663278
Conc: 21.61 ng/ml

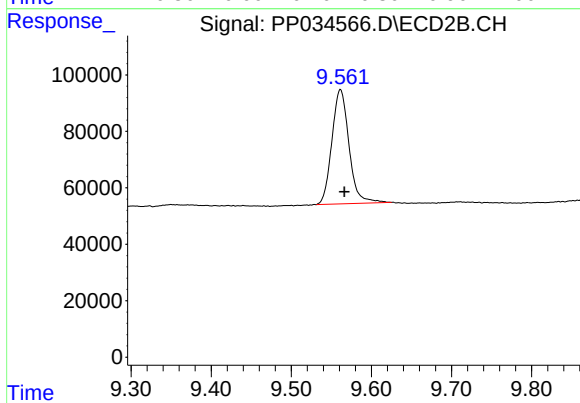

#2 Decachlorobiphenyl


R.T.: 9.561 min
Delta R.T.: -0.005 min
Response: 602343
Conc: 21.33 ng/ml

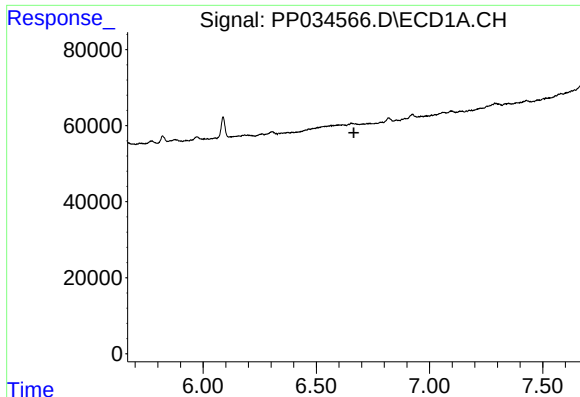

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

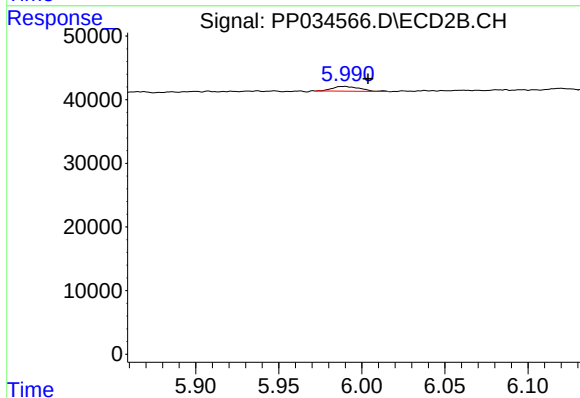


#7 AR-1016-5

R.T.: 5.989 min
Delta R.T.: -0.014 min
Response: 8891
Conc: 9.72 ng/ml

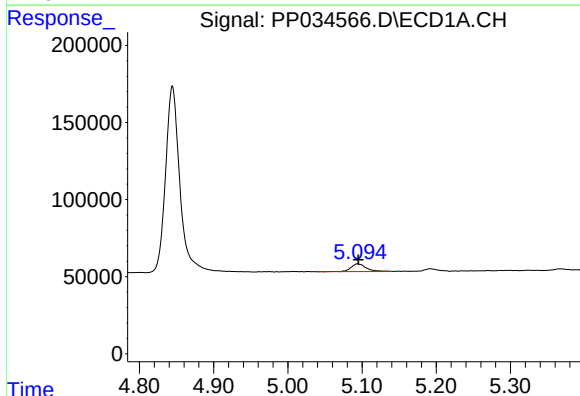


#8 AR-1221-1

R.T.: 5.094 min
Delta R.T.: 0.000 min
Response: 71763
Conc: 98.17 ng/ml

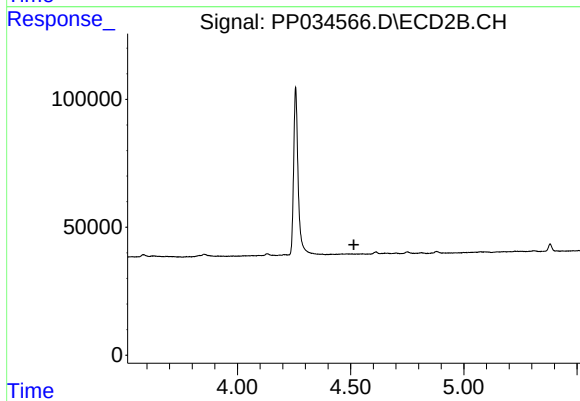

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.514 min
Response: 0
Conc: N.D.

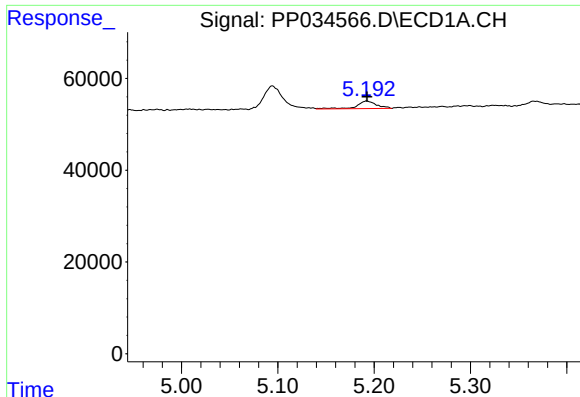

#9 AR-1221-2

R.T.: 5.192 min
Delta R.T.: 0.000 min
Response: 23601
Conc: 41.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

#9 AR-1221-2


R.T.: 4.612 min
Delta R.T.: -0.002 min
Response: 9239
Conc: 26.48 ng/ml

#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

#15 AR-1232-5


R.T.: 5.989 min
Delta R.T.: -0.014 min
Response: 8891
Conc: 25.01 ng/ml

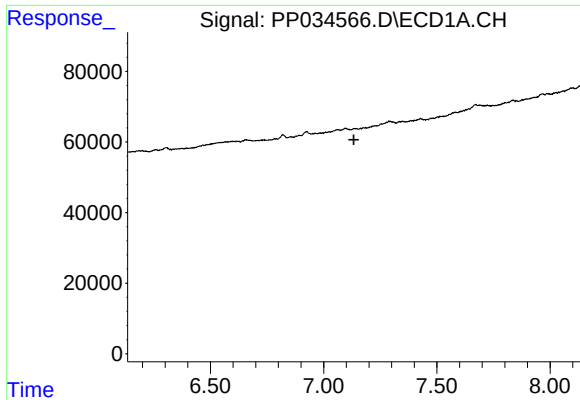

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

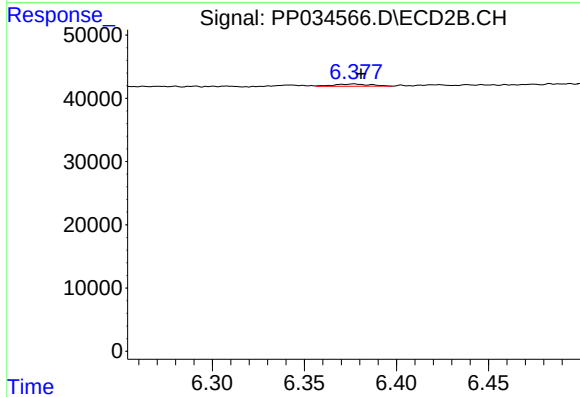


#20 AR-1242-5

R.T.: 6.377 min
Delta R.T.: -0.004 min
Response: 5062
Conc: 6.17 ng/ml

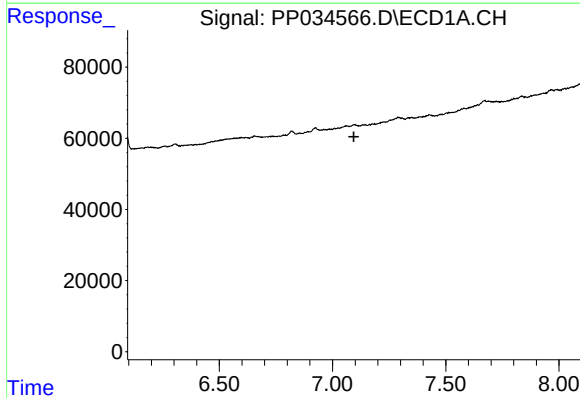


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 7.094 min
Response: 0
Conc: N.D.

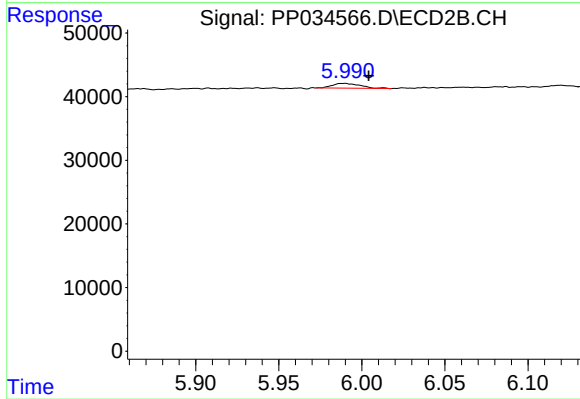

#24 AR-1248-4


R.T.: 5.989 min
Delta R.T.: -0.015 min
Response: 8891
Conc: 7.04 ng/ml

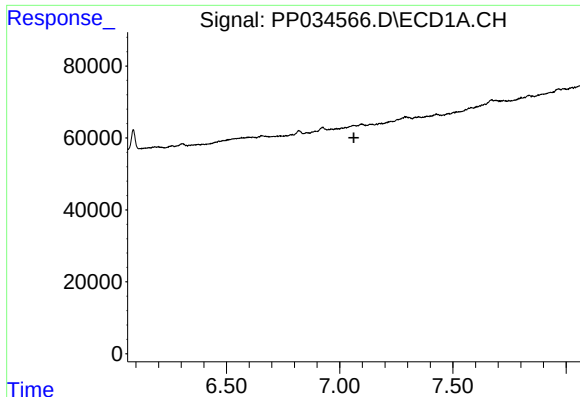

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 7.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

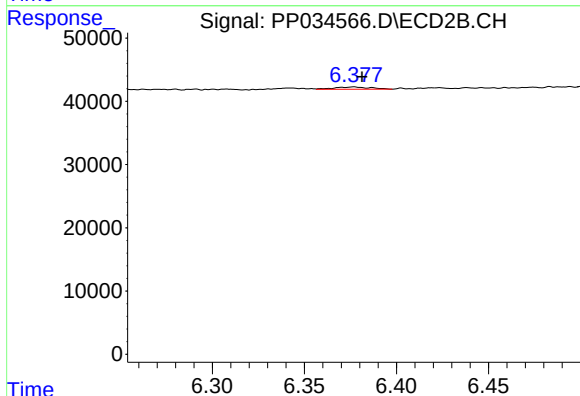


#26 AR-1254-1

R.T.: 6.377 min
Delta R.T.: -0.004 min
Response: 5062
Conc: 2.74 ng/ml

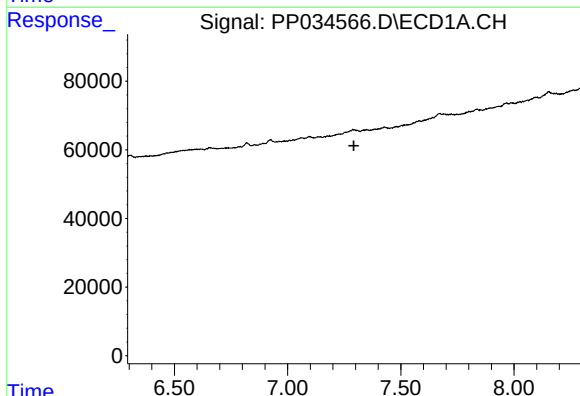


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 7.293 min
Response: 0
Conc: N.D.

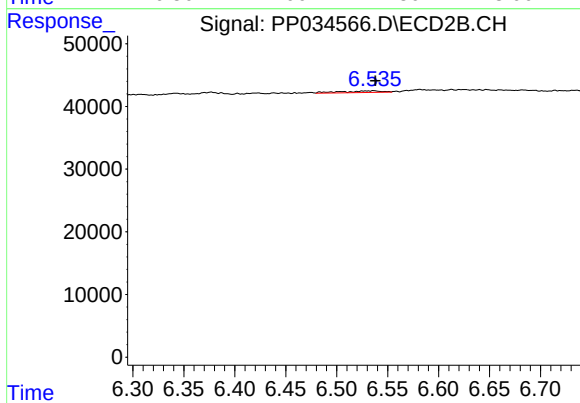

#27 AR-1254-2


R.T.: 6.536 min
Delta R.T.: -0.002 min
Response: 6842
Conc: 4.28 ng/ml

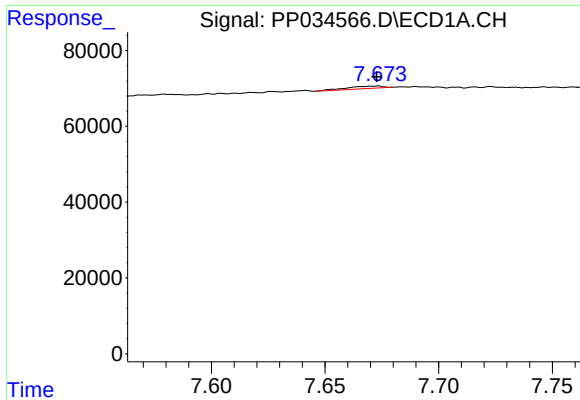

#28 AR-1254-3


R.T.: 7.673 min
Delta R.T.: 0.000 min
Response: 6974
Conc: 1.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

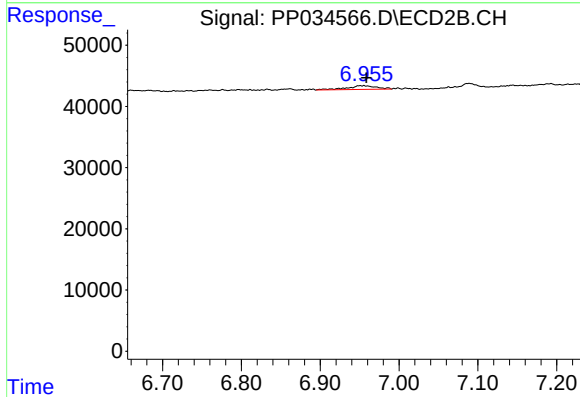


#28 AR-1254-3

R.T.: 6.956 min
Delta R.T.: -0.003 min
Response: 16089
Conc: 6.45 ng/ml

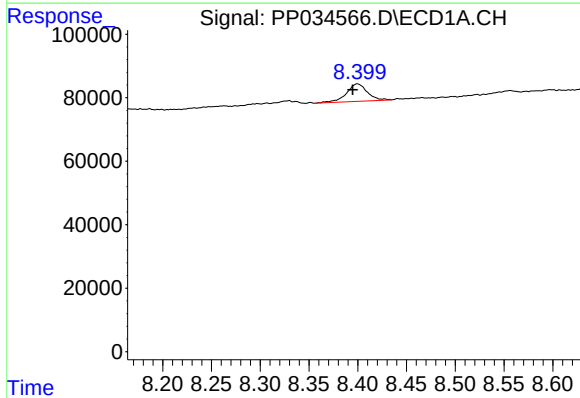


#30 AR-1254-5

R.T.: 8.400 min
Delta R.T.: 0.005 min
Response: 82143
Conc: 23.11 ng/ml

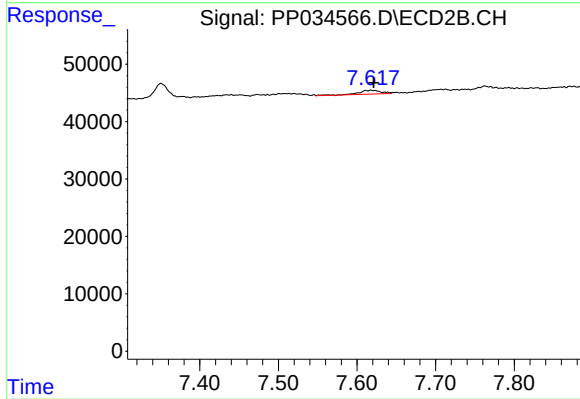

#30 AR-1254-5


R.T.: 7.618 min
Delta R.T.: -0.003 min
Response: 13475
Conc: 6.63 ng/ml

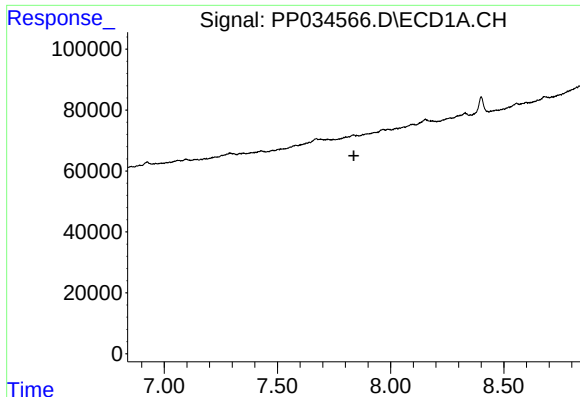

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

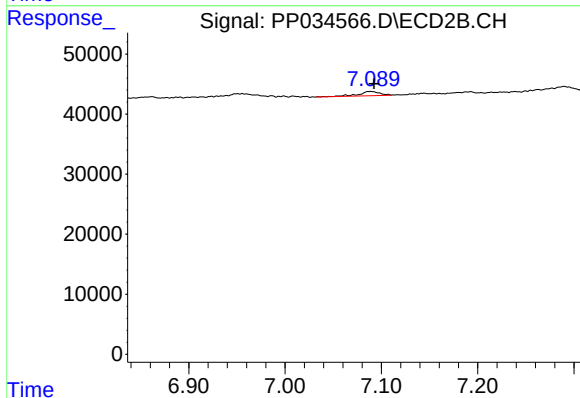


#31 AR-1260-1

R.T.: 7.089 min
Delta R.T.: -0.004 min
Response: 10680
Conc: 6.95 ng/ml

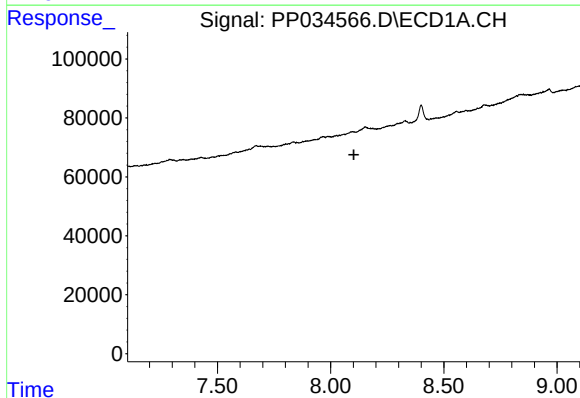


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 8.103 min
Response: 0
Conc: N.D.

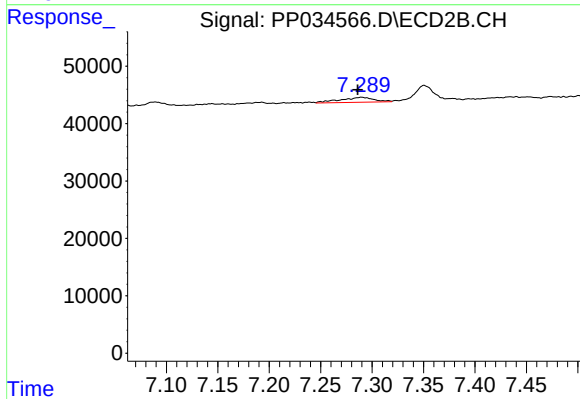

#32 AR-1260-2


R.T.: 7.290 min
Delta R.T.: 0.004 min
Response: 19750
Conc: 10.93 ng/ml

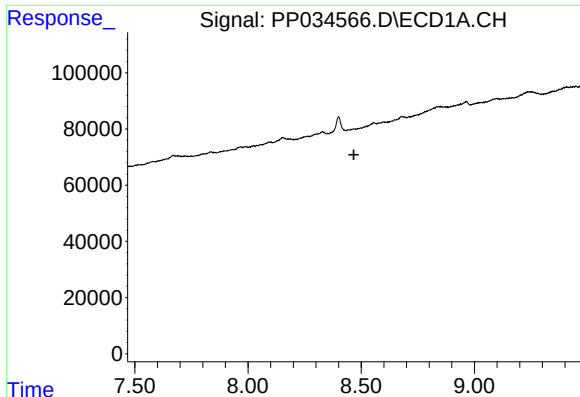

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

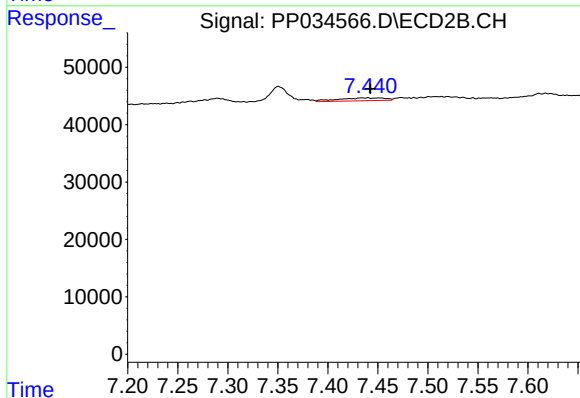


#33 AR-1260-3

R.T.: 7.440 min
Delta R.T.: -0.002 min
Response: 16088
Conc: 9.27 ng/ml

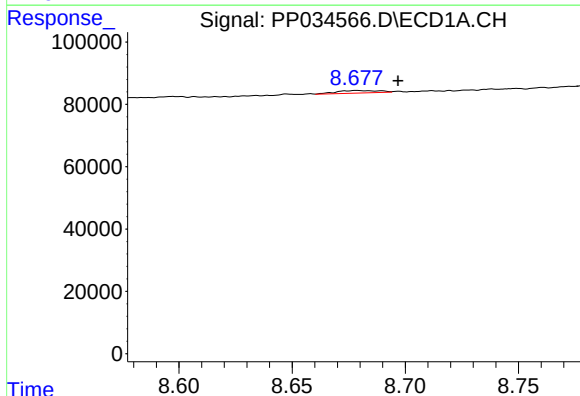


#34 AR-1260-4

R.T.: 8.678 min
Delta R.T.: -0.019 min
Response: 10584
Conc: 3.03 ng/ml

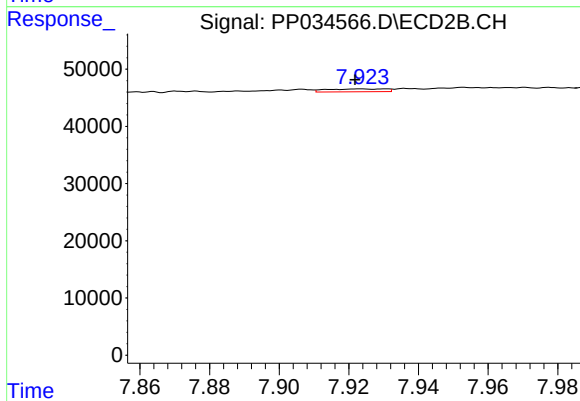

#34 AR-1260-4


R.T.: 7.923 min
Delta R.T.: 0.001 min
Response: 5749
Conc: 4.01 ng/ml

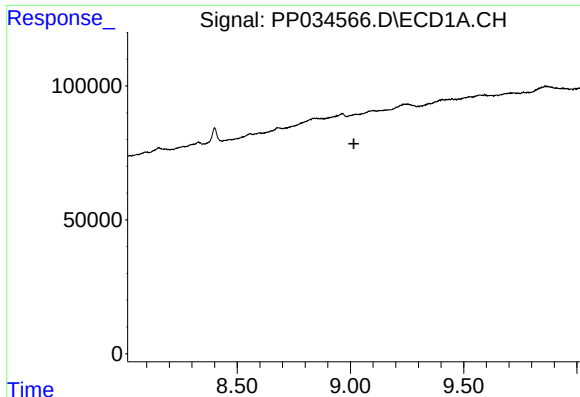

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.015 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

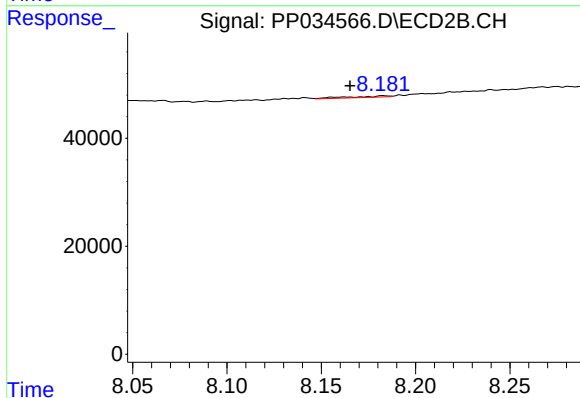


#35 AR-1260-5

R.T.: 8.183 min
Delta R.T.: 0.018 min
Response: 3489
Conc: 1.02 ng/ml

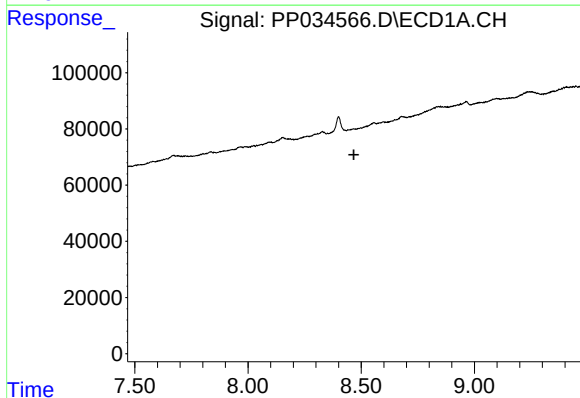


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.468 min
Response: 0
Conc: N.D.

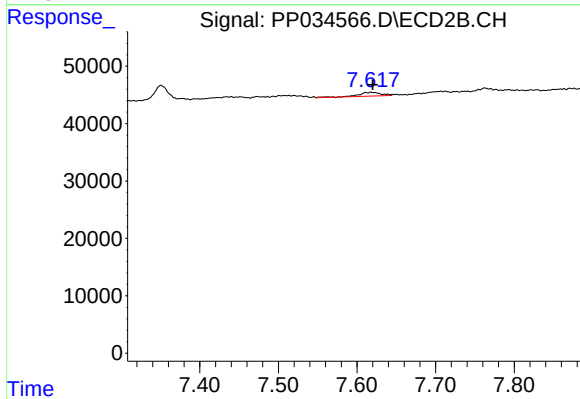

#36 AR-1262-1


R.T.: 7.618 min
Delta R.T.: -0.002 min
Response: 13475
Conc: 12.55 ng/ml

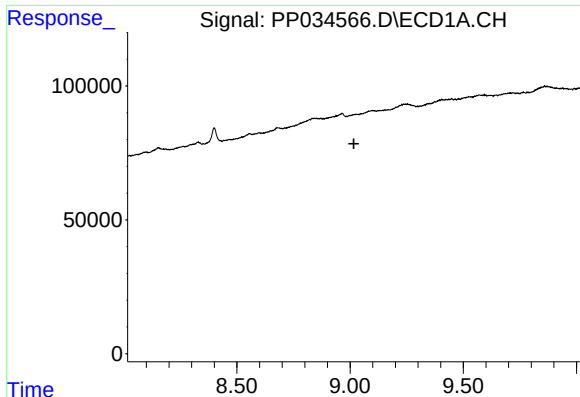

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 9.017 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

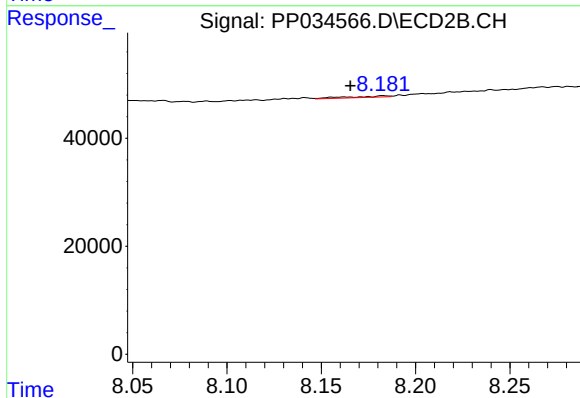


#37 AR-1262-2

R.T.: 8.183 min
Delta R.T.: 0.018 min
Response: 3489
Conc: 1.02 ng/ml

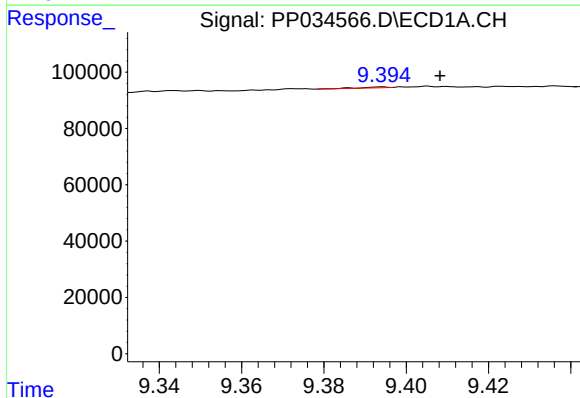


#39 AR-1262-4

R.T.: 9.394 min
Delta R.T.: -0.014 min
Response: 1368
Conc: 0.31 ng/ml

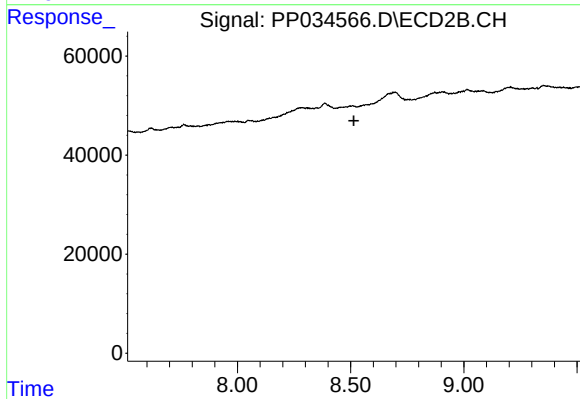

#39 AR-1262-4


R.T.: 8.509 min
Delta R.T.: -0.005 min
Response: -3217
Conc: N.D.

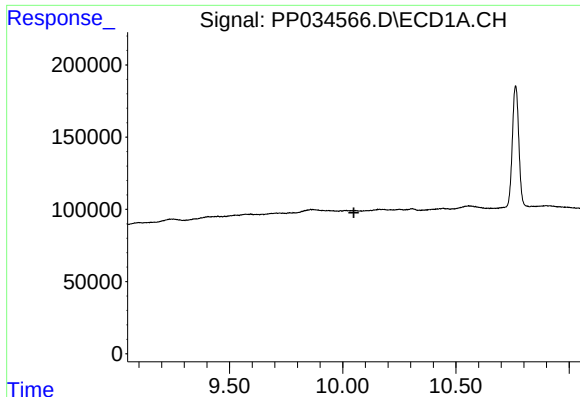

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

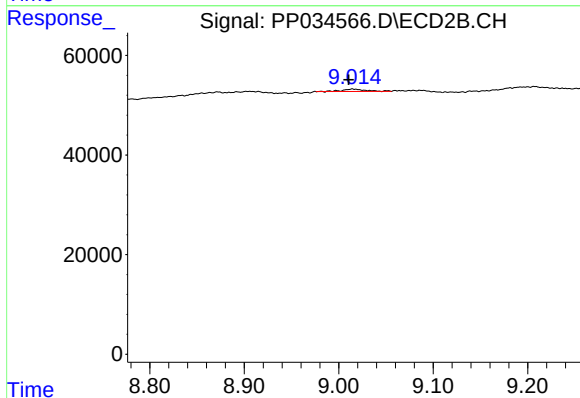


#40 AR-1262-5

R.T.: 9.015 min
Delta R.T.: 0.005 min
Response: 8228
Conc: 7.25 ng/ml

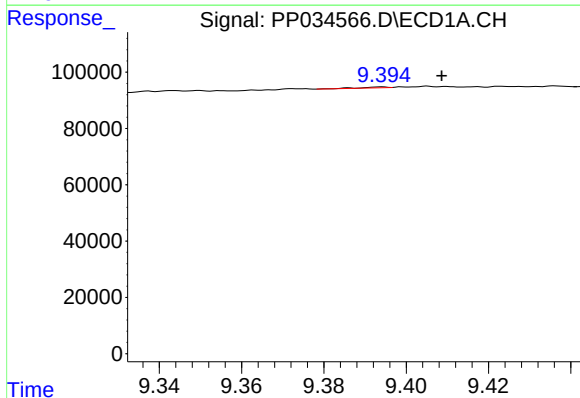


#42 AR-1268-2

R.T.: 9.394 min
Delta R.T.: -0.014 min
Response: 1368
Conc: 0.14 ng/ml

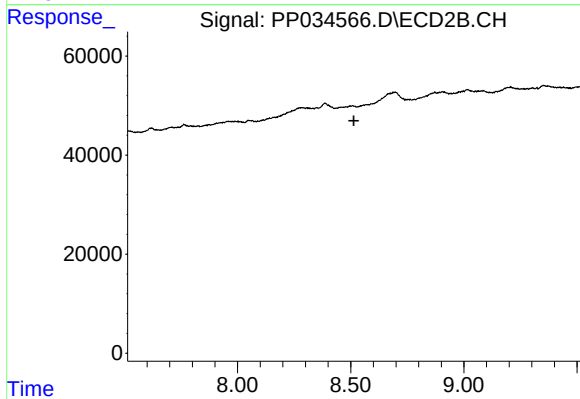

#42 AR-1268-2


R.T.: 8.509 min
Delta R.T.: -0.005 min
Response: -3217
Conc: N.D.

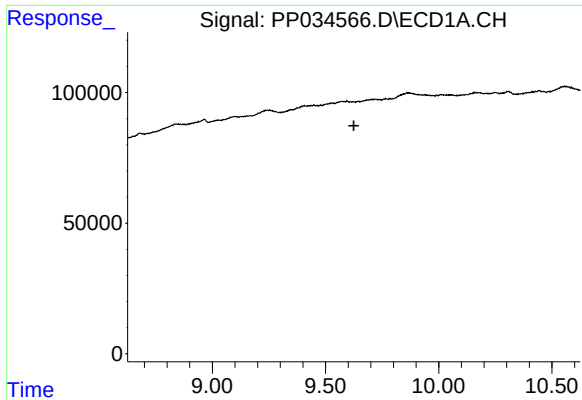

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

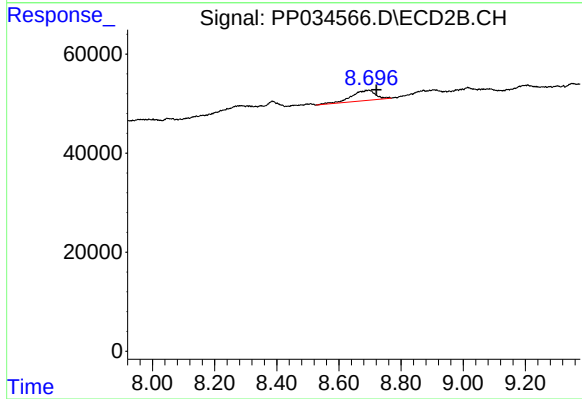


#43 AR-1268-3

R.T.: 8.696 min
Delta R.T.: -0.025 min
Response: 111185
Conc: 30.56 ng/ml

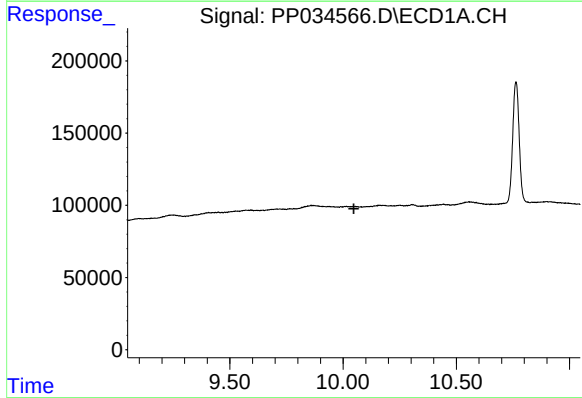


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 10.048 min
Response: 0
Conc: N.D.

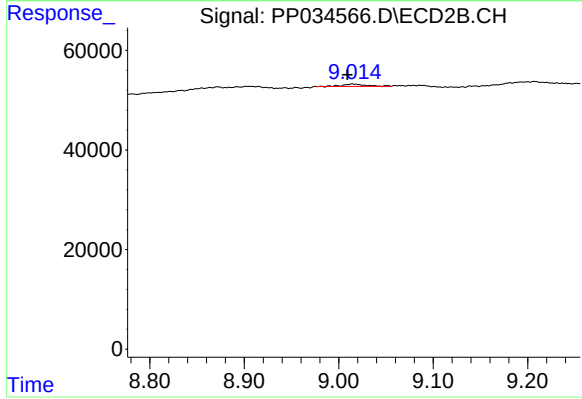

#44 AR-1268-4


R.T.: 9.015 min
Delta R.T.: 0.006 min
Response: 8228
Conc: 6.39 ng/ml

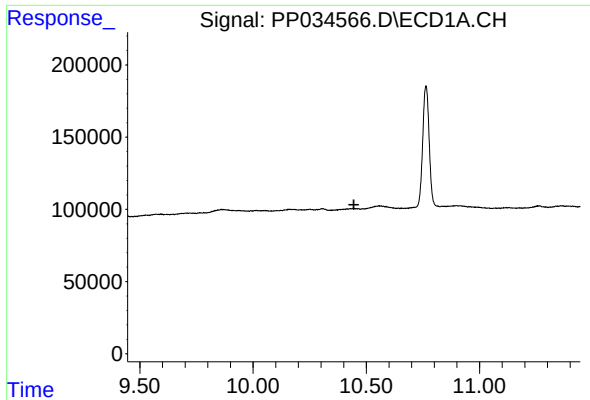

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.445 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SG1-8015-8025

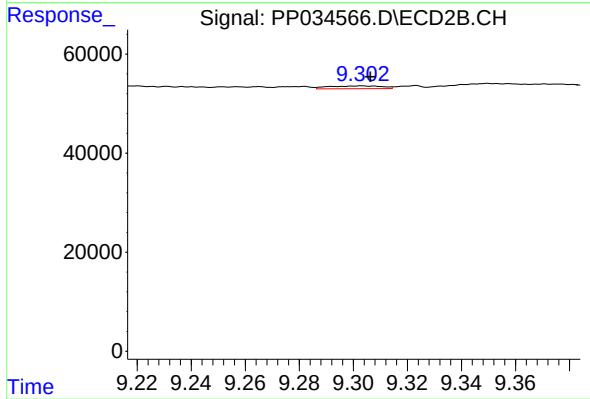

#45 AR-1268-5

R.T.: 9.303 min
Delta R.T.: -0.003 min
Response: 7646
Conc: 0.74 ng/ml