

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
 Data File : PP034531.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2021 12:22
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 4/2/2021 11:29:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 14:57:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.256	4153356	2244852	54.446	49.972
2) SA Decachlor...	10.771	9.565	3879858	1295946	50.401m	45.897m
Target Compounds						
21) L5 AR-1248-1	6.160	5.510	659022	303505	463.306	416.031
22) L5 AR-1248-2	6.453	5.771	971864	463736	491.113	451.762
23) L5 AR-1248-3	6.668	5.816	1181764	493058	497.146	449.874
24) L5 AR-1248-4	7.097	6.002	1165985	558551	456.910	442.547
25) L5 AR-1248-5	7.136	6.422	1188910	452931	466.570	400.774

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
Data File : PP034531.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2021 12:22
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 14:57:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

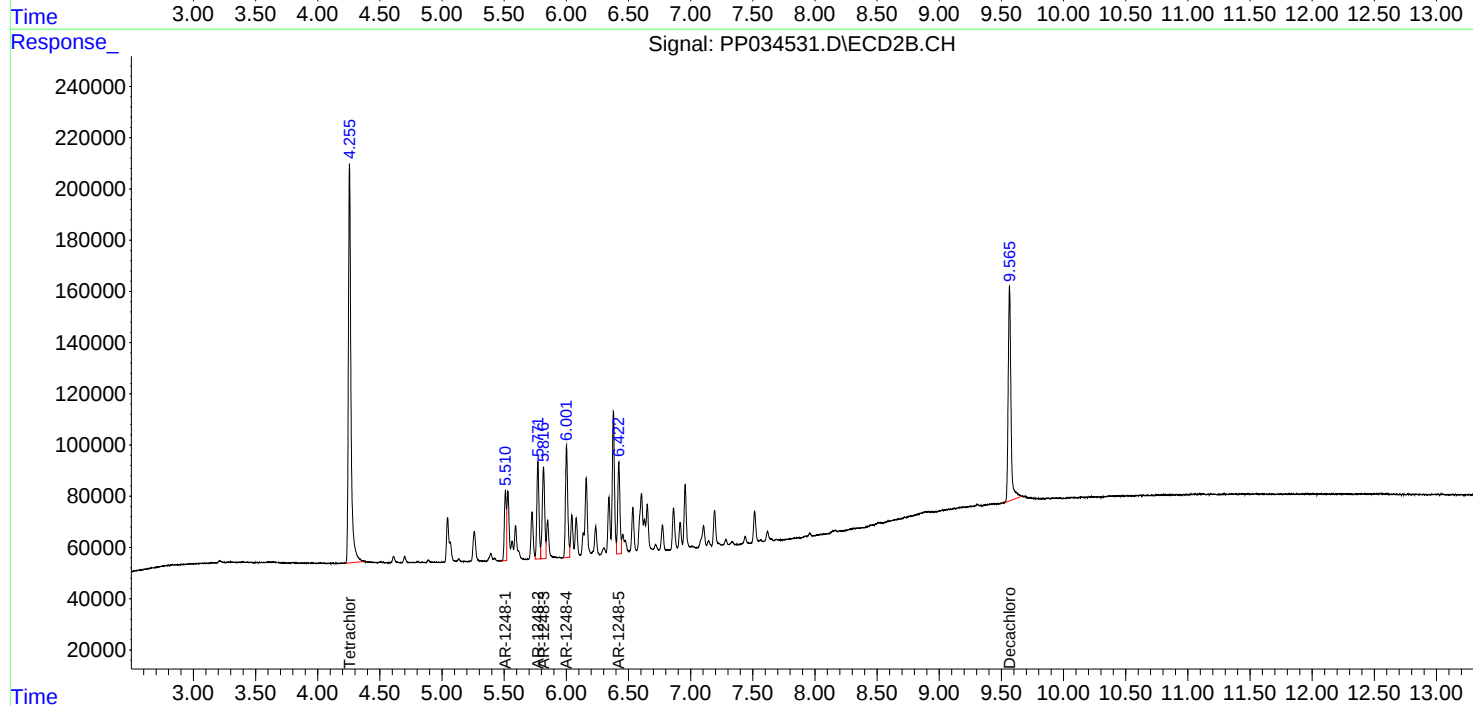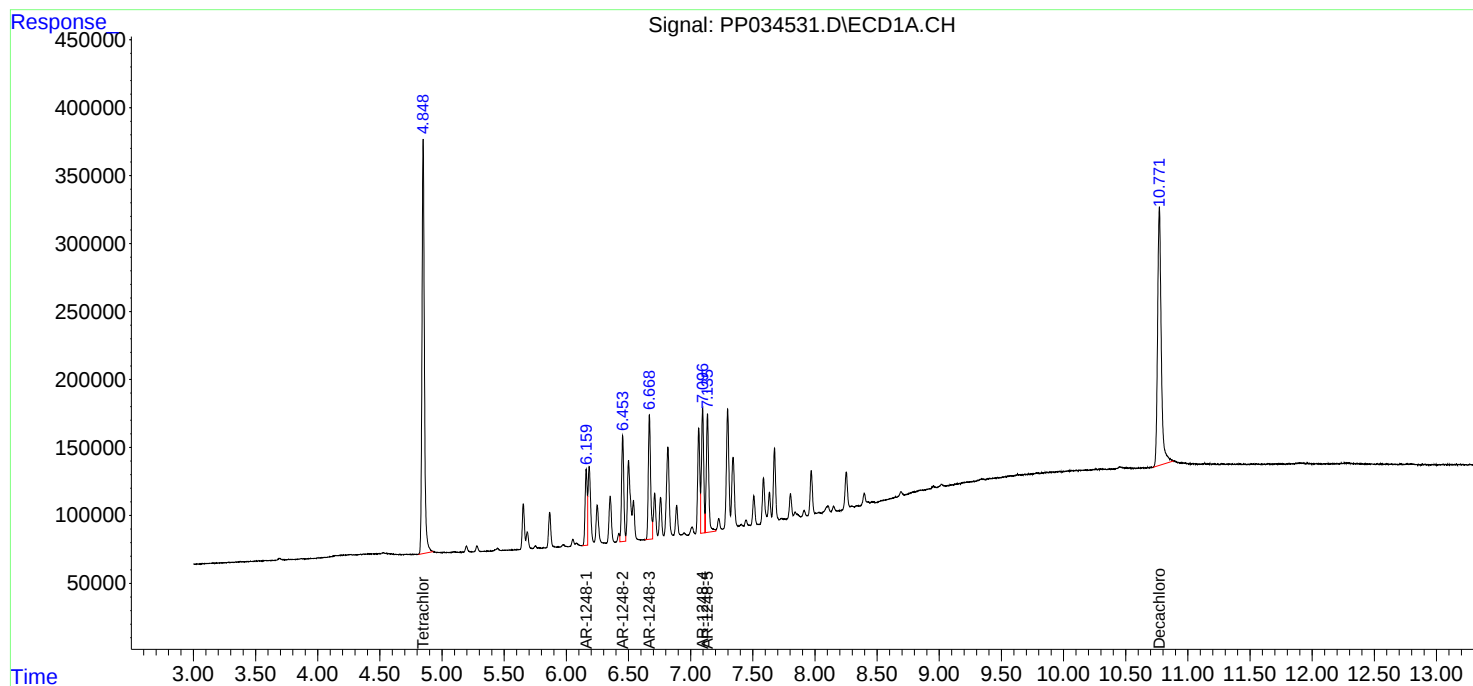

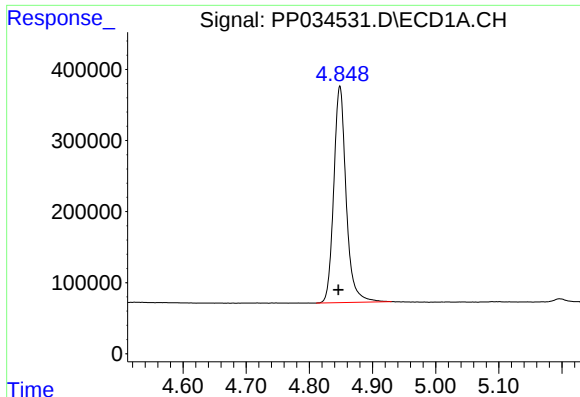


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: 0.002 min
Response: 4153356
Conc: 54.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:10 AM

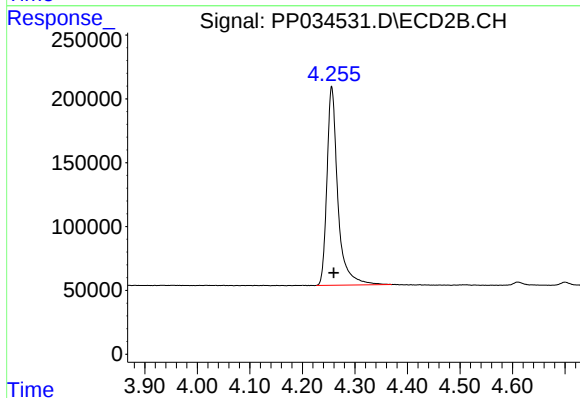


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: -0.004 min
Response: 2244852
Conc: 49.97 ng/ml

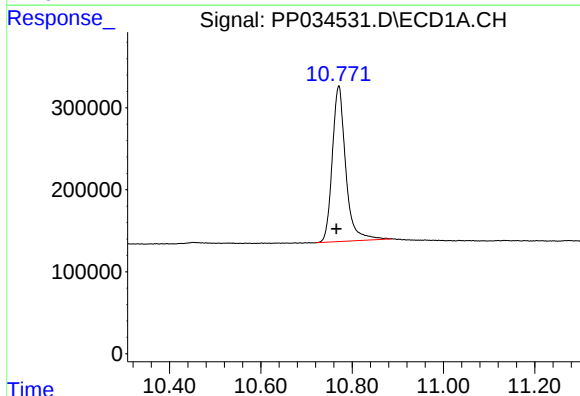


#2 Decachlorobiphenyl

R.T.: 10.771 min
Delta R.T.: 0.006 min
Response: 3879858
Conc: 50.40 ng/ml m

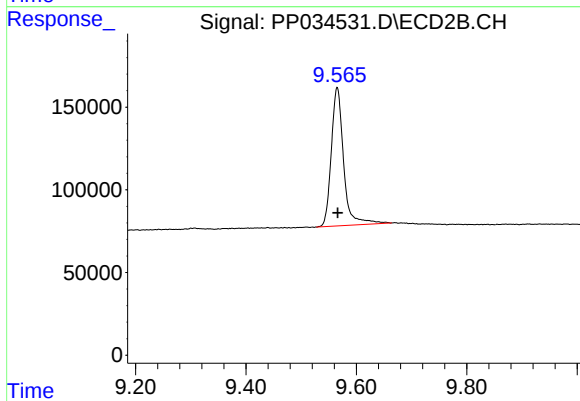

#2 Decachlorobiphenyl

R.T.: 9.565 min
Delta R.T.: -0.001 min
Response: 1295946
Conc: 45.90 ng/ml m

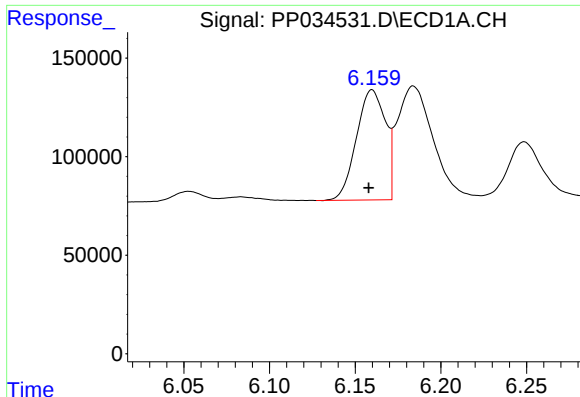


#21 AR-1248-1

R.T.: 6.160 min
Delta R.T.: 0.002 min
Response: 659022
Conc: 463.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:10 AM

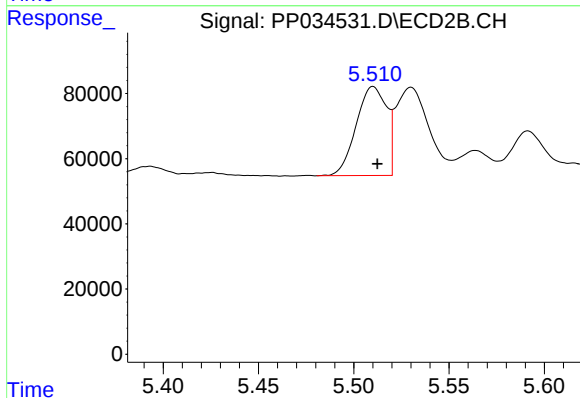


#21 AR-1248-1

R.T.: 5.510 min
Delta R.T.: -0.002 min
Response: 303505
Conc: 416.03 ng/ml

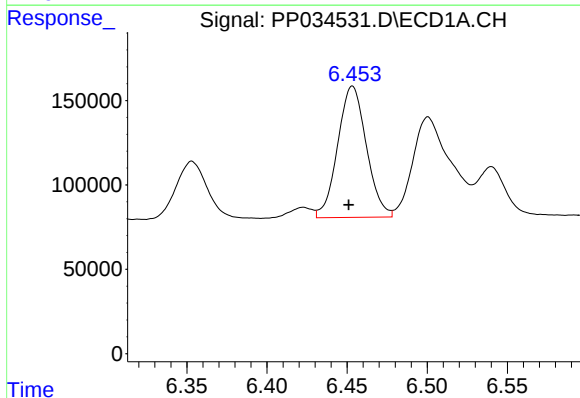


#22 AR-1248-2

R.T.: 6.453 min
Delta R.T.: 0.002 min
Response: 971864
Conc: 491.11 ng/ml

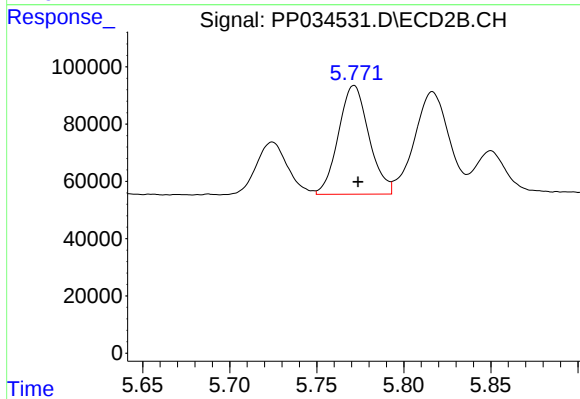

#22 AR-1248-2

R.T.: 5.771 min
Delta R.T.: -0.002 min
Response: 463736
Conc: 451.76 ng/ml

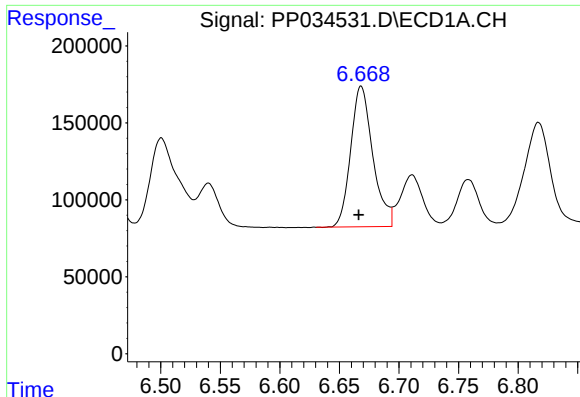


#23 AR-1248-3

R.T.: 6.668 min
Delta R.T.: 0.002 min
Response: 1181764
Conc: 497.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:10 AM

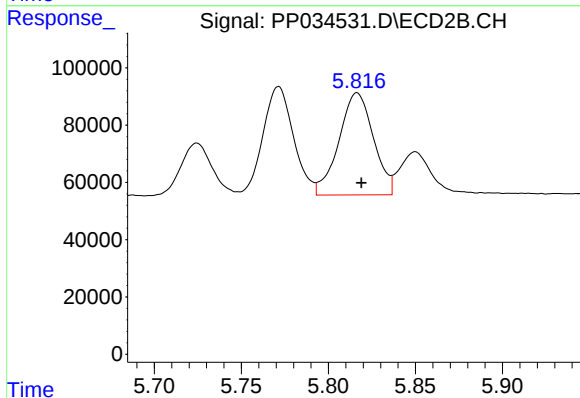


#23 AR-1248-3

R.T.: 5.816 min
Delta R.T.: -0.002 min
Response: 493058
Conc: 449.87 ng/ml

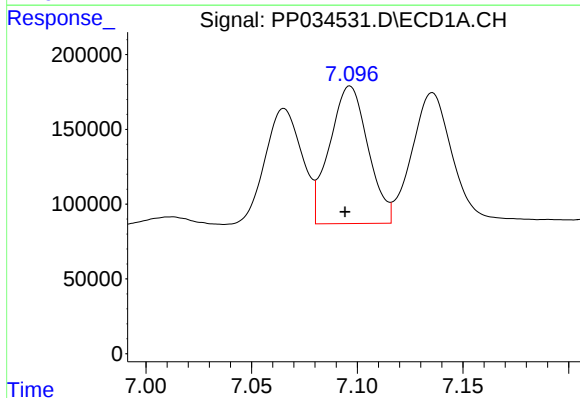


#24 AR-1248-4

R.T.: 7.097 min
Delta R.T.: 0.002 min
Response: 1165985
Conc: 456.91 ng/ml

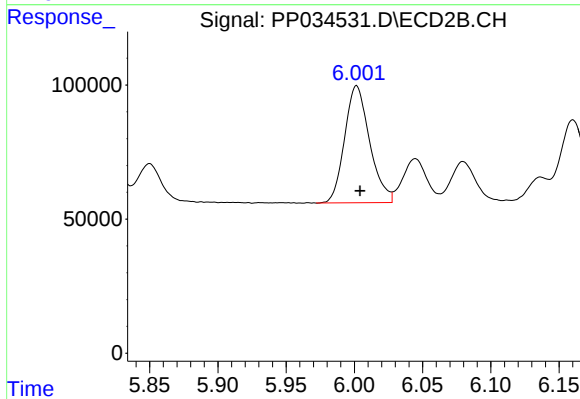

#24 AR-1248-4

R.T.: 6.002 min
Delta R.T.: -0.002 min
Response: 558551
Conc: 442.55 ng/ml

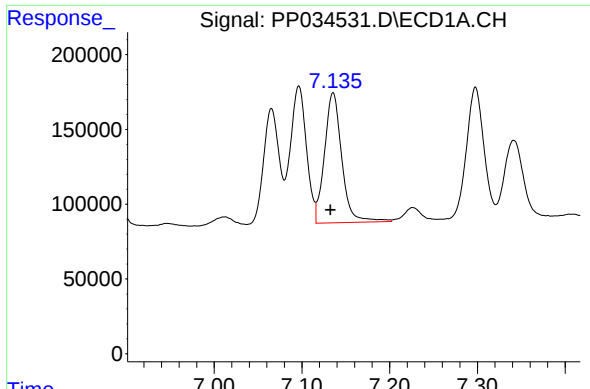


#25 AR-1248-5

R.T.: 7.136 min
Delta R.T.: 0.003 min
Response: 1188910
Conc: 466.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:10 AM

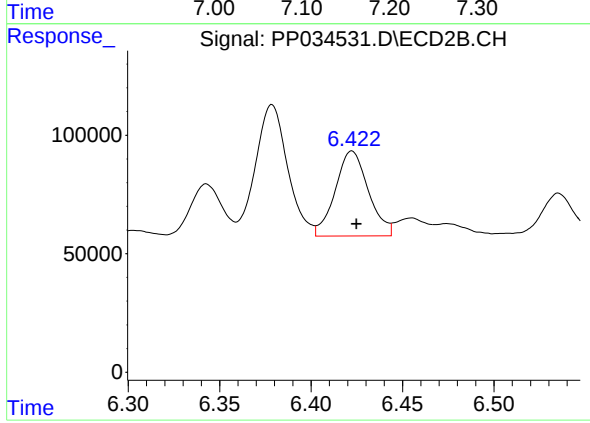

#25 AR-1248-5

R.T.: 6.422 min
Delta R.T.: -0.002 min
Response: 452931
Conc: 400.77 ng/ml