

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
 Data File : PP034534.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2021 13:13
 Operator : DD\AJ
 Sample : M1873-09 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TOTE-COMP

Manual Integrations
 APPROVED

Ankita
 4/2/2021 11:29:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 14:59:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.845	4.256	187721	113270	2.461	2.521m
2) SA Decachlor...	10.770	9.564	188103	63994	2.444	2.266

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
Data File : PP034534.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2021 13:13
Operator : DD\AJ
Sample : M1873-09 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 14:59:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

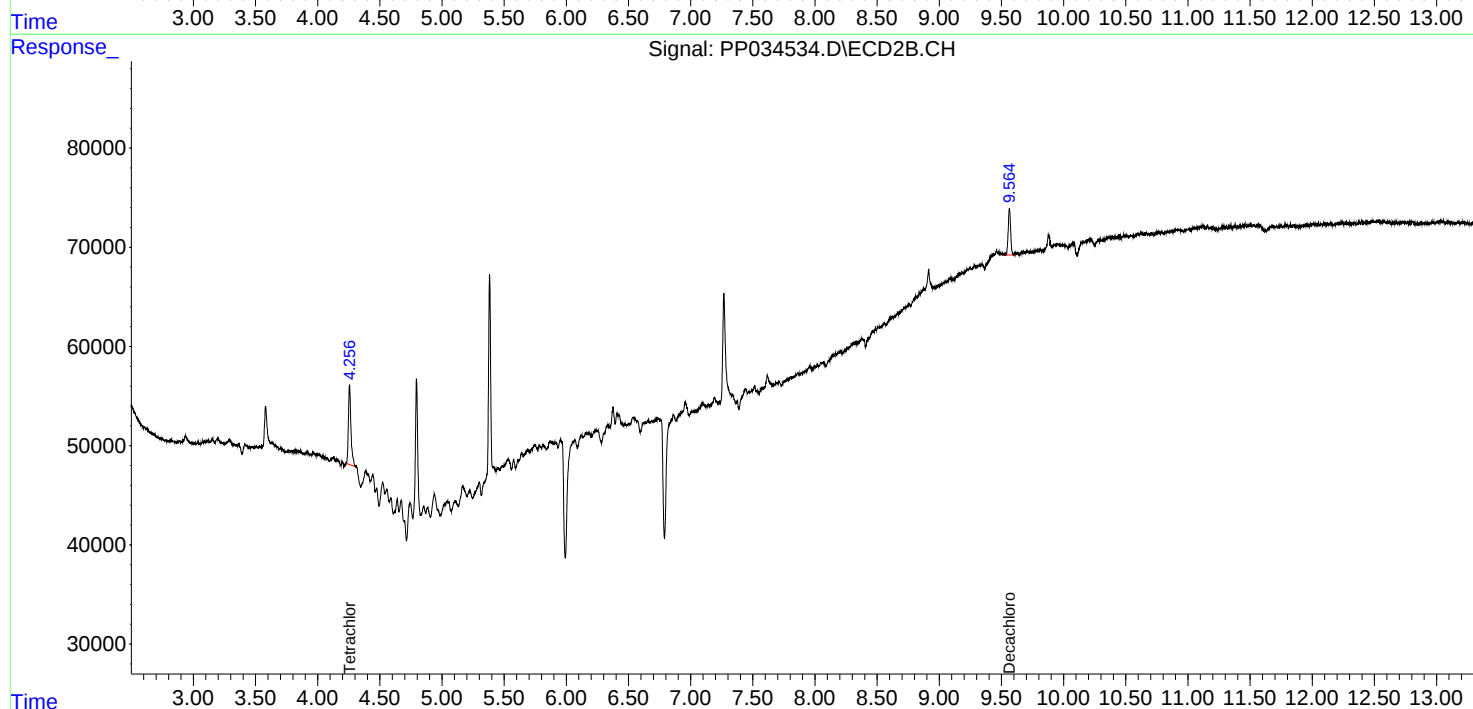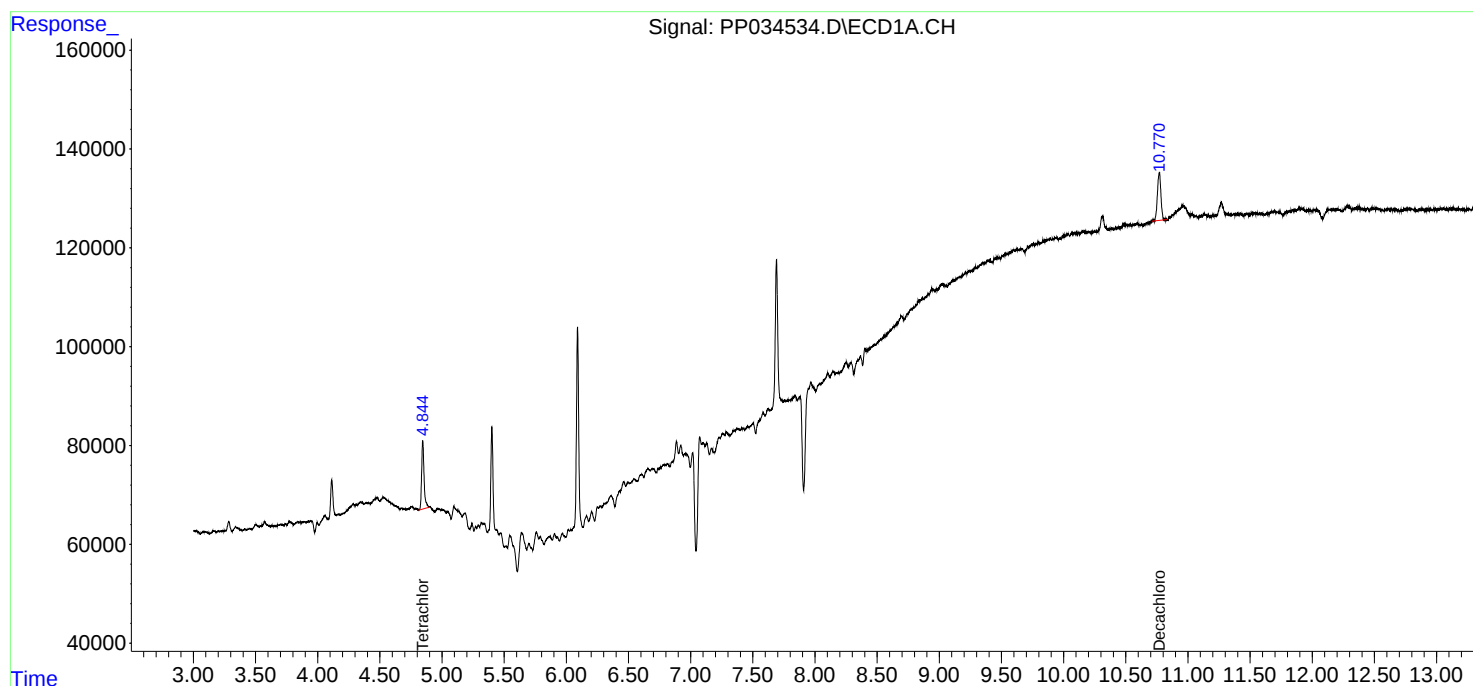

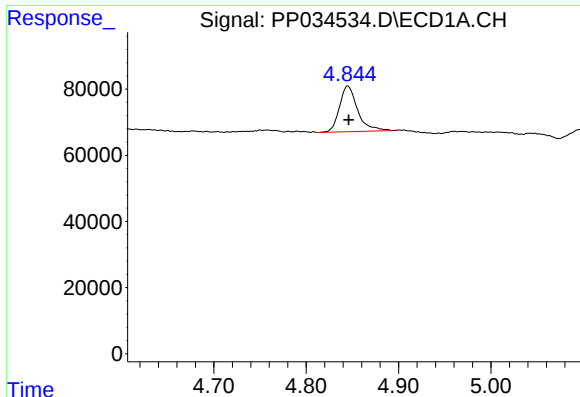


#1 Tetrachloro-m-xylene

R.T.: 4.845 min
Delta R.T.: -0.001 min
Response: 187721
Conc: 2.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:14 AM

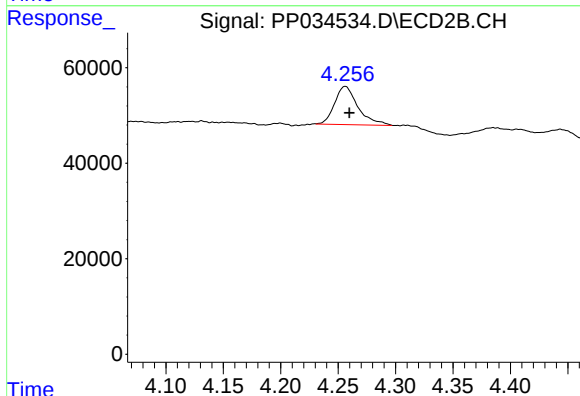


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: -0.004 min
Response: 113270
Conc: 2.52 ng/ml m

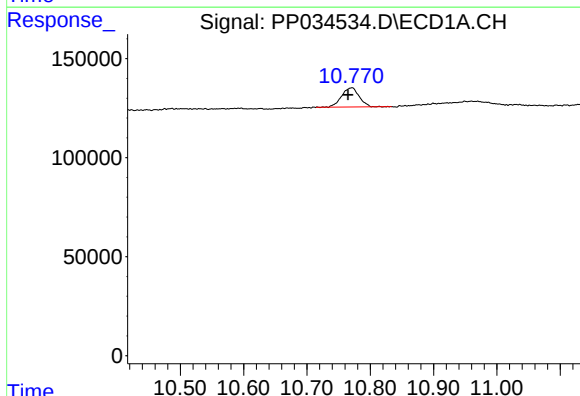

#2 Decachlorobiphenyl

R.T.: 10.770 min
Delta R.T.: 0.005 min
Response: 188103
Conc: 2.44 ng/ml

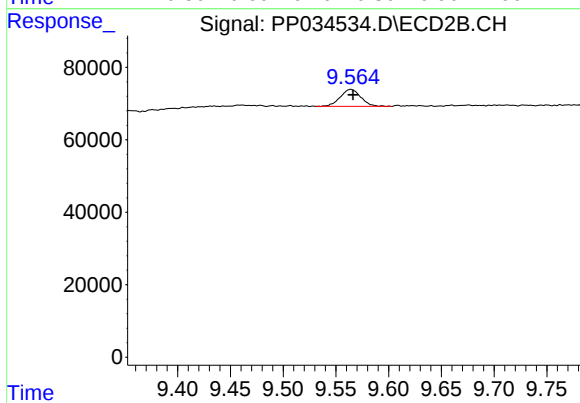

#2 Decachlorobiphenyl

R.T.: 9.564 min
Delta R.T.: -0.002 min
Response: 63994
Conc: 2.27 ng/ml