

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
 Data File : PP034536.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2021 13:47
 Operator : DD\AJ
 Sample : M1865-06DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-030321-SR-06DL

Manual Integrations
 APPROVED

Ankita
 4/2/2021 11:29:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 14:59:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.845	4.256	337251	196968	4.421	4.385
2)	SA Decachlor...	10.767	9.563	313212	137307	4.069m	4.863
Target Compounds							
26)	L6 AR-1254-1	7.063	6.378	2391635	1430996	869.834	775.647
27)	L6 AR-1254-2	7.292	6.536	3359739	1070847	790.130	669.326
28)	L6 AR-1254-3	7.673	6.956	3036249	1421760	665.234	569.670
29)	L6 AR-1254-4	7.968	7.192	1487680	568897	481.160	432.772
30)	L6 AR-1254-5	8.396	7.618	1404115	811500	395.099	399.276

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
Data File : PP034536.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2021 13:47
Operator : DD\AJ
Sample : M1865-06DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 14:59:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

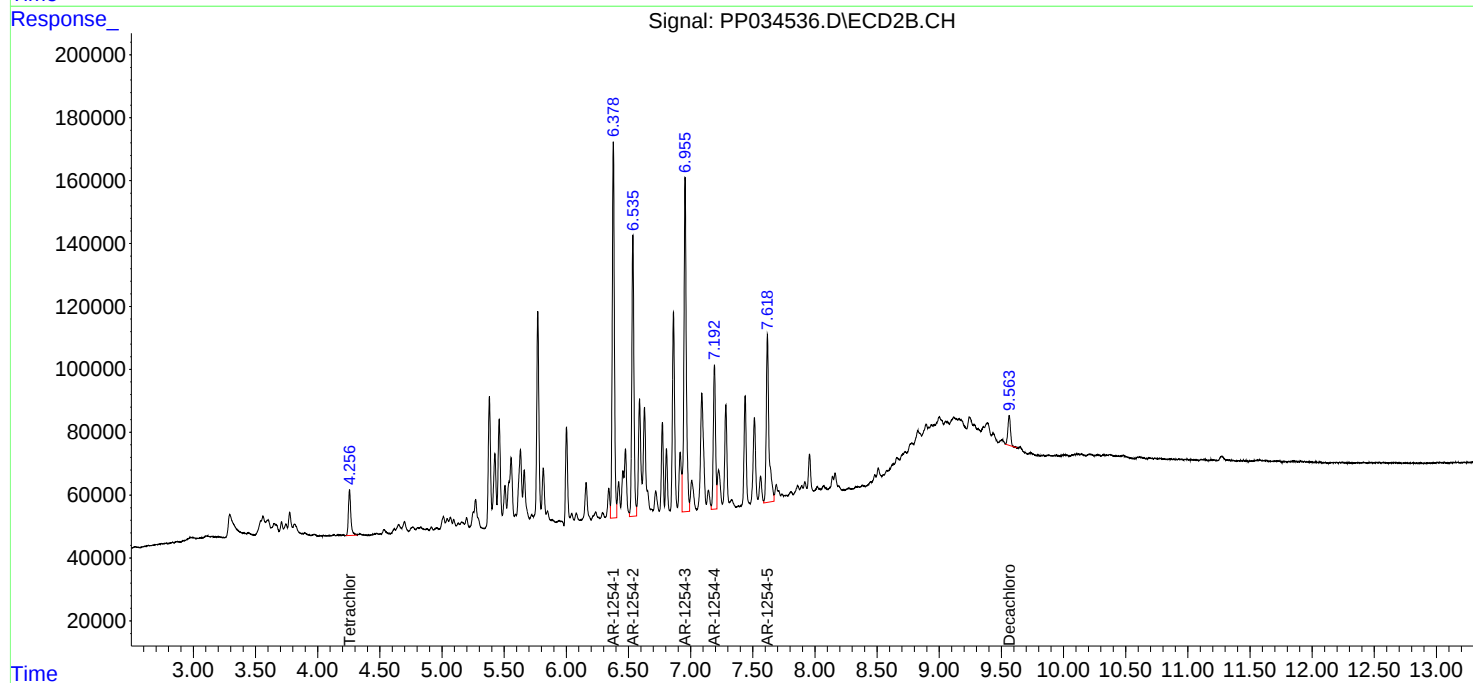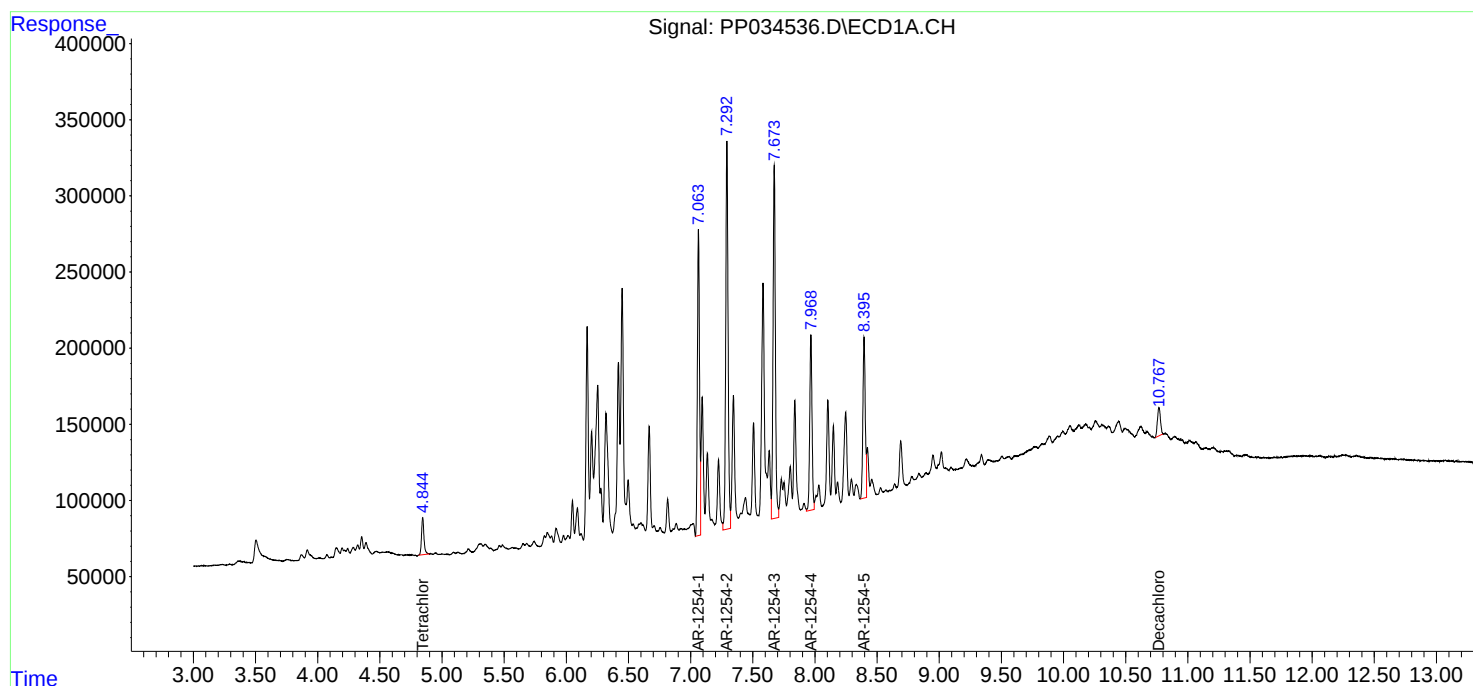

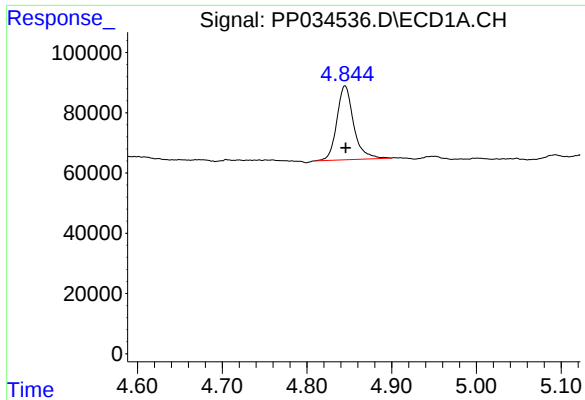


#1 Tetrachloro-m-xylene

R.T.: 4.845 min
Delta R.T.: -0.001 min
Response: 337251
Conc: 4.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:16 AM

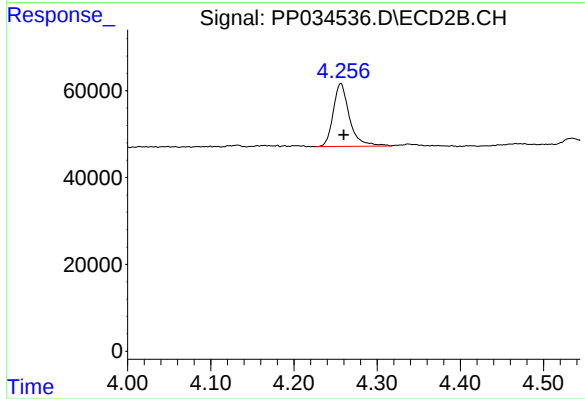


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: -0.003 min
Response: 196968
Conc: 4.38 ng/ml

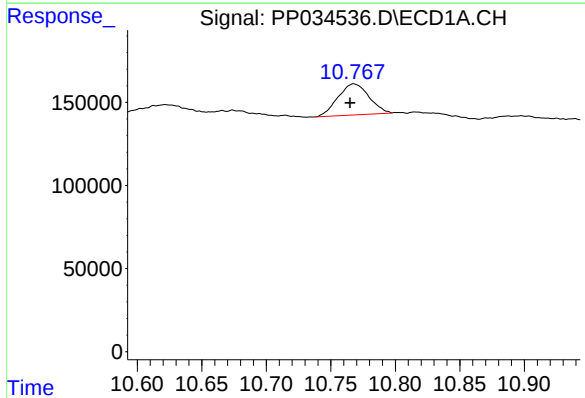


#2 Decachlorobiphenyl

R.T.: 10.767 min
Delta R.T.: 0.002 min
Response: 313212
Conc: 4.07 ng/ml m

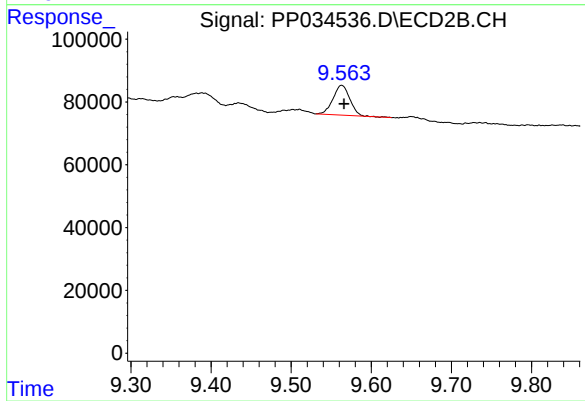

#2 Decachlorobiphenyl

R.T.: 9.563 min
Delta R.T.: -0.003 min
Response: 137307
Conc: 4.86 ng/ml

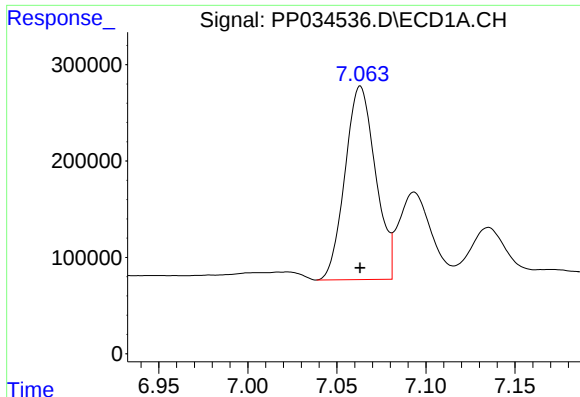


#26 AR-1254-1

R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 2391635
Conc: 869.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:16 AM

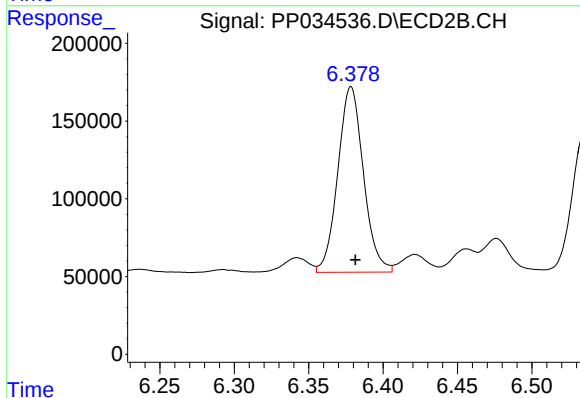


#26 AR-1254-1

R.T.: 6.378 min
Delta R.T.: -0.003 min
Response: 1430996
Conc: 775.65 ng/ml

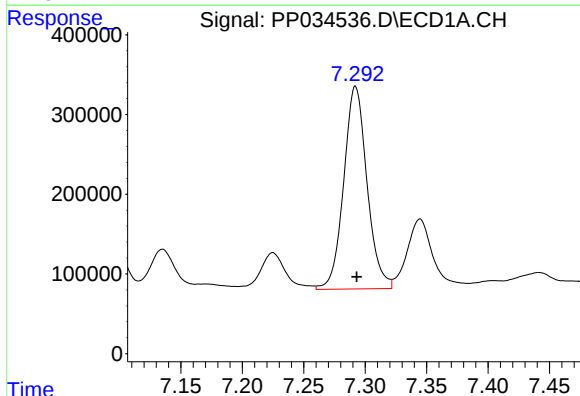


#27 AR-1254-2

R.T.: 7.292 min
Delta R.T.: 0.000 min
Response: 3359739
Conc: 790.13 ng/ml

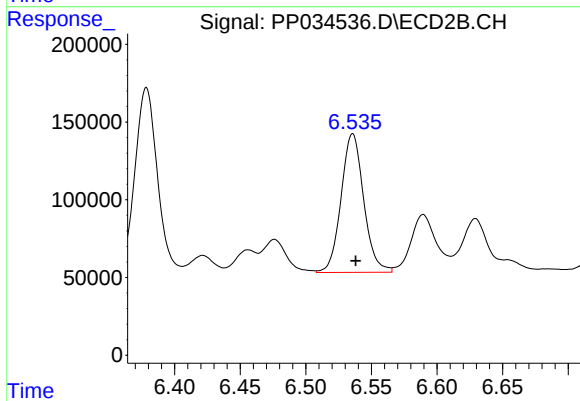

#27 AR-1254-2

R.T.: 6.536 min
Delta R.T.: -0.002 min
Response: 1070847
Conc: 669.33 ng/ml

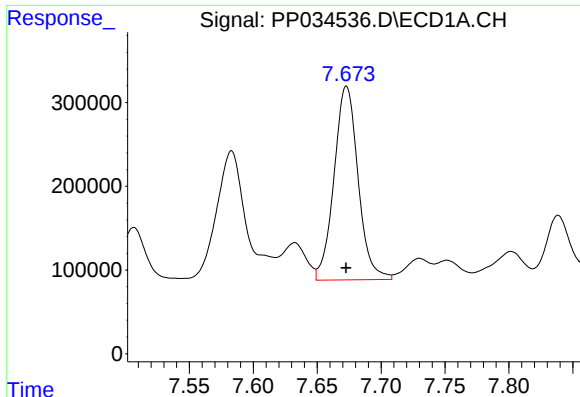


#28 AR-1254-3

R.T.: 7.673 min
Delta R.T.: 0.000 min
Response: 3036249
Conc: 665.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:16 AM

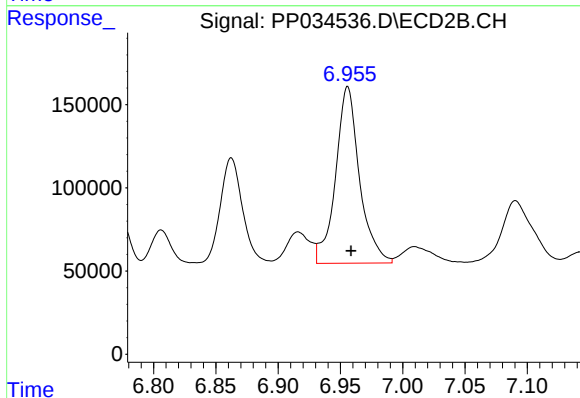


#28 AR-1254-3

R.T.: 6.956 min
Delta R.T.: -0.003 min
Response: 1421760
Conc: 569.67 ng/ml

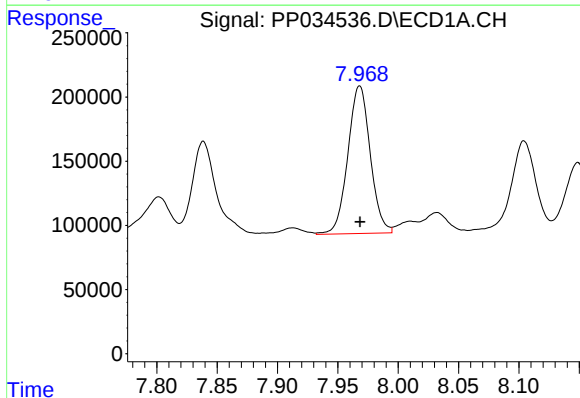


#29 AR-1254-4

R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 1487680
Conc: 481.16 ng/ml

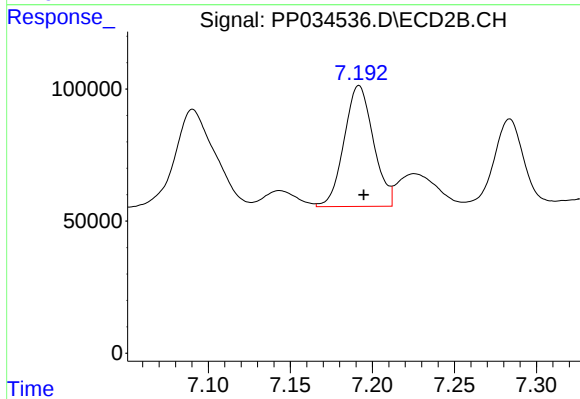

#29 AR-1254-4

R.T.: 7.192 min
Delta R.T.: -0.003 min
Response: 568897
Conc: 432.77 ng/ml

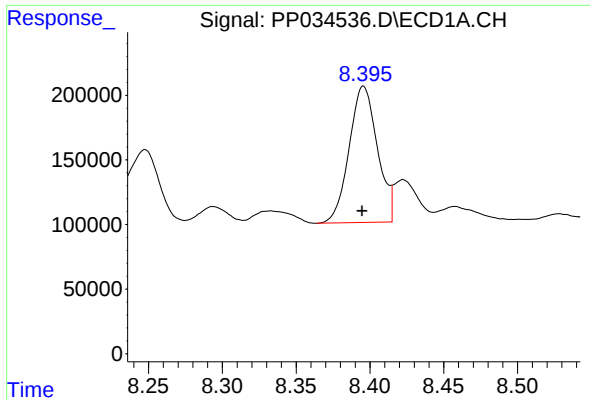


#30 AR-1254-5

R.T.: 8.396 min
Delta R.T.: 0.000 min
Response: 1404115
Conc: 395.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-030321-SR-06DL

Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:16 AM

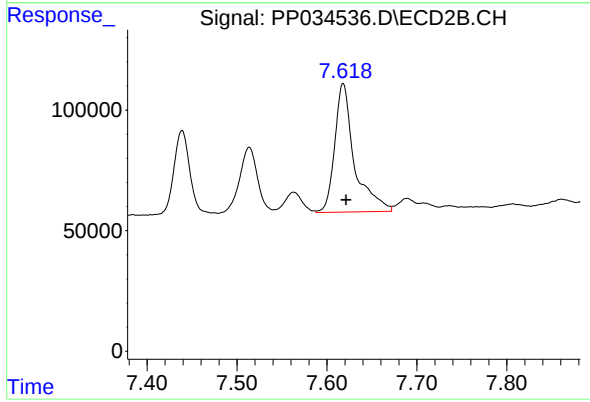

#30 AR-1254-5

R.T.: 7.618 min
Delta R.T.: -0.003 min
Response: 811500
Conc: 399.28 ng/ml