

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
 Data File : PP034565.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Apr 2021 22:31
 Operator : DD\AJ
 Sample : M1854-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-1D-(4-10)

Manual Integrations
 APPROVED

Ankita
 4/2/2021 11:29:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 03:01:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.844	4.257	1731469	937995	22.698	20.880
2)	SA Decachlor...	10.764	9.562	1586629	544961	20.611	19.300
Target Compounds							
31)	L7 AR-1260-1	7.836	7.089	233844	111905	75.329	72.871m
32)	L7 AR-1260-2	8.101	7.281	829738	76906	220.944	42.574m#
33)	L7 AR-1260-3	8.466	7.438	162523	97814	53.767	56.381m
34)	L7 AR-1260-4	8.695	7.918	307763	94435	88.153	65.865 #
35)	L7 AR-1260-5	9.015	8.162	495904	247940	69.245	72.583

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
Data File : PP034565.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Apr 2021 22:31
Operator : DD\AJ
Sample : M1854-05
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
TP-1D-(4-10)


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 03:01:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

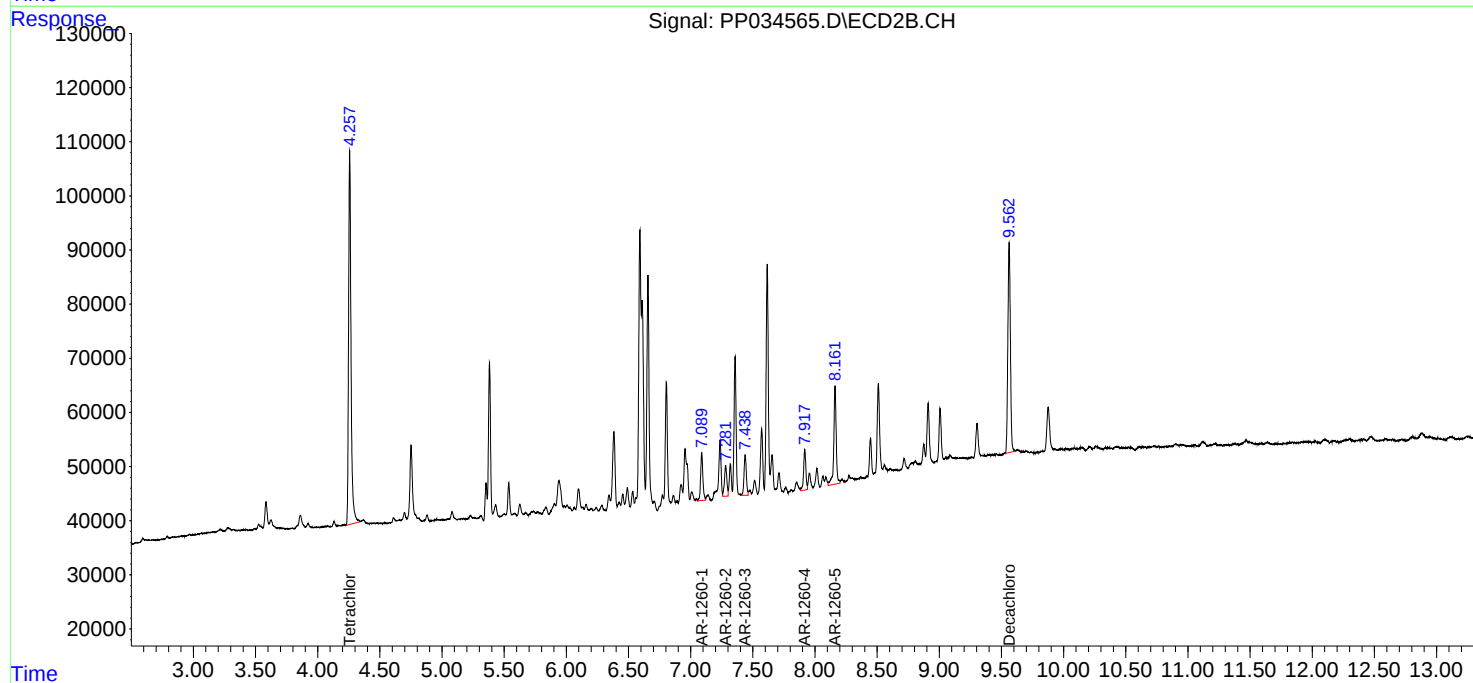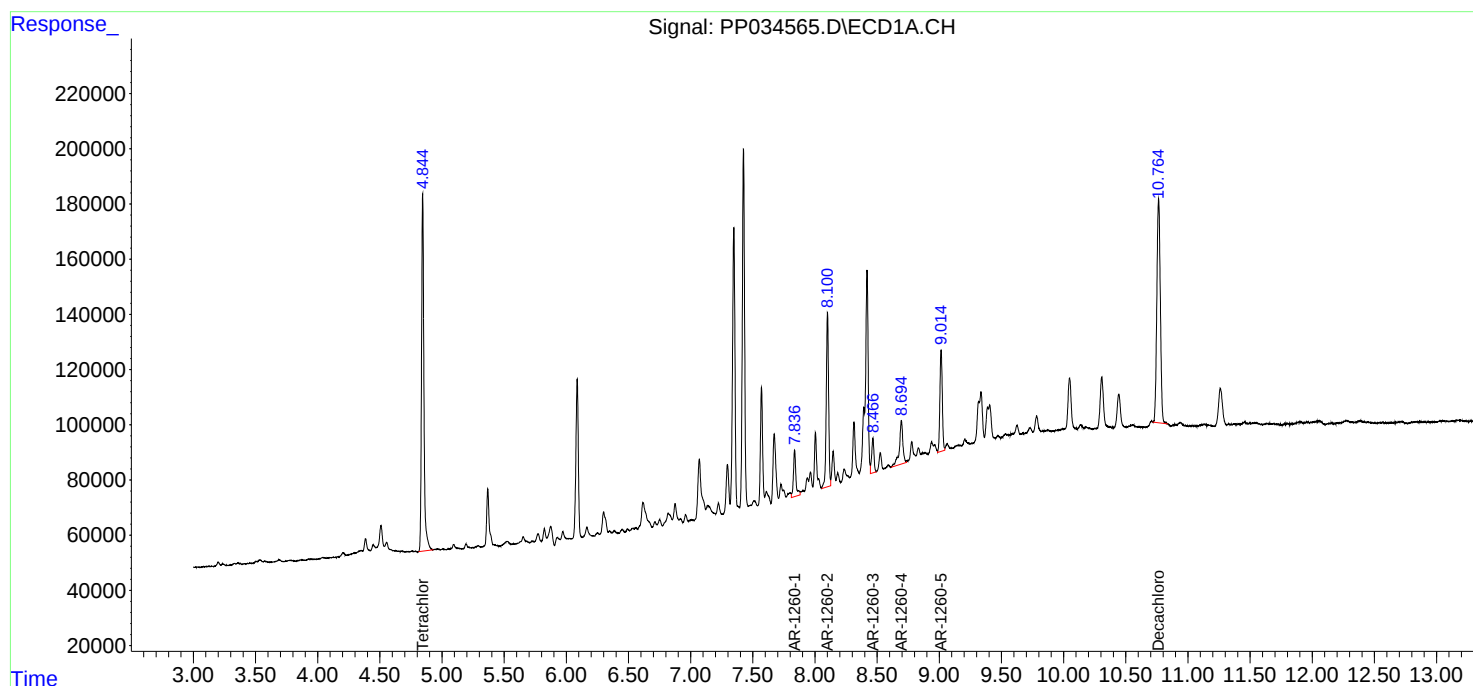

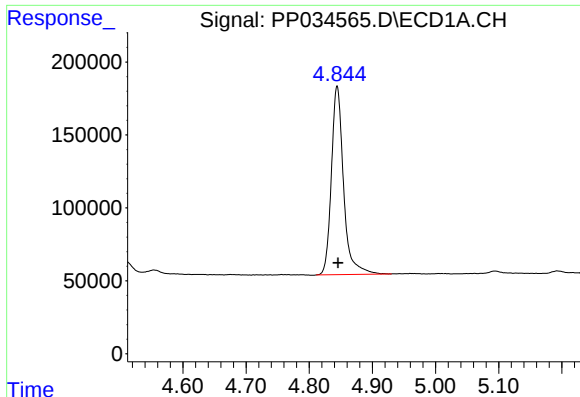


#1 Tetrachloro-m-xylene

R.T.: 4.844 min
Delta R.T.: -0.002 min
Response: 1731469
Conc: 22.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1D-(4-10)


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:34 AM

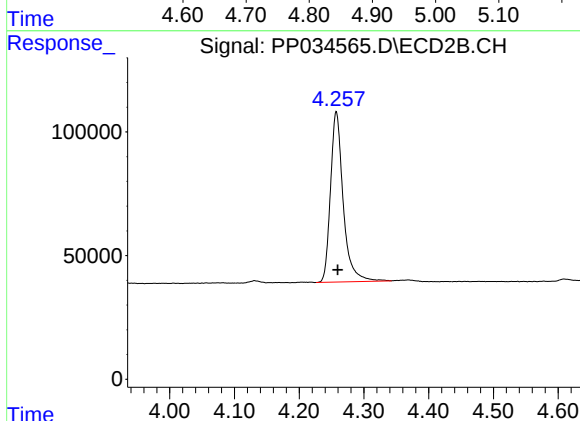


#1 Tetrachloro-m-xylene

R.T.: 4.257 min
Delta R.T.: -0.002 min
Response: 937995
Conc: 20.88 ng/ml

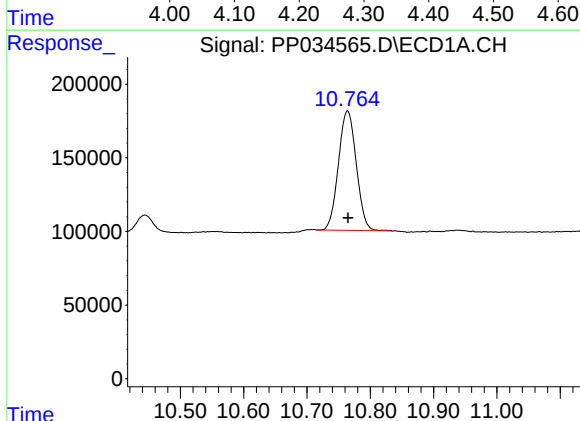


#2 Decachlorobiphenyl

R.T.: 10.764 min
Delta R.T.: 0.000 min
Response: 1586629
Conc: 20.61 ng/ml

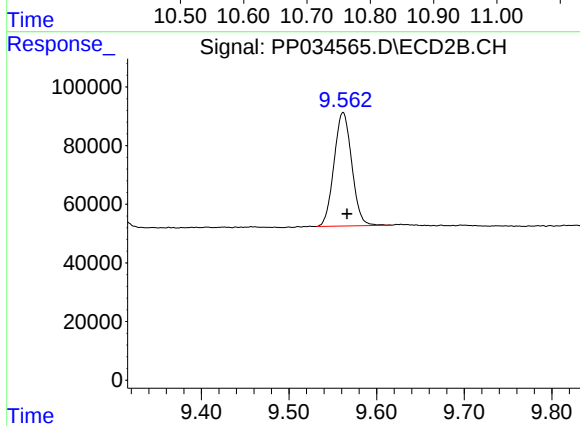

#2 Decachlorobiphenyl

R.T.: 9.562 min
Delta R.T.: -0.004 min
Response: 544961
Conc: 19.30 ng/ml

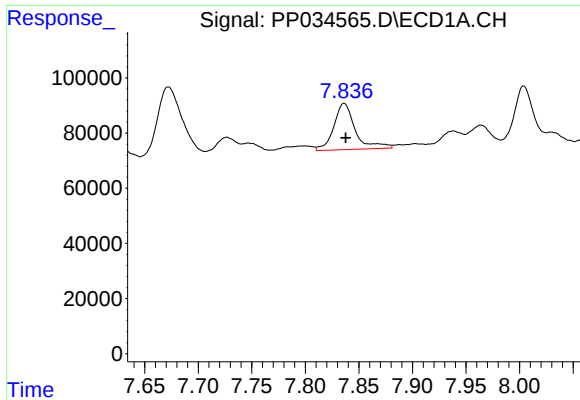


#31 AR-1260-1

R.T.: 7.836 min
Delta R.T.: -0.001 min
Response: 233844
Conc: 75.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1D-(4-10)


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:34 AM

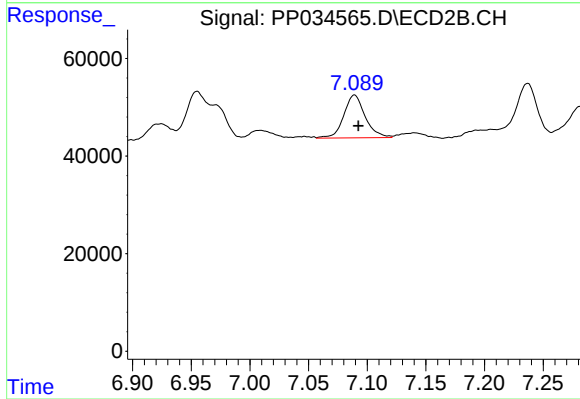


#31 AR-1260-1

R.T.: 7.089 min
Delta R.T.: -0.004 min
Response: 111905
Conc: 72.87 ng/ml m

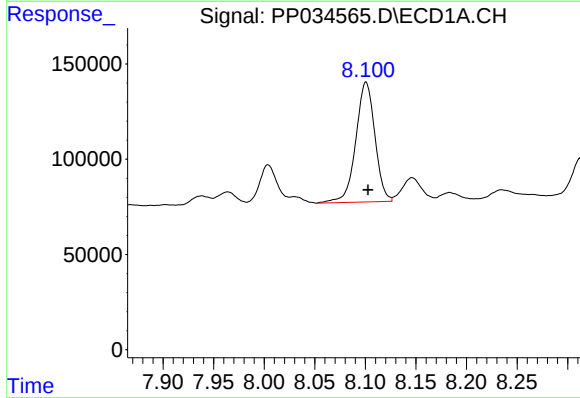


#32 AR-1260-2

R.T.: 8.101 min
Delta R.T.: -0.002 min
Response: 829738
Conc: 220.94 ng/ml

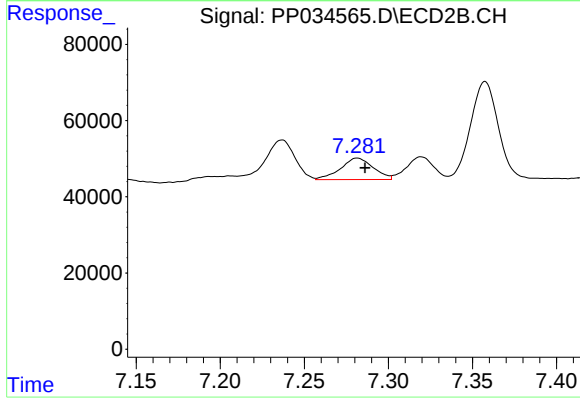

#32 AR-1260-2

R.T.: 7.281 min
Delta R.T.: -0.005 min
Response: 76906
Conc: 42.57 ng/ml m

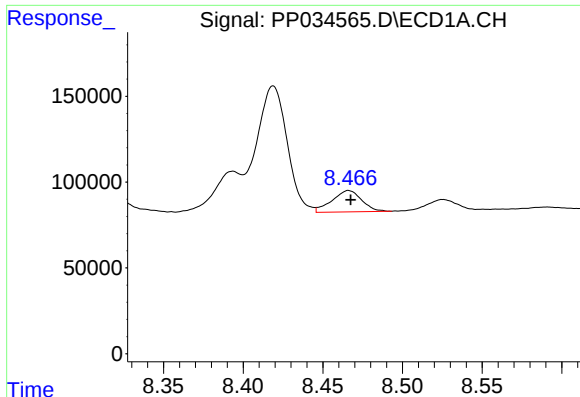


#33 AR-1260-3

R.T.: 8.466 min
Delta R.T.: -0.001 min
Response: 162523
Conc: 53.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1D-(4-10)


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:34 AM

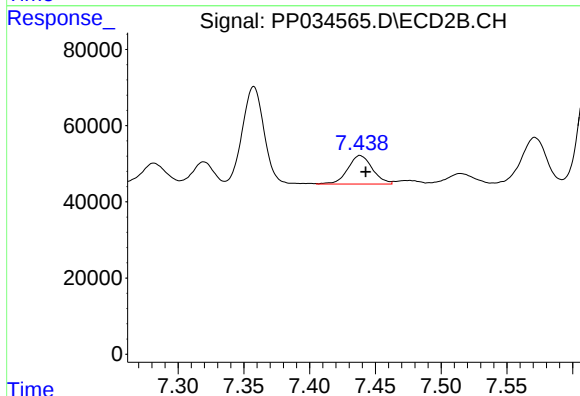


#33 AR-1260-3

R.T.: 7.438 min
Delta R.T.: -0.005 min
Response: 97814
Conc: 56.38 ng/ml m

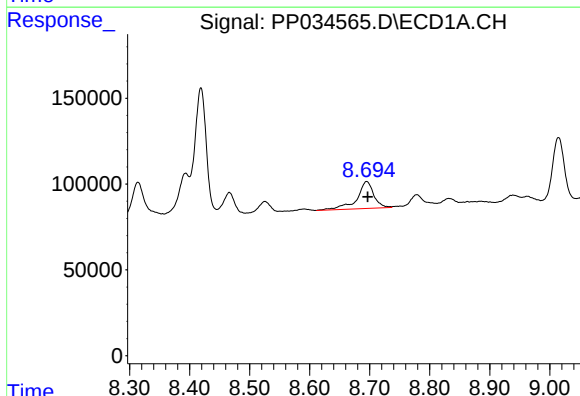


#34 AR-1260-4

R.T.: 8.695 min
Delta R.T.: -0.002 min
Response: 307763
Conc: 88.15 ng/ml

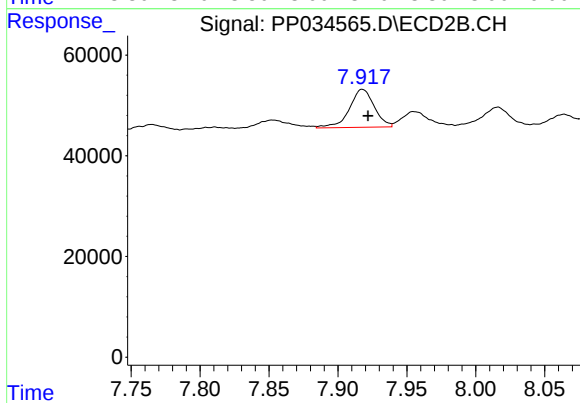

#34 AR-1260-4

R.T.: 7.918 min
Delta R.T.: -0.004 min
Response: 94435
Conc: 65.86 ng/ml

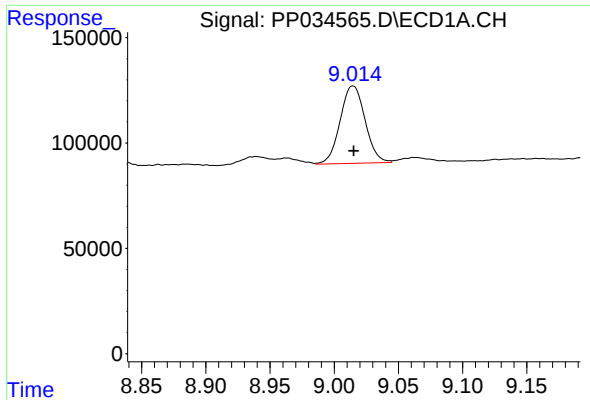


#35 AR-1260-5

R.T.: 9.015 min
Delta R.T.: 0.000 min
Response: 495904
Conc: 69.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1D-(4-10)

Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:34 AM

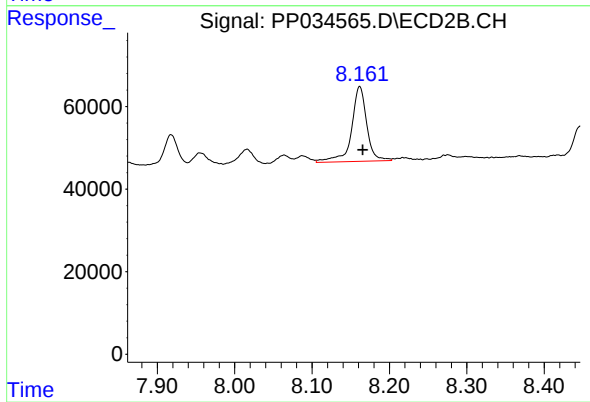

#35 AR-1260-5

R.T.: 8.162 min
Delta R.T.: -0.004 min
Response: 247940
Conc: 72.58 ng/ml