

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
 Data File : PP034584.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2021 4:25
 Operator : DD\AJ
 Sample : M1886-07
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RO-124037

Manual Integrations
 APPROVED

Ankita
 4/2/2021 11:29:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 02 06:45:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.842	4.254	1300383	774392	17.047m	17.238m
2)	SA Decachlor...	10.763	9.560	984012	340620	12.783	12.063
Target Compounds							
26)	L6 AR-1254-1	7.059	6.376	56239	37326	20.454m	20.232m
27)	L6 AR-1254-2	7.290	6.532	139161	48449	32.727m	30.283m
28)	L6 AR-1254-3	7.671	6.952	105437	86337	23.101m	34.593m#
29)	L6 AR-1254-4	7.964	7.188	115461	63857	37.343m	48.577m#
30)	L6 AR-1254-5	8.392	7.615	161697	122138	45.499m	60.095m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040121\
Data File : PP034584.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2021 4:25
Operator : DD\AJ
Sample : M1886-07
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
RO-124037


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 02 06:45:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

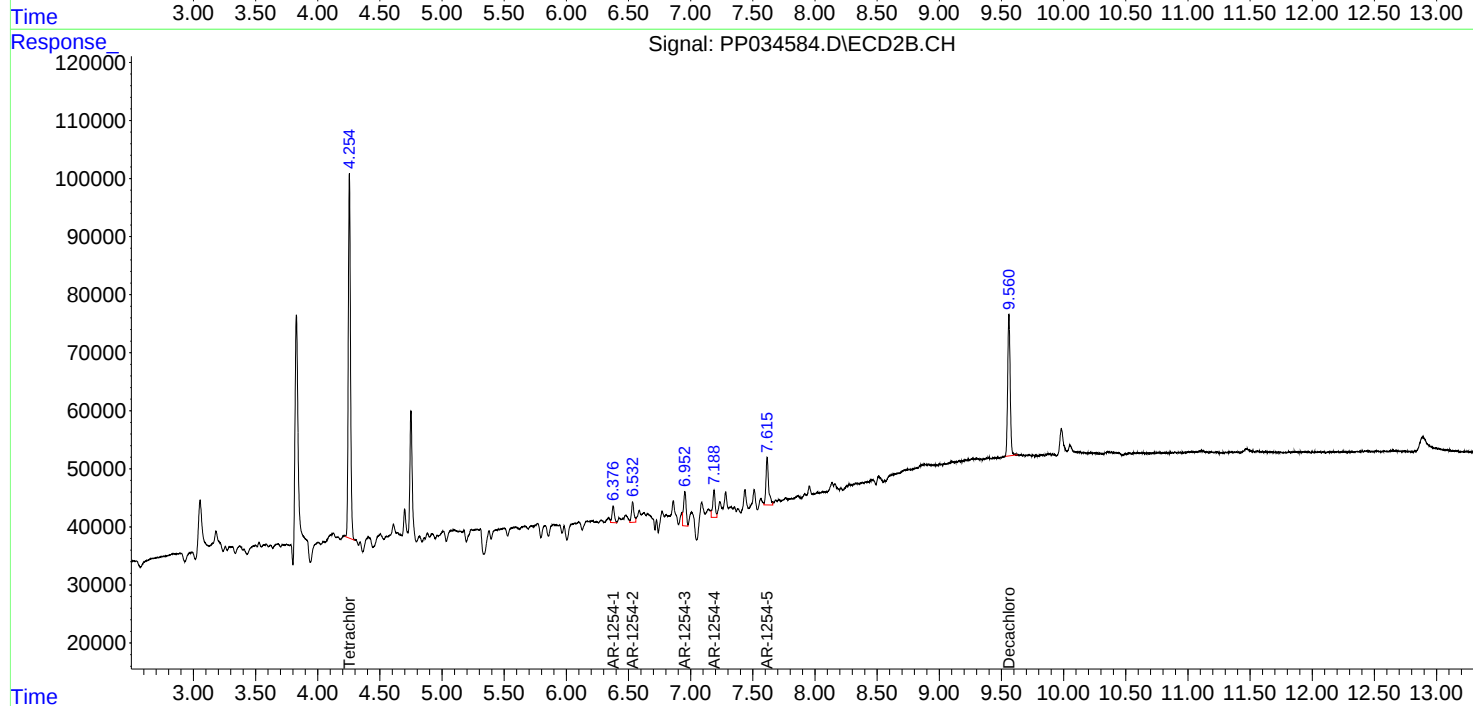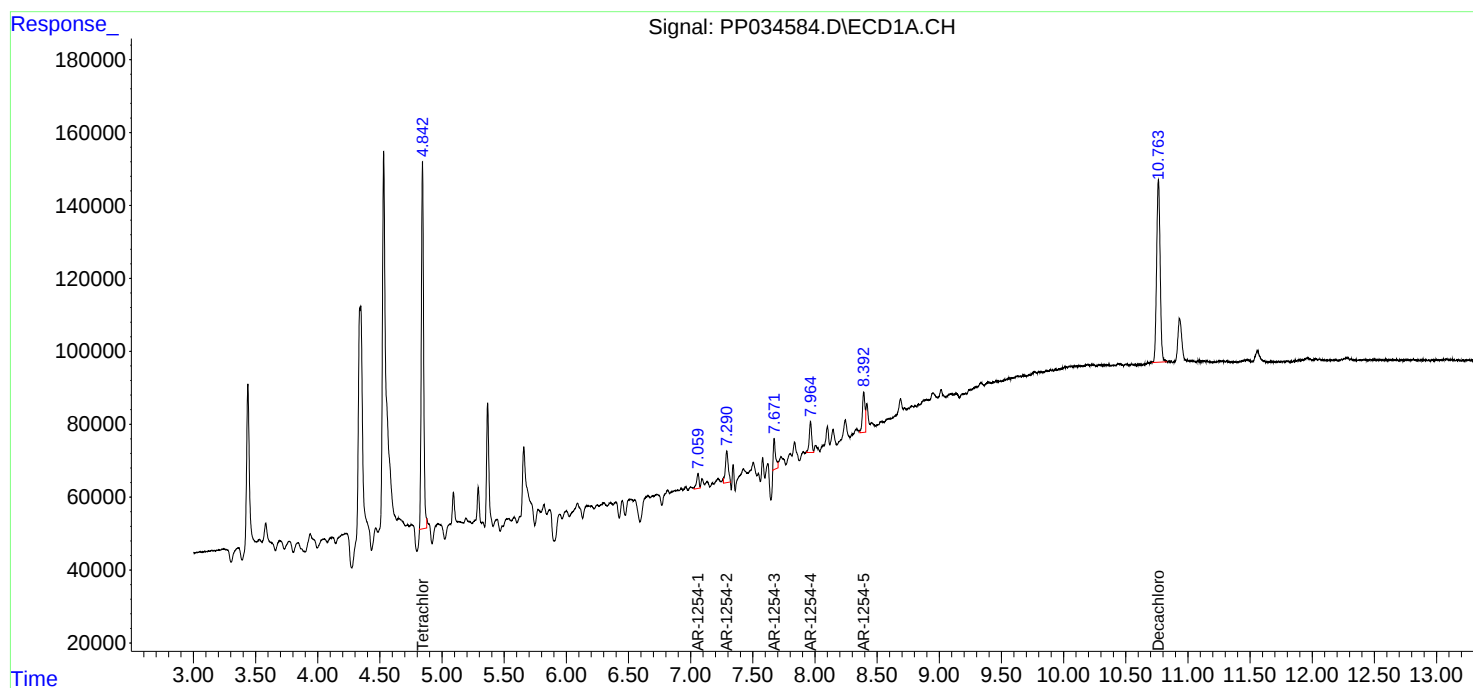

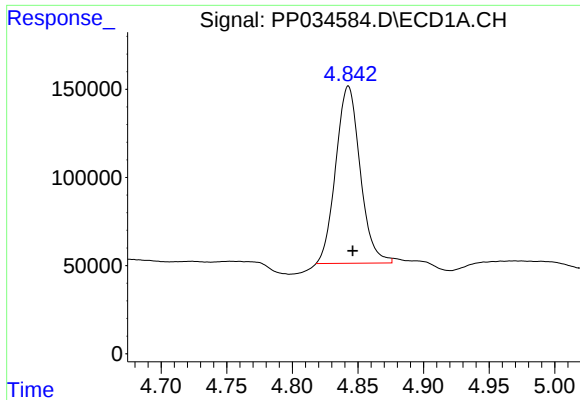


#1 Tetrachloro-m-xylene

R.T.: 4.842 min
Delta R.T.: -0.004 min
Response: 1300383
Conc: 17.05 ng/ml m

Instrument :
ECD_P
ClientSampleId :
RO-124037


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:37 AM

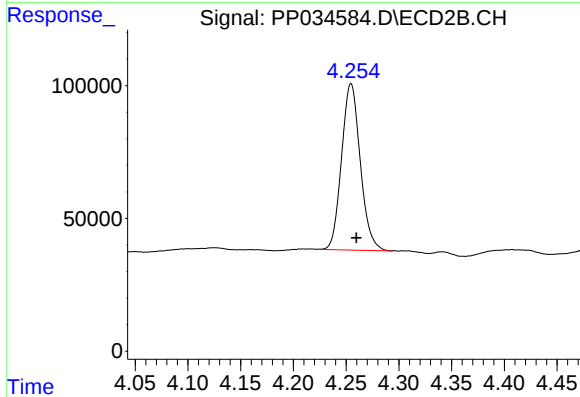


#1 Tetrachloro-m-xylene

R.T.: 4.254 min
Delta R.T.: -0.006 min
Response: 774392
Conc: 17.24 ng/ml m

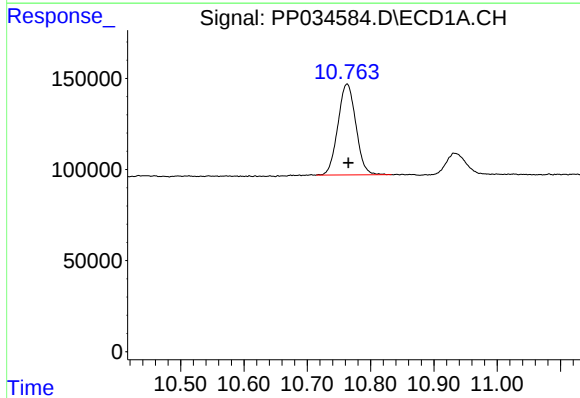


#2 Decachlorobiphenyl

R.T.: 10.763 min
Delta R.T.: -0.002 min
Response: 984012
Conc: 12.78 ng/ml

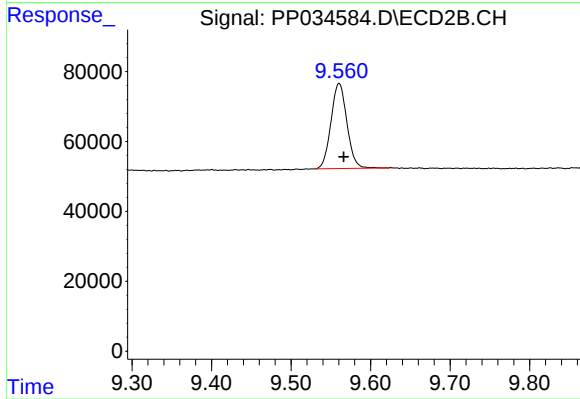

#2 Decachlorobiphenyl

R.T.: 9.560 min
Delta R.T.: -0.006 min
Response: 340620
Conc: 12.06 ng/ml

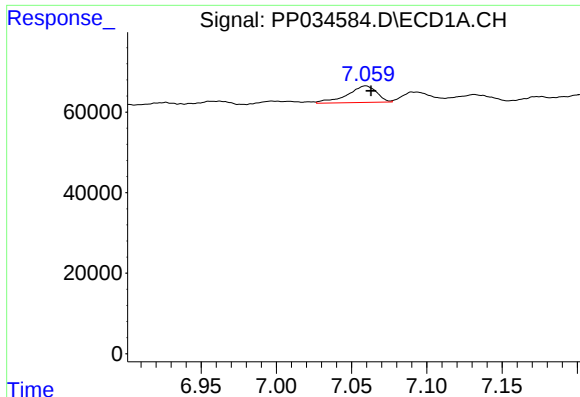


#26 AR-1254-1

R.T.: 7.059 min
Delta R.T.: -0.004 min
Response: 56239
Conc: 20.45 ng/ml m

Instrument :
ECD_P
ClientSampleId :
RO-124037


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:37 AM

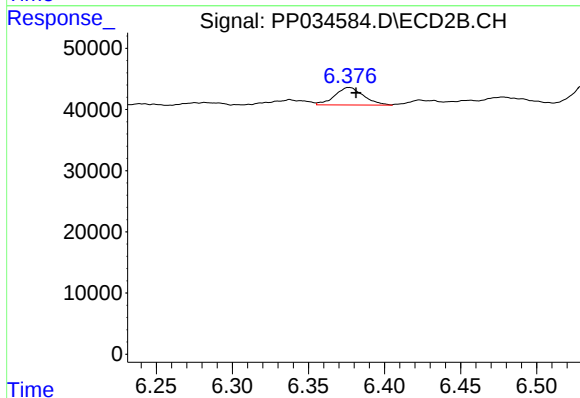


#26 AR-1254-1

R.T.: 6.376 min
Delta R.T.: -0.006 min
Response: 37326
Conc: 20.23 ng/ml m

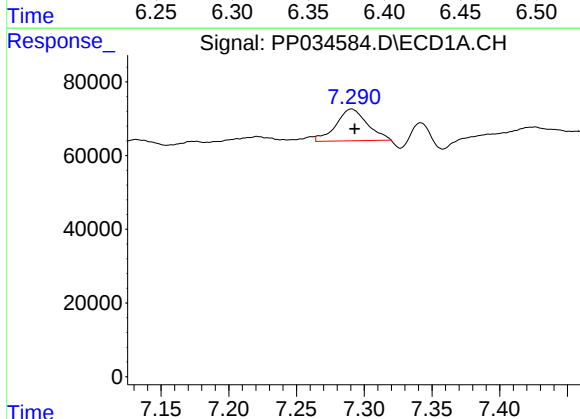


#27 AR-1254-2

R.T.: 7.290 min
Delta R.T.: -0.003 min
Response: 139161
Conc: 32.73 ng/ml m

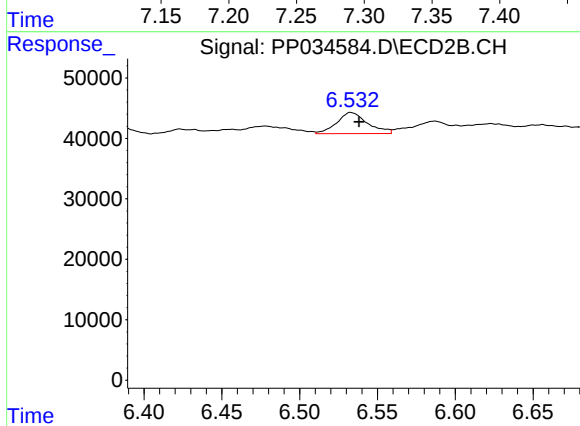

#27 AR-1254-2

R.T.: 6.532 min
Delta R.T.: -0.006 min
Response: 48449
Conc: 30.28 ng/ml m

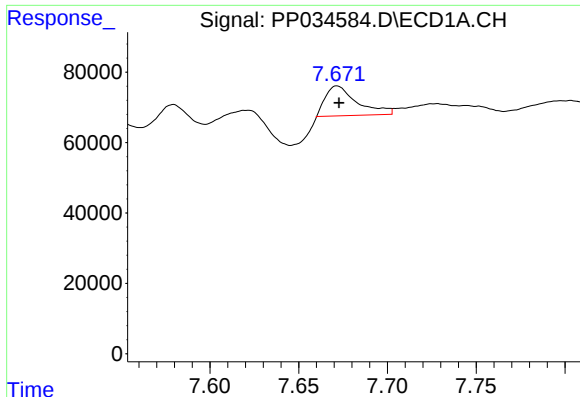


#28 AR-1254-3

R.T.: 7.671 min
Delta R.T.: -0.002 min
Response: 105437
Conc: 23.10 ng/ml m

Instrument :
ECD_P
ClientSampleId :
RO-124037


Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:37 AM

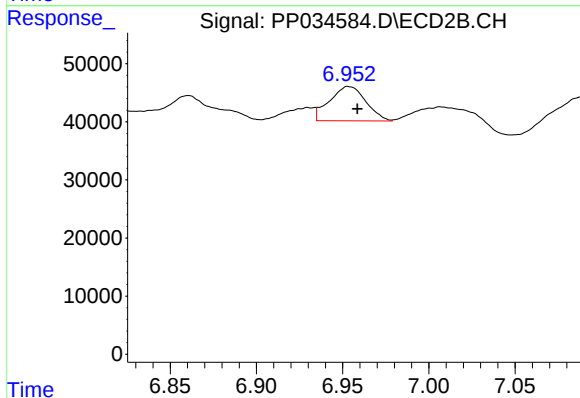


#28 AR-1254-3

R.T.: 6.952 min
Delta R.T.: -0.006 min
Response: 86337
Conc: 34.59 ng/ml m

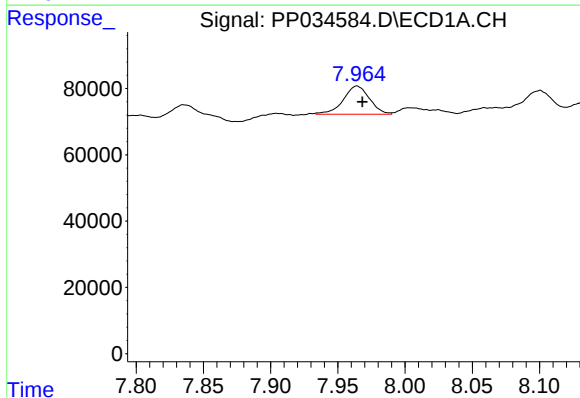


#29 AR-1254-4

R.T.: 7.964 min
Delta R.T.: -0.005 min
Response: 115461
Conc: 37.34 ng/ml m

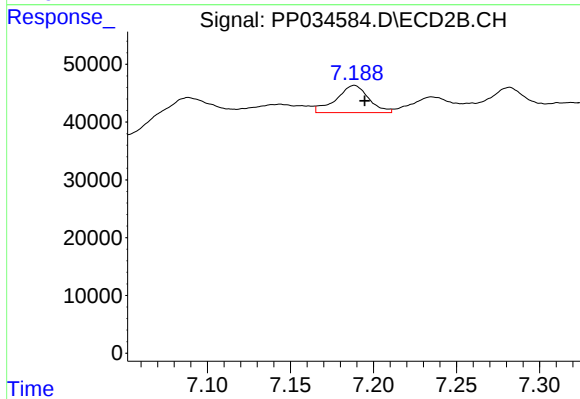

#29 AR-1254-4

R.T.: 7.188 min
Delta R.T.: -0.006 min
Response: 63857
Conc: 48.58 ng/ml m

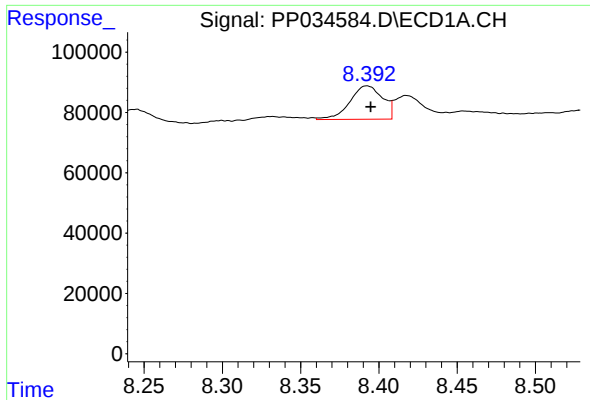


#30 AR-1254-5

R.T.: 8.392 min
Delta R.T.: -0.003 min
Response: 161697
Conc: 45.50 ng/ml m

Instrument :
ECD_P
ClientSampleId :
RO-124037

Manual Integrations
APPROVED

Ankita
4/2/2021 11:29:37 AM

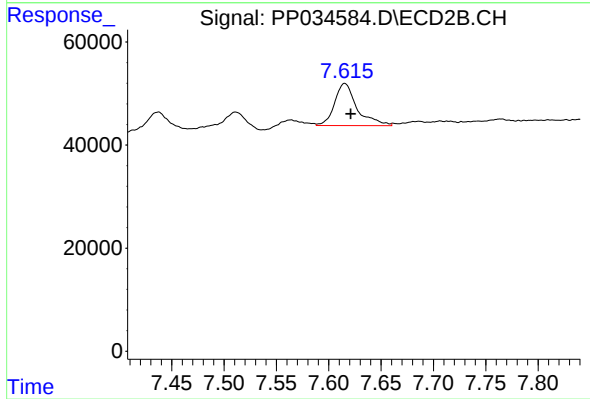

#30 AR-1254-5

R.T.: 7.615 min
Delta R.T.: -0.006 min
Response: 122138
Conc: 60.09 ng/ml m