

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040221\
 Data File : PP034649.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Apr 2021 00:20
 Operator : DD\AJ
 Sample : M1911-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-6S-(0-4)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 02:18:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.845	4.257	1544611	901797	20.248	20.075
2)	SA Decachlor...	10.759	9.557	1405698	507695	18.261	17.980
Target Compounds							
8)	L2 AR-1221-1	5.092	4.530f	148637	7363	203.329	16.224 #
9)	L2 AR-1221-2	5.194	4.643f	12494	5277	21.933	15.124 #
10)	L2 AR-1221-3	5.308f	0.000	31558	0	17.340	N.D. #
11)	L3 AR-1232-1	5.308f	0.000	31558	0	21.248	N.D. #
20)	L4 AR-1242-5	0.000	6.378	0	8030	N.D.	9.793 #
26)	L6 AR-1254-1	0.000	6.378	0	8030	N.D.	4.353 #
27)	L6 AR-1254-2	7.292	6.531	15493	7015	3.644	4.384
28)	L6 AR-1254-3	7.685	6.971	30589	21067	6.702	8.441 #
29)	L6 AR-1254-4	7.968	7.184	4918	7043	1.591	5.357 #
30)	L6 AR-1254-5	8.392	7.613	19070	16998	5.366	8.363 #
31)	L7 AR-1260-1	0.000	7.084	0	5773	N.D.	3.759 #
32)	L7 AR-1260-2	8.100	7.278	59100	15490	15.737	8.575 #
33)	L7 AR-1260-3	8.461	7.442	10006	10023	3.310	5.777 #
34)	L7 AR-1260-4	8.700	7.912	4260	7509	1.220	5.237 #
35)	L7 AR-1260-5	0.000	8.158	0	5698	N.D.	1.668 #
36)	L8 AR-1262-1	8.461	7.613	10006	16998	2.187	15.827 #
37)	L8 AR-1262-2	0.000	8.158	0	5698	N.D.	1.661 #
38)	L8 AR-1262-3	0.000	8.444	0	8974	N.D.	5.989 #
39)	L8 AR-1262-4	9.398	8.507	18950	6442	4.267	2.339 #
41)	L9 AR-1268-1	0.000	8.444	0	8974	N.D.	2.077 #
42)	L9 AR-1268-2	9.398	8.507	18950	6442	1.981	1.556
45)	L9 AR-1268-5	10.437	9.300	22468	22778	0.787	2.193 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040221\
Data File : PP034649.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Apr 2021 00:20
Operator : DD\AJ
Sample : M1911-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
TP-6S-(0-4)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 02:18:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

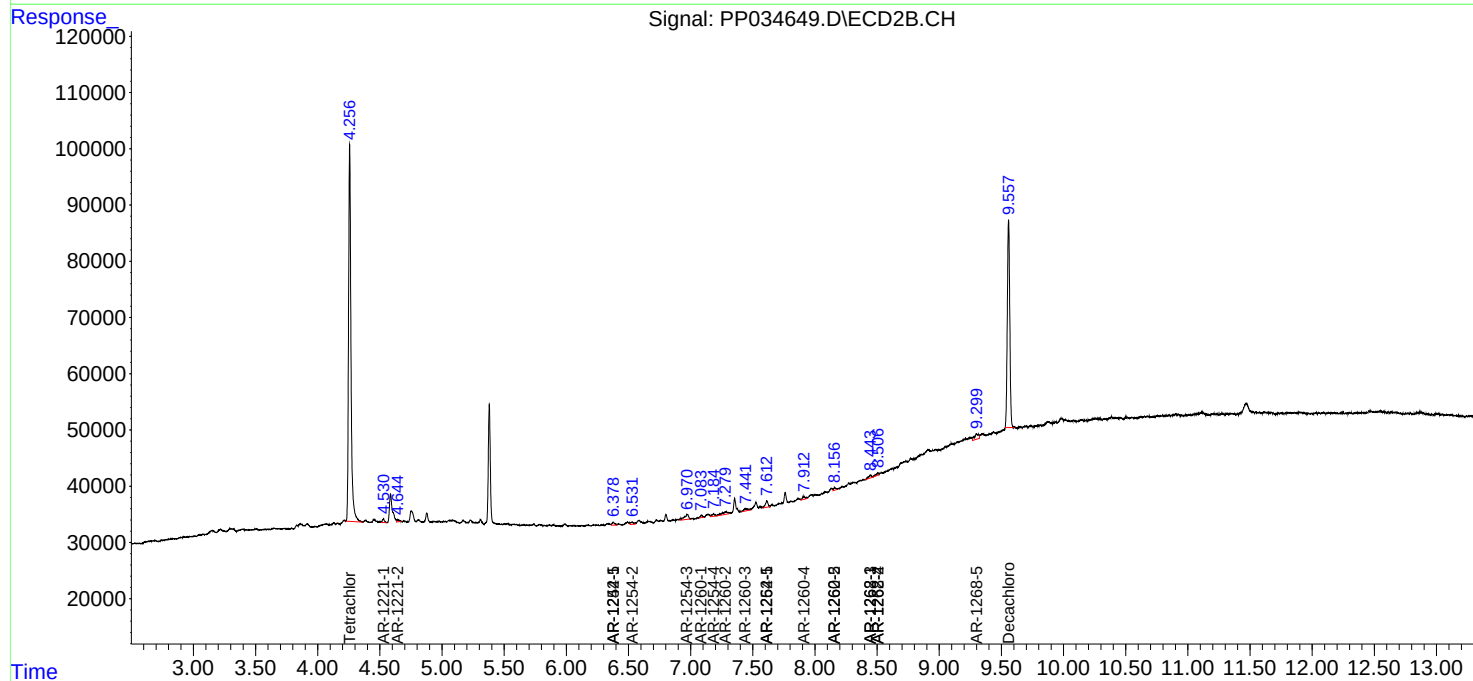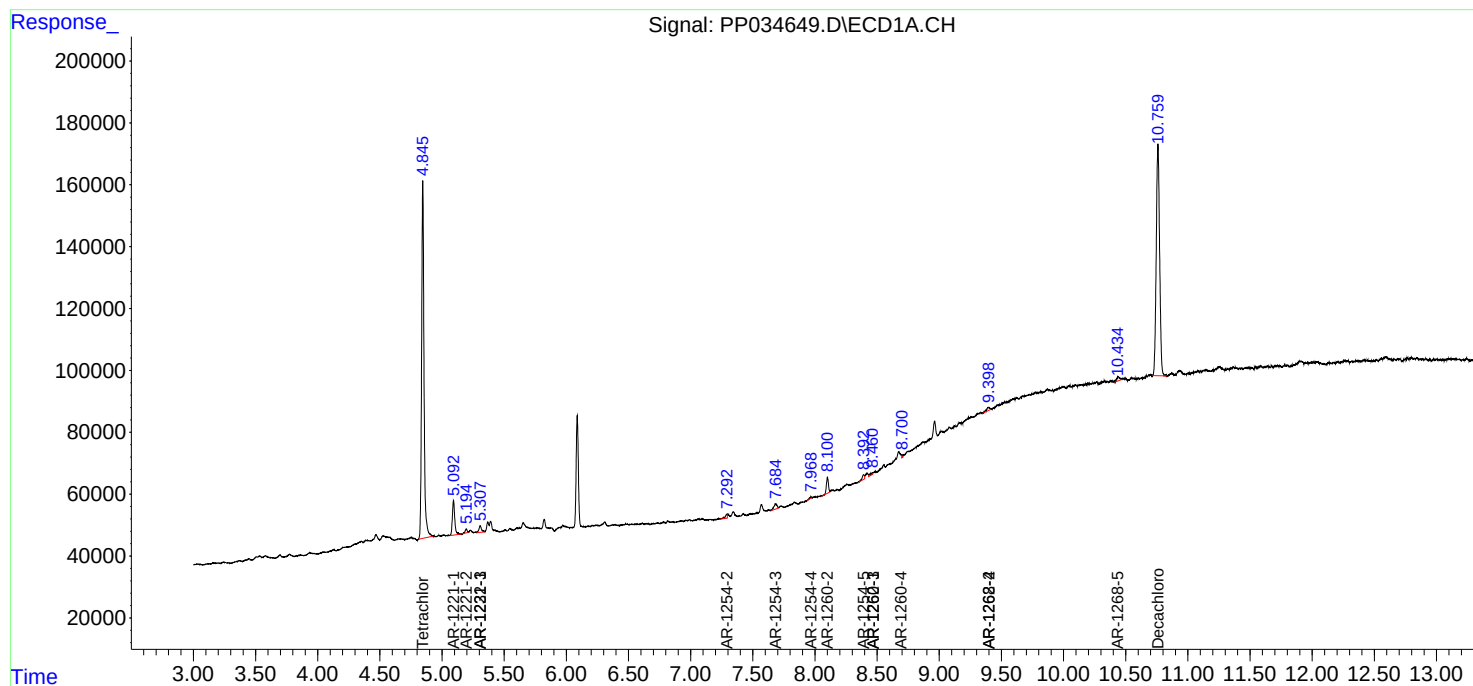


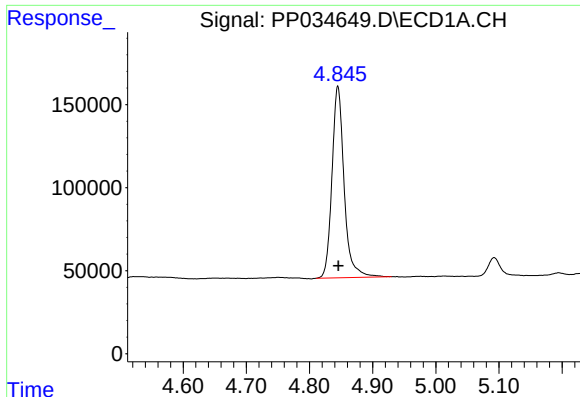

#1 Tetrachloro-m-xylene


R.T.: 4.845 min
Delta R.T.: -0.001 min
Response: 1544611
Conc: 20.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

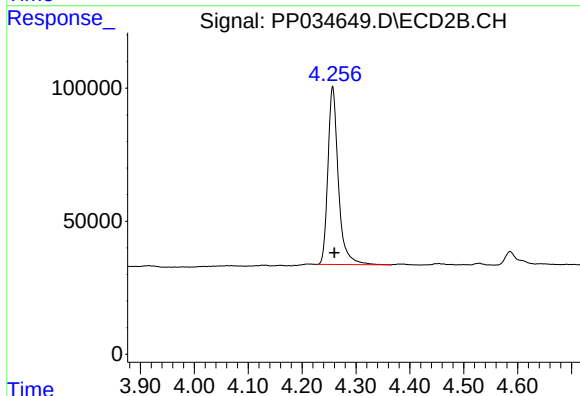


#1 Tetrachloro-m-xylene

R.T.: 4.257 min
Delta R.T.: -0.003 min
Response: 901797
Conc: 20.07 ng/ml

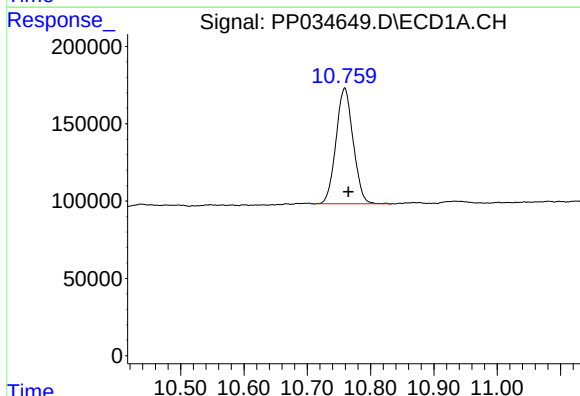


#2 Decachlorobiphenyl

R.T.: 10.759 min
Delta R.T.: -0.006 min
Response: 1405698
Conc: 18.26 ng/ml

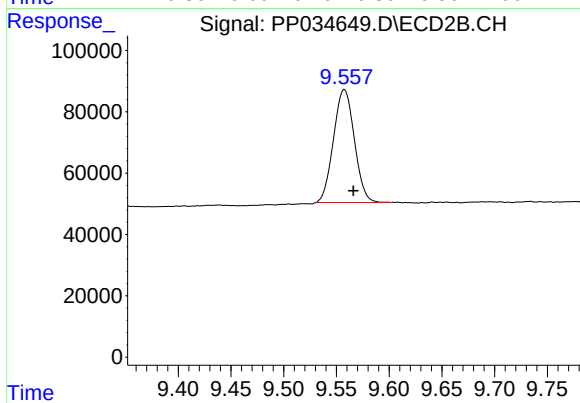

#2 Decachlorobiphenyl


R.T.: 9.557 min
Delta R.T.: -0.009 min
Response: 507695
Conc: 17.98 ng/ml

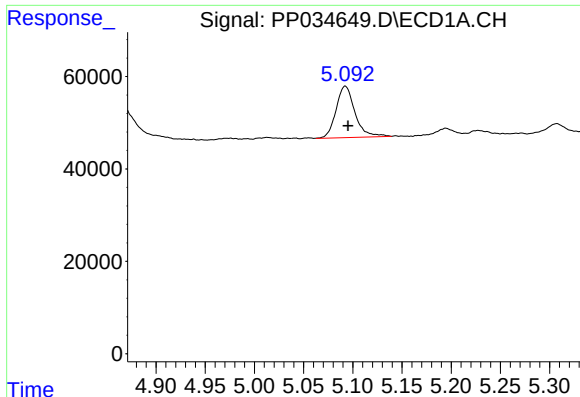

#8 AR-1221-1


R.T.: 5.092 min
Delta R.T.: -0.003 min
Response: 148637
Conc: 203.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

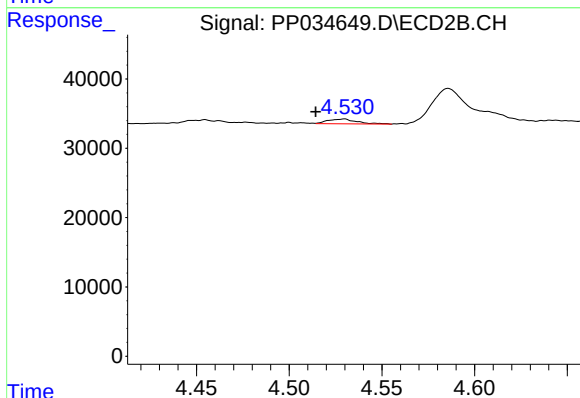


#8 AR-1221-1

R.T.: 4.530 min
Delta R.T.: 0.015 min
Response: 7363
Conc: 16.22 ng/ml

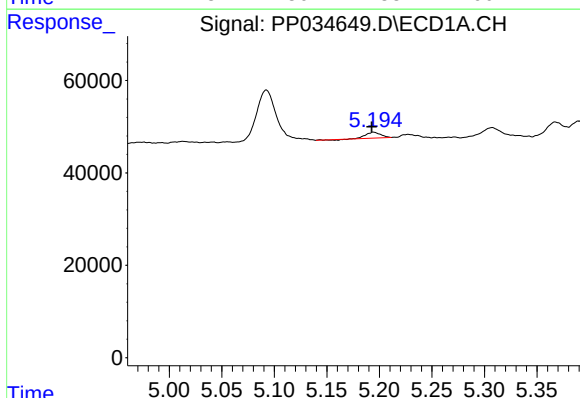


#9 AR-1221-2

R.T.: 5.194 min
Delta R.T.: 0.002 min
Response: 12494
Conc: 21.93 ng/ml

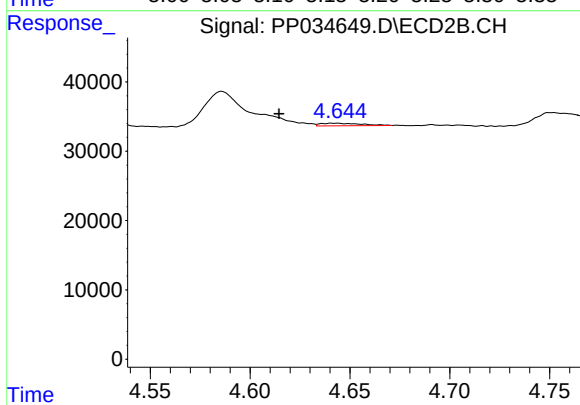

#9 AR-1221-2


R.T.: 4.643 min
Delta R.T.: 0.028 min
Response: 5277
Conc: 15.12 ng/ml

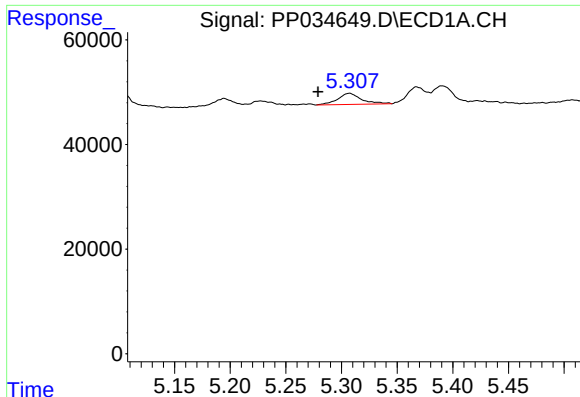

#10 AR-1221-3


R.T.: 5.308 min
Delta R.T.: 0.028 min
Response: 31558
Conc: 17.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

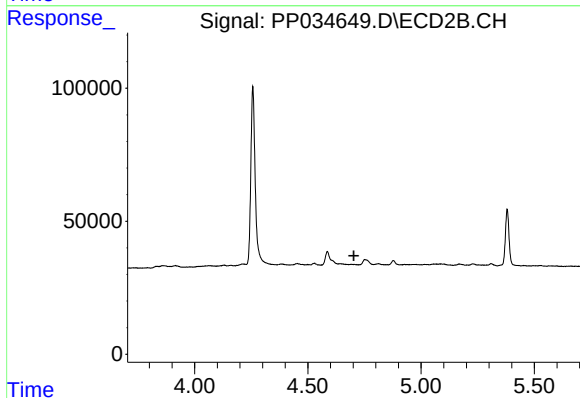


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.703 min
Response: 0
Conc: N.D.

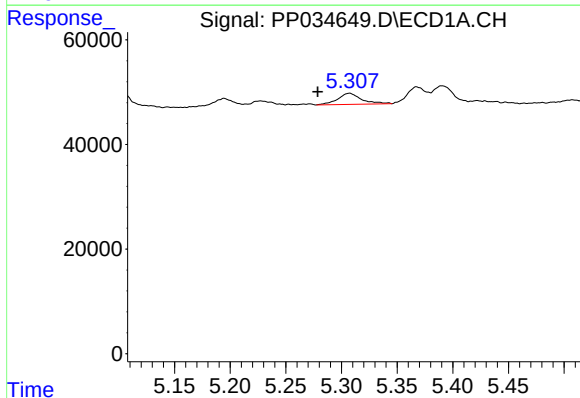


#11 AR-1232-1

R.T.: 5.308 min
Delta R.T.: 0.029 min
Response: 31558
Conc: 21.25 ng/ml

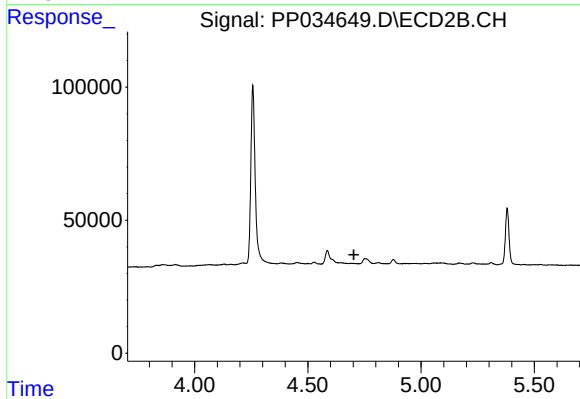

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.703 min
Response: 0
Conc: N.D.

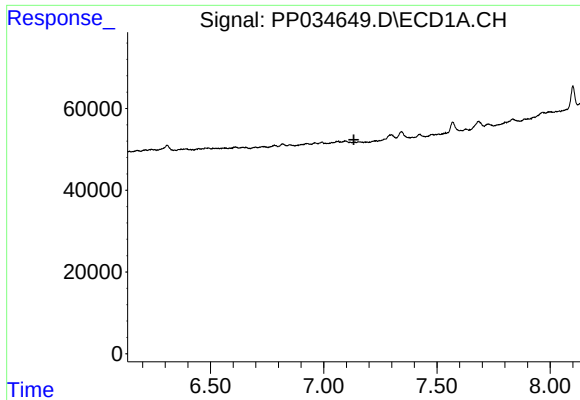

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

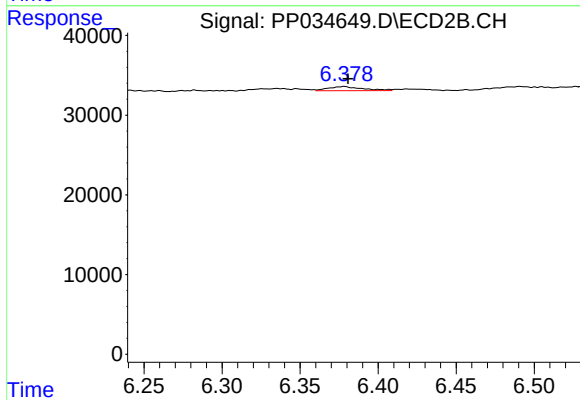


#20 AR-1242-5

R.T.: 6.378 min
Delta R.T.: -0.002 min
Response: 8030
Conc: 9.79 ng/ml

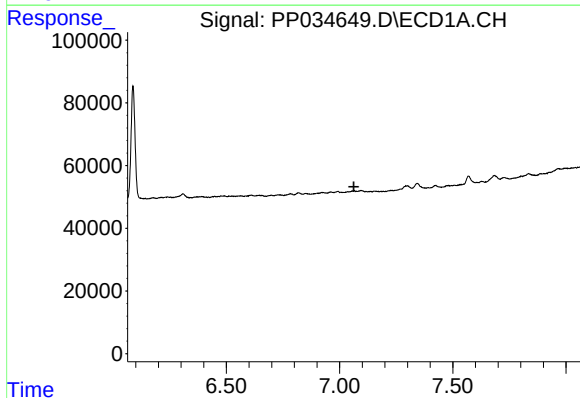


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 7.063 min
Response: 0
Conc: N.D.

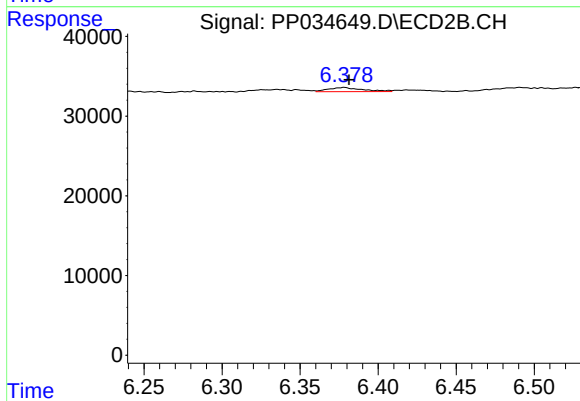

#26 AR-1254-1


R.T.: 6.378 min
Delta R.T.: -0.003 min
Response: 8030
Conc: 4.35 ng/ml

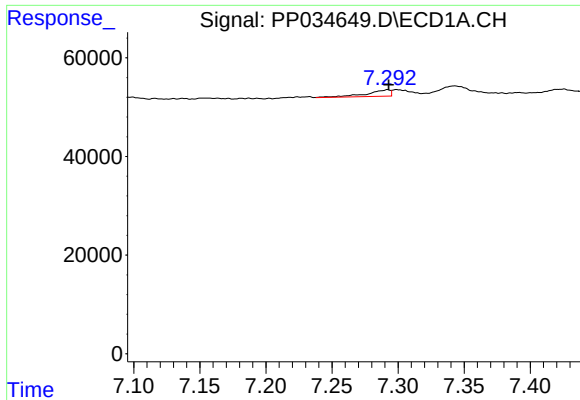

#27 AR-1254-2


R.T.: 7.292 min
Delta R.T.: 0.000 min
Response: 15493
Conc: 3.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

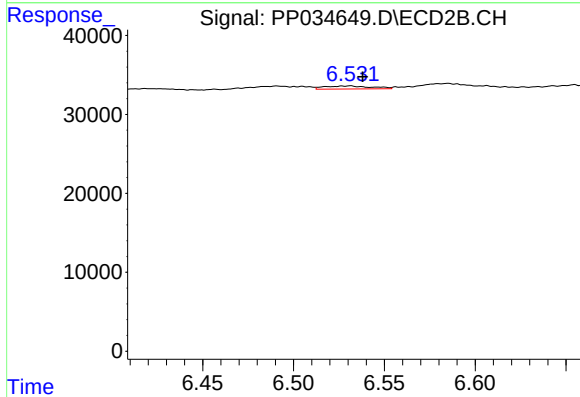


#27 AR-1254-2

R.T.: 6.531 min
Delta R.T.: -0.007 min
Response: 7015
Conc: 4.38 ng/ml

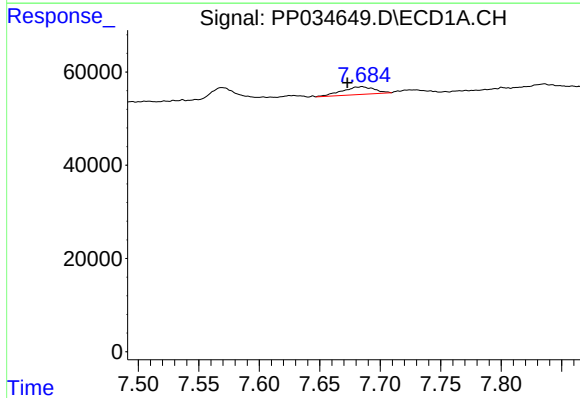


#28 AR-1254-3

R.T.: 7.685 min
Delta R.T.: 0.012 min
Response: 30589
Conc: 6.70 ng/ml

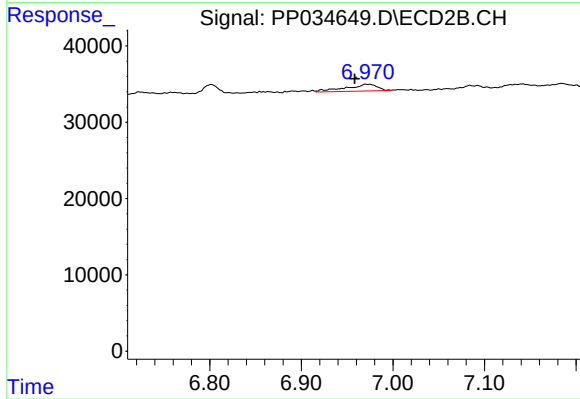

#28 AR-1254-3


R.T.: 6.971 min
Delta R.T.: 0.013 min
Response: 21067
Conc: 8.44 ng/ml

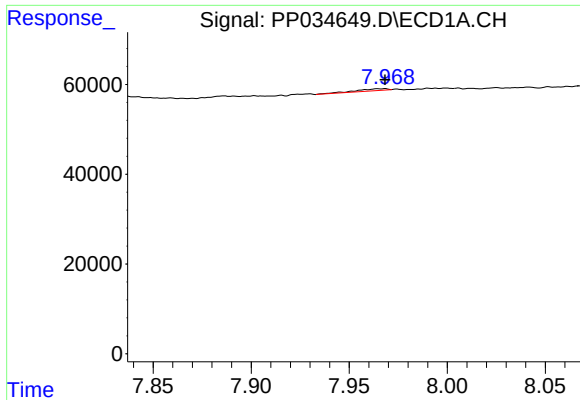

#29 AR-1254-4


R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 4918
Conc: 1.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

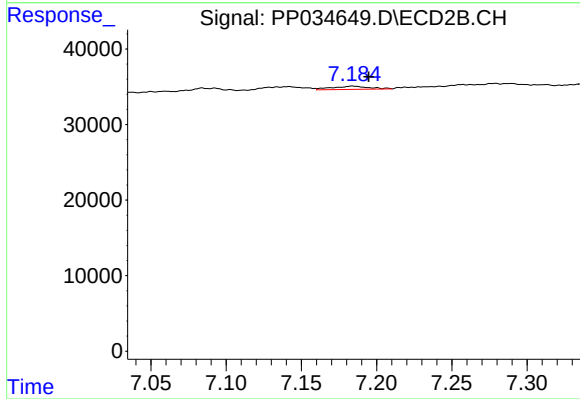


#29 AR-1254-4

R.T.: 7.184 min
Delta R.T.: -0.010 min
Response: 7043
Conc: 5.36 ng/ml

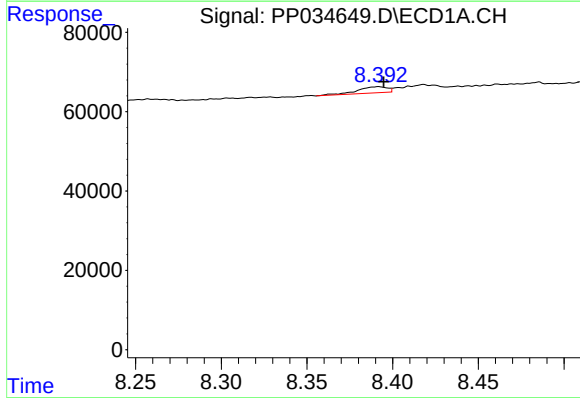


#30 AR-1254-5

R.T.: 8.392 min
Delta R.T.: -0.003 min
Response: 19070
Conc: 5.37 ng/ml

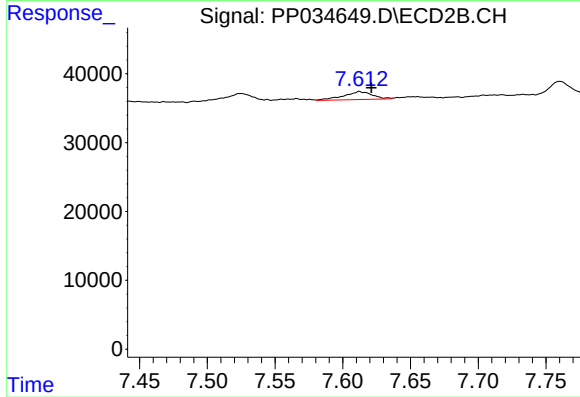

#30 AR-1254-5


R.T.: 7.613 min
Delta R.T.: -0.009 min
Response: 16998
Conc: 8.36 ng/ml

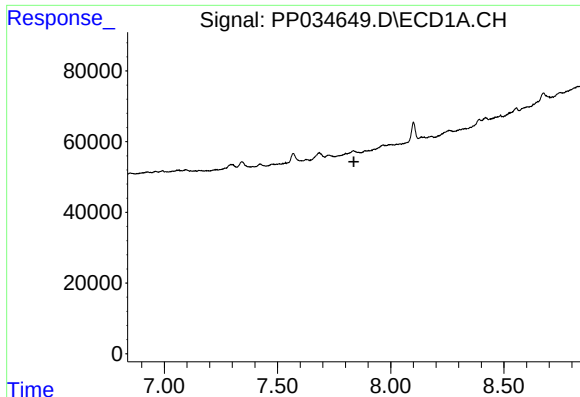

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

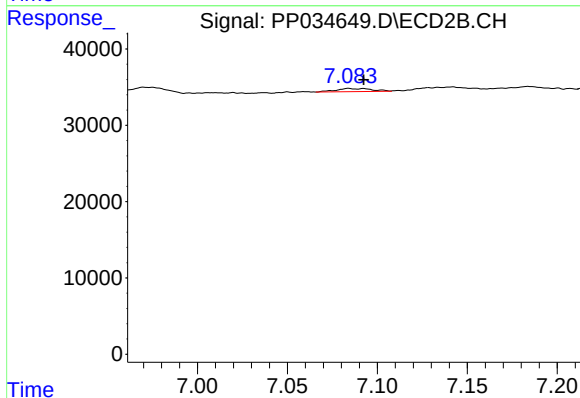


#31 AR-1260-1

R.T.: 7.084 min
Delta R.T.: -0.008 min
Response: 5773
Conc: 3.76 ng/ml

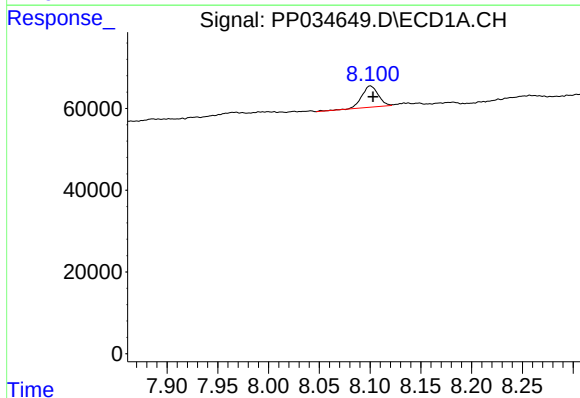


#32 AR-1260-2

R.T.: 8.100 min
Delta R.T.: -0.003 min
Response: 59100
Conc: 15.74 ng/ml

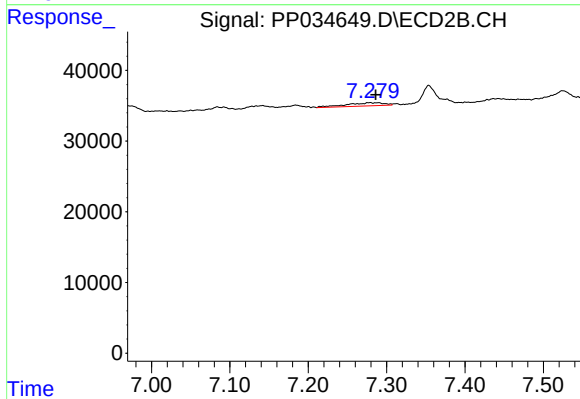

#32 AR-1260-2


R.T.: 7.278 min
Delta R.T.: -0.008 min
Response: 15490
Conc: 8.58 ng/ml

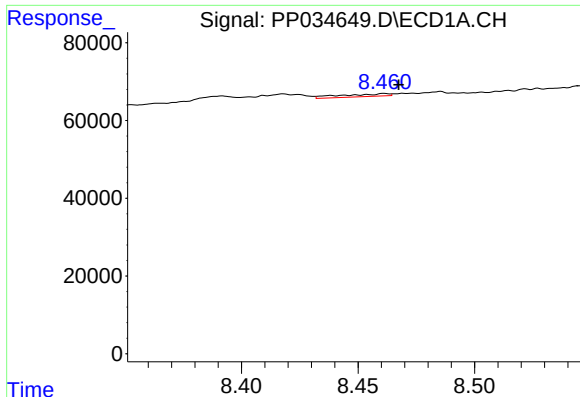

#33 AR-1260-3


R.T.: 8.461 min
Delta R.T.: -0.006 min
Response: 10006
Conc: 3.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

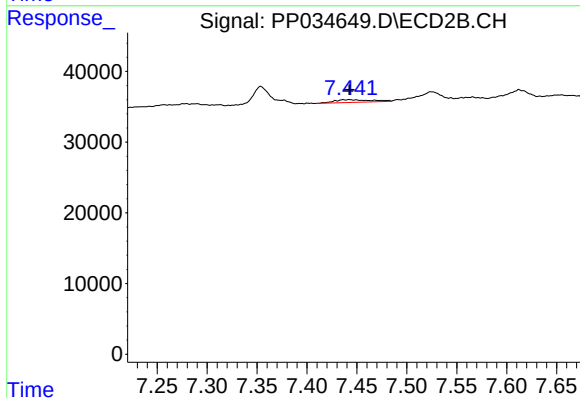


#33 AR-1260-3

R.T.: 7.442 min
Delta R.T.: 0.000 min
Response: 10023
Conc: 5.78 ng/ml

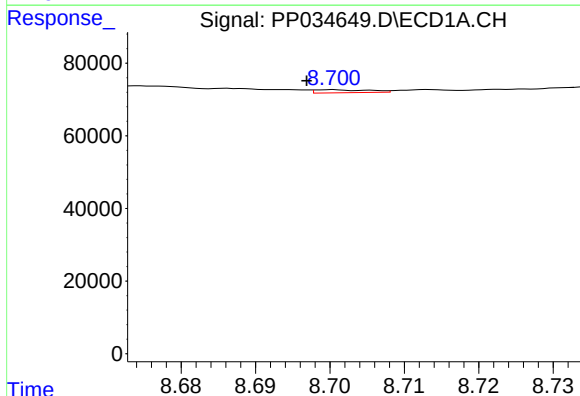


#34 AR-1260-4

R.T.: 8.700 min
Delta R.T.: 0.003 min
Response: 4260
Conc: 1.22 ng/ml

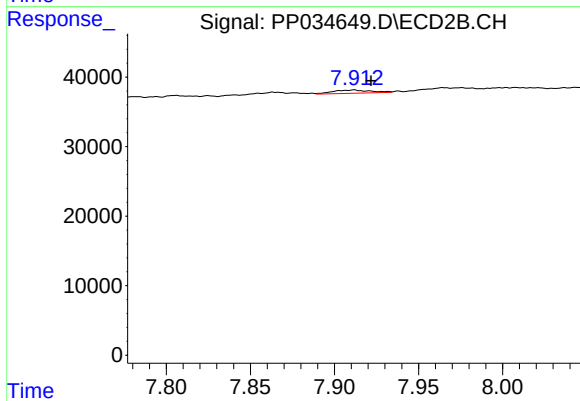

#34 AR-1260-4


R.T.: 7.912 min
Delta R.T.: -0.010 min
Response: 7509
Conc: 5.24 ng/ml

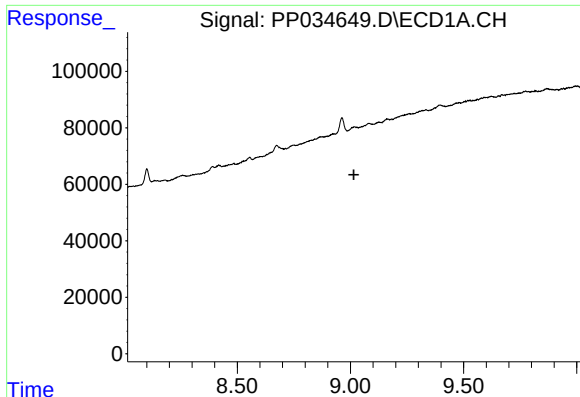

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.015 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

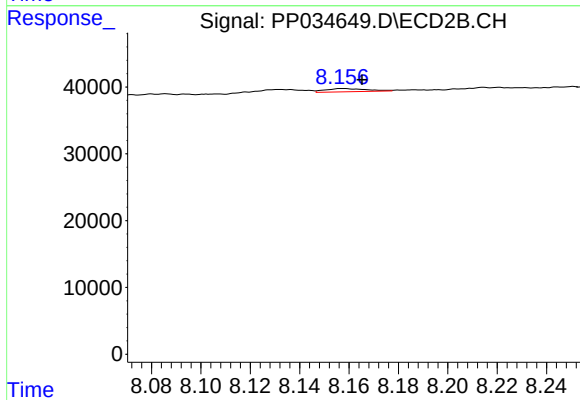


#35 AR-1260-5

R.T.: 8.158 min
Delta R.T.: -0.008 min
Response: 5698
Conc: 1.67 ng/ml

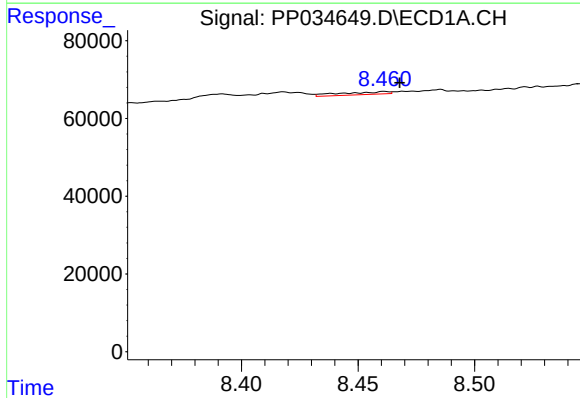


#36 AR-1262-1

R.T.: 8.461 min
Delta R.T.: -0.007 min
Response: 10006
Conc: 2.19 ng/ml

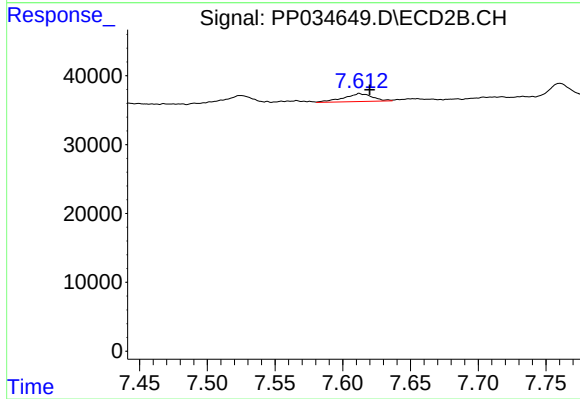

#36 AR-1262-1


R.T.: 7.613 min
Delta R.T.: -0.008 min
Response: 16998
Conc: 15.83 ng/ml

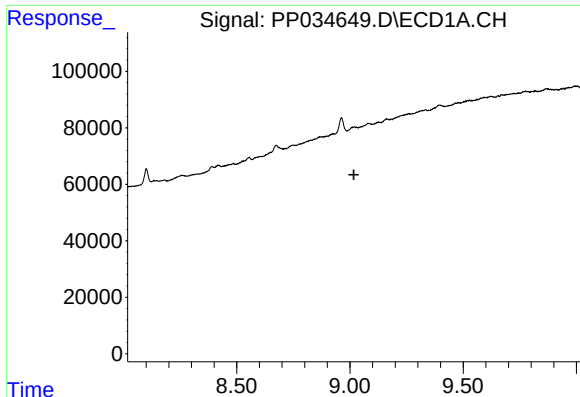

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 9.017 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

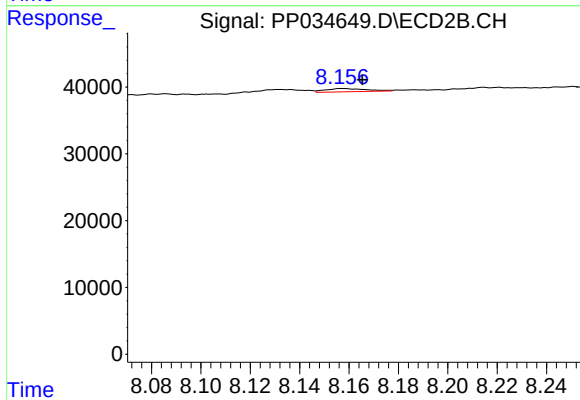


#37 AR-1262-2

R.T.: 8.158 min
Delta R.T.: -0.008 min
Response: 5698
Conc: 1.66 ng/ml

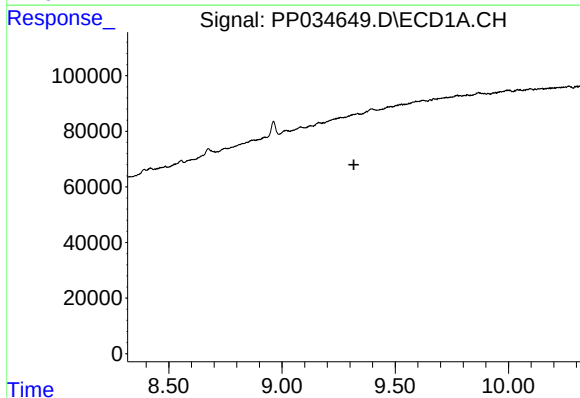


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.318 min
Response: 0
Conc: N.D.

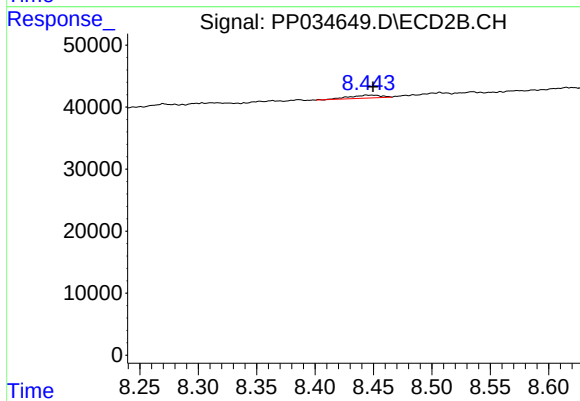

#38 AR-1262-3


R.T.: 8.444 min
Delta R.T.: -0.005 min
Response: 8974
Conc: 5.99 ng/ml

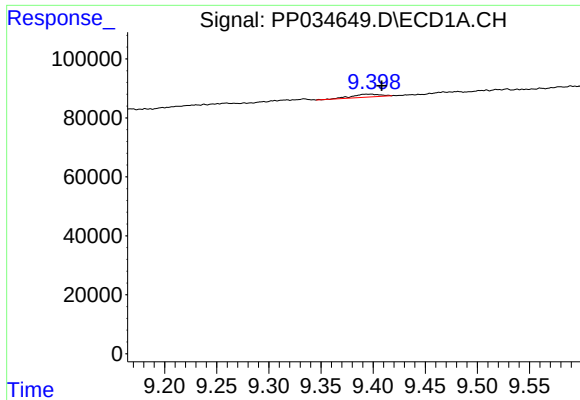

#39 AR-1262-4


R.T.: 9.398 min
Delta R.T.: -0.011 min
Response: 18950
Conc: 4.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

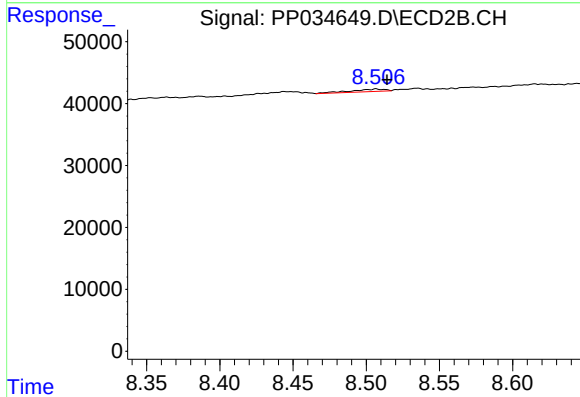


#39 AR-1262-4

R.T.: 8.507 min
Delta R.T.: -0.007 min
Response: 6442
Conc: 2.34 ng/ml

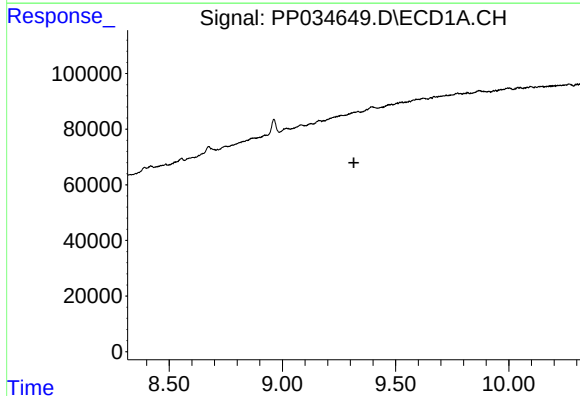


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.315 min
Response: 0
Conc: N.D.

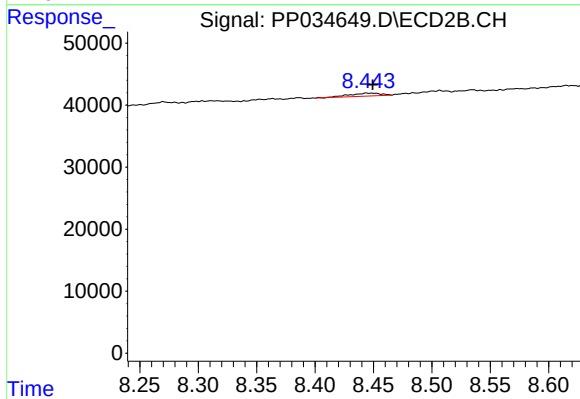

#41 AR-1268-1


R.T.: 8.444 min
Delta R.T.: -0.005 min
Response: 8974
Conc: 2.08 ng/ml

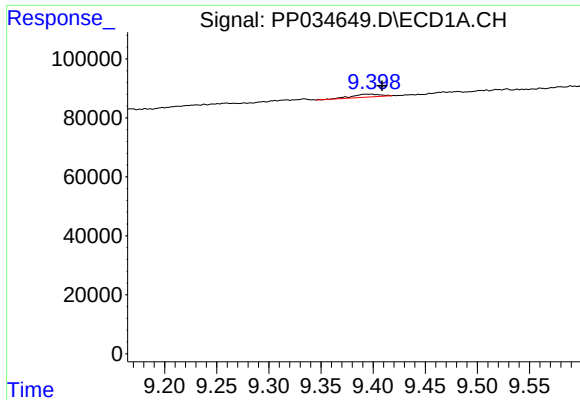

#42 AR-1268-2


R.T.: 9.398 min
Delta R.T.: -0.011 min
Response: 18950
Conc: 1.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-6S-(0-4)

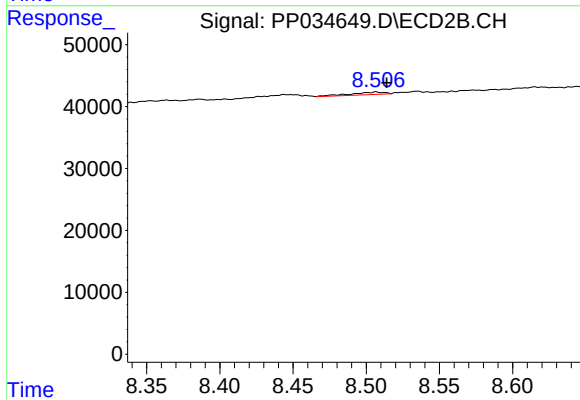


#42 AR-1268-2

R.T.: 8.507 min
Delta R.T.: -0.007 min
Response: 6442
Conc: 1.56 ng/ml

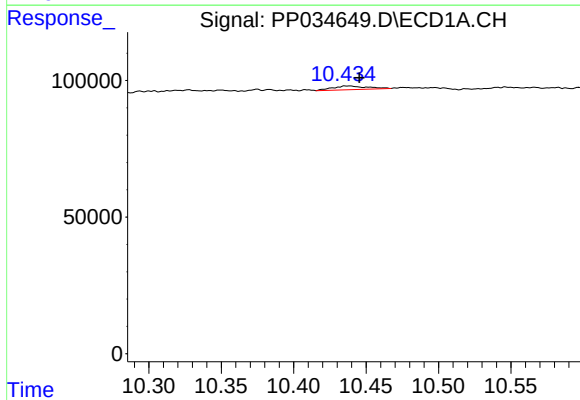

#45 AR-1268-5

R.T.: 10.437 min
Delta R.T.: -0.008 min
Response: 22468
Conc: 0.79 ng/ml

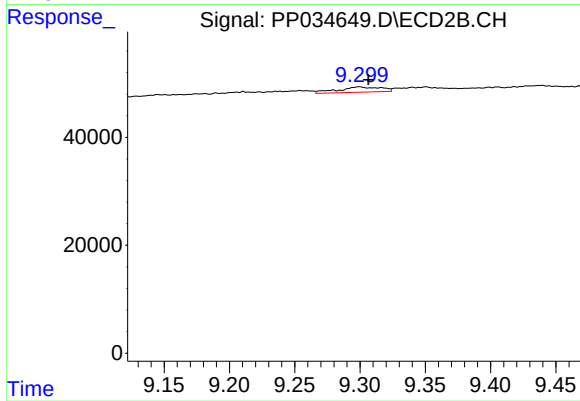

#45 AR-1268-5

R.T.: 9.300 min
Delta R.T.: -0.007 min
Response: 22778
Conc: 2.19 ng/ml