

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040221\
 Data File : PP034604.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2021 11:02
 Operator : DD\AJ
 Sample : M1885-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SG2-8035-8045

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 04:59:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.843	4.256	2015611	1112284	26.422	24.760
2)	SA Decachlor...	10.761	9.560	2078097	726599	26.995	25.733

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040221\
Data File : PP034604.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2021 11:02
Operator : DD\AJ
Sample : M1885-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SG2-8035-8045

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 04:59:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

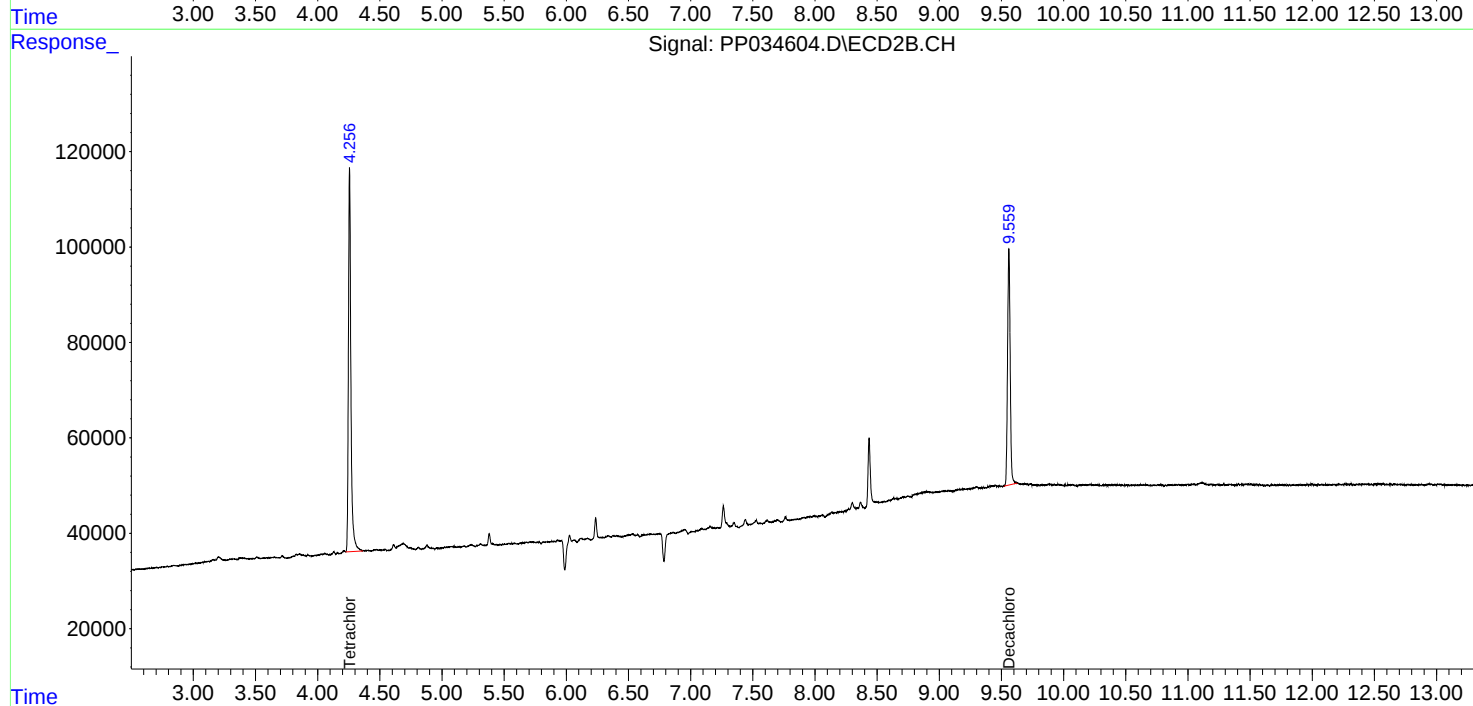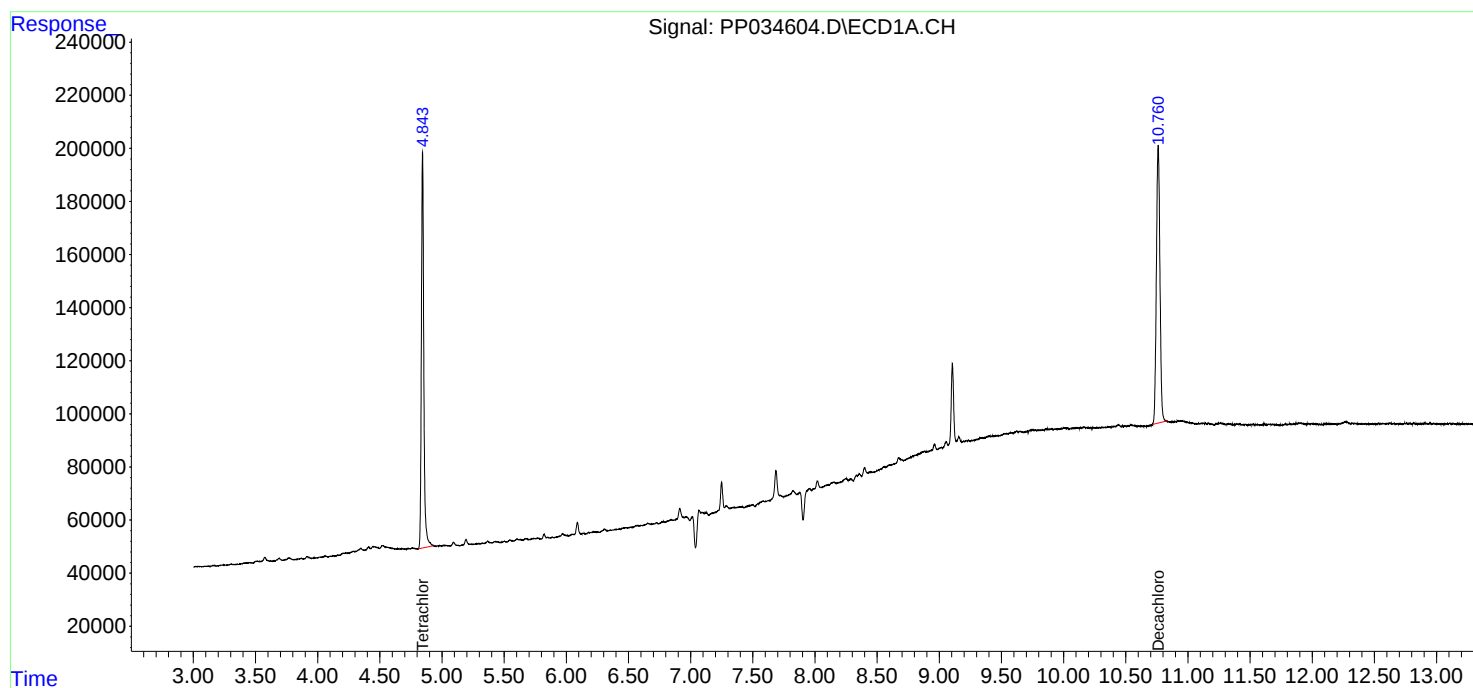


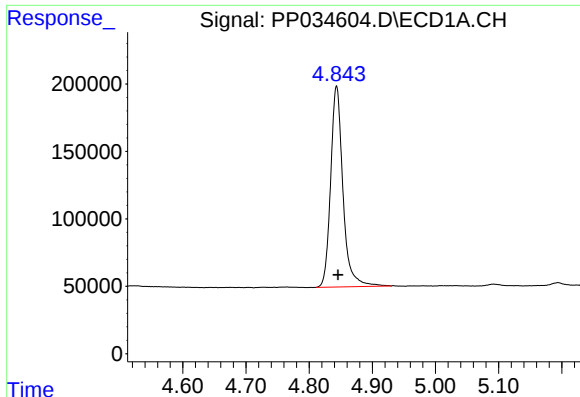

#1 Tetrachloro-m-xylene


R.T.: 4.843 min
Delta R.T.: -0.003 min
Response: 2015611
Conc: 26.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
SG2-8035-8045

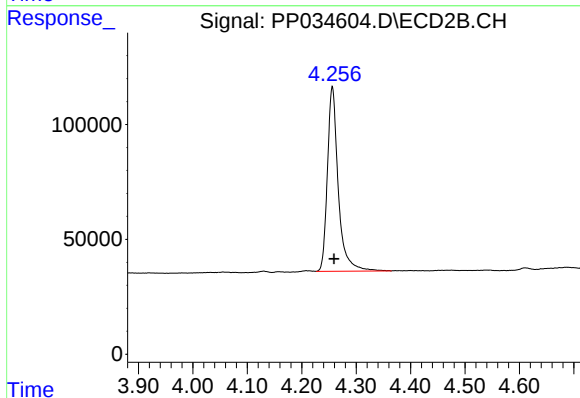


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: -0.004 min
Response: 1112284
Conc: 24.76 ng/ml

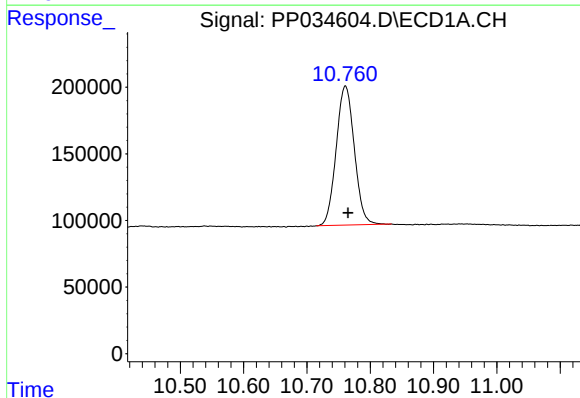

#2 Decachlorobiphenyl

R.T.: 10.761 min
Delta R.T.: -0.004 min
Response: 2078097
Conc: 27.00 ng/ml

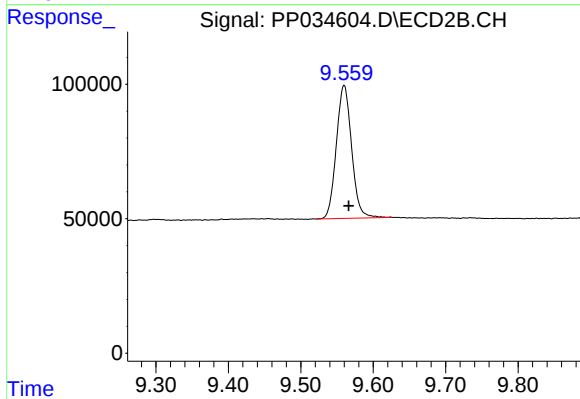

#2 Decachlorobiphenyl

R.T.: 9.560 min
Delta R.T.: -0.006 min
Response: 726599
Conc: 25.73 ng/ml