

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040221\
 Data File : PP034626.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2021 17:18
 Operator : DD\AJ
 Sample : M1888-04MSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-3D-(4-10)MSD

Manual Integrations
 APPROVED

Ankita
 4/5/2021 3:29:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 05:36:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.844	4.257	1852603	1060179	24.286	23.600
2)	SA Decachlor...	10.761	9.558	1508452	602571	19.595	21.341
Target Compounds							
3)	L1 AR-1016-1	6.155	5.507	1313042	666043	558.081	561.433
4)	L1 AR-1016-2	6.179	5.528	1937376	945771	545.477	532.639
5)	L1 AR-1016-3	6.244	5.720	1240223	528789	580.820	565.928
6)	L1 AR-1016-4	6.350	5.769	1042789	415949	585.562	572.704
7)	L1 AR-1016-5	6.663	5.999	975723	515979	565.526	564.123
31)	L7 AR-1260-1	7.835	7.087	1739232	948797	560.268	617.843
32)	L7 AR-1260-2	8.101	7.281	1992810	1015441	530.649	562.137m
33)	L7 AR-1260-3	8.465	7.436	1275389	988233	421.934	569.626m#
34)	L7 AR-1260-4	8.694	7.916	1663708	705193	476.540	491.847
35)	L7 AR-1260-5	9.014	8.160	3249084	1565796	453.682	458.378

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040221\
Data File : PP034626.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2021 17:18
Operator : DD\AJ
Sample : M1888-04MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
TP-3D-(4-10)MSD


Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 05:36:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

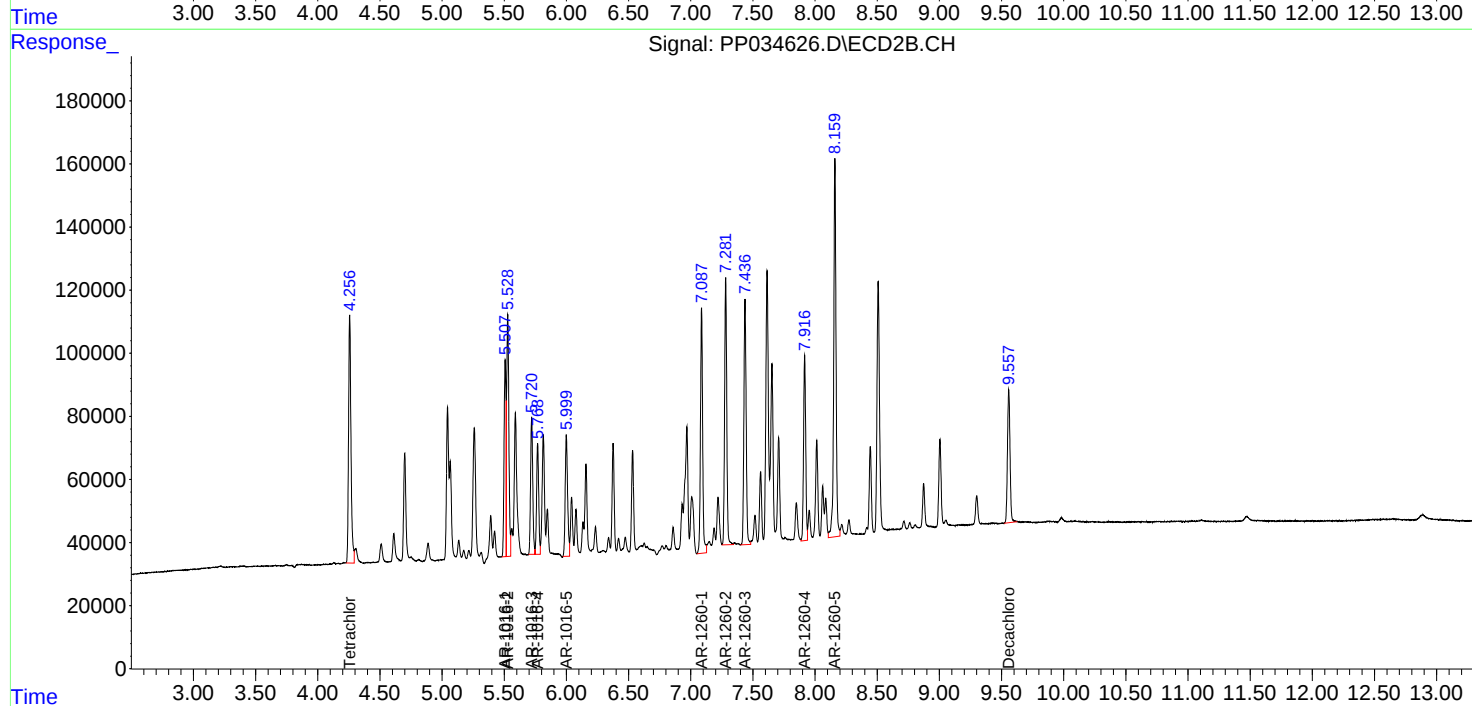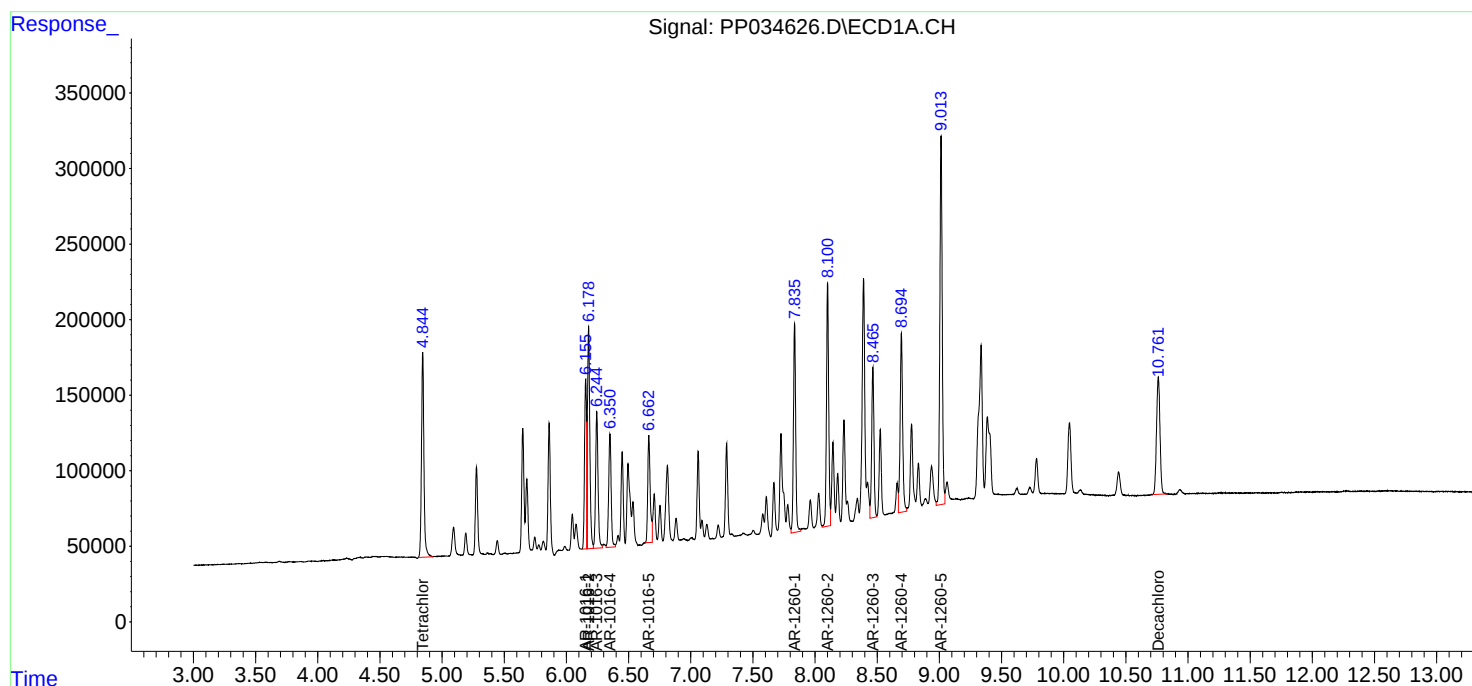

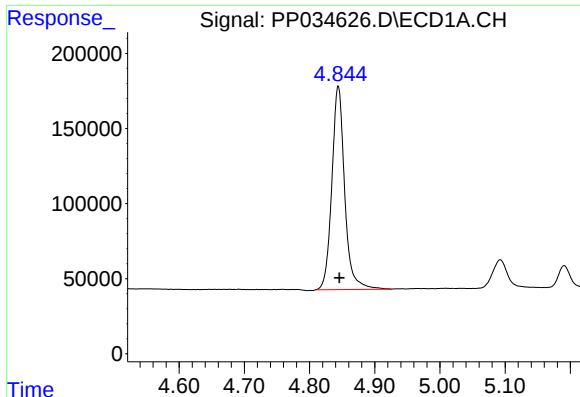


#1 Tetrachloro-m-xylene

R.T.: 4.844 min
Delta R.T.: -0.002 min
Response: 1852603
Conc: 24.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-3D-(4-10)MSD


Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:40 PM

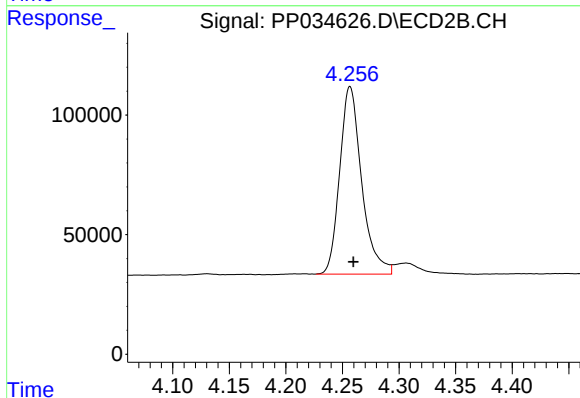


#1 Tetrachloro-m-xylene

R.T.: 4.257 min
Delta R.T.: -0.003 min
Response: 1060179
Conc: 23.60 ng/ml

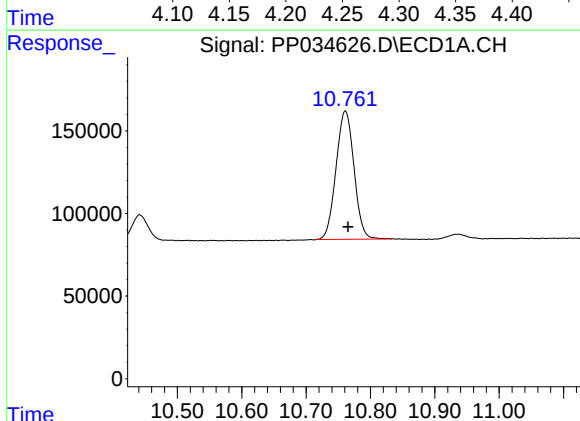


#2 Decachlorobiphenyl

R.T.: 10.761 min
Delta R.T.: -0.004 min
Response: 1508452
Conc: 19.60 ng/ml

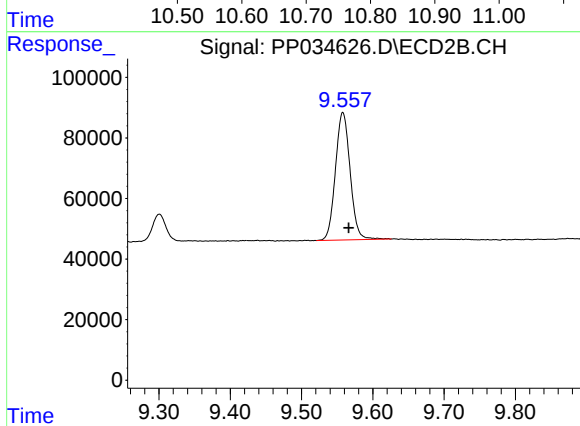

#2 Decachlorobiphenyl

R.T.: 9.558 min
Delta R.T.: -0.008 min
Response: 602571
Conc: 21.34 ng/ml

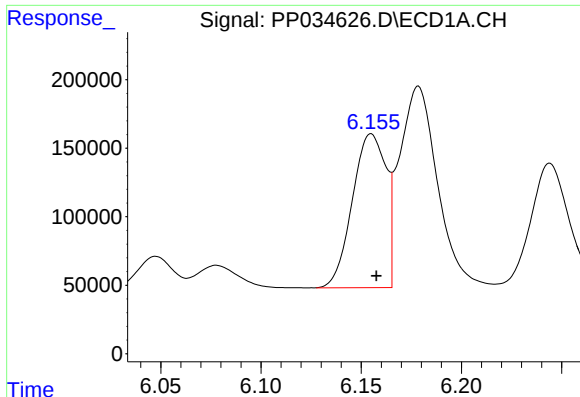


#3 AR-1016-1

R.T.: 6.155 min
Delta R.T.: -0.003 min
Response: 1313042
Conc: 558.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-3D-(4-10)MSD


Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:40 PM

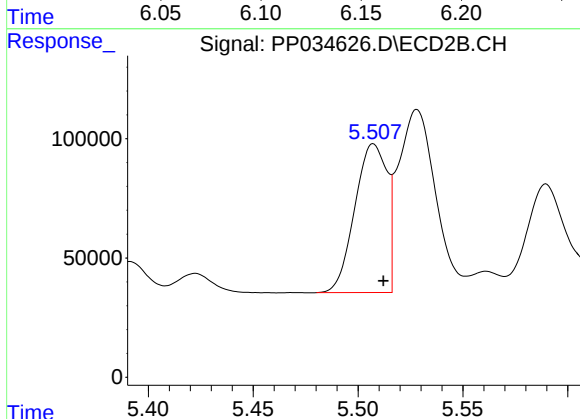


#3 AR-1016-1

R.T.: 5.507 min
Delta R.T.: -0.005 min
Response: 666043
Conc: 561.43 ng/ml

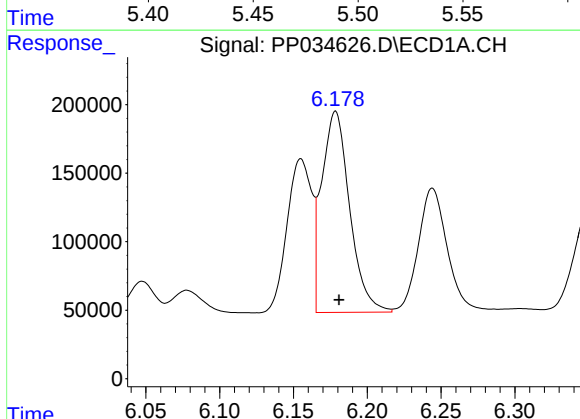


#4 AR-1016-2

R.T.: 6.179 min
Delta R.T.: -0.002 min
Response: 1937376
Conc: 545.48 ng/ml

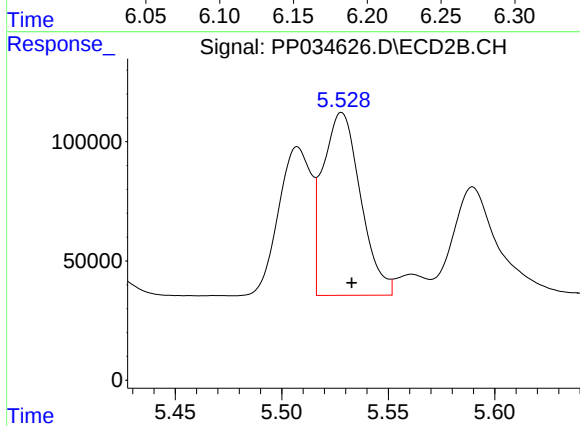

#4 AR-1016-2

R.T.: 5.528 min
Delta R.T.: -0.005 min
Response: 945771
Conc: 532.64 ng/ml

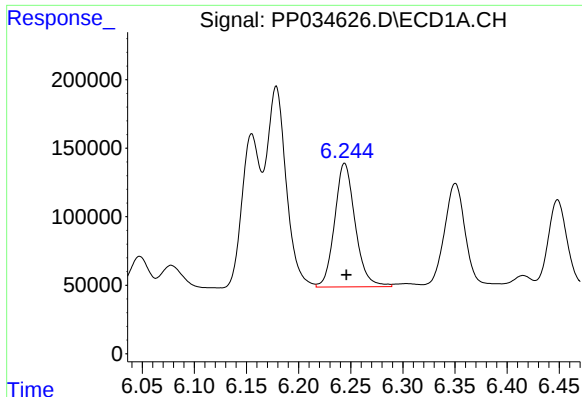


#5 AR-1016-3

R.T.: 6.244 min
Delta R.T.: -0.002 min
Response: 1240223
Conc: 580.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-3D-(4-10)MSD


Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:40 PM

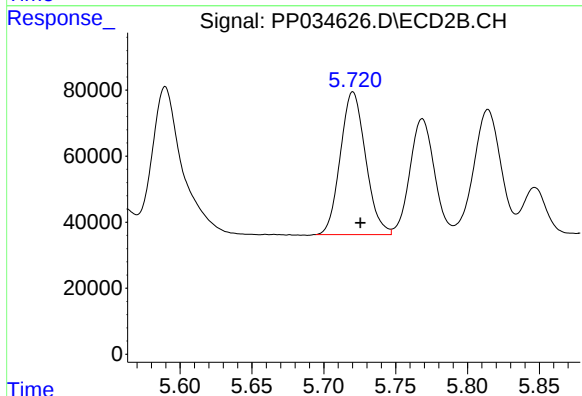


#5 AR-1016-3

R.T.: 5.720 min
Delta R.T.: -0.005 min
Response: 528789
Conc: 565.93 ng/ml

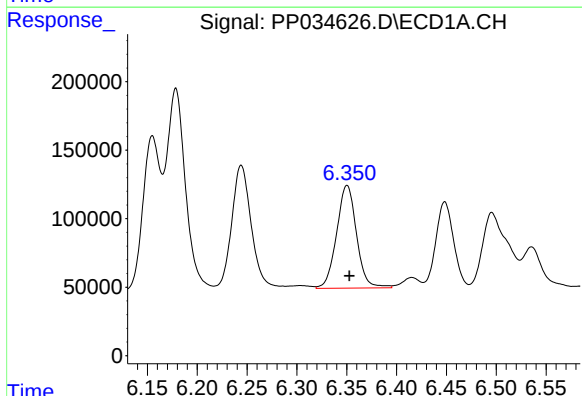


#6 AR-1016-4

R.T.: 6.350 min
Delta R.T.: -0.002 min
Response: 1042789
Conc: 585.56 ng/ml

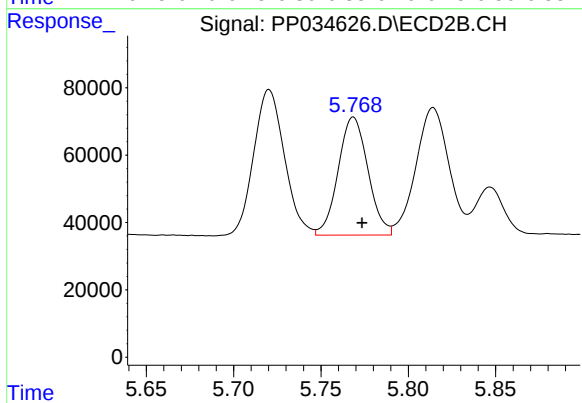

#6 AR-1016-4

R.T.: 5.769 min
Delta R.T.: -0.005 min
Response: 415949
Conc: 572.70 ng/ml

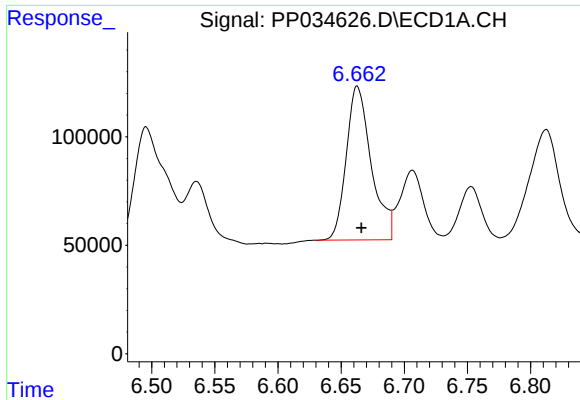


#7 AR-1016-5

R.T.: 6.663 min
Delta R.T.: -0.003 min
Response: 975723
Conc: 565.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-3D-(4-10)MSD


Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:40 PM

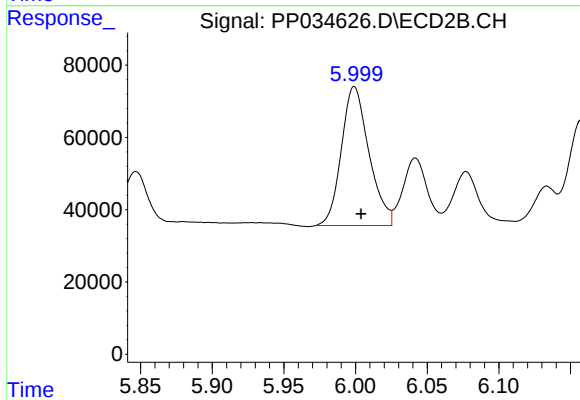


#7 AR-1016-5

R.T.: 5.999 min
Delta R.T.: -0.005 min
Response: 515979
Conc: 564.12 ng/ml

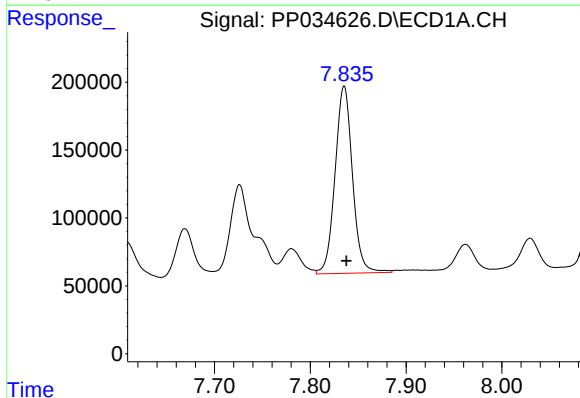


#31 AR-1260-1

R.T.: 7.835 min
Delta R.T.: -0.002 min
Response: 1739232
Conc: 560.27 ng/ml

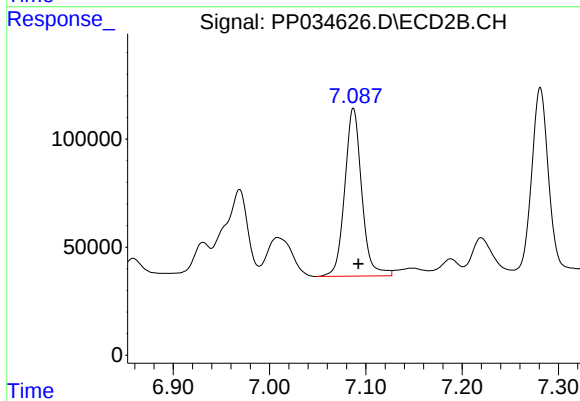

#31 AR-1260-1

R.T.: 7.087 min
Delta R.T.: -0.005 min
Response: 948797
Conc: 617.84 ng/ml

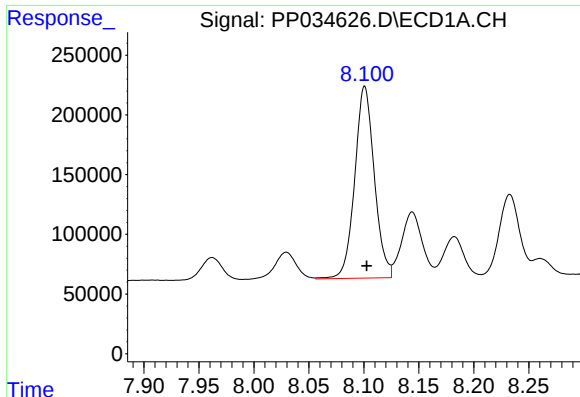


#32 AR-1260-2

R.T.: 8.101 min
Delta R.T.: -0.002 min
Response: 1992810
Conc: 530.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-3D-(4-10)MSD


Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:40 PM

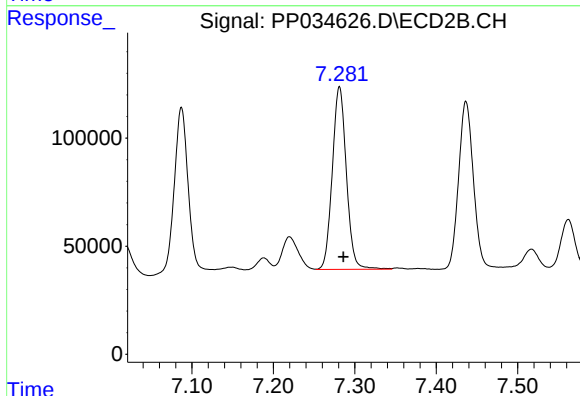


#32 AR-1260-2

R.T.: 7.281 min
Delta R.T.: -0.005 min
Response: 1015441
Conc: 562.14 ng/ml m

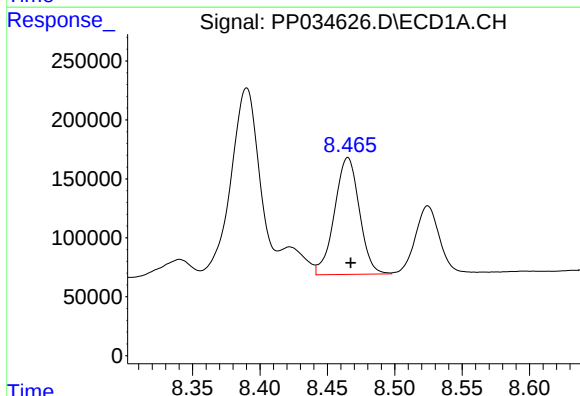


#33 AR-1260-3

R.T.: 8.465 min
Delta R.T.: -0.002 min
Response: 1275389
Conc: 421.93 ng/ml

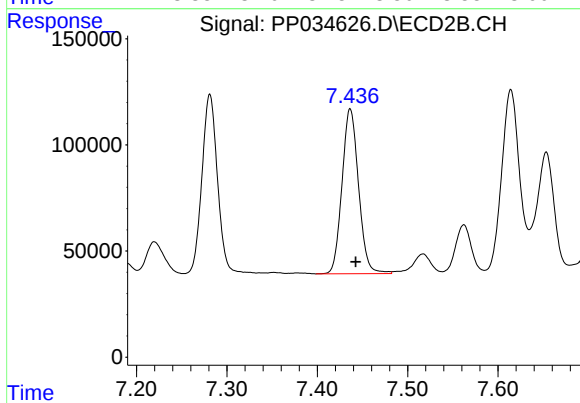

#33 AR-1260-3

R.T.: 7.436 min
Delta R.T.: -0.007 min
Response: 988233
Conc: 569.63 ng/ml m

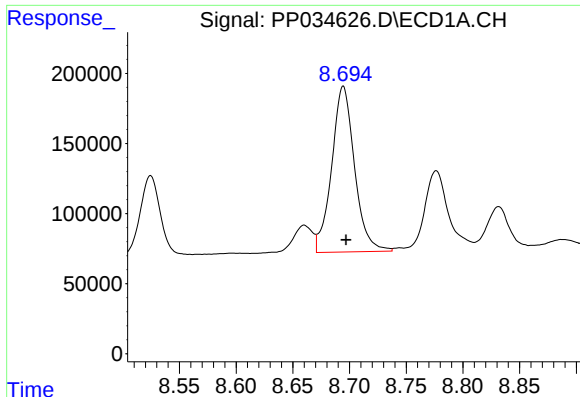


#34 AR-1260-4

R.T.: 8.694 min
Delta R.T.: -0.002 min
Response: 1663708
Conc: 476.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-3D-(4-10)MSD


Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:40 PM

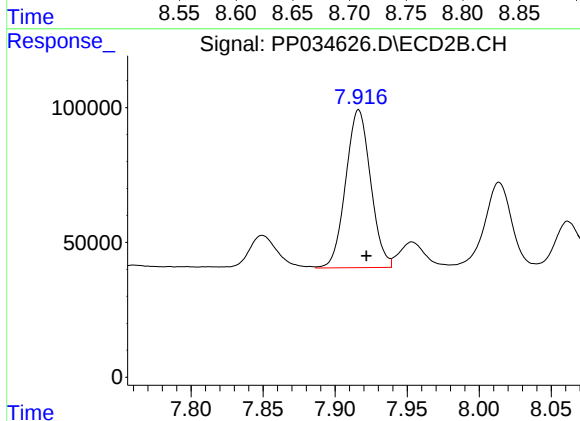


#34 AR-1260-4

R.T.: 7.916 min
Delta R.T.: -0.005 min
Response: 705193
Conc: 491.85 ng/ml

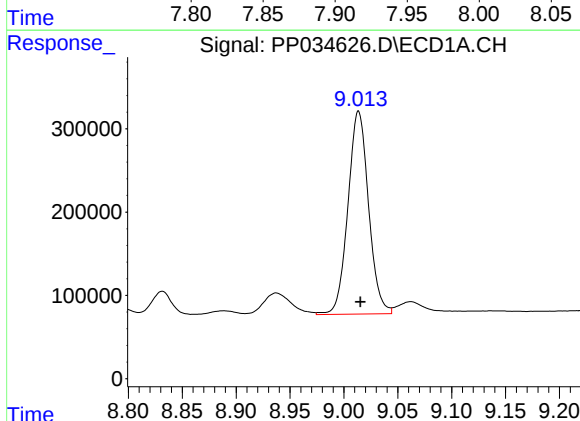

#35 AR-1260-5

R.T.: 9.014 min
Delta R.T.: -0.002 min
Response: 3249084
Conc: 453.68 ng/ml

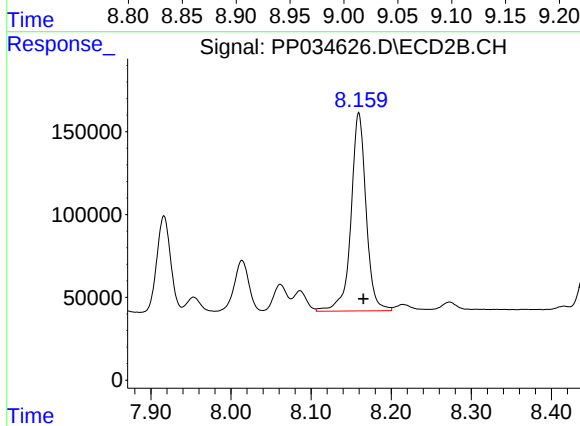

#35 AR-1260-5

R.T.: 8.160 min
Delta R.T.: -0.006 min
Response: 1565796
Conc: 458.38 ng/ml