

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040221\
 Data File : PP034631.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2021 19:00
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 4/5/2021 3:29:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 05:48:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.846	4.257	3934408	2318401	51.576	51.609
2)	SA Decachlor...	10.764	9.559	3912450	1500051	50.824	53.126
Target Compounds							
26)	L6 AR-1254-1	7.062	6.376	1223871	909331	445.120m	492.887m
27)	L6 AR-1254-2	7.291	6.533	2069202	797982	486.627	498.773m
28)	L6 AR-1254-3	7.671	6.953	2321464	1243355	508.626	498.187m
29)	L6 AR-1254-4	7.966	7.189	1493381	670476	483.004	510.045m
30)	L6 AR-1254-5	8.394	7.616	1697631	1130029	477.690	555.999

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040221\
Data File : PP034631.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2021 19:00
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 05:48:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

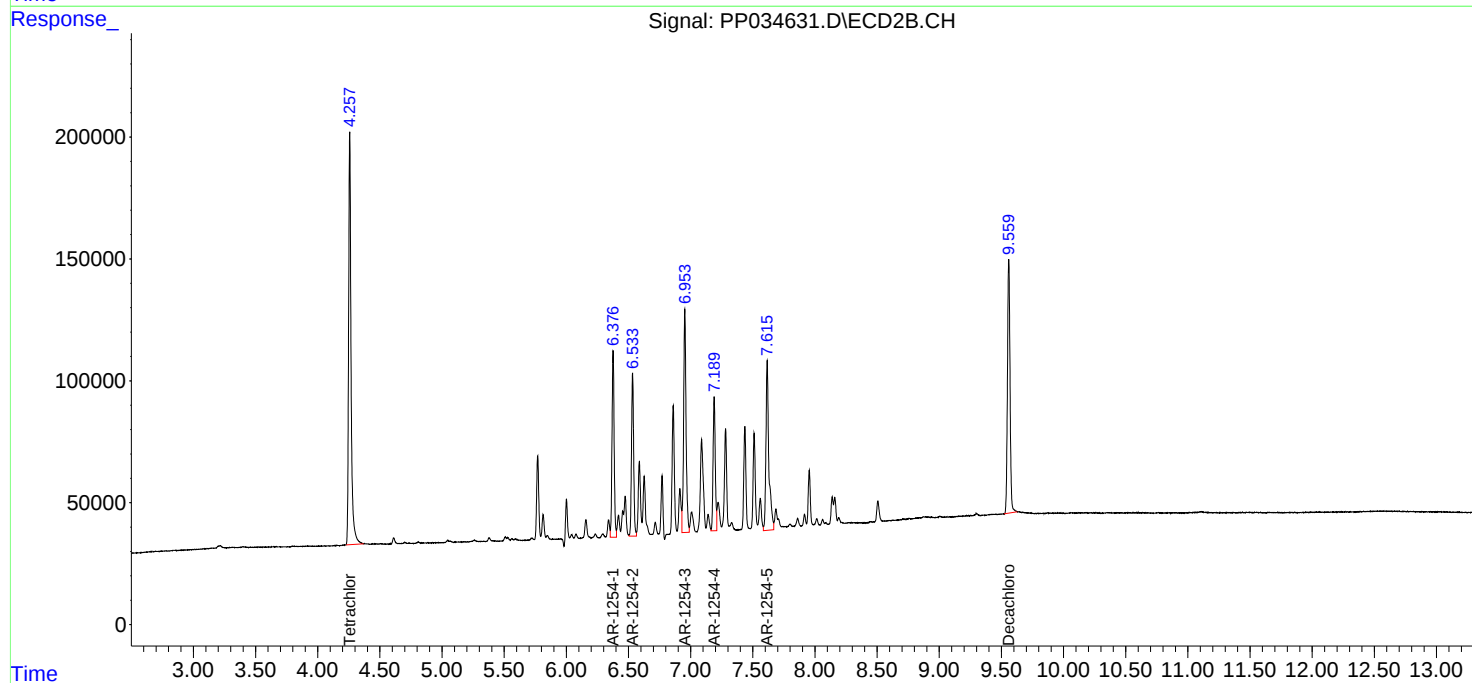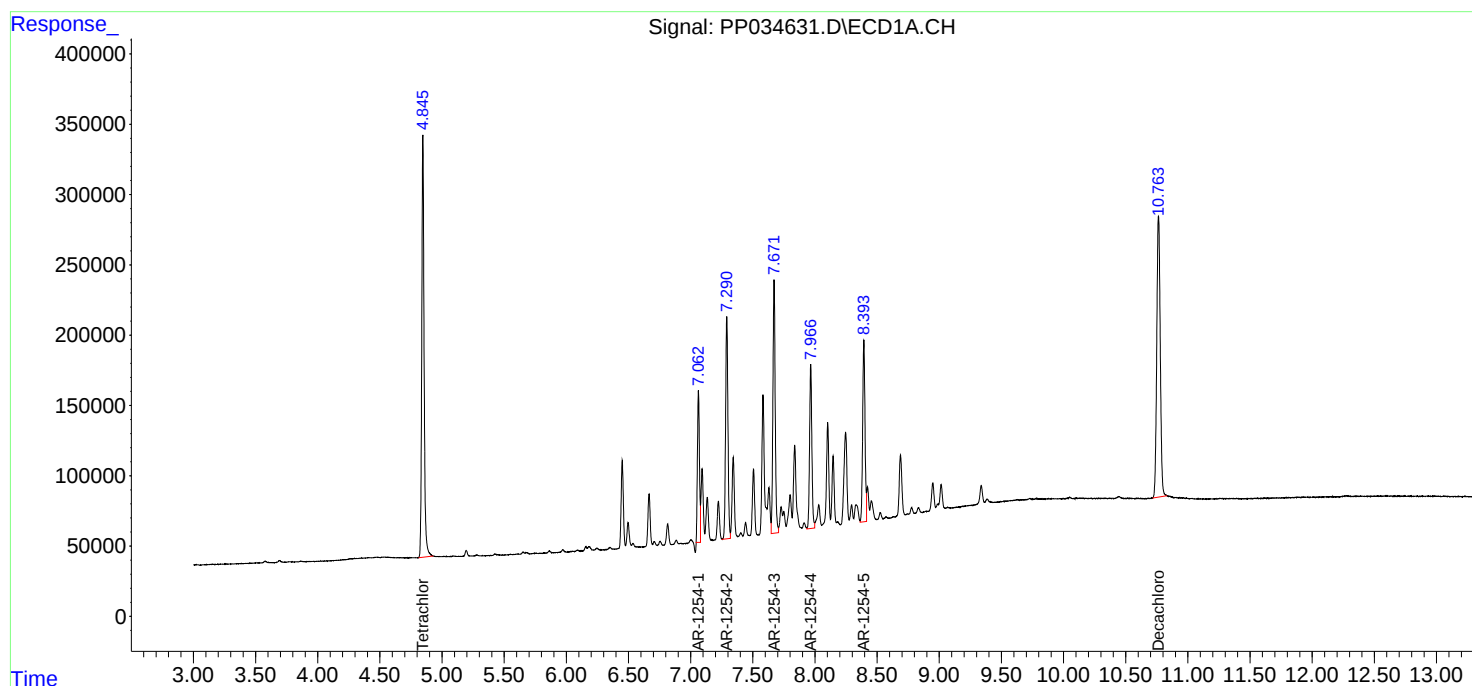

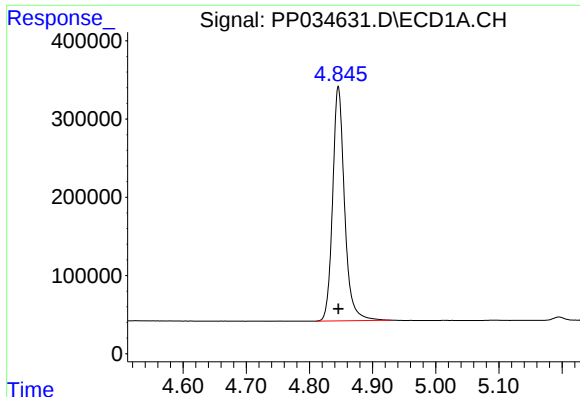


#1 Tetrachloro-m-xylene

R.T.: 4.846 min
Delta R.T.: 0.000 min
Response: 3934408
Conc: 51.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:42 PM

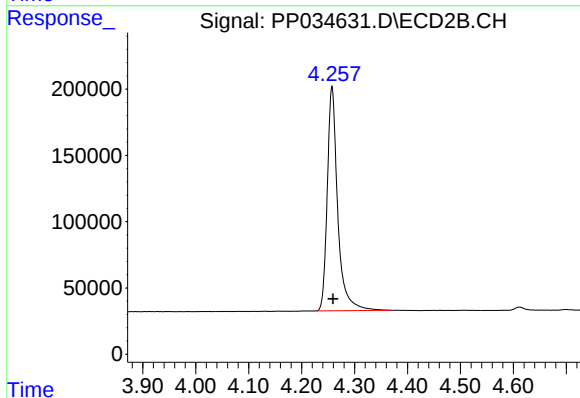


#1 Tetrachloro-m-xylene

R.T.: 4.257 min
Delta R.T.: -0.002 min
Response: 2318401
Conc: 51.61 ng/ml

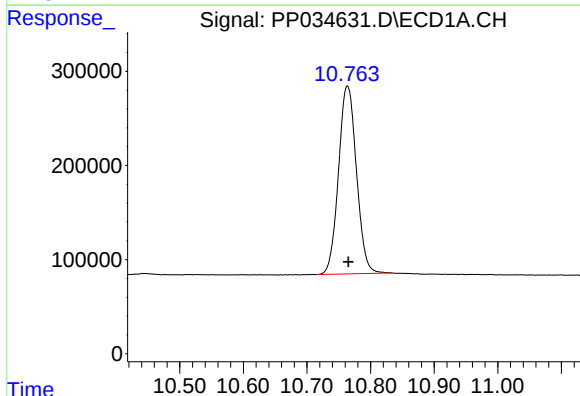


#2 Decachlorobiphenyl

R.T.: 10.764 min
Delta R.T.: -0.002 min
Response: 3912450
Conc: 50.82 ng/ml

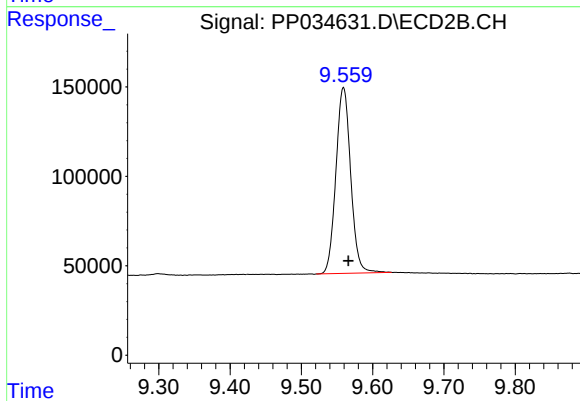

#2 Decachlorobiphenyl

R.T.: 9.559 min
Delta R.T.: -0.007 min
Response: 1500051
Conc: 53.13 ng/ml

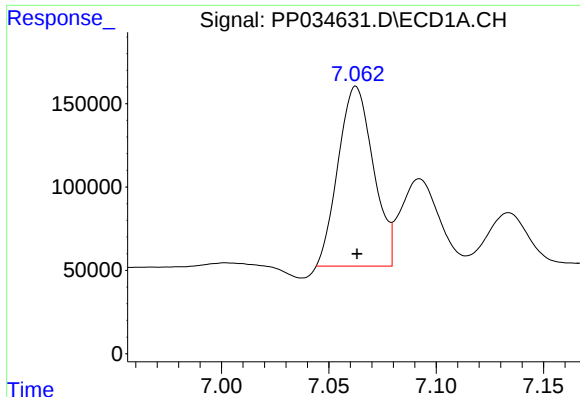


#26 AR-1254-1

R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 1223871
Conc: 445.12 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:42 PM

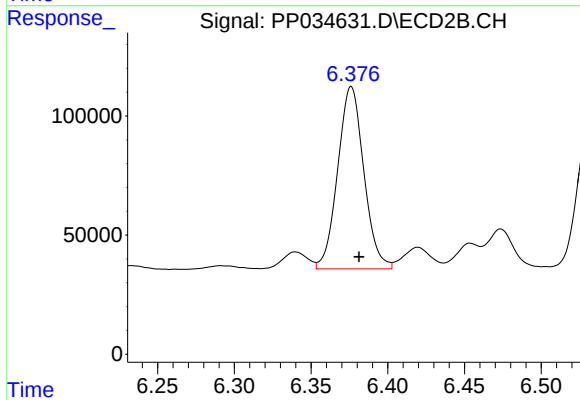


#26 AR-1254-1

R.T.: 6.376 min
Delta R.T.: -0.006 min
Response: 909331
Conc: 492.89 ng/ml m

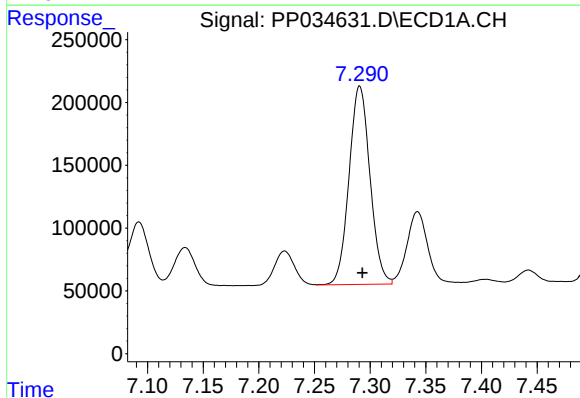


#27 AR-1254-2

R.T.: 7.291 min
Delta R.T.: -0.002 min
Response: 2069202
Conc: 486.63 ng/ml

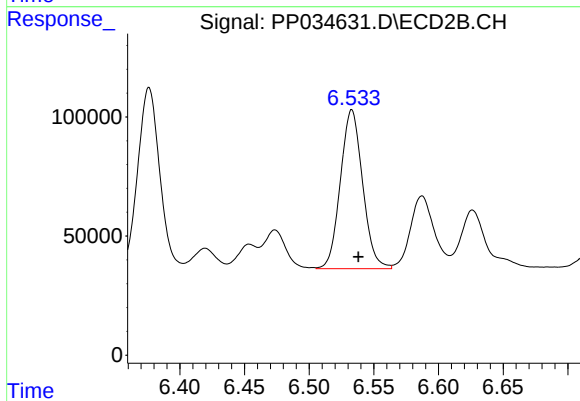

#27 AR-1254-2

R.T.: 6.533 min
Delta R.T.: -0.006 min
Response: 797982
Conc: 498.77 ng/ml m

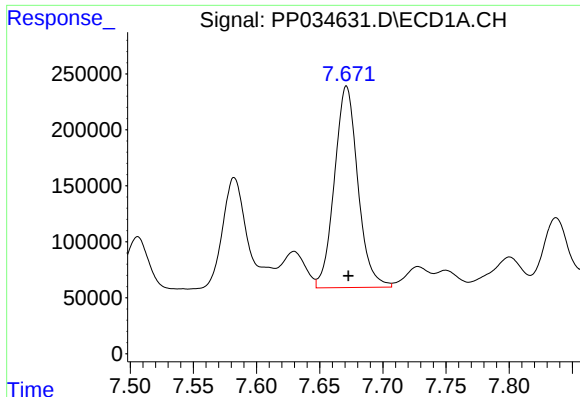


#28 AR-1254-3

R.T.: 7.671 min
Delta R.T.: -0.002 min
Response: 2321464
Conc: 508.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:42 PM

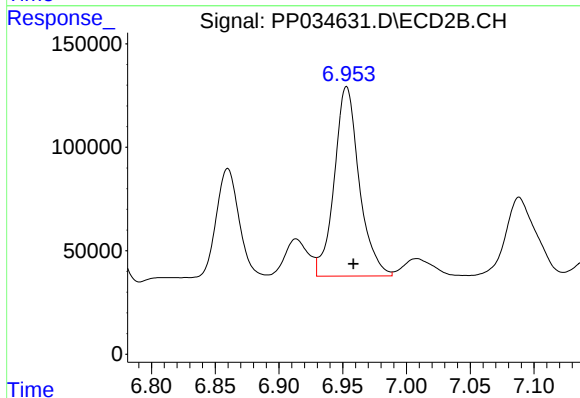


#28 AR-1254-3

R.T.: 6.953 min
Delta R.T.: -0.006 min
Response: 1243355
Conc: 498.19 ng/ml m

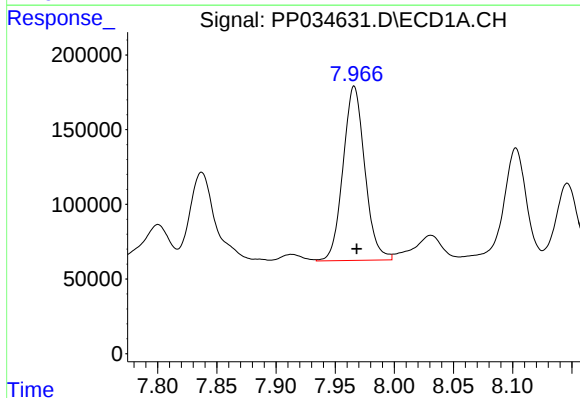


#29 AR-1254-4

R.T.: 7.966 min
Delta R.T.: -0.002 min
Response: 1493381
Conc: 483.00 ng/ml

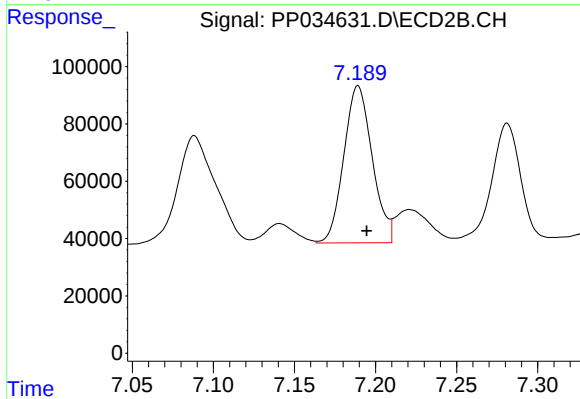

#29 AR-1254-4

R.T.: 7.189 min
Delta R.T.: -0.006 min
Response: 670476
Conc: 510.05 ng/ml m

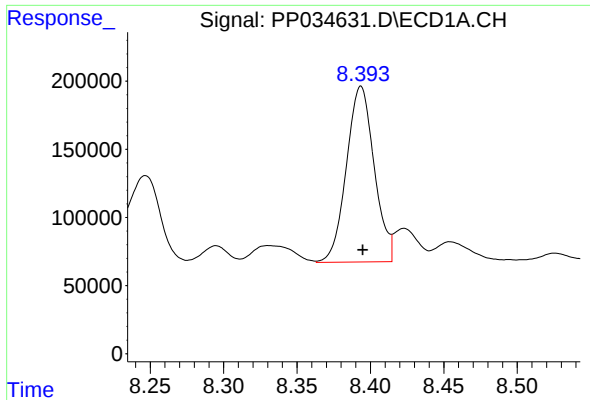


#30 AR-1254-5

R.T.: 8.394 min
Delta R.T.: -0.001 min
Response: 1697631
Conc: 477.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
4/5/2021 3:29:42 PM

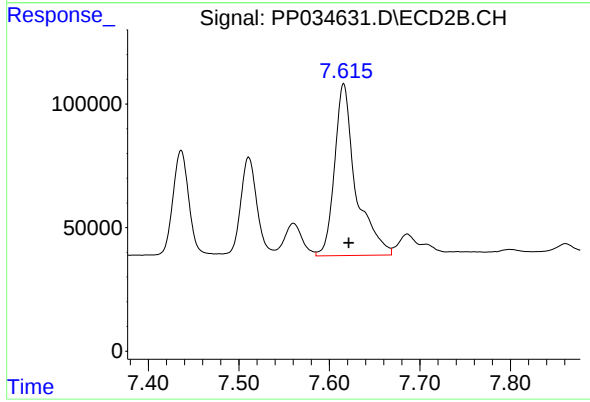

#30 AR-1254-5

R.T.: 7.616 min
Delta R.T.: -0.005 min
Response: 1130029
Conc: 556.00 ng/ml