

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040221\
 Data File : PP034640.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Apr 2021 21:32
 Operator : DD\AJ
 Sample : M1908-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FILL(0.5-1.0)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 06:36:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.845	4.256	1661142	1017904	21.776	22.659
2) SA Decachlor...	10.760	9.557	1472410	577275	19.127	20.445

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040221\
Data File : PP034640.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Apr 2021 21:32
Operator : DD\AJ
Sample : M1908-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FILL(0.5-1.0)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 06:36:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

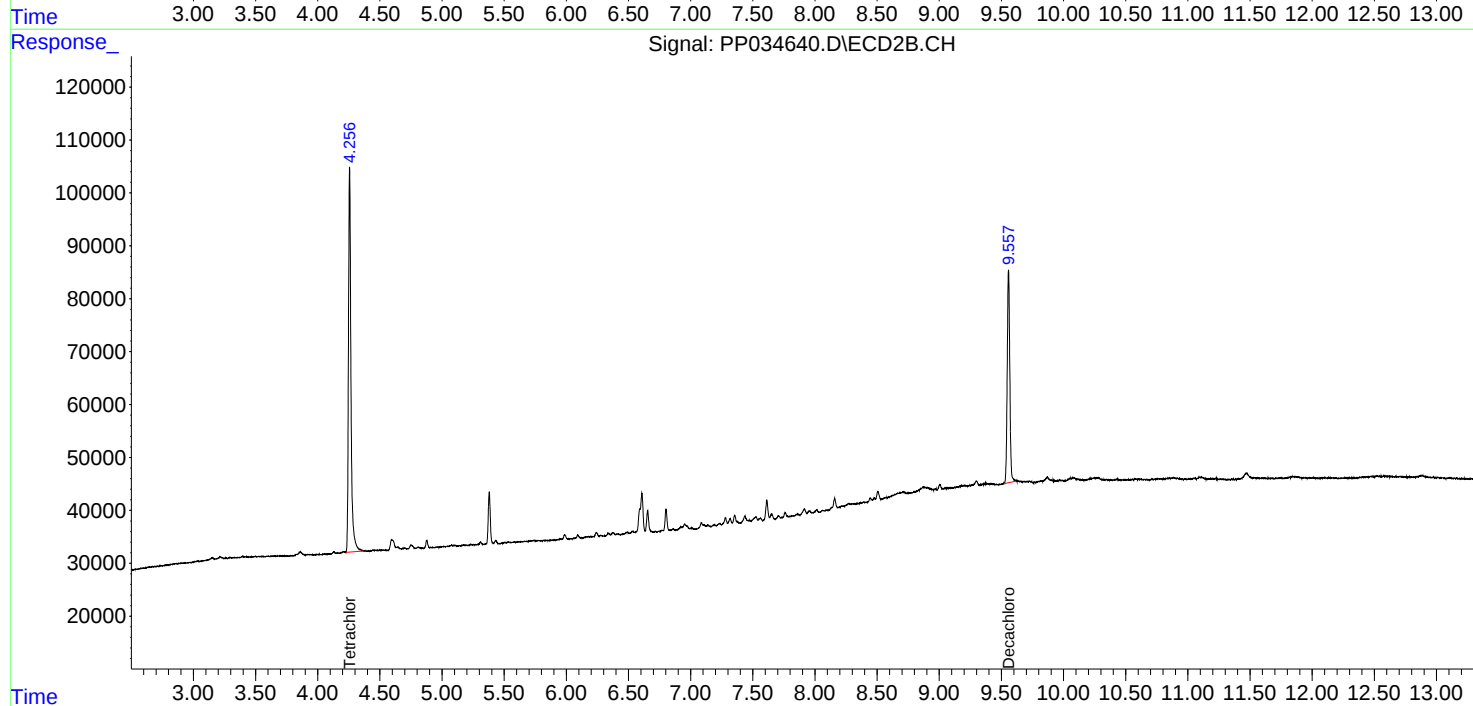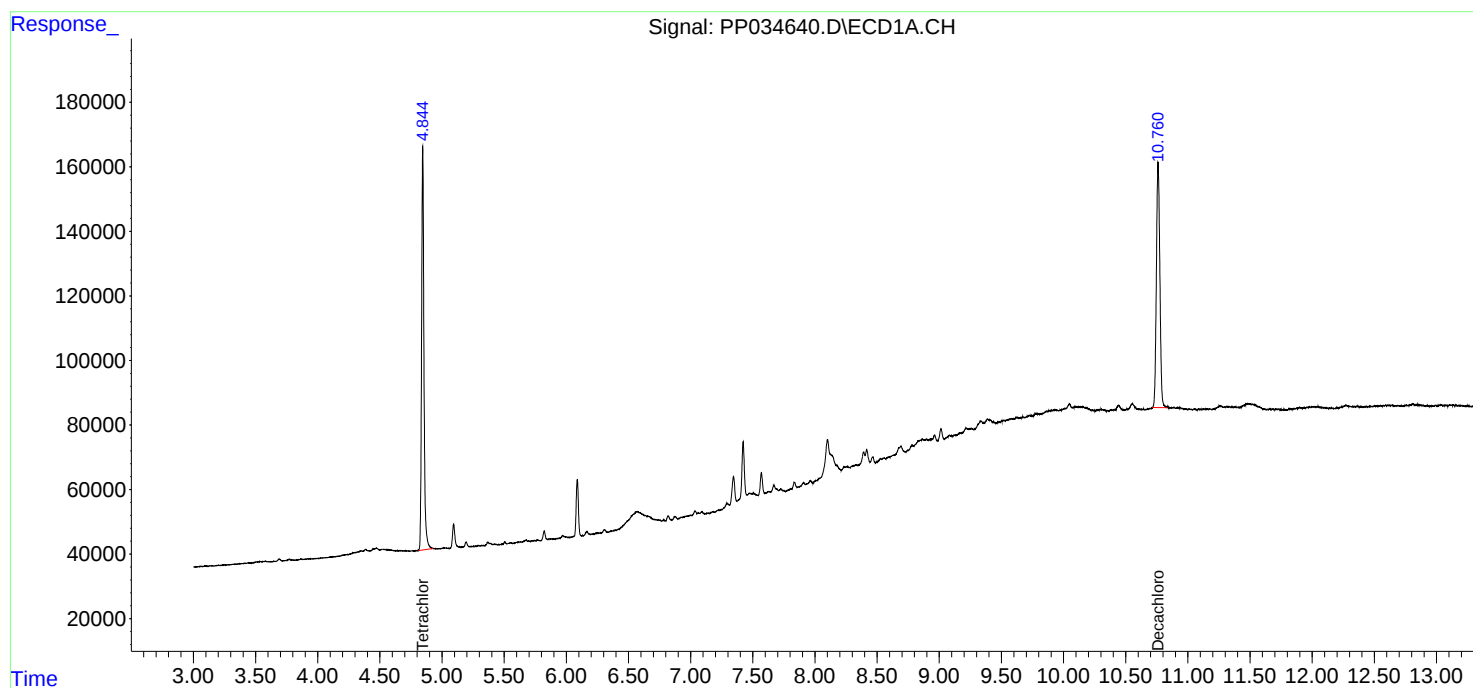


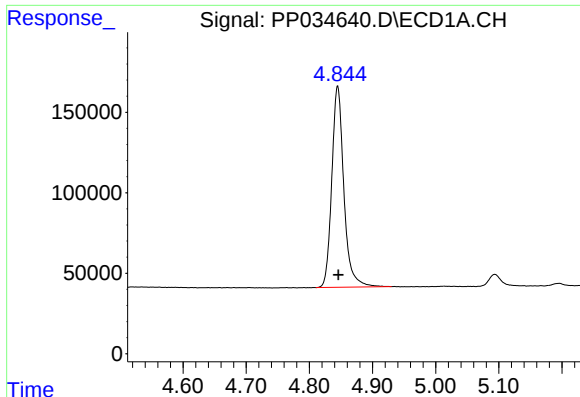

#1 Tetrachloro-m-xylene


R.T.: 4.845 min
Delta R.T.: -0.001 min
Response: 1661142
Conc: 21.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
FILL(0.5-1.0)

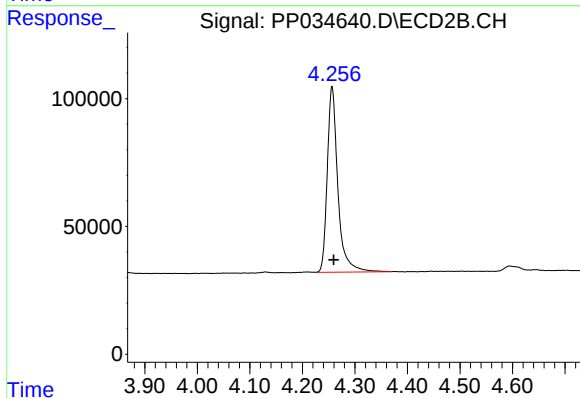


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: -0.003 min
Response: 1017904
Conc: 22.66 ng/ml

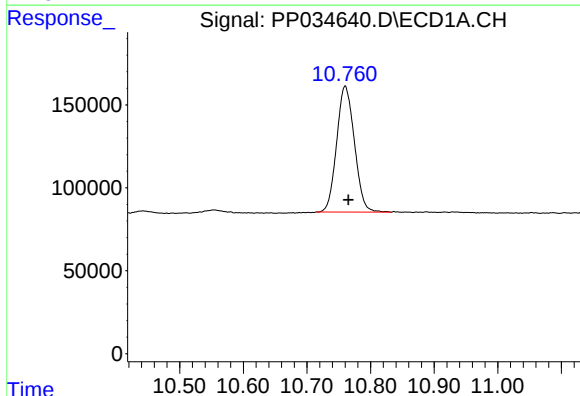

#2 Decachlorobiphenyl

R.T.: 10.760 min
Delta R.T.: -0.005 min
Response: 1472410
Conc: 19.13 ng/ml

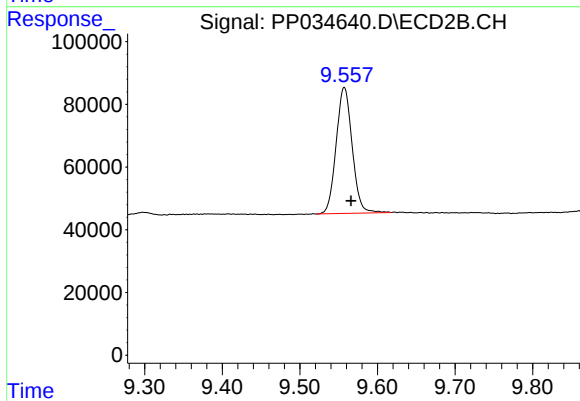

#2 Decachlorobiphenyl

R.T.: 9.557 min
Delta R.T.: -0.009 min
Response: 577275
Conc: 20.44 ng/ml