

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040323\
 Data File : PP056625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2023 23:59
 Operator : YP\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/04/2023
 Supervised By :Ankita Jodhani 04/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 03:09:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 03:08:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.435	3.663	9474252	8116123	4.682	4.937
2) SA Decachlor...	10.272	8.755	8293229	11786550	4.645	5.302
Target Compounds						
41) L9 AR-1268-1	8.718	7.620	7640552	9861266	46.418	51.268
42) L9 AR-1268-2	8.815	7.684	7538668	8864428	50.371	50.289
43) L9 AR-1268-3	9.051	7.895	6238826	8637746	45.883	52.125
44) L9 AR-1268-4	9.487	8.184	2067461	2880072	46.609	50.687
45) L9 AR-1268-5	9.918	8.487	16276979	21557862	44.078m	49.592

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040323\
Data File : PP056625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2023 23:59
Operator : YP\AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2023
Supervised By :Ankita Jodhani 04/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 03:09:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 03:08:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

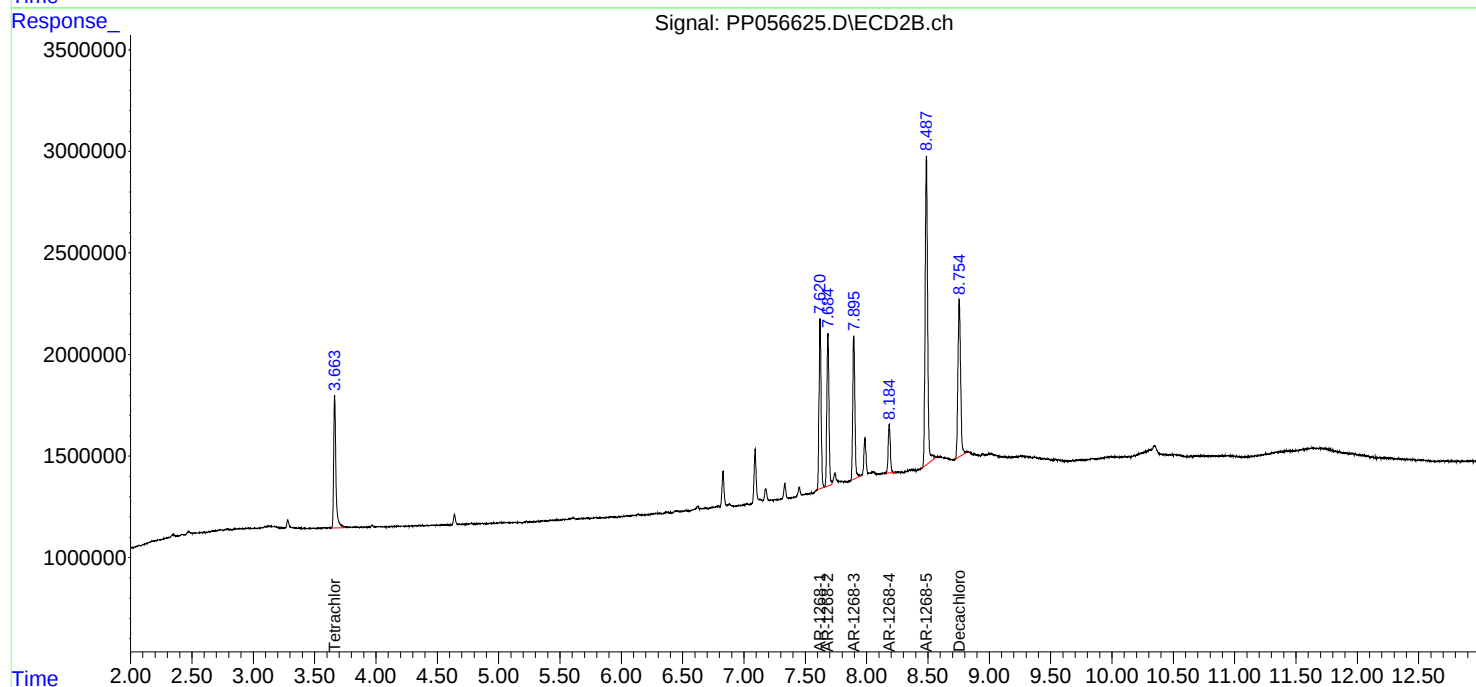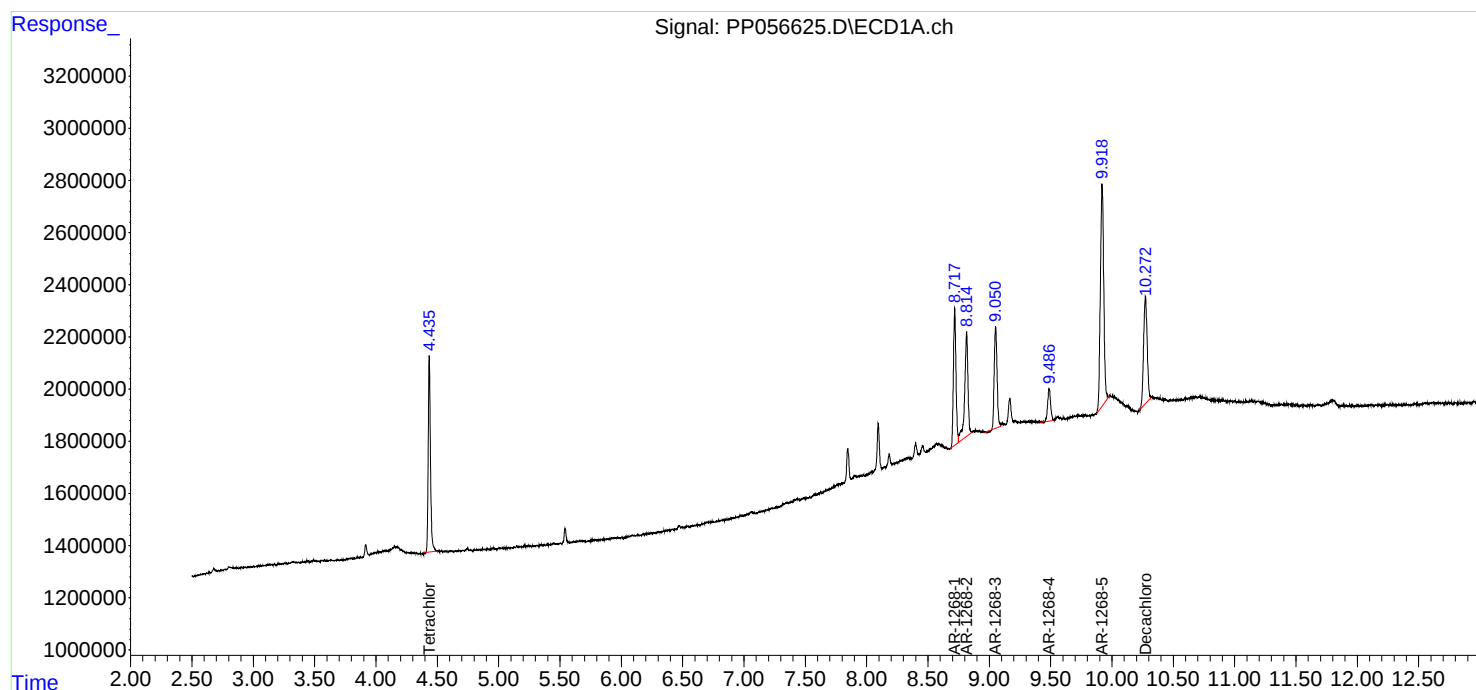

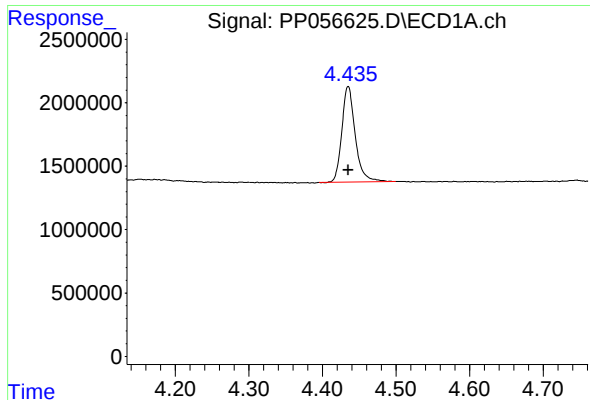


#1 Tetrachloro-m-xylene

R.T.: 4.435 min
Delta R.T.: 0.000 min
Response: 9474252
Conc: 4.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2023
Supervised By :Ankita Jodhani 04/04/2023

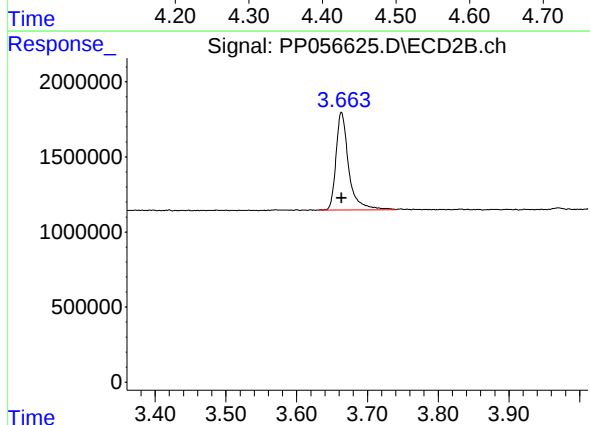


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 8116123
Conc: 4.94 ng/ml

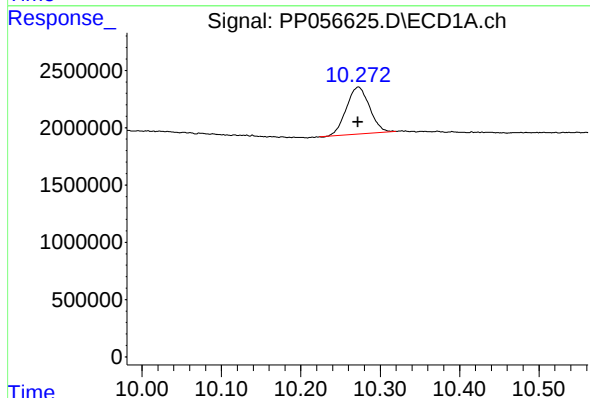


#2 Decachlorobiphenyl

R.T.: 10.272 min
Delta R.T.: 0.000 min
Response: 8293229
Conc: 4.64 ng/ml

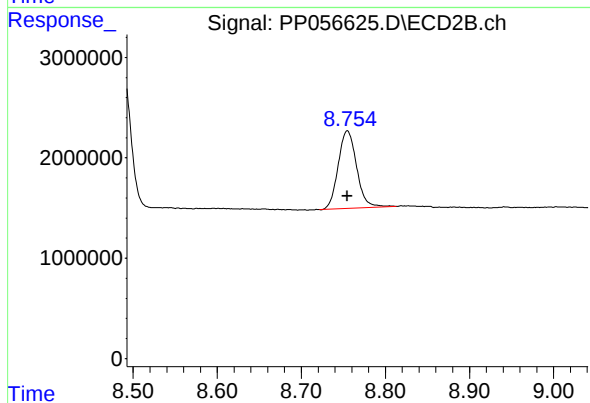

#2 Decachlorobiphenyl

R.T.: 8.755 min
Delta R.T.: 0.000 min
Response: 11786550
Conc: 5.30 ng/ml

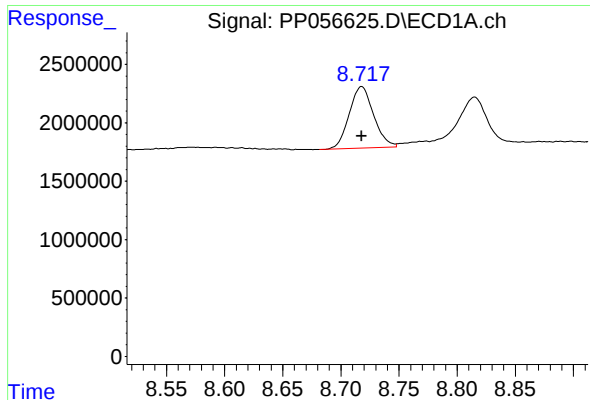


#41 AR-1268-1

R.T.: 8.718 min
Delta R.T.: 0.000 min
Response: 7640552
Conc: 46.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2023
Supervised By :Ankita Jodhani 04/04/2023

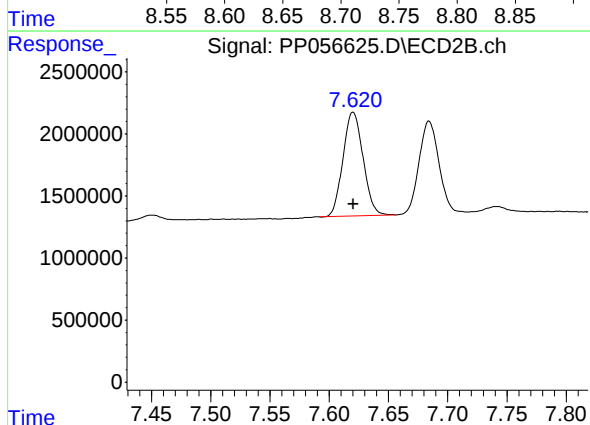


#41 AR-1268-1

R.T.: 7.620 min
Delta R.T.: 0.000 min
Response: 9861266
Conc: 51.27 ng/ml

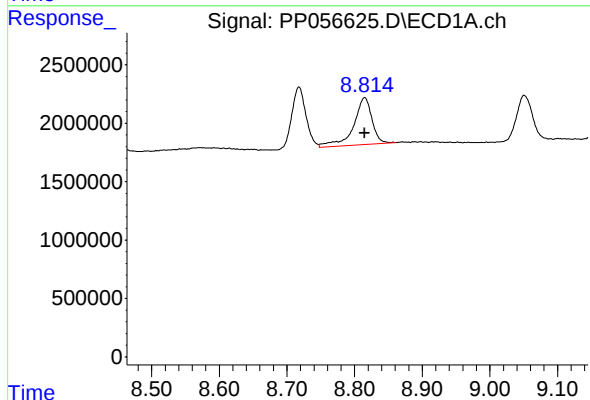


#42 AR-1268-2

R.T.: 8.815 min
Delta R.T.: 0.000 min
Response: 7538668
Conc: 50.37 ng/ml

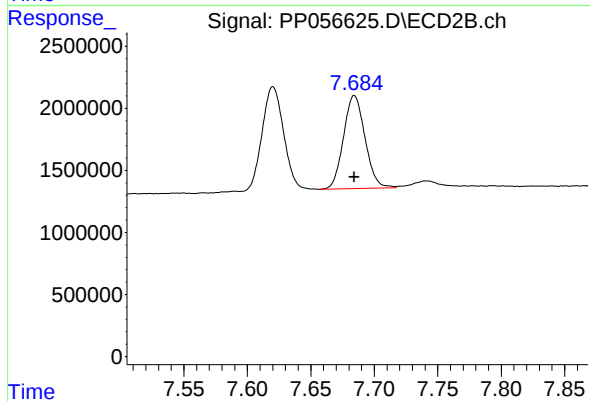

#42 AR-1268-2

R.T.: 7.684 min
Delta R.T.: 0.000 min
Response: 8864428
Conc: 50.29 ng/ml

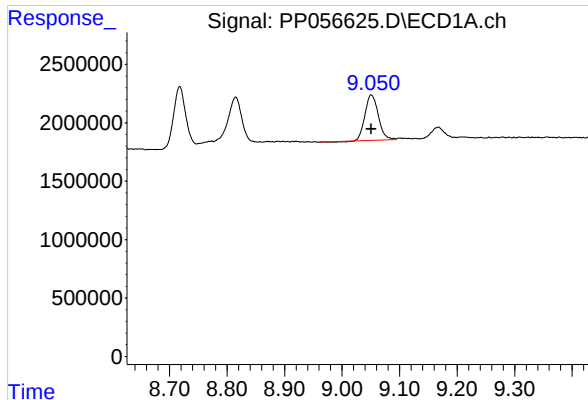


#43 AR-1268-3

R.T.: 9.051 min
Delta R.T.: 0.000 min
Response: 6238826
Conc: 45.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2023
Supervised By :Ankita Jodhani 04/04/2023

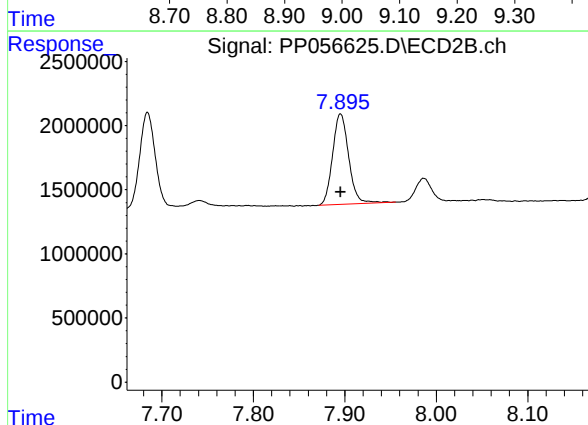


#43 AR-1268-3

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 8637746
Conc: 52.12 ng/ml

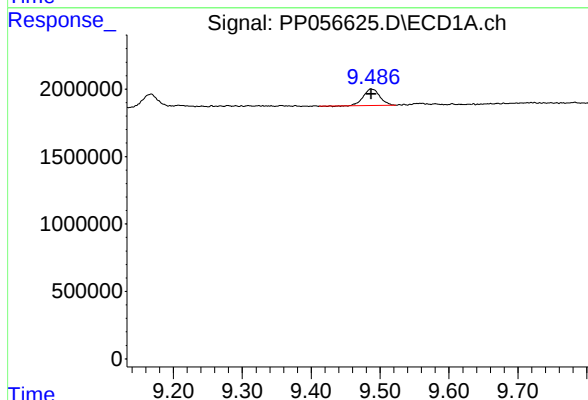


#44 AR-1268-4

R.T.: 9.487 min
Delta R.T.: 0.000 min
Response: 2067461
Conc: 46.61 ng/ml

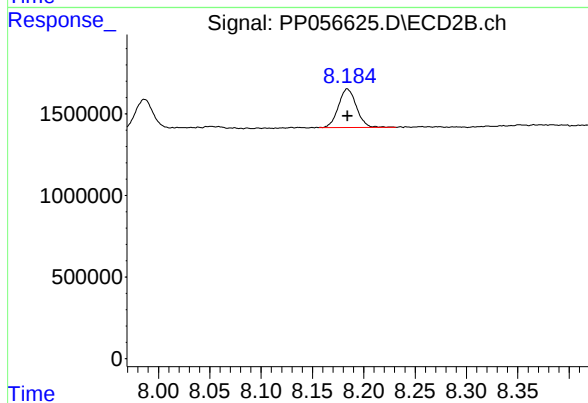

#44 AR-1268-4

R.T.: 8.184 min
Delta R.T.: 0.000 min
Response: 2880072
Conc: 50.69 ng/ml

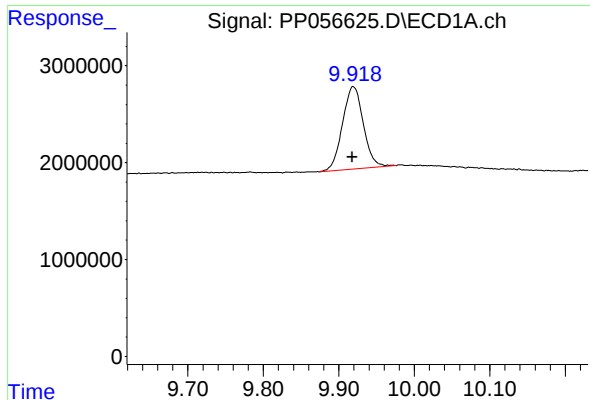


#45 AR-1268-5

R.T.: 9.918 min
Delta R.T.: 0.000 min
Response: 16276979
Conc: 44.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2023
Supervised By :Ankita Jodhani 04/04/2023

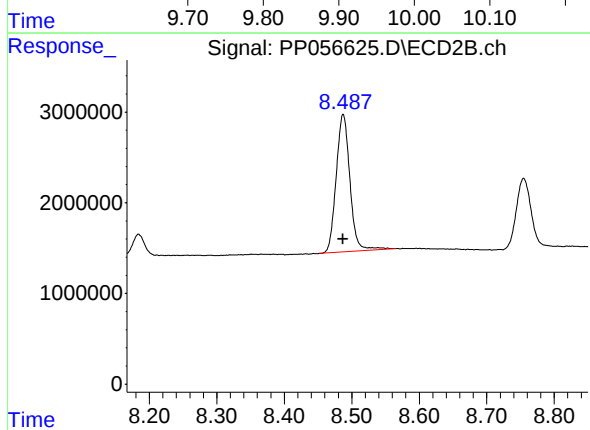

#45 AR-1268-5

R.T.: 8.487 min
Delta R.T.: 0.000 min
Response: 21557862
Conc: 49.59 ng/ml