

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040325\
 Data File : PP071079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2025 19:54
 Operator : YP\AJ
 Sample : Q1710-01 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 34848

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/04/2025
 Supervised By :mohammad ahmed 04/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 01:55:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.508	3.822	13785721	7249323	9.432m	6.993 #
2) SA Decachlor...	10.215	8.862	10241003	6949577	9.729m	8.817

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040325\
Data File : PP071079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2025 19:54
Operator : YP\AJ
Sample : Q1710-01 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
34848


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2025
Supervised By :mohammad ahmed 04/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 01:55:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

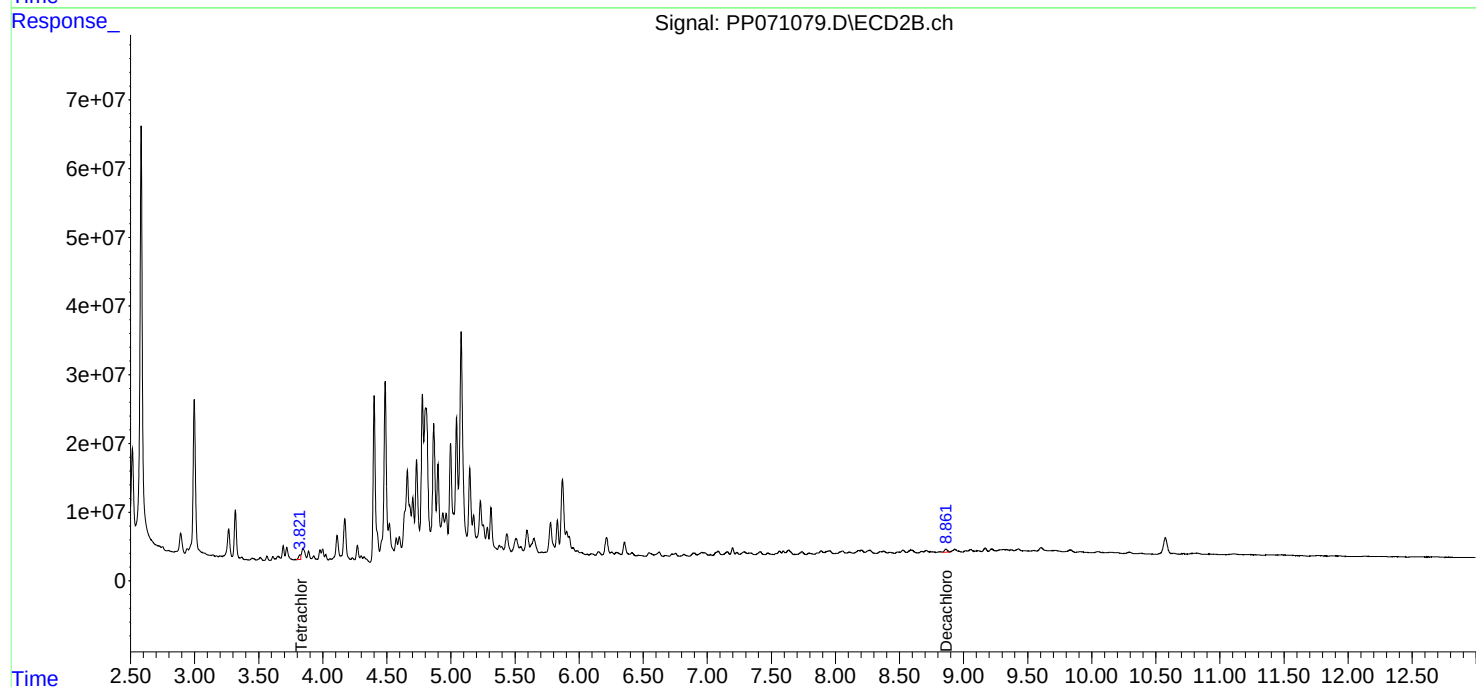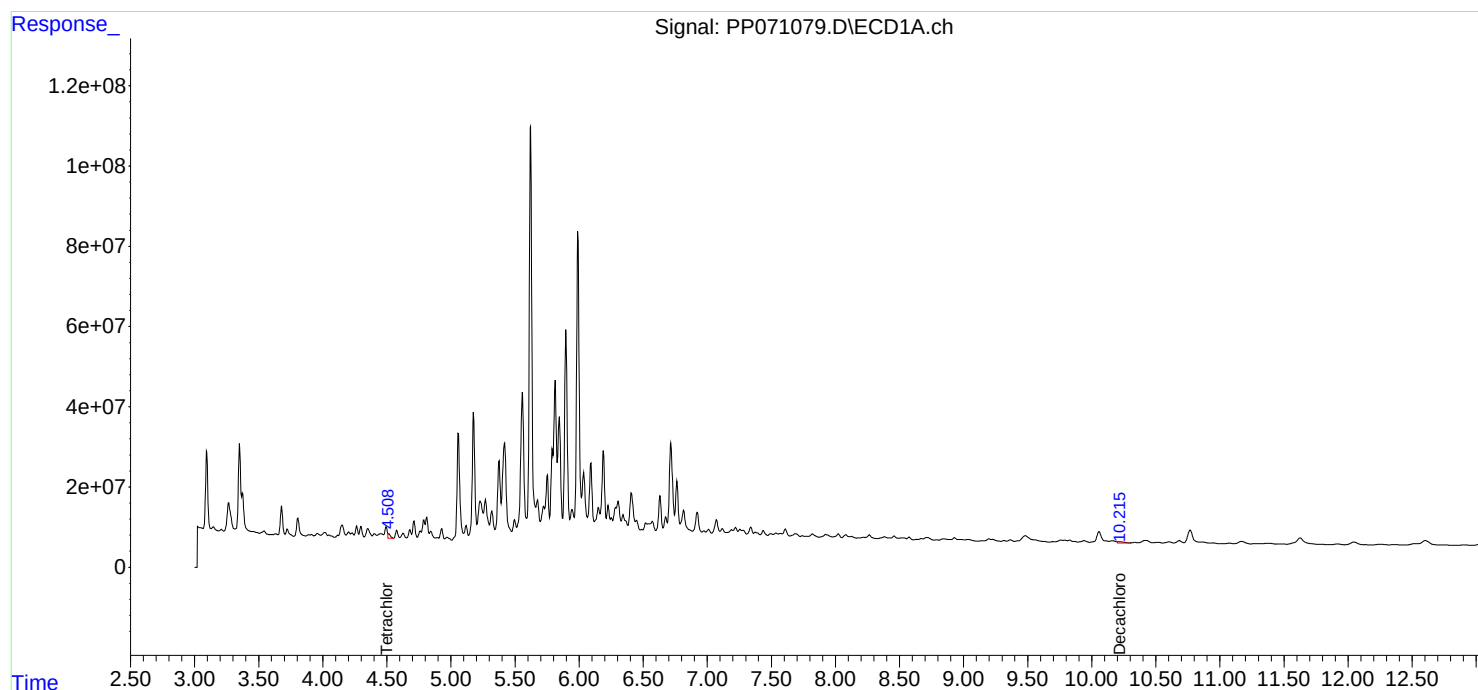

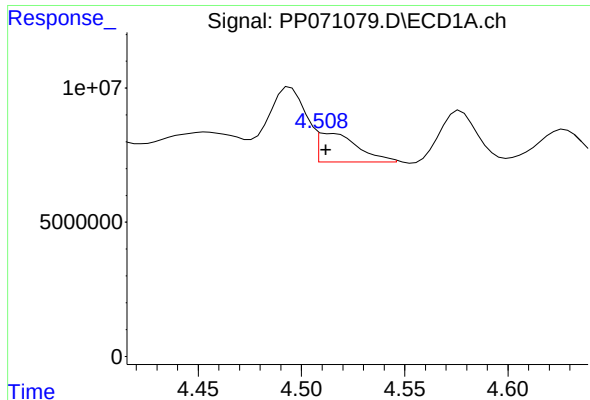


#1 Tetrachloro-m-xylene

R.T.: 4.508 min
Delta R.T.: -0.004 min
Response: 13785721
Conc: 9.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
34848


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/04/2025
Supervised By :mohammad ahmed 04/05/2025

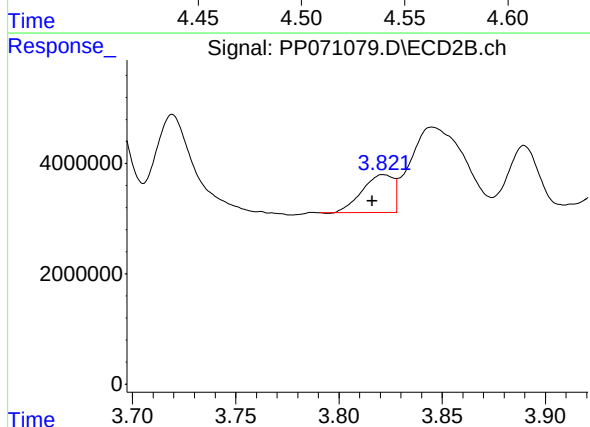


#1 Tetrachloro-m-xylene

R.T.: 3.822 min
Delta R.T.: 0.006 min
Response: 7249323
Conc: 6.99 ng/ml

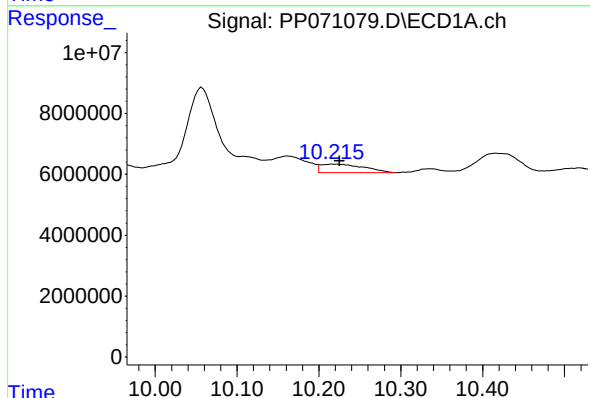

#2 Decachlorobiphenyl

R.T.: 10.215 min
Delta R.T.: -0.010 min
Response: 10241003
Conc: 9.73 ng/ml m

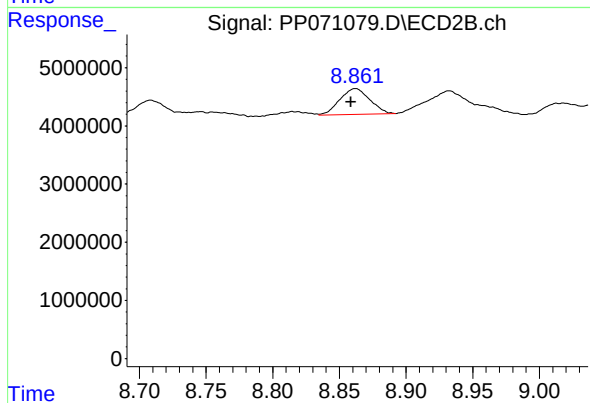

#2 Decachlorobiphenyl

R.T.: 8.862 min
Delta R.T.: 0.003 min
Response: 6949577
Conc: 8.82 ng/ml