

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040422\
 Data File : PP045458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2022 13:15
 Operator : YP\AJ
 Sample : N2205-04 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-032322-SR-04

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/05/2022
 Supervised By :mohammad ahmed 04/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 06:15:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 31 07:54:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.886	3.145	4134317	3854624	1.713m	2.436m#
2) SA Decachlor...	9.999	8.494	814204	4633542	0.568m	3.056 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040422\
Data File : PP045458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2022 13:15
Operator : YP\AJ
Sample : N2205-04 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-032322-SR-04


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2022
Supervised By :mohammad ahmed 04/05/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 06:15:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 31 07:54:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

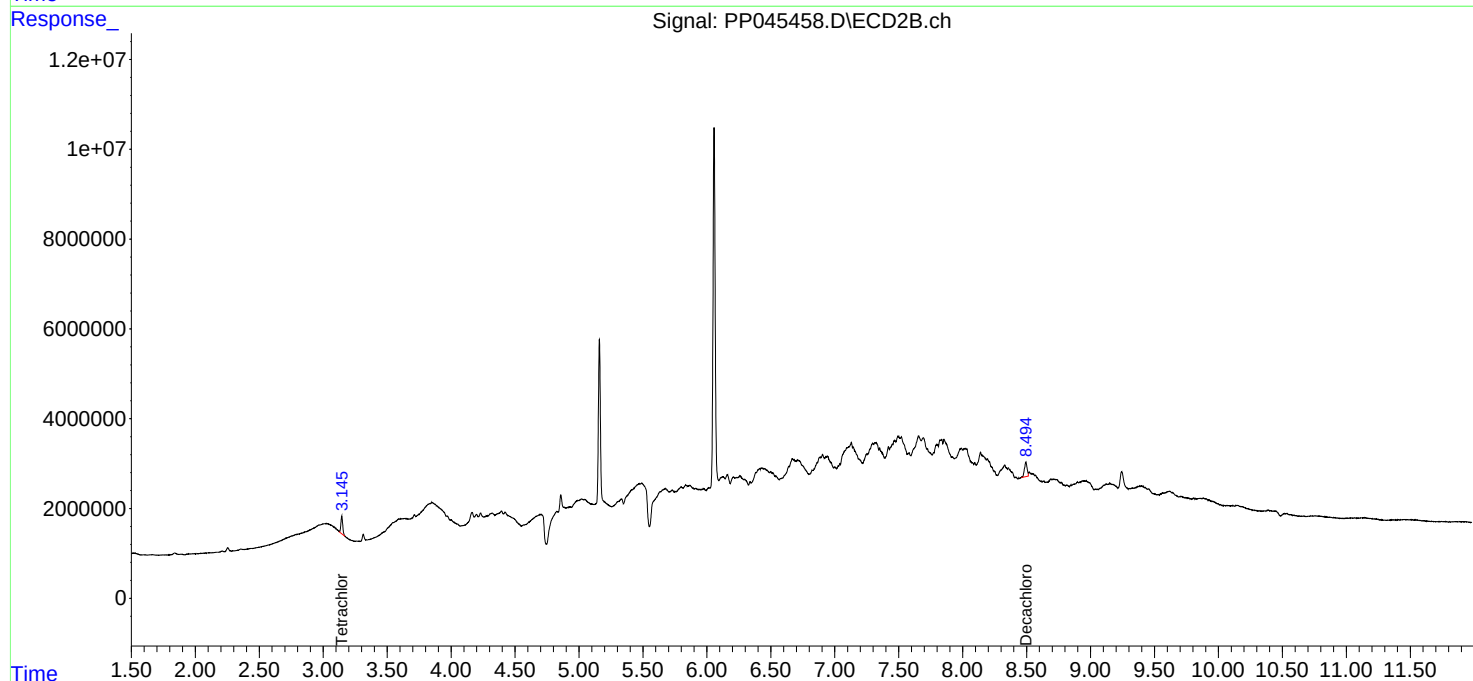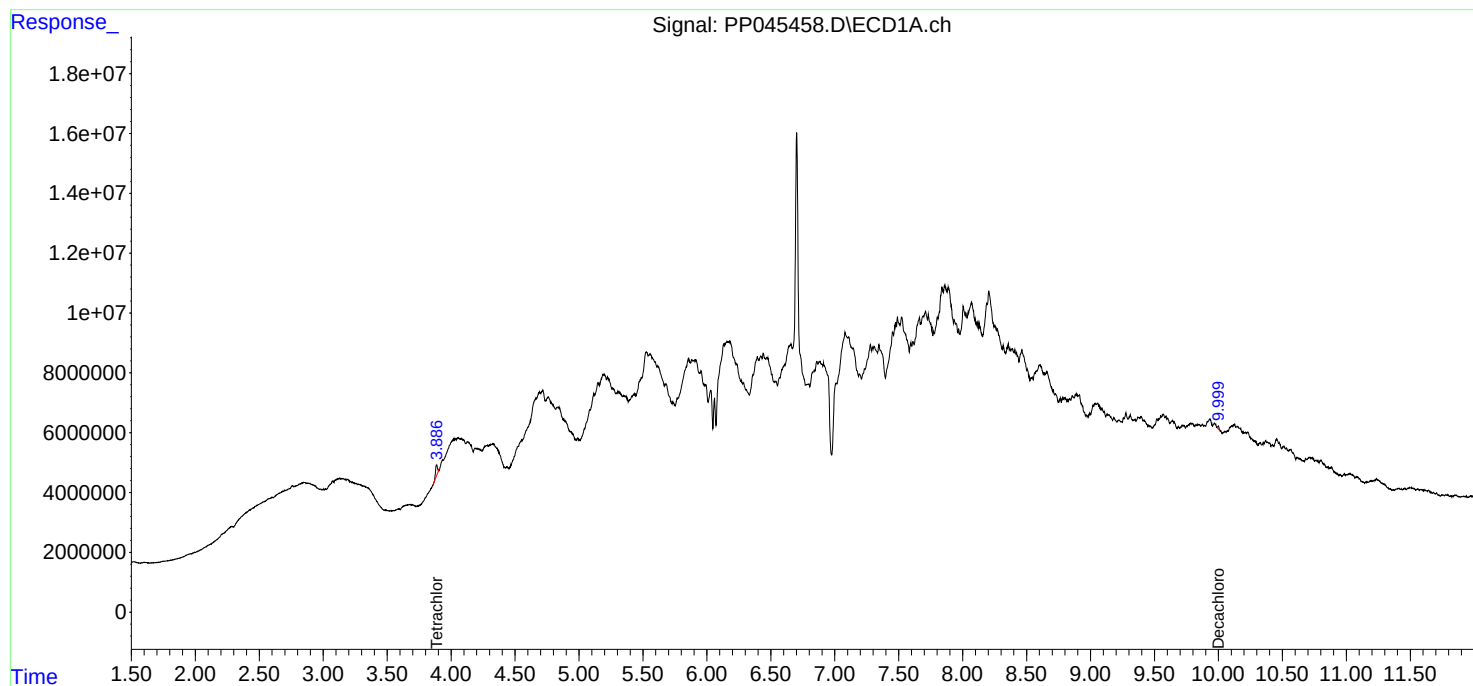

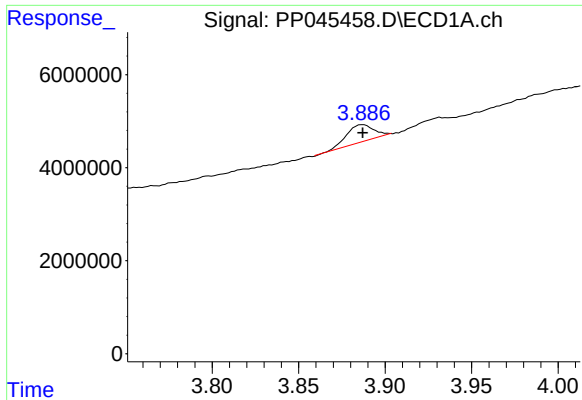


#1 Tetrachloro-m-xylene

R.T.: 3.886 min
Delta R.T.: 0.000 min
Response: 4134317
Conc: 1.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-032322-SR-04


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2022
Supervised By :mohammad ahmed 04/05/2022

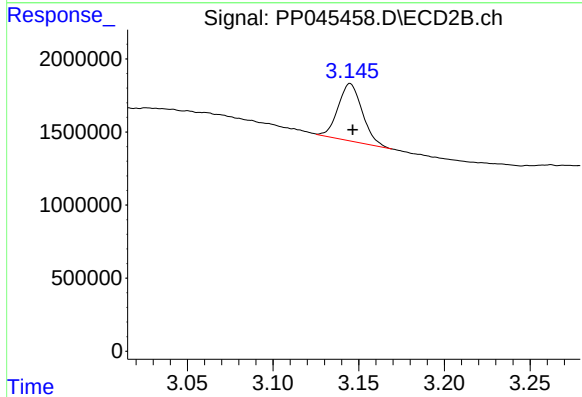


#1 Tetrachloro-m-xylene

R.T.: 3.145 min
Delta R.T.: -0.002 min
Response: 3854624
Conc: 2.44 ng/ml m

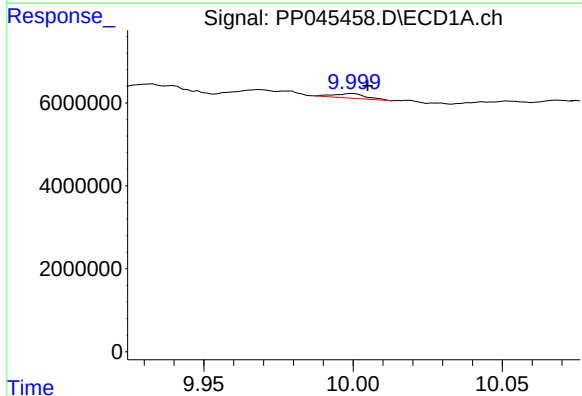

#2 Decachlorobiphenyl

R.T.: 9.999 min
Delta R.T.: -0.005 min
Response: 814204
Conc: 0.57 ng/ml m

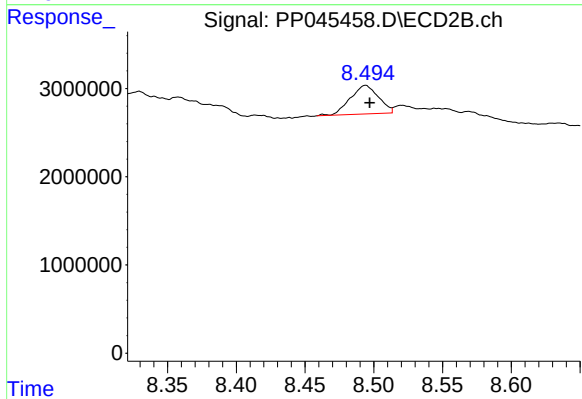

#2 Decachlorobiphenyl

R.T.: 8.494 min
Delta R.T.: -0.003 min
Response: 4633542
Conc: 3.06 ng/ml