

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040422\
 Data File : PP045492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2022 23:51
 Operator : YP\AJ
 Sample : N2207-10
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-096-21-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 06:47:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 31 07:54:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.888	3.147	44300138	29675314	18.360	18.754
2) SA Decachlor...	9.996	8.491	28846463	29397868	20.132	19.386

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040422\
Data File : PP045492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2022 23:51
Operator : YP\AJ
Sample : N2207-10
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SPLP-LEACHATE-AMENDED-096-21-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 06:47:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033022.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 31 07:54:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

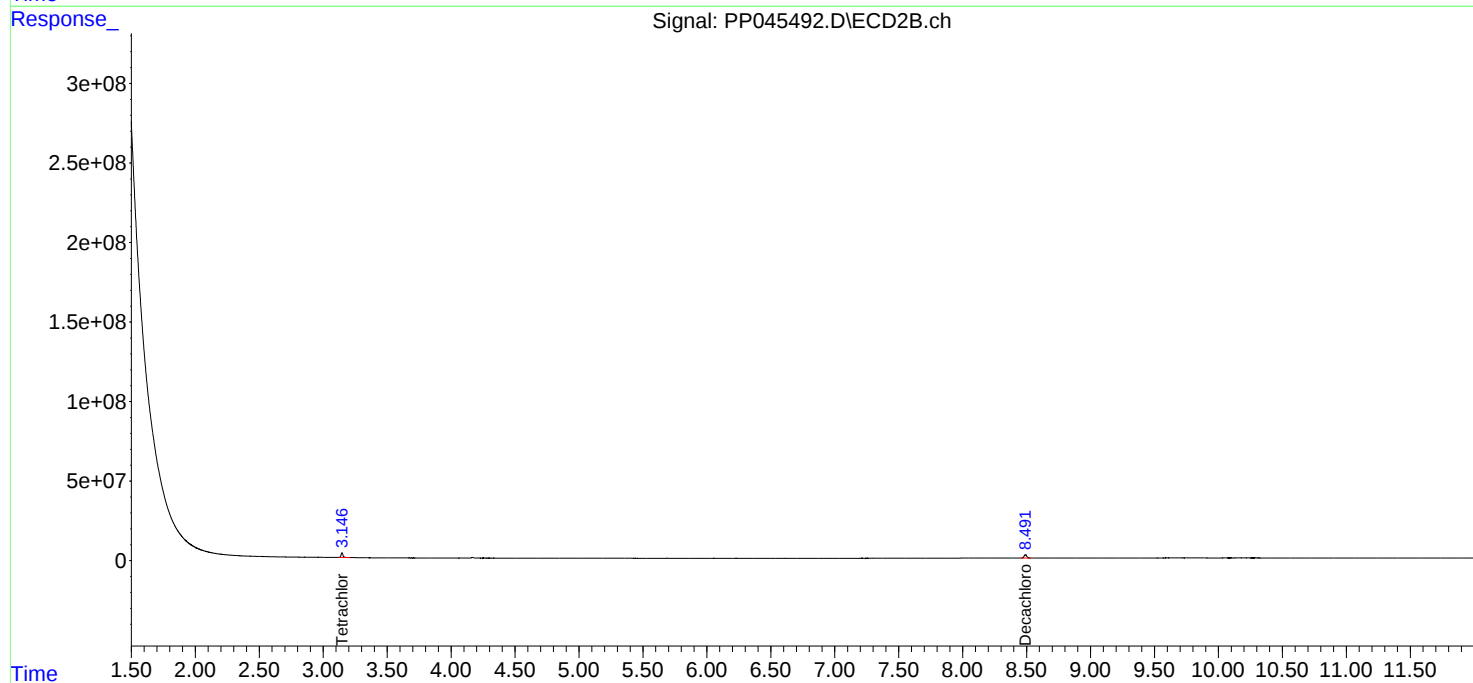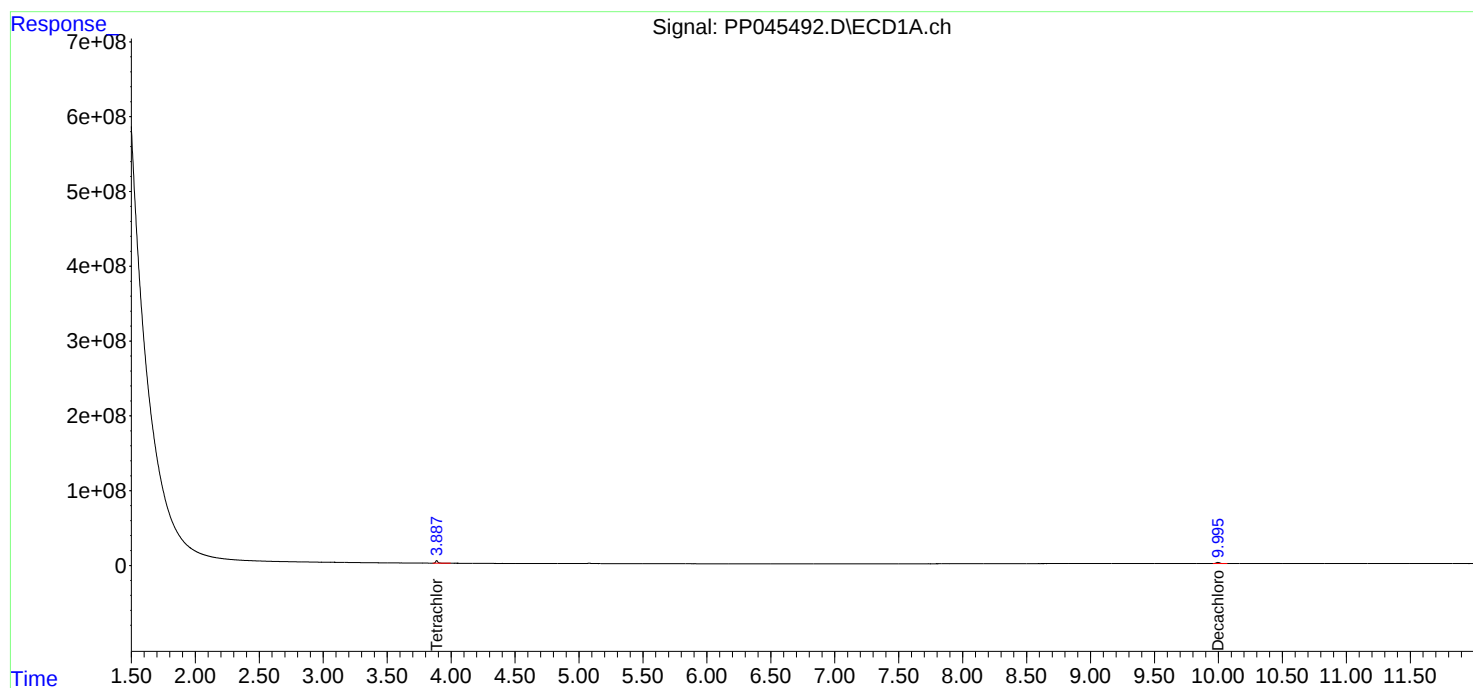

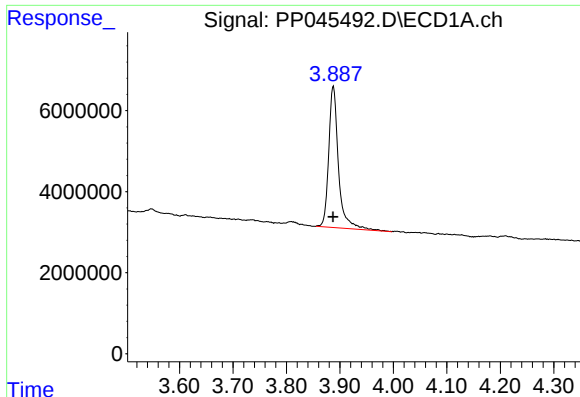

#1 Tetrachloro-m-xylene


R.T.: 3.888 min
Delta R.T.: 0.000 min
Response: 44300138
Conc: 18.36 ng/ml

Instrument :

ECD_P


ClientSampleId :

SPLP-LEACHATE-AMENDED-096-21-02

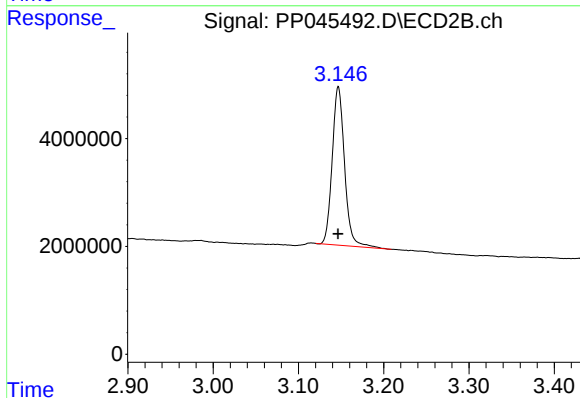


#1 Tetrachloro-m-xylene

R.T.: 3.147 min
Delta R.T.: 0.000 min
Response: 29675314
Conc: 18.75 ng/ml

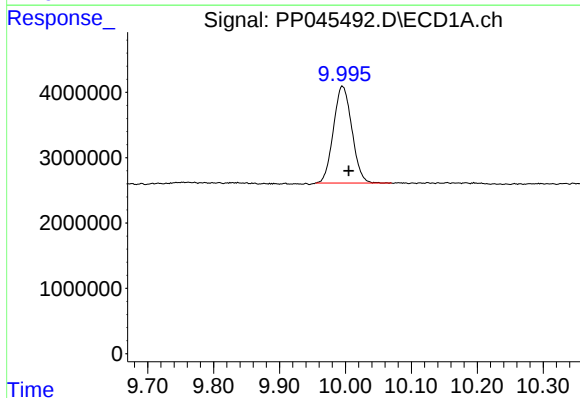

#2 Decachlorobiphenyl

R.T.: 9.996 min
Delta R.T.: -0.009 min
Response: 28846463
Conc: 20.13 ng/ml

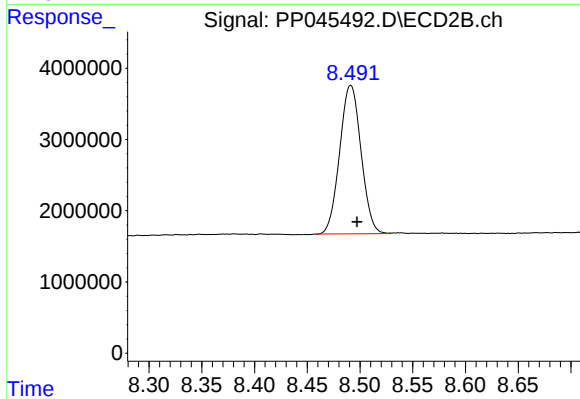

#2 Decachlorobiphenyl

R.T.: 8.491 min
Delta R.T.: -0.006 min
Response: 29397868
Conc: 19.39 ng/ml