

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040423\
 Data File : PP056653.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2023 18:50
 Operator : YP\AJ
 Sample : 02179-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-86-02

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/05/2023
 Supervised By :Ankita Jodhani 04/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 22:01:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 03:37:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.438	3.666	48303747	38762131	24.409	24.054
2) SA Decachlor...	10.275	8.757	31969283	36919055	33.305	30.299

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040423\
Data File : PP056653.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2023 18:50
Operator : YP\AJ
Sample : 02179-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-86-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2023
Supervised By :Ankita Jodhani 04/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 22:01:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 03:37:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

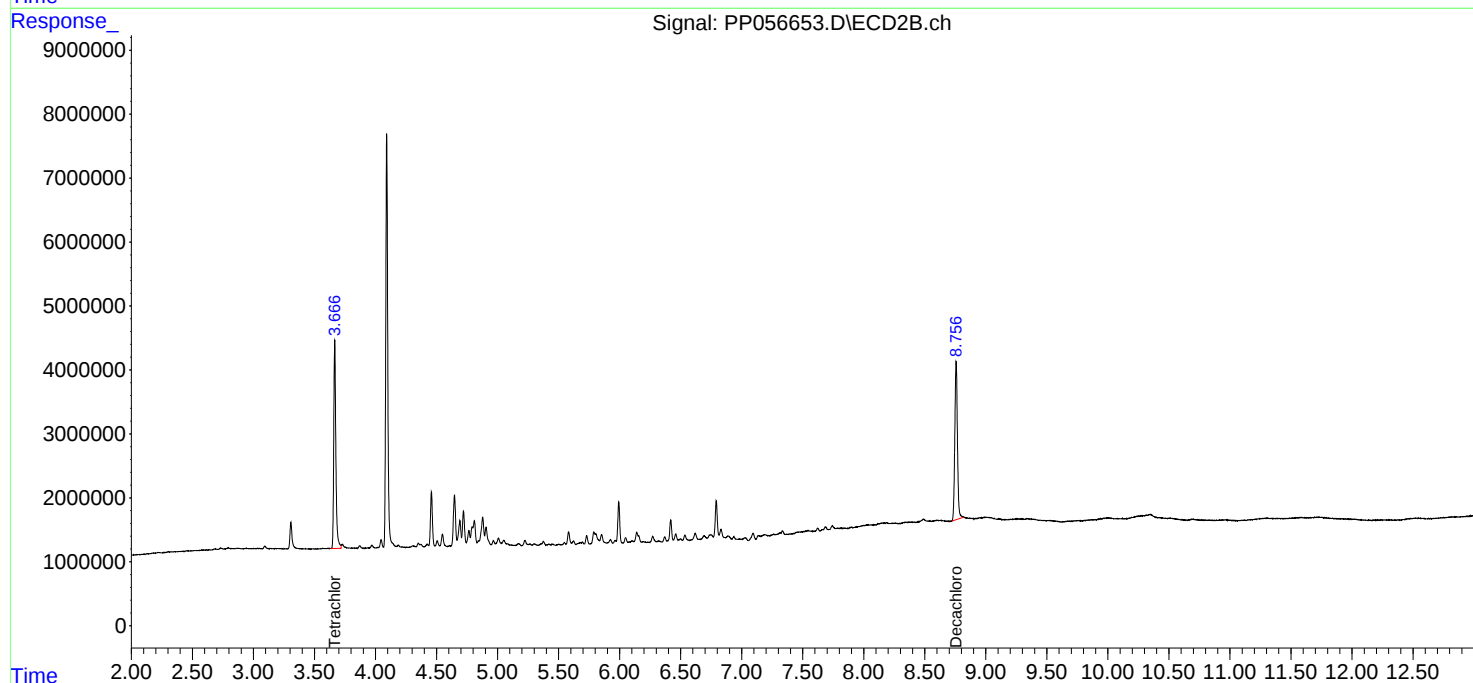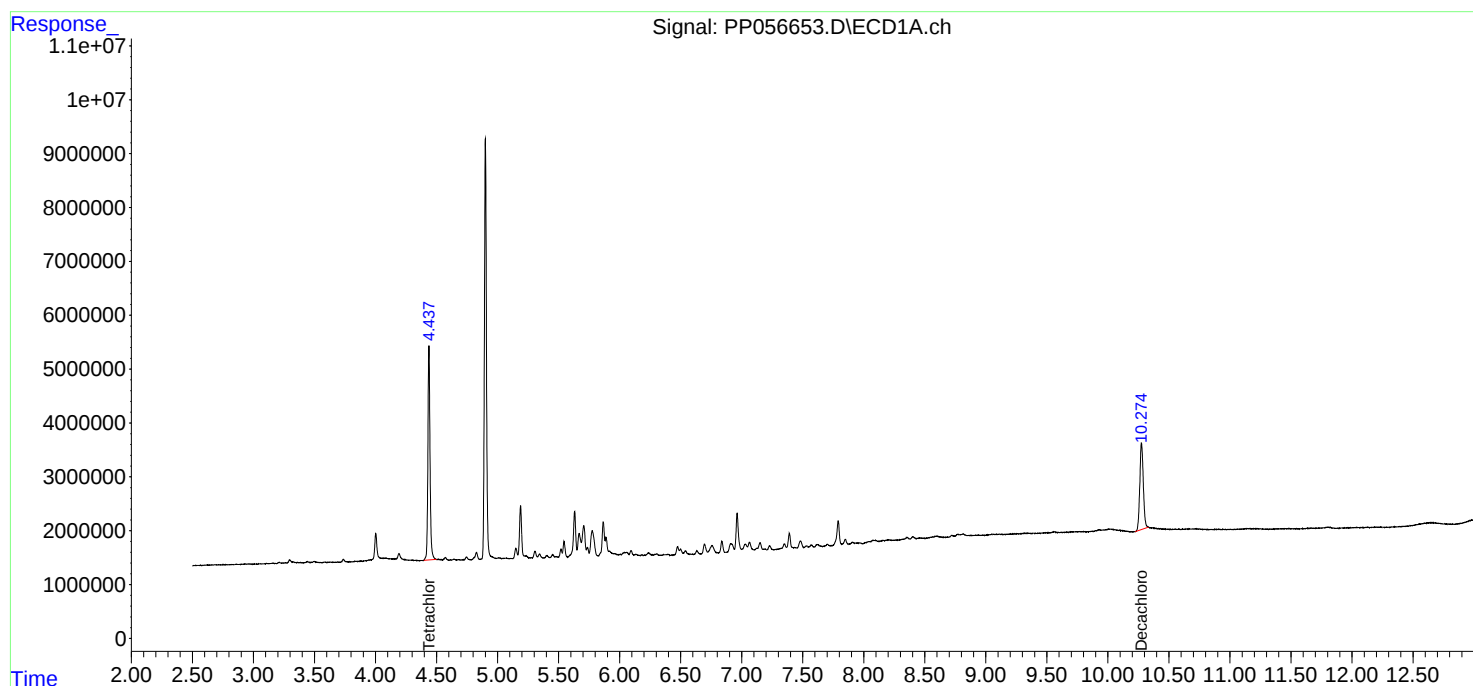

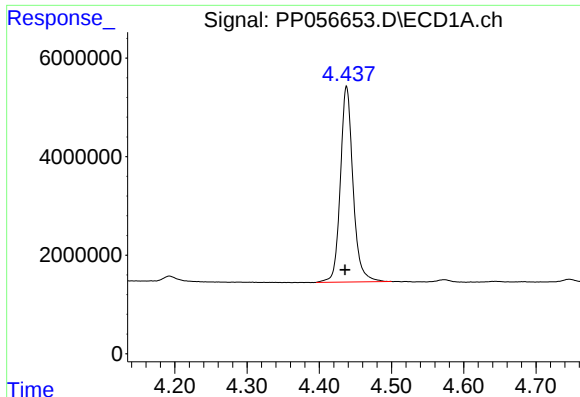


#1 Tetrachloro-m-xylene

R.T.: 4.438 min
Delta R.T.: 0.002 min
Response: 48303747
Conc: 24.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-86-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/05/2023
Supervised By :Ankita Jodhani 04/05/2023

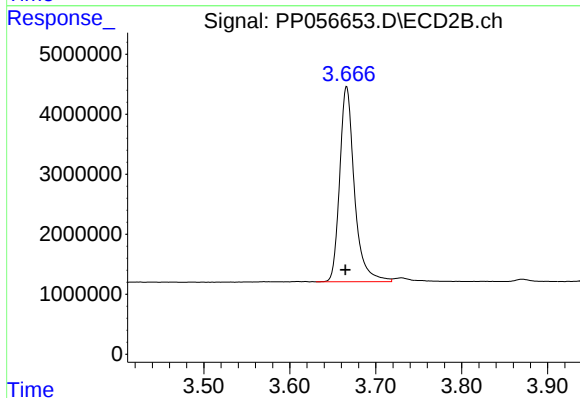


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.001 min
Response: 38762131
Conc: 24.05 ng/ml

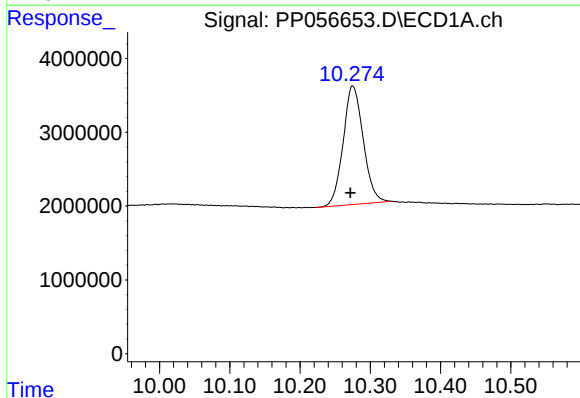

#2 Decachlorobiphenyl

R.T.: 10.275 min
Delta R.T.: 0.003 min
Response: 31969283
Conc: 33.31 ng/ml

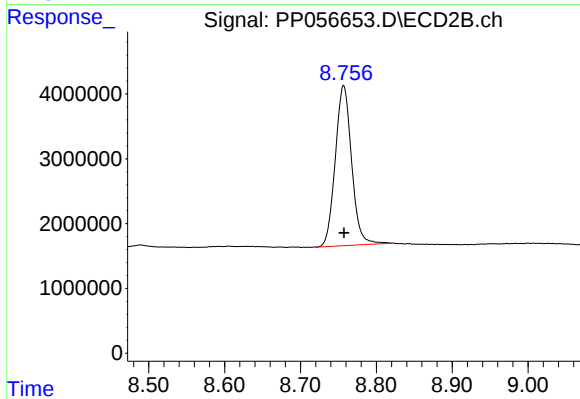

#2 Decachlorobiphenyl

R.T.: 8.757 min
Delta R.T.: 0.000 min
Response: 36919055
Conc: 30.30 ng/ml