

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040521\
 Data File : PP034677.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2021 14:49
 Operator : DD\AJ
 Sample : M1919-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MSRO-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 03:06:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.846	4.257	1875112	1116283	24.581	24.849
2)	SA Decachlor...	10.767	9.559	2086554	813758	27.105	28.820
Target Compounds							
3)	L1 AR-1016-1	0.000	5.533f	0	10493	N.D.	8.845 #
4)	L1 AR-1016-2	0.000	5.533	0	10493	N.D.	5.909 #
5)	L1 AR-1016-3	0.000	5.714	0	17103	N.D.	18.305 #
6)	L1 AR-1016-4	6.341	5.785	14006	7275	7.865	10.017 #
7)	L1 AR-1016-5	0.000	5.992	0	24788	N.D.	27.100 #
8)	L2 AR-1221-1	5.095	0.000	830029	0	1135.442	N.D. #
9)	L2 AR-1221-2	5.195	4.591f	22832	340672	40.082	976.494 #
10)	L2 AR-1221-3	5.293	4.699	105754	54451	58.109	51.906
11)	L3 AR-1232-1	5.293	4.699	105754	54451	71.205	64.459
12)	L3 AR-1232-2	0.000	5.533	0	10493	N.D.	13.942 #
13)	L3 AR-1232-3	0.000	5.714	0	17103	N.D.	43.090 #
14)	L3 AR-1232-4	6.341	5.834f	14006	8197	19.498	23.830
15)	L3 AR-1232-5	0.000	5.992	0	24788	N.D.	69.734 #
16)	L4 AR-1242-1	0.000	5.533f	0	10493	N.D.	11.199 #
17)	L4 AR-1242-2	0.000	5.533	0	10493	N.D.	7.381 #
18)	L4 AR-1242-3	0.000	5.714	0	17103	N.D.	22.907 #
19)	L4 AR-1242-4	6.341	5.834	14006	8197	10.015	11.140
20)	L4 AR-1242-5	0.000	6.382	0	79281	N.D.	96.688 #
21)	L5 AR-1248-1	0.000	5.533f	0	10493	N.D.	14.383 #
22)	L5 AR-1248-2	0.000	5.785	0	7275	N.D.	7.087 #
23)	L5 AR-1248-3	0.000	5.834	0	8197	N.D.	7.479 #
24)	L5 AR-1248-4	7.096	5.992	62470	24788	24.480	19.639
25)	L5 AR-1248-5	0.000	6.419	0	19281	N.D.	17.061 #
26)	L6 AR-1254-1	7.073	6.382	113923	79281	41.434	42.973
27)	L6 AR-1254-2	7.297	6.530	177511	27974	41.746	17.485 #
28)	L6 AR-1254-3	7.675	6.955	128136	52664	28.074	21.101
29)	L6 AR-1254-4	7.968	7.190	589153	35084	190.550	26.689 #
30)	L6 AR-1254-5	8.401	7.613	289326	80111	81.412	39.417 #
31)	L7 AR-1260-1	7.837	7.088	35478	72436	11.429	47.169 #
32)	L7 AR-1260-2	8.100	7.287	299213	67803	79.675	37.535 #
33)	L7 AR-1260-3	8.467	7.438	40094	36104	13.264	20.811 #
34)	L7 AR-1260-4	8.692	7.927	430317	165706	123.257	115.574
35)	L7 AR-1260-5	9.016	8.158	59717	31921	8.338	9.345
36)	L8 AR-1262-1	8.467	7.613	40094	80111	8.762	74.592 #
37)	L8 AR-1262-2	9.016	8.158	59717	31921	7.654	9.304
38)	L8 AR-1262-3	9.339f	8.443	65676	6311	12.204	4.212 #
39)	L8 AR-1262-4	9.415	8.509	56175	20973	12.649	7.615 #
40)	L8 AR-1262-5	0.000	9.004	0	5603	N.D.	4.938 #
41)	L9 AR-1268-1	9.293f	8.443	124978	6311	12.483	1.461 #
42)	L9 AR-1268-2	9.415	8.509	56175	20973	5.873	5.067

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040521\
 Data File : PP034677.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2021 14:49
 Operator : DD\AJ
 Sample : M1919-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MSRO-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 03:06:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	8.720	0	44696	N.D.	12.286 #
44) L9	AR-1268-4	0.000	9.004	0	5603	N.D.	4.349 #
45) L9	AR-1268-5	10.446	9.303	44319	33525	1.552	3.228 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040521\
Data File : PP034677.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2021 14:49
Operator : DD\AJ
Sample : M1919-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 03:06:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

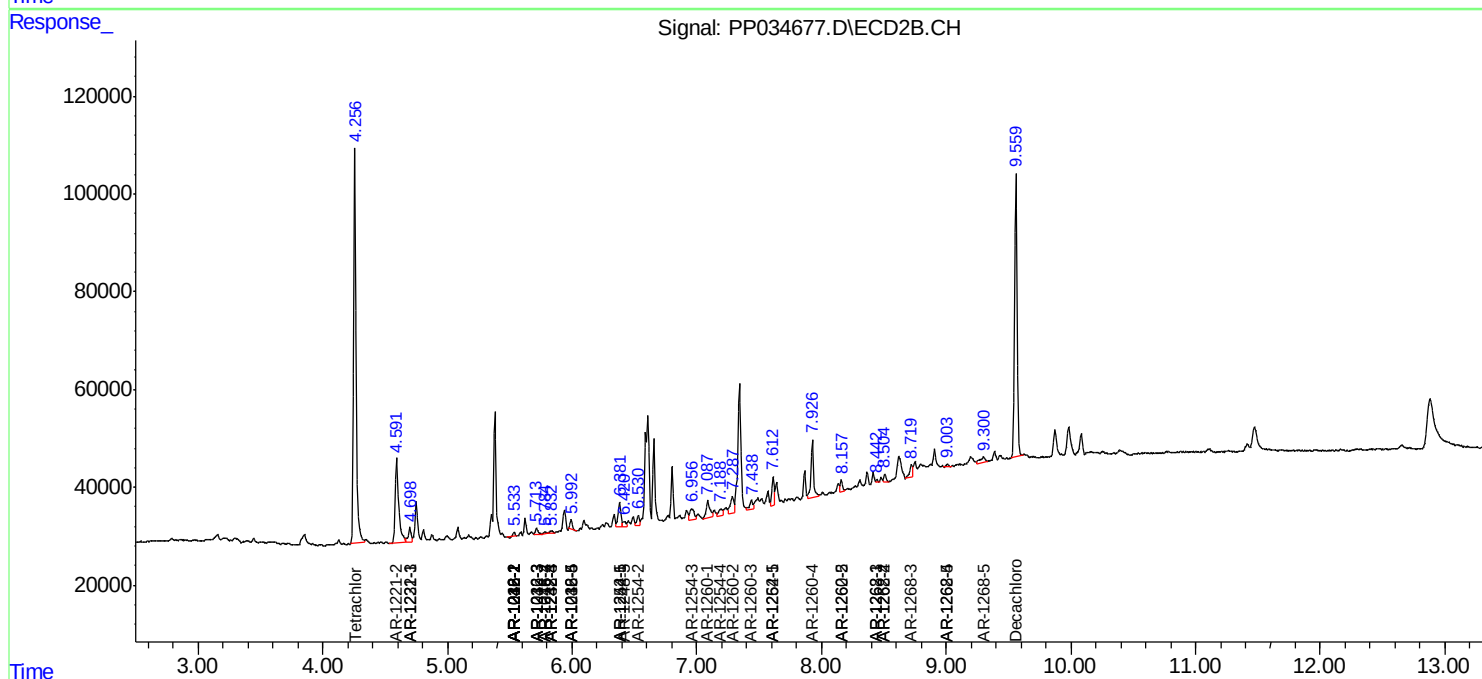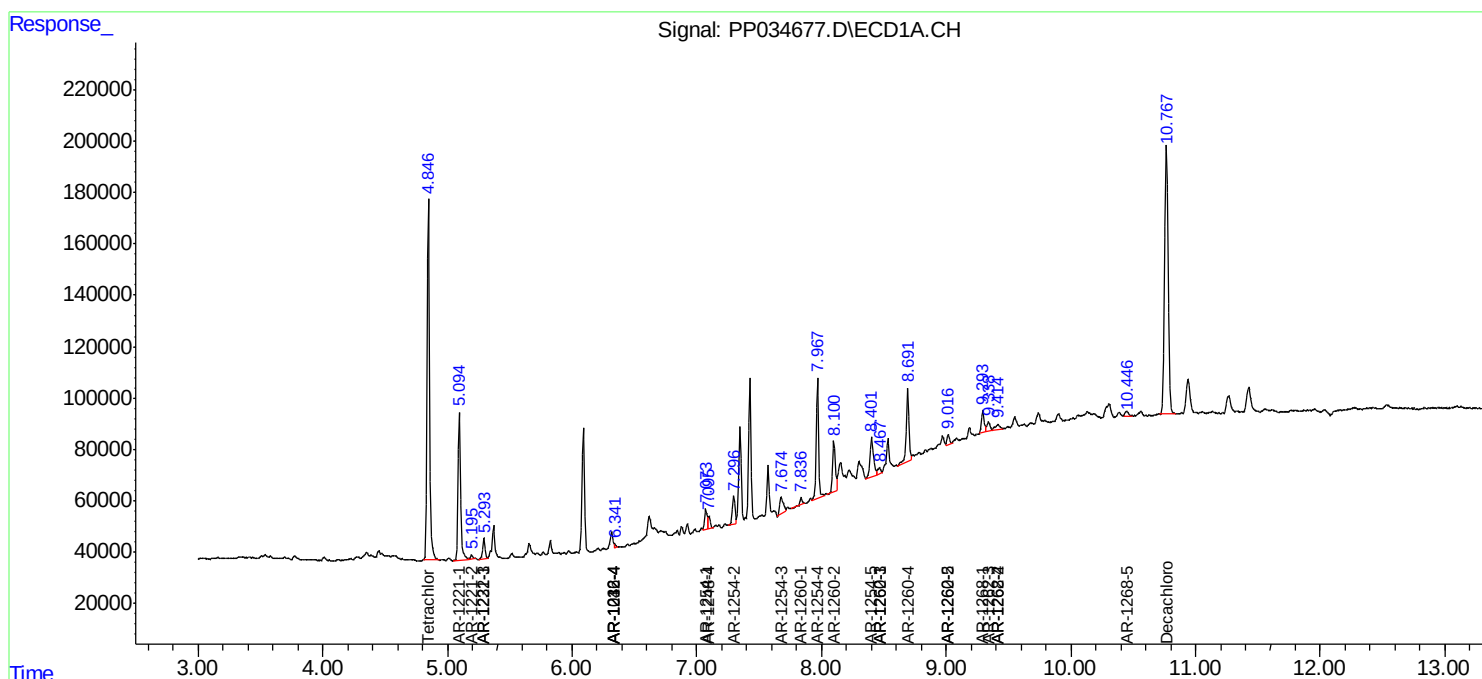


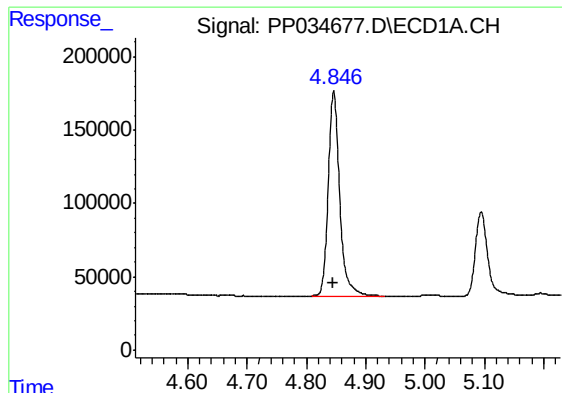

#1 Tetrachloro-m-xylene


R.T.: 4.846 min
Delta R.T.: 0.000 min
Response: 1875112
Conc: 24.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

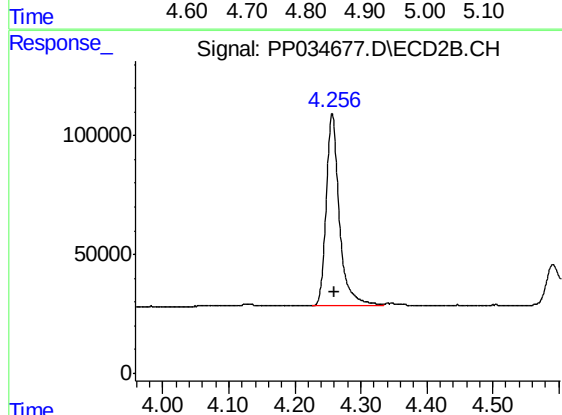


#1 Tetrachloro-m-xylene

R.T.: 4.257 min
Delta R.T.: -0.003 min
Response: 1116283
Conc: 24.85 ng/ml

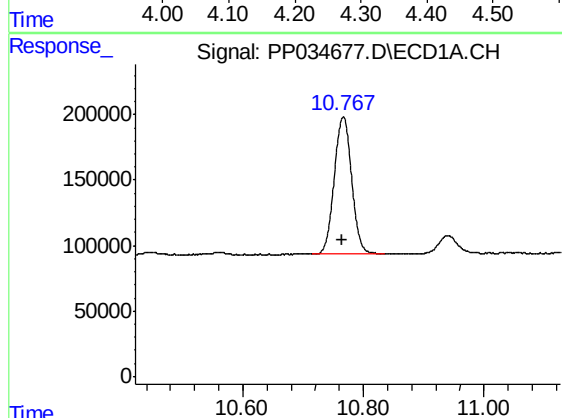


#2 Decachlorobiphenyl

R.T.: 10.767 min
Delta R.T.: 0.002 min
Response: 2086554
Conc: 27.11 ng/ml

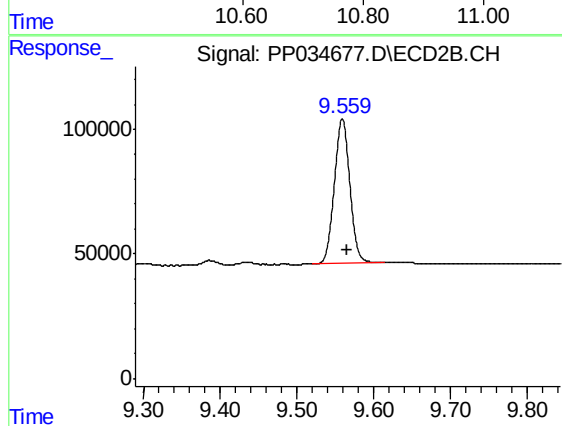

#2 Decachlorobiphenyl


R.T.: 9.559 min
Delta R.T.: -0.007 min
Response: 813758
Conc: 28.82 ng/ml

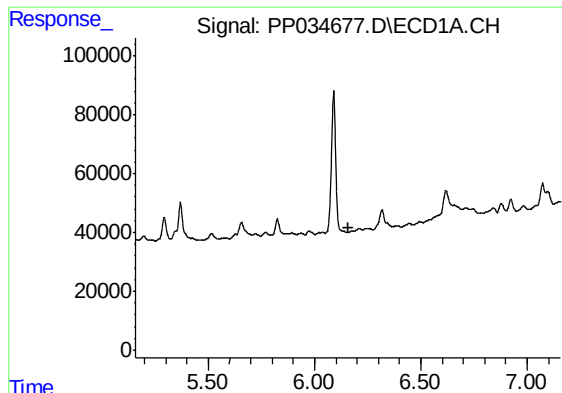

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

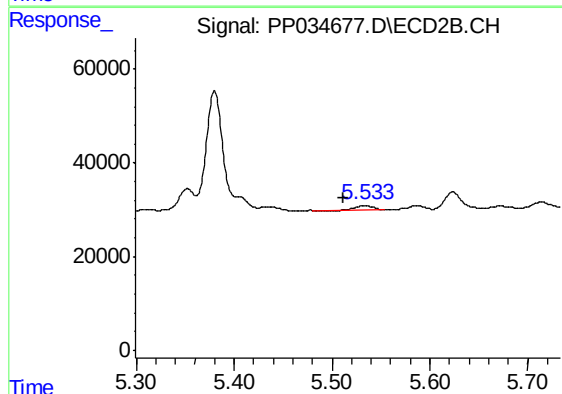


#3 AR-1016-1

R.T.: 5.533 min
Delta R.T.: 0.021 min
Response: 10493
Conc: 8.84 ng/ml

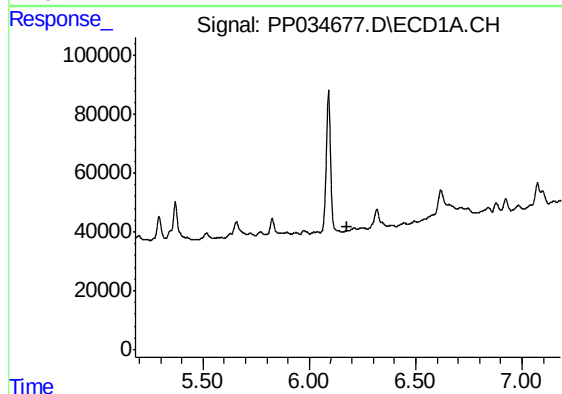


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 6.181 min
Response: 0
Conc: N.D.

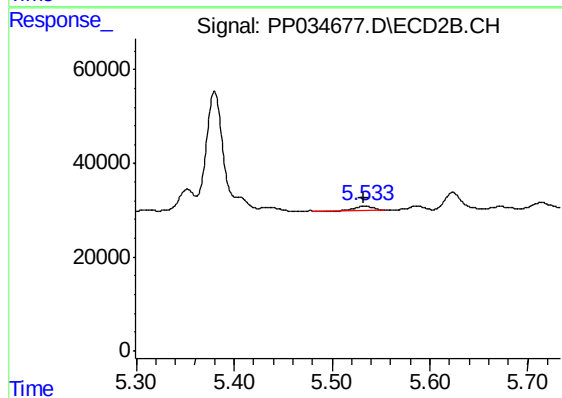

#4 AR-1016-2


R.T.: 5.533 min
Delta R.T.: 0.000 min
Response: 10493
Conc: 5.91 ng/ml

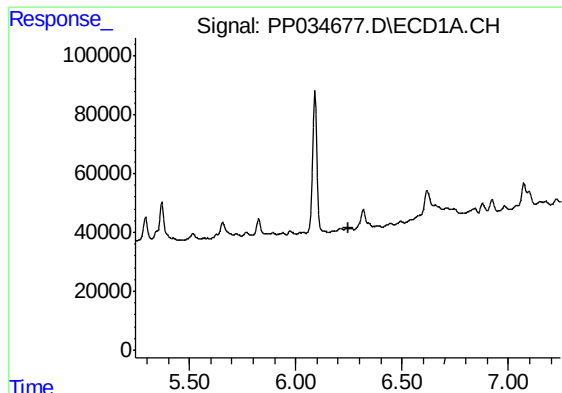

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

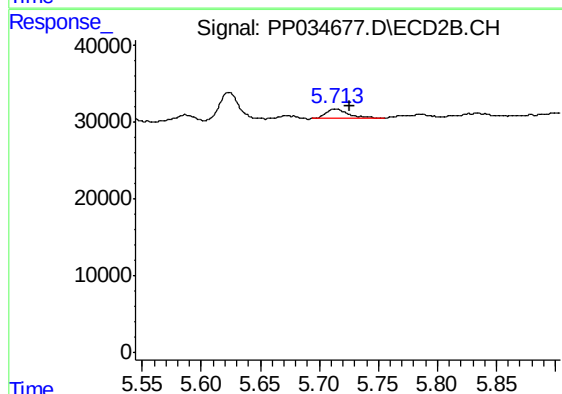


#5 AR-1016-3

R.T.: 5.714 min
Delta R.T.: -0.012 min
Response: 17103
Conc: 18.30 ng/ml

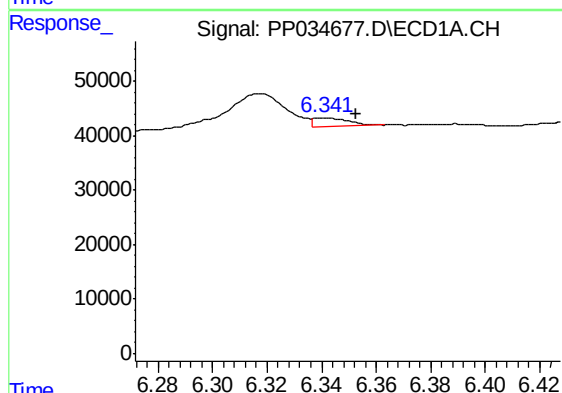


#6 AR-1016-4

R.T.: 6.341 min
Delta R.T.: -0.011 min
Response: 14006
Conc: 7.86 ng/ml

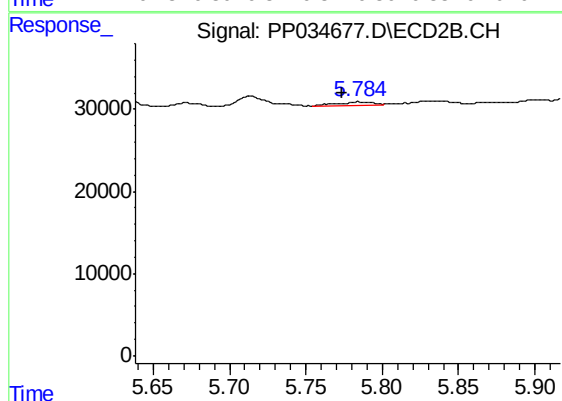

#6 AR-1016-4


R.T.: 5.785 min
Delta R.T.: 0.011 min
Response: 7275
Conc: 10.02 ng/ml



#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP




#7 AR-1016-5

R.T.: 5.992 min
Delta R.T.: -0.012 min
Response: 24788
Conc: 27.10 ng/ml




#8 AR-1221-1

R.T.: 5.095 min
Delta R.T.: 0.000 min
Response: 830029
Conc: 1135.44 ng/ml

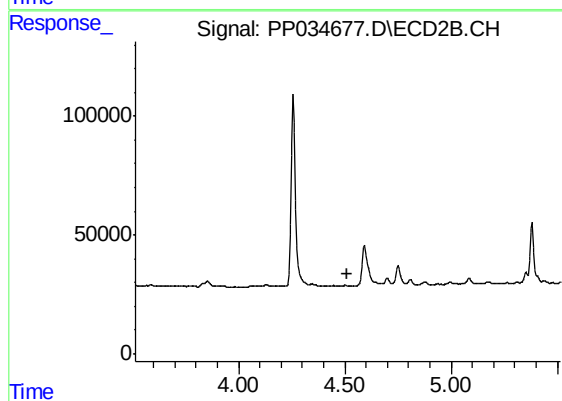

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.514 min
Response: 0
Conc: N.D.



#9 AR-1221-2


R.T.: 5.195 min
Delta R.T.: 0.002 min
Response: 22832
Conc: 40.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP




#9 AR-1221-2

R.T.: 4.591 min
Delta R.T.: -0.023 min
Response: 340672
Conc: 976.49 ng/ml




#10 AR-1221-3

R.T.: 5.293 min
Delta R.T.: 0.014 min
Response: 105754
Conc: 58.11 ng/ml

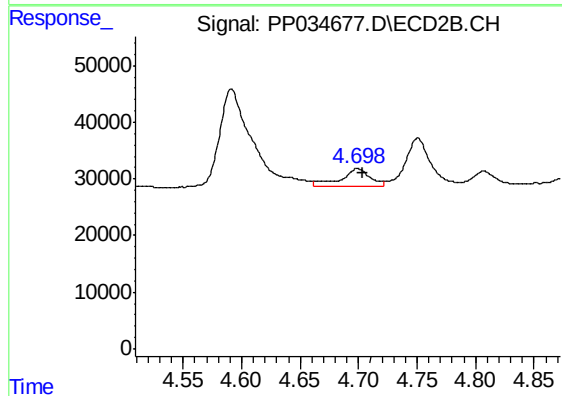

#10 AR-1221-3


R.T.: 4.699 min
Delta R.T.: -0.004 min
Response: 54451
Conc: 51.91 ng/ml

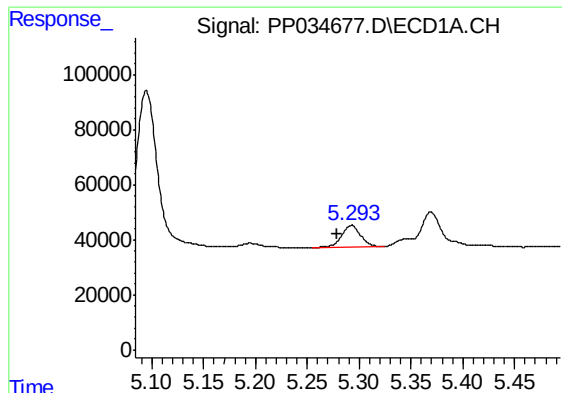

#11 AR-1232-1


R.T.: 5.293 min
Delta R.T.: 0.014 min
Response: 105754
Conc: 71.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

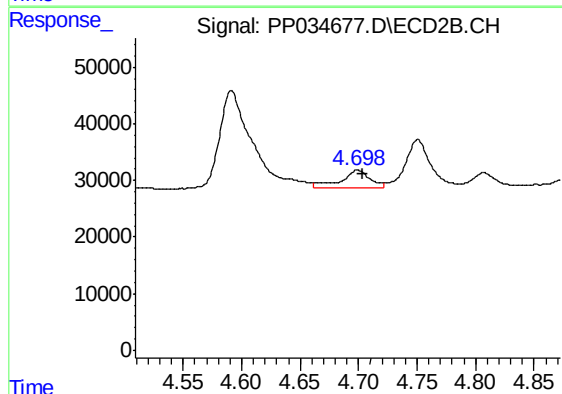


#11 AR-1232-1

R.T.: 4.699 min
Delta R.T.: -0.004 min
Response: 54451
Conc: 64.46 ng/ml

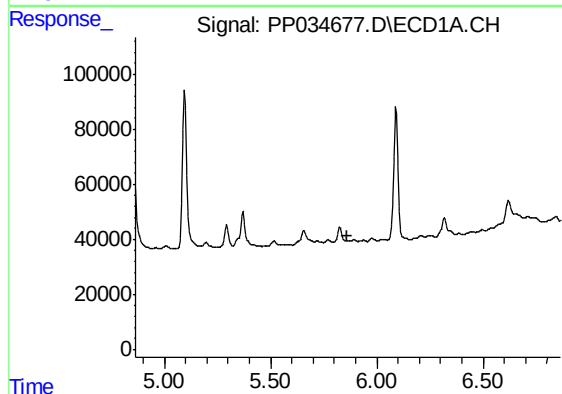


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.863 min
Response: 0
Conc: N.D.

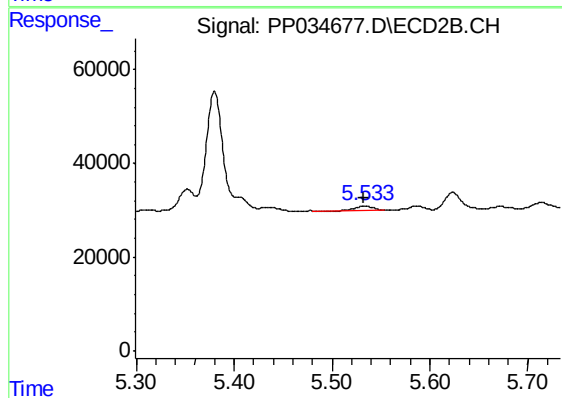

#12 AR-1232-2


R.T.: 5.533 min
Delta R.T.: 0.001 min
Response: 10493
Conc: 13.94 ng/ml



#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 6.180 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP




#13 AR-1232-3

R.T.: 5.714 min
Delta R.T.: -0.011 min
Response: 17103
Conc: 43.09 ng/ml




#14 AR-1232-4

R.T.: 6.341 min
Delta R.T.: -0.012 min
Response: 14006
Conc: 19.50 ng/ml

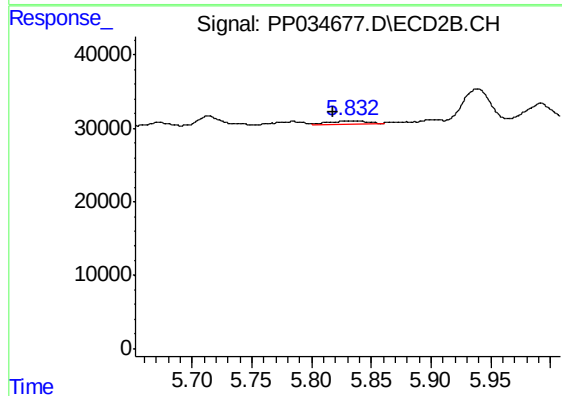

#14 AR-1232-4


R.T.: 5.834 min
Delta R.T.: 0.015 min
Response: 8197
Conc: 23.83 ng/ml

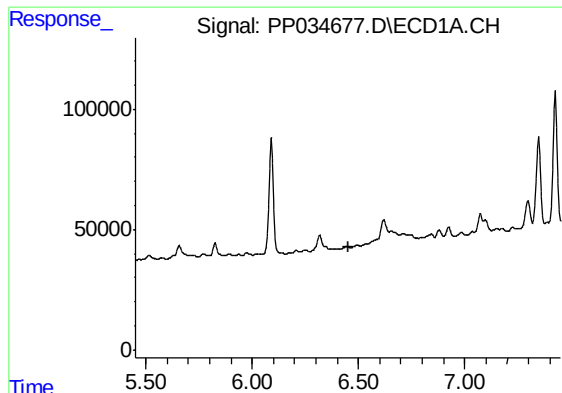

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

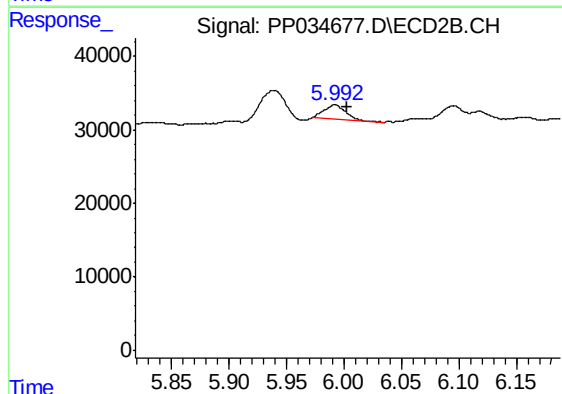


#15 AR-1232-5

R.T.: 5.992 min
Delta R.T.: -0.011 min
Response: 24788
Conc: 69.73 ng/ml




#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

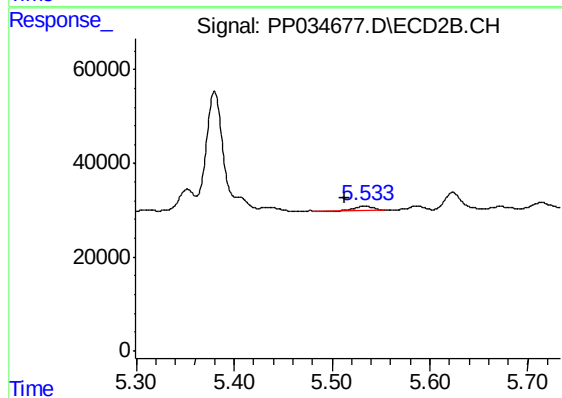

#16 AR-1242-1


R.T.: 5.533 min
Delta R.T.: 0.021 min
Response: 10493
Conc: 11.20 ng/ml



#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 6.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP




#17 AR-1242-2

R.T.: 5.533 min
Delta R.T.: 0.000 min
Response: 10493
Conc: 7.38 ng/ml




#18 AR-1242-3

R.T.: 0.000 min
Exp R.T. : 6.247 min
Response: 0
Conc: N.D.

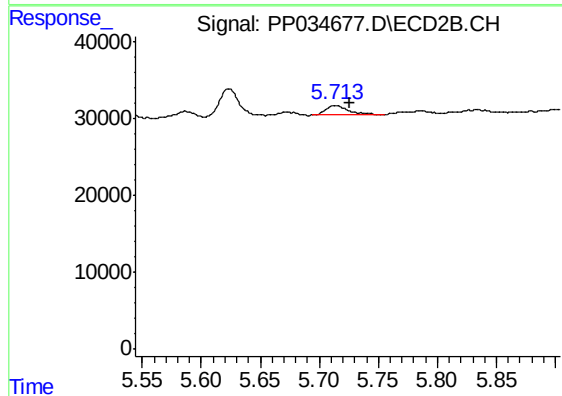

#18 AR-1242-3


R.T.: 5.714 min
Delta R.T.: -0.012 min
Response: 17103
Conc: 22.91 ng/ml

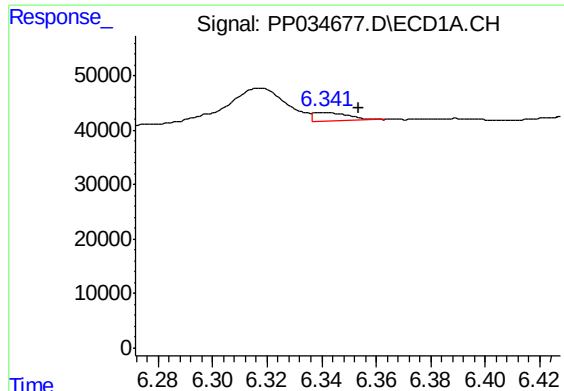

#19 AR-1242-4


R.T.: 6.341 min
Delta R.T.: -0.012 min
Response: 14006
Conc: 10.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

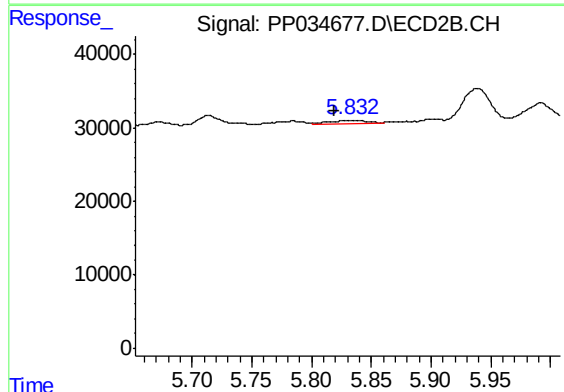


#19 AR-1242-4

R.T.: 5.834 min
Delta R.T.: 0.014 min
Response: 8197
Conc: 11.14 ng/ml

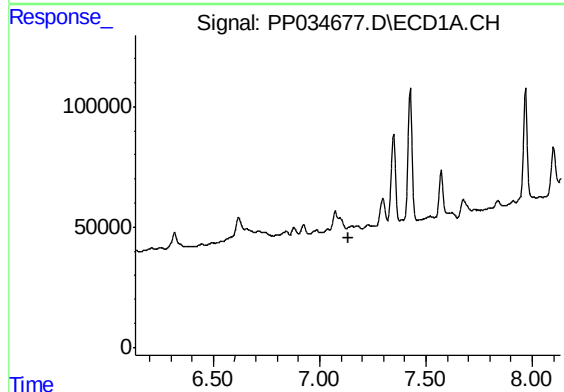


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

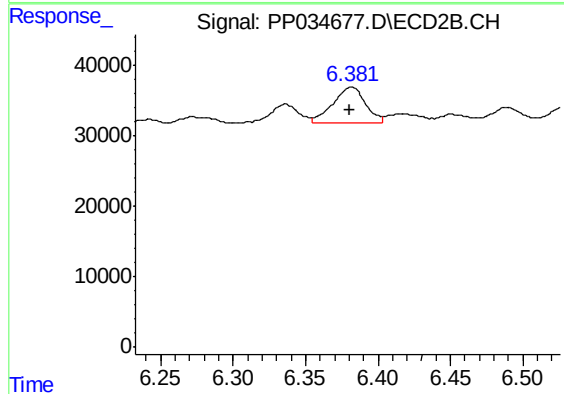

#20 AR-1242-5


R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 79281
Conc: 96.69 ng/ml



#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP




#21 AR-1248-1

R.T.: 5.533 min
Delta R.T.: 0.021 min
Response: 10493
Conc: 14.38 ng/ml

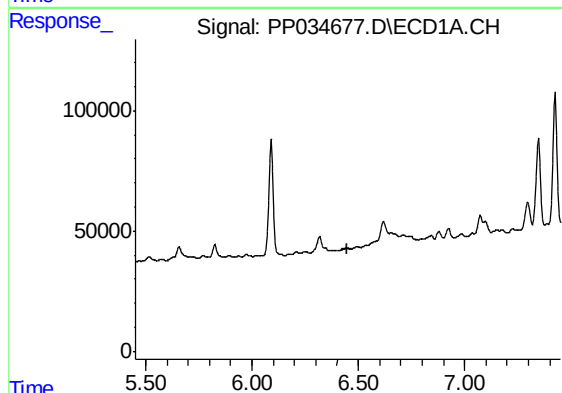


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

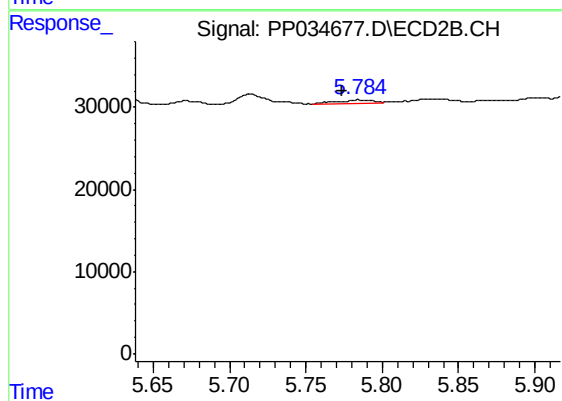

#22 AR-1248-2


R.T.: 5.785 min
Delta R.T.: 0.011 min
Response: 7275
Conc: 7.09 ng/ml

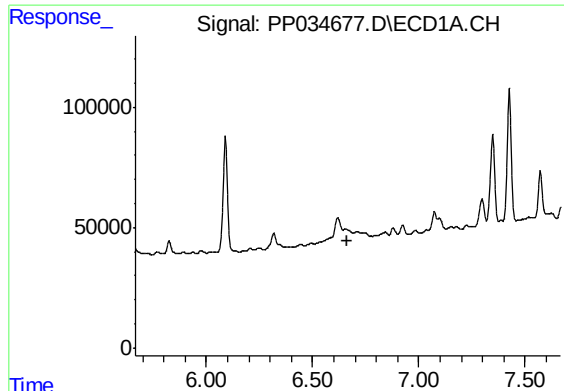

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

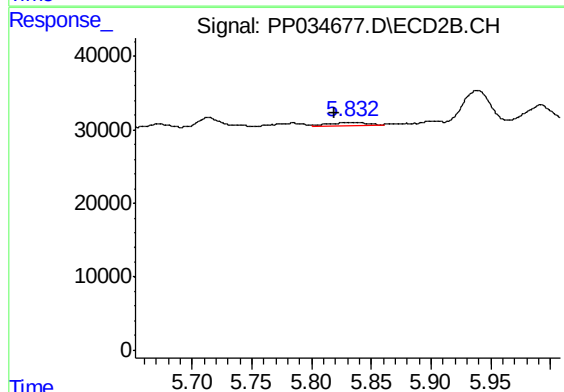


#23 AR-1248-3

R.T.: 5.834 min
Delta R.T.: 0.015 min
Response: 8197
Conc: 7.48 ng/ml

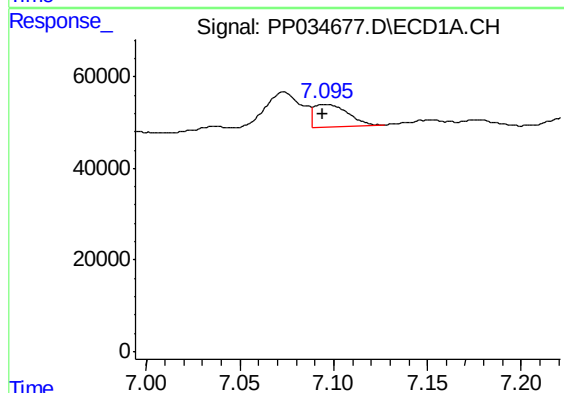


#24 AR-1248-4

R.T.: 7.096 min
Delta R.T.: 0.002 min
Response: 62470
Conc: 24.48 ng/ml

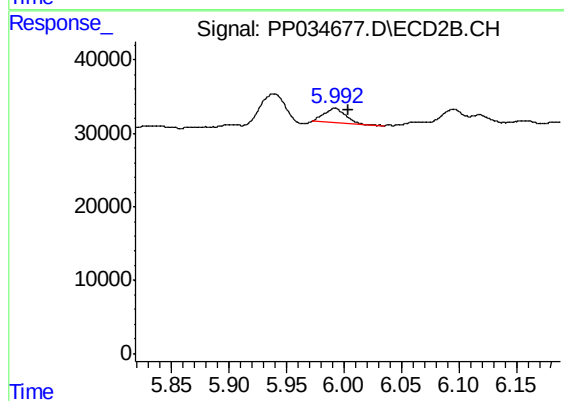

#24 AR-1248-4


R.T.: 5.992 min
Delta R.T.: -0.012 min
Response: 24788
Conc: 19.64 ng/ml



#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP




#25 AR-1248-5

R.T.: 6.419 min
Delta R.T.: -0.006 min
Response: 19281
Conc: 17.06 ng/ml




#26 AR-1254-1

R.T.: 7.073 min
Delta R.T.: 0.010 min
Response: 113923
Conc: 41.43 ng/ml

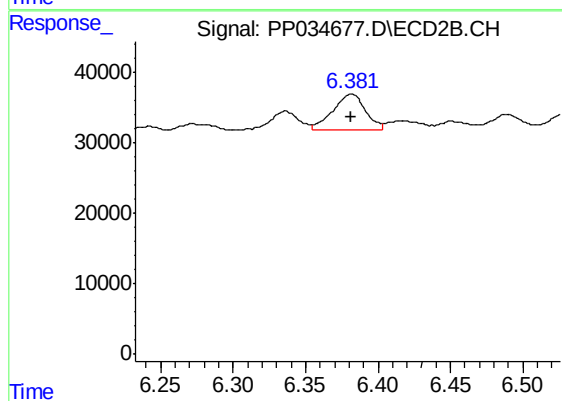

#26 AR-1254-1


R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 79281
Conc: 42.97 ng/ml



#27 AR-1254-2


R.T.: 7.297 min
Delta R.T.: 0.004 min
Response: 177511
Conc: 41.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP




#27 AR-1254-2

R.T.: 6.530 min
Delta R.T.: -0.008 min
Response: 27974
Conc: 17.49 ng/ml




#28 AR-1254-3

R.T.: 7.675 min
Delta R.T.: 0.003 min
Response: 128136
Conc: 28.07 ng/ml

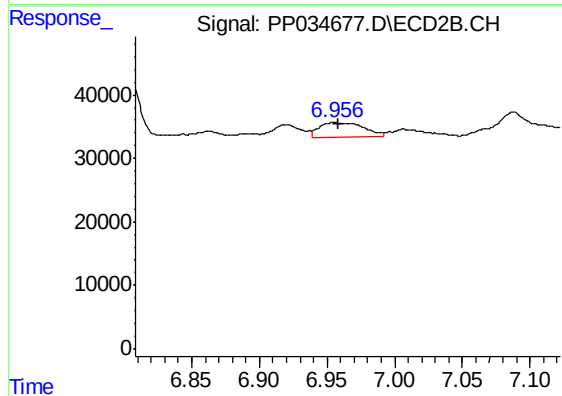

#28 AR-1254-3


R.T.: 6.955 min
Delta R.T.: -0.003 min
Response: 52664
Conc: 21.10 ng/ml

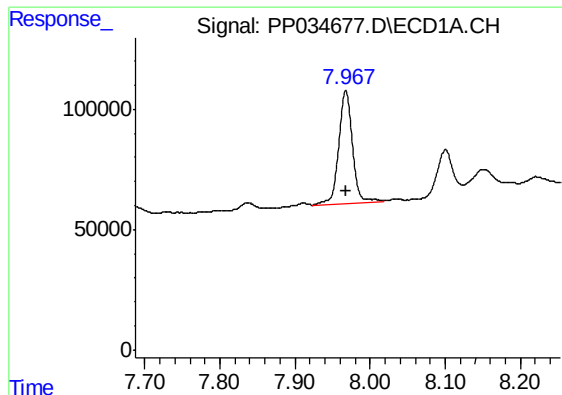

#29 AR-1254-4


R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 589153
Conc: 190.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

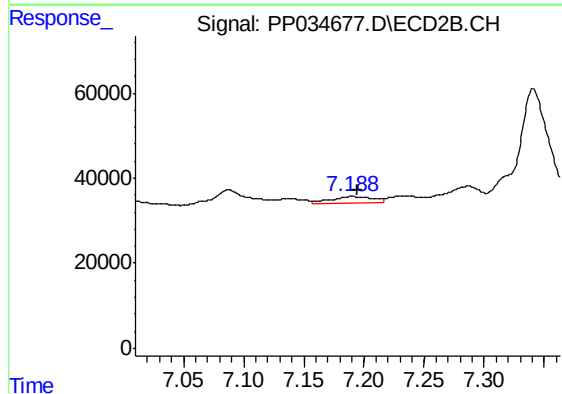


#29 AR-1254-4

R.T.: 7.190 min
Delta R.T.: -0.005 min
Response: 35084
Conc: 26.69 ng/ml

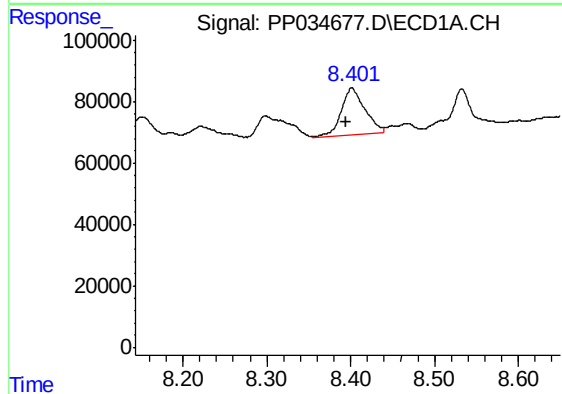


#30 AR-1254-5

R.T.: 8.401 min
Delta R.T.: 0.007 min
Response: 289326
Conc: 81.41 ng/ml

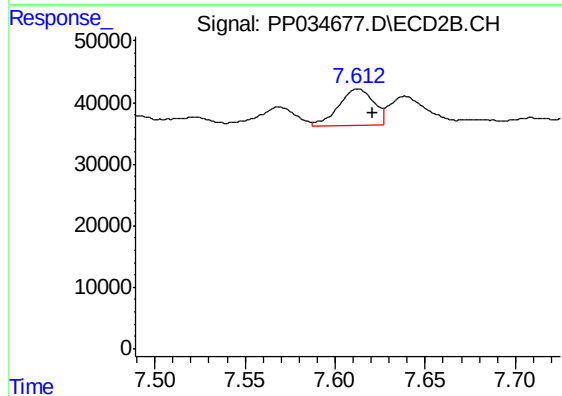

#30 AR-1254-5


R.T.: 7.613 min
Delta R.T.: -0.008 min
Response: 80111
Conc: 39.42 ng/ml

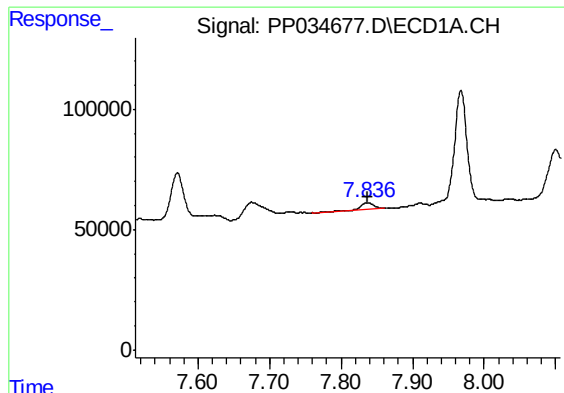

#31 AR-1260-1


R.T.: 7.837 min
Delta R.T.: 0.000 min
Response: 35478
Conc: 11.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

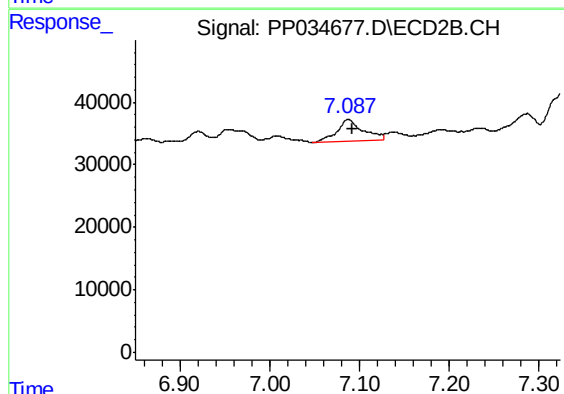


#31 AR-1260-1

R.T.: 7.088 min
Delta R.T.: -0.005 min
Response: 72436
Conc: 47.17 ng/ml

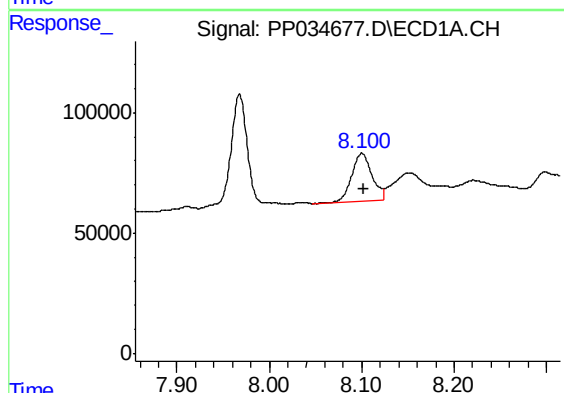


#32 AR-1260-2

R.T.: 8.100 min
Delta R.T.: -0.003 min
Response: 299213
Conc: 79.68 ng/ml

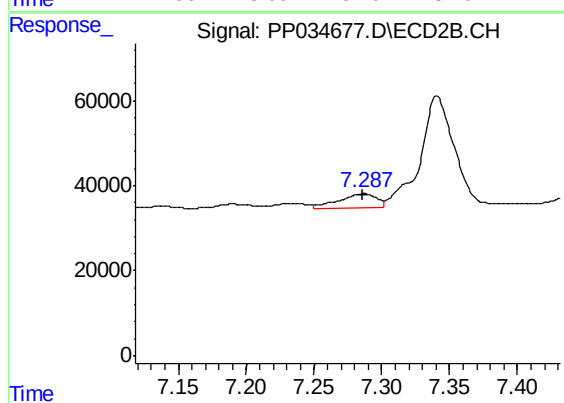

#32 AR-1260-2


R.T.: 7.287 min
Delta R.T.: 0.000 min
Response: 67803
Conc: 37.53 ng/ml

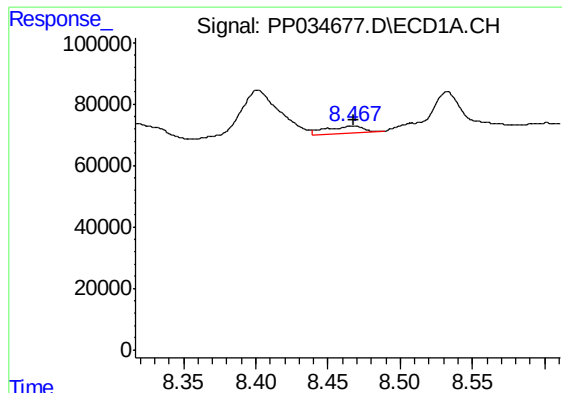

#33 AR-1260-3


R.T.: 8.467 min
Delta R.T.: 0.000 min
Response: 40094
Conc: 13.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

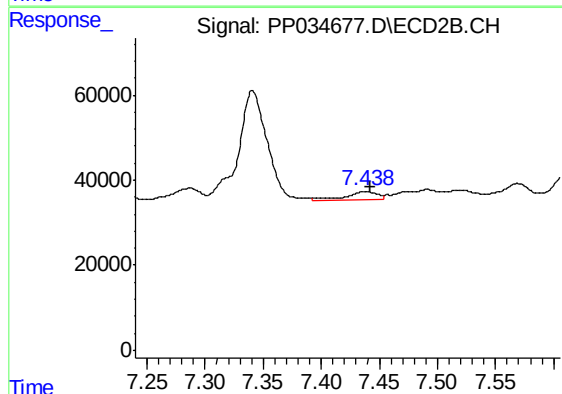


#33 AR-1260-3

R.T.: 7.438 min
Delta R.T.: -0.005 min
Response: 36104
Conc: 20.81 ng/ml

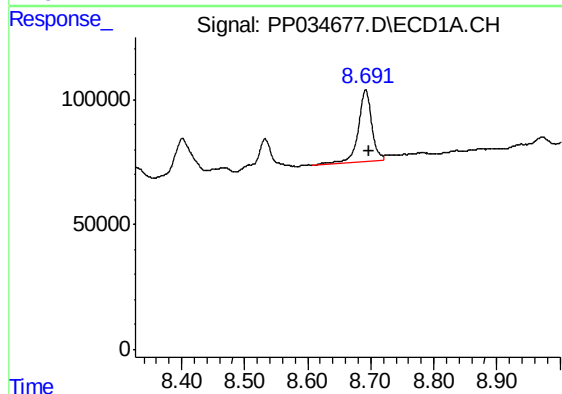


#34 AR-1260-4

R.T.: 8.692 min
Delta R.T.: -0.005 min
Response: 430317
Conc: 123.26 ng/ml

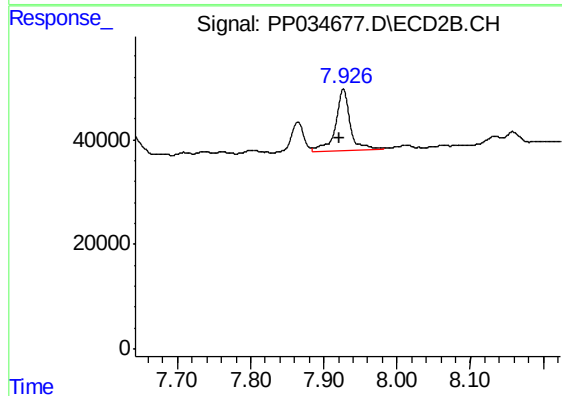

#34 AR-1260-4


R.T.: 7.927 min
Delta R.T.: 0.005 min
Response: 165706
Conc: 115.57 ng/ml

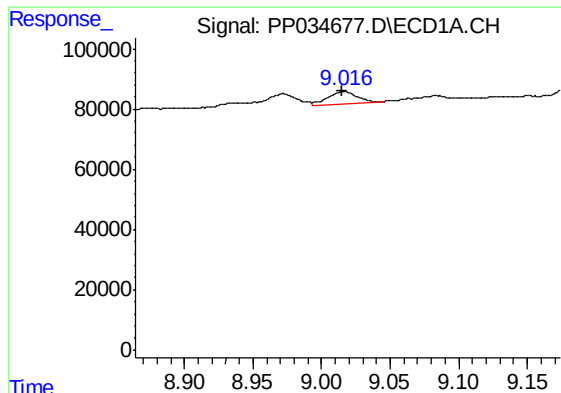

#35 AR-1260-5


R.T.: 9.016 min
Delta R.T.: 0.000 min
Response: 59717
Conc: 8.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

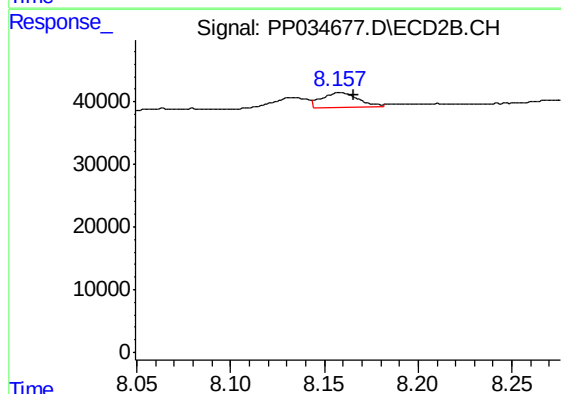


#35 AR-1260-5

R.T.: 8.158 min
Delta R.T.: -0.007 min
Response: 31921
Conc: 9.34 ng/ml

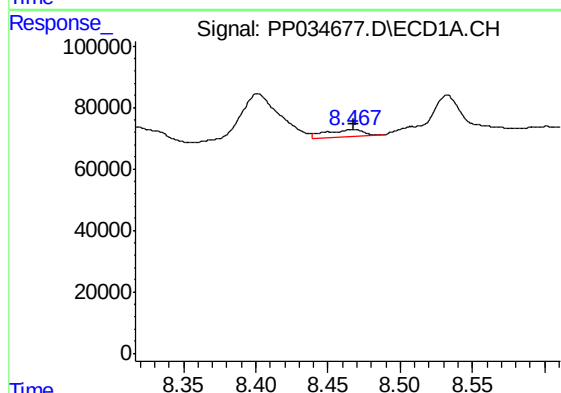


#36 AR-1262-1

R.T.: 8.467 min
Delta R.T.: -0.001 min
Response: 40094
Conc: 8.76 ng/ml

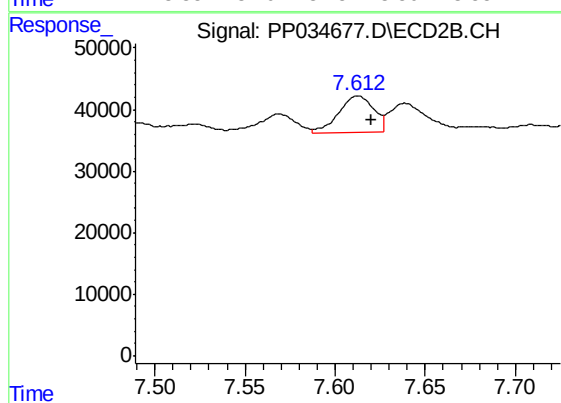

#36 AR-1262-1


R.T.: 7.613 min
Delta R.T.: -0.007 min
Response: 80111
Conc: 74.59 ng/ml

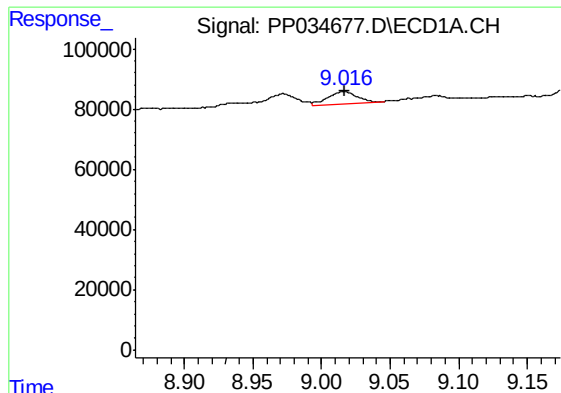

#37 AR-1262-2


R.T.: 9.016 min
Delta R.T.: -0.001 min
Response: 59717
Conc: 7.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

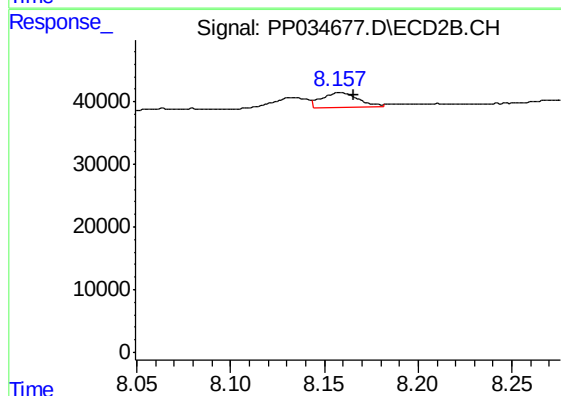


#37 AR-1262-2

R.T.: 8.158 min
Delta R.T.: -0.007 min
Response: 31921
Conc: 9.30 ng/ml

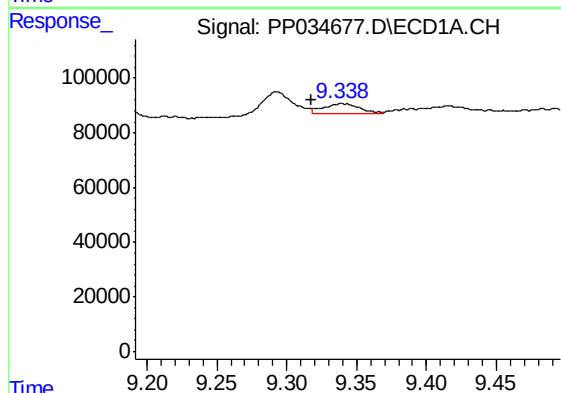


#38 AR-1262-3

R.T.: 9.339 min
Delta R.T.: 0.022 min
Response: 65676
Conc: 12.20 ng/ml

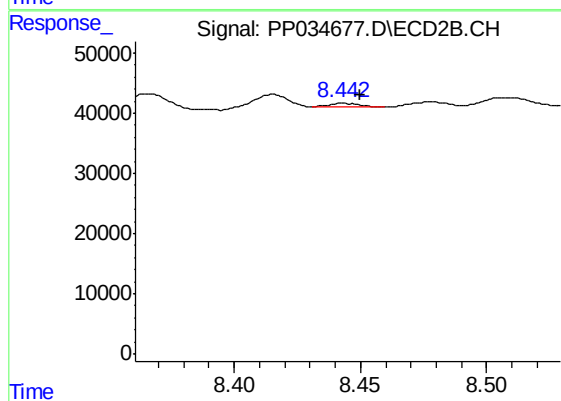

#38 AR-1262-3


R.T.: 8.443 min
Delta R.T.: -0.007 min
Response: 6311
Conc: 4.21 ng/ml

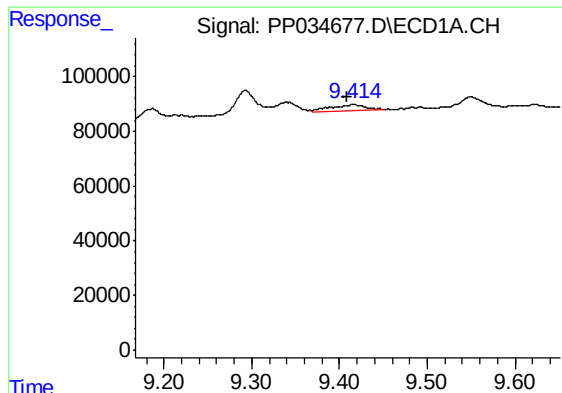

#39 AR-1262-4


R.T.: 9.415 min
Delta R.T.: 0.007 min
Response: 56175
Conc: 12.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

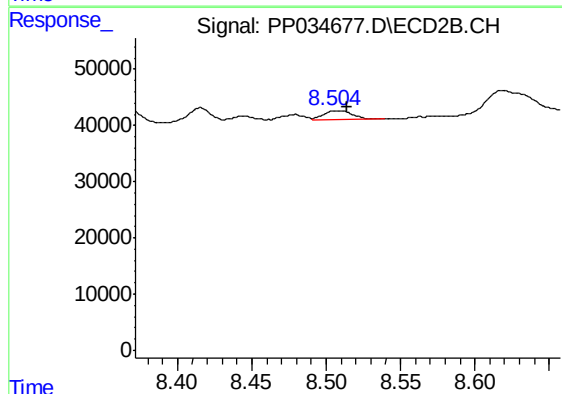


#39 AR-1262-4

R.T.: 8.509 min
Delta R.T.: -0.006 min
Response: 20973
Conc: 7.62 ng/ml

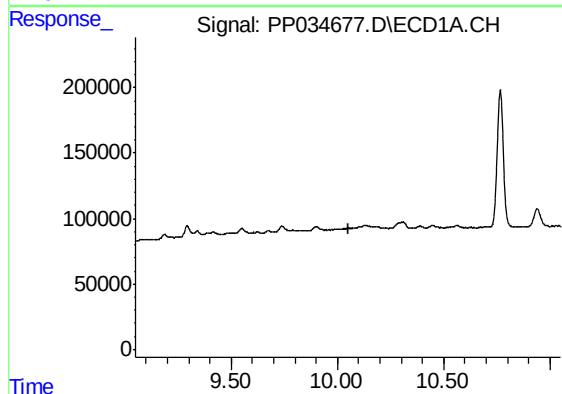


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 10.050 min
Response: 0
Conc: N.D.

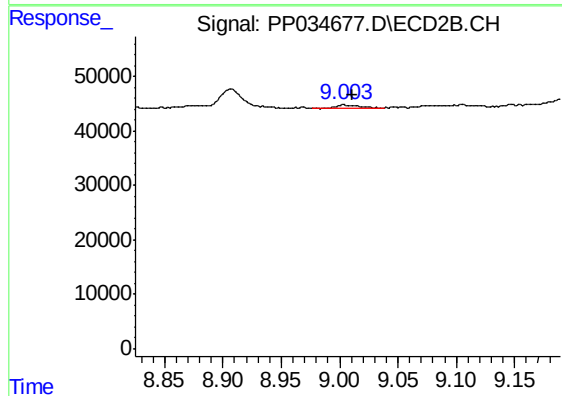

#40 AR-1262-5


R.T.: 9.004 min
Delta R.T.: -0.007 min
Response: 5603
Conc: 4.94 ng/ml



#41 AR-1268-1


R.T.: 9.293 min
Delta R.T.: -0.023 min
Response: 124978
Conc: 12.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP




#41 AR-1268-1

R.T.: 8.443 min
Delta R.T.: -0.006 min
Response: 6311
Conc: 1.46 ng/ml




#42 AR-1268-2

R.T.: 9.415 min
Delta R.T.: 0.007 min
Response: 56175
Conc: 5.87 ng/ml

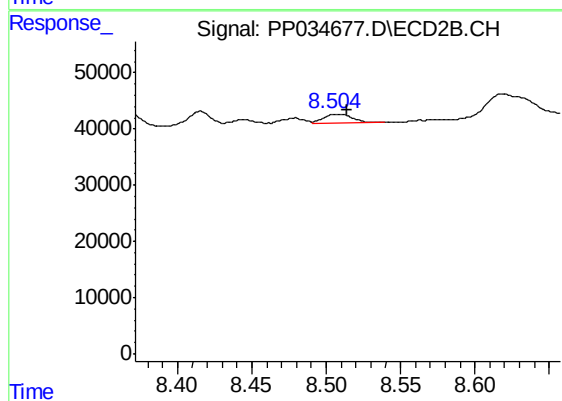

#42 AR-1268-2


R.T.: 8.509 min
Delta R.T.: -0.005 min
Response: 20973
Conc: 5.07 ng/ml

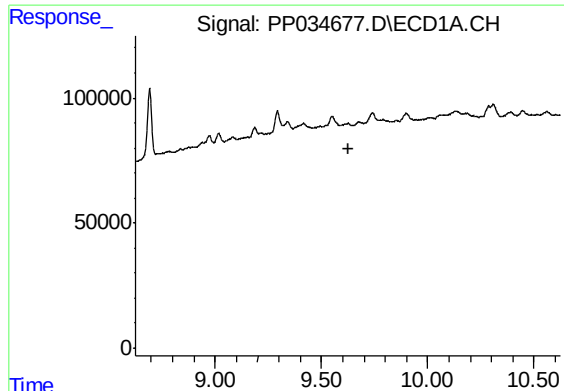

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 9.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

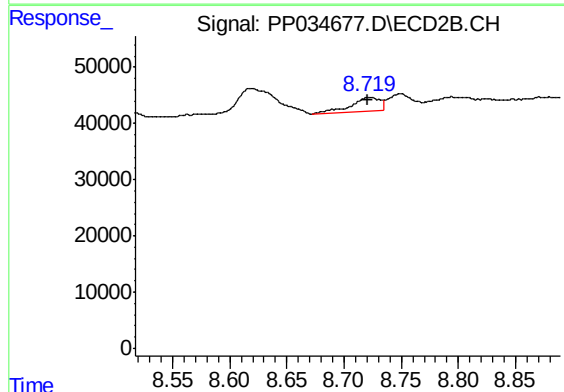


#43 AR-1268-3

R.T.: 8.720 min
Delta R.T.: 0.000 min
Response: 44696
Conc: 12.29 ng/ml

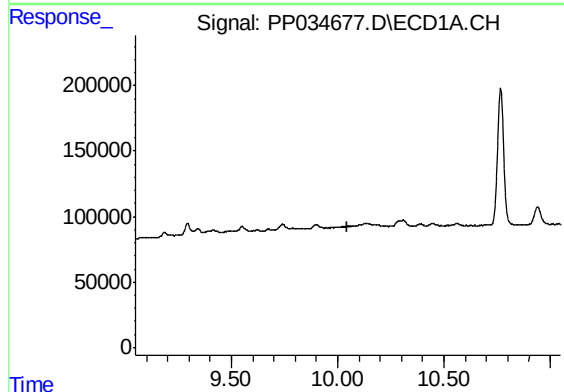


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 10.048 min
Response: 0
Conc: N.D.

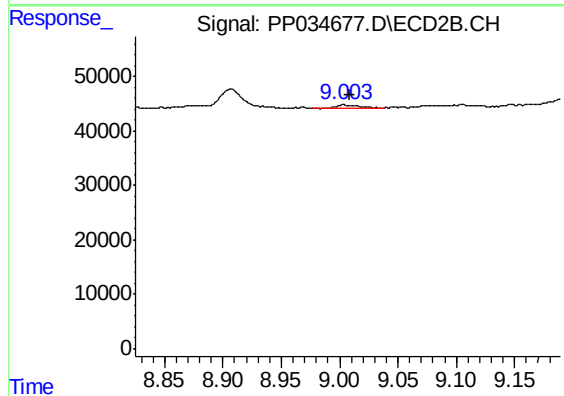

#44 AR-1268-4


R.T.: 9.004 min
Delta R.T.: -0.006 min
Response: 5603
Conc: 4.35 ng/ml

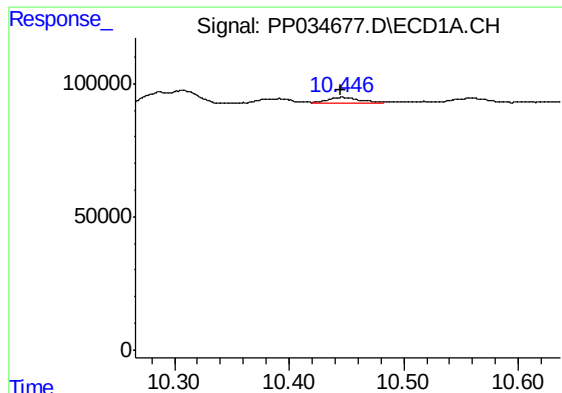

#45 AR-1268-5

R.T.: 10.446 min
Delta R.T.: 0.000 min
Response: 44319
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MSRO-COMP

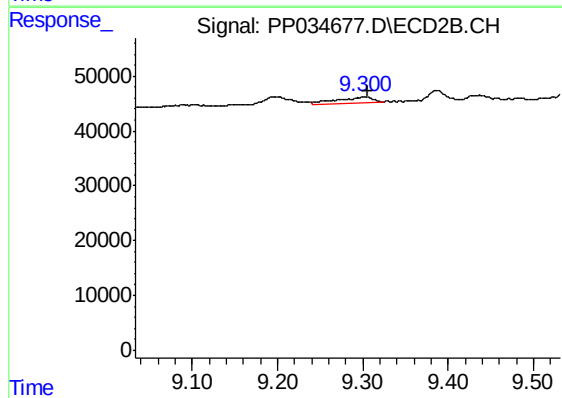

#45 AR-1268-5

R.T.: 9.303 min
Delta R.T.: -0.003 min
Response: 33525
Conc: 3.23 ng/ml