

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040521\
 Data File : PP034669.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2021 12:28
 Operator : DD\AJ
 Sample : M1909-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FS-SB-10-26-27

Manual Integrations
 APPROVED

Ankita
 4/6/2021 2:56:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 03:00:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.855	4.256	1463073	993242	19.179m	22.110m
2) SA Decachlor...	10.780f	9.564	1806608	689775	23.469	24.429

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040521\
Data File : PP034669.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2021 12:28
Operator : DD\AJ
Sample : M1909-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FS-SB-10-26-27


Manual Integrations
APPROVED

Ankita
4/6/2021 2:56:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 03:00:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

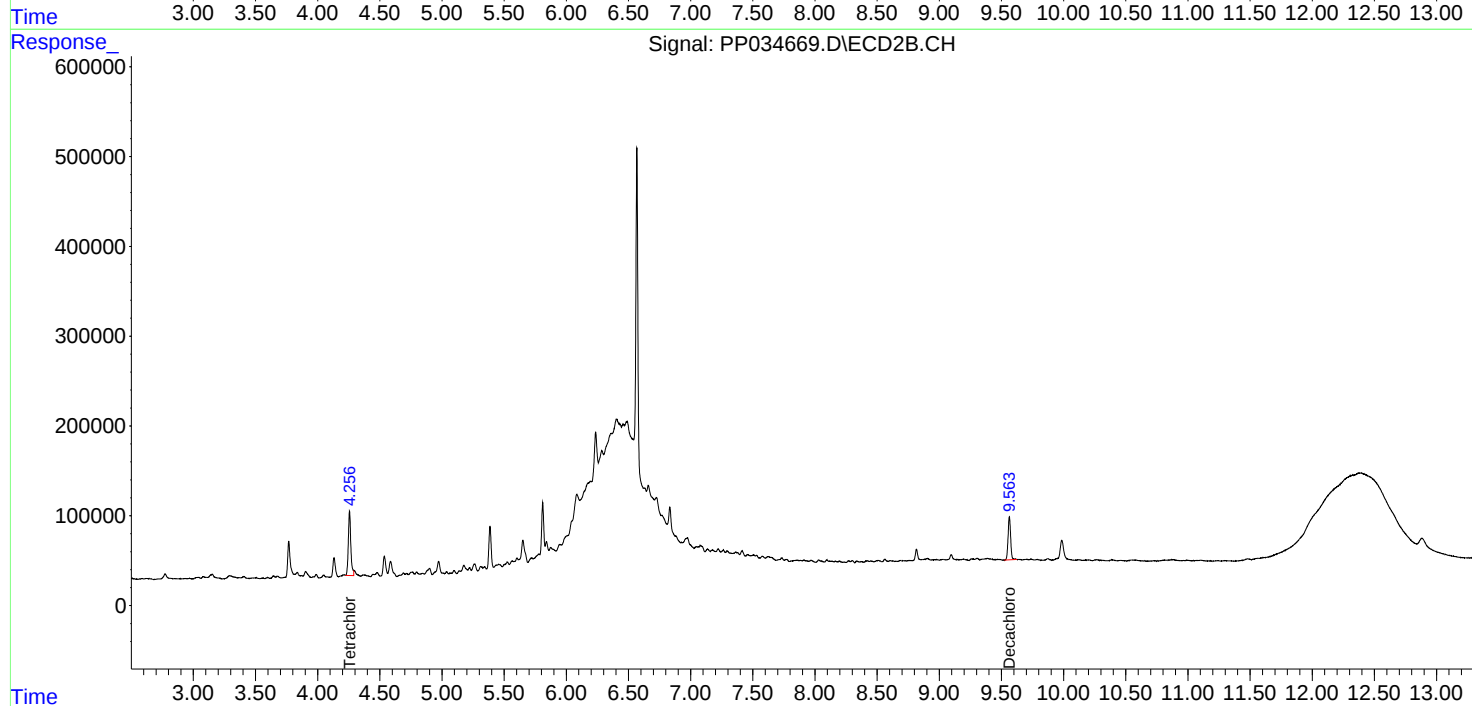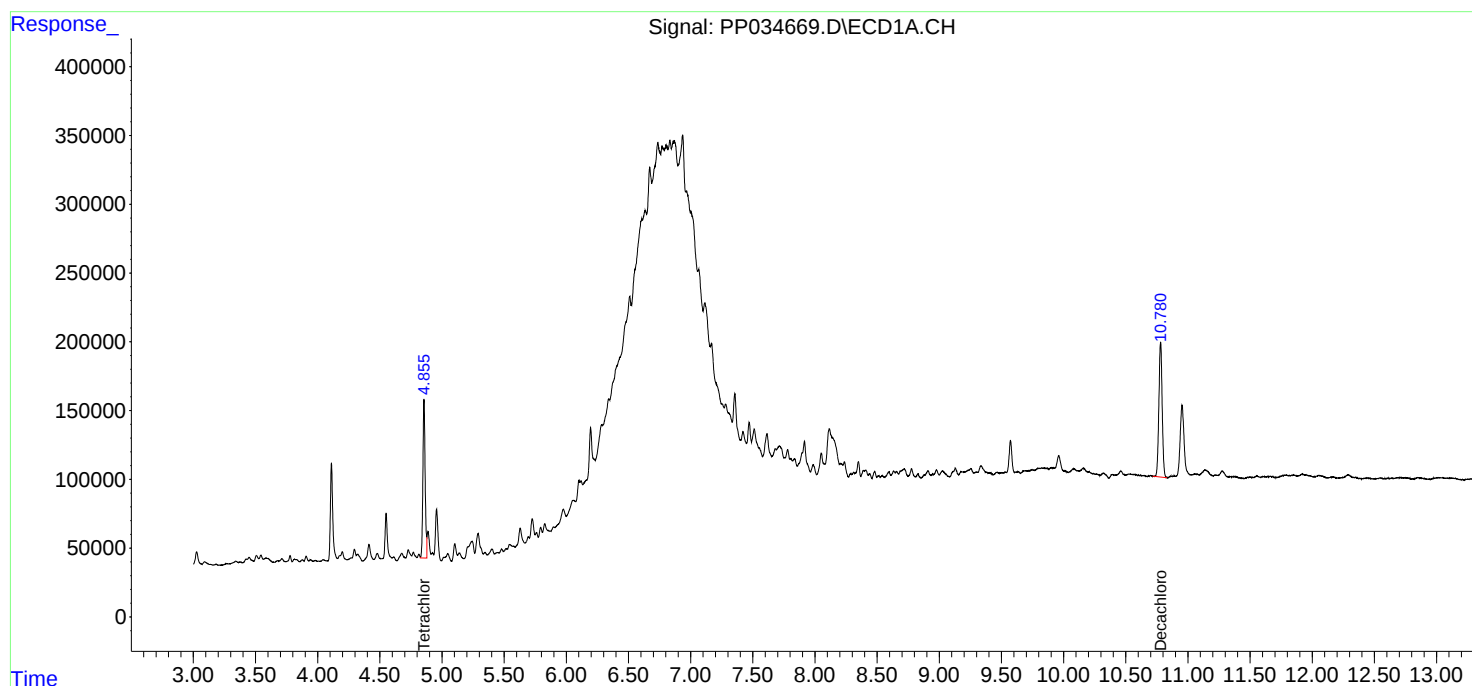

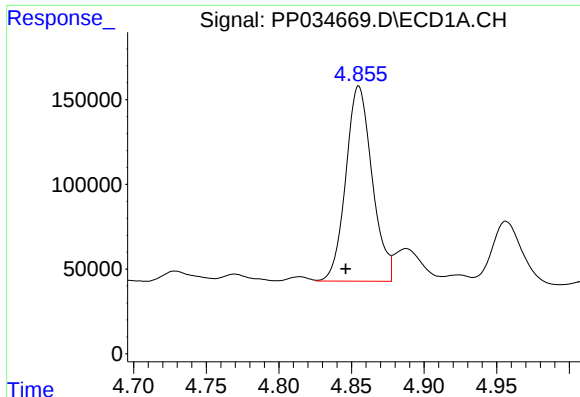


#1 Tetrachloro-m-xylene

R.T.: 4.855 min
Delta R.T.: 0.009 min
Response: 1463073
Conc: 19.18 ng/ml m

Instrument :
ECD_P
ClientSampleId :
FS-SB-10-26-27


Manual Integrations
APPROVED

Ankita
4/6/2021 2:56:35 PM

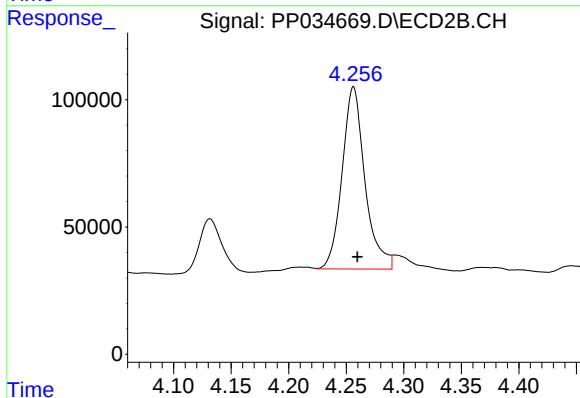


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: -0.004 min
Response: 993242
Conc: 22.11 ng/ml m

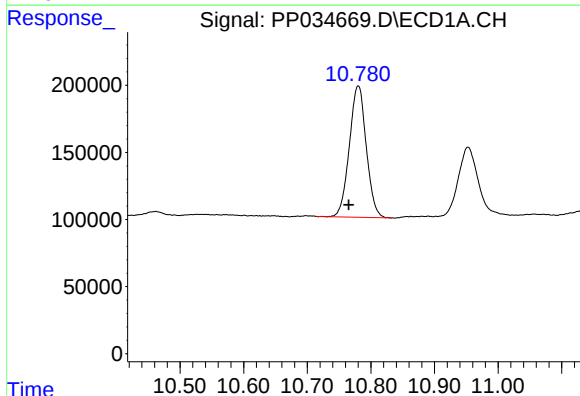

#2 Decachlorobiphenyl

R.T.: 10.780 min
Delta R.T.: 0.015 min
Response: 1806608
Conc: 23.47 ng/ml

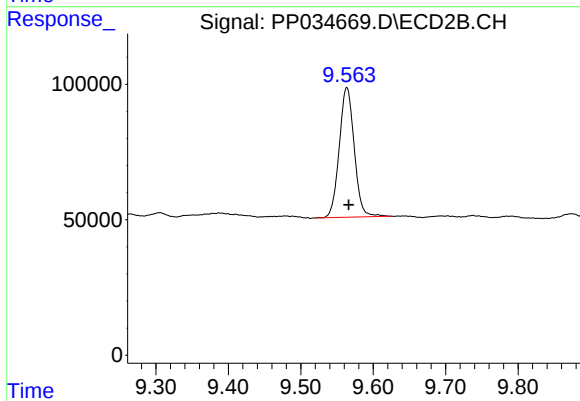

#2 Decachlorobiphenyl

R.T.: 9.564 min
Delta R.T.: -0.002 min
Response: 689775
Conc: 24.43 ng/ml