

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040619\
 Data File : PP029777.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2019 8:58
 Operator : EI\MA
 Sample : I.BLK
 Misc : hexane
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:04:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040519.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 05 15:13:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.169	12.361	13402876	14808547	403.842	321.407
Target Compounds							
5) T	DICAMBA	0.000	12.640	0	857313	N.D.	5.518 #
6) T	MCP	0.000	12.925	0	860400	N.D.	28.365 #
8) T	DICHLORPROP	13.632	0.000	2892982	0	67.052	N.D. #
12) T	2,4,5-T	0.000	16.136	0	182737	N.D.	1.053 #
13) T	2,4-DB	16.491	0.000	109996	0	4.628	N.D. #
14) T	DINOSEB	17.974	17.122	116464	66753	0.745	0.496 #
15) T	Picloram	17.758	18.544	237835	146233	0.891	0.704
16) T	DCPA	18.304	0.000	91436	0	0.279	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040619\
Data File : PP029777.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2019 8:58
Operator : EI\MA
Sample : I.BLK
Misc : hexane
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:04:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040519.M
Quant Title : 8080.M
QLast Update : Fri Apr 05 15:13:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

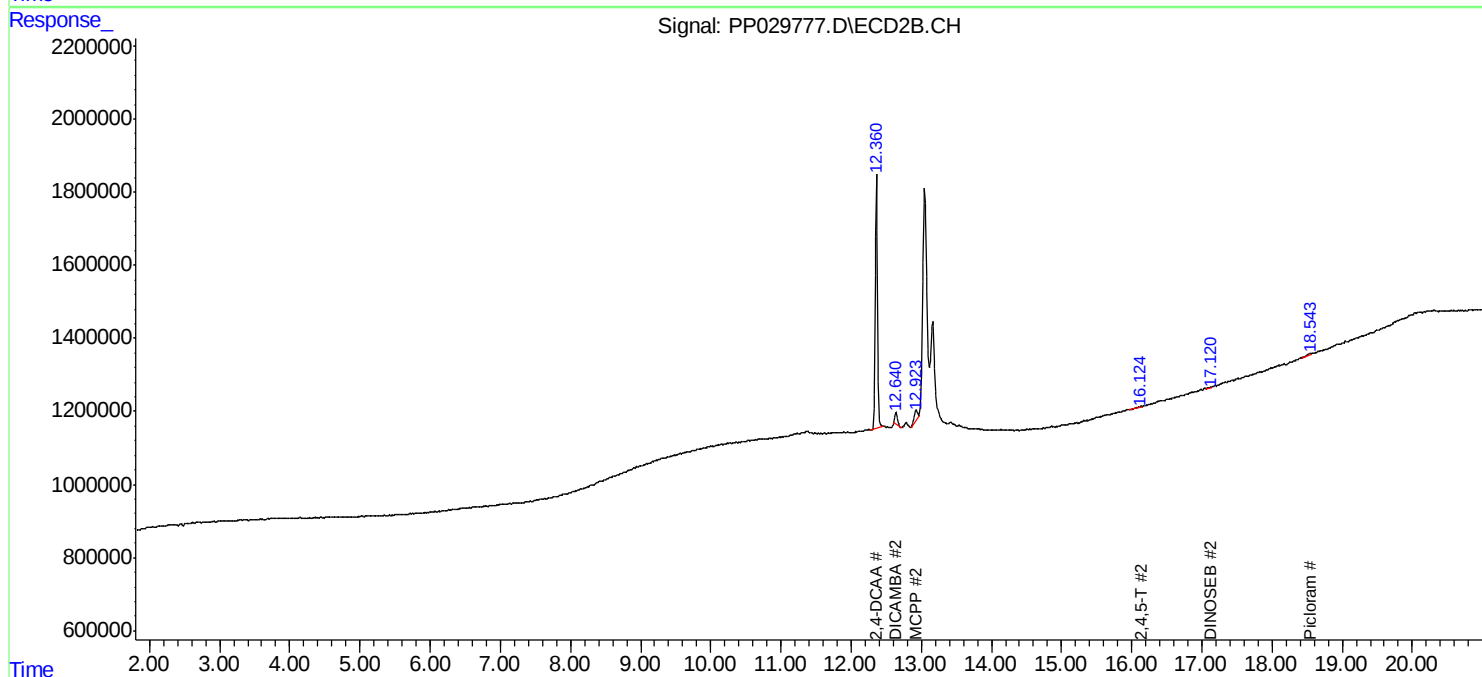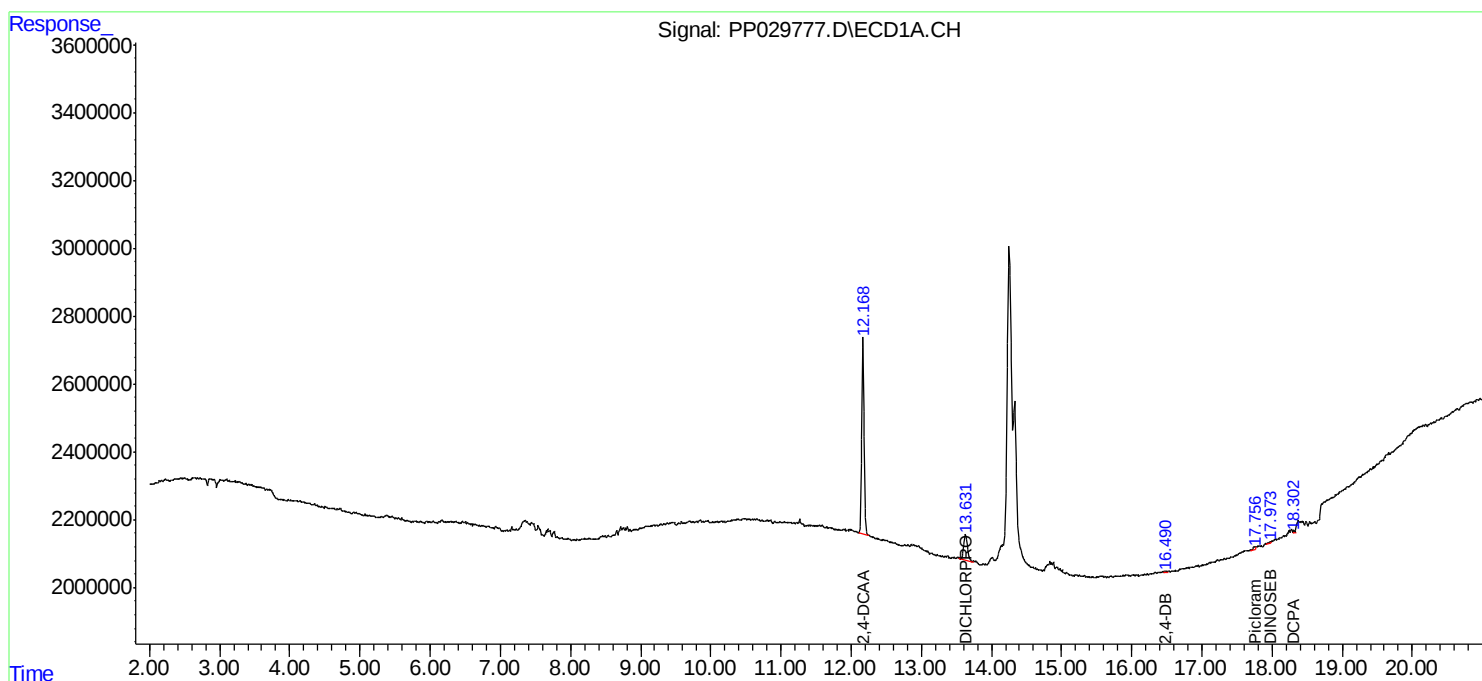


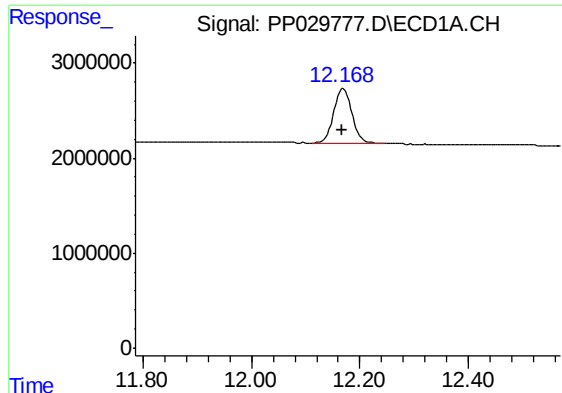

#4 2,4-DCAA


R.T.: 12.169 min
Delta R.T.: 0.002 min
Response: 13402876
Conc: 403.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

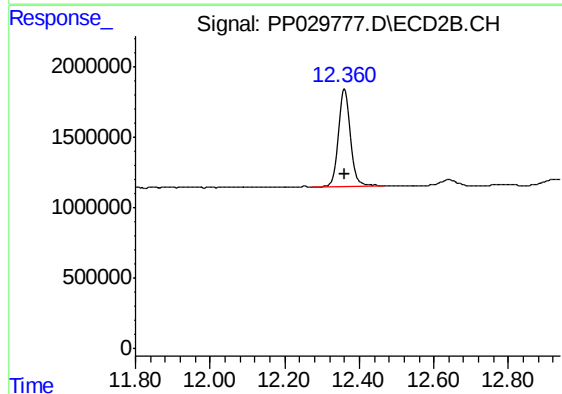


#4 2,4-DCAA

R.T.: 12.361 min
Delta R.T.: 0.000 min
Response: 14808547
Conc: 321.41 ng/ml

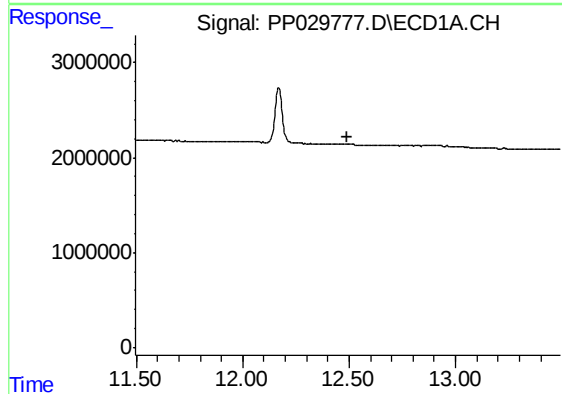


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.494 min
Response: 0
Conc: N.D.

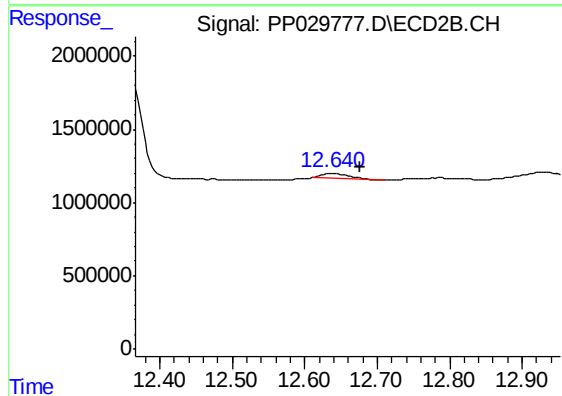

#5 DICAMBA


R.T.: 12.640 min
Delta R.T.: -0.036 min
Response: 857313
Conc: 5.52 ng/ml

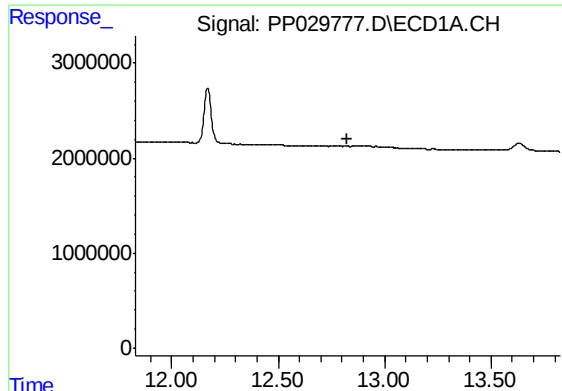

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 12.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

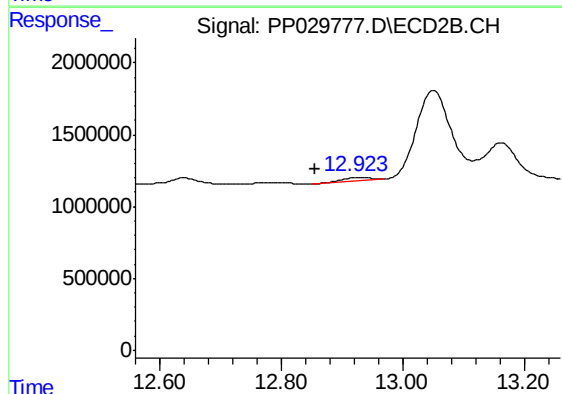


#6 MCPP

R.T.: 12.925 min
Delta R.T.: 0.069 min
Response: 860400
Conc: 28.36 ug/ml

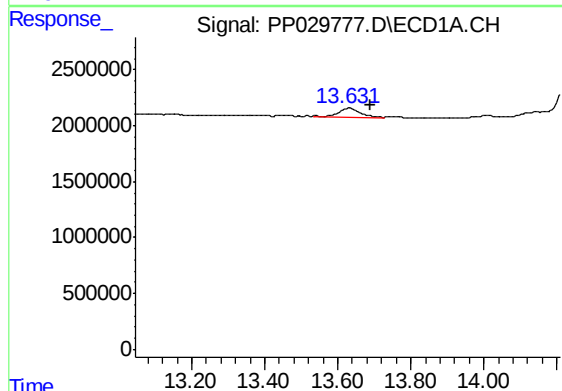


#8 DICHLORPROP

R.T.: 13.632 min
Delta R.T.: -0.057 min
Response: 2892982
Conc: 67.05 ng/ml

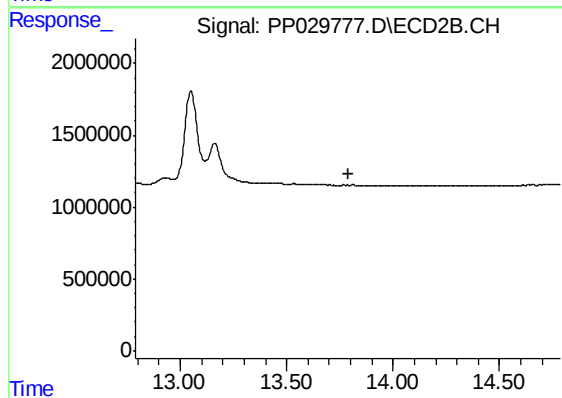

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 13.789 min
Response: 0
Conc: N.D.

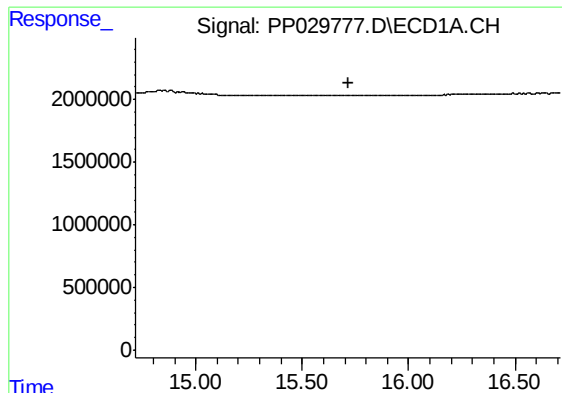

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 15.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

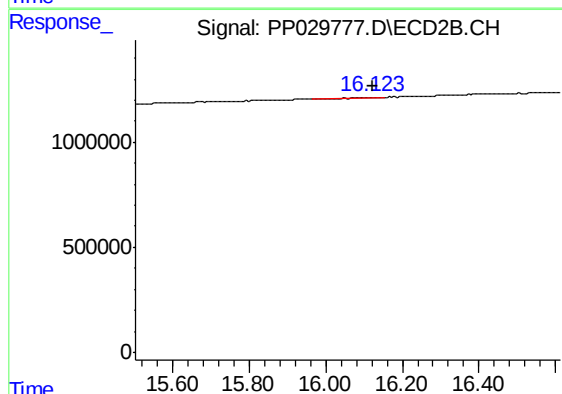


#12 2,4,5-T

R.T.: 16.136 min
Delta R.T.: 0.013 min
Response: 182737
Conc: 1.05 ng/ml

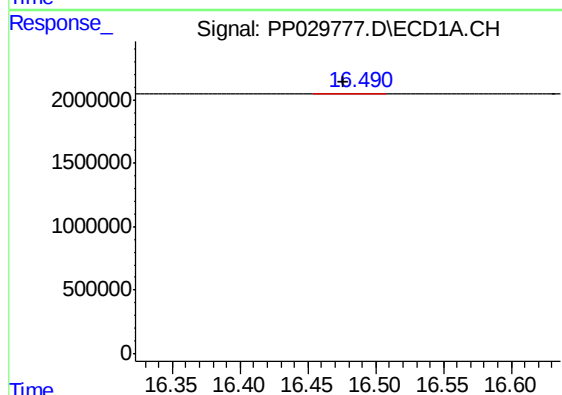


#13 2,4-DB

R.T.: 16.491 min
Delta R.T.: 0.015 min
Response: 109996
Conc: 4.63 ng/ml

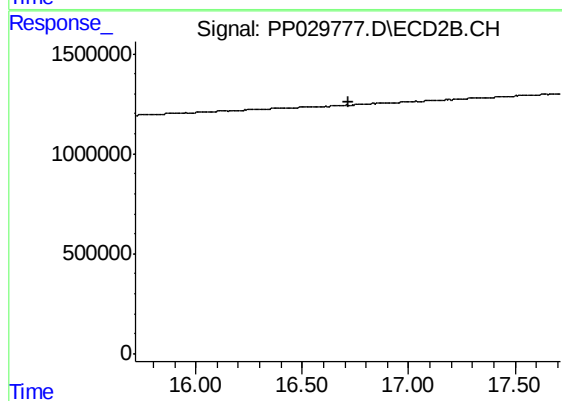

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 16.715 min
Response: 0
Conc: N.D.

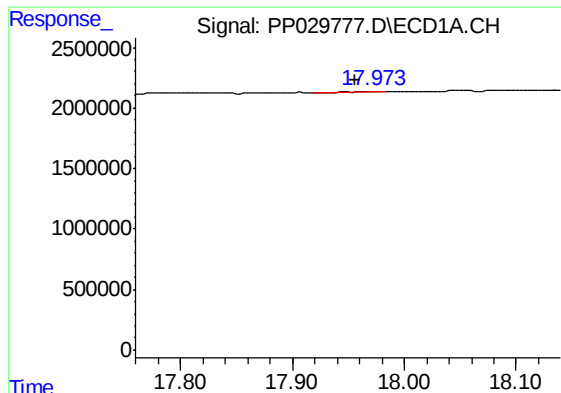

#14 DINOSEB


R.T.: 17.974 min
Delta R.T.: 0.018 min
Response: 116464
Conc: 0.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

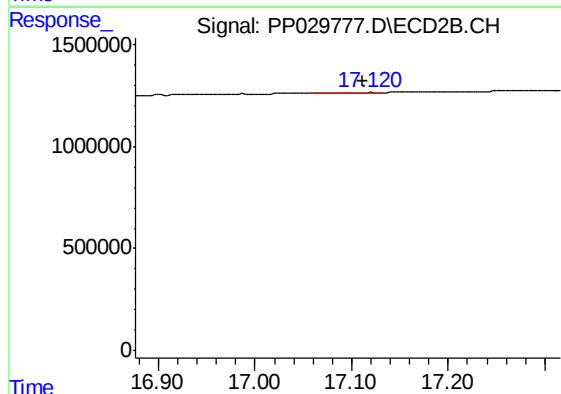


#14 DINOSEB

R.T.: 17.122 min
Delta R.T.: 0.010 min
Response: 66753
Conc: 0.50 ng/ml

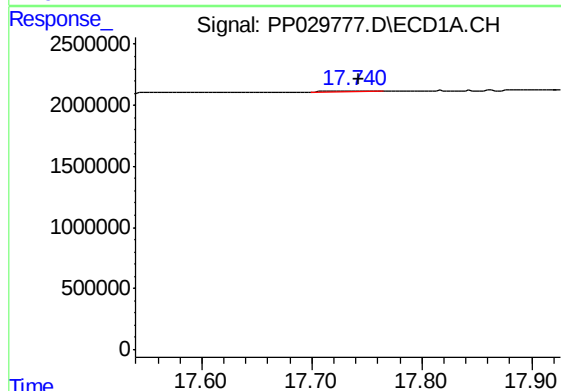


#15 Picloram

R.T.: 17.758 min
Delta R.T.: 0.014 min
Response: 237835
Conc: 0.89 ng/ml

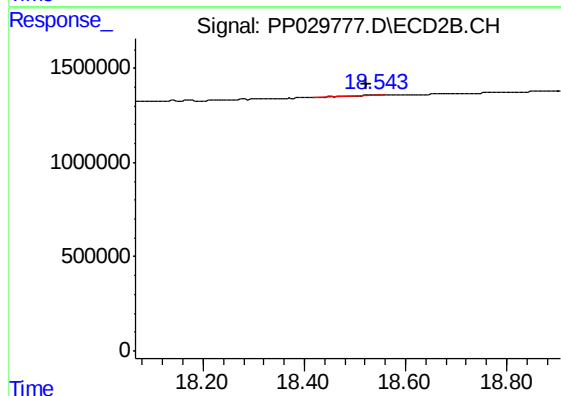

#15 Picloram


R.T.: 18.544 min
Delta R.T.: 0.021 min
Response: 146233
Conc: 0.70 ng/ml

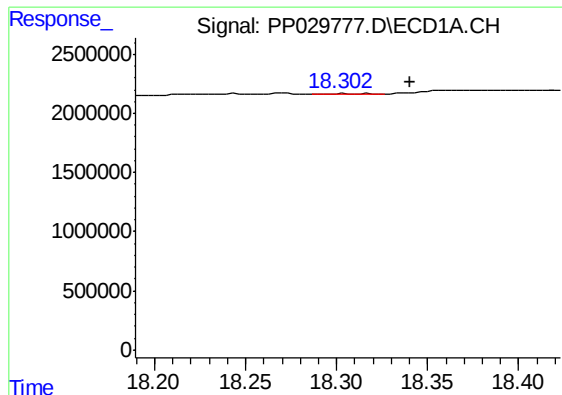

#16 DCPA

R.T.: 18.304 min
Delta R.T.: -0.036 min
Response: 91436
Conc: 0.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

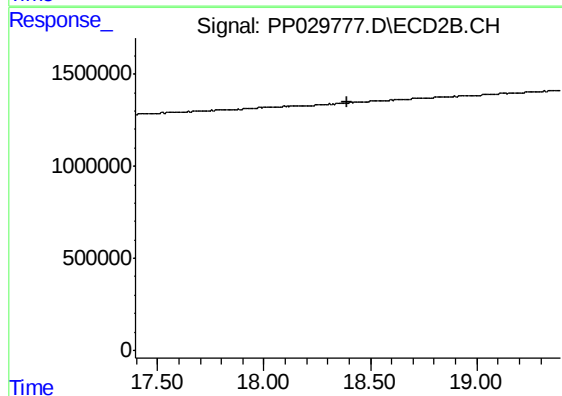

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.393 min
Response: 0
Conc: N.D.