

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040619\
 Data File : PP029779.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2019 10:52
 Operator : EI\MA
 Sample : PB118400BL
 Misc : hexane
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB118400BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:04:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040519.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 05 15:13:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.169	12.360	11299117	13177941	340.453	286.016
Target Compounds							
2) T	3,5-DICHL...	10.629	0.000	33639	0	0.455	N.D. #
5) T	DICAMBA	0.000	12.639	0	691970	N.D.	4.454 #
8) T	DICHLORPROP	13.628	0.000	3126132	0	72.455	N.D. #
11) T	2,4,5-TP ...	0.000	15.467	0	66600	N.D.	0.301 #
12) T	2,4,5-T	0.000	16.106	0	2911842	N.D.	16.774 #
13) T	2,4-DB	16.485	0.000	1892451	0	79.616	N.D. #
14) T	DINOSEB	17.947	17.171	56972	2920153	0.365	21.716 #
15) T	Picloram	17.755	18.526	919820	288941	3.445	1.391 #
16) T	DCPA	18.310	0.000	752123	0	2.294	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040619\
Data File : PP029779.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2019 10:52
Operator : EI\MA
Sample : PB118400BL
Misc : hexane
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
PB118400BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:04:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP040519.M
Quant Title : 8080.M
QLast Update : Fri Apr 05 15:13:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

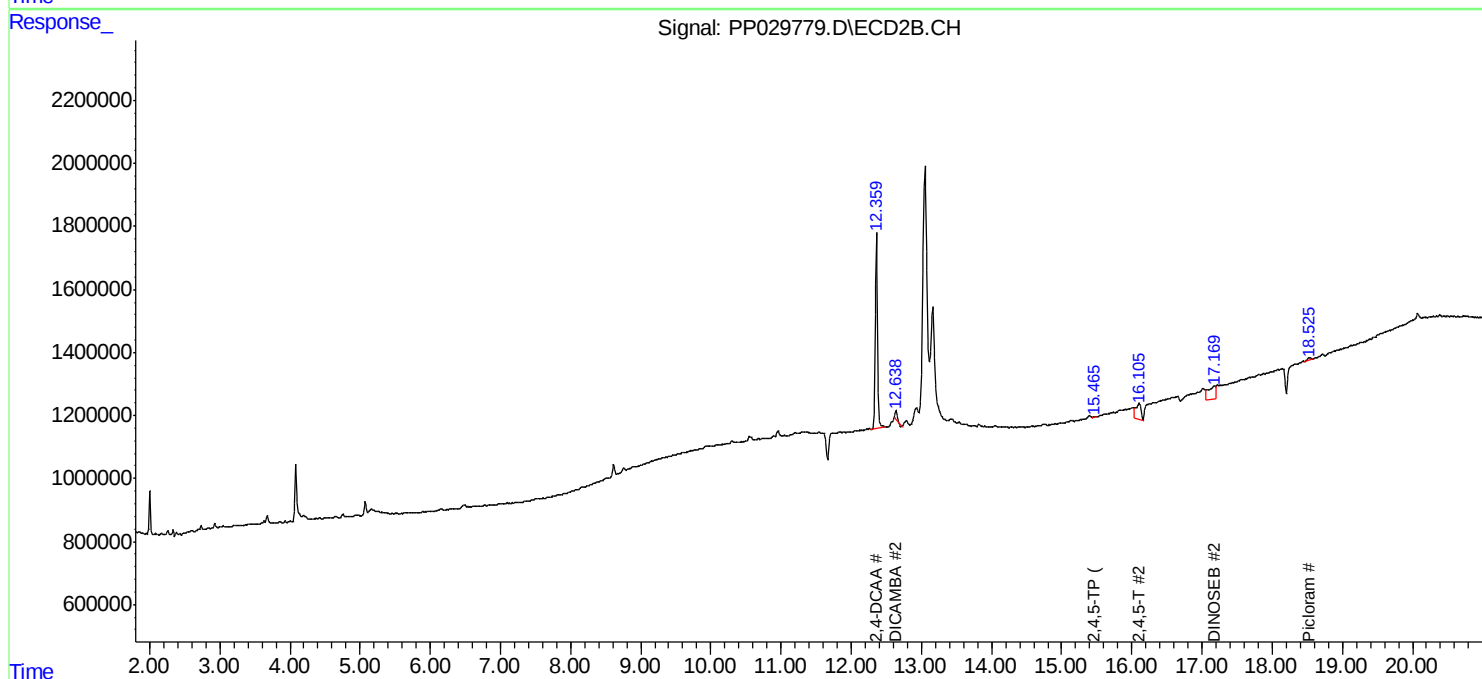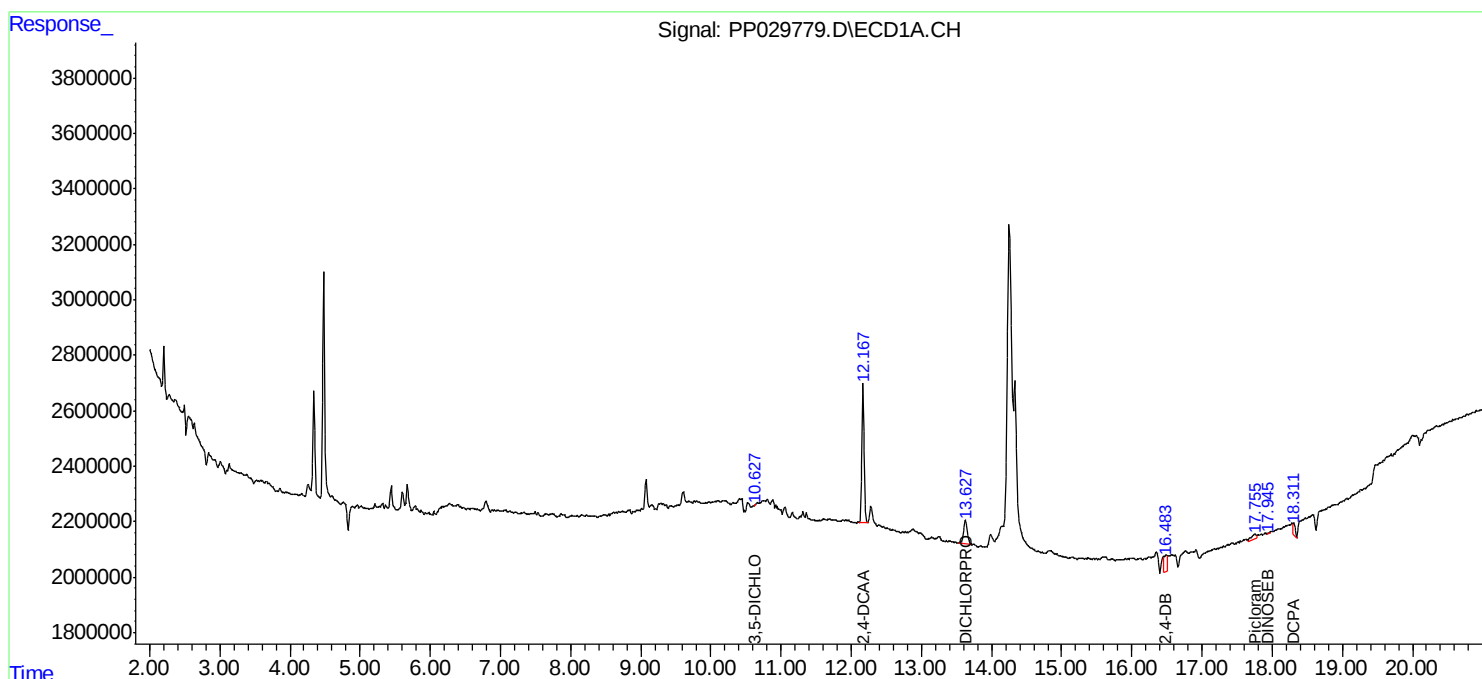


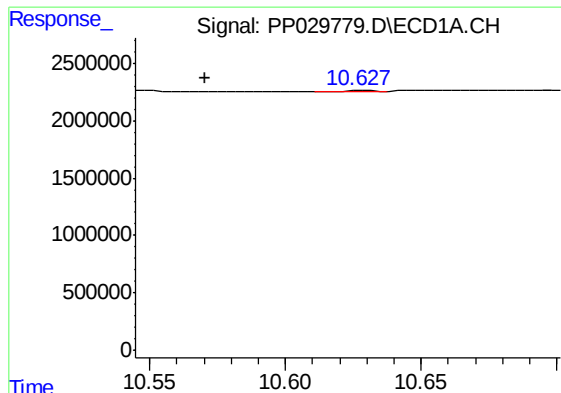

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 10.629 min
Delta R.T.: 0.059 min
Response: 33639
Conc: 0.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118400BL

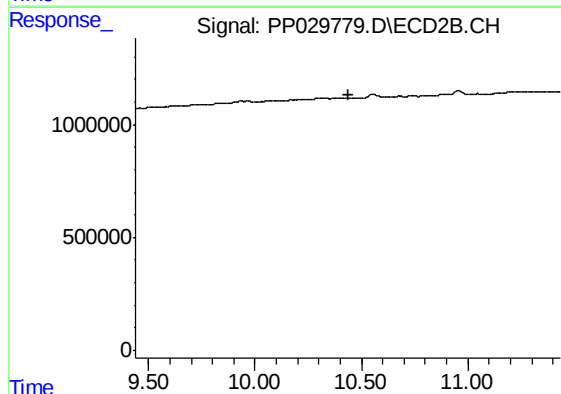


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.437 min
Response: 0
Conc: N.D.

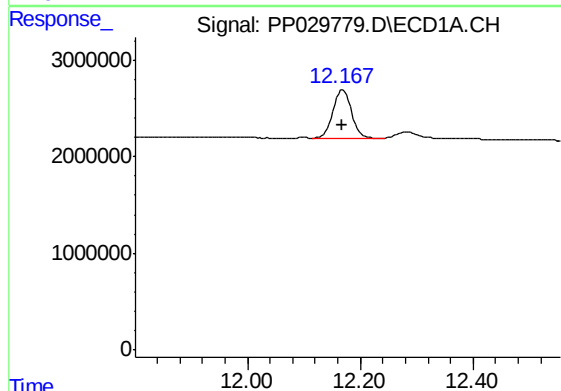


#4 2,4-DCAA

R.T.: 12.169 min
Delta R.T.: 0.001 min
Response: 11299117
Conc: 340.45 ng/ml

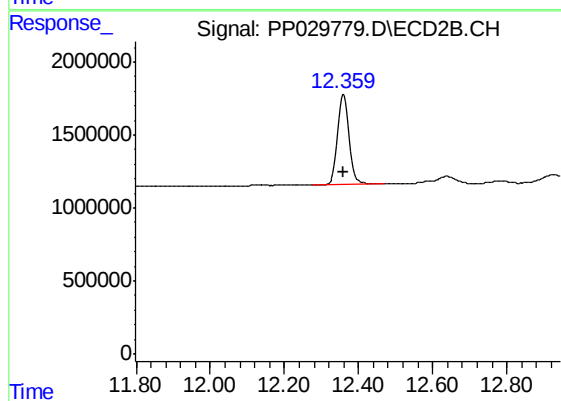

#4 2,4-DCAA


R.T.: 12.360 min
Delta R.T.: 0.000 min
Response: 13177941
Conc: 286.02 ng/ml

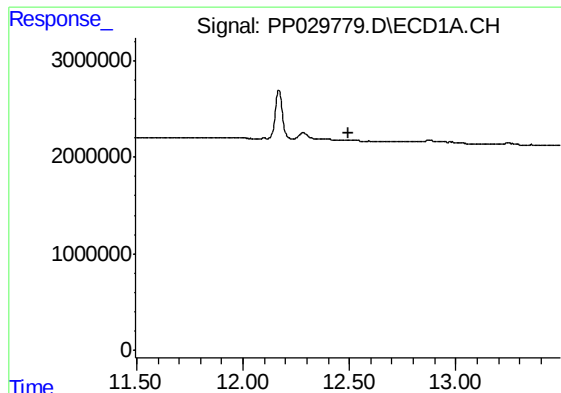

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB118400BL

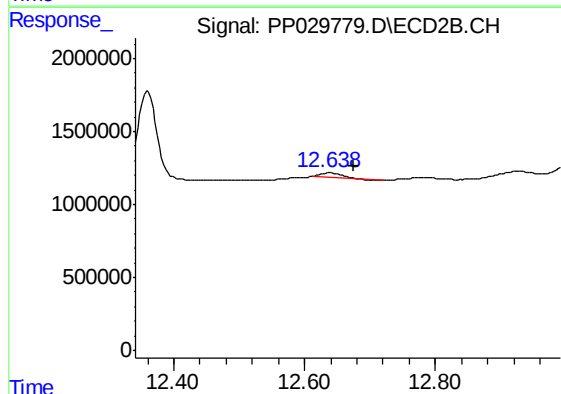


#5 DICAMBA

R.T.: 12.639 min
Delta R.T.: -0.037 min
Response: 691970
Conc: 4.45 ng/ml

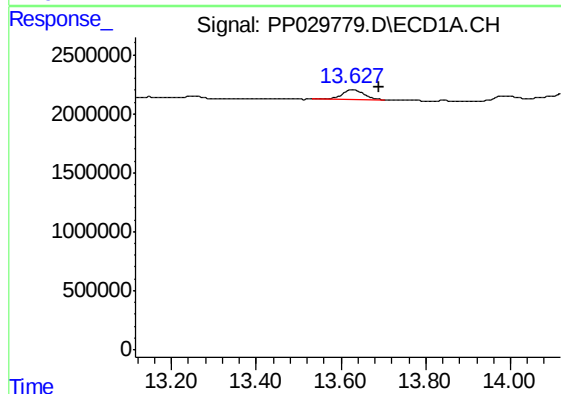


#8 DICHLORPROP

R.T.: 13.628 min
Delta R.T.: -0.061 min
Response: 3126132
Conc: 72.46 ng/ml

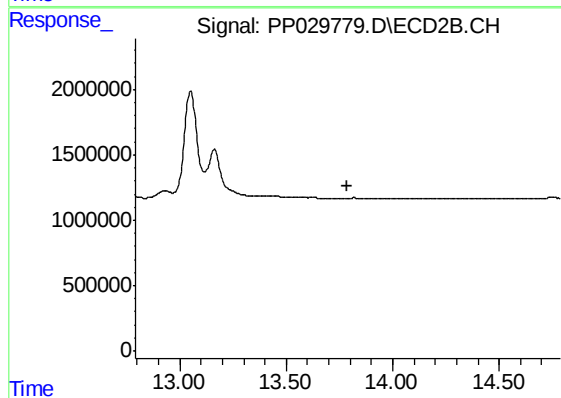

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.789 min
Response: 0
Conc: N.D.

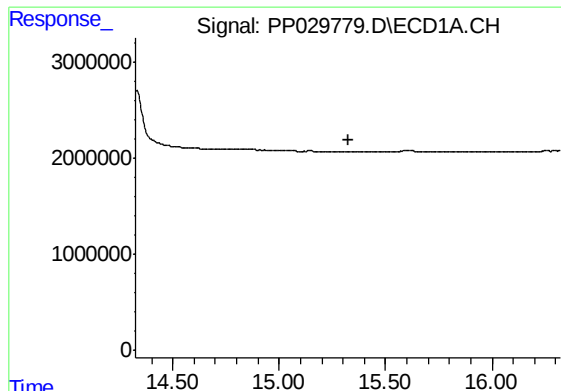

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB118400BL

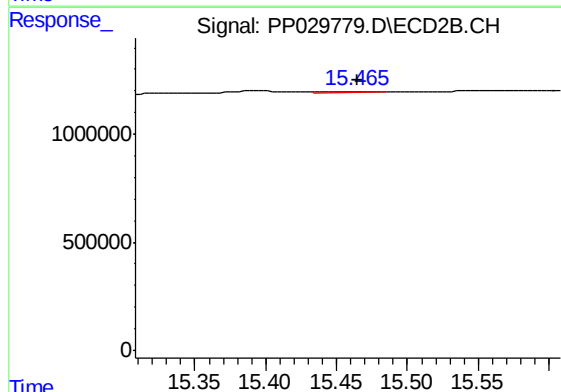


#11 2,4,5-TP (SILVEX)

R.T.: 15.467 min
Delta R.T.: 0.003 min
Response: 66600
Conc: 0.30 ng/ml

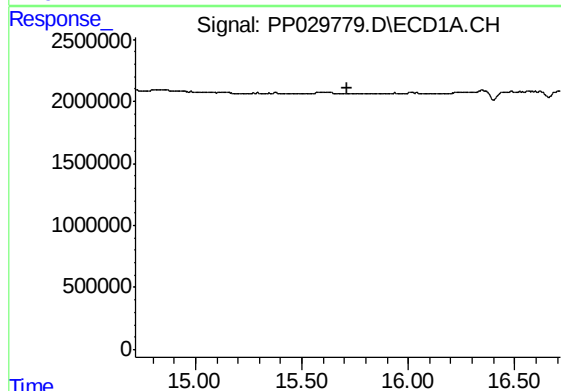


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.715 min
Response: 0
Conc: N.D.

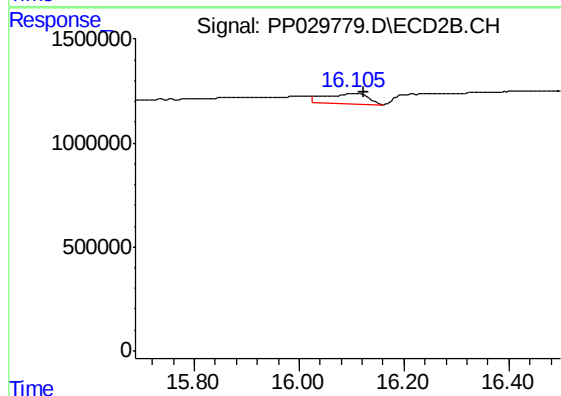

#12 2,4,5-T


R.T.: 16.106 min
Delta R.T.: -0.017 min
Response: 2911842
Conc: 16.77 ng/ml

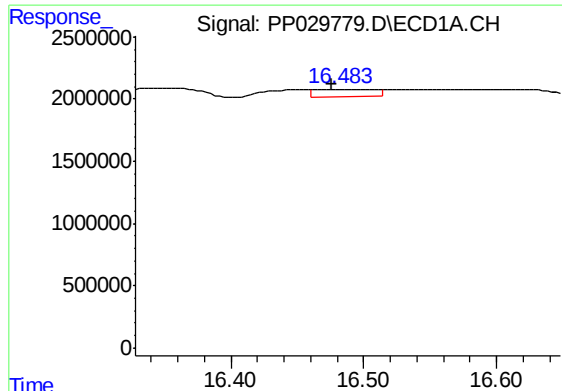

#13 2,4-DB


R.T.: 16.485 min
Delta R.T.: 0.009 min
Response: 1892451
Conc: 79.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118400BL

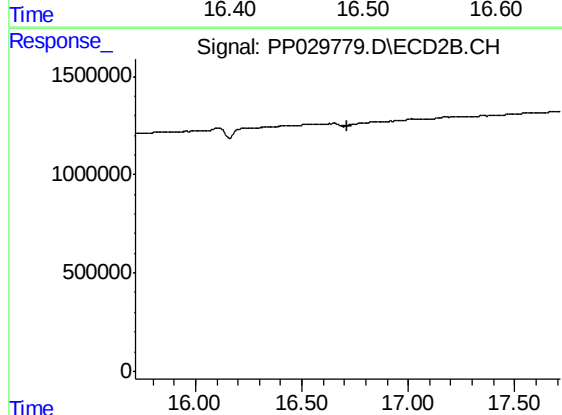


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.715 min
Response: 0
Conc: N.D.

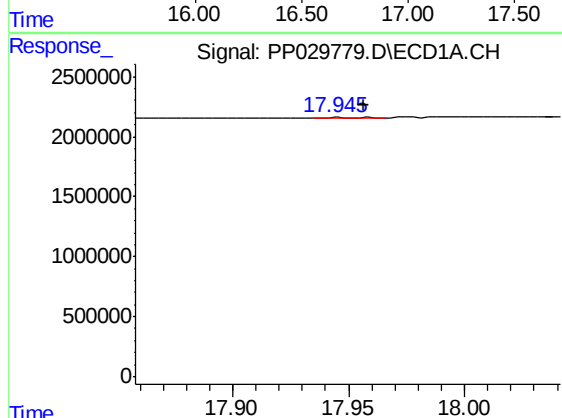


#14 DINOSEB

R.T.: 17.947 min
Delta R.T.: -0.009 min
Response: 56972
Conc: 0.36 ng/ml

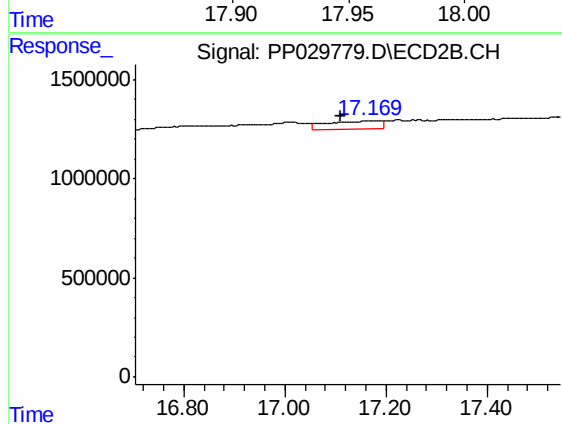

#14 DINOSEB


R.T.: 17.171 min
Delta R.T.: 0.059 min
Response: 2920153
Conc: 21.72 ng/ml

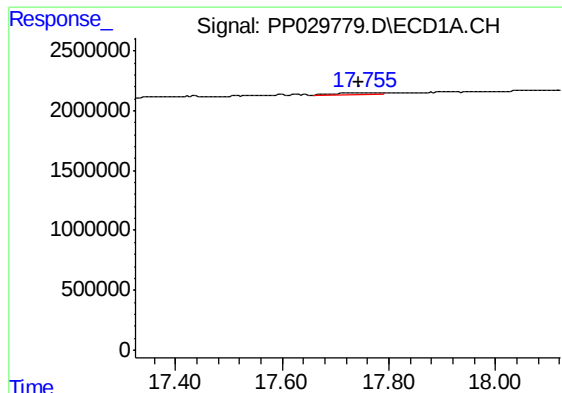

#15 Picloram


R.T.: 17.755 min
Delta R.T.: 0.012 min
Response: 919820
Conc: 3.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118400BL

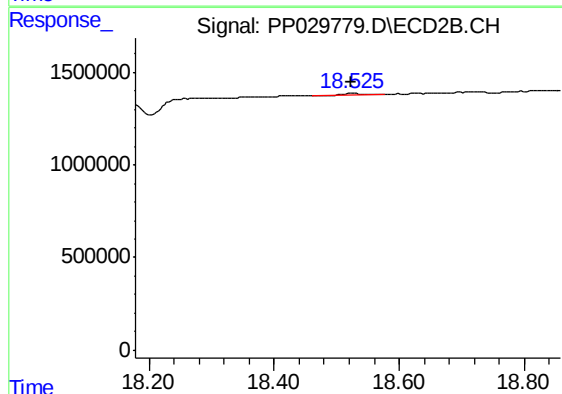


#15 Picloram

R.T.: 18.526 min
Delta R.T.: 0.003 min
Response: 288941
Conc: 1.39 ng/ml

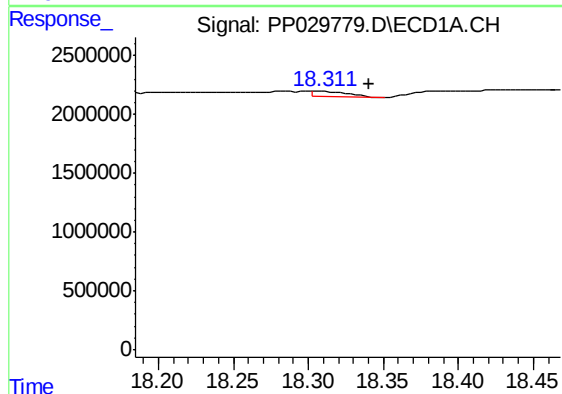

#16 DCPA

R.T.: 18.310 min
Delta R.T.: -0.030 min
Response: 752123
Conc: 2.29 ng/ml

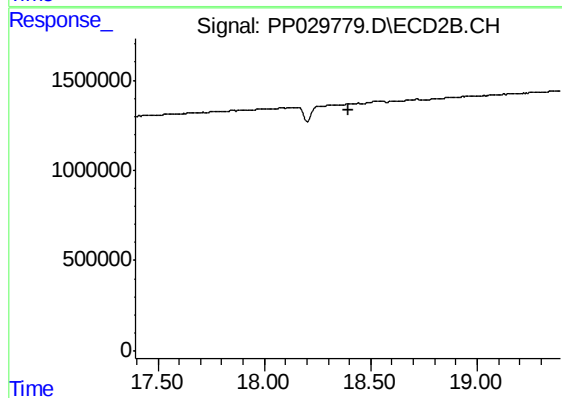

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.393 min
Response: 0
Conc: N.D.