

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040621\
 Data File : PP034696.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2021 13:52
 Operator : DD\AJ
 Sample : M1936-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEE066K-END-1

Manual Integrations
 APPROVED

Ankita
 4/7/2021 4:47:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:39:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.845	4.256	187373	109167	2.456	2.430
2) SA Decachlor...	10.765	9.559	215938	67871	2.805m	2.404
Target Compounds						
26) L6 AR-1254-1	7.062	6.376	77957	35151	28.353	19.053m#
27) L6 AR-1254-2	7.292	6.531	142827	38882	33.590m	24.303m#
28) L6 AR-1254-3	7.671	6.951	127832	68221	28.008	27.335m
29) L6 AR-1254-4	7.969	7.187	108322	36781	35.035	27.980m
30) L6 AR-1254-5	8.394	7.615	128917	77739	36.276	38.249

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP040621\
Data File : PP034696.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2021 13:52
Operator : DD\AJ
Sample : M1936-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
HEE066K-END-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:39:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

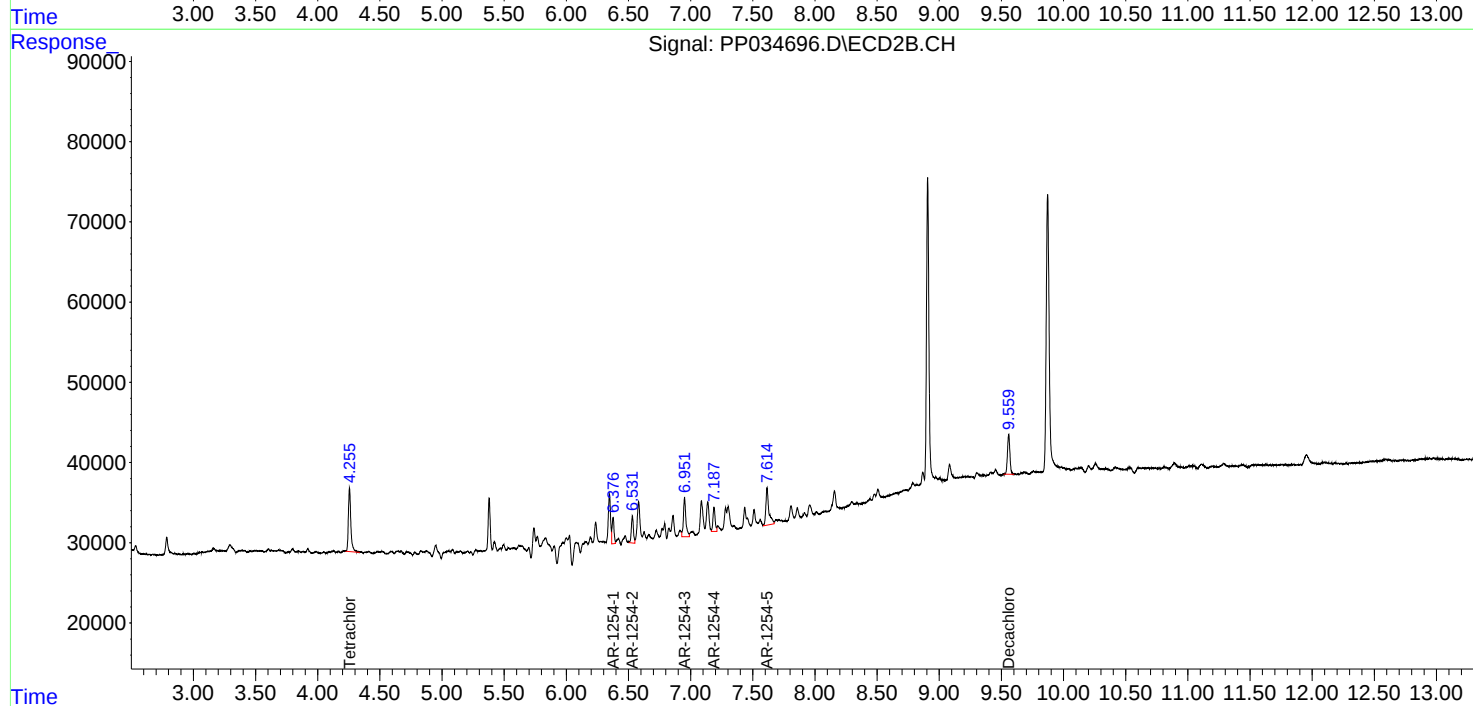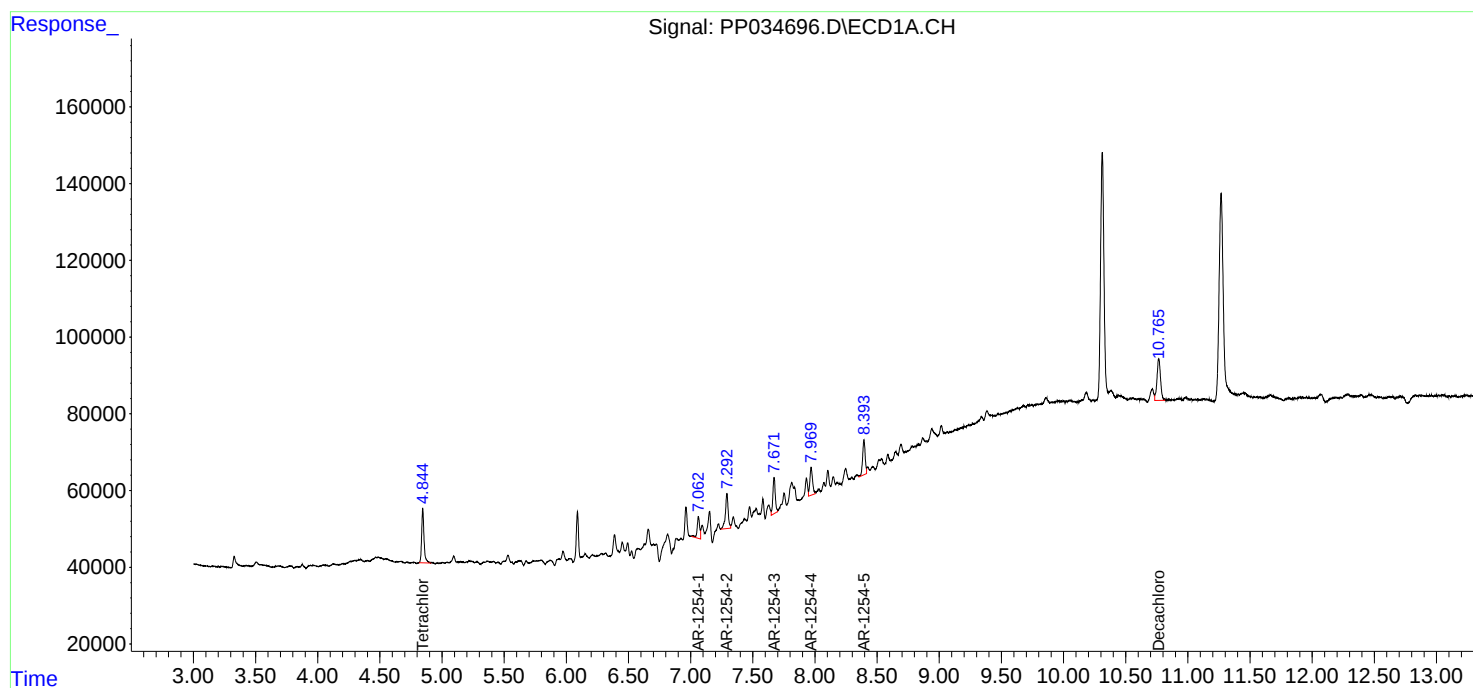

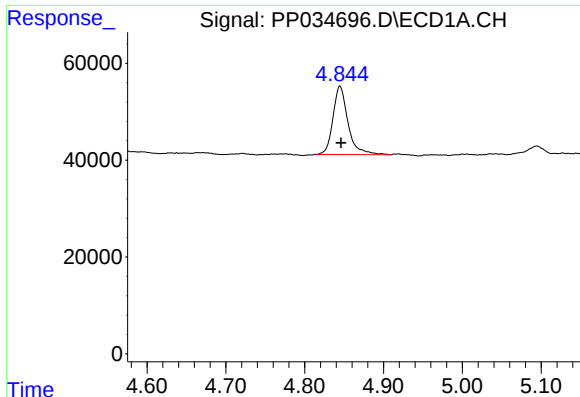


#1 Tetrachloro-m-xylene

R.T.: 4.845 min
Delta R.T.: -0.001 min
Response: 187373
Conc: 2.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE066K-END-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:26 PM

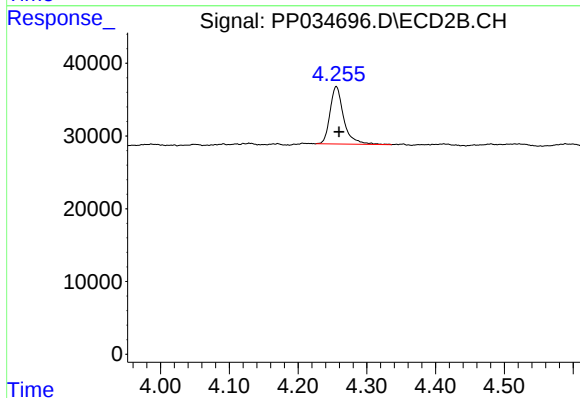


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: -0.004 min
Response: 109167
Conc: 2.43 ng/ml

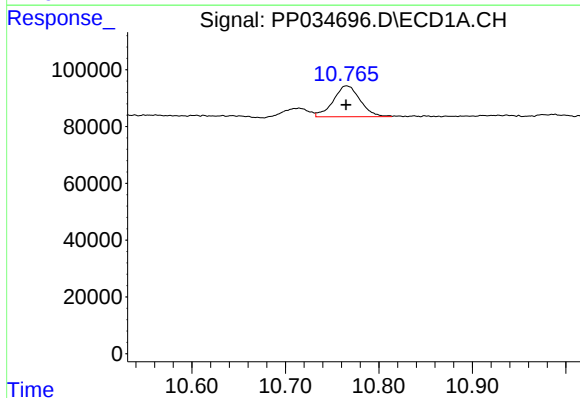


#2 Decachlorobiphenyl

R.T.: 10.765 min
Delta R.T.: 0.000 min
Response: 215938
Conc: 2.81 ng/ml m

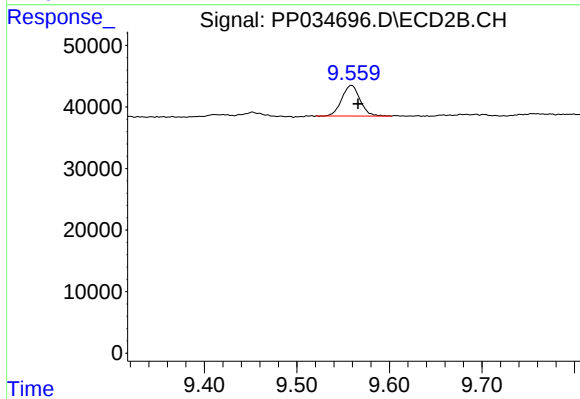

#2 Decachlorobiphenyl

R.T.: 9.559 min
Delta R.T.: -0.007 min
Response: 67871
Conc: 2.40 ng/ml

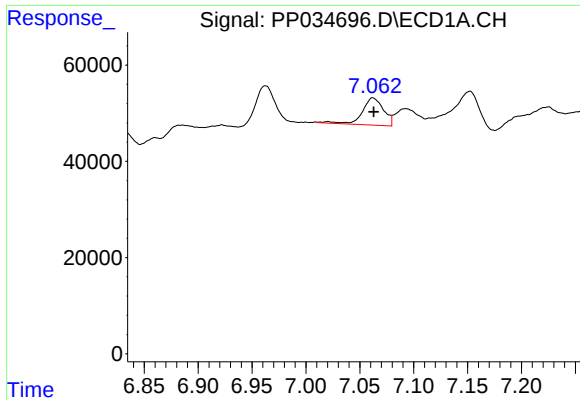


#26 AR-1254-1

R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 77957
Conc: 28.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE066K-END-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:26 PM

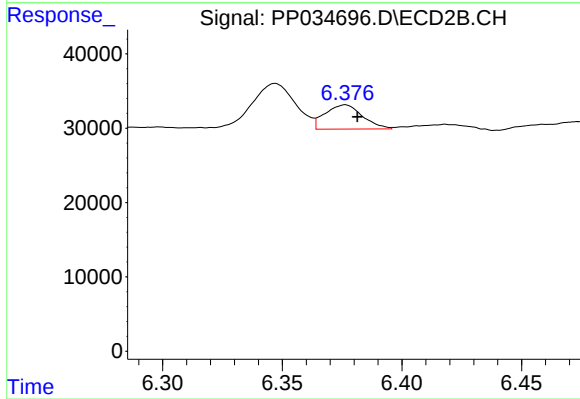


#26 AR-1254-1

R.T.: 6.376 min
Delta R.T.: -0.005 min
Response: 35151
Conc: 19.05 ng/ml m

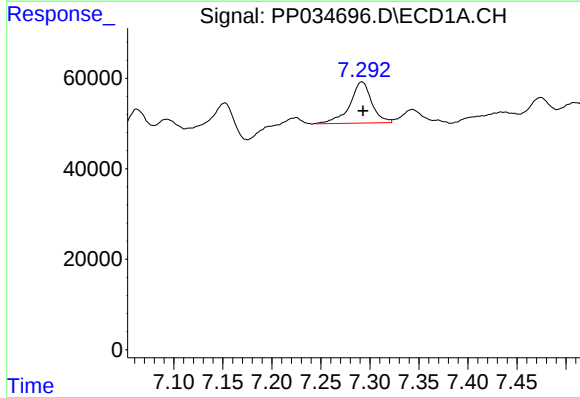


#27 AR-1254-2

R.T.: 7.292 min
Delta R.T.: -0.001 min
Response: 142827
Conc: 33.59 ng/ml m

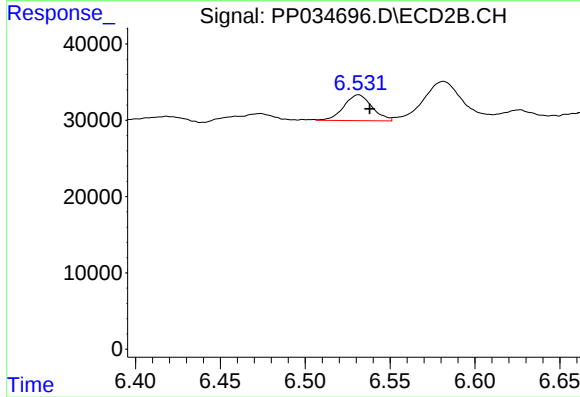

#27 AR-1254-2

R.T.: 6.531 min
Delta R.T.: -0.007 min
Response: 38882
Conc: 24.30 ng/ml m

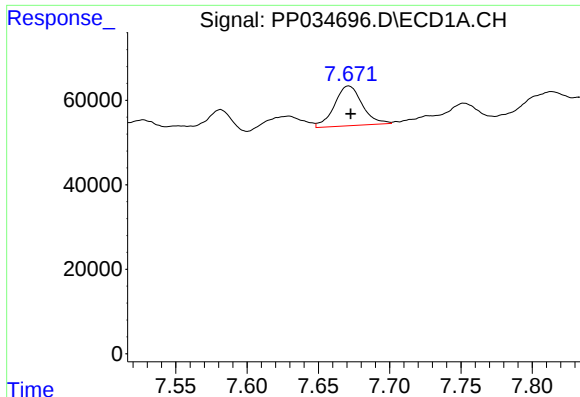


#28 AR-1254-3

R.T.: 7.671 min
Delta R.T.: -0.001 min
Response: 127832
Conc: 28.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE066K-END-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:26 PM

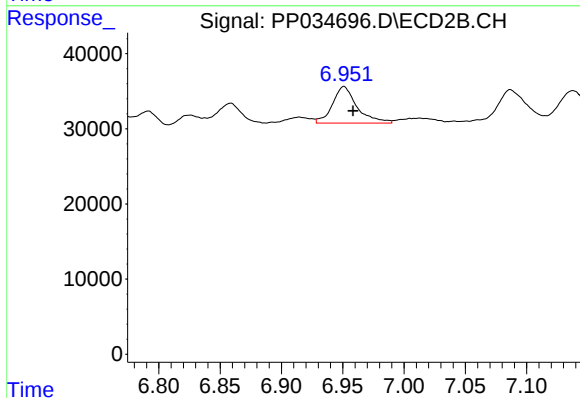


#28 AR-1254-3

R.T.: 6.951 min
Delta R.T.: -0.008 min
Response: 68221
Conc: 27.33 ng/ml m

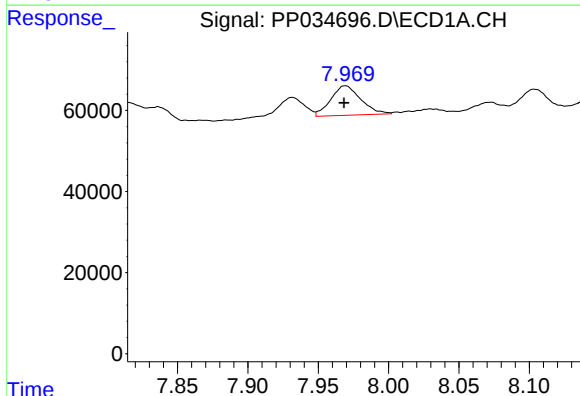


#29 AR-1254-4

R.T.: 7.969 min
Delta R.T.: 0.000 min
Response: 108322
Conc: 35.03 ng/ml

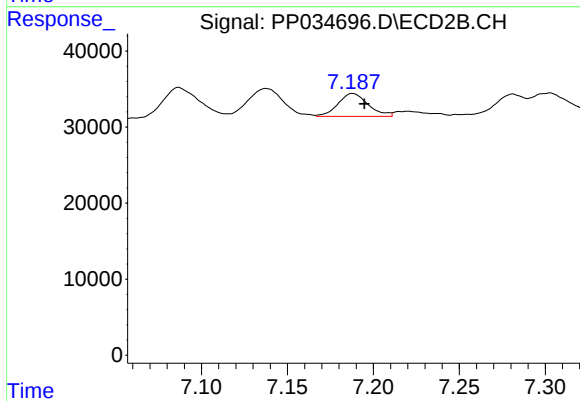

#29 AR-1254-4

R.T.: 7.187 min
Delta R.T.: -0.008 min
Response: 36781
Conc: 27.98 ng/ml m

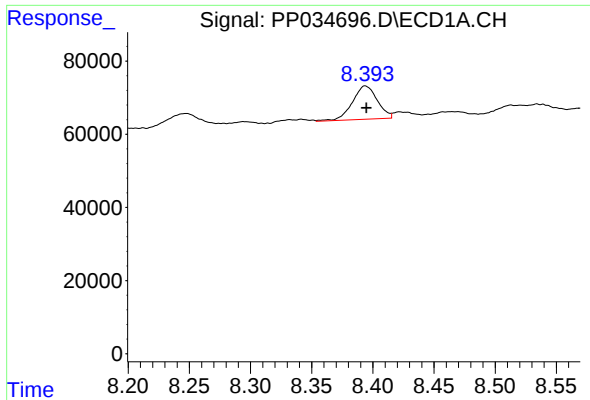


#30 AR-1254-5

R.T.: 8.394 min
Delta R.T.: 0.000 min
Response: 128917
Conc: 36.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE066K-END-1

Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:26 PM

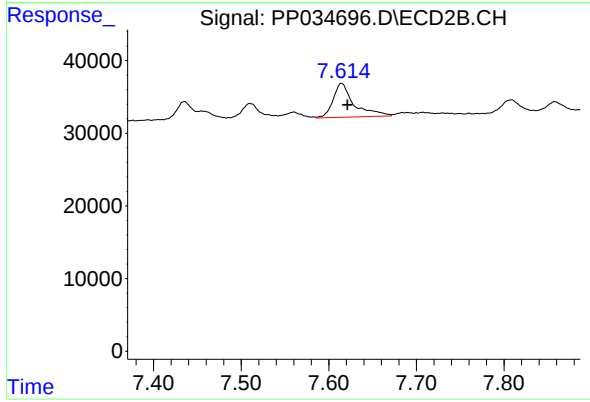

#30 AR-1254-5

R.T.: 7.615 min
Delta R.T.: -0.007 min
Response: 77739
Conc: 38.25 ng/ml